




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112423\
 Data File : BN028852.D
 Acq On : 24 Nov 2023 10:52
 Operator : MA/JU
 Sample : PB157174BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 SBLK174

Manual IntegrationsAPPROVED

Quant Time: Nov 25 01:01:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2023
 Supervised By :mohammad ahmed 11/28/2023

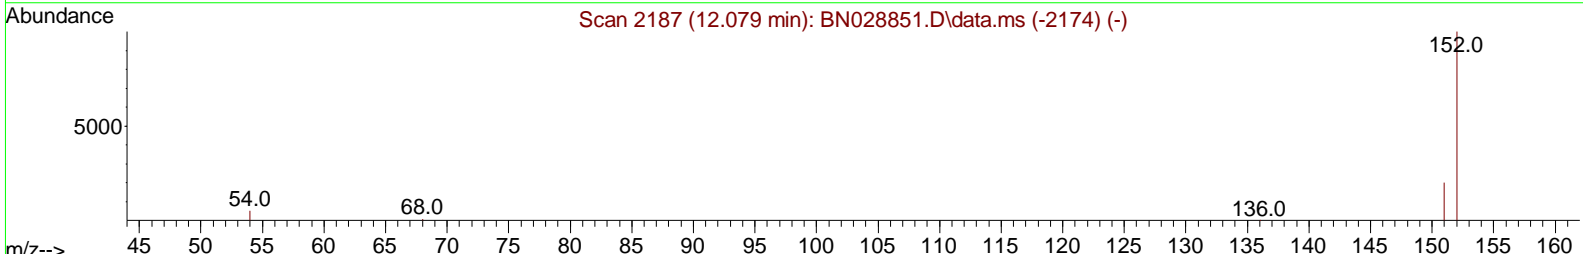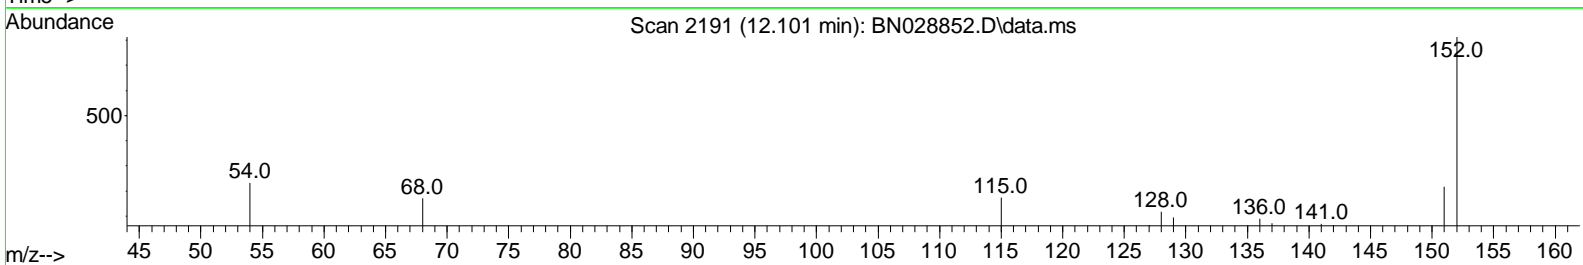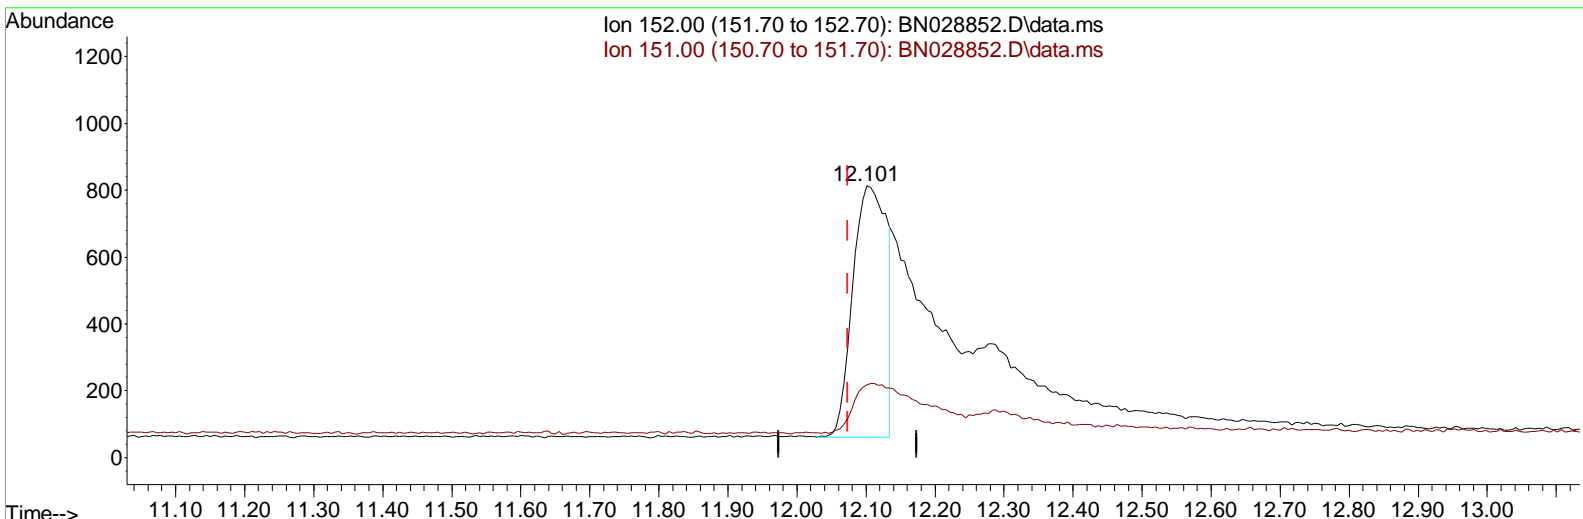

TIC: BN028852.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.101min (+ 0.027) 0.11 ng/ul

response	2565	
Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	18.21
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112423\
 Data File : BN028852.D
 Acq On : 24 Nov 2023 10:52
 Operator : MA/JU
 Sample : PB157174BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 SBLK174

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2023
 Supervised By :mohammad ahmed 11/28/2023

Quant Time: Nov 25 01:01:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

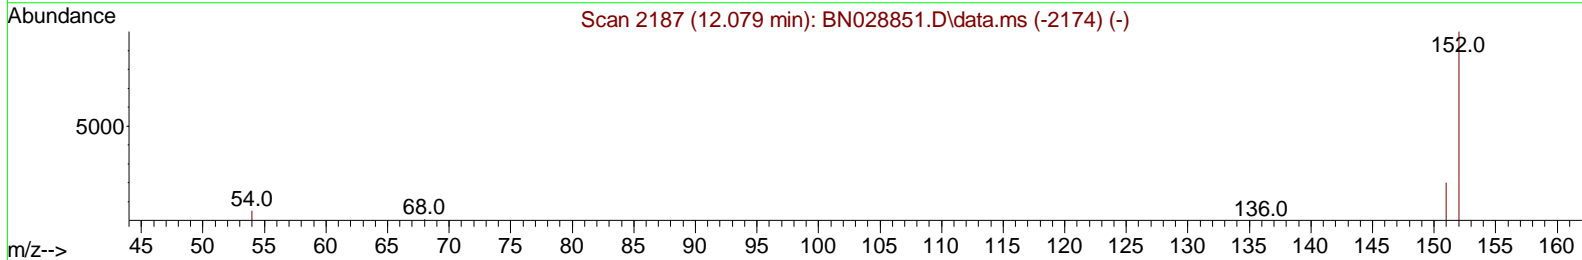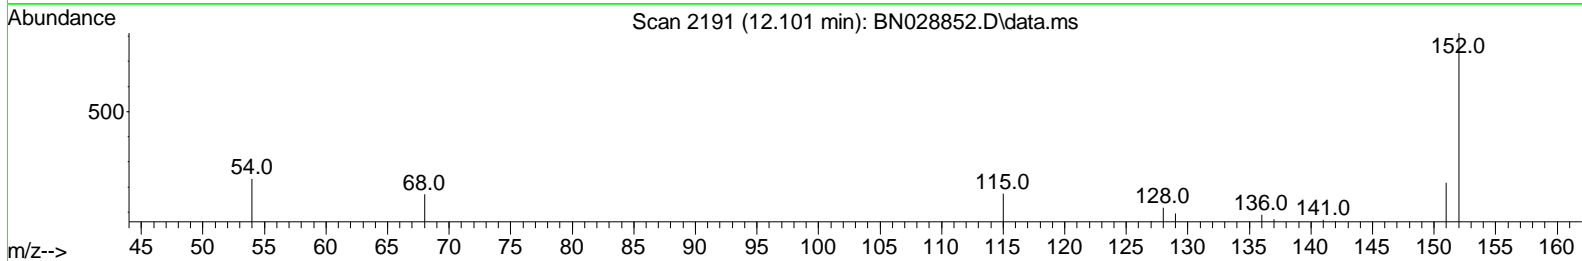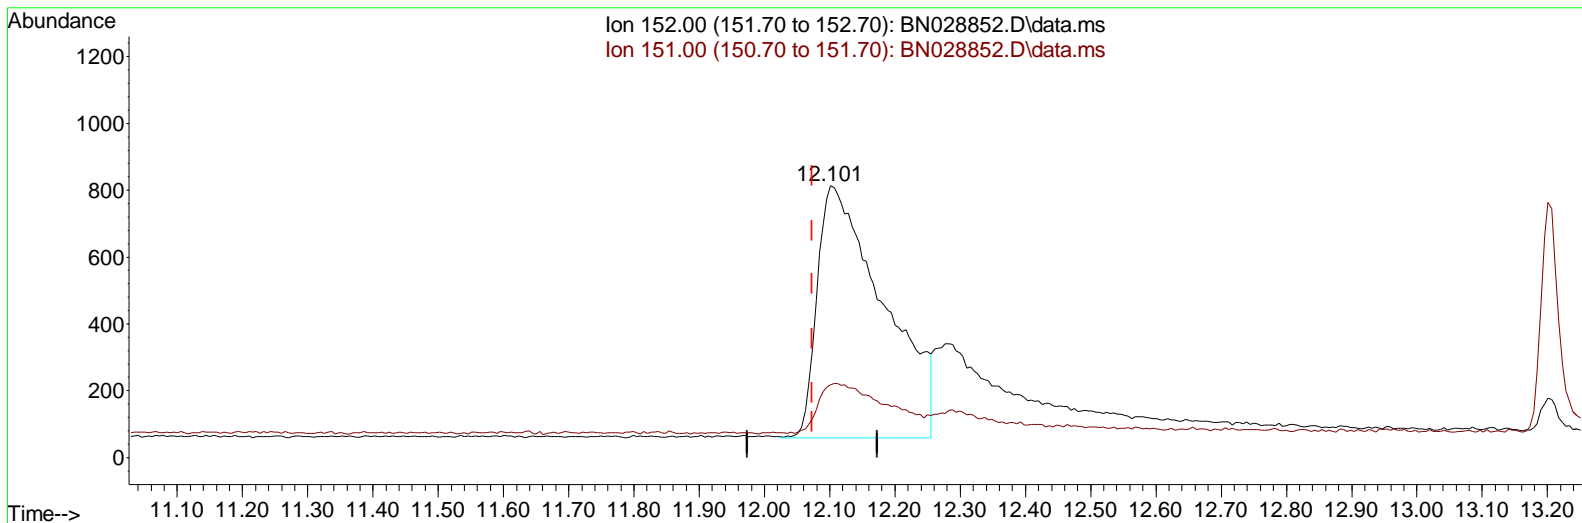

TIC: BN028852.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.101min (+ 0.027) 0.22 ng/ul m

response 5333

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	8.76#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112423\
 Data File : BNO28852.D
 Acq On : 24 Nov 2023 10:52
 Operator : MA/JU
 Sample : PB157174BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 SBLK174

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2023
 Supervised By :mohammad ahmed 11/28/2023

Quant Time: Nov 25 01:01:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Compound	R.T.	QI on	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.694	152	5279	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.446	136	16013	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.297	164	10076	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.060	188	16811	0.400	ng/ul	0.00
17) Chrysene-d12	21.286	240	10264	0.400	ng/ul	# 0.02
23) Perylene-d12	23.543	264	14677	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.099	96	44295	7.592	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.101	152	5333m	0.221	ng/ul	0.03
18) Fluoranthene-d10	19.098	212	11672	0.353	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112423\
 Data File : BN028852.D
 Acq On : 24 Nov 2023 10:52
 Operator : MA/JU
 Sample : PB157174BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 SBLK174

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2023
 Supervised By :mohammad ahmed 11/28/2023

Quant Time: Nov 25 01:01:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SI M-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

