




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112423\
 Data File : BN028858.D
 Acq On : 24 Nov 2023 15:10
 Operator : MA/JU
 Sample : 05336-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCKB8

Manual IntegrationsAPPROVED

Quant Time: Nov 25 01:02:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2023
 Supervised By :mohammad ahmed 11/28/2023

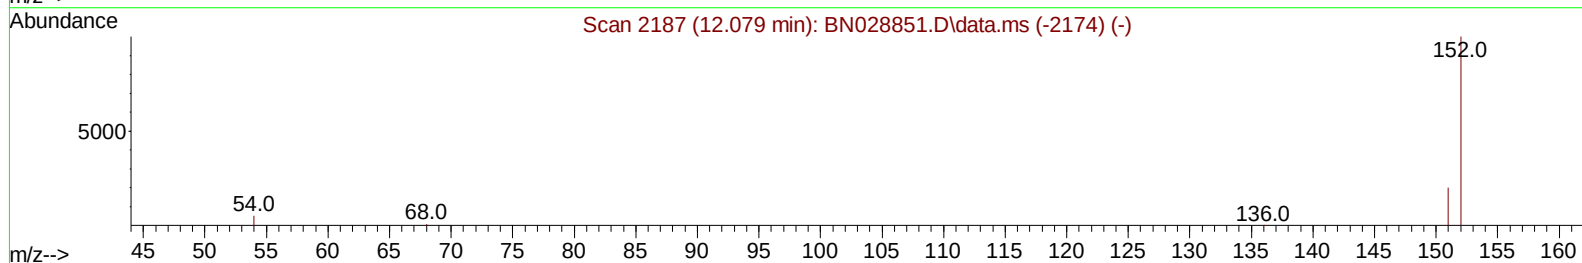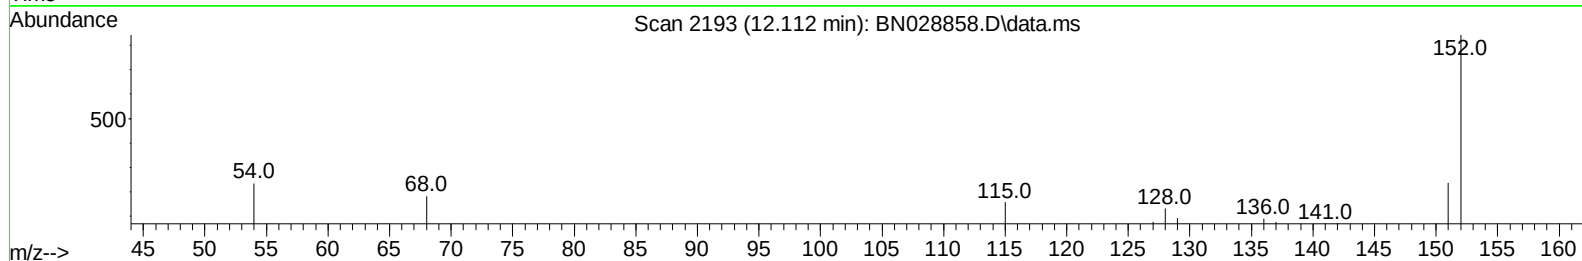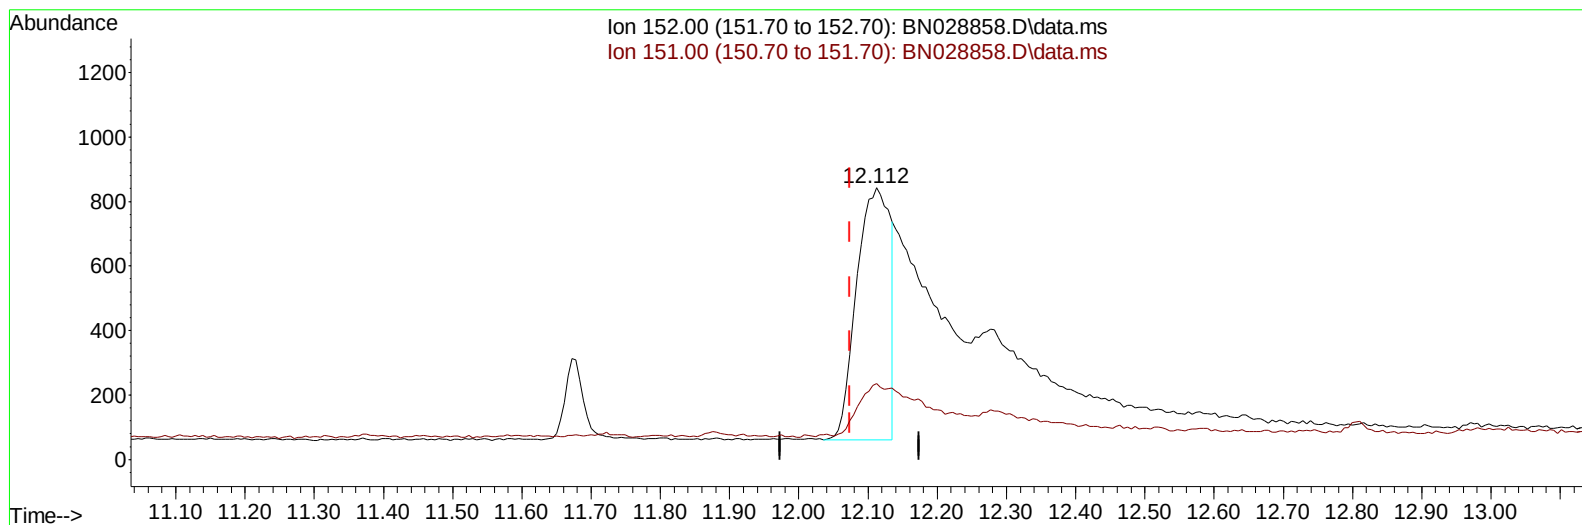

TIC: BN028858.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.112min (+ 0.039) 0.08 ng/ul

response 2613

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	17.64
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112423\
Data File : BN028858.D
Acq On : 24 Nov 2023 15:10
Operator : MA/JU
Sample : 05336-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCKB8

Manual IntegrationsAPPROVED

Quant Time: Nov 25 01:02:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2023
Supervised By :mohammad ahmed 11/28/2023

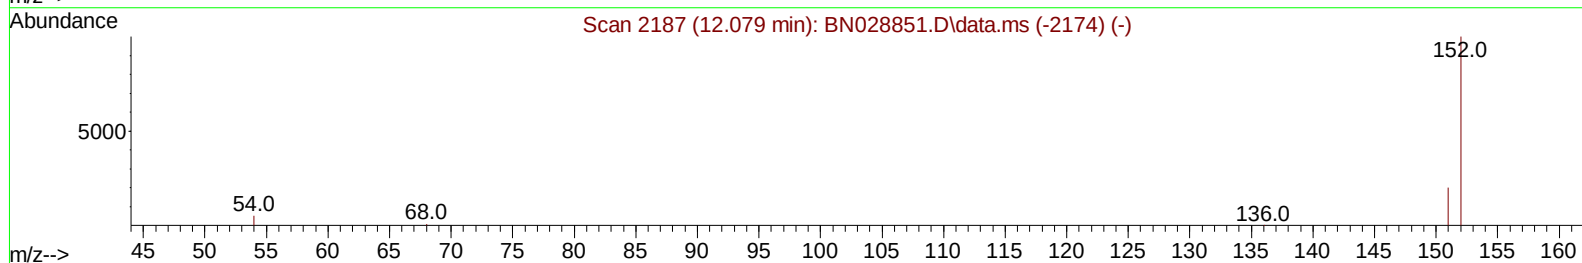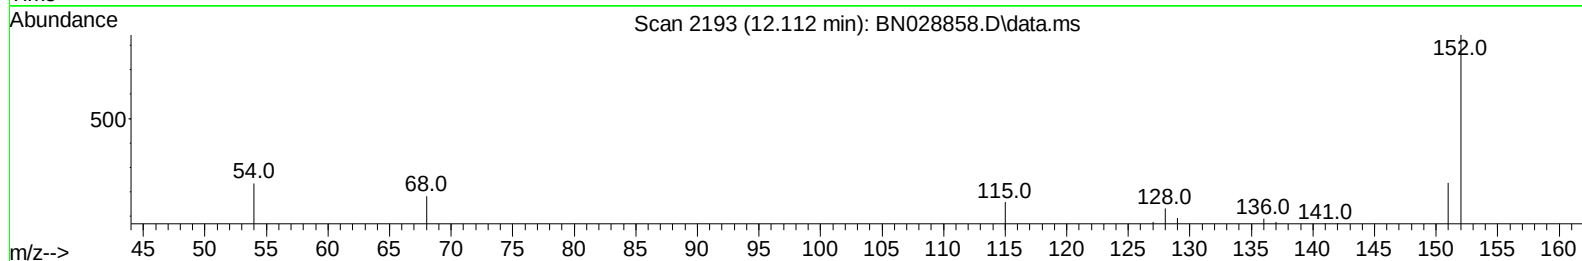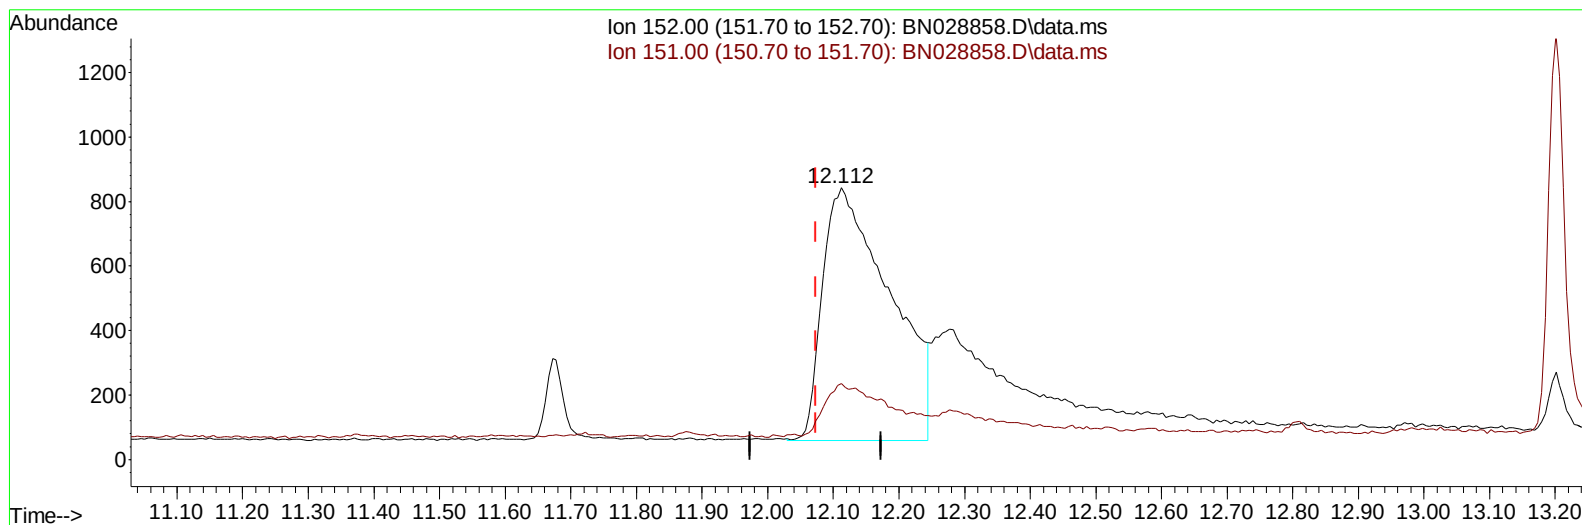

TIC: BN028858.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.112min (+ 0.039) 0.18 ng/ul m

response 5615

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	8.21#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112423\
 Data File : BN028858.D
 Acq On : 24 Nov 2023 15:10
 Operator : MA/JU
 Sample : 05336-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCKB8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2023
 Supervised By :mohammad ahmed 11/28/2023

Quant Time: Nov 25 01:02:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.715	152		4891	0.400	ng/ul	#-0.02
4) Naphthalene-d8	10.446	136		20433	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.297	164		11625	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.056	188		21813	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.283	240		12098	0.400	ng/ul	# 0.01
23) Perylene-d12	23.540	264		15861	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.099	96		28260	5.228	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.112	152		5615m	0.183	ng/ul	0.04
18) Fluoranthene-d10	19.094	212		18293	0.470	ng/ul	0.00
Target Compounds							Qvalue
14) Pentachlorophenol	16.710	266		3351	0.640	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112423\
Data File : BN028858.D
Acq On : 24 Nov 2023 15:10
Operator : MA/JU
Sample : 05336-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCKB8

Manual IntegrationsAPPROVED

Quant Time: Nov 25 01:02:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2023
Supervised By :mohammad ahmed 11/28/2023

