




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112423\
Data File : BN028864.D
Acq On : 24 Nov 2023 18:49
Operator : MA/JU
Sample : PB157190BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK190

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2023
Supervised By :mohammad ahmed 11/28/2023

Quant Time: Nov 25 01:03:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

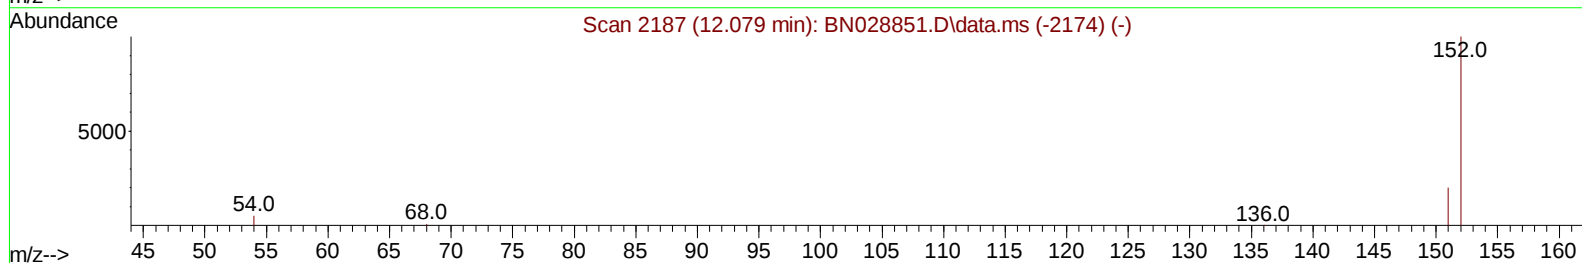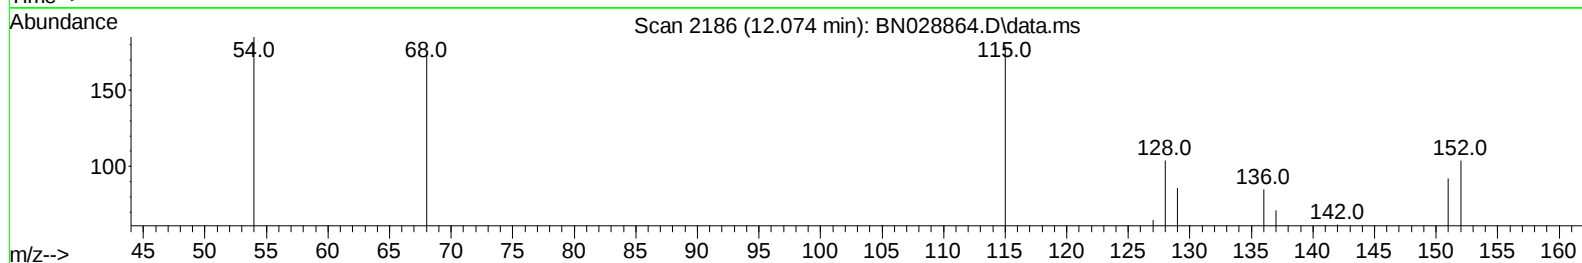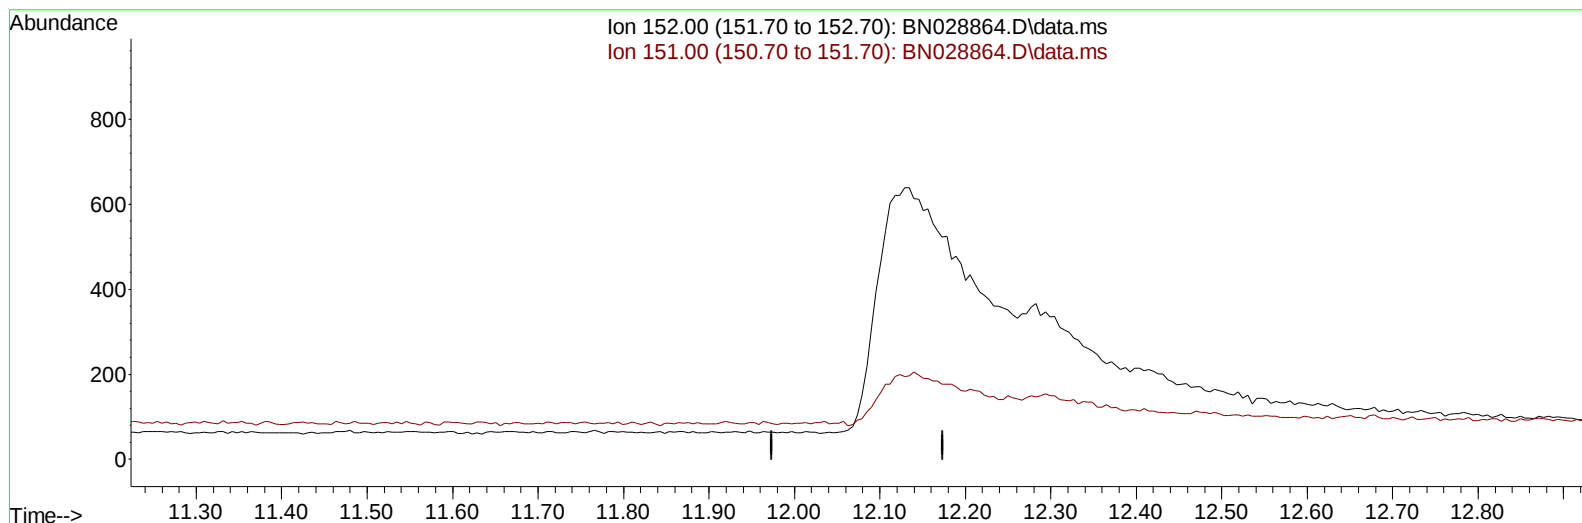

TIC: BN028864.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.074min (-12.074) 0.00 ng/u1

response 0

Ion	Exp%	Act%
152.00	100.00	0.00
151.00	20.50	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112423\
 Data File : BN028864.D
 Acq On : 24 Nov 2023 18:49
 Operator : MA/JU
 Sample : PB157190BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK190

Manual IntegrationsAPPROVED

Quant Time: Nov 25 01:03:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2023
 Supervised By :mohammad ahmed 11/28/2023

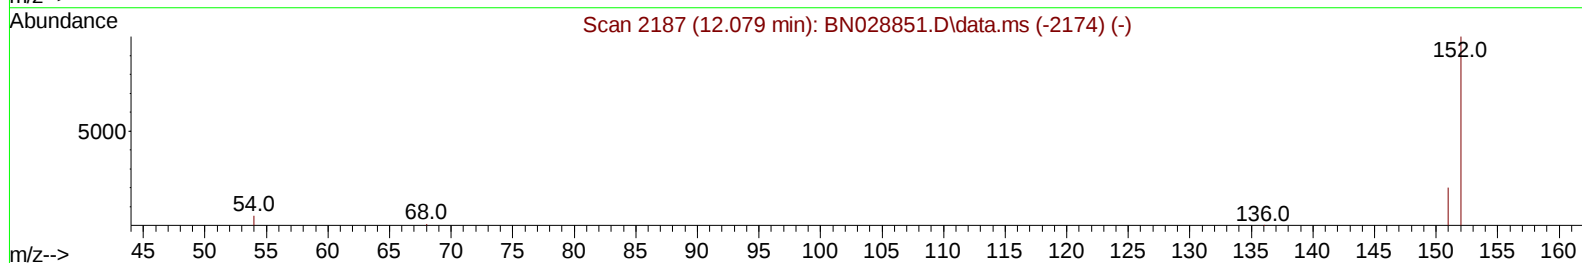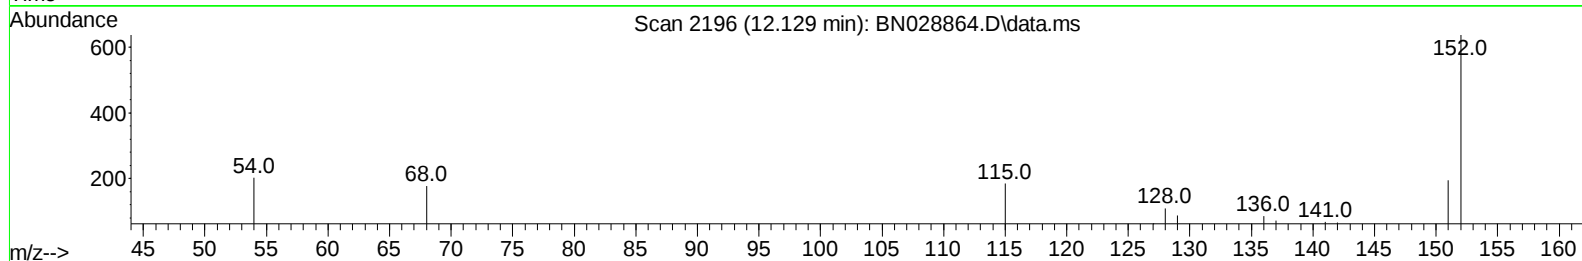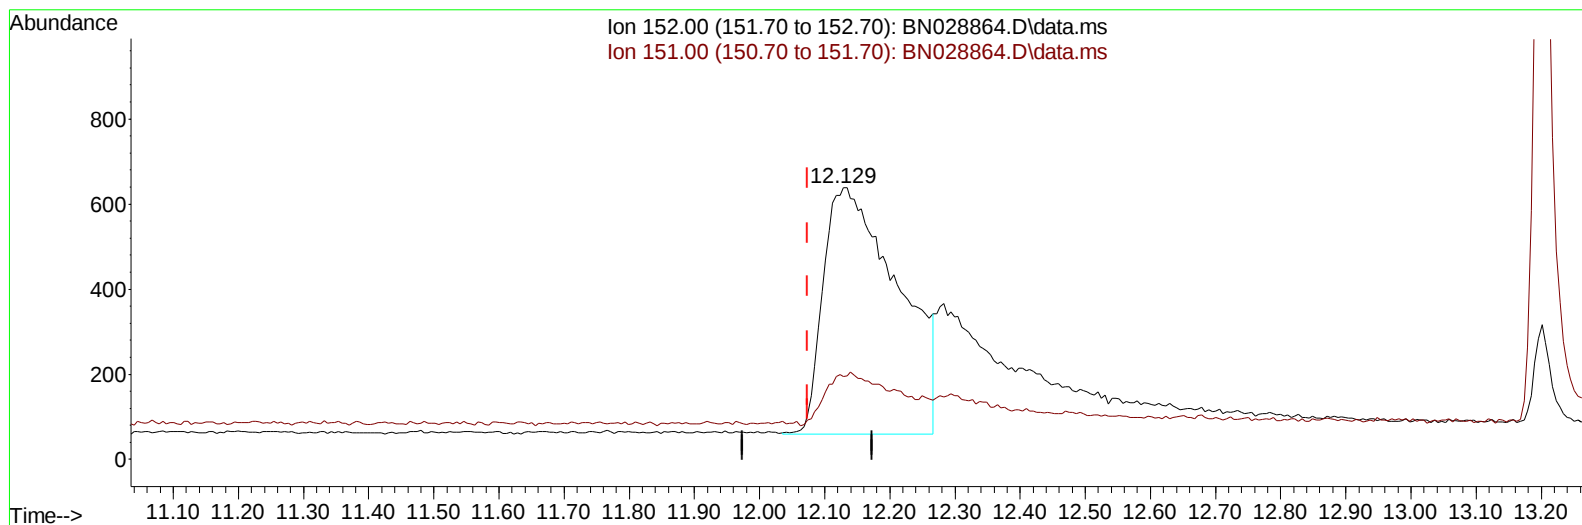

TIC: BN028864.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.129min (+ 0.055) 0.22 ng/ul m

response 4631

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112423\
 Data File : BN028864.D
 Acq On : 24 Nov 2023 18:49
 Operator : MA/JU
 Sample : PB157190BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK190

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2023
 Supervised By :mohammad ahmed 11/28/2023

Quant Time: Nov 25 01:03:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.715	152	4636	0.400	ng/ul	#-0.02
4) Naphthalene-d8	10.446	136	14041	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.297	164	10124	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.060	188	17843	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.287	240	9391	0.400	ng/ul	# 0.02
23) Perylene-d12	23.540	264	13296	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.099	96	40260	7.857	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.129	152	4631m	0.219	ng/ul	0.06
18) Fluoranthene-d10	19.094	212	11546	0.382	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112423\
Data File : BN028864.D
Acq On : 24 Nov 2023 18:49
Operator : MA/JU
Sample : PB157190BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK190

Manual IntegrationsAPPROVED

Quant Time: Nov 25 01:03:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2023
Supervised By :mohammad ahmed 11/28/2023

