

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN112519\
 Data File : BN008744.D
 Acq On : 25 Nov 2019 19:28
 Operator : JU
 Sample : PB124746BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB124746BL

Quant Time: Nov 26 03:17:05 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN112219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 25 10:49:40 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	5054	0.40	ng	0.00
7) Naphthalene-d8	10.35	136	18126	0.40	ng	0.00
13) Acenaphthene-d10	14.21	164	10056	0.40	ng	0.00
19) Phenanthrene-d10	16.95	188	21112	0.40	ng	-0.01
27) Chrysene-d12	21.15	240	19130	0.40	ng	-0.01
34) Perylene-d12	23.32	264	13121	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.23	112	3211	0.24	ng	0.00
5) Phenol-d6	6.78	99	3013	0.18	ng	0.00
8) Nitrobenzene-d5	8.72	82	5945	0.37	ng	-0.01
11) 2-Methylnaphthalene-d10	11.94	152	10182	0.36	ng	0.00
14) 2,4,6-Tribromophenol	15.71	330	1853	0.40	ng	0.00
15) 2-Fluorobiphenyl	12.83	172	17631	0.45	ng	-0.01
25) Fluoranthene-d10	18.99	212	23973	0.39	ng	0.00
29) Terphenyl-d14	19.60	244	20608	0.45	ng	0.00
Target Compounds						Qvalue
32) Bis(2-ethylhexyl)phthalate	21.10	149	1833	0.040	ng	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN112519\
Data File : BN008744.D
Acq On : 25 Nov 2019 19:28
Operator : JU
Sample : PB124746BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB124746BL

Quant Time: Nov 26 03:17:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN112219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 25 10:49:40 2019
Response via : Initial Calibration

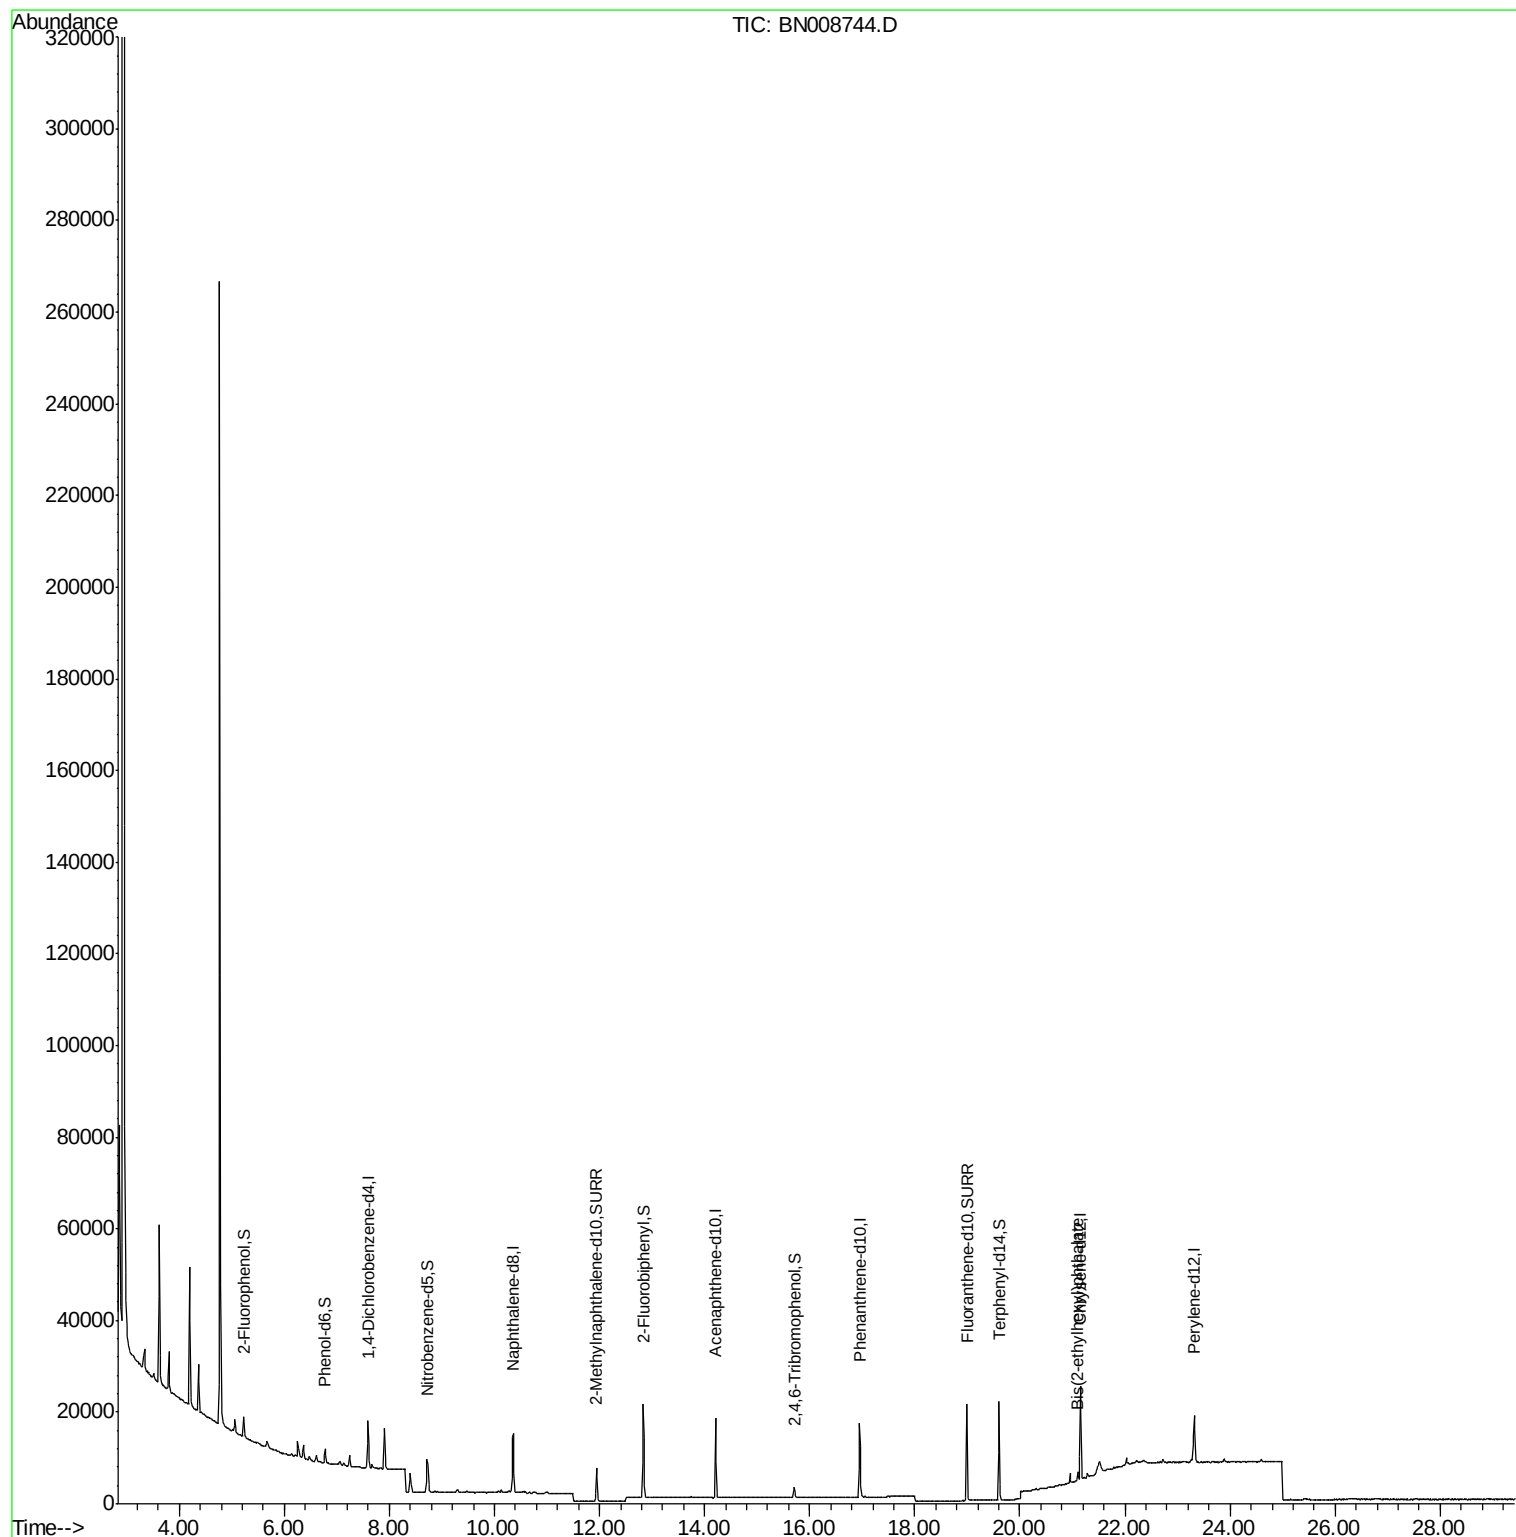




#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.60 min Scan# 592
Delta R.T. 0.00 min
Lab File: BN008744.D
Acq: 25 Nov 2019 19:28

Instrument :
BNA_N
ClientSampleId :
PB124746BL

Tot Ion:152 Resp: 5054
Ion Ratio Lower Upper
152 100
150 148.7 124.0 186.0
115 58.5 49.8 74.8

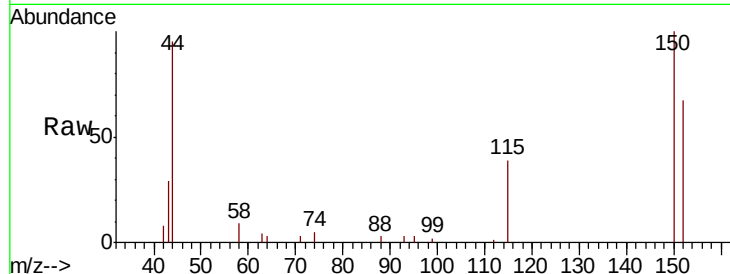


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

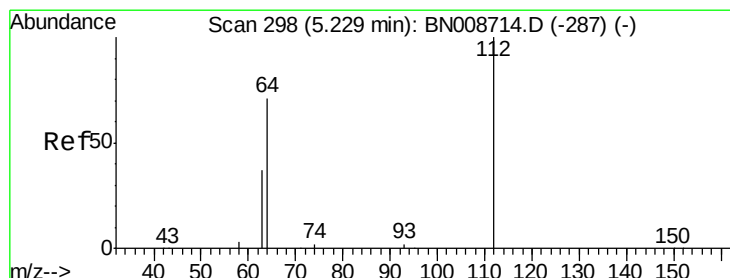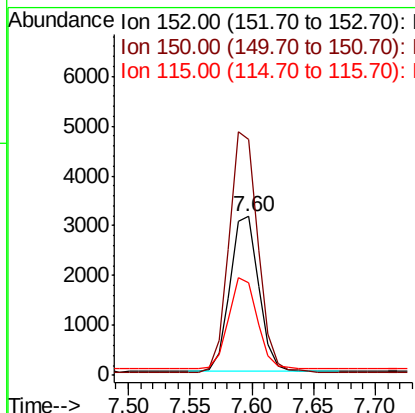



#4


2-Fluorophenol
Concen: 0.243 ng
RT: 5.23 min Scan# 298
Delta R.T. 0.00 min
Lab File: BN008744.D
Acq: 25 Nov 2019 19:28

Tgt Ion:112 Resp: 3211
Ion Ratio Lower Upper
112 100
64 71.2 57.1 85.7
63 36.0 29.7 44.5

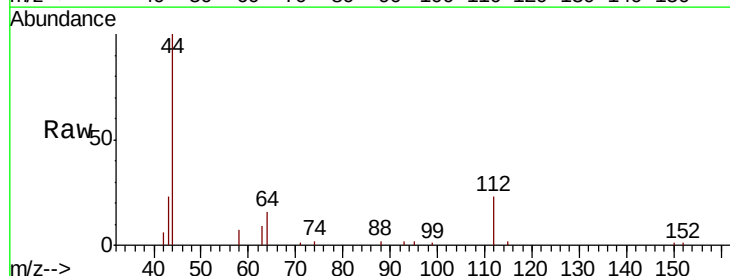

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BNC
Ion 63.00 (62.70 to 63.70): BNC

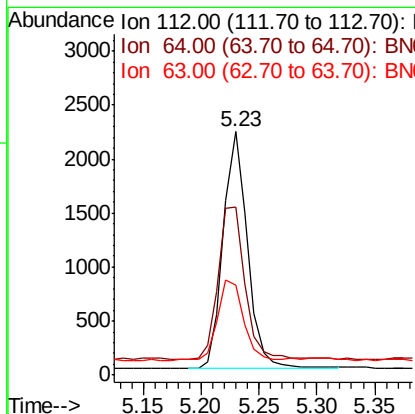



#5

Phenol-d6

Concen: 0.180 ng

RT: 6.78 min Scan# 491

Delta R.T. 0.00 min

Lab File: BN008744.D

Acq: 25 Nov 2019 19:28

Instrument :

BNA_N

ClientSampleId :

PB124746BL


Tot Ion: 99 Resp: 3013

Ion Ratio Lower Upper

99 100

42 23.9 19.4 29.2




71 37.2 27.5 41.3

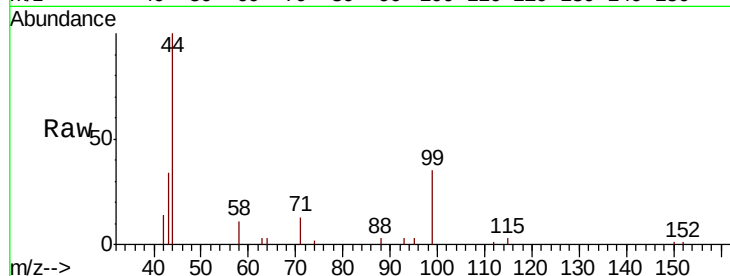

Abundance Ion 99.00 (98.70 to 99.70): BN008714.D (-481) (-)

Ion 42.00 (41.70 to 42.70): BN008714.D (-481) (-)

Ion 71.00 (70.70 to 71.70): BN008714.D (-481) (-)

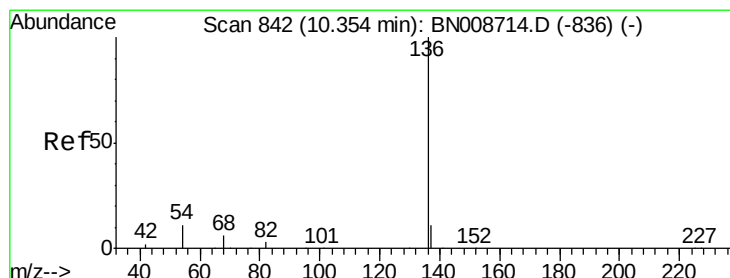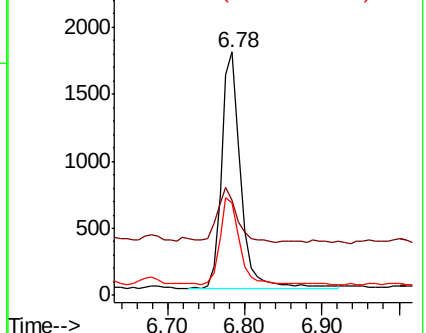

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.35 min Scan# 842

Delta R.T. 0.00 min

Lab File: BN008744.D

Acq: 25 Nov 2019 19:28

Tgt Ion: 136 Resp: 18126


Ion Ratio Lower Upper

136 100

137 11.5 9.3 13.9

54 8.9 9.4 14.2#

68 5.8 5.8 8.6


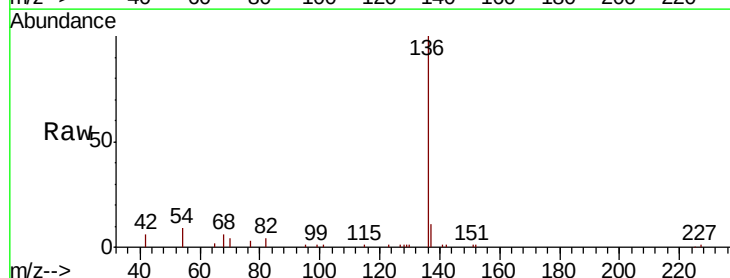



Abundance Ion 136.00 (135.70 to 136.70): BN008714.D (-836) (-)

Ion 137.00 (136.70 to 137.70): BN008714.D (-836) (-)

Ion 54.00 (53.70 to 54.70): BN008714.D (-836) (-)

Ion 68.00 (67.70 to 68.70): BN008714.D (-836) (-)

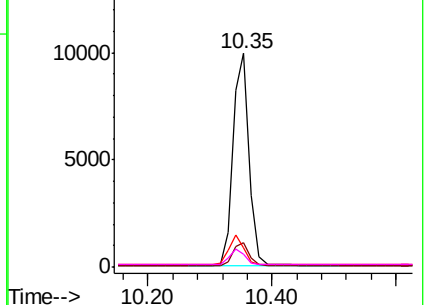

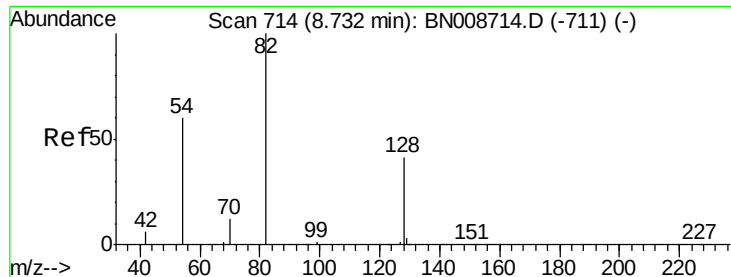

#8

Nitrobenzene-d5

Concen: 0.365 ng

RT: 8.72 min Scan# 713

Delta R.T. -0.01 min

Lab File: BN008744.D

Acq: 25 Nov 2019 19:28

Instrument :

BNA_N

ClientSampleId :

PB124746BL


Tot Ion: 82 Resp: 5945

Ion Ratio Lower Upper

82 100

128 34.0 34.6 52.0#

54 75.2 50.2 75.4



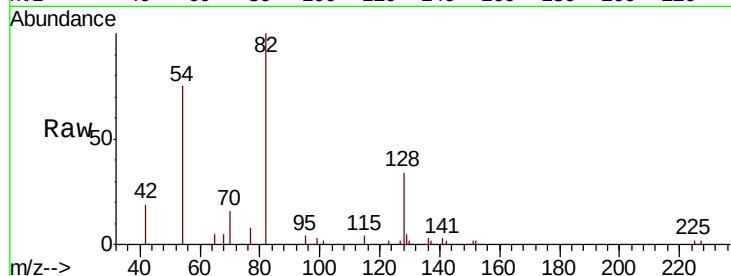


Abundance Ion 82.00 (81.70 to 82.70): BN008714.D (-711) (-)

Ion 128.00 (127.70 to 128.70): BN008714.D (-711) (-)

Ion 54.00 (53.70 to 54.70): BN008714.D (-711) (-)

Time-->

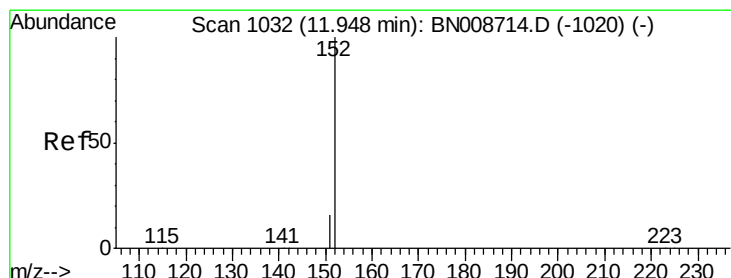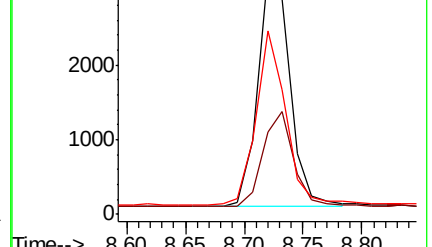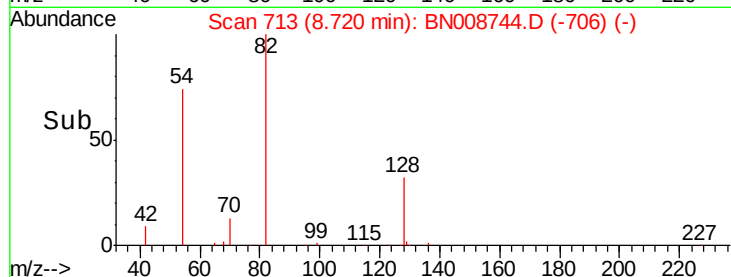

#11

2-Methylnaphthalene-d10

Concen: 0.356 ng

RT: 11.94 min Scan# 1031

Delta R.T. -0.00 min

Lab File: BN008744.D


Acq: 25 Nov 2019 19:28

Tgt Ion: 152 Resp: 10182

Ion Ratio Lower Upper

152 100



151 19.0 15.2 22.8

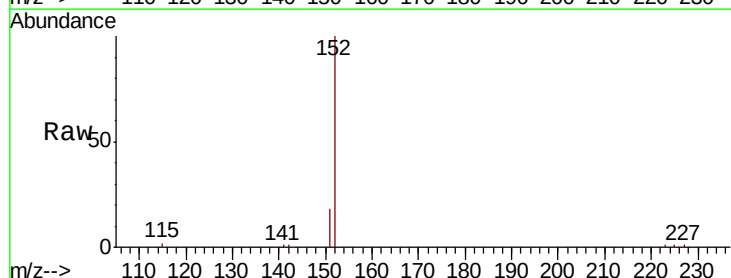


Abundance Ion 152.00 (151.70 to 152.70): BN008714.D (-1020) (-)

Ion 151.00 (150.70 to 151.70): BN008714.D (-1020) (-)

Time-->

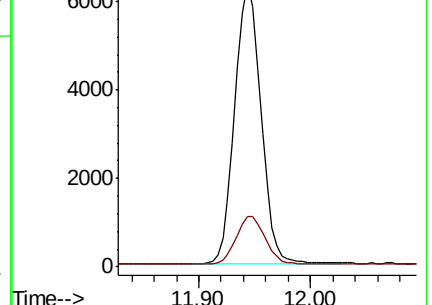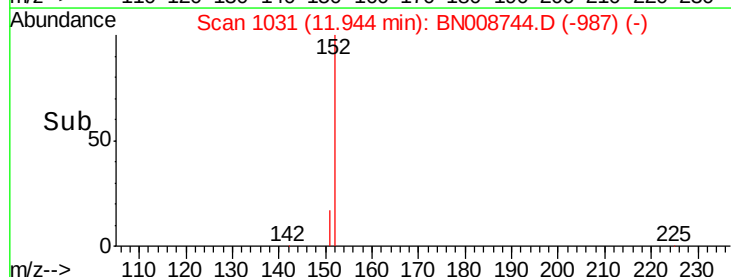


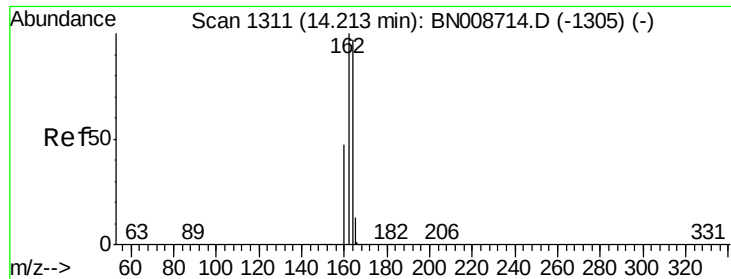




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.21 min Scan# 1311
Delta R.T. 0.00 min
Lab File: BN008744.D
Acq: 25 Nov 2019 19:28

Instrument :
BNA_N
ClientSampleId :
PB124746BL

Tot Ion:164 Resp: 10056
Ion Ratio Lower Upper
164 100
162 100.1 82.2 123.4
160 46.6 38.7 58.1

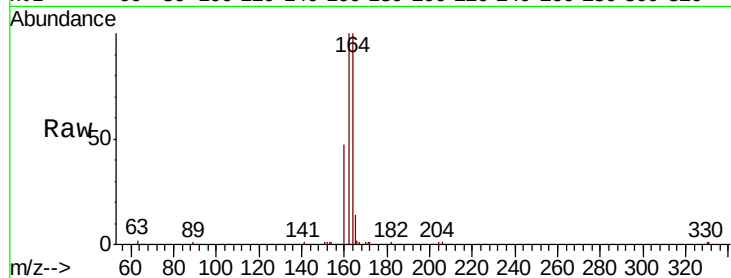


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

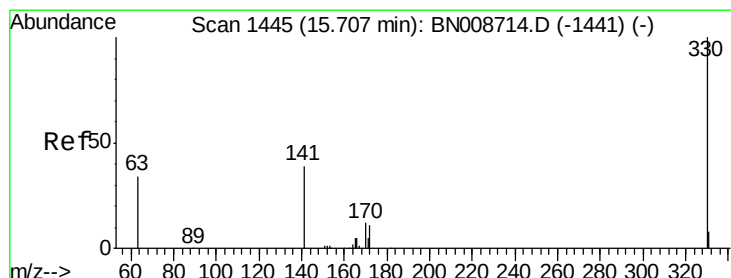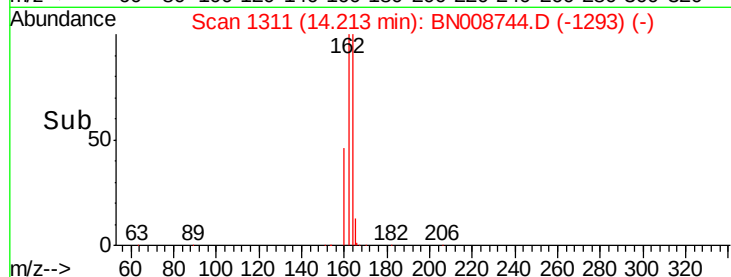
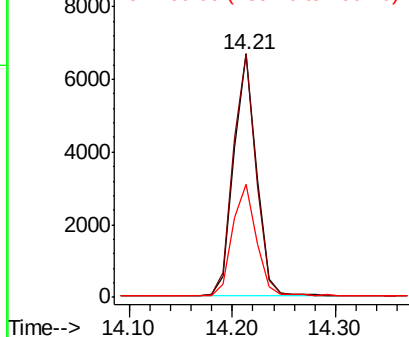



#14
2,4,6-Tribromophenol
Concen: 0.396 ng
RT: 15.71 min Scan# 1445
Delta R.T. 0.00 min
Lab File: BN008744.D
Acq: 25 Nov 2019 19:28

Tgt Ion:330 Resp: 1853
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 35.7 29.5 44.3

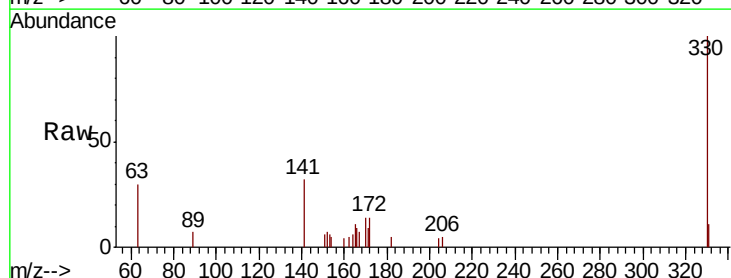

Abundance Ion 330.00 (329.70 to 330.70): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E



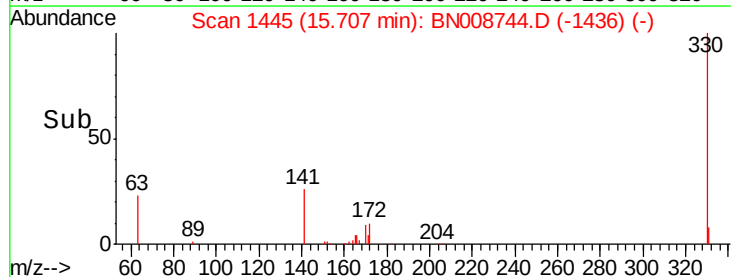
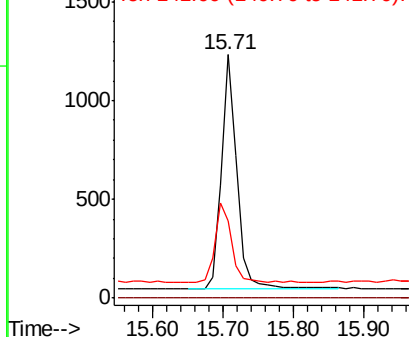


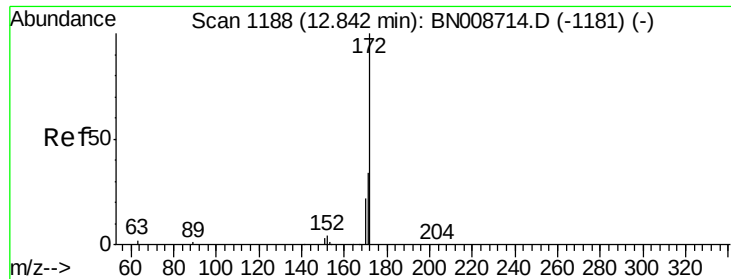

#15
2-Fluorobiphenyl
Concen: 0.449 ng
RT: 12.83 min Scan# 1187
Delta R.T. -0.01 min
Lab File: BN008744.D
Acq: 25 Nov 2019 19:28




Instrument :
BNA_N
ClientSampleId :
PB124746BL


Tot Ion:172 Resp: 17631
Ion Ratio Lower Upper
172 100
171 35.2 27.3 40.9
170 23.7 17.8 26.6

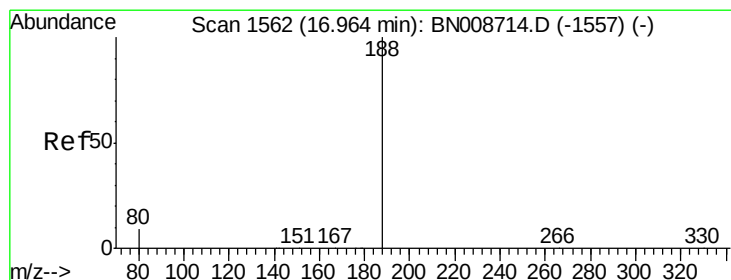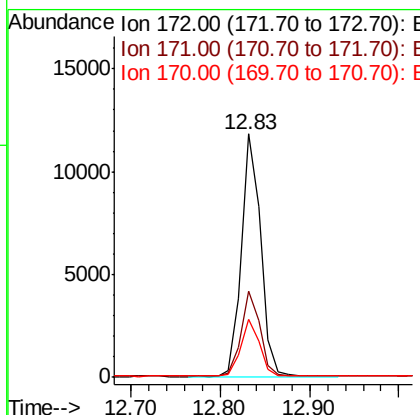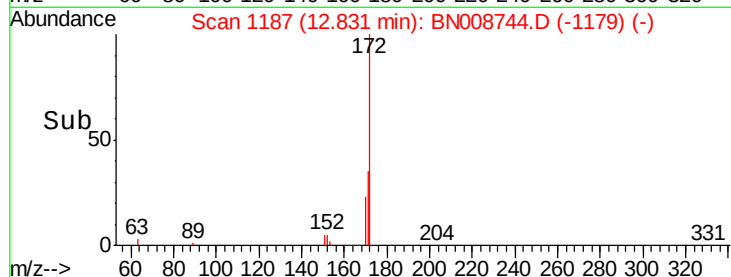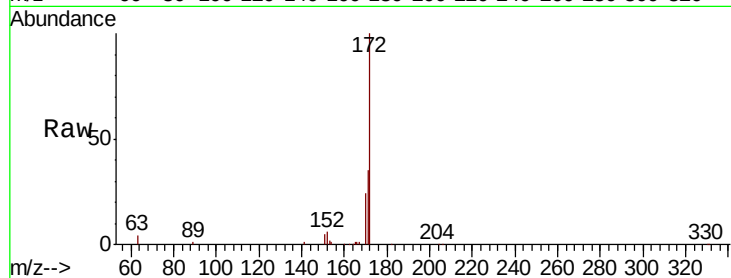

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.95 min Scan# 1561
Delta R.T. -0.01 min
Lab File: BN008744.D
Acq: 25 Nov 2019 19:28

Tgt Ion:188 Resp: 21112
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.0 7.4 11.0#


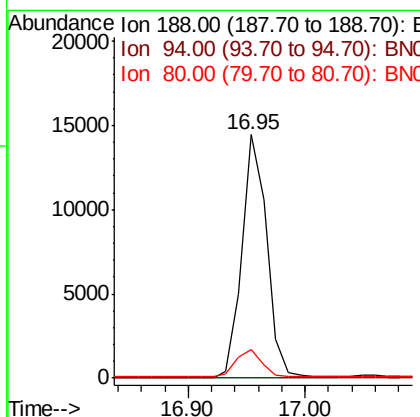
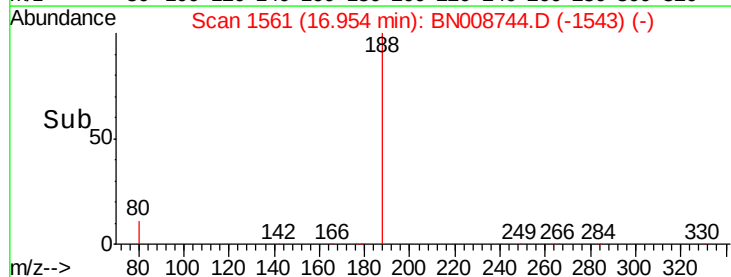
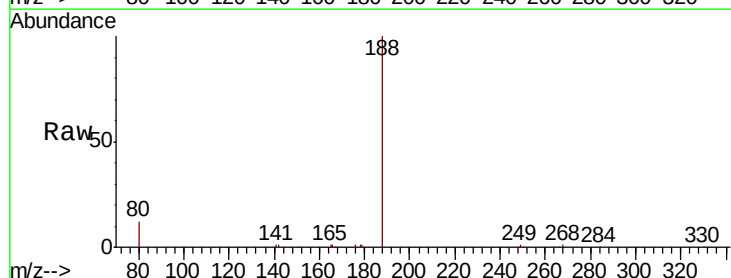


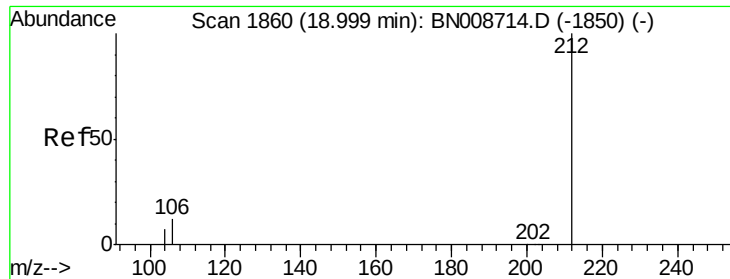

#25
 Fluoranthene-d10
 Concen: 0.386 ng
 RT: 18.99 min Scan# 1859
 Delta R.T. -0.00 min
 Lab File: BN008744.D
 Acq: 25 Nov 2019 19:28




Instrument :
 BNA_N
 ClientSampleId :
 PB124746BL


Tot Ion:212 Resp: 23973
 Ion Ratio Lower Upper
 212 100
 106 13.4 10.6 15.8
 104 7.4 6.0 9.0

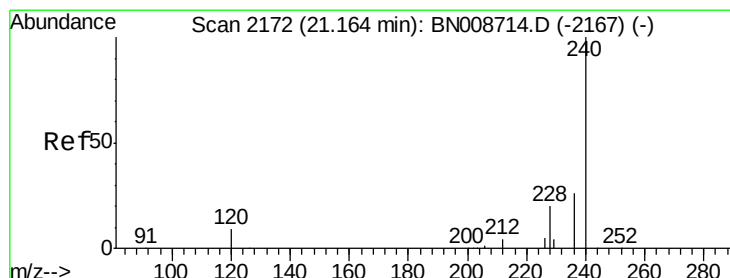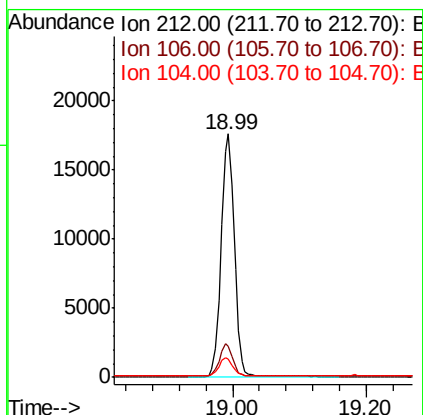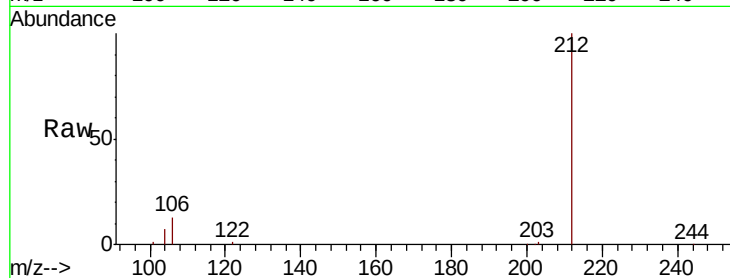

#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.15 min Scan# 2171
 Delta R.T. -0.01 min
 Lab File: BN008744.D
 Acq: 25 Nov 2019 19:28

Tgt Ion:240 Resp: 19130
 Ion Ratio Lower Upper
 240 100
 120 15.6 9.0 13.4#
 236 28.0 21.8 32.6

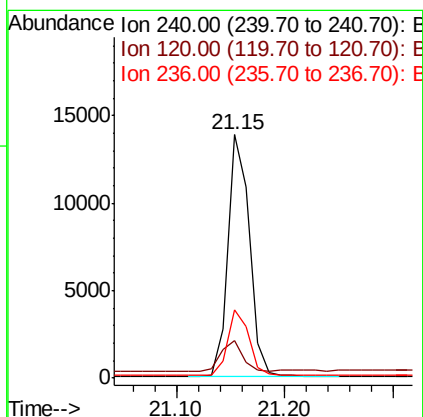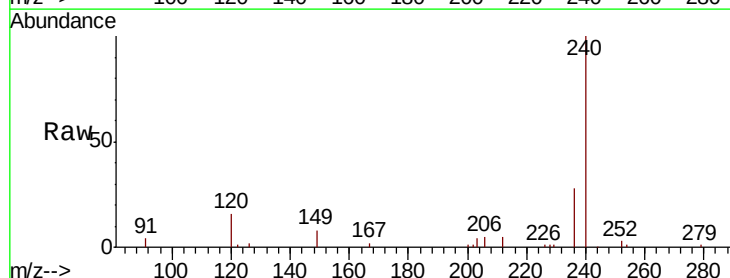



#29

Terphenyl-d14

Concen: 0.448 ng

RT: 19.60 min Scan# 1982

Delta R.T. -0.00 min

Lab File: BN008744.D

Acq: 25 Nov 2019 19:28

Instrument :

BNA_N

ClientSampleId :

PB124746BL





Tot Ion:244 Resp: 20608

Ion Ratio Lower Upper

244 100

212 7.7 6.6 9.8

122 12.9 10.1 15.1

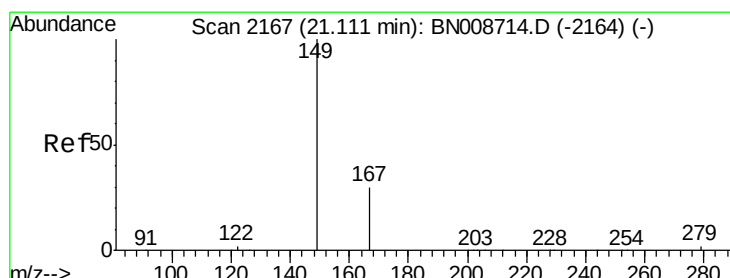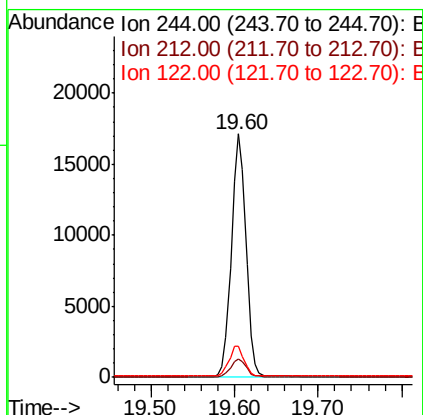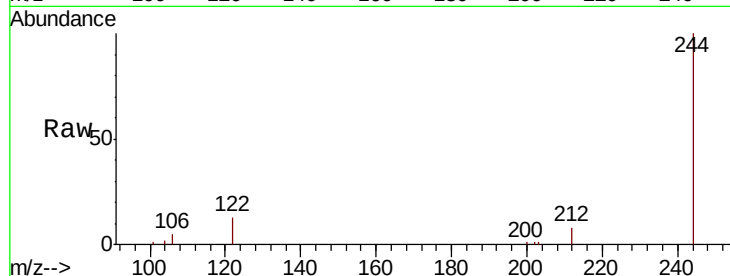

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.040 ng

RT: 21.10 min Scan# 2166

Delta R.T. -0.01 min

Lab File: BN008744.D

Acq: 25 Nov 2019 19:28




Tgt Ion:149 Resp: 1833




Ion Ratio Lower Upper

149 100

167 25.6 23.5 35.3

279 3.7 3.4 5.0

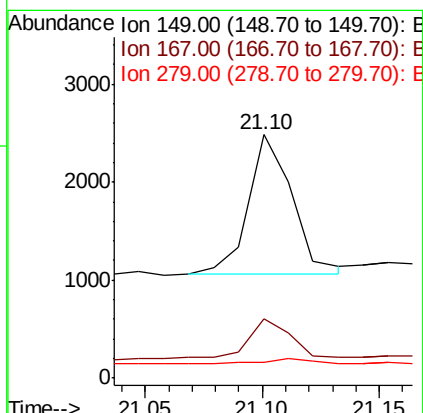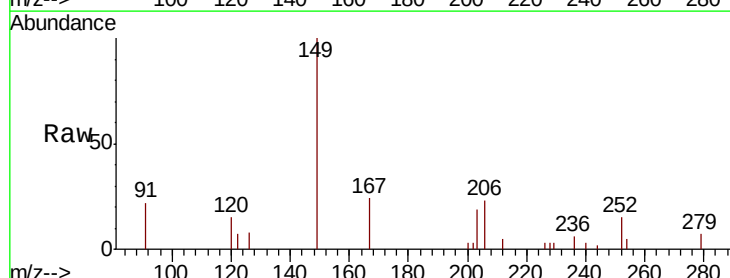

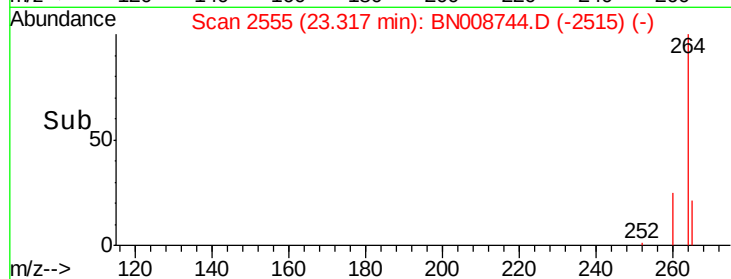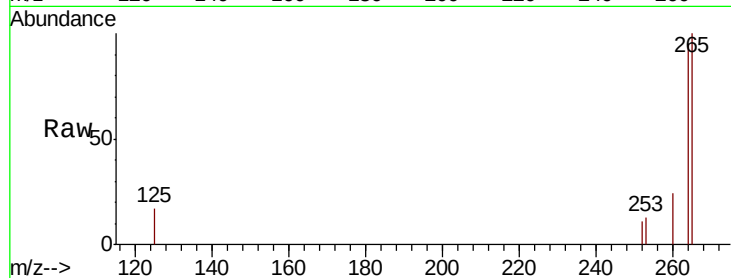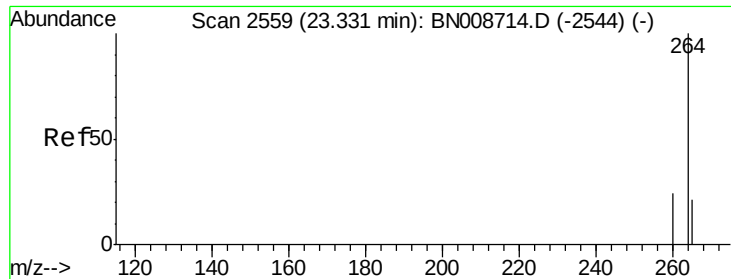

#34

Pervlene-d12

Concen: 0.400 ng

RT: 23.32 min Scan# 2555

Delta R.T. -0.01 min

Lab File: BN008744.D

Acq: 25 Nov 2019 19:28

Instrument :

BNA_N

ClientSampleId :

PB124746BL

Tot Ion:264 Resp: 13121

Ion Ratio Lower Upper

264 100

260 25.8 19.6 29.4

265 105.5 61.8 92.6

