


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112519\
 Data File : BN008740.D
 Acq On : 25 Nov 2019 16:27
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN112219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 25 10:49:40 2019

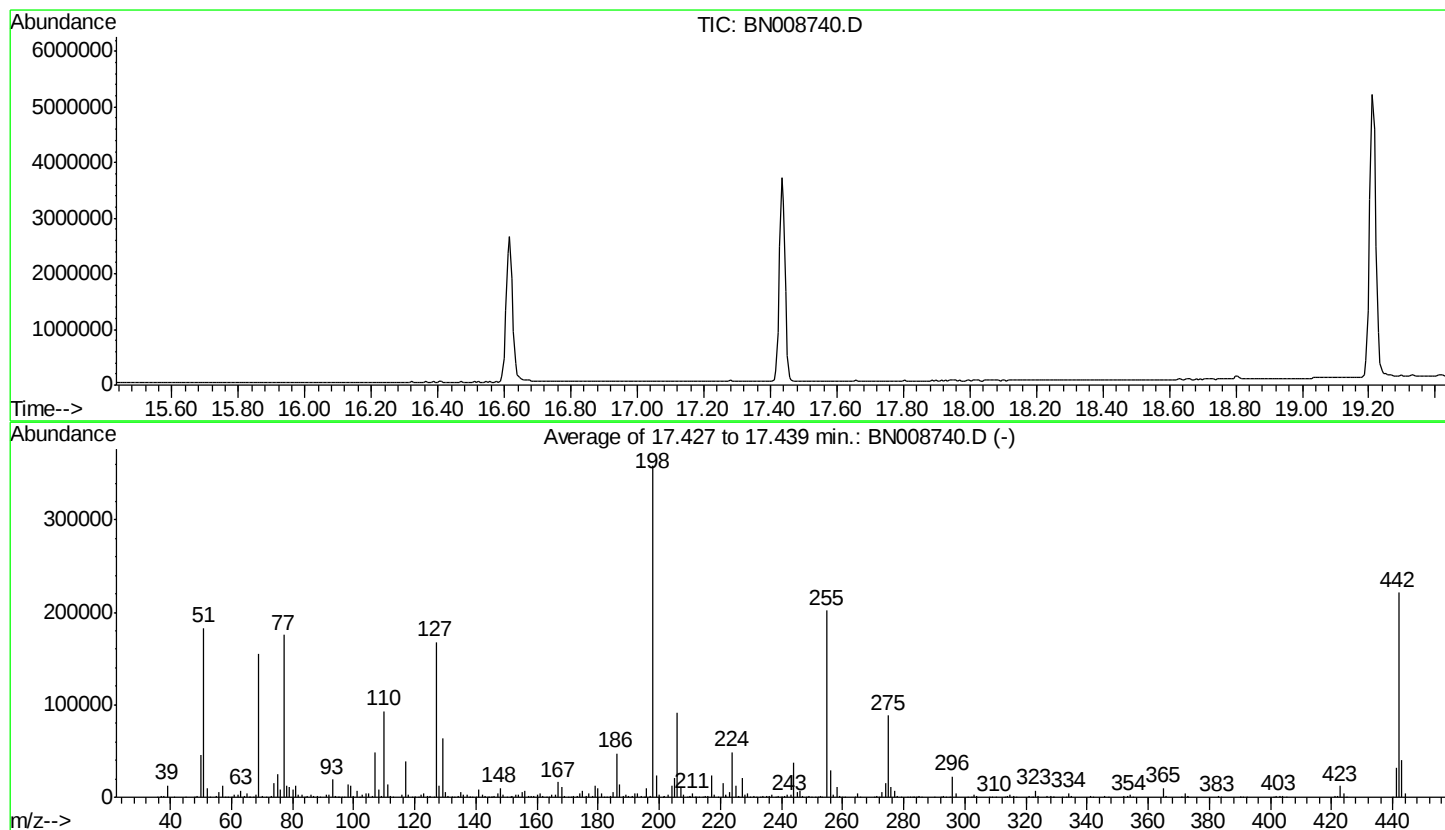

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.0	183136	PASS
68	69	0.00	2	2.0	3050	PASS
69	198	0.00	100	43.3	155434	PASS
70	69	0.00	2	0.6	860	PASS
127	198	10	80	46.9	168149	PASS
197	198	0.00	2	0.6	2117	PASS
198	198	100	100	100.0	358741	PASS
199	198	5	9	6.6	23792	PASS
275	198	10	60	24.7	88453	PASS
365	198	1	100	2.8	10140	PASS
441	198	0.01	100	9.1	32522	PASS
442	198	50	100	61.7	221477	PASS
443	442	15	24	17.9	39634	PASS