

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112622\
 Data File : BN022884.D
 Acq On : 26 Nov 2022 16:52
 Operator : CG/JU
 Sample : PB149029BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK029

Quant Time: Nov 28 03:48:45 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 28 03:16:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.070	152	6937	0.400	ng/ul	0.00
4) Naphthalene-d8	10.892	136	19923	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.710	164	11386	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.453	188	23798	0.400	ng/ul	0.00
17) Chrysene-d12	21.639	240	13406	0.400	ng/ul	0.00
23) Perylene-d12	24.130	264	11198	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.412	96	57324	6.886	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.476	152	10740	0.354	ng/ul	0.00
18) Fluoranthene-d10	19.481	212	20509	0.414	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.705	166	4124	0.082	ng/ul#	12
20) Pyrene	19.843	202	3365	0.050	ng/ul#	1
26) Benzo(a)pyrene	23.972	252	5553	0.128	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112622\
Data File : BN022884.D
Acq On : 26 Nov 2022 16:52
Operator : CG/JU
Sample : PB149029BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK029

Quant Time: Nov 28 03:48:45 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 28 03:16:56 2022
Response via : Initial Calibration




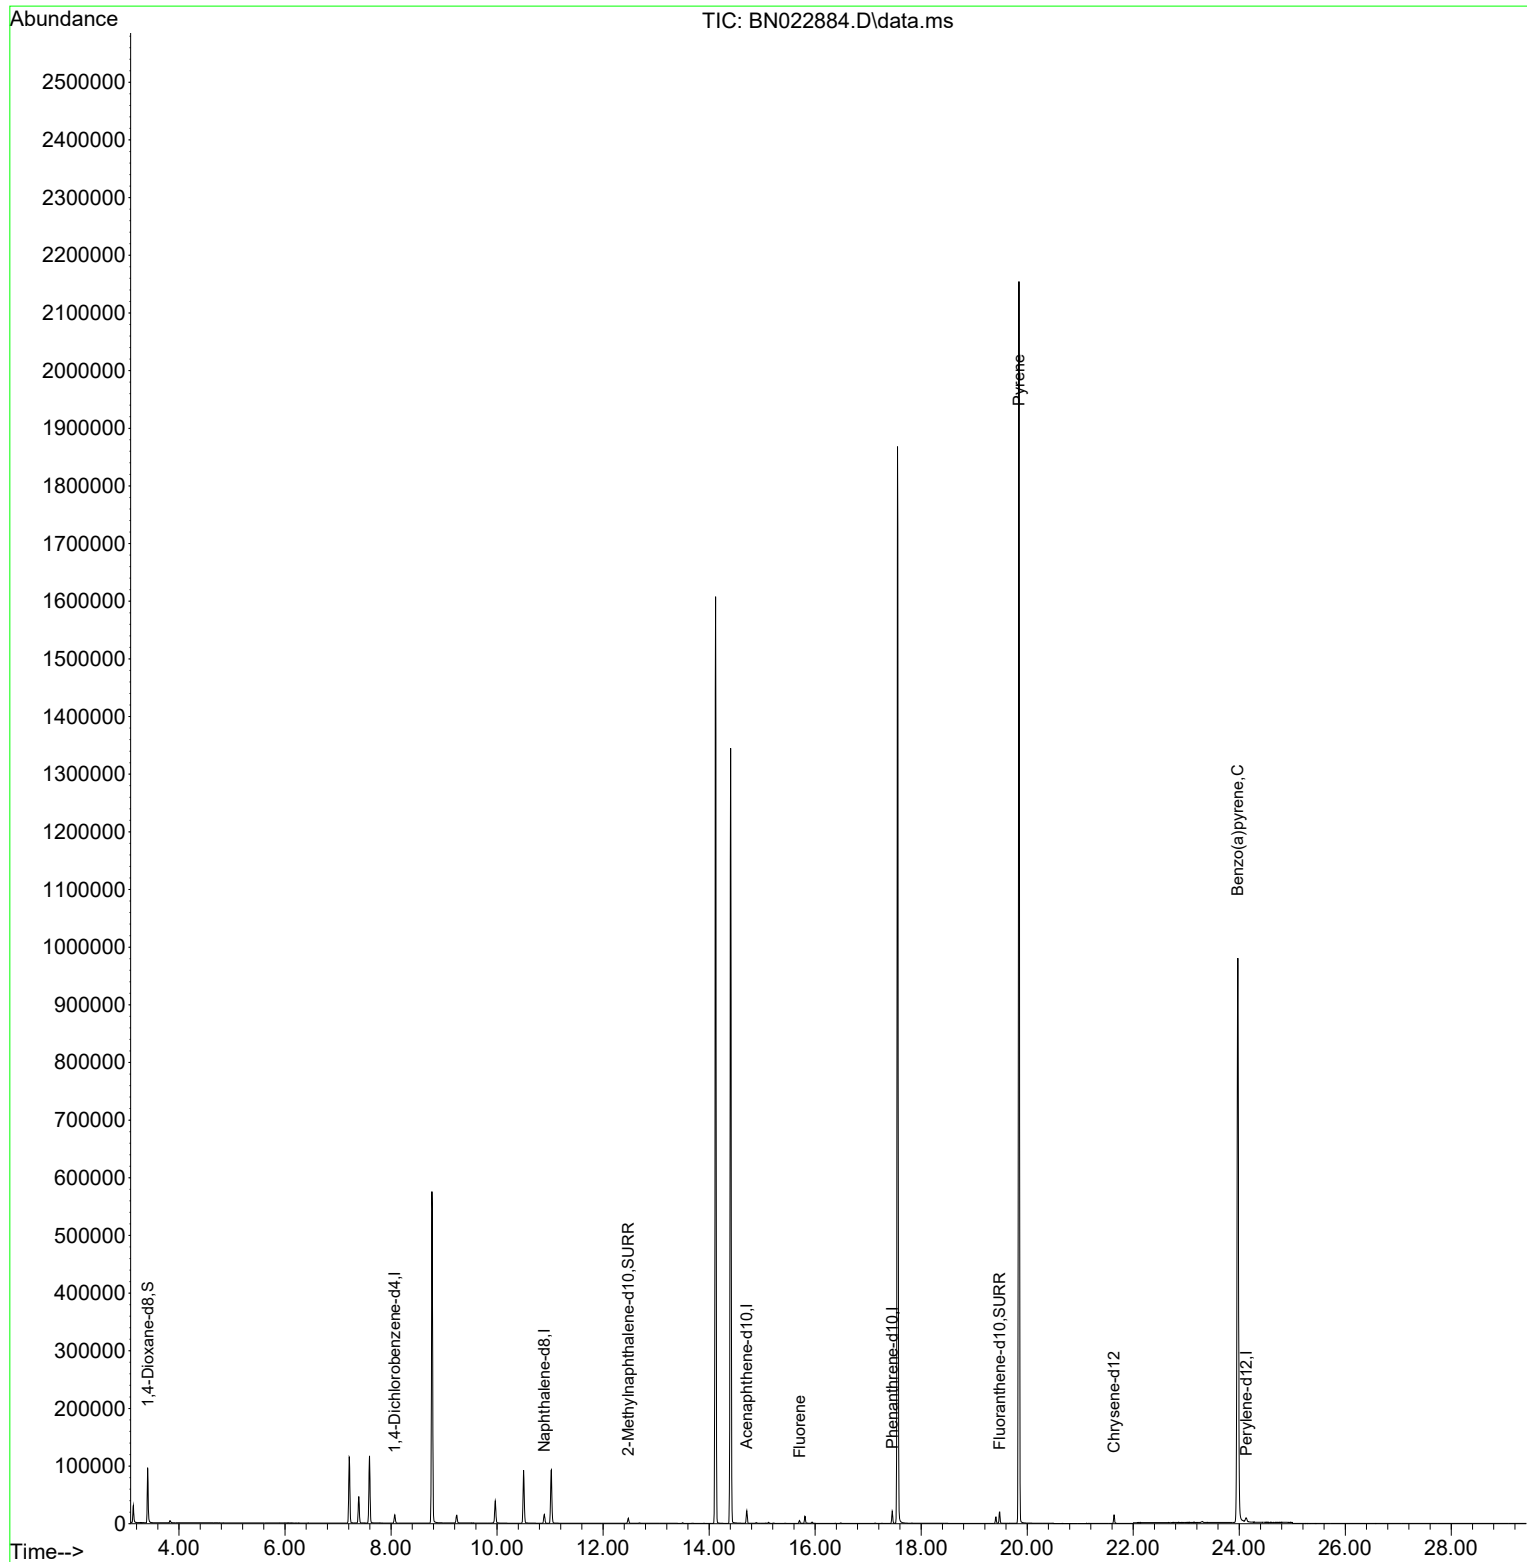


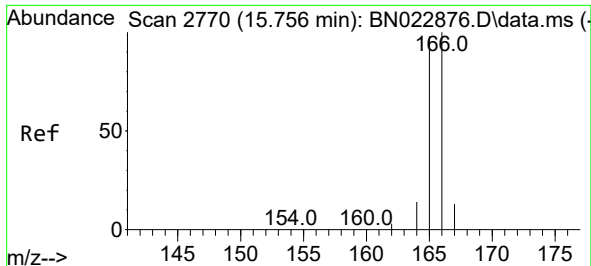

#12
Fluorene
Concen: 0.082 ng/ul
RT: 15.705 min Scan# 21
Delta R.T. -0.051 min
Lab File: BN022884.D
Acq: 26 Nov 2022 16:52




Instrument :
BNA_N
ClientSampleId :
SBLK029


Tgt Ion:166 Resp: 4124
Ion Ratio Lower Upper
166 100
165 6.9 78.7 118.1#
167 34.6 10.8 16.2#

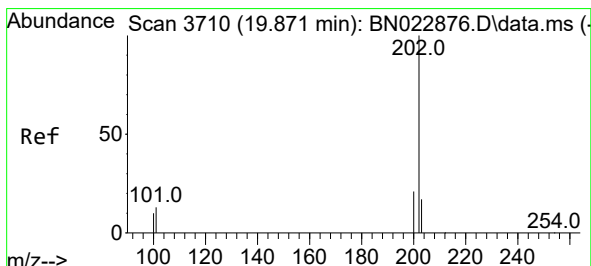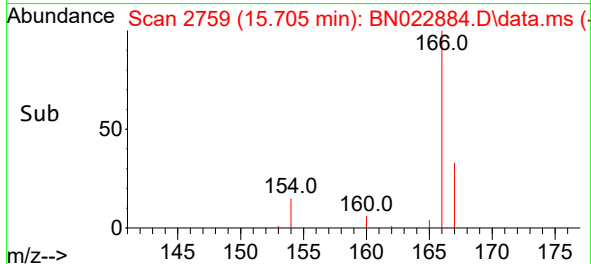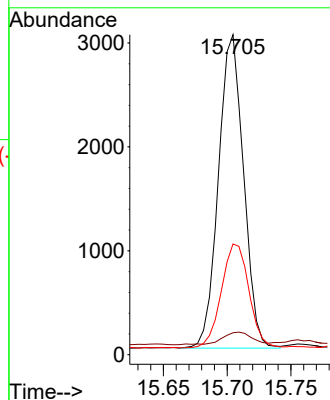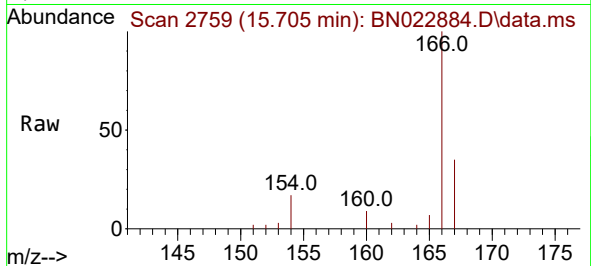

#20
Pyrene
Concen: 0.050 ng/ul
RT: 19.843 min Scan# 3704
Delta R.T. -0.028 min
Lab File: BN022884.D
Acq: 26 Nov 2022 16:52


Tgt Ion:202 Resp: 3365
Ion Ratio Lower Upper
202 100
101 164.4 10.6 16.0#
100 1256.2 8.2 12.4#

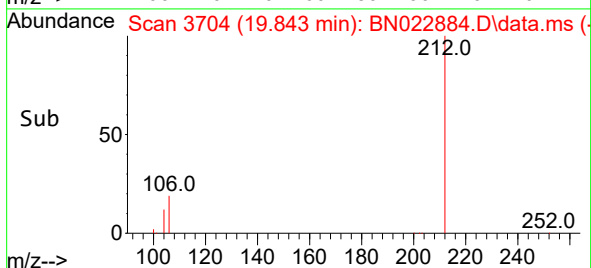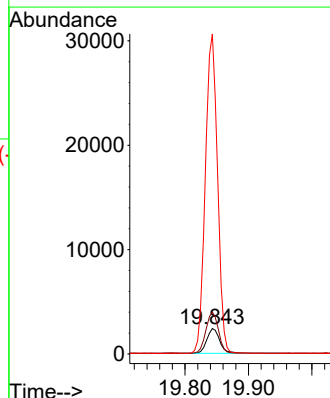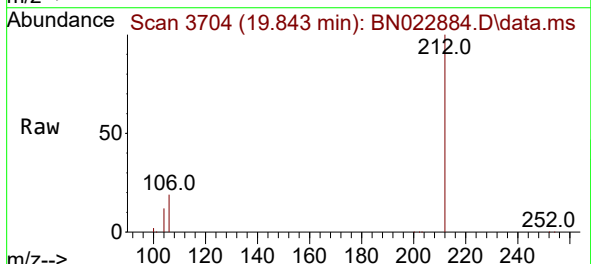

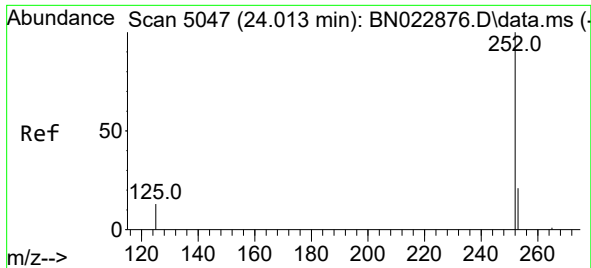

#26
Benzo(a)pyrene
Concen: 0.128 ng/ul
RT: 23.972 min Scan# 50
Delta R.T. -0.041 min
Lab File: BN022884.D
Acq: 26 Nov 2022 16:52

Instrument :
BNA_N
ClientSampleId :
SBLK029

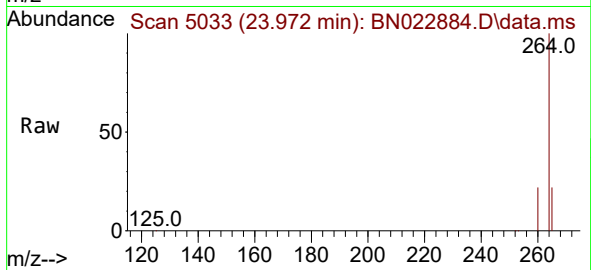

Tgt Ion:252 Resp: 5553
Ion Ratio Lower Upper
252 100
253 36.1 19.7 29.5#
125 32.5 13.7 20.5#

