

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112622\
 Data File : BN022894.D
 Acq On : 26 Nov 2022 22:59
 Operator : CG/JU
 Sample : N5591-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C9806

Quant Time: Nov 28 03:50:06 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 28 03:16:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.069	152	8501	0.400	ng/ul	0.00
4) Naphthalene-d8	10.892	136	24073	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.710	164	13095	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.453	188	26298	0.400	ng/ul	0.00
17) Chrysene-d12	21.636	240	13899	0.400	ng/ul	0.00
23) Perylene-d12	24.124	264	12066	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.412	96	44269	4.339	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.476	152	9896	0.270	ng/ul	0.00
18) Fluoranthene-d10	19.476	212	17731	0.345	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.450	88	1584	0.149	ng/ul#	81
20) Pyrene	19.843	202	2867	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.966	252	4510	0.097	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112622\
Data File : BN022894.D
Acq On : 26 Nov 2022 22:59
Operator : CG/JU
Sample : N5591-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C9806

Quant Time: Nov 28 03:50:06 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 28 03:16:56 2022
Response via : Initial Calibration




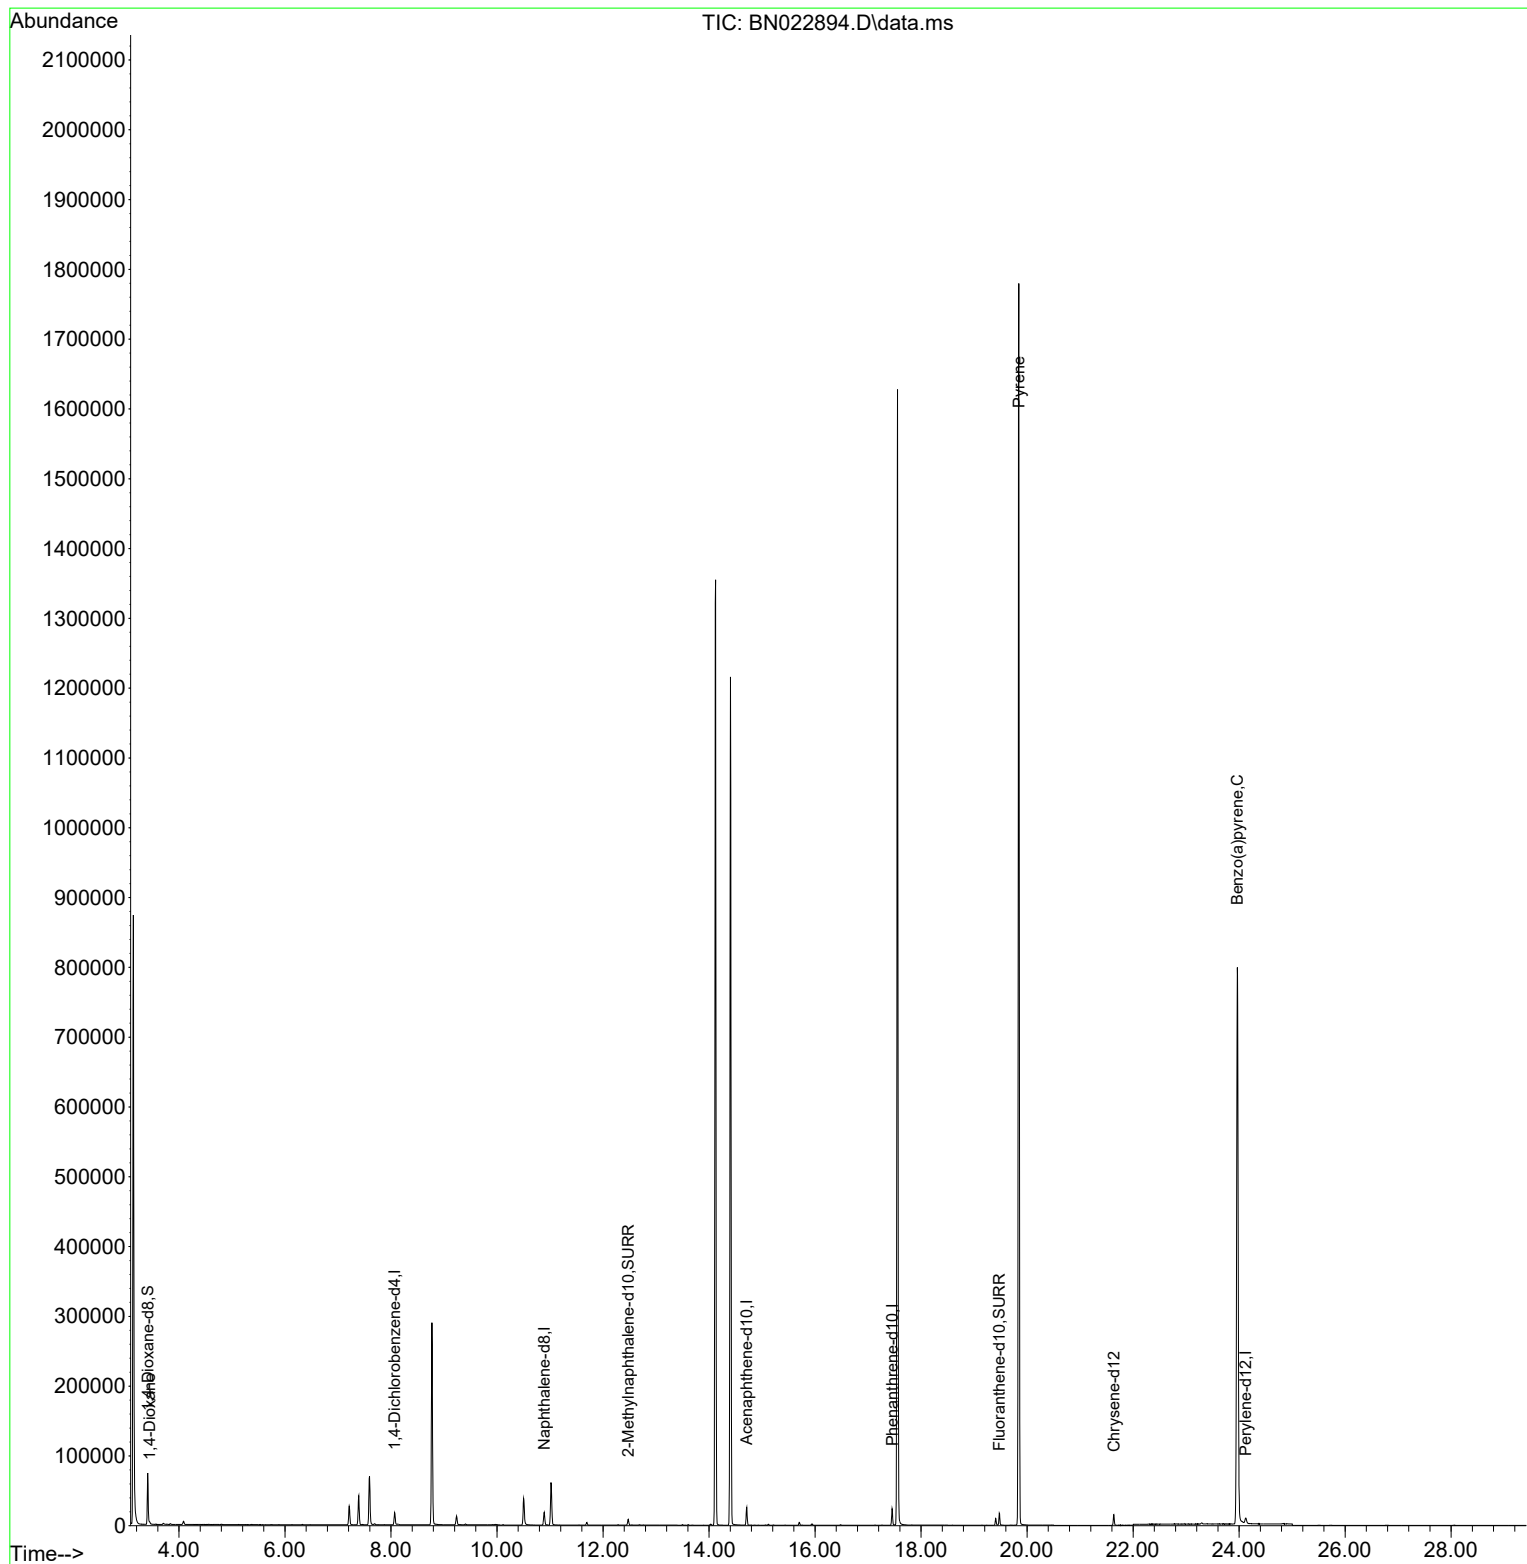


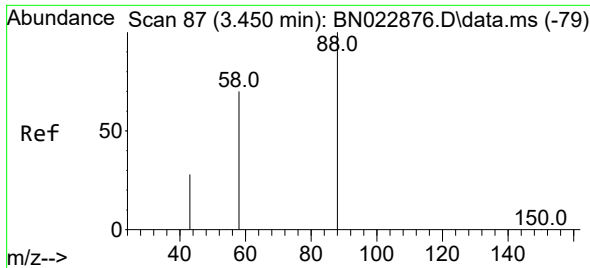

#2
1,4-Dioxane
Concen: 0.149 ng/ul
RT: 3.450 min Scan# 87
Delta R.T. -0.000 min
Lab File: BN022894.D
Acq: 26 Nov 2022 22:59




Instrument :
BNA_N
ClientSampleId :
C9806


Tgt Ion: 88 Resp: 1584
Ion Ratio Lower Upper
88 100
43 42.5 26.2 39.4#
58 44.3 47.6 71.4#

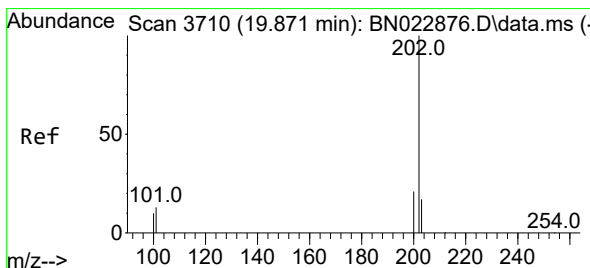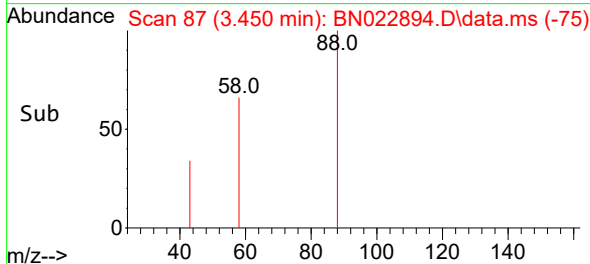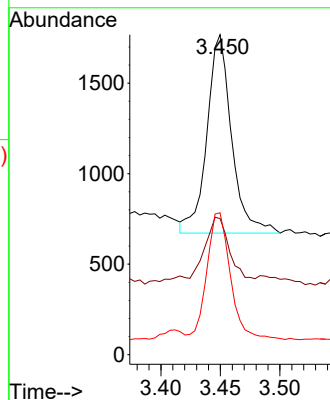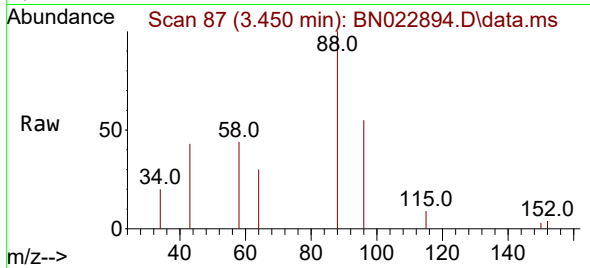

#20
Pyrene
Concen: 0.041 ng/ul
RT: 19.843 min Scan# 3704
Delta R.T. -0.028 min
Lab File: BN022894.D
Acq: 26 Nov 2022 22:59


Tgt Ion: 202 Resp: 2867
Ion Ratio Lower Upper
202 100
101 160.6 10.6 16.0#
100 1186.1 8.2 12.4#

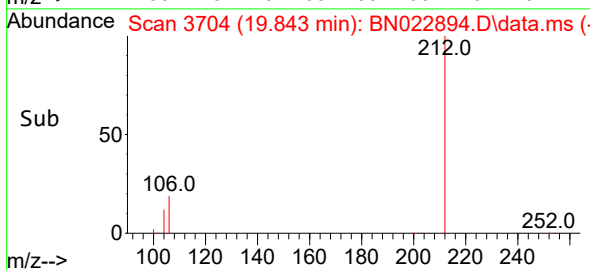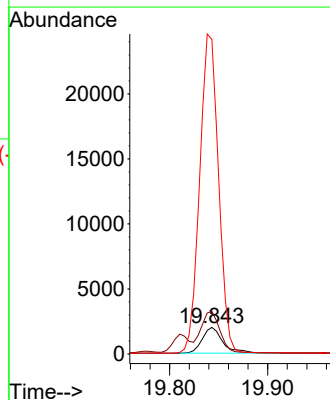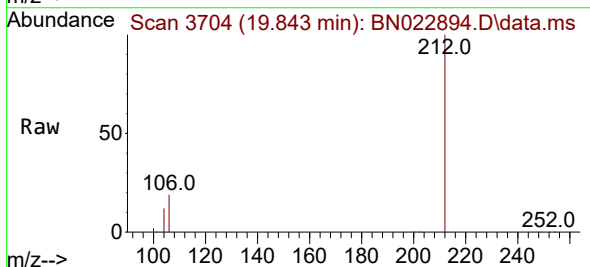

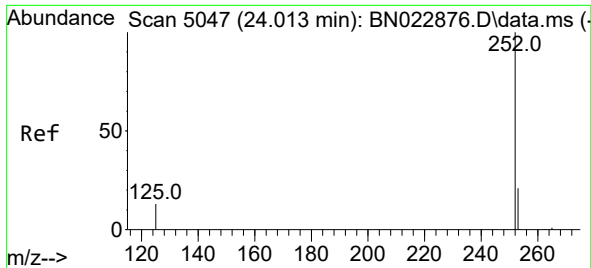

#26
Benzo(a)pyrene
Concen: 0.097 ng/ul
RT: 23.966 min Scan# 50
Delta R.T. -0.047 min
Lab File: BN022894.D
Acq: 26 Nov 2022 22:59

Instrument :
BNA_N
ClientSampleId :
C9806

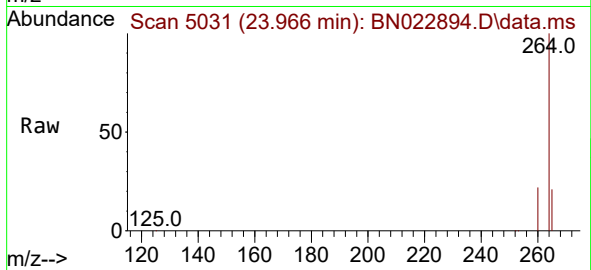

Tgt Ion:252 Resp: 4510
Ion Ratio Lower Upper
252 100
253 37.3 19.7 29.5#
125 35.5 13.7 20.5#

