

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112622\
 Data File : BN022897.D
 Acq On : 27 Nov 2022 00:49
 Operator : CG/JU
 Sample : N5591-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C9804

Quant Time: Nov 28 03:50:23 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 28 03:16:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.070	152	8453	0.400	ng/ul	0.00
4) Naphthalene-d8	10.892	136	24175	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.706	164	12927	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.454	188	25691	0.400	ng/ul	0.00
17) Chrysene-d12	21.634	240	14988	0.400	ng/ul	0.00
23) Perylene-d12	24.122	264	13156	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.412	96	48346	4.766	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.471	152	12242	0.332	ng/ul	0.00
18) Fluoranthene-d10	19.477	212	22445	0.405	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.450	88	1328	0.126	ng/ul#	75
20) Pyrene	19.844	202	3744	0.049	ng/ul#	1
26) Benzo(a)pyrene	23.967	252	6238	0.123	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112622\
Data File : BN022897.D
Acq On : 27 Nov 2022 00:49
Operator : CG/JU
Sample : N5591-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C9804

Quant Time: Nov 28 03:50:23 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 28 03:16:56 2022
Response via : Initial Calibration




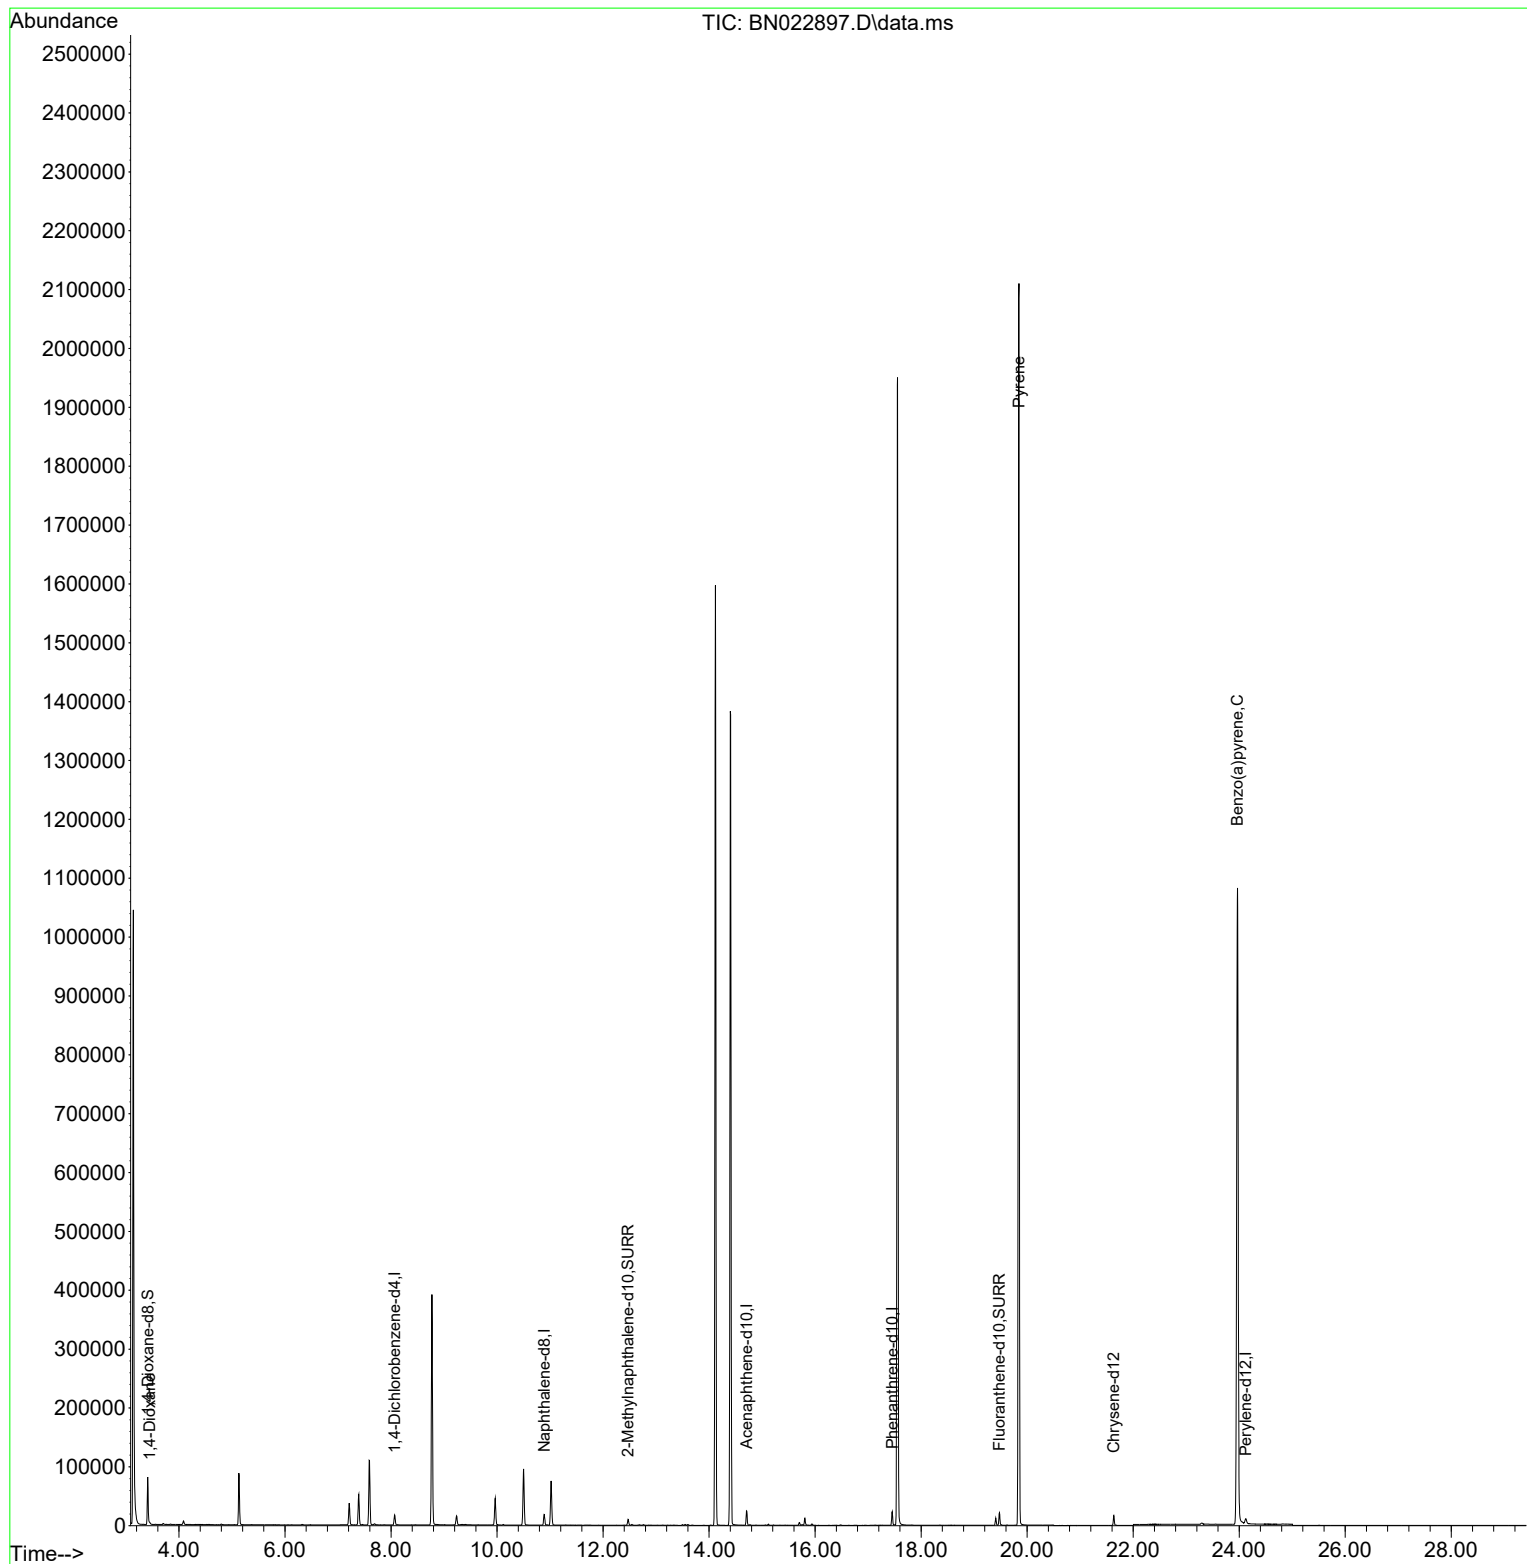


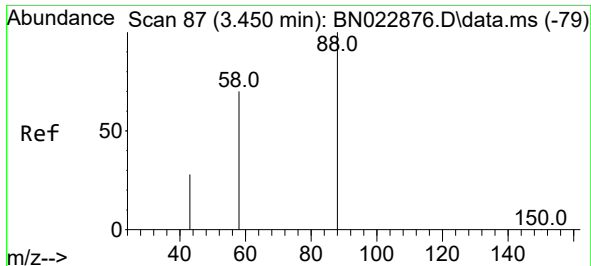

#2
 1,4-Dioxane
 Concen: 0.126 ng/ul
 RT: 3.450 min Scan# 81
 Delta R.T. 0.000 min
 Lab File: BN022897.D
 Acq: 27 Nov 2022 00:49




Instrument :
 BNA_N
 ClientSampleId :
 C9804


Tgt Ion: 88 Resp: 1328
 Ion Ratio Lower Upper
 88 100
 43 49.5 26.2 39.4#
 58 42.7 47.6 71.4#

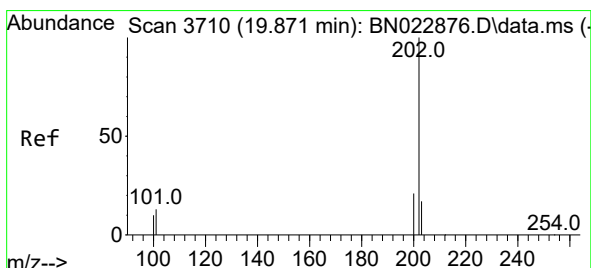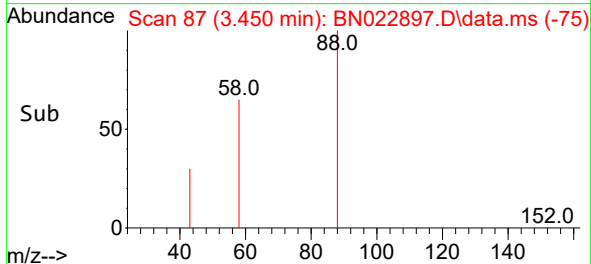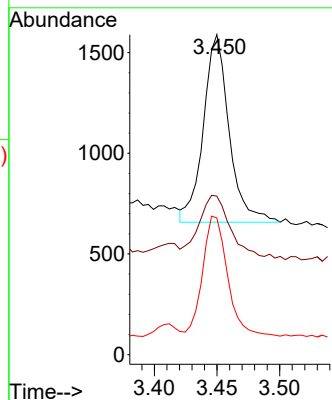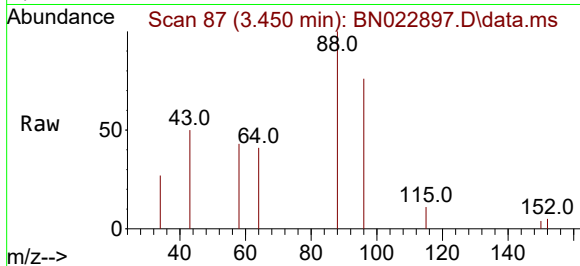

#20
 Pyrene
 Concen: 0.049 ng/ul
 RT: 19.844 min Scan# 3704
 Delta R.T. -0.027 min
 Lab File: BN022897.D
 Acq: 27 Nov 2022 00:49


Tgt Ion: 202 Resp: 3744
 Ion Ratio Lower Upper
 202 100
 101 153.6 10.6 16.0#
 100 1108.1 8.2 12.4#

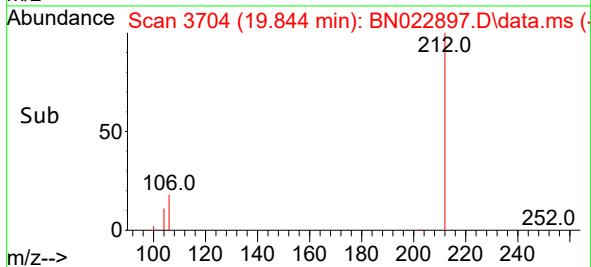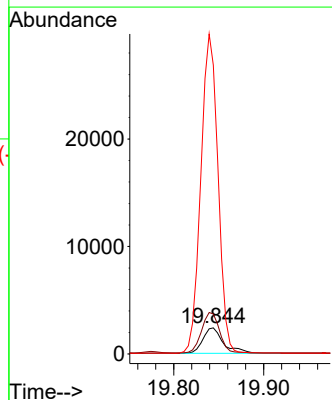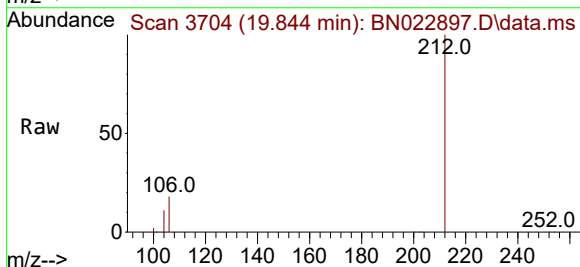

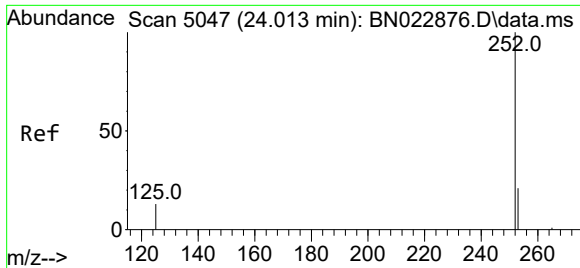

#26
Benzo(a)pyrene
Concen: 0.123 ng/ul
RT: 23.967 min Scan# 50
Delta R.T. -0.046 min
Lab File: BN022897.D
Acq: 27 Nov 2022 00:49

Instrument :
BNA_N
ClientSampleId :
C9804

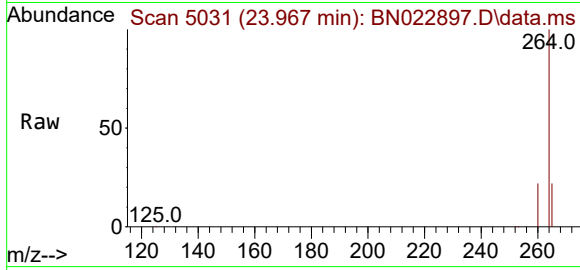

Tgt Ion:252 Resp: 6238
Ion Ratio Lower Upper
252 100
253 36.0 19.7 29.5#
125 32.8 13.7 20.5#

