

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112622\
 Data File : BN022899.D
 Acq On : 27 Nov 2022 02:03
 Operator : CG/JU
 Sample : N5591-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C9807

Quant Time: Nov 28 03:50:35 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 28 03:16:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.070	152	8141	0.400	ng/ul	0.00
4) Naphthalene-d8	10.887	136	23454	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.710	164	12818	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.453	188	25498	0.400	ng/ul	0.00
17) Chrysene-d12	21.633	240	14062	0.400	ng/ul	0.00
23) Perylene-d12	24.121	264	12374	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.412	96	46221	4.731	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.470	152	11567	0.324	ng/ul	0.00
18) Fluoranthene-d10	19.476	212	21589	0.416	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.450	88	1375	0.135	ng/ul#	80
20) Pyrene	19.843	202	3578	0.050	ng/ul#	1
26) Benzo(a)pyrene	23.963	252	5823	0.122	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112622\
Data File : BN022899.D
Acq On : 27 Nov 2022 02:03
Operator : CG/JU
Sample : N5591-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C9807

Quant Time: Nov 28 03:50:35 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 28 03:16:56 2022
Response via : Initial Calibration




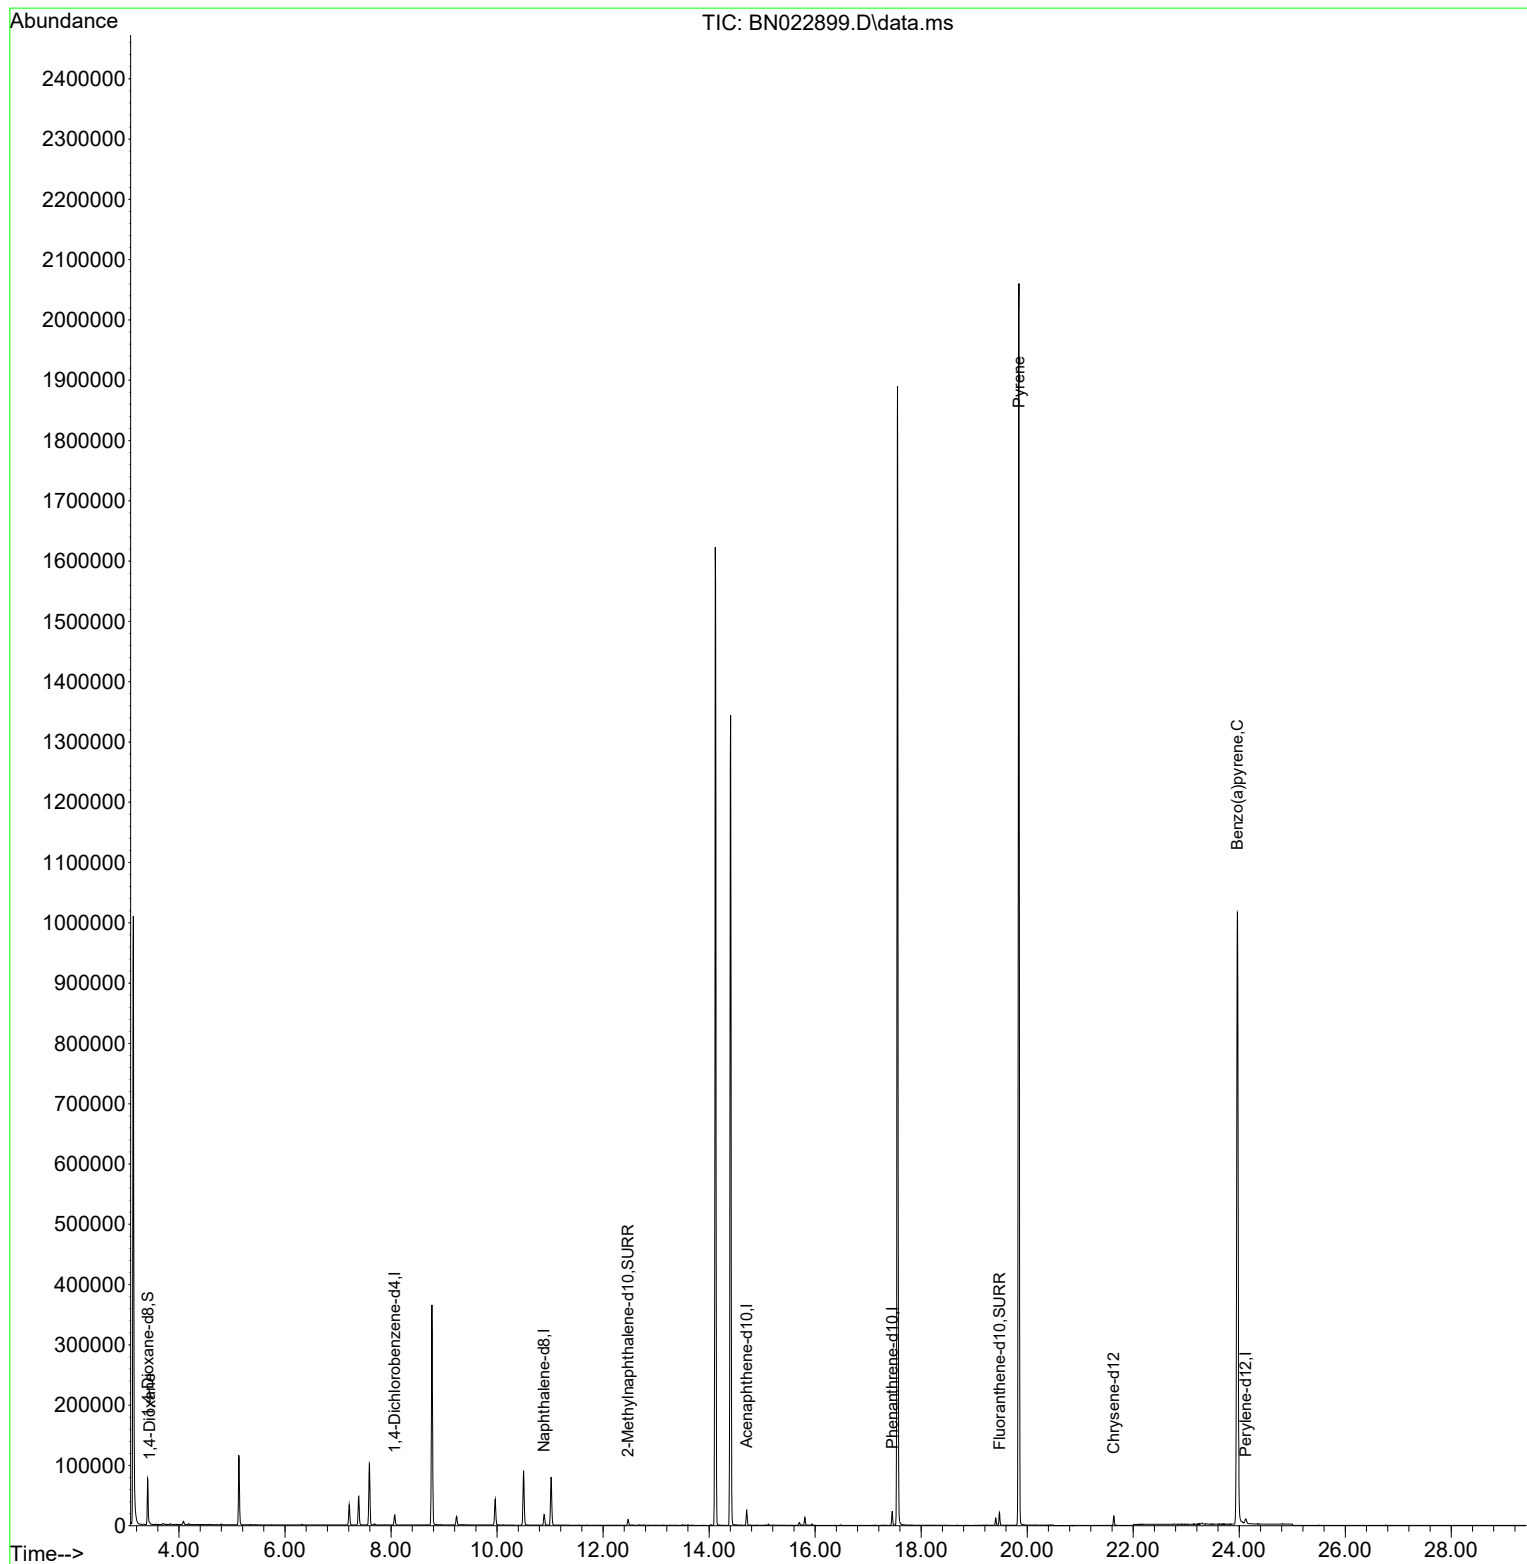


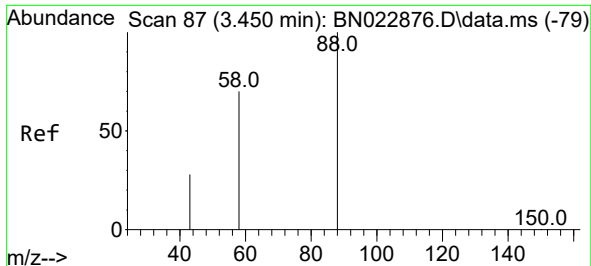

#2
 1,4-Dioxane
 Concen: 0.135 ng/ul
 RT: 3.450 min Scan# 81
 Delta R.T. -0.000 min
 Lab File: BN022899.D
 Acq: 27 Nov 2022 02:03




Instrument :
 BNA_N
 ClientSampleId :
 C9807


Tgt Ion: 88 Resp: 1375
 Ion Ratio Lower Upper
 88 100
 43 41.2 26.2 39.4#
 58 42.7 47.6 71.4#

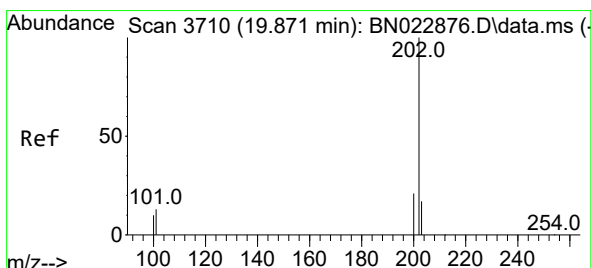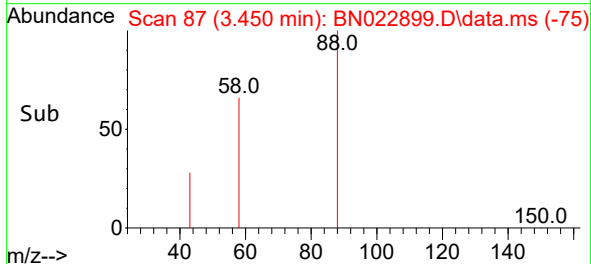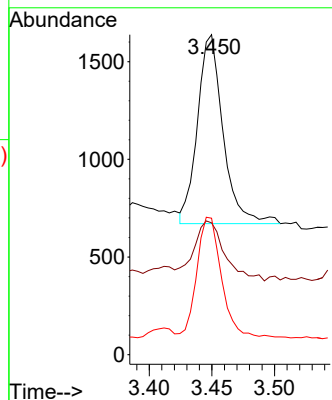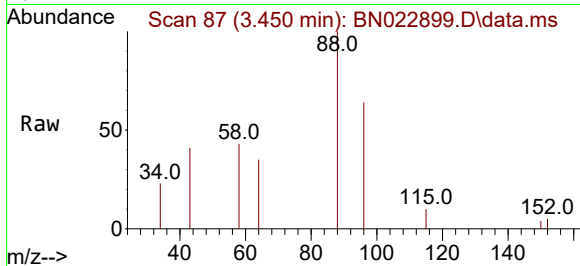

#20
 Pyrene
 Concen: 0.050 ng/ul
 RT: 19.843 min Scan# 3704
 Delta R.T. -0.028 min
 Lab File: BN022899.D
 Acq: 27 Nov 2022 02:03


Tgt Ion: 202 Resp: 3578
 Ion Ratio Lower Upper
 202 100
 101 152.8 10.6 16.0#
 100 1116.4 8.2 12.4#

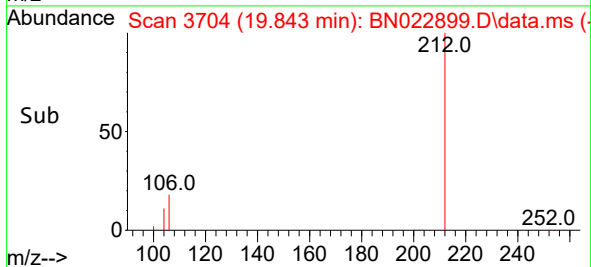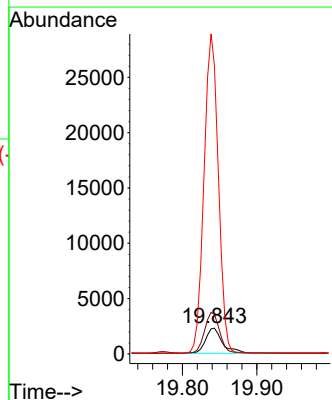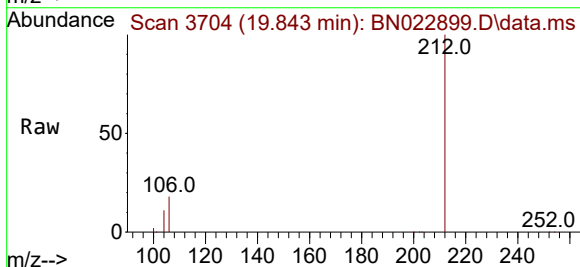

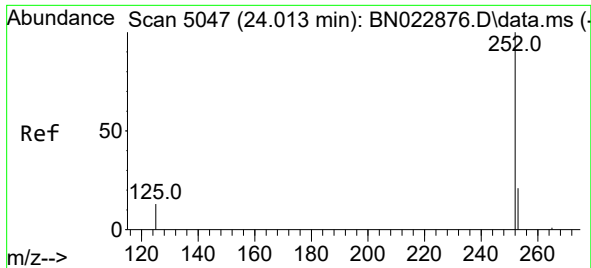

#26
Benzo(a)pyrene
Concen: 0.122 ng/ul
RT: 23.963 min Scan# 50
Delta R.T. -0.050 min
Lab File: BN022899.D
Acq: 27 Nov 2022 02:03

Instrument :
BNA_N
ClientSampleId :
C9807

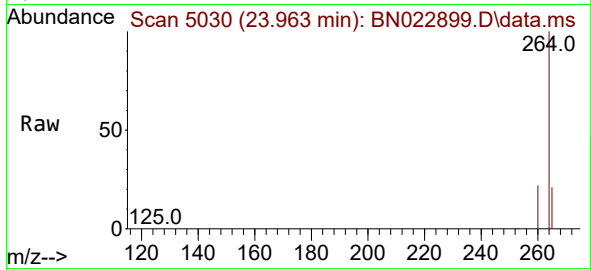

Tgt Ion:252 Resp: 5823
Ion Ratio Lower Upper
252 100
253 35.8 19.7 29.5#
125 33.3 13.7 20.5#

