

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112622\
 Data File : BN022901.D
 Acq On : 27 Nov 2022 03:53
 Operator : CG/JU
 Sample : PB149071BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK071

Quant Time: Nov 28 03:50:51 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 28 03:16:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.070	152	8854	0.400	ng/ul	0.00
4) Naphthalene-d8	10.887	136	26011	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.710	164	14865	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.453	188	30953	0.400	ng/ul	0.00
17) Chrysene-d12	21.633	240	17333	0.400	ng/ul	0.00
23) Perylene-d12	24.124	264	14099	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.408	96	64473	6.068	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.470	152	12539	0.316	ng/ul	0.00
18) Fluoranthene-d10	19.476	212	23901	0.373	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.700	166	4654	0.071	ng/ul#	13
20) Pyrene	19.843	202	3726	0.042	ng/ul#	1
26) Benzo(a)pyrene	23.963	252	6146	0.113	ng/ul#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112622\
Data File : BN022901.D
Acq On : 27 Nov 2022 03:53
Operator : CG/JU
Sample : PB149071BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK071

Quant Time: Nov 28 03:50:51 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 28 03:16:56 2022
Response via : Initial Calibration




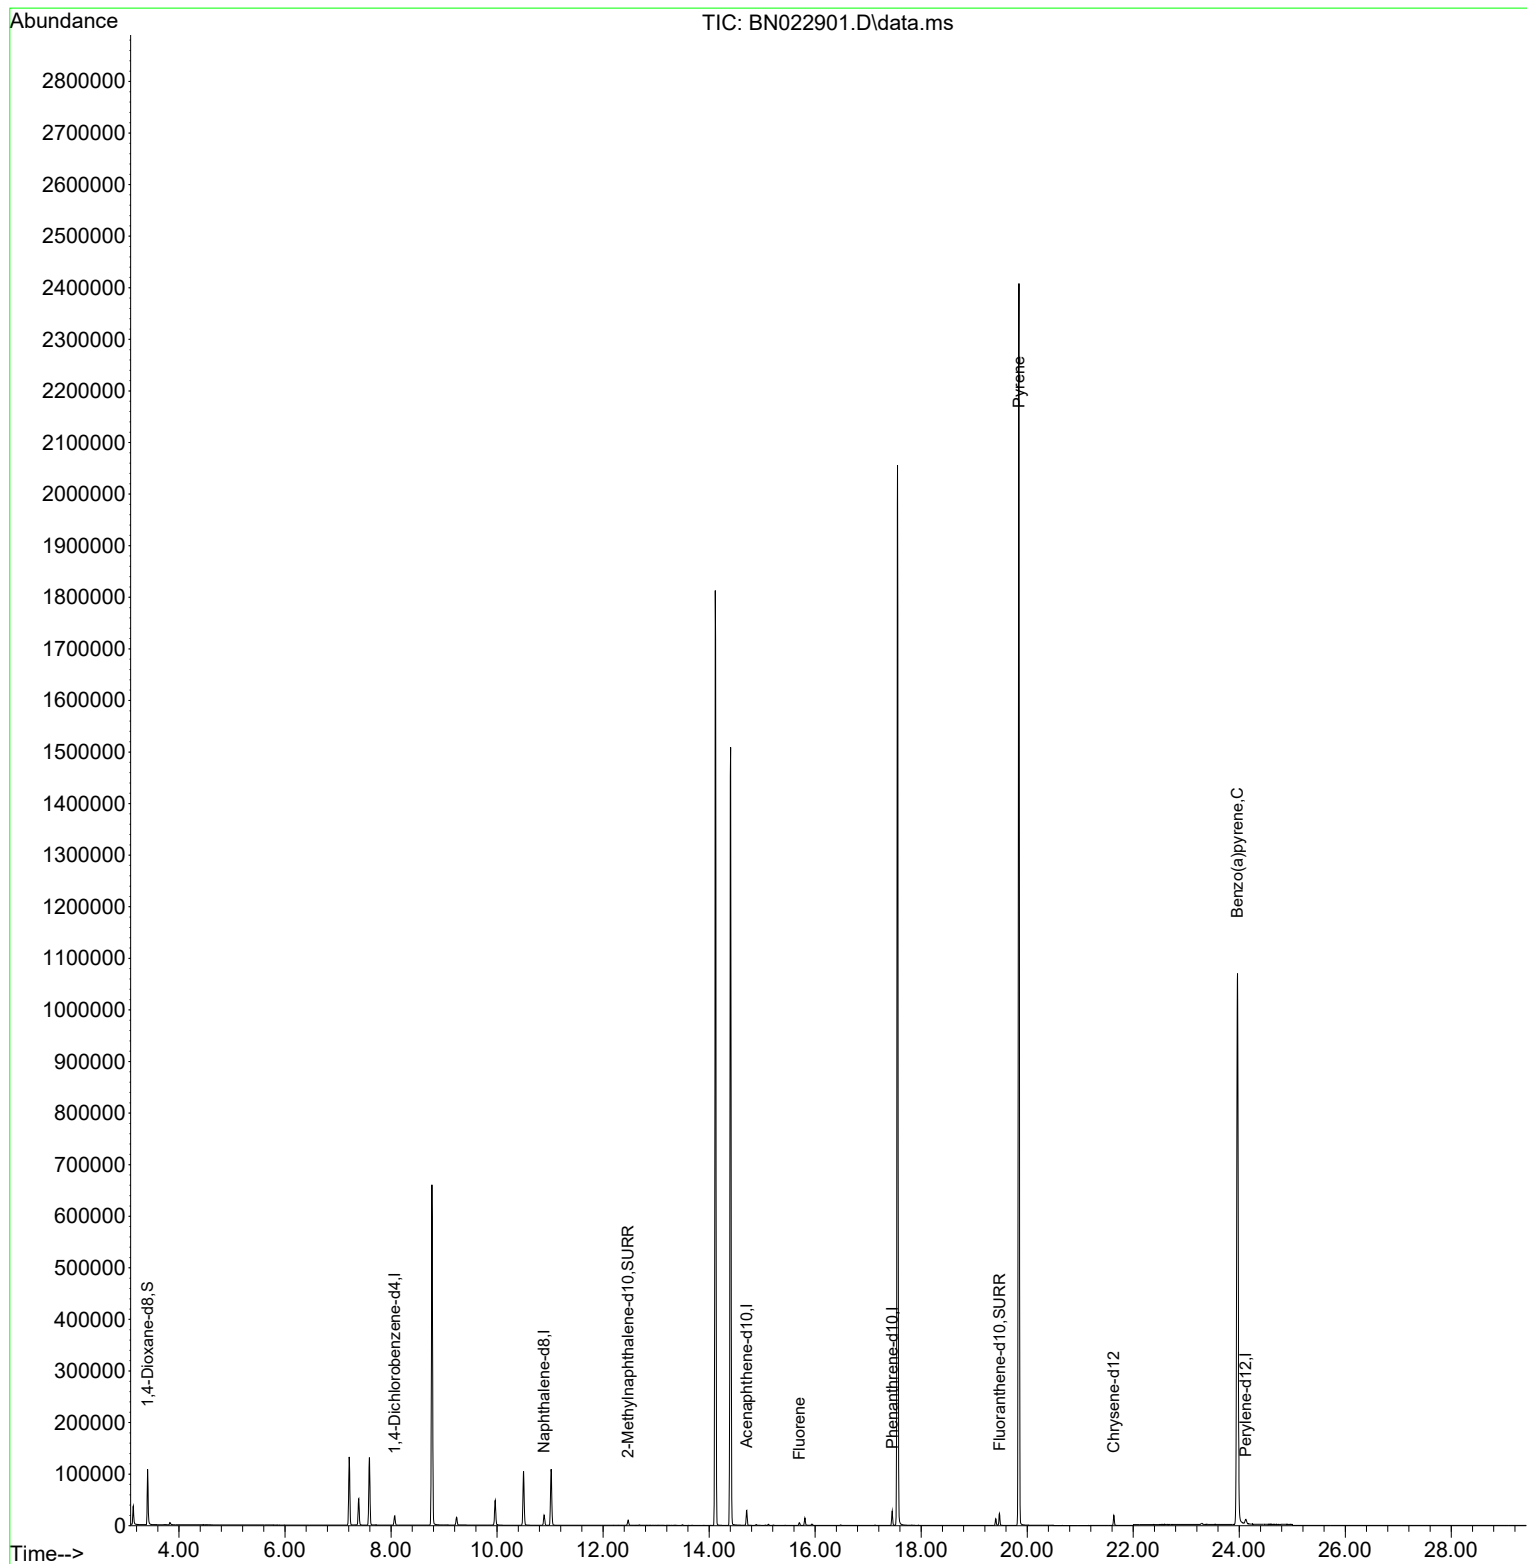


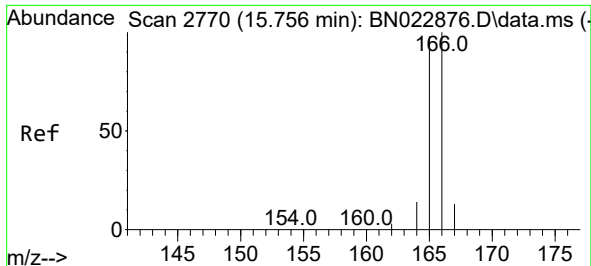

#12
Fluorene
Concen: 0.071 ng/ul
RT: 15.700 min Scan# 21
Delta R.T. -0.056 min
Lab File: BN022901.D
Acq: 27 Nov 2022 03:53




Instrument :
BNA_N
ClientSampleId :
SBLK071


Tgt Ion:166 Resp: 4654
Ion Ratio Lower Upper
166 100
165 6.1 78.7 118.1#
167 31.5 10.8 16.2#

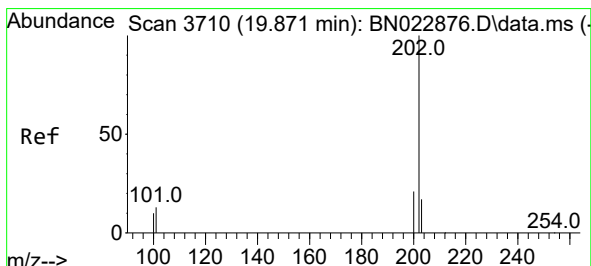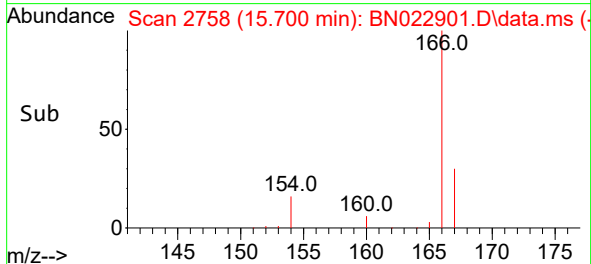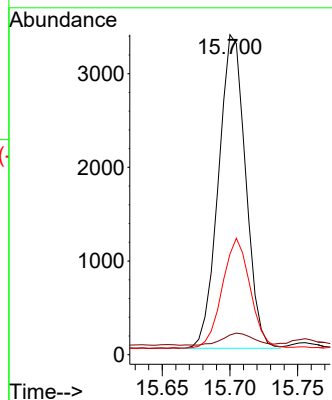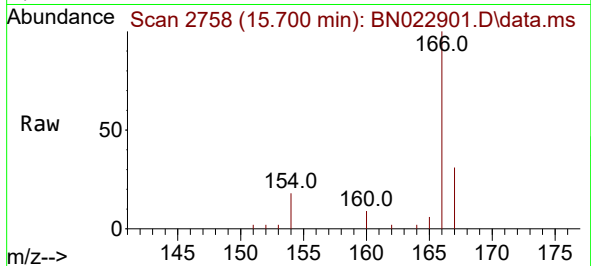

#20
Pyrene
Concen: 0.042 ng/ul
RT: 19.843 min Scan# 3704
Delta R.T. -0.028 min
Lab File: BN022901.D
Acq: 27 Nov 2022 03:53


Tgt Ion:202 Resp: 3726
Ion Ratio Lower Upper
202 100
101 157.8 10.6 16.0#
100 1167.2 8.2 12.4#

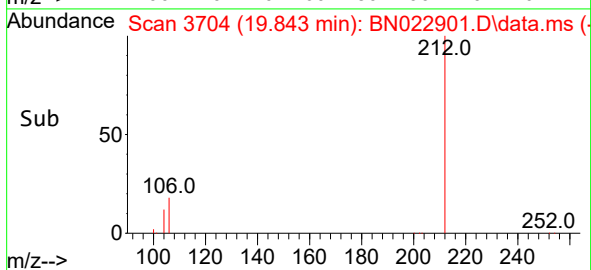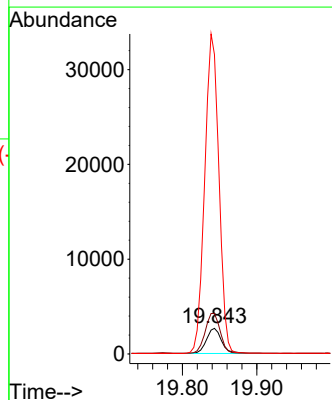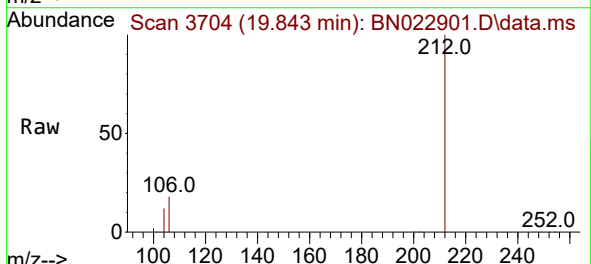

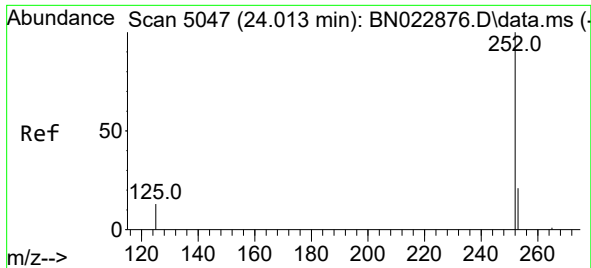

#26
Benzo(a)pyrene
Concen: 0.113 ng/ul
RT: 23.963 min Scan# 50
Delta R.T. -0.050 min
Lab File: BN022901.D
Acq: 27 Nov 2022 03:53

Instrument :
BNA_N
ClientSampleId :
SBLK071

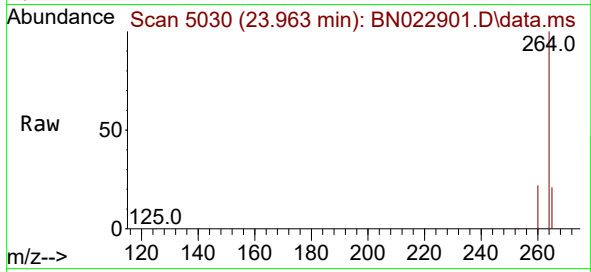

Tgt Ion:252 Resp: 6146
Ion Ratio Lower Upper
252 100
253 35.1 19.7 29.5#
125 32.7 13.7 20.5#

