

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112622\
 Data File : BN022902.D
 Acq On : 27 Nov 2022 04:30
 Operator : CG/JU
 Sample : PB149073BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK073

Quant Time: Nov 28 03:50:57 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 28 03:16:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.070	152	7853	0.400	ng/ul	0.00
4) Naphthalene-d8	10.887	136	23291	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.710	164	13433	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.454	188	28516	0.400	ng/ul	0.00
17) Chrysene-d12	21.634	240	16558	0.400	ng/ul	0.00
23) Perylene-d12	24.121	264	13632	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.408	96	62053	6.585	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.471	152	12253	0.345	ng/ul	0.00
18) Fluoranthene-d10	19.476	212	24477	0.400	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.843	202	3767	0.045	ng/ul#	1
26) Benzo(a)pyrene	23.966	252	6351	0.121	ng/ul#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112622\
Data File : BN022902.D
Acq On : 27 Nov 2022 04:30
Operator : CG/JU
Sample : PB149073BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK073

Quant Time: Nov 28 03:50:57 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 28 03:16:56 2022
Response via : Initial Calibration




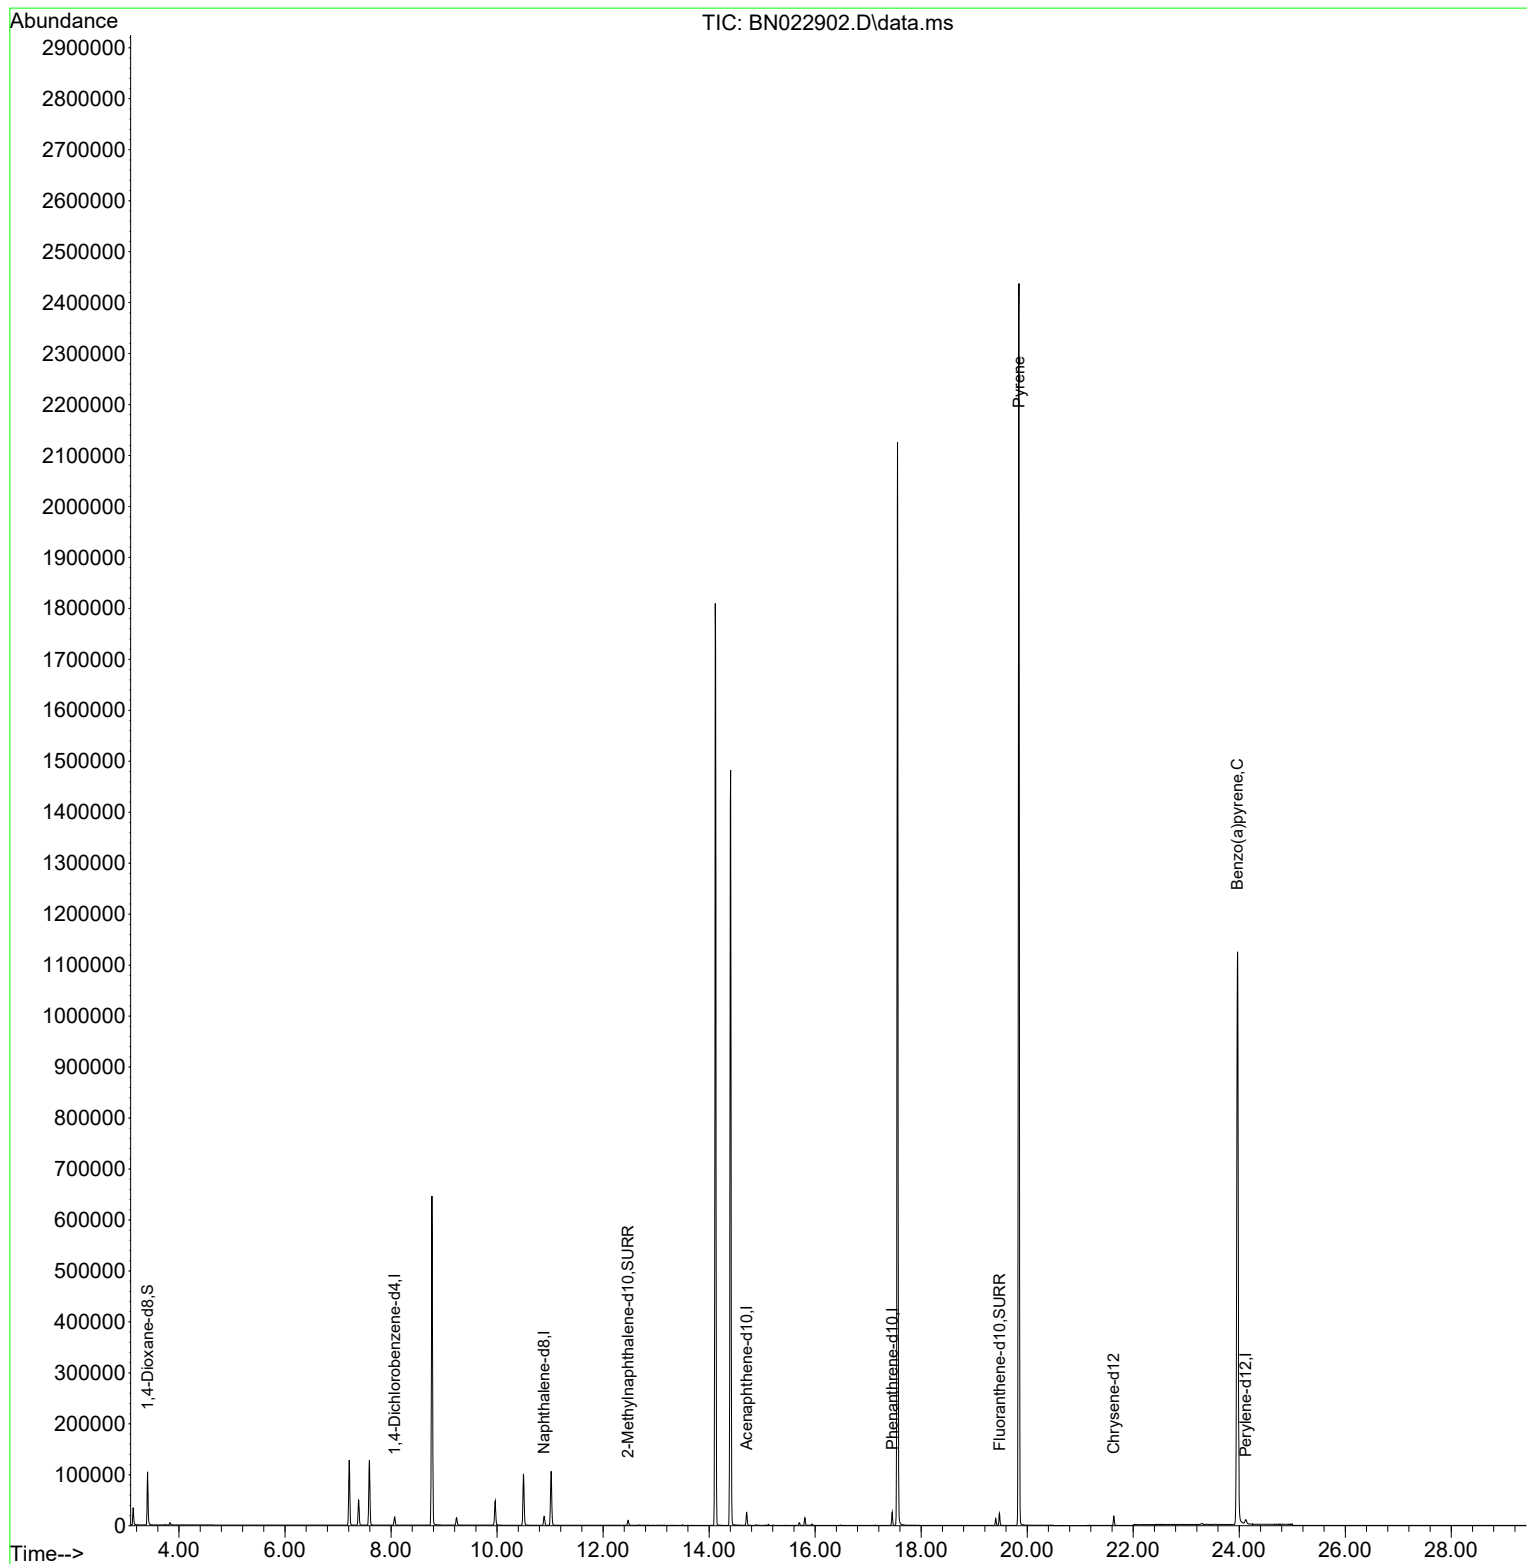


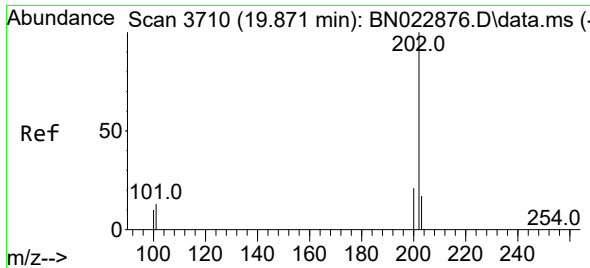

#20
Pyrene
Concen: 0.045 ng/ul
RT: 19.843 min Scan# 31
Delta R.T. -0.028 min
Lab File: BN022902.D
Acq: 27 Nov 2022 04:30

Instrument :
BNA_N
ClientSampleId :
SBLK073

Tgt Ion:202 Resp: 3767
Ion Ratio Lower Upper
202 100
101 158.2 10.6 16.0#
100 1168.1 8.2 12.4#

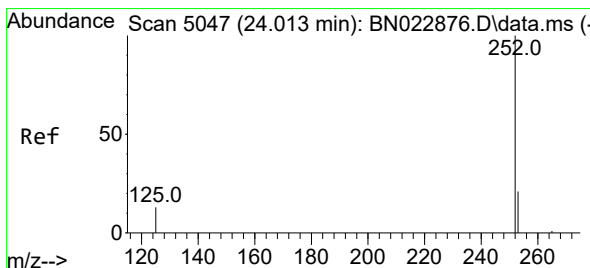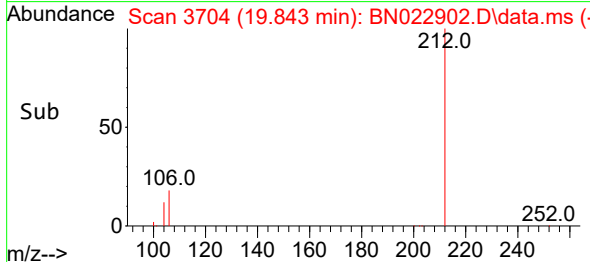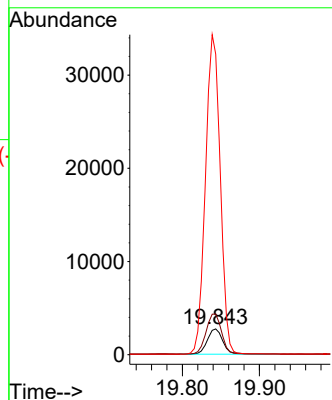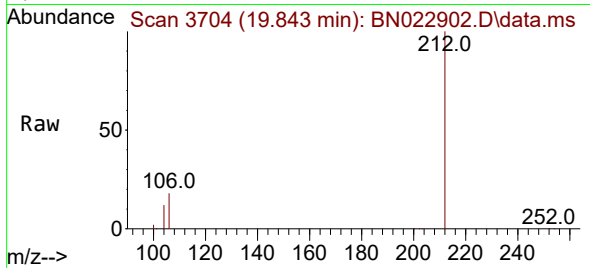

#26
Benzo(a)pyrene
Concen: 0.121 ng/ul
RT: 23.966 min Scan# 5031
Delta R.T. -0.047 min
Lab File: BN022902.D
Acq: 27 Nov 2022 04:30

Tgt Ion:252 Resp: 6351
Ion Ratio Lower Upper
252 100
253 35.1 19.7 29.5#
125 32.2 13.7 20.5#

