

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112622\
 Data File : BN022907.D
 Acq On : 27 Nov 2022 07:34
 Operator : CG/JU
 Sample : N5591-07
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C9808

Quant Time: Nov 28 03:51:40 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 28 03:16:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.066	152	8747	0.400	ng/ul	0.00
4) Naphthalene-d8	10.887	136	24901	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.705	164	13205	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.454	188	26659	0.400	ng/ul	0.00
17) Chrysene-d12	21.633	240	15943	0.400	ng/ul	0.00
23) Perylene-d12	24.124	264	14018	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.412	96	43050	4.101	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.471	152	10136	0.267	ng/ul	0.00
18) Fluoranthene-d10	19.476	212	20014	0.340	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.450	88	1349	0.123	ng/ul#	80
20) Pyrene	19.843	202	3154	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.963	252	5188	0.096	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112622\
Data File : BN022907.D
Acq On : 27 Nov 2022 07:34
Operator : CG/JU
Sample : N5591-07
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C9808

Quant Time: Nov 28 03:51:40 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 28 03:16:56 2022
Response via : Initial Calibration




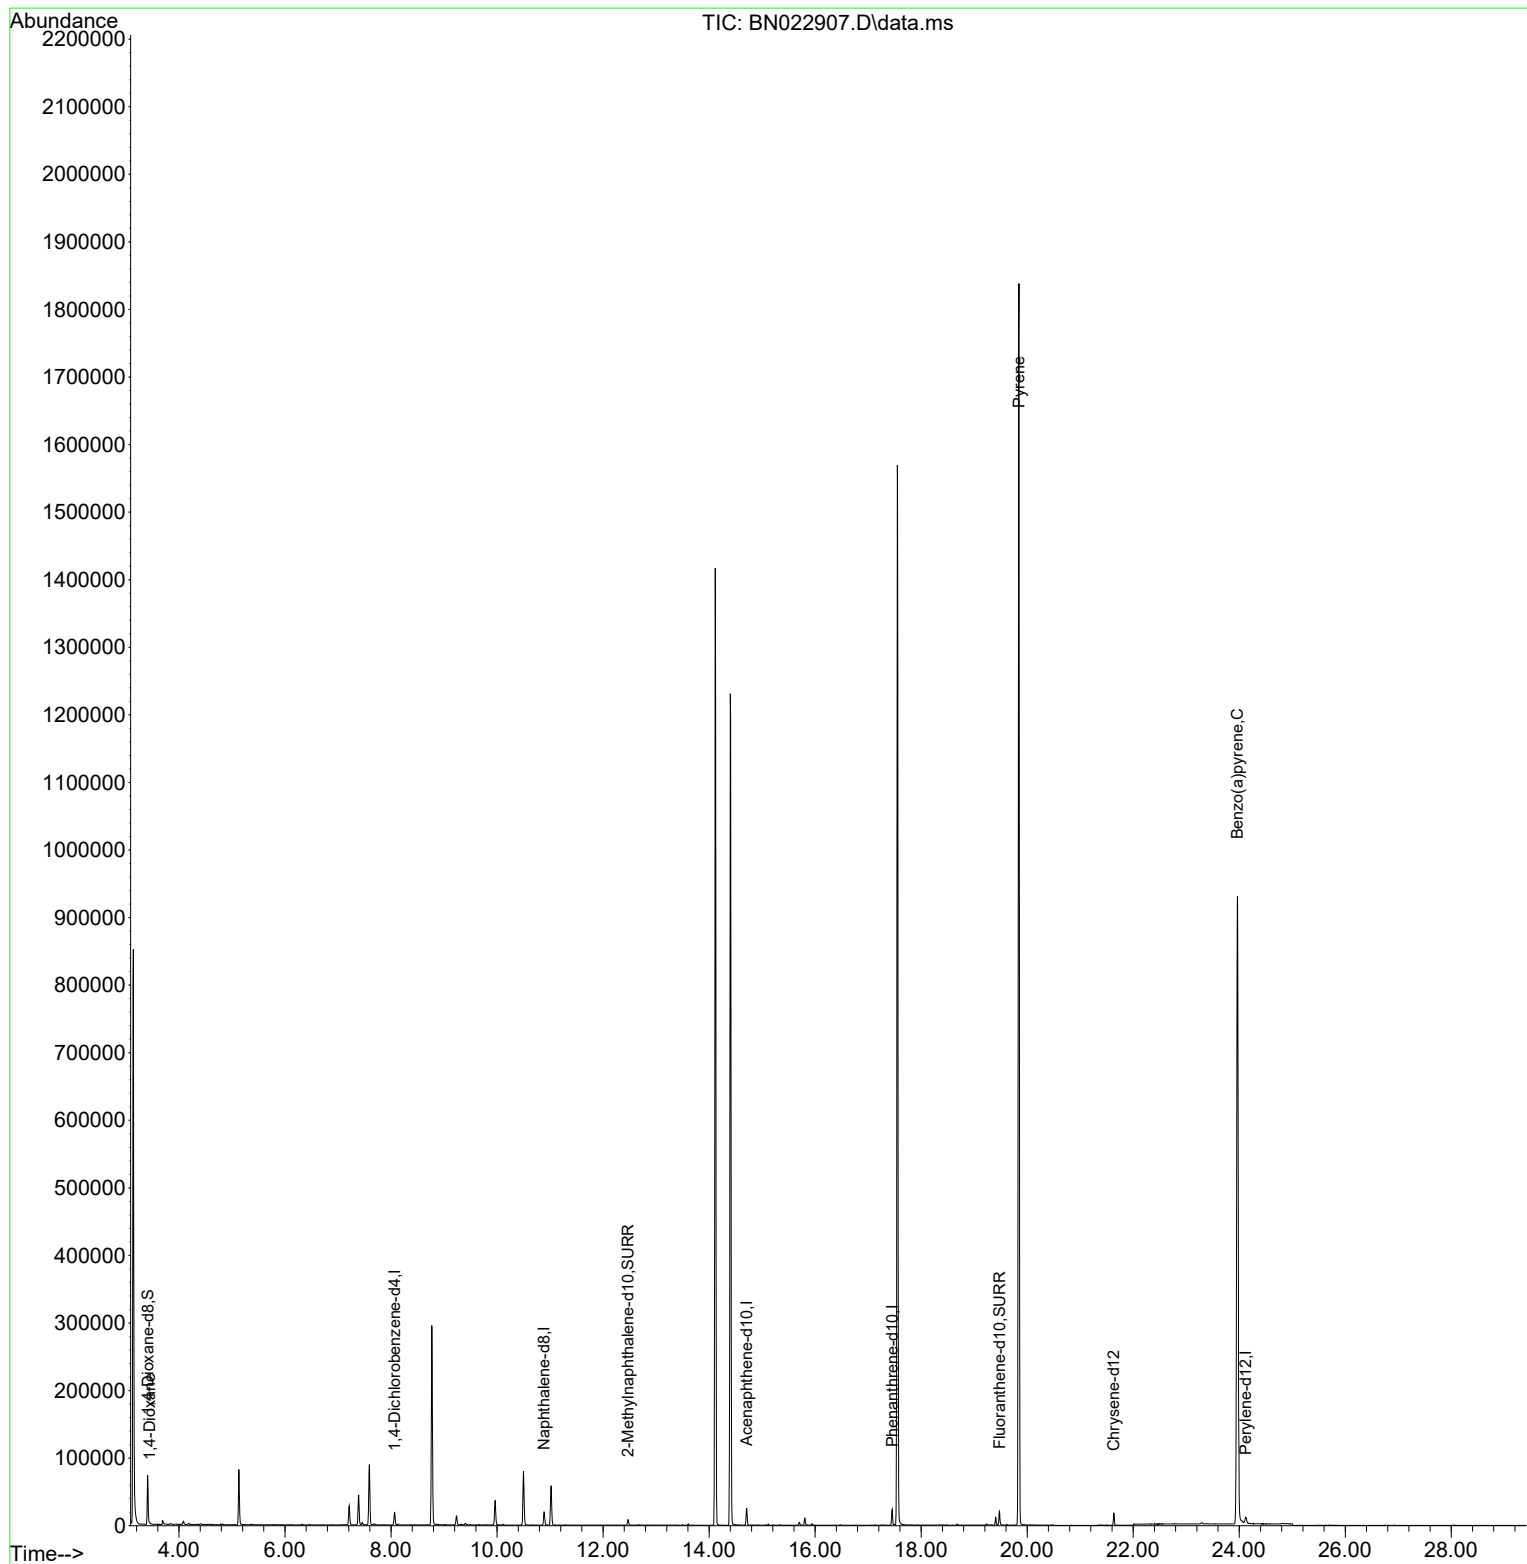


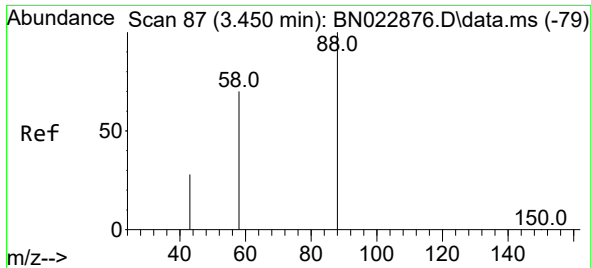

#2
1,4-Dioxane
Concen: 0.123 ng/ul
RT: 3.450 min Scan# 81
Delta R.T. 0.000 min
Lab File: BN022907.D
Acq: 27 Nov 2022 07:34




Instrument :
BNA_N
ClientSampleId :
C9808


Tgt Ion: 88 Resp: 1349
Ion Ratio Lower Upper
88 100
43 42.9 26.2 39.4#
58 43.8 47.6 71.4#

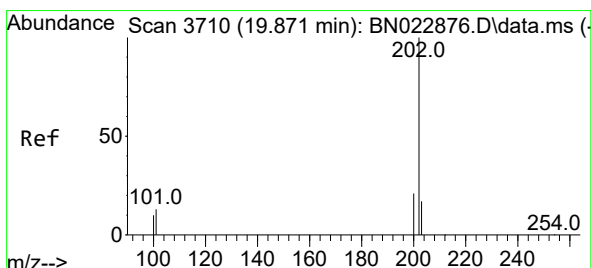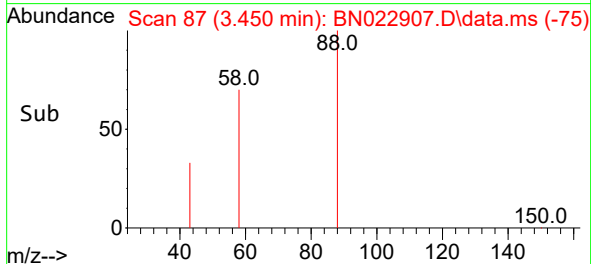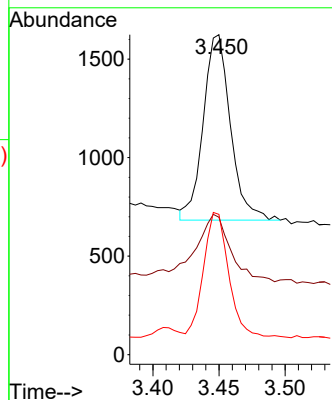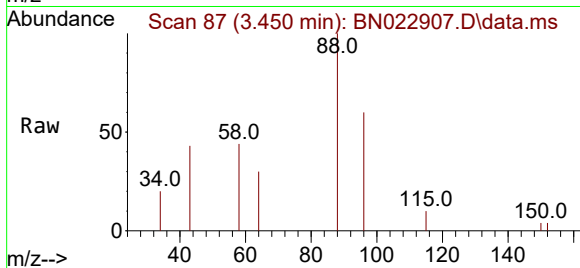

#20
Pyrene
Concen: 0.039 ng/ul
RT: 19.843 min Scan# 3704
Delta R.T. -0.028 min
Lab File: BN022907.D
Acq: 27 Nov 2022 07:34

Tgt Ion: 202 Resp: 3154
Ion Ratio Lower Upper
202 100
101 155.5 10.6 16.0#
100 1111.2 8.2 12.4#

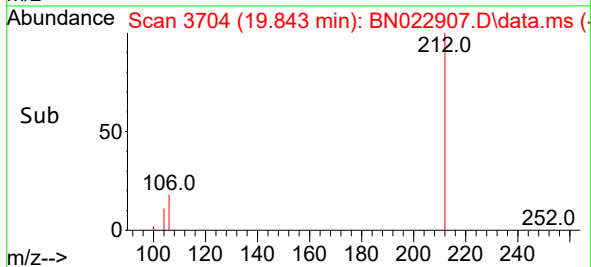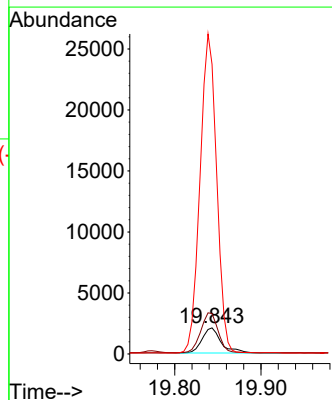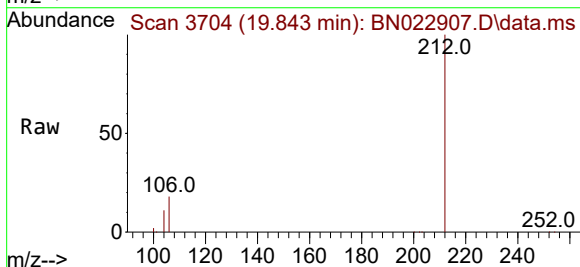

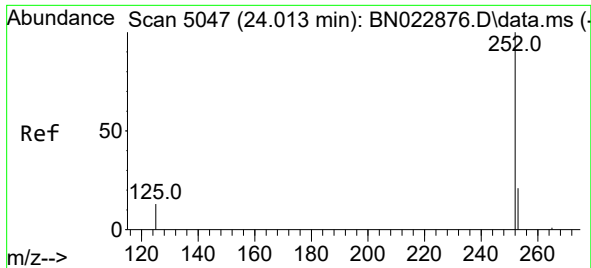

#26

Benzo(a)pyrene

Concen: 0.096 ng/ul

RT: 23.963 min Scan# 50

Delta R.T. -0.050 min

Lab File: BN022907.D


Acq: 27 Nov 2022 07:34

Instrument :

BNA_N

ClientSampleId :

C9808

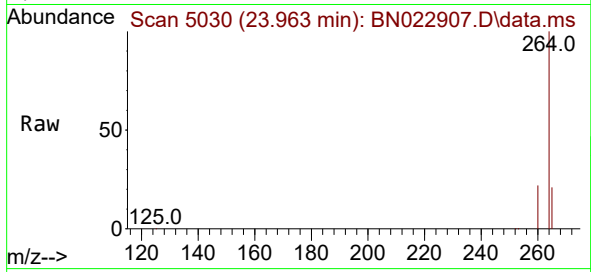

Tgt Ion:252 Resp: 5188

Ion Ratio Lower Upper

252 100

253 37.0 19.7 29.5#

125 35.0 13.7 20.5#

