

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
 Data File : BN035324.D
 Acq On : 26 Nov 2024 20:43
 Operator : RC/JU
 Sample : P4996-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHF71

Quant Time: Nov 26 22:14:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 26 06:09:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.310	152	3334	0.400	ng/ul	0.00
4) Naphthalene-d8	10.059	136	9129	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.967	164	5774	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.74
17) Chrysene-d12	20.976	240	6485	0.400	ng/ul	# 0.00
23) Perylene-d12	22.943	264	570742	0.400	ng/ul	#-0.13
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.972	96	13405	4.399	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.659	152	3874	0.290	ng/ul	0.00
18) Fluoranthene-d10	18.786	212	9483	0.530	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	14.981	166	1499	0.073	ng/ul#	15
20) Pyrene	19.158	202	1377	0.059	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035324.D
Acq On : 26 Nov 2024 20:43
Operator : RC/JU
Sample : P4996-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHF71

Quant Time: Nov 26 22:14:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration




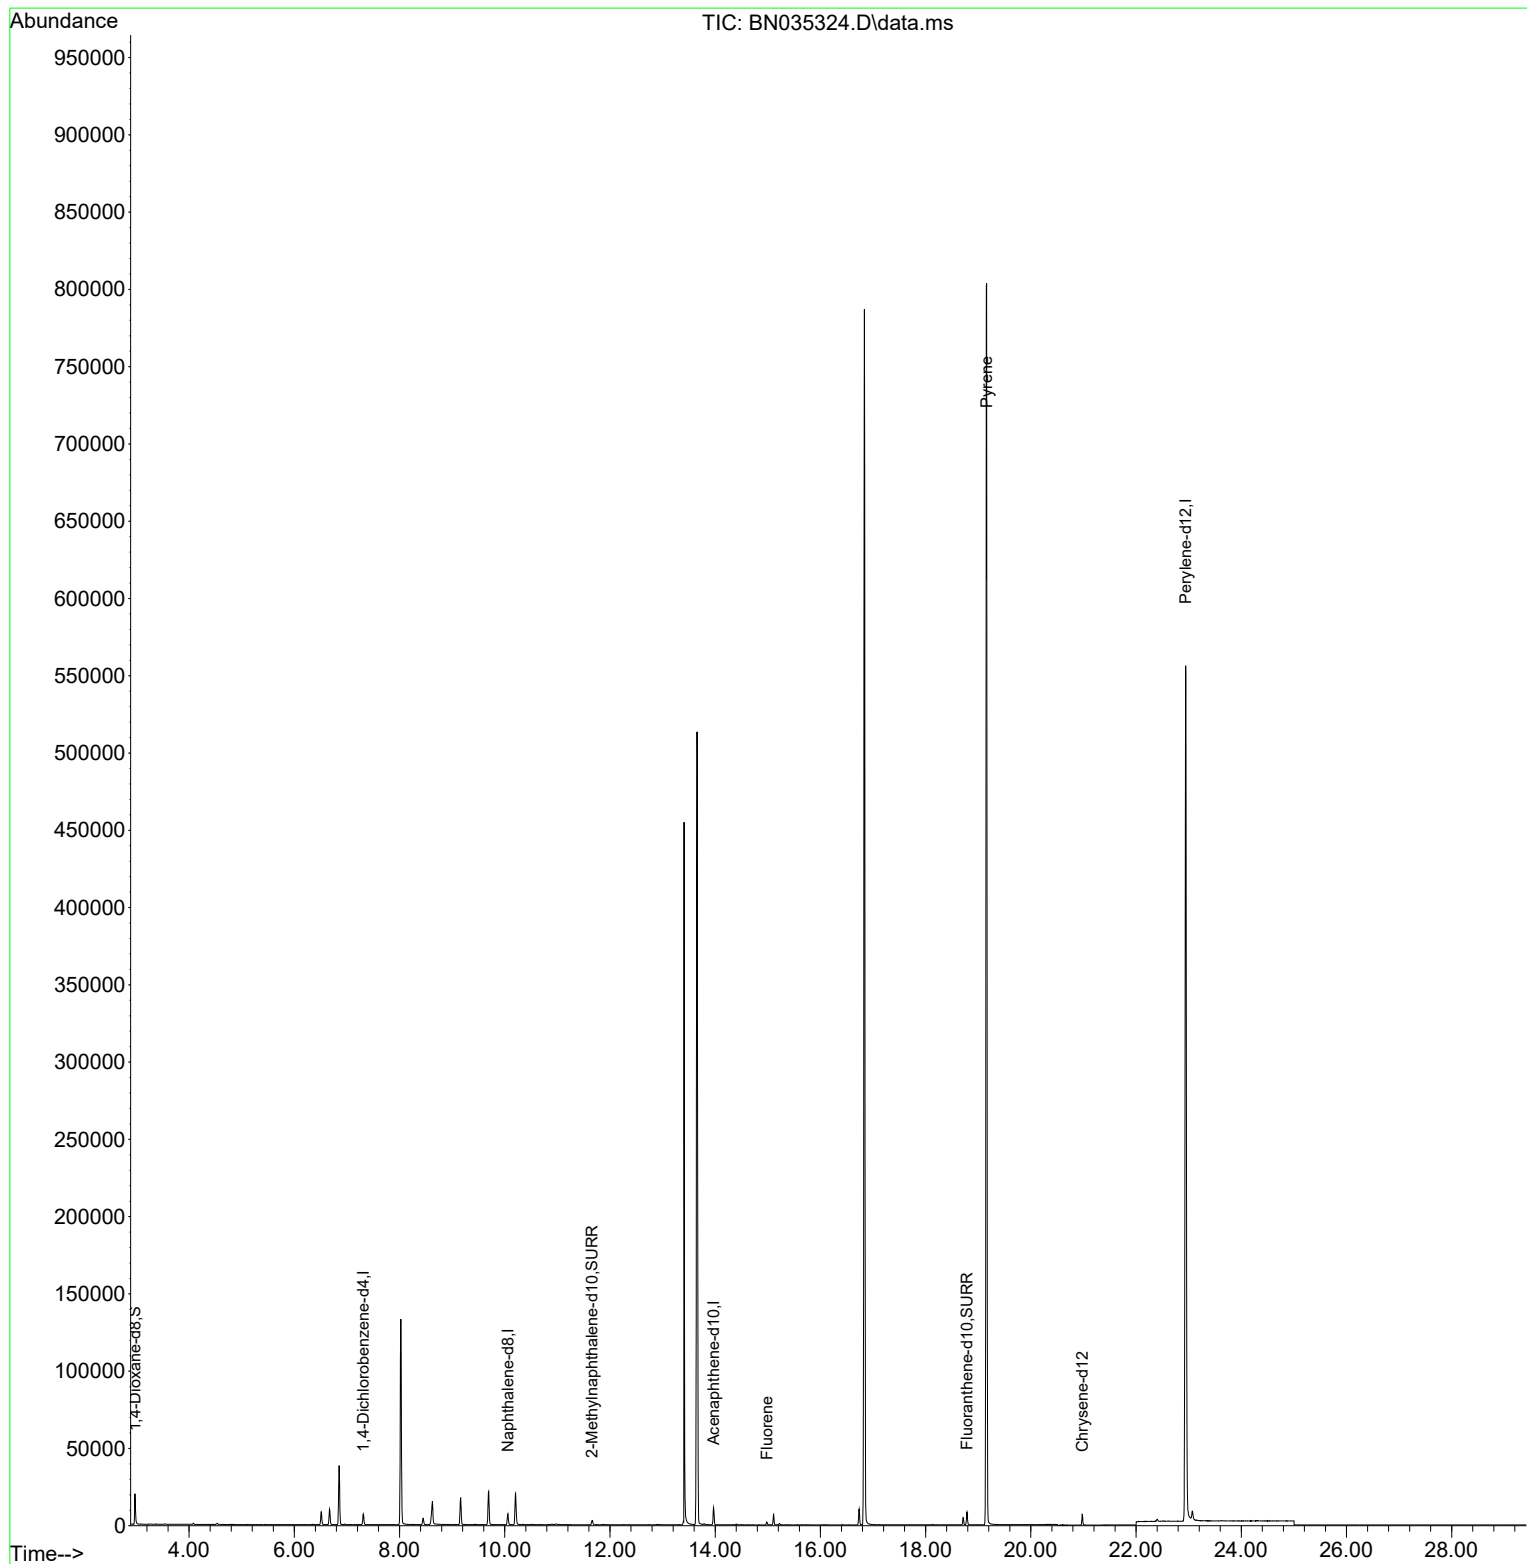


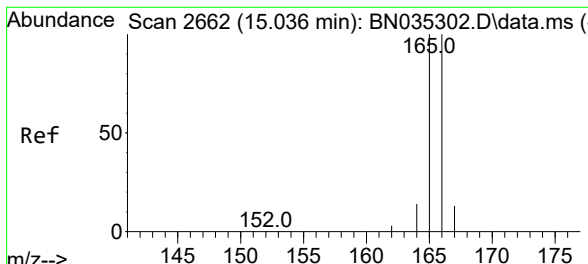

#12
 Fluorene
 Concen: 0.073 ng/ul
 RT: 14.981 min Scan# 2650
 Delta R.T. -0.055 min
 Lab File: BN035324.D
 Acq: 26 Nov 2024 20:43

Instrument :
 BNA_N
 ClientSampleId :
 BHF71

Tgt Ion:	166	Resp:	1499
Ion Ratio	Lower	Upper	
166	100		
165	9.3	78.6	118.0#
167	36.8	11.8	17.6#

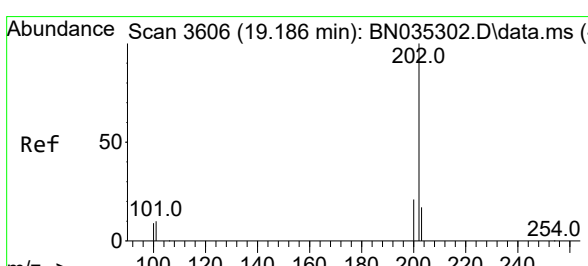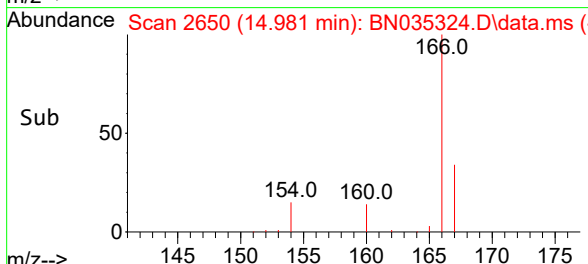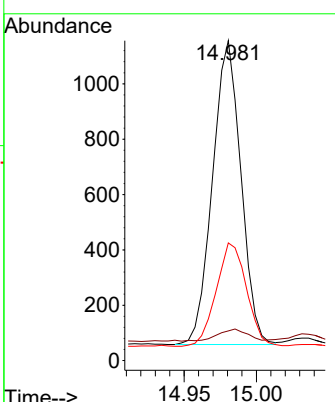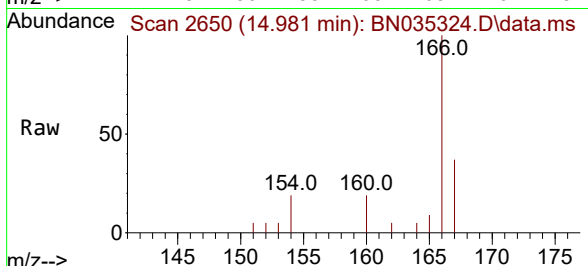

#20
 Pyrene
 Concen: 0.059 ng/ul
 RT: 19.158 min Scan# 3600
 Delta R.T. -0.028 min
 Lab File: BN035324.D
 Acq: 26 Nov 2024 20:43

Tgt Ion:	202	Resp:	1377
Ion Ratio	Lower	Upper	
202	100		
101	138.9	6.2	9.4#
100	934.7	5.1	7.7#

