




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035304.D
Acq On : 26 Nov 2024 06:20
Operator : RC/JU
Sample : P4965-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1PJ0

Manual IntegrationsAPPROVED

Quant Time: Nov 26 06:46:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

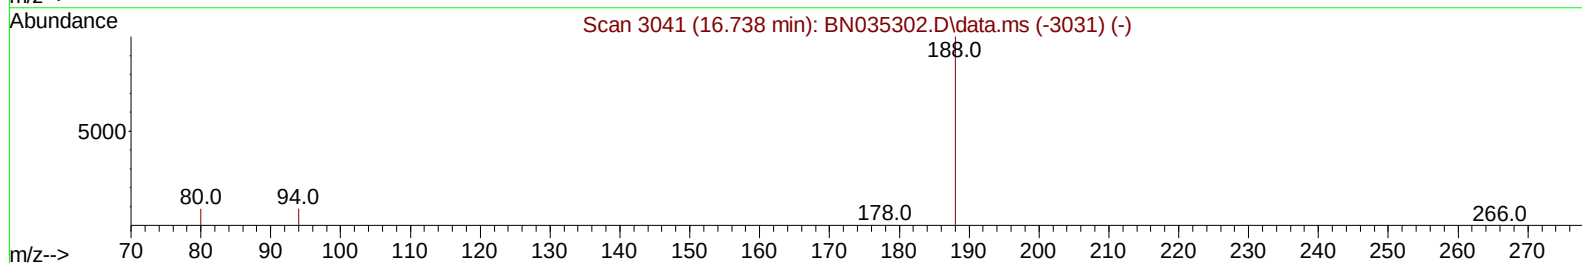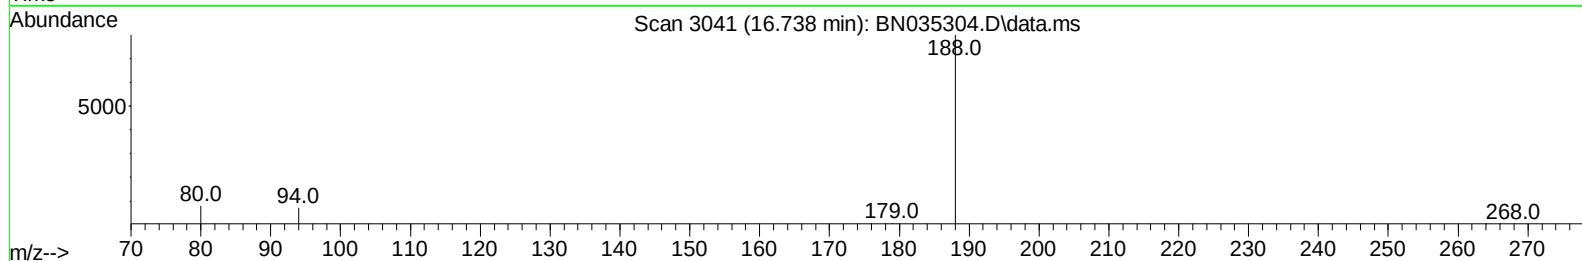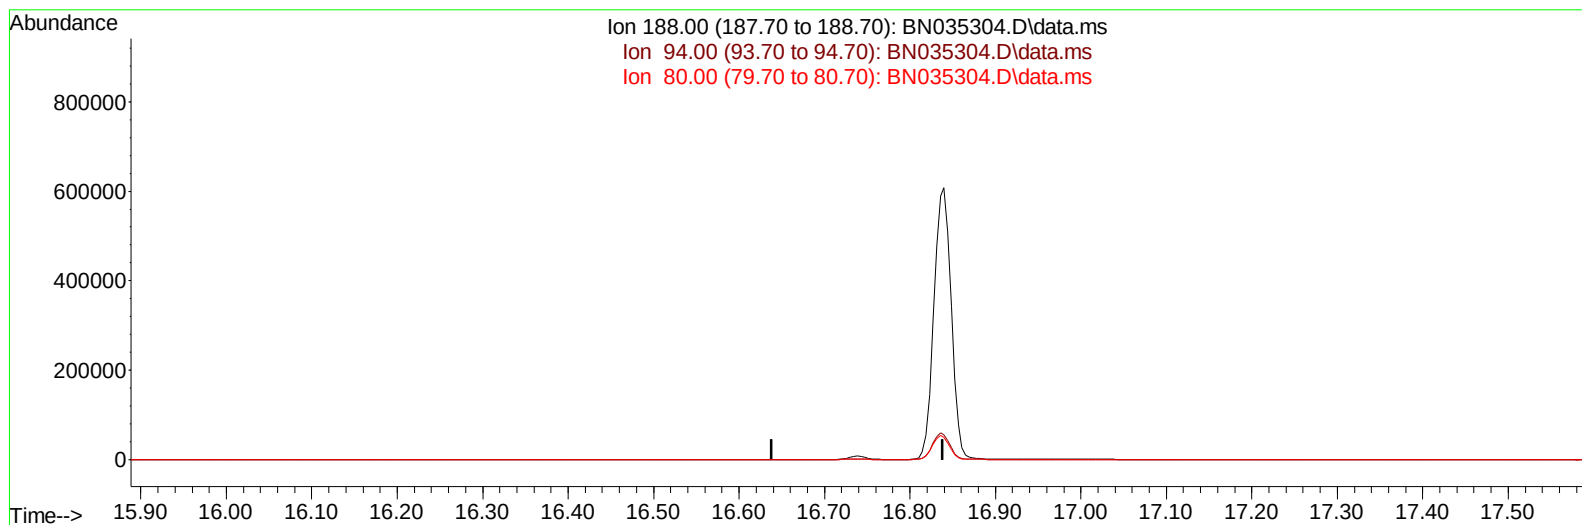

TIC: BN035304.D\data.ms

(13) Phenanthrene-d10 (I)

16.738min (-16.738) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	7.00	0.00#
80.00	7.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
 Data File : BN035304.D
 Acq On : 26 Nov 2024 06:20
 Operator : RC/JU
 Sample : P4965-03
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1PJ0

Manual IntegrationsAPPROVED

Quant Time: Nov 26 06:46:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 26 06:09:15 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
 Supervised By :mohammad ahmed 11/28/2024

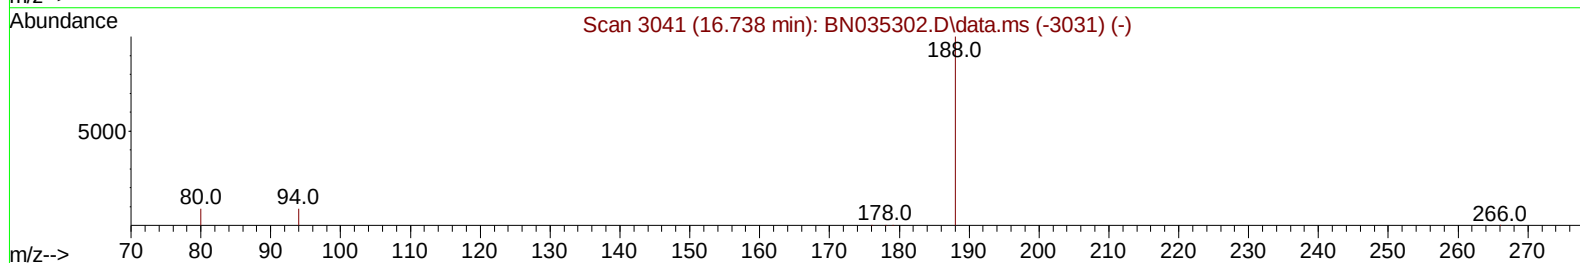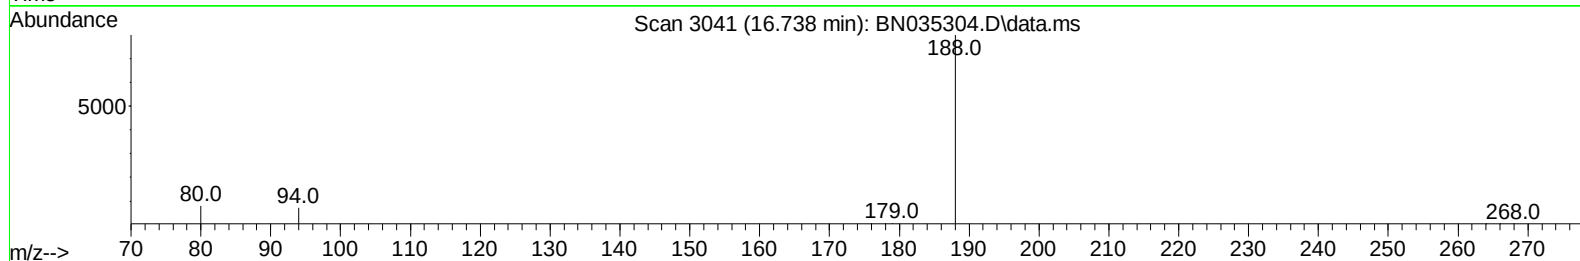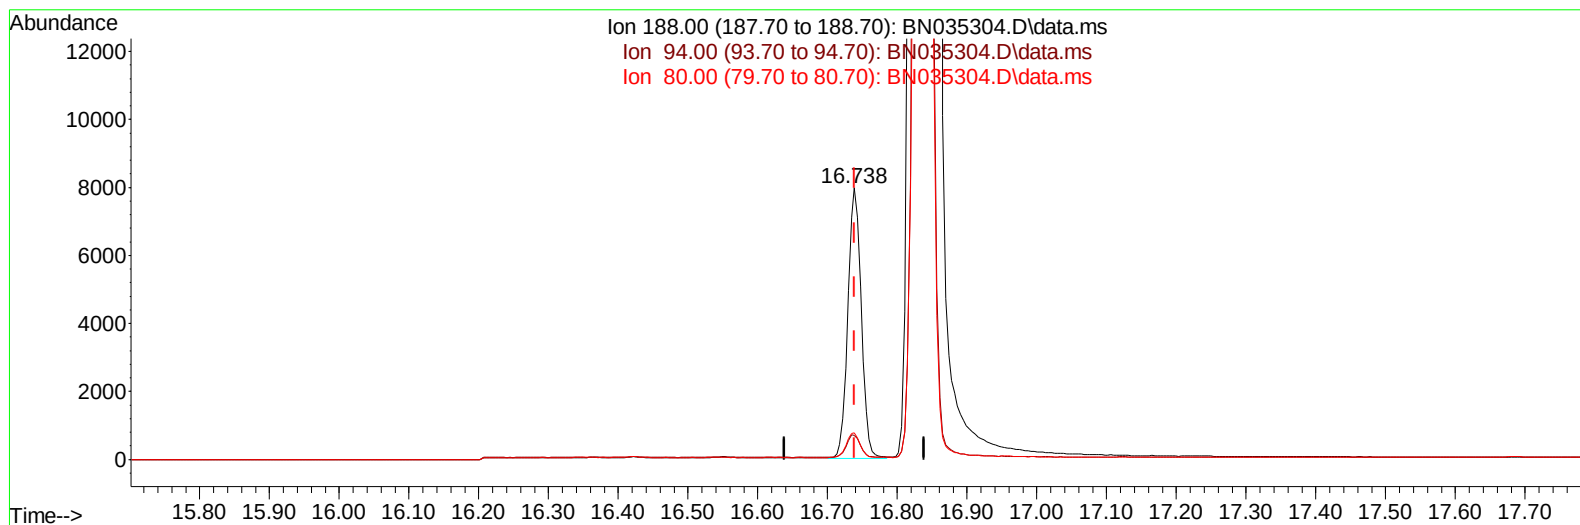

TIC: BN035304.D\data.ms

(13) Phenanthrene-d10 (I)

16.738min (-0.000) 0.40 ng/ul m

response 10598

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.00	8.89#
80.00	7.60	9.88#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035304.D
Acq On : 26 Nov 2024 06:20
Operator : RC/JU
Sample : P4965-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1PJ0

Manual IntegrationsAPPROVED

Quant Time: Nov 26 06:46:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

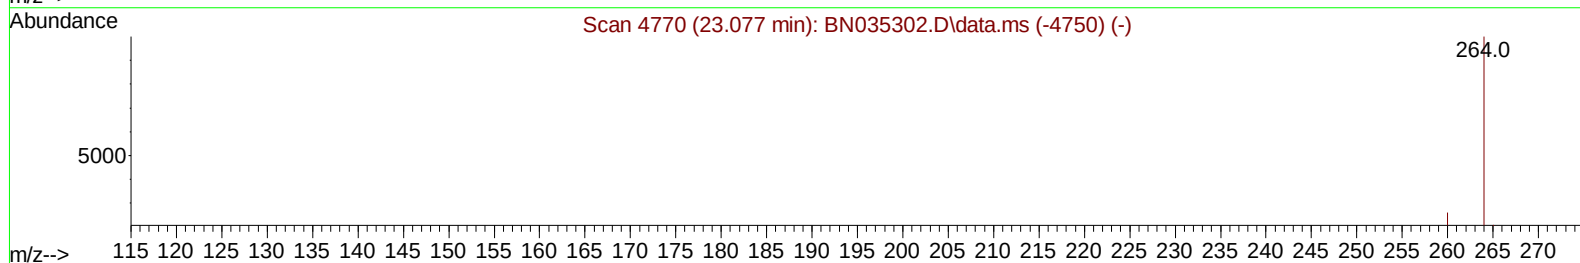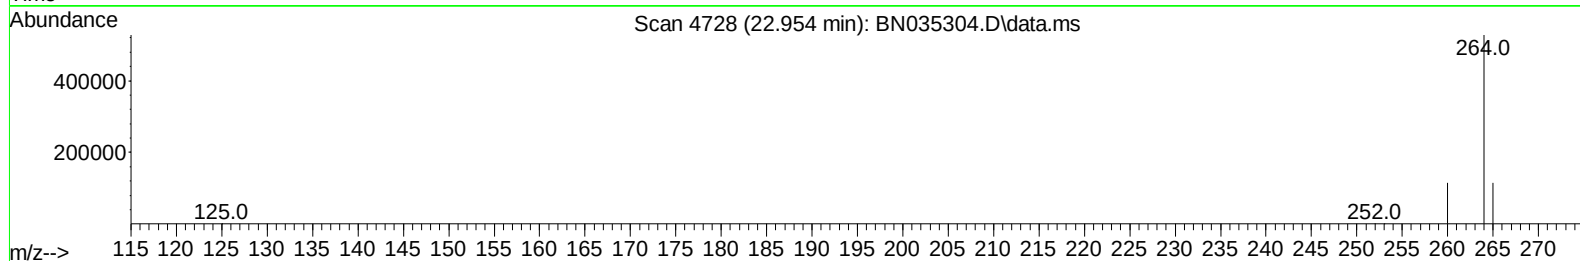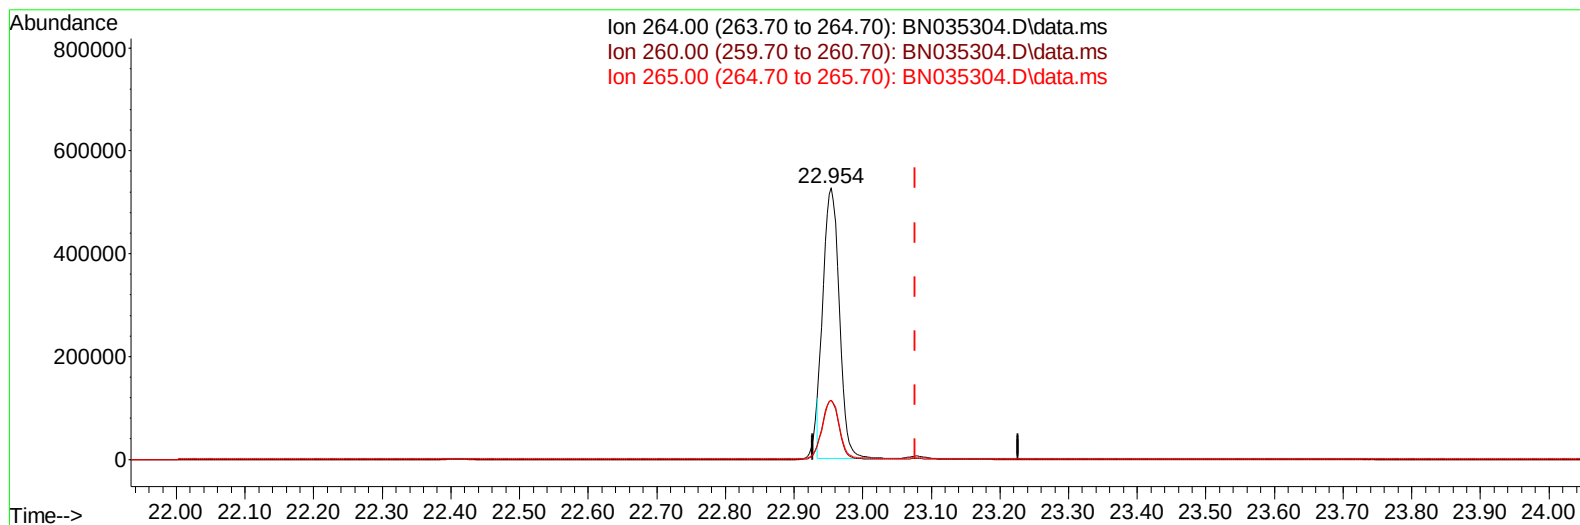

TIC: BN035304.D\data.ms

(23) Perylene-d12 (I)

22.954min (-0.123) 0.40 ng/u1

response 862390

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	21.79
265.00	75.50	21.73#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035304.D
Acq On : 26 Nov 2024 06:20
Operator : RC/JU
Sample : P4965-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1PJ0

Manual IntegrationsAPPROVED

Quant Time: Nov 26 06:46:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

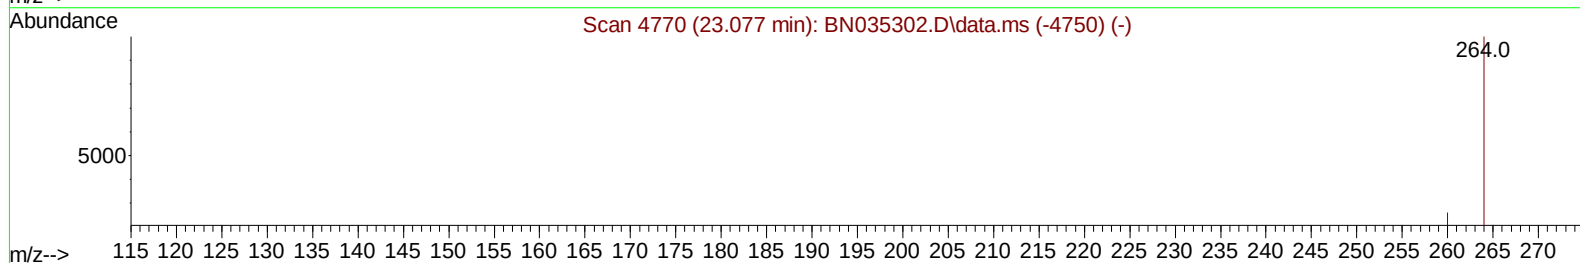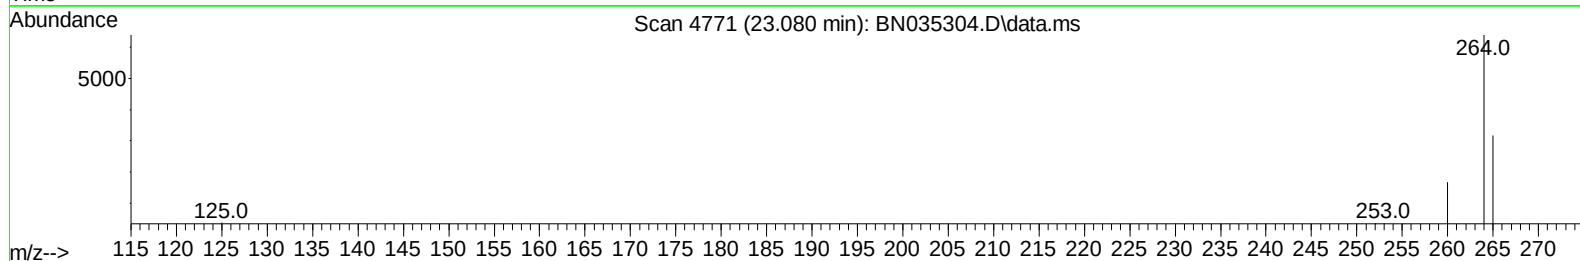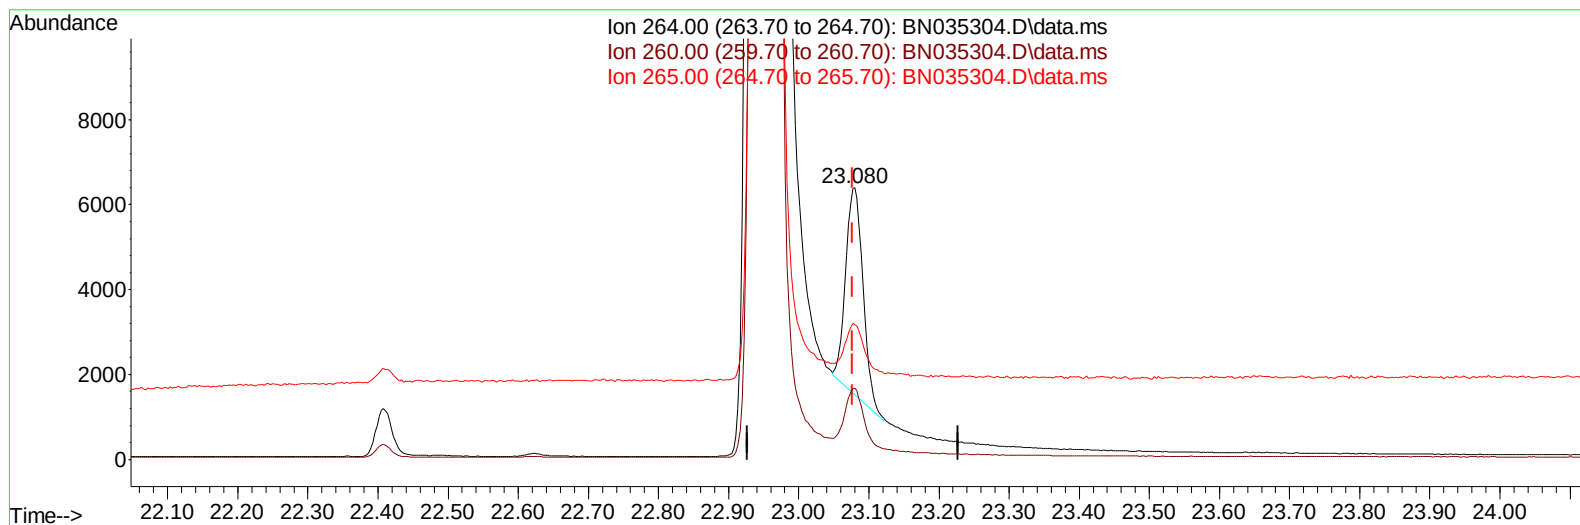

TIC: BN035304.D\data.ms

(23) Perylene-d12 (I)

23.080min (+ 0.003) 0.40 ng/ul m

response 8324

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	26.25
265.00	75.50	49.54#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
 Data File : BN035304.D
 Acq On : 26 Nov 2024 06:20
 Operator : RC/JU
 Sample : P4965-03
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1PJ0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2024
 Supervised By :mohammad ahmed 11/28/2024

Quant Time: Nov 26 06:46:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 26 06:09:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.314	152	3189	0.400	ng/ul	0.00
4) Naphthalene-d8	10.059	136	8125	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.972	164	4852	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.738	188	10598m	0.400	ng/ul	0.00
17) Chrysene-d12	20.982	240	8765	0.400	ng/ul	# 0.00
23) Perylene-d12	23.080	264	8324m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.976	96	14636	5.021	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.664	152	3713	0.312	ng/ul	0.00
18) Fluoranthene-d10	18.791	212	10301	0.426	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035304.D
Acq On : 26 Nov 2024 06:20
Operator : RC/JU
Sample : P4965-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1PJ0

Manual IntegrationsAPPROVED

Quant Time: Nov 26 06:46:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

