




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035308.D
Acq On : 26 Nov 2024 09:59
Operator : RC/JU
Sample : P4875-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2A24

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:12:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

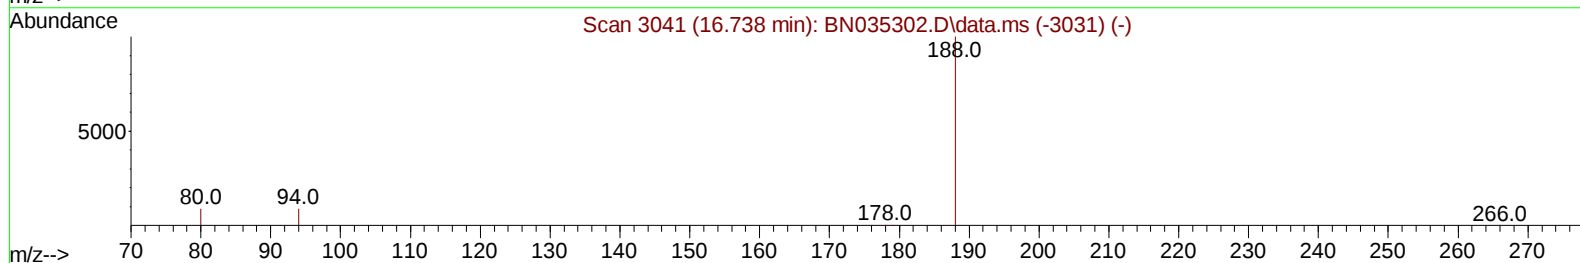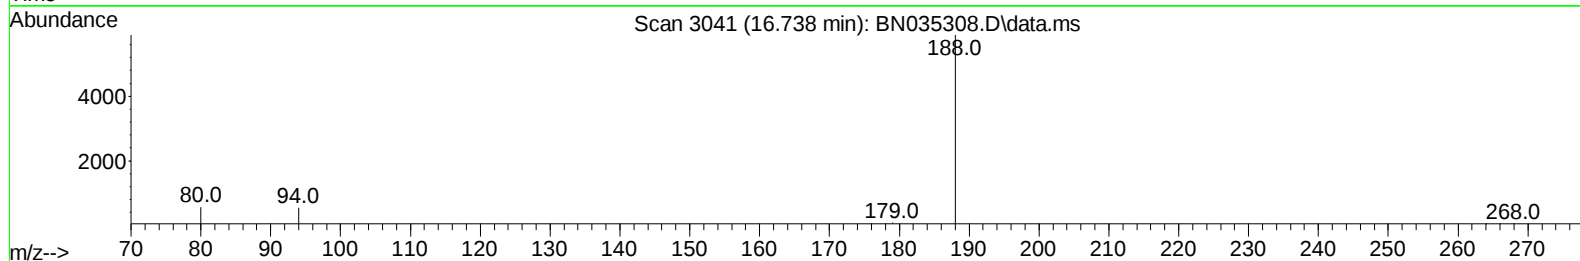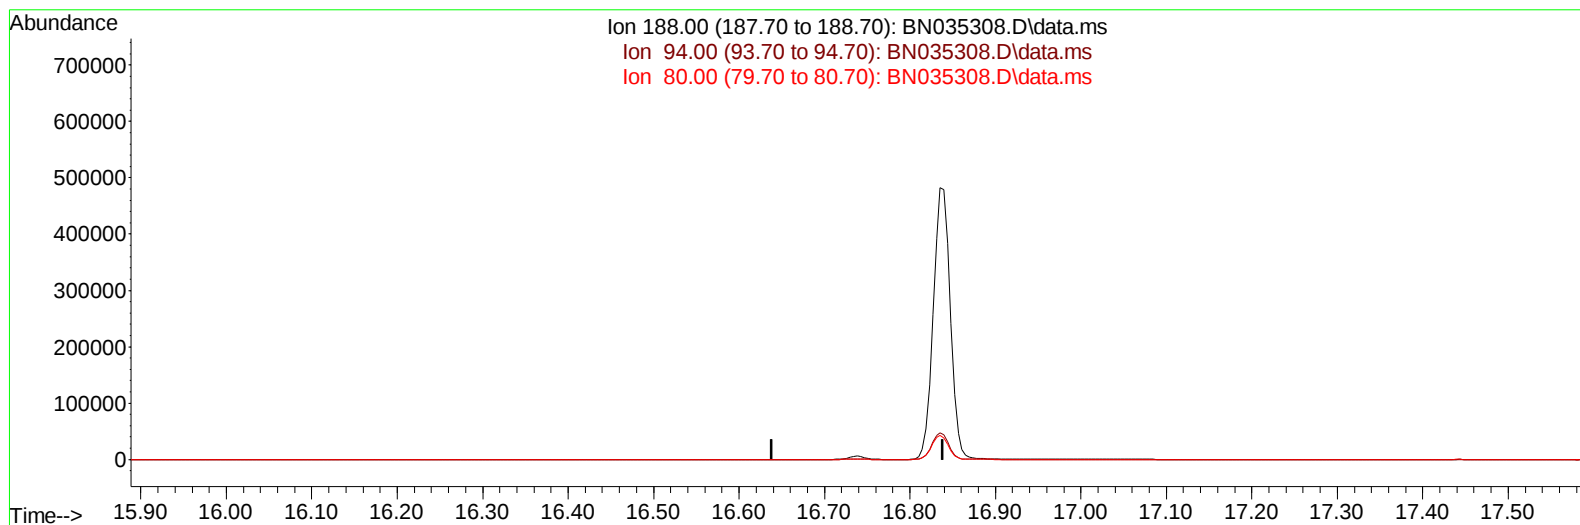

TIC: BN035308.D\data.ms

(13) Phenanthrene-d10 (I)

16.738min (-16.738) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	7.00	0.00#
80.00	7.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035308.D
Acq On : 26 Nov 2024 09:59
Operator : RC/JU
Sample : P4875-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2A24

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:12:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

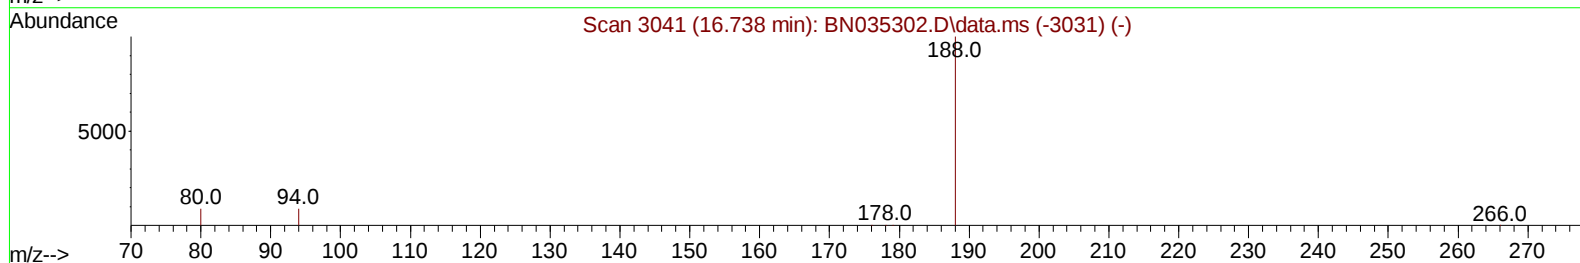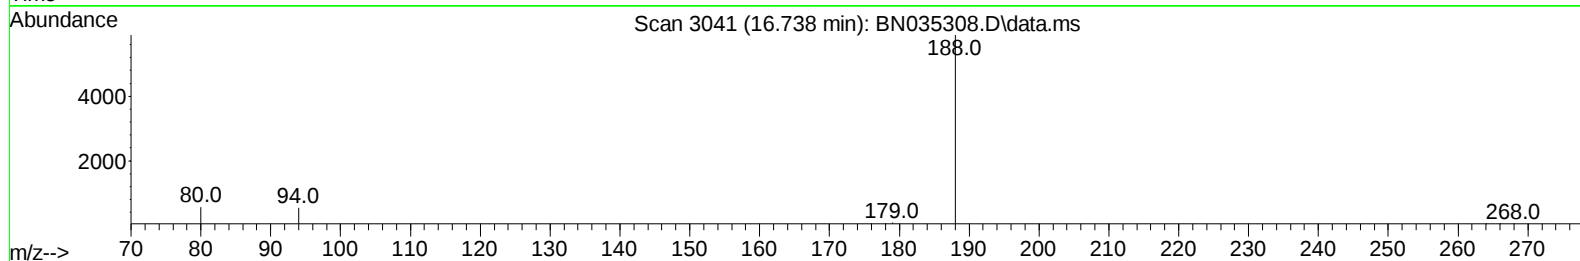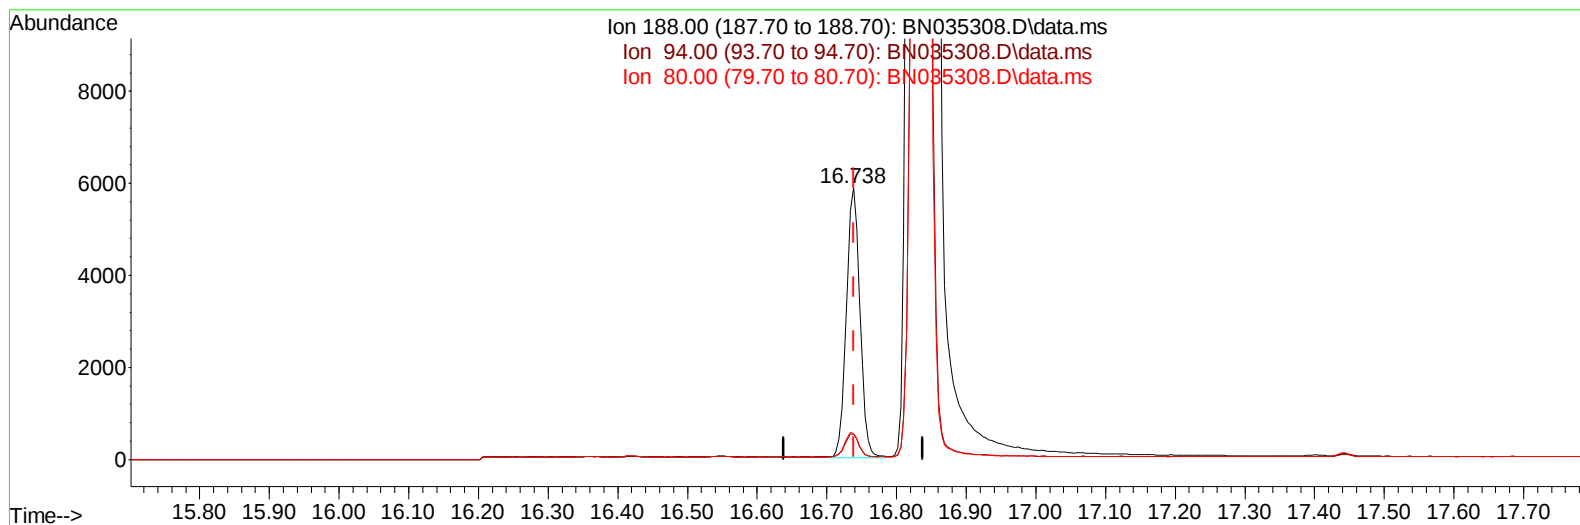

TIC: BN035308.D\data.ms

(13) Phenanthrene-d10 (I)

16.738min (-0.000) 0.40 ng/ul m

response 7906

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.00	9.29#
80.00	7.60	9.68#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035308.D
Acq On : 26 Nov 2024 09:59
Operator : RC/JU
Sample : P4875-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2A24

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

Quant Time: Nov 26 22:12:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

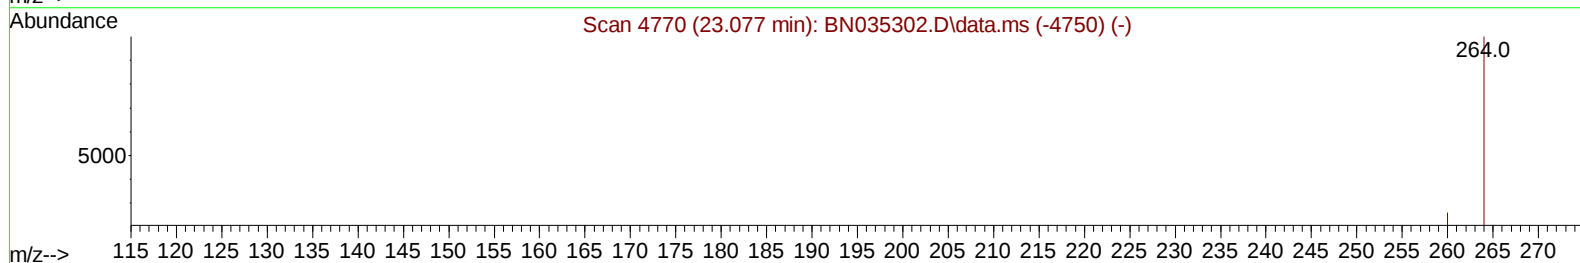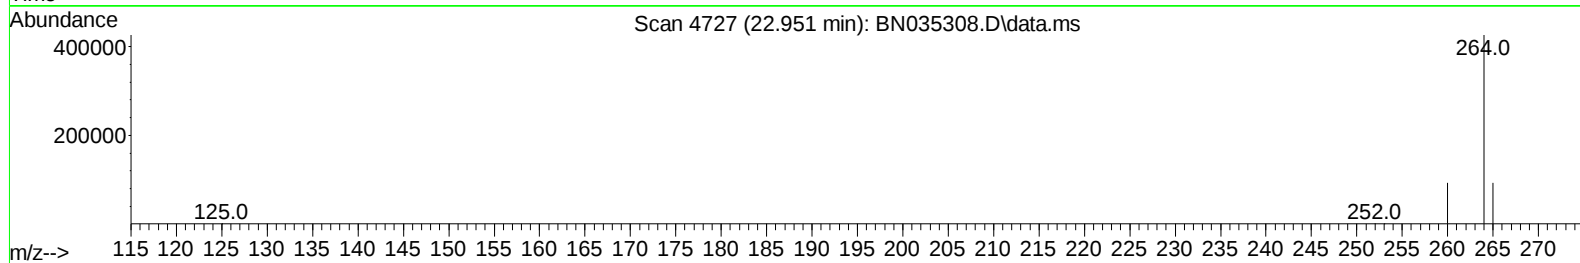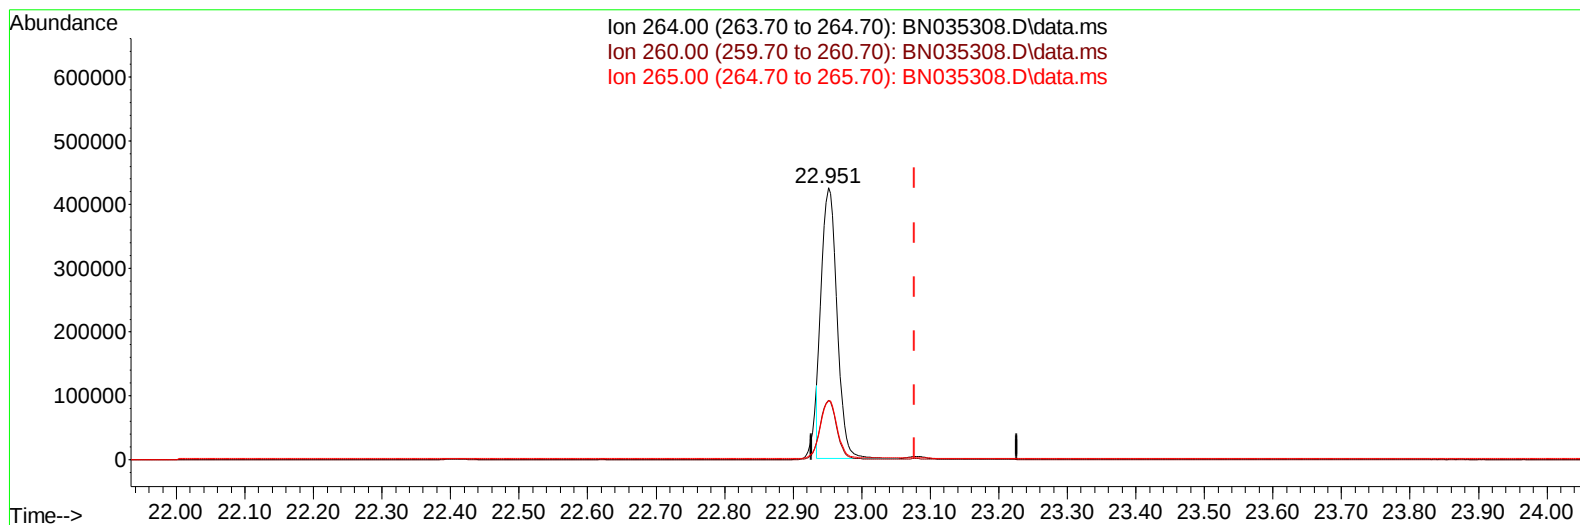

TIC: BN035308.D\data.ms

(23) Perylene-d12 (I)

22.951min (-0.126) 0.40 ng/u1

response 674243

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	21.86
265.00	75.50	21.69#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035308.D
Acq On : 26 Nov 2024 09:59
Operator : RC/JU
Sample : P4875-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2A24

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:12:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

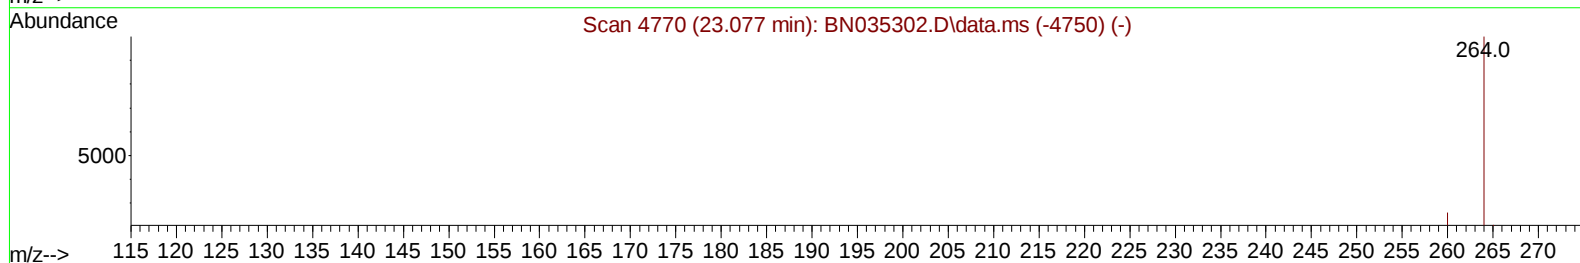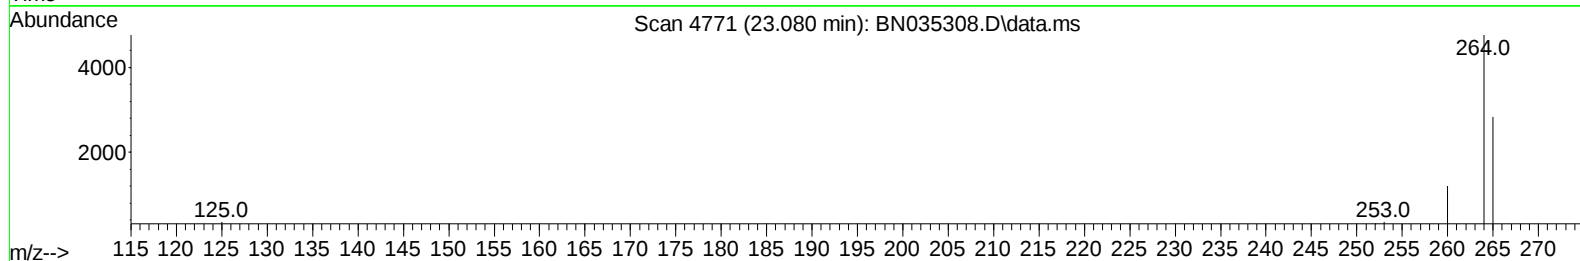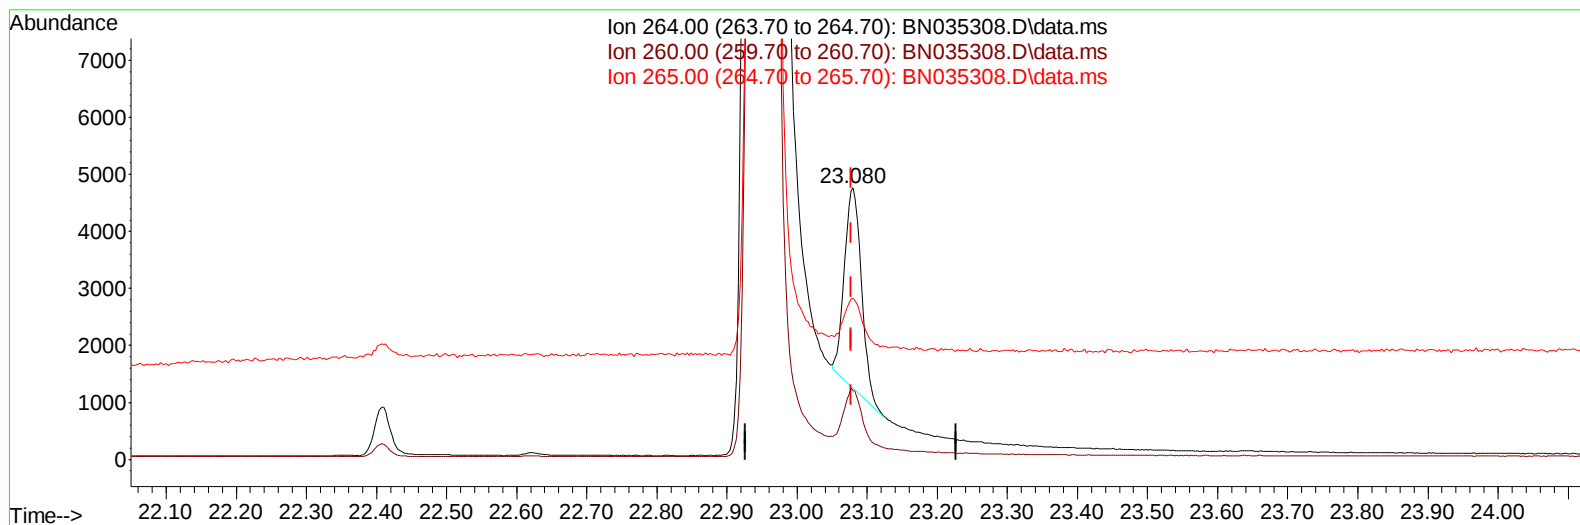

TIC: BN035308.D\data.ms

(23) Perylene-d12 (I)

23.080min (+ 0.003) 0.40 ng/ul m

response 5876

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	25.40
265.00	75.50	59.35#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
 Data File : BN035308.D
 Acq On : 26 Nov 2024 09:59
 Operator : RC/JU
 Sample : P4875-22
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2A24

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2024
 Supervised By :mohammad ahmed 11/28/2024

Quant Time: Nov 26 22:12:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN11624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 26 06:09:15 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.309	152		2861	0.400	ng/ul	0.00
4) Naphthalene-d8	10.058	136		6920	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.972	164		3919	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.738	188		7906m	0.400	ng/ul	0.00
17) Chrysene-d12	20.982	240		6097	0.400	ng/ul	# 0.00
23) Perylene-d12	23.080	264		5876m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	2.972	96		14095	5.390	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.664	152		2982	0.294	ng/ul	0.00
18) Fluoranthene-d10	18.791	212		7563	0.450	ng/ul	0.00
Target Compounds							Qvalue
5) Naphthalene	10.108	128		357	0.020	ng/ul#	61

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035308.D
Acq On : 26 Nov 2024 09:59
Operator : RC/JU
Sample : P4875-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2A24

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:12:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

