




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035309.D
Acq On : 26 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y4

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:12:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

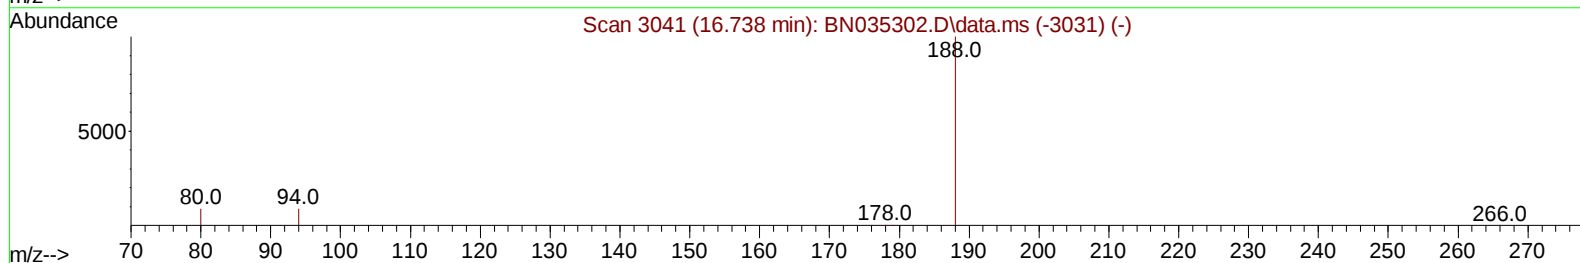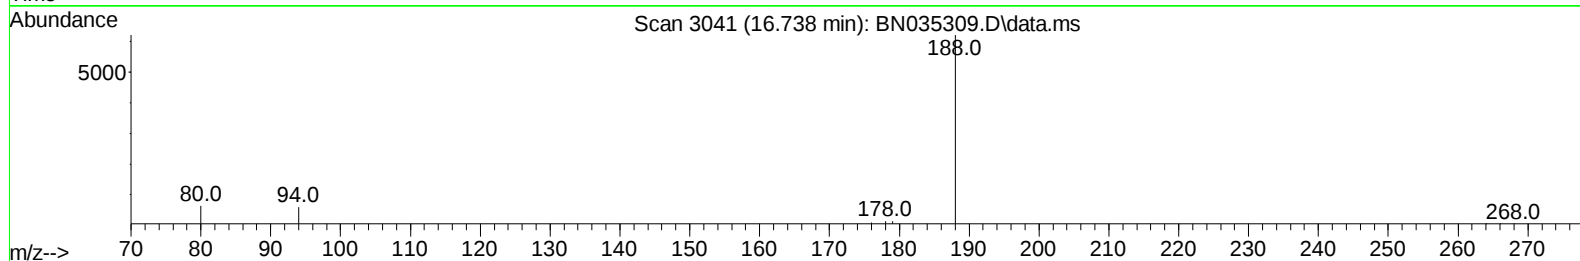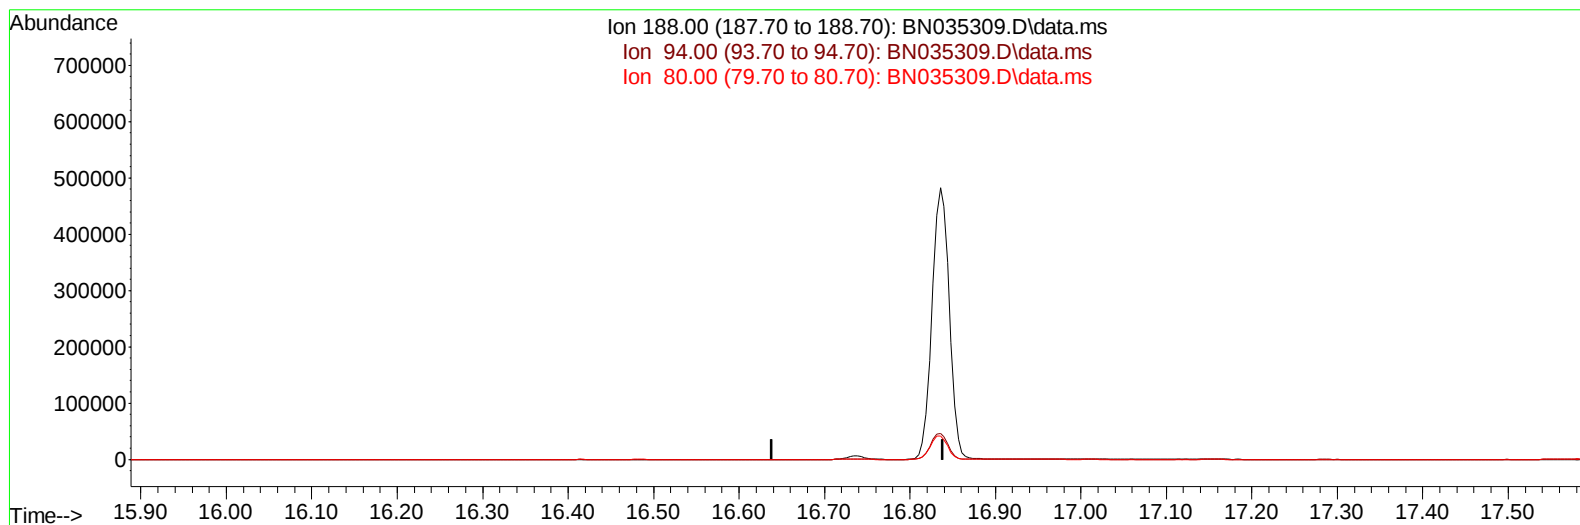

TIC: BN035309.D\data.ms

(13) Phenanthrene-d10 (I)

16.738min (-16.738) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	7.00	0.00#
80.00	7.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035309.D
Acq On : 26 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y4

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:12:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

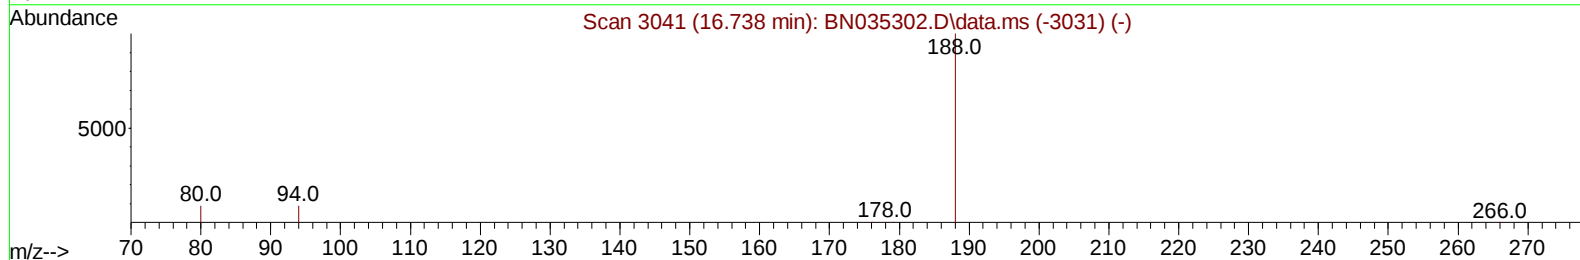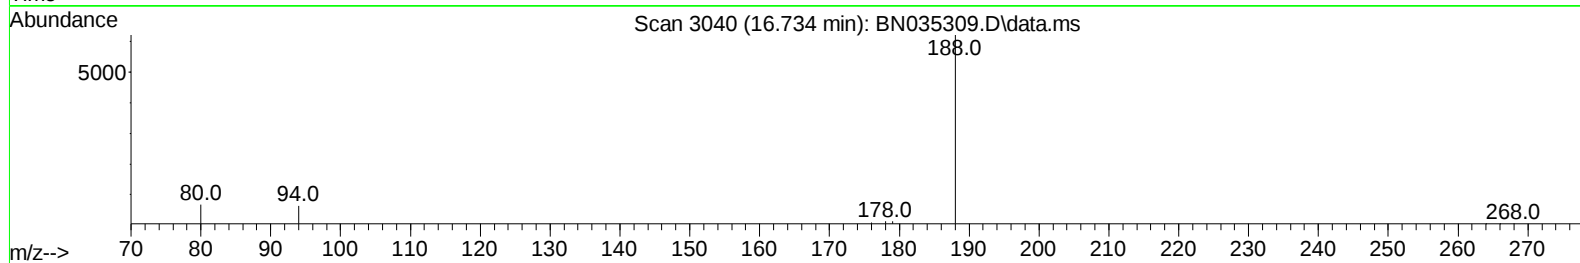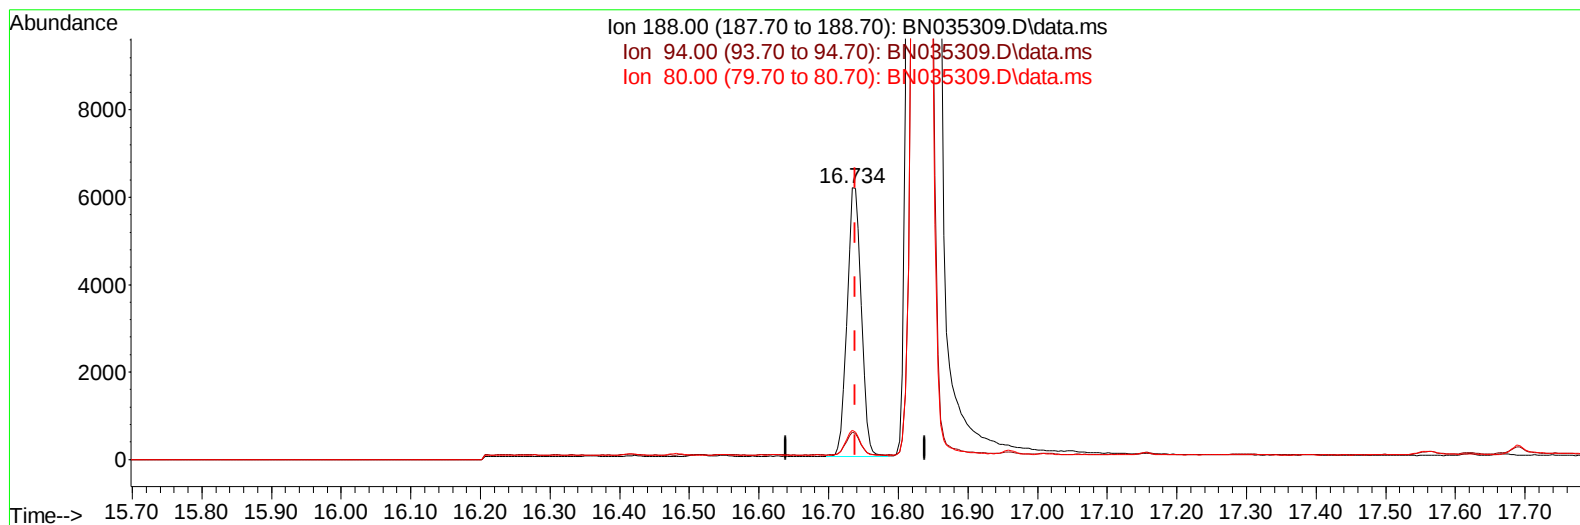

TIC: BN035309.D\data.ms

(13) Phenanthrene-d10 (I)

16.734min (-0.004) 0.40 ng/u1 m

response 8708

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.00	10.02#
80.00	7.60	10.72#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035309.D
Acq On : 26 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y4

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:12:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

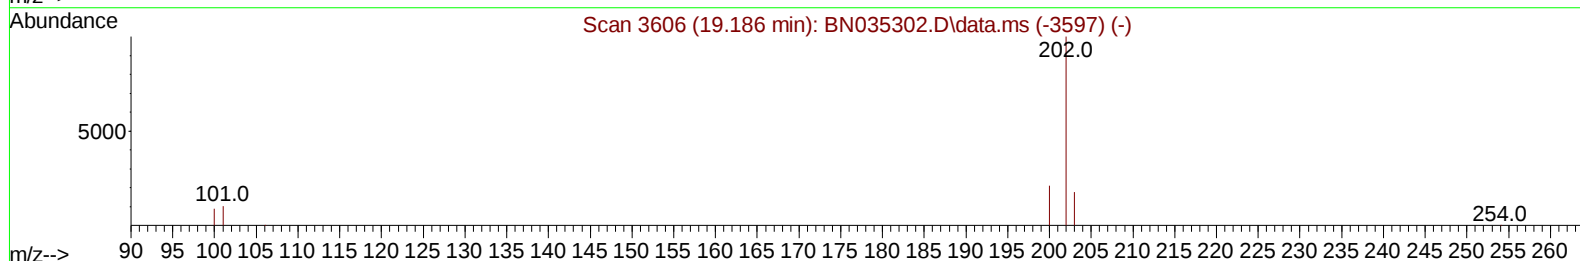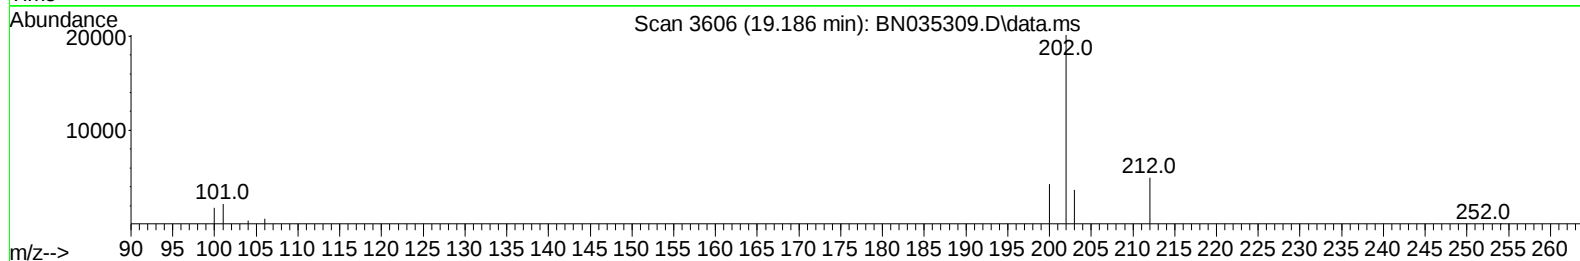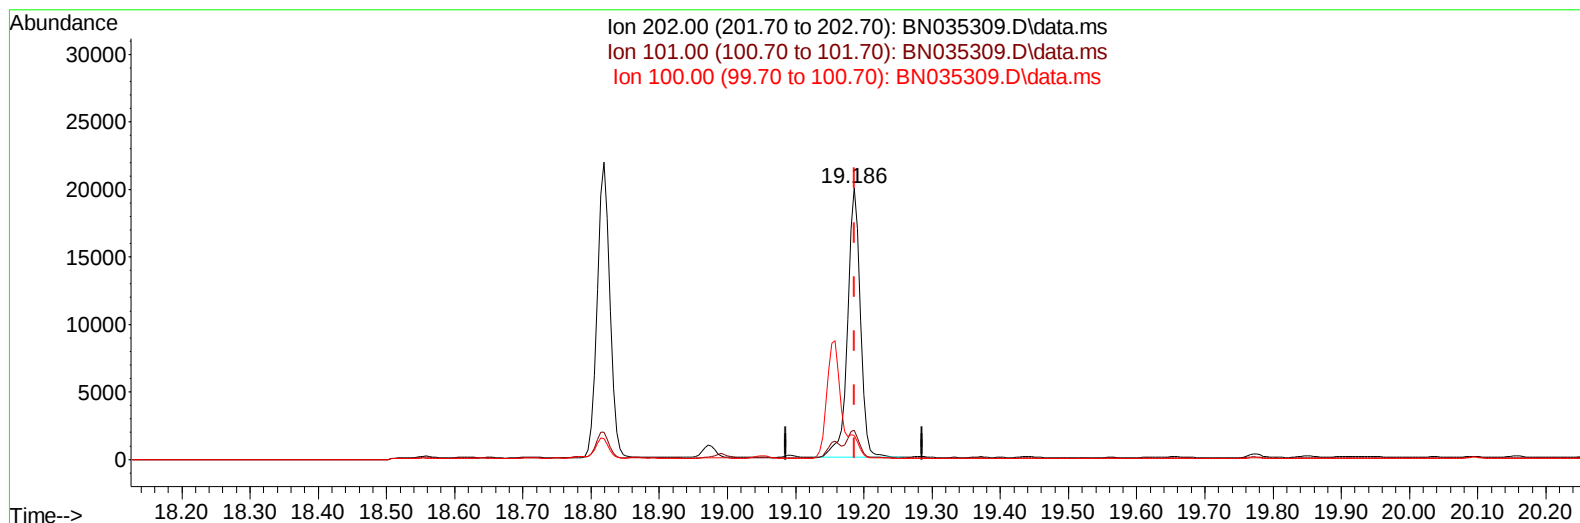

TIC: BN035309.D\data.ms

(20) Pyrene

19.186min (-0.000) 0.96 ng/u1

response 25828

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	7.80	10.80#
100.00	6.40	8.88#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035309.D
Acq On : 26 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y4

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:12:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

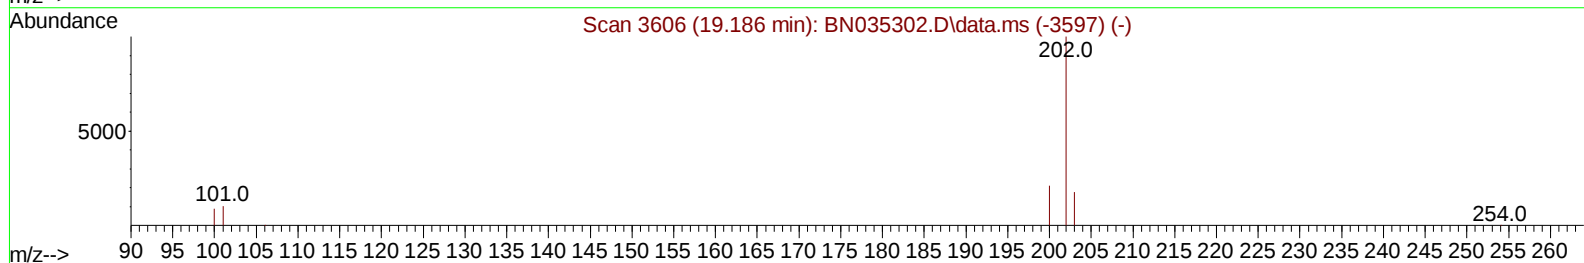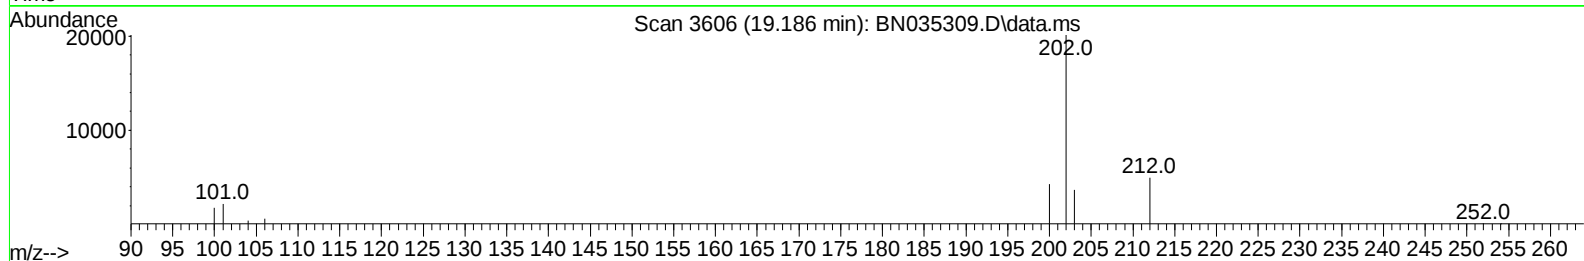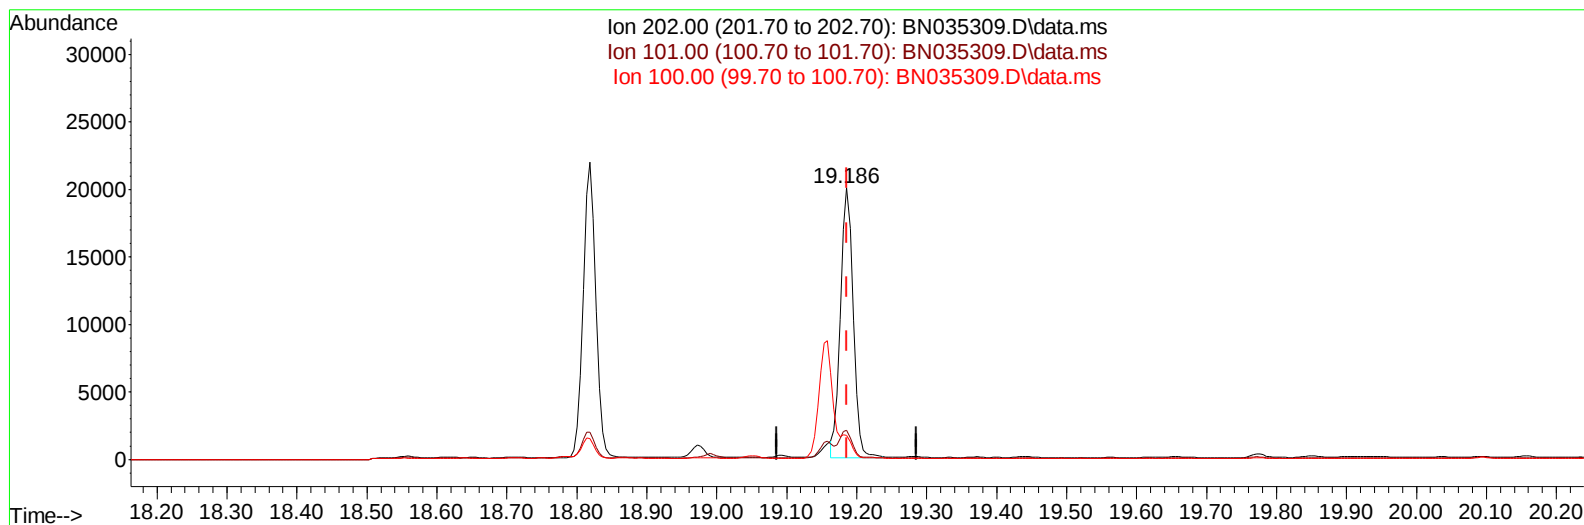

TIC: BN035309.D\data.ms

(20) Pyrene

19.186min (-0.000) 0.92 ng/u1 m

response 24762

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	7.80	10.80#
100.00	6.40	8.88#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035309.D
Acq On : 26 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y4

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:12:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

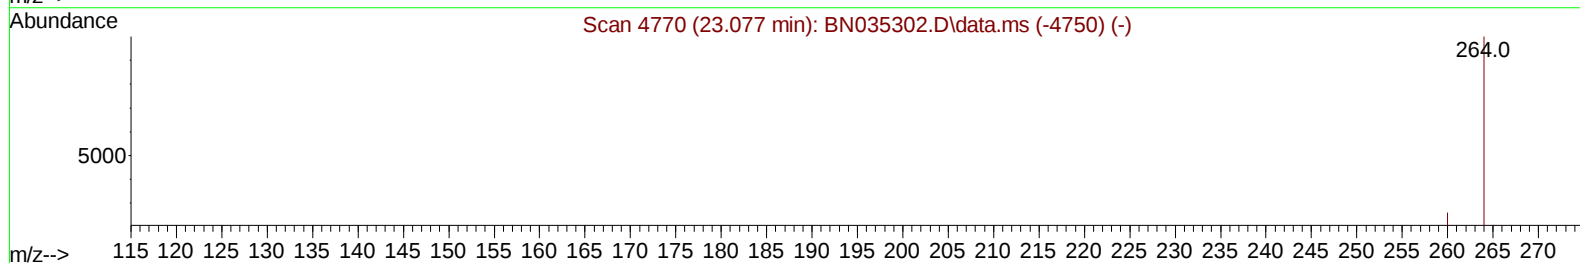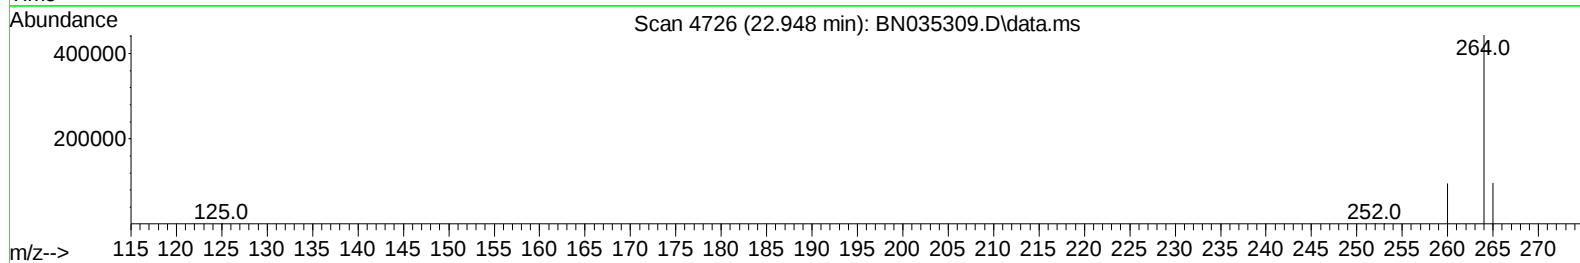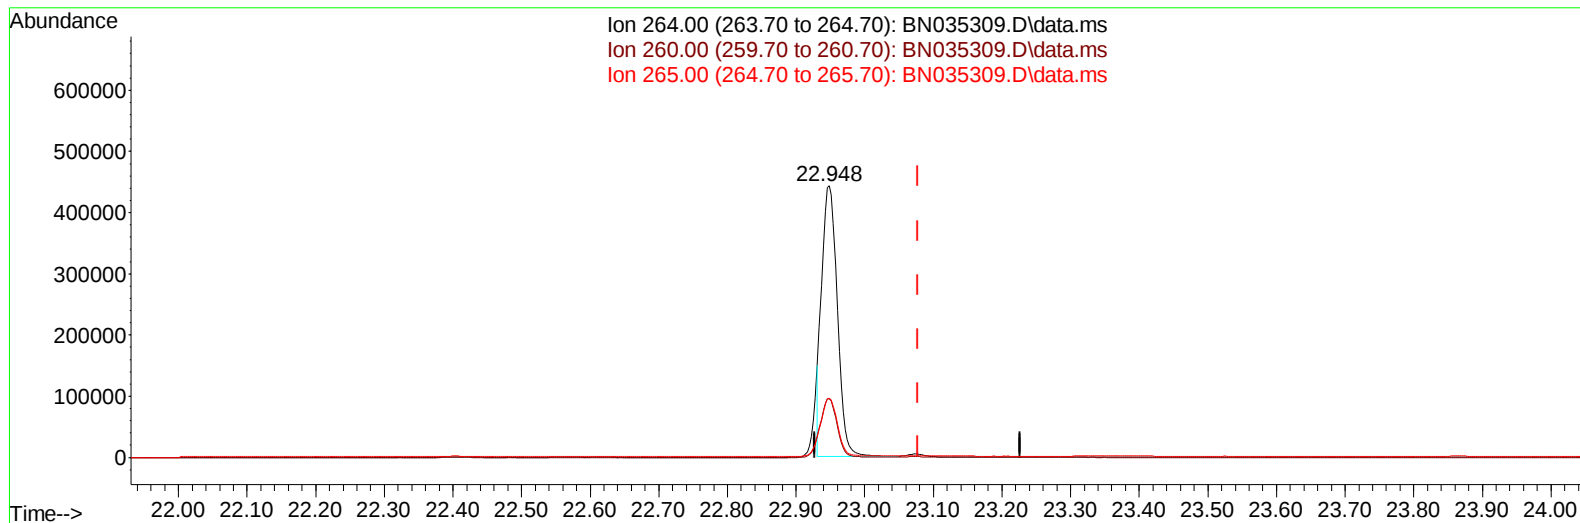

TIC: BN035309.D\data.ms

(23) Perylene-d12 (I)

22.948min (-0.129) 0.40 ng/u1

response 696802

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	21.62
265.00	75.50	21.93#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035309.D
Acq On : 26 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y4

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:12:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

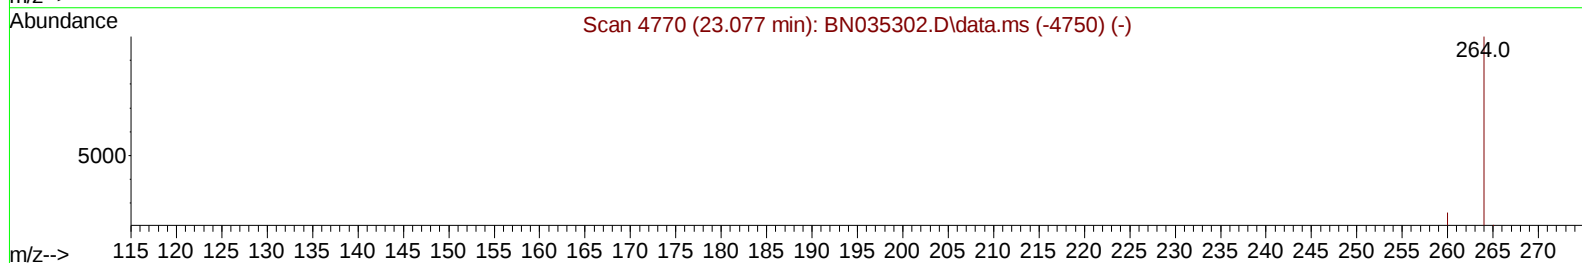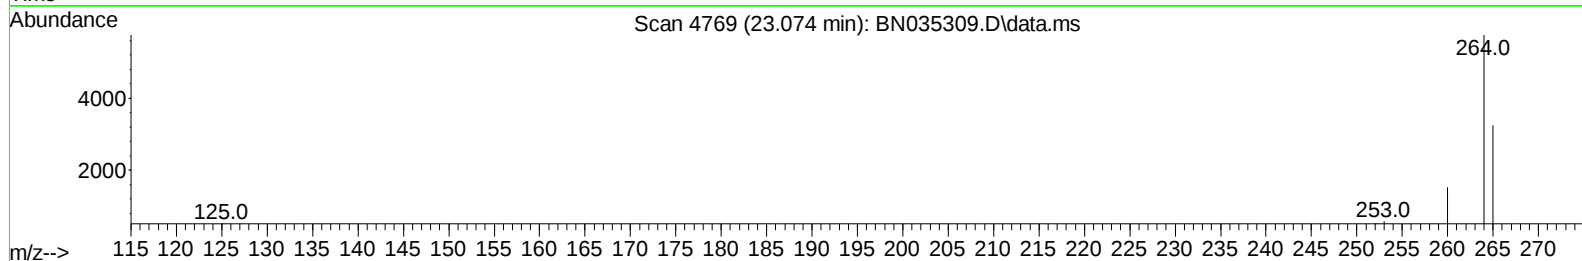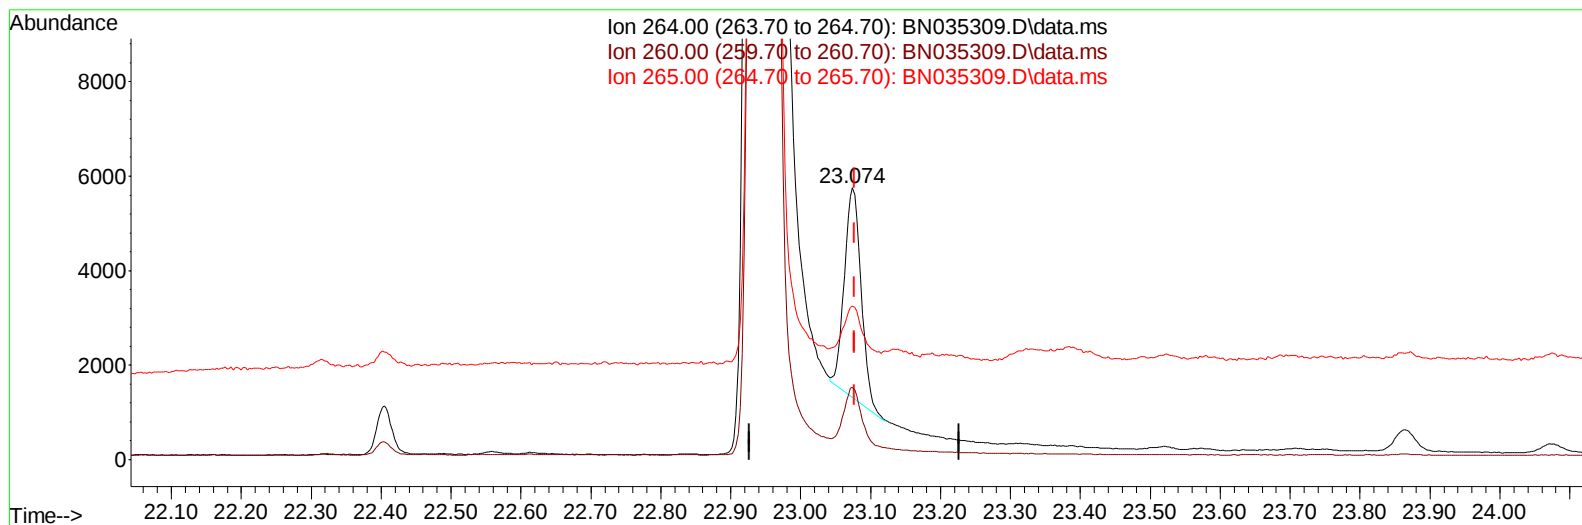

TIC: BN035309.D\data.ms

(23) Perylene-d12 (I)

23.074min (-0.003) 0.40 ng/ul m

response 7319

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	26.60
265.00	75.50	56.53#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035309.D
Acq On : 26 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y4

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:12:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

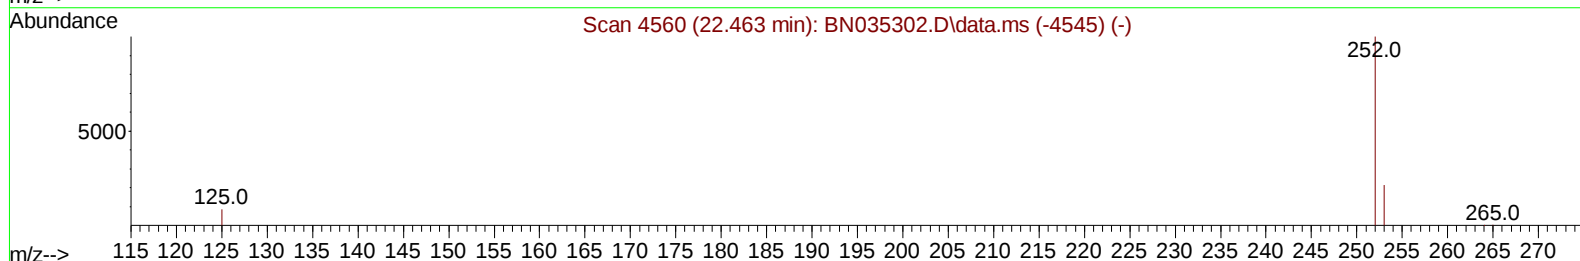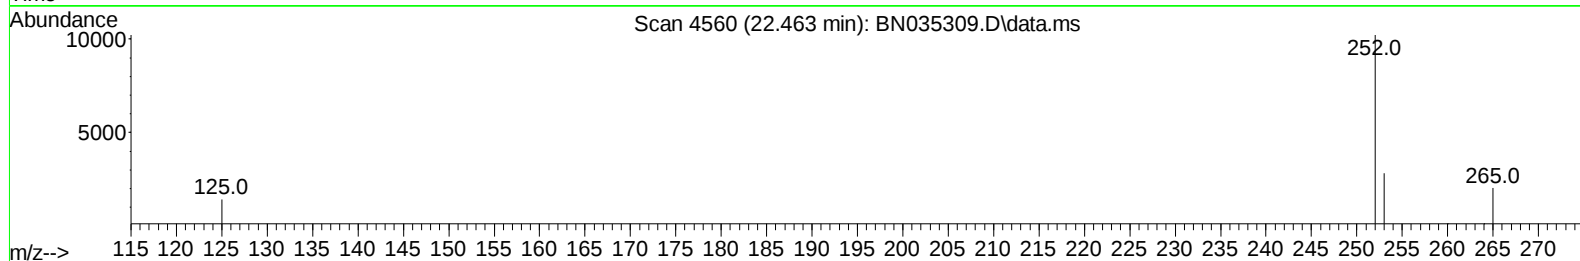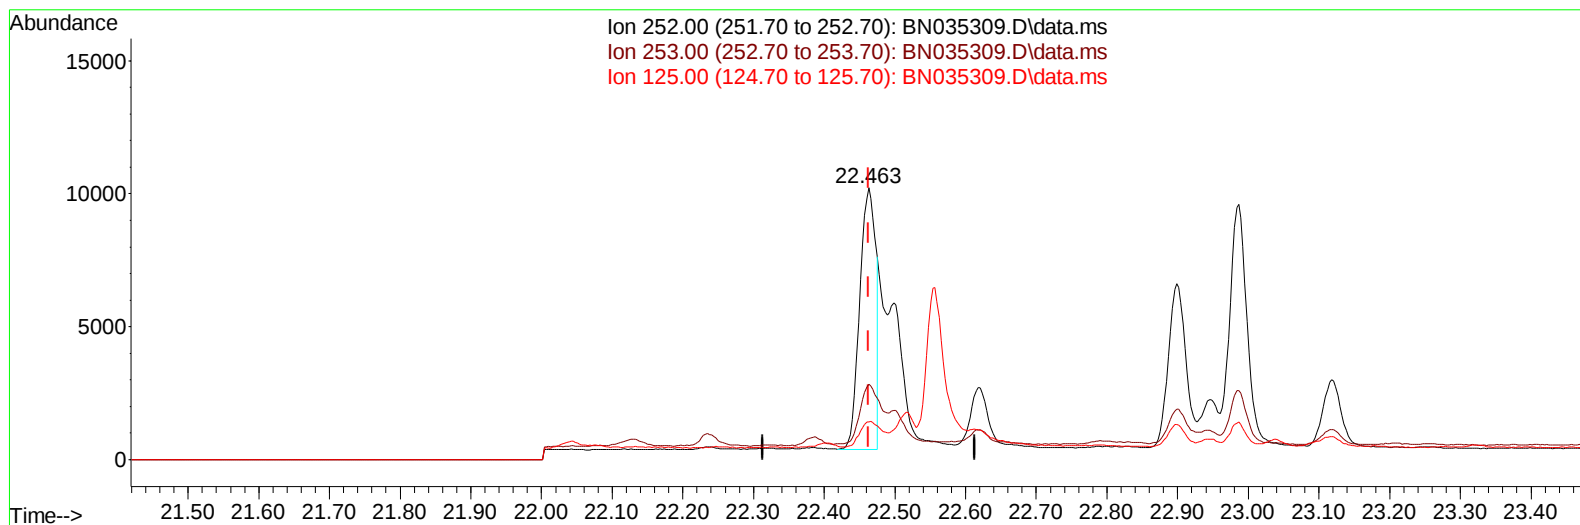

TIC: BN035309.D\data.ms

(24) Benzo(b)fluoranthene

22.463min (-0.000) 0.64 ng/u1

response 15391

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.00	27.64
125.00	9.70	13.86
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035309.D
Acq On : 26 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

Quant Time: Nov 26 22:12:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

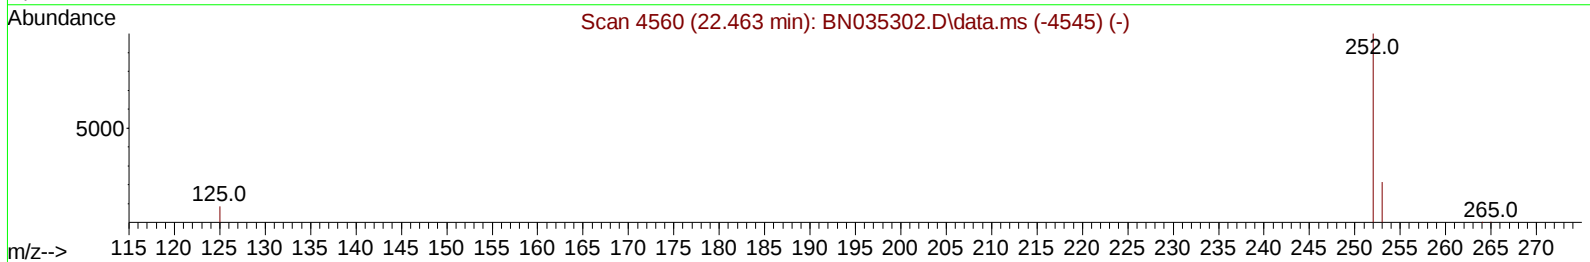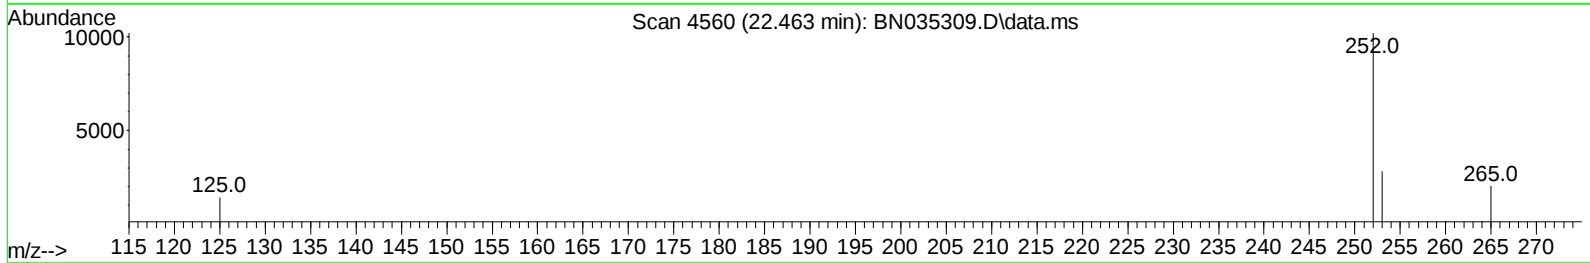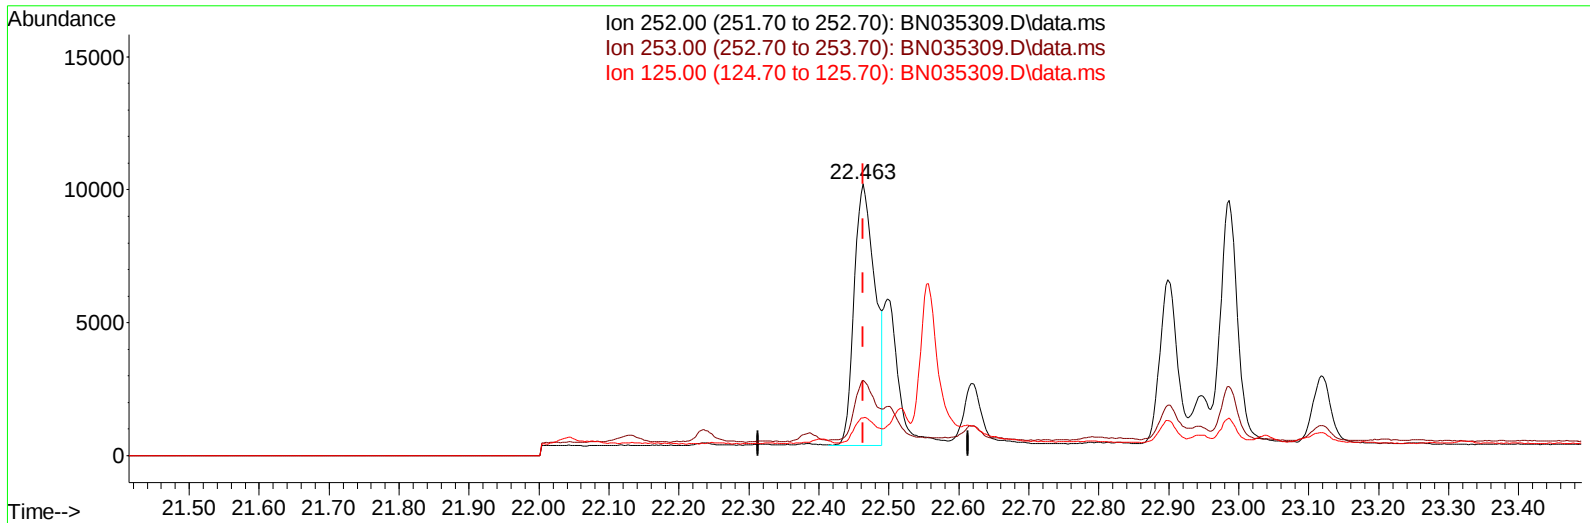

TIC: BN035309.D\data.ms

(24) Benzo(b)fluoranthene

22.463min (-0.000) 0.84 ng/u1 m

response 20379

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.00	27.64
125.00	9.70	13.86
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035309.D
Acq On : 26 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y4

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:12:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

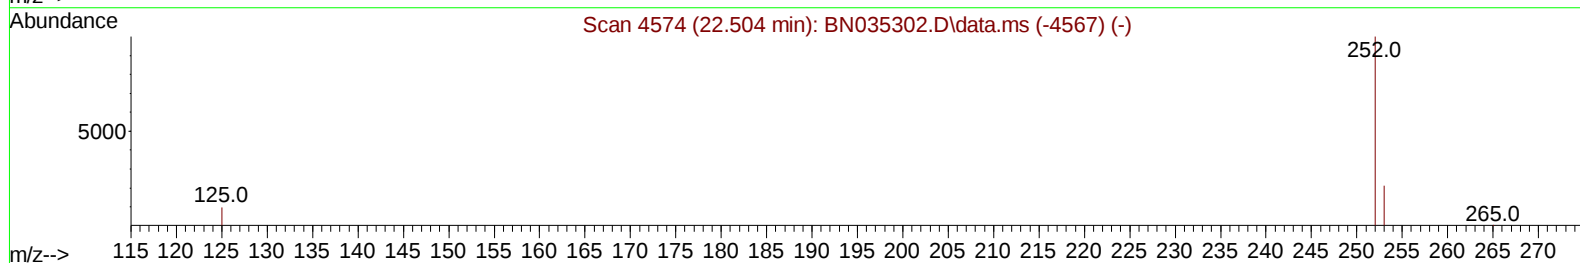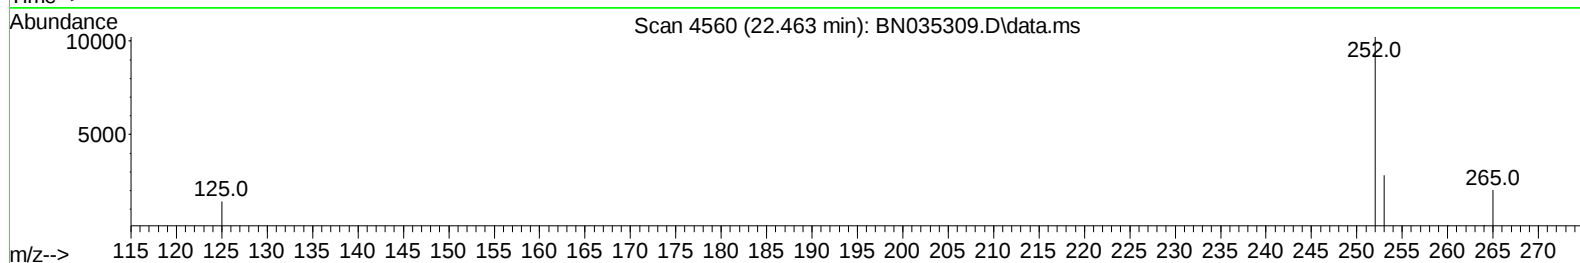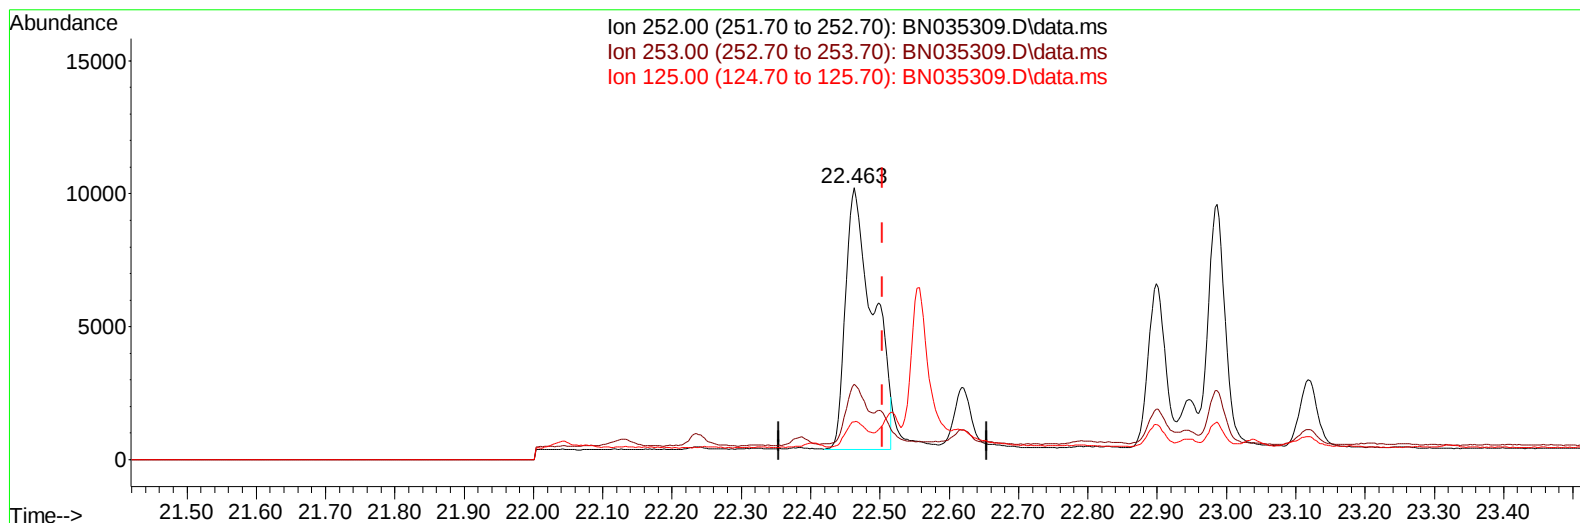

TIC: BN035309.D\data.ms

(25) Benzo(k)fluoranthene

22.463min (-0.041) 1.09 ng/u1

response 27109

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.20	27.64
125.00	10.70	13.86#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035309.D
Acq On : 26 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y4

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:12:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

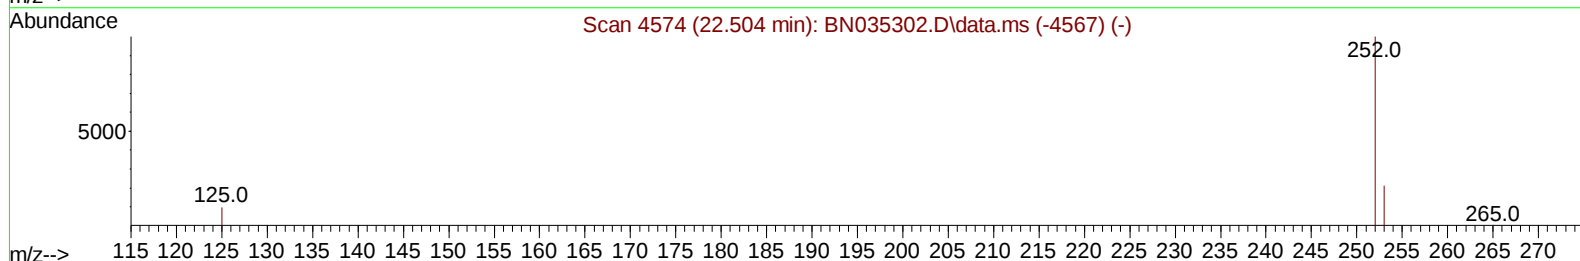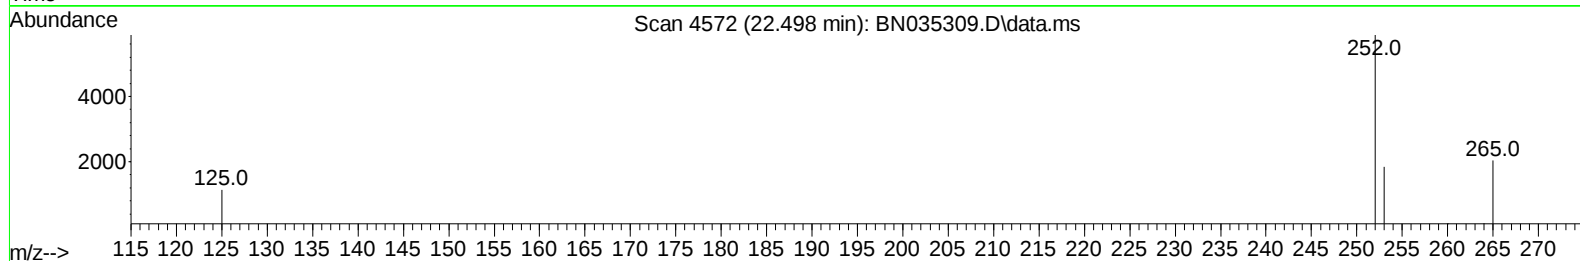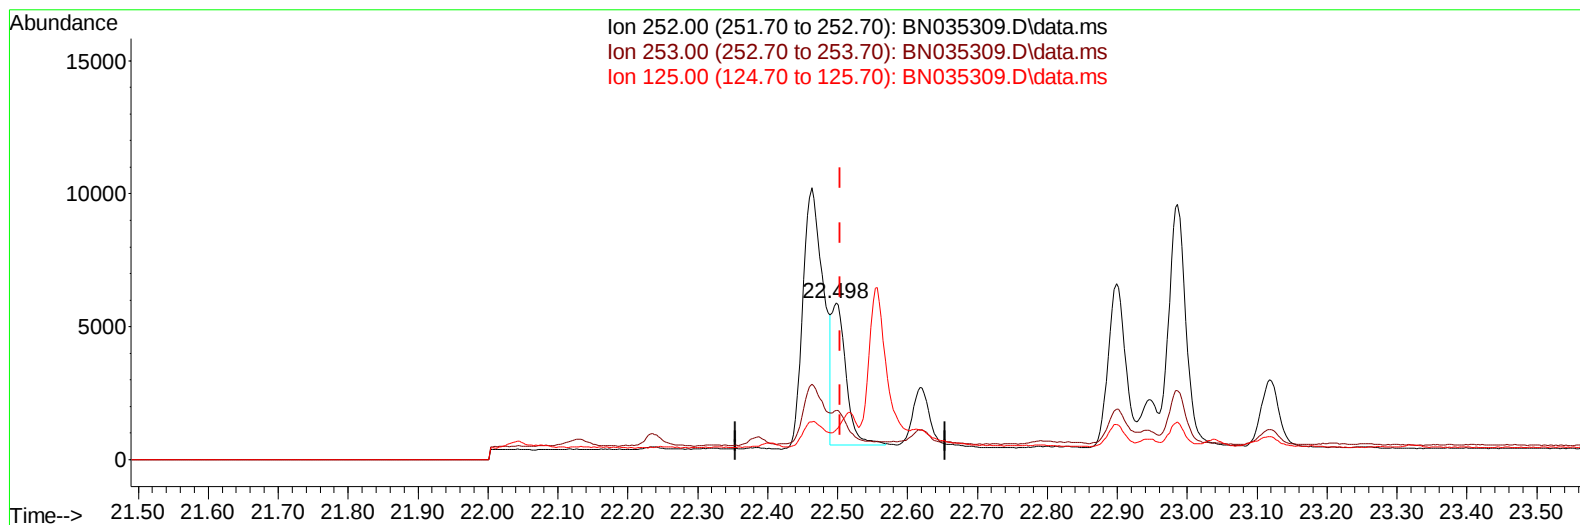

TIC: BN035309.D\data.ms

(25) Benzo(k)fluoranthene

22.498min (-0.006) 0.30 ng/u1 m

response 7507

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.20	31.30
125.00	10.70	19.28#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035309.D
Acq On : 26 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y4

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:12:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

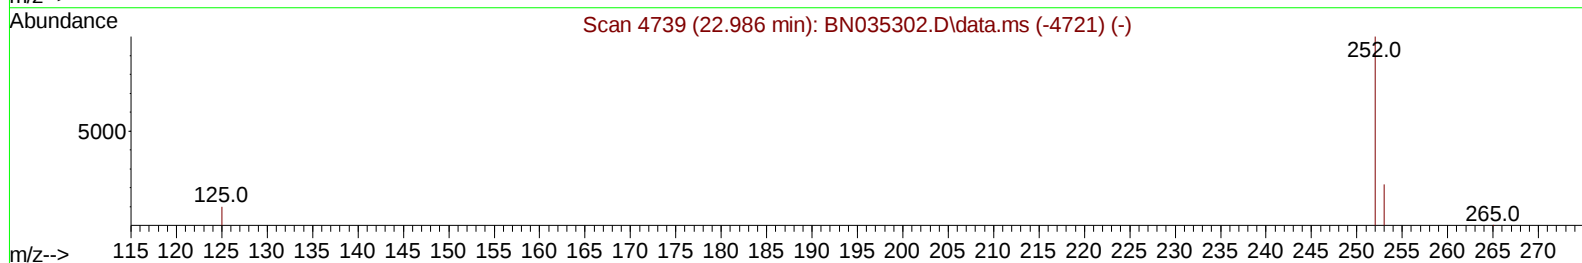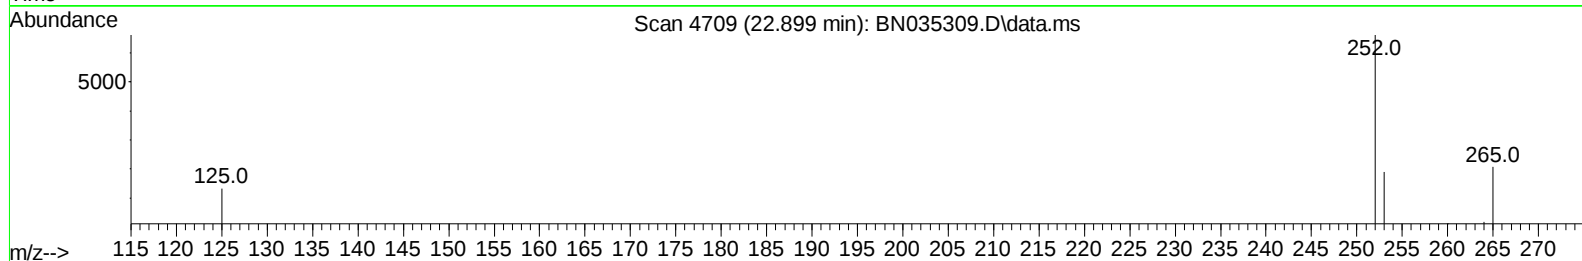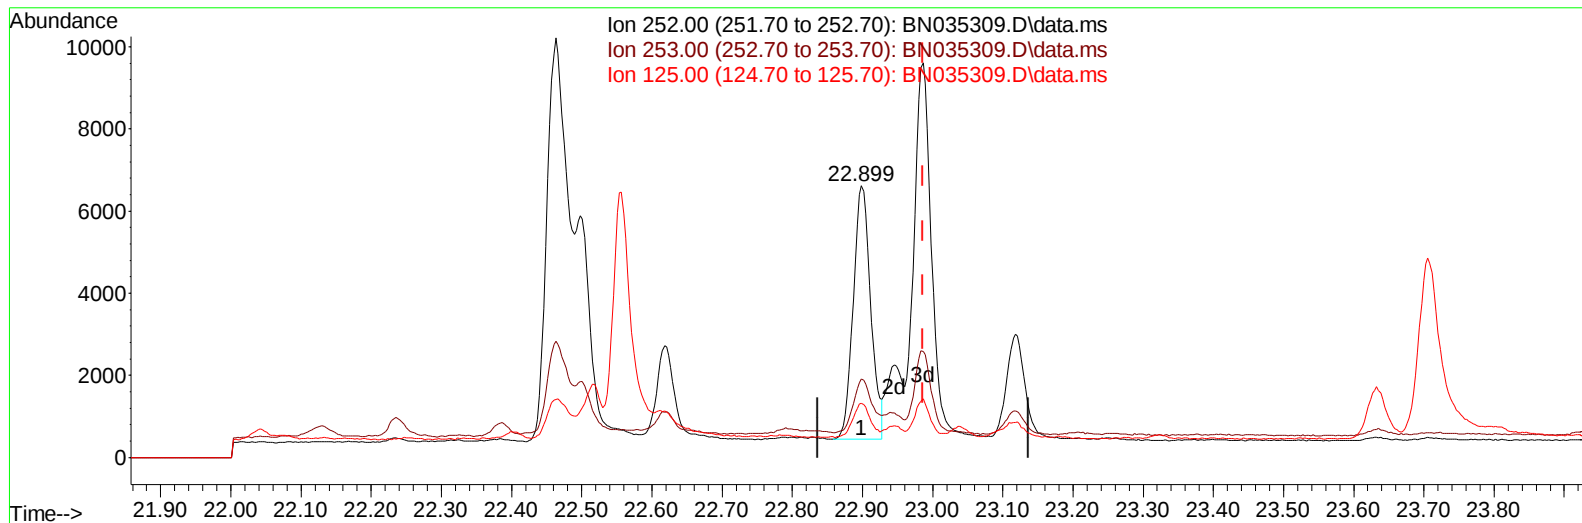

TIC: BN035309.D\data.ms

(26) Benzo(a)pyrene (C)

22.899min (-0.088) 0.49 ng/u1

response 10742

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	28.60	28.82
125.00	11.80	20.03#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035309.D
Acq On : 26 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y4

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:12:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

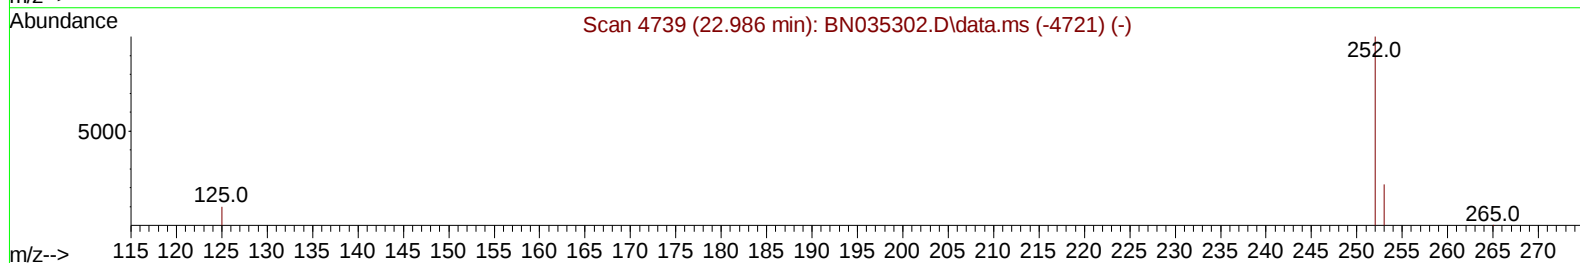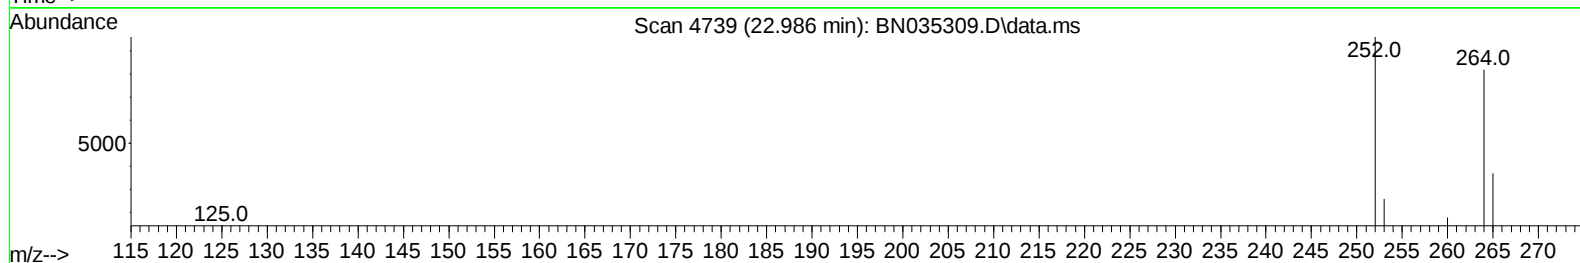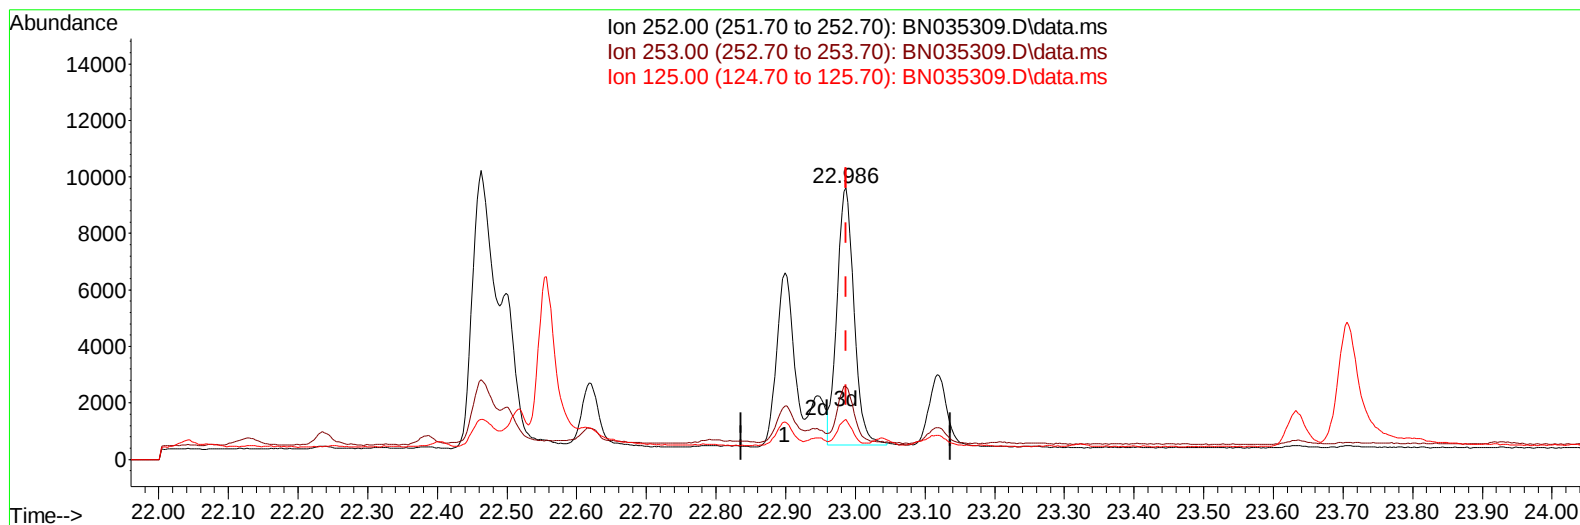

TIC: BN035309.D\data.ms

(26) Benzo(a)pyrene (C)

22.986min (-0.000) 0.70 ng/u1 m

response 15400

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	28.60	26.88
125.00	11.80	14.79#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035309.D
Acq On : 26 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

Quant Time: Nov 26 22:12:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

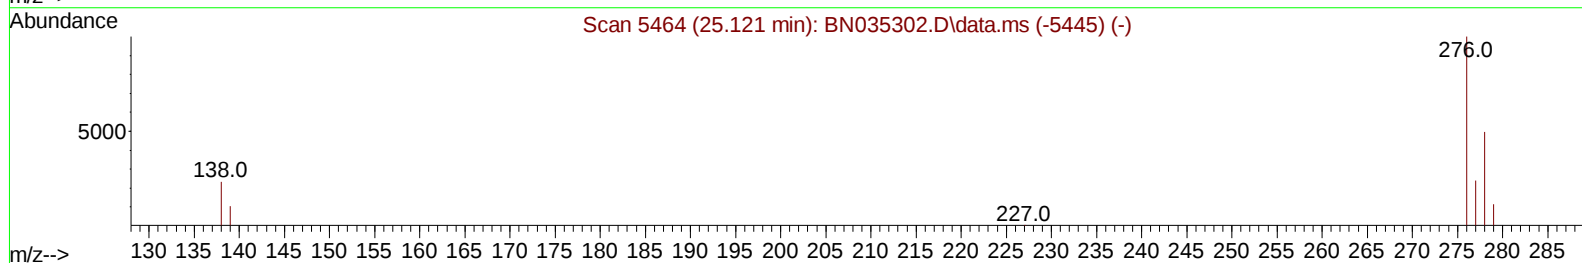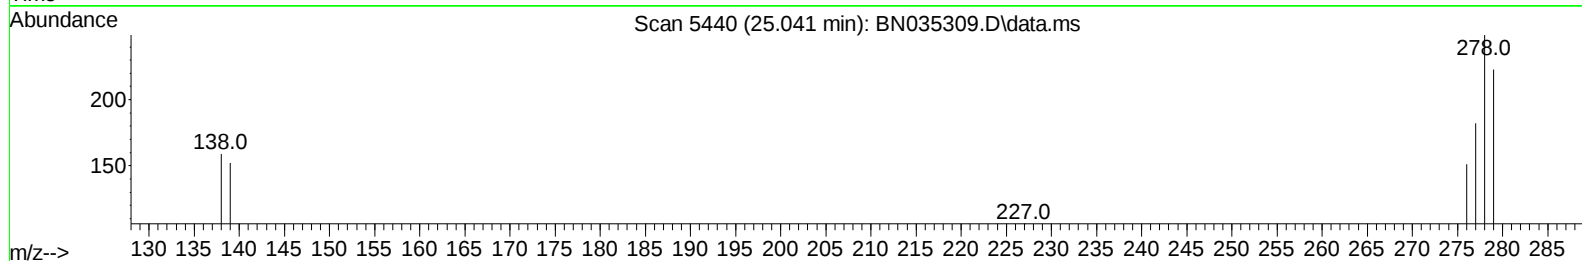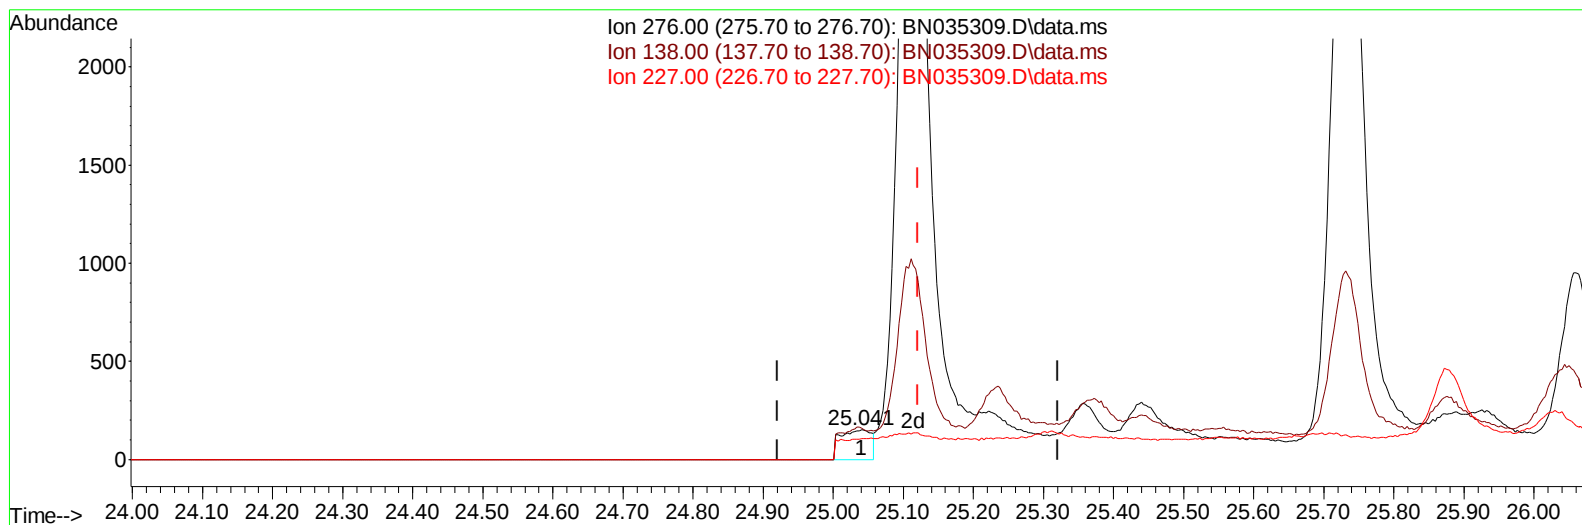

TIC: BN035309.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

25.041min (-0.081) 0.02 ng/u1

response 458

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	17.30	121.40#
227.00	0.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035309.D
Acq On : 26 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y4

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:12:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

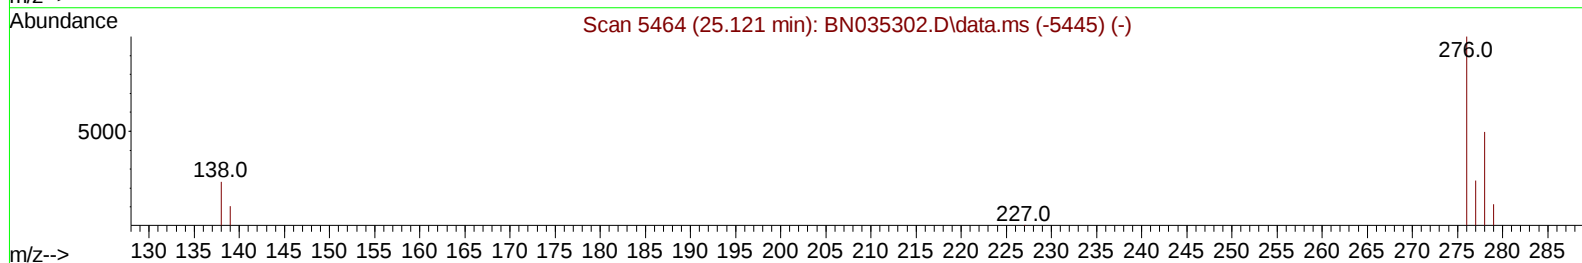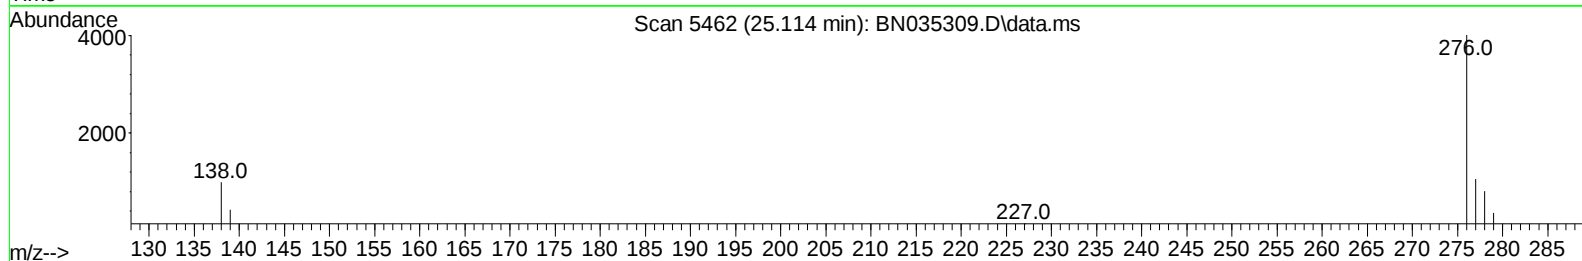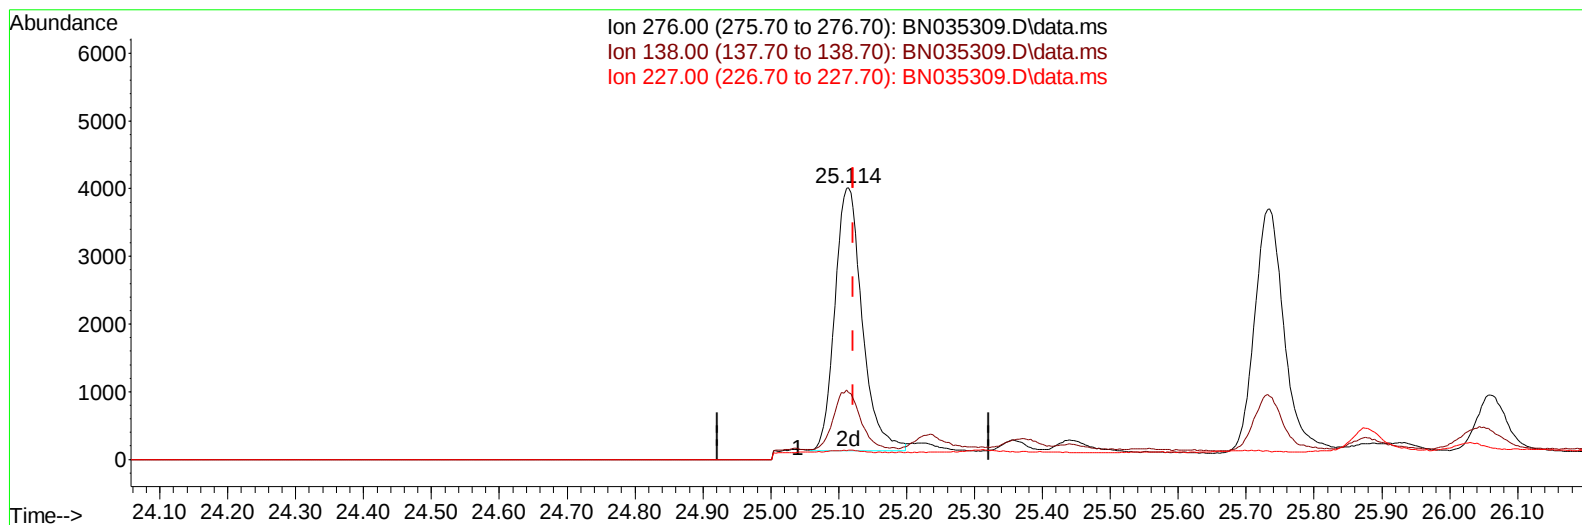

TIC: BN035309.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

25.114min (-0.007) 0.36 ng/ul m

response 10873

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	17.30	5.11#
227.00	0.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035309.D
Acq On : 26 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y4

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:12:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

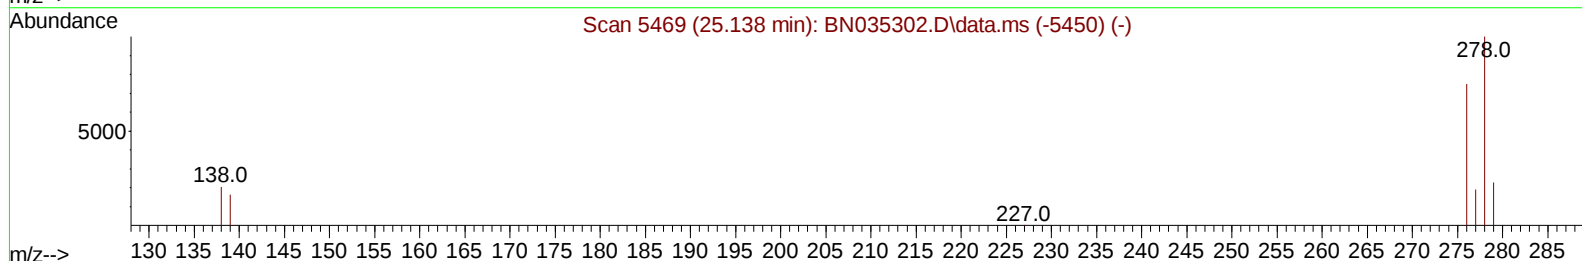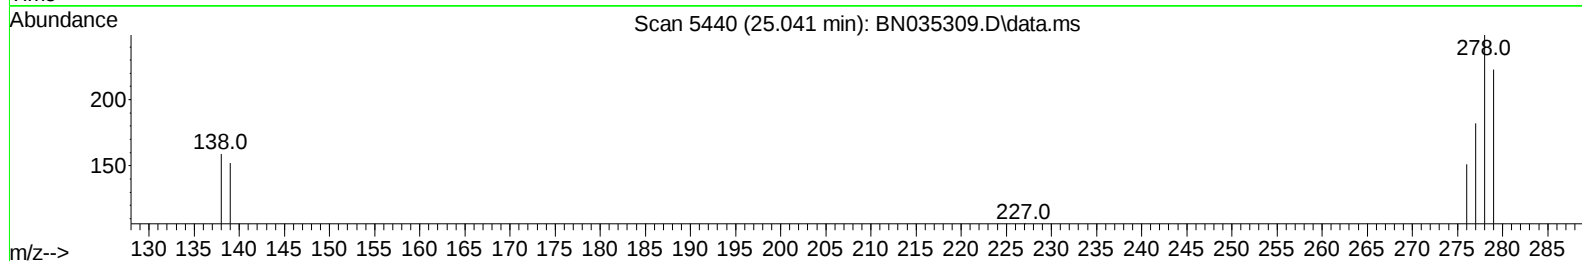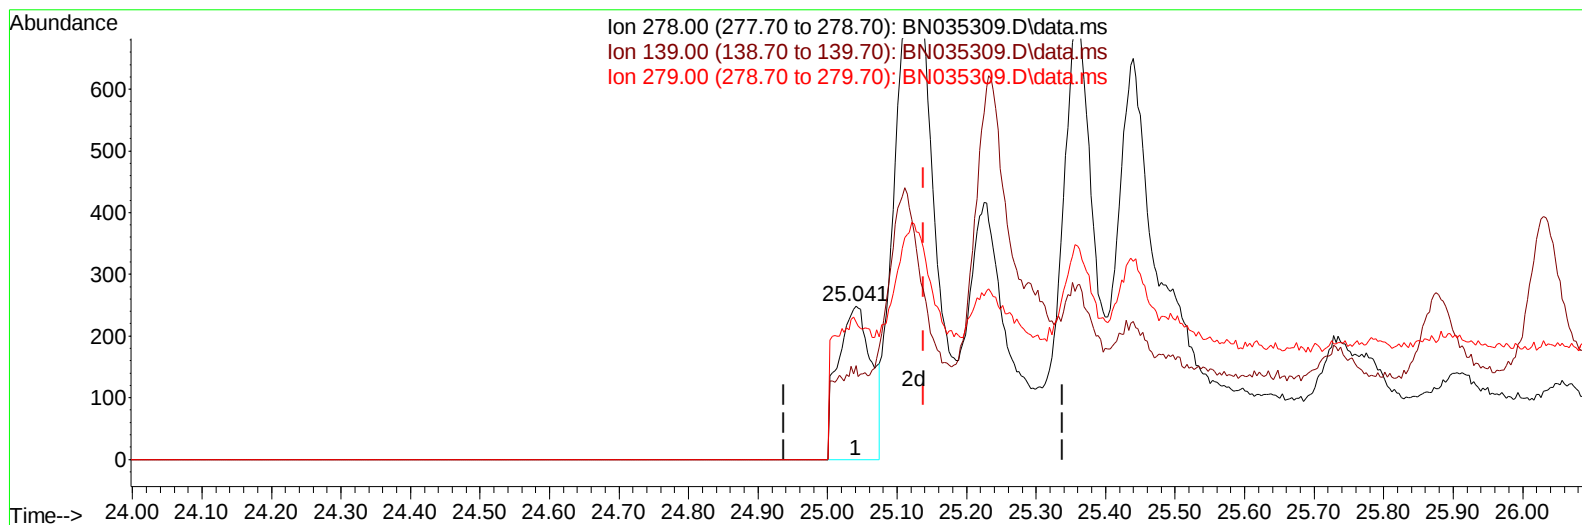

TIC: BN035309.D\data.ms

(28) Dibenzo(a,h)anthracene

25.041min (-0.097) 0.04 ng/u1

response 820

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	13.40	61.04#
279.00	28.50	89.56#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035309.D
Acq On : 26 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y4

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:12:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

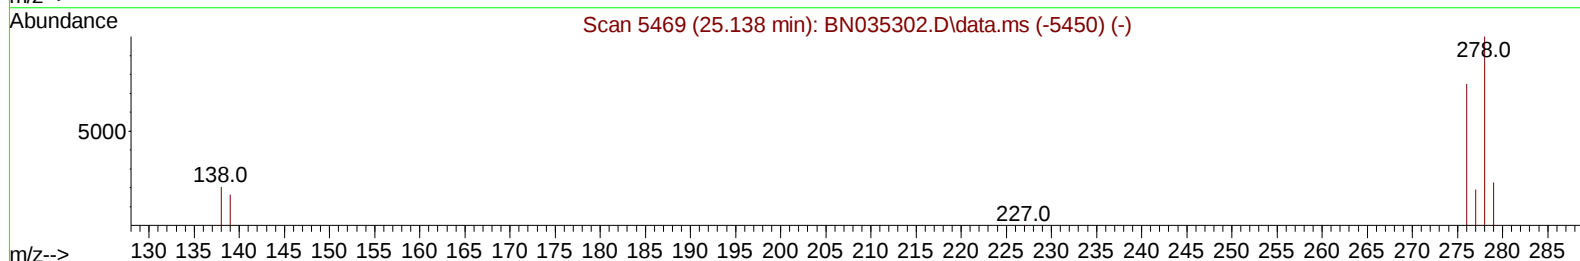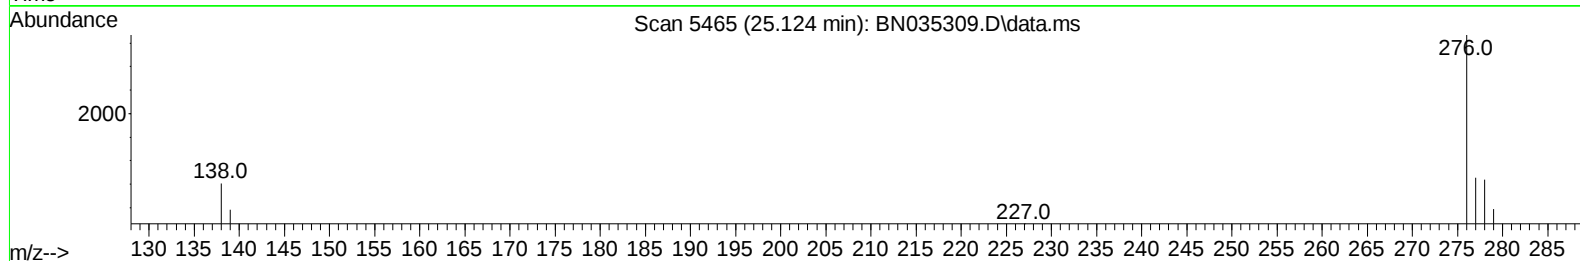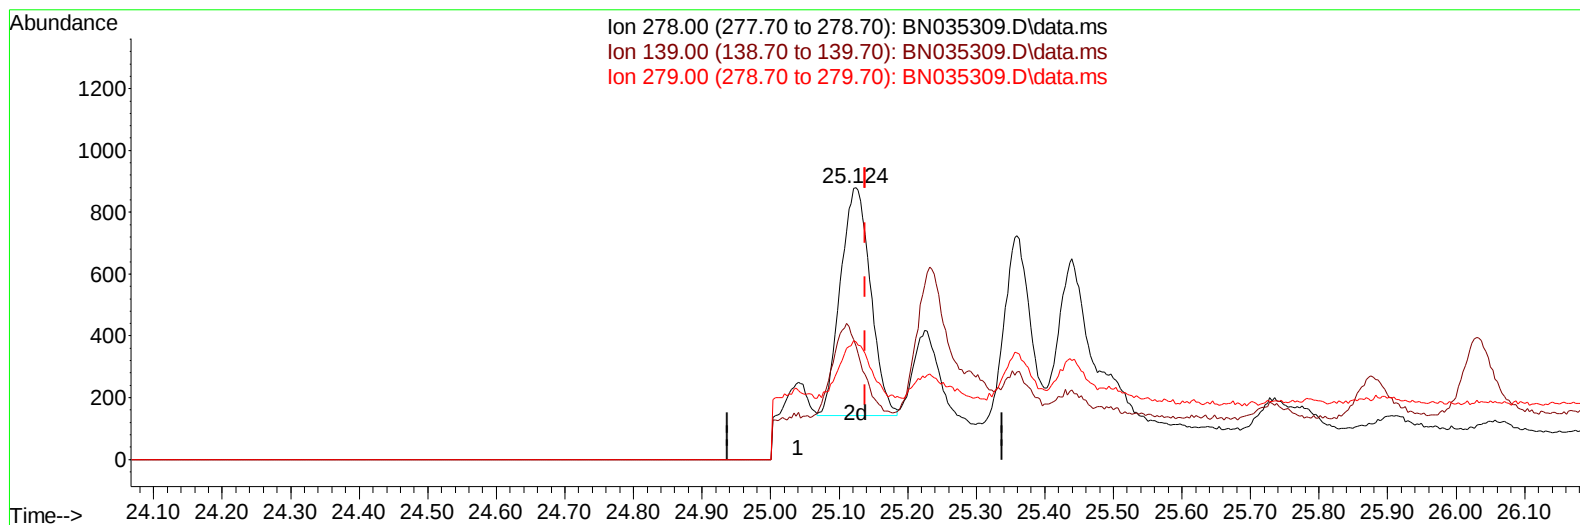

TIC: BN035309.D\data.ms

(28) Dibenzo(a,h)anthracene

25.124min (-0.013) 0.10 ng/ul m

response 2244

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	13.40	41.64#
279.00	28.50	43.34#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035309.D
Acq On : 26 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y4

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:12:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

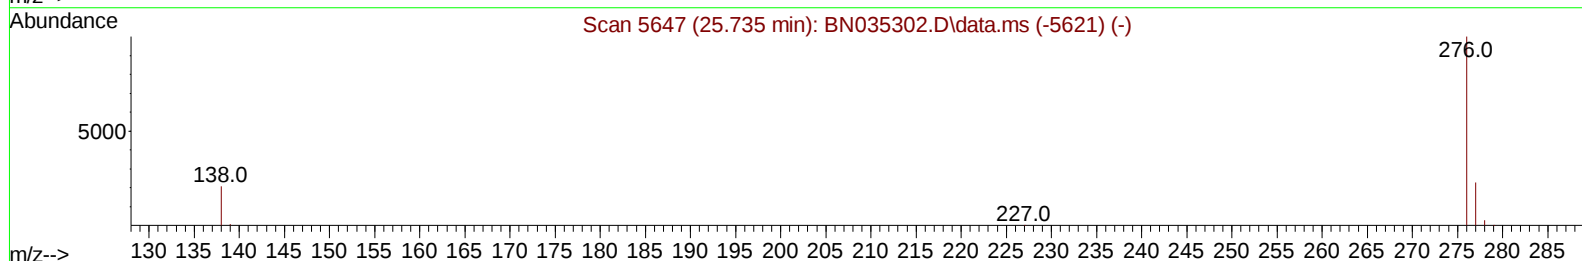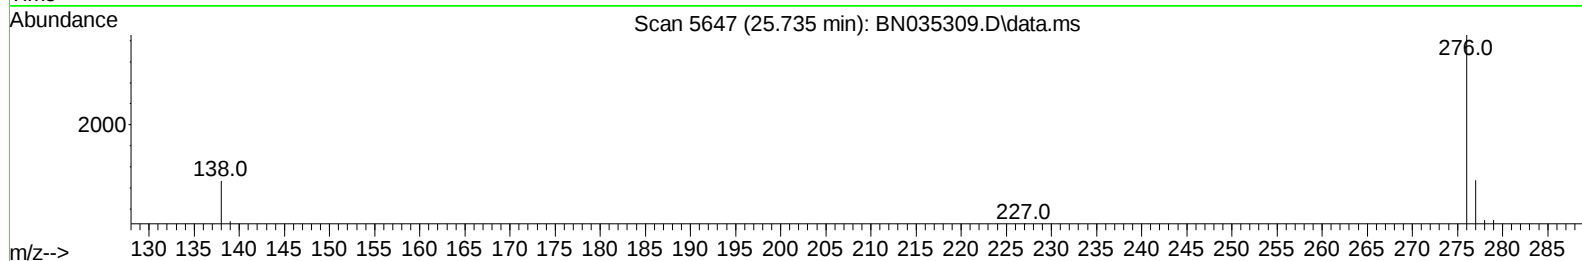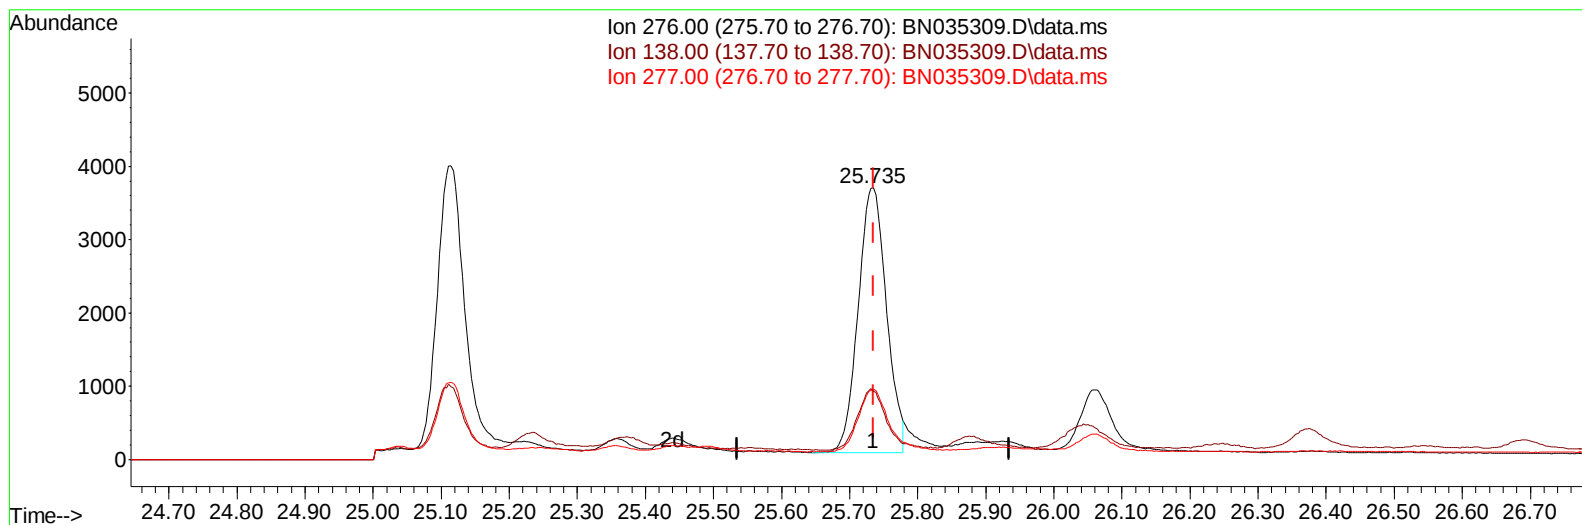

TIC: BN035309.D\data.ms

(29) Benzo(g,h,i)perylene

25.735min (-0.000) 0.45 ng/u1

response 10478

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	16.30	25.20#
277.00	25.60	25.72
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035309.D
Acq On : 26 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y4

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:12:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

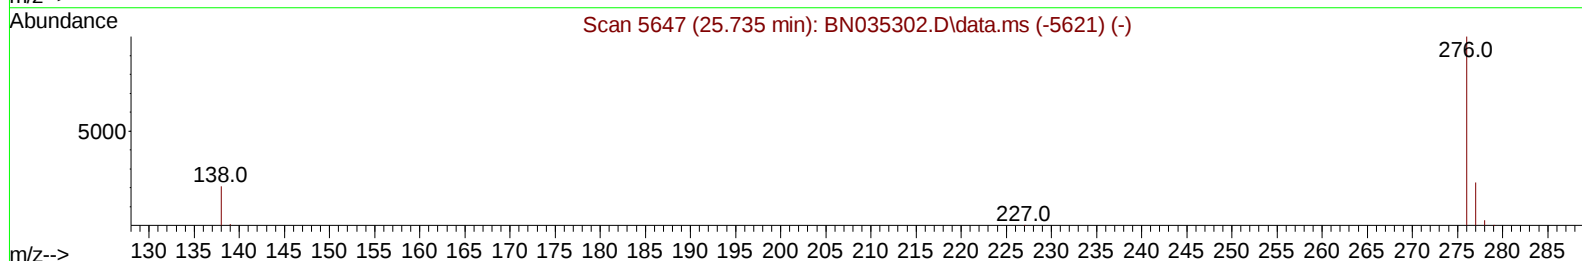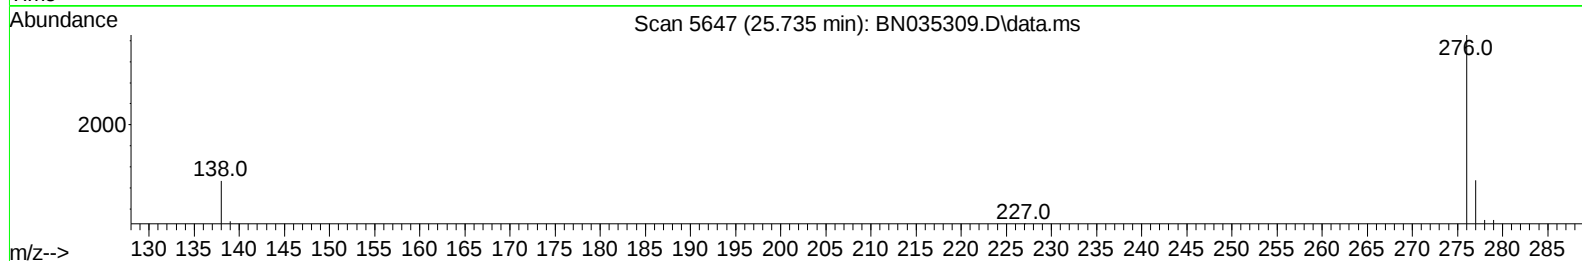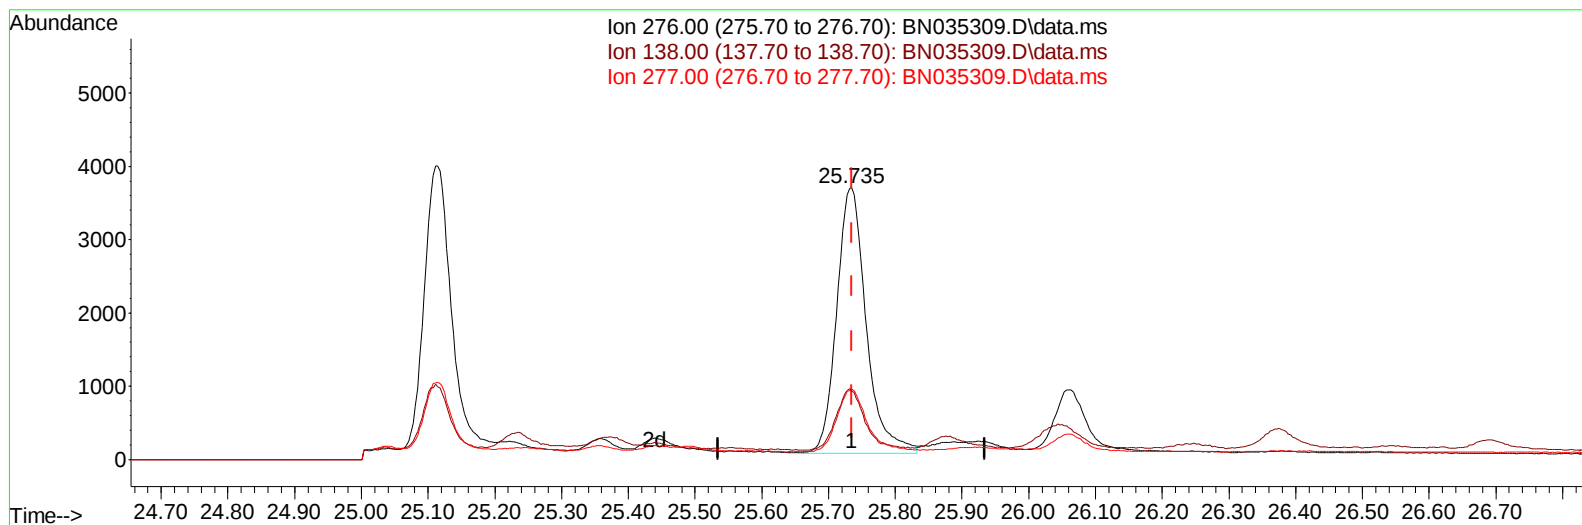

TIC: BN035309.D\data.ms

(29) Benzo(g,h,i)perylene

25.735min (-0.000) 0.47 ng/ul m

response 11148

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	16.30	25.20#
277.00	25.60	25.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
 Data File : BN035309.D
 Acq On : 26 Nov 2024 10:35
 Operator : RC/JU
 Sample : P4872-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E29Y4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2024
 Supervised By :mohammad ahmed 11/28/2024

Quant Time: Nov 26 22:12:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 26 06:09:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.314	152	3337	0.400	ng/ul	0.00
4) Naphthalene-d8	10.058	136	8210	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	13.972	164	4570	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.734	188	8708m	0.400	ng/ul	0.00
17) Chrysene-d12	20.979	240	7393	0.400	ng/ul	# 0.00
23) Perylene-d12	23.074	264	7319m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.976	96	17156	5.625	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.664	152	3952	0.328	ng/ul	0.00
18) Fluoranthene-d10	18.786	212	8896	0.436	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.108	128	511	0.025	ng/ul#	71
10) Acenaphthylene	13.685	152	3067	0.169	ng/ul#	93
12) Fluorene	15.036	166	908	0.056	ng/ul#	95
15) Phenanthrene	16.776	178	9136	0.397	ng/ul	99
16) Anthracene	16.869	178	3334	0.156	ng/ul#	92
19) Fluoranthene	18.819	202	27841	1.082	ng/ul#	95
20) Pyrene	19.186	202	24762m	0.924	ng/ul	
21) Benzo(a)anthracene	20.964	228	13858	0.540	ng/ul	93
22) Chrysene	21.014	228	13918	0.539	ng/ul	98
24) Benzo(b)fluoranthene	22.463	252	20379m	0.842	ng/ul	
25) Benzo(k)fluoranthene	22.498	252	7507m	0.301	ng/ul	
26) Benzo(a)pyrene	22.986	252	15400m	0.697	ng/ul	
27) Indeno(1,2,3-cd)pyrene	25.114	276	10873m	0.364	ng/ul	
28) Dibenzo(a,h)anthracene	25.124	278	2244m	0.096	ng/ul	
29) Benzo(g,h,i)perylene	25.735	276	11148m	0.474	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035309.D
Acq On : 26 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y4

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:12:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

