




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035321.D
Acq On : 26 Nov 2024 18:55
Operator : RC/JU
Sample : P5016-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1PJ2

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:14:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

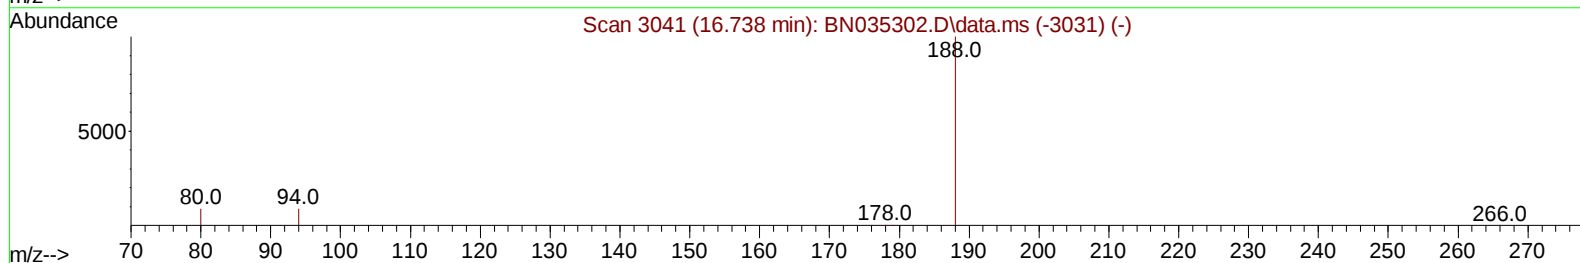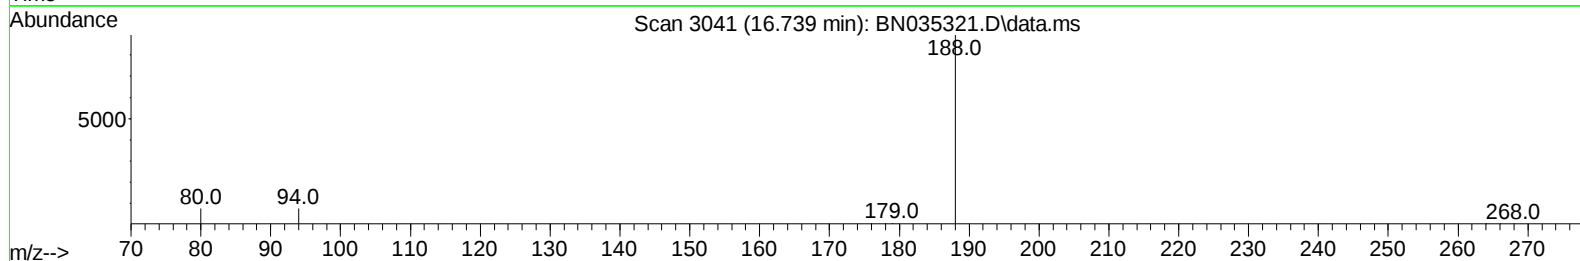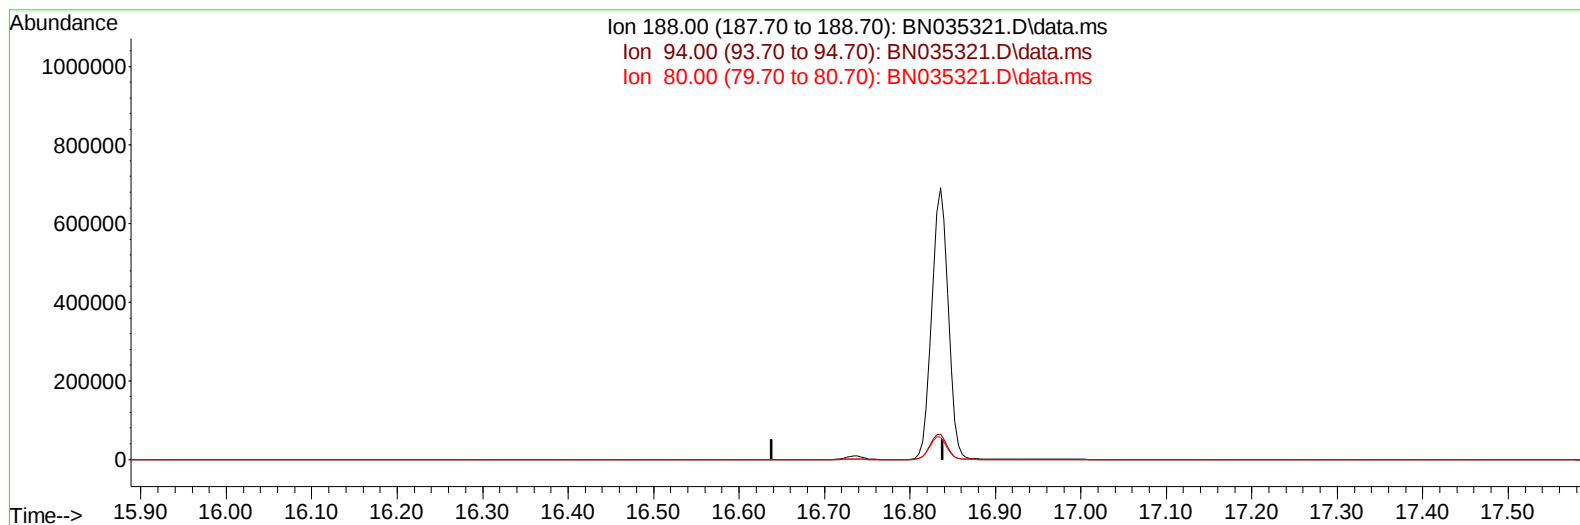

TIC: BN035321.D\data.ms

(13) Phenanthrene-d10 (I)

16.738min (-16.738) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	7.00	0.00#
80.00	7.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035321.D
Acq On : 26 Nov 2024 18:55
Operator : RC/JU
Sample : P5016-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1PJ2

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:14:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

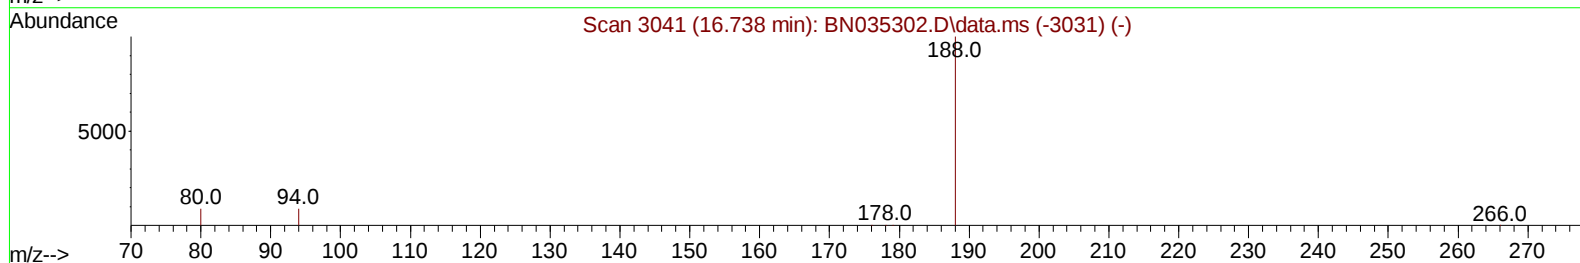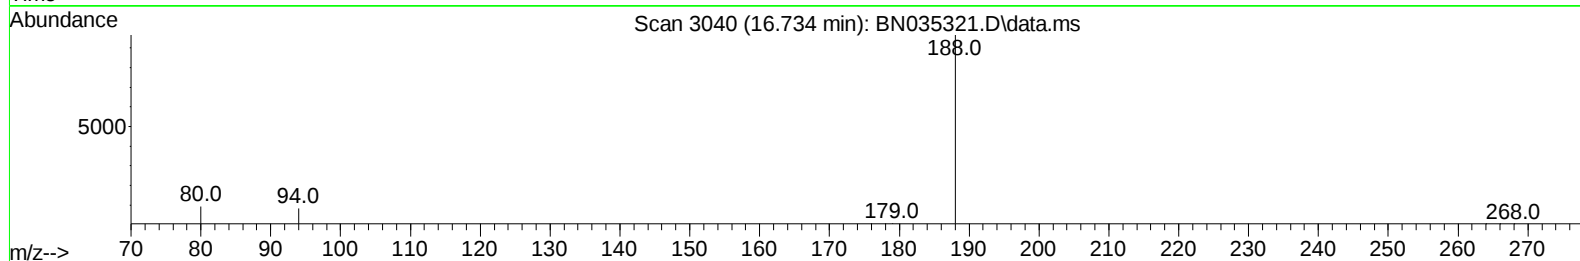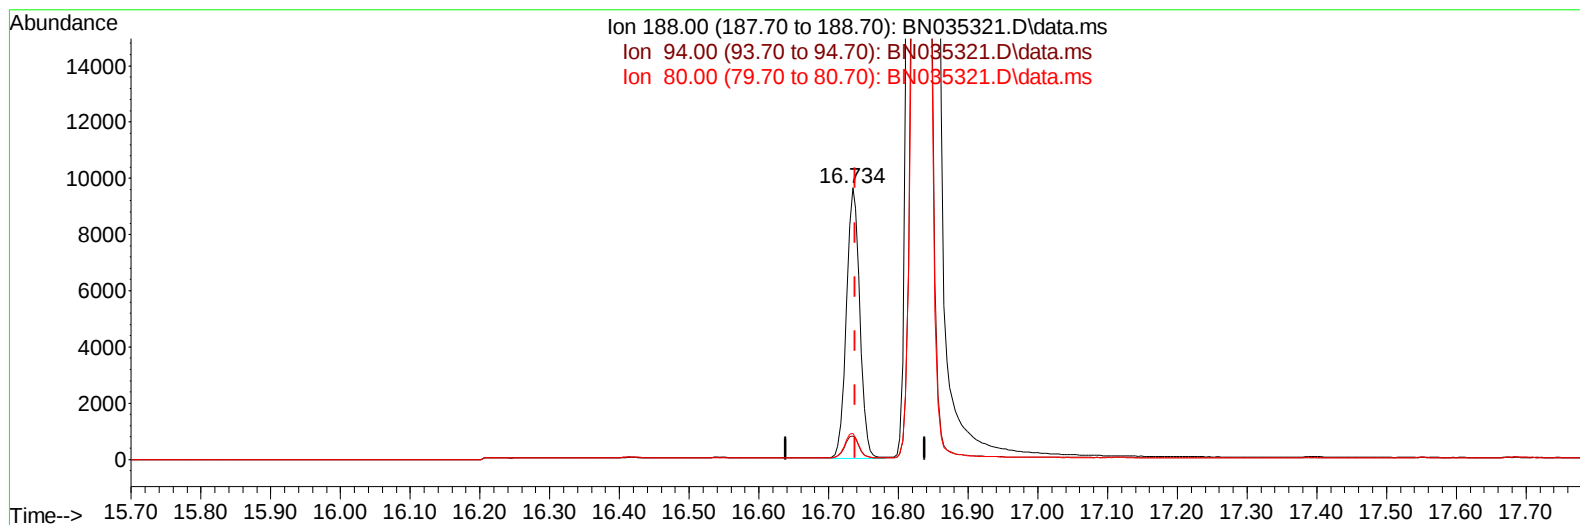

TIC: BN035321.D\data.ms

(13) Phenanthrene-d10 (I)

16.734min (-0.004) 0.40 ng/u1 m

response 12775

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.00	8.74#
80.00	7.60	9.63#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035321.D
Acq On : 26 Nov 2024 18:55
Operator : RC/JU
Sample : P5016-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1PJ2

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:14:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

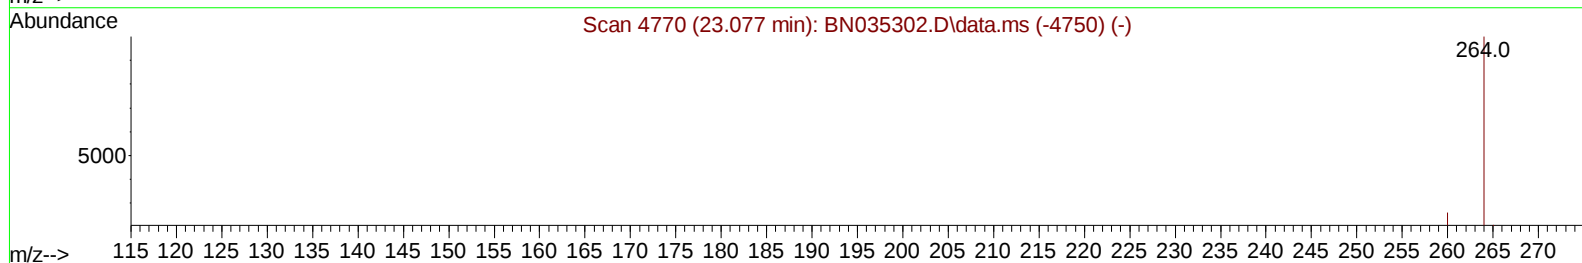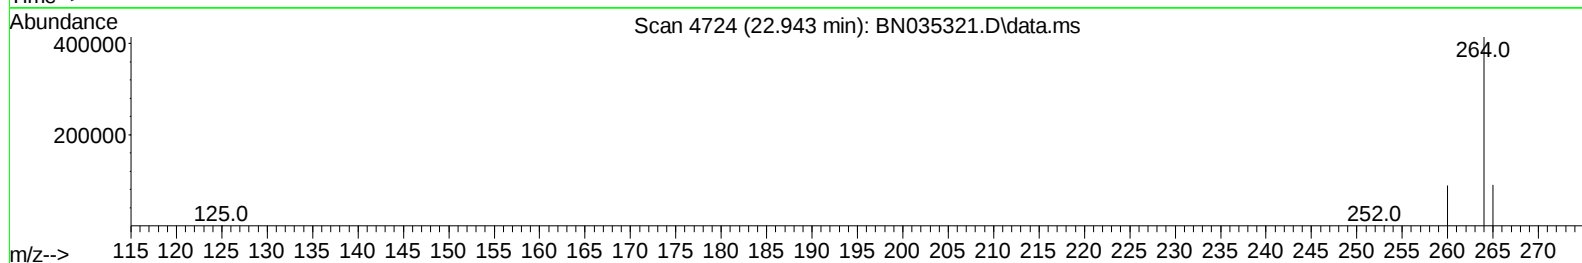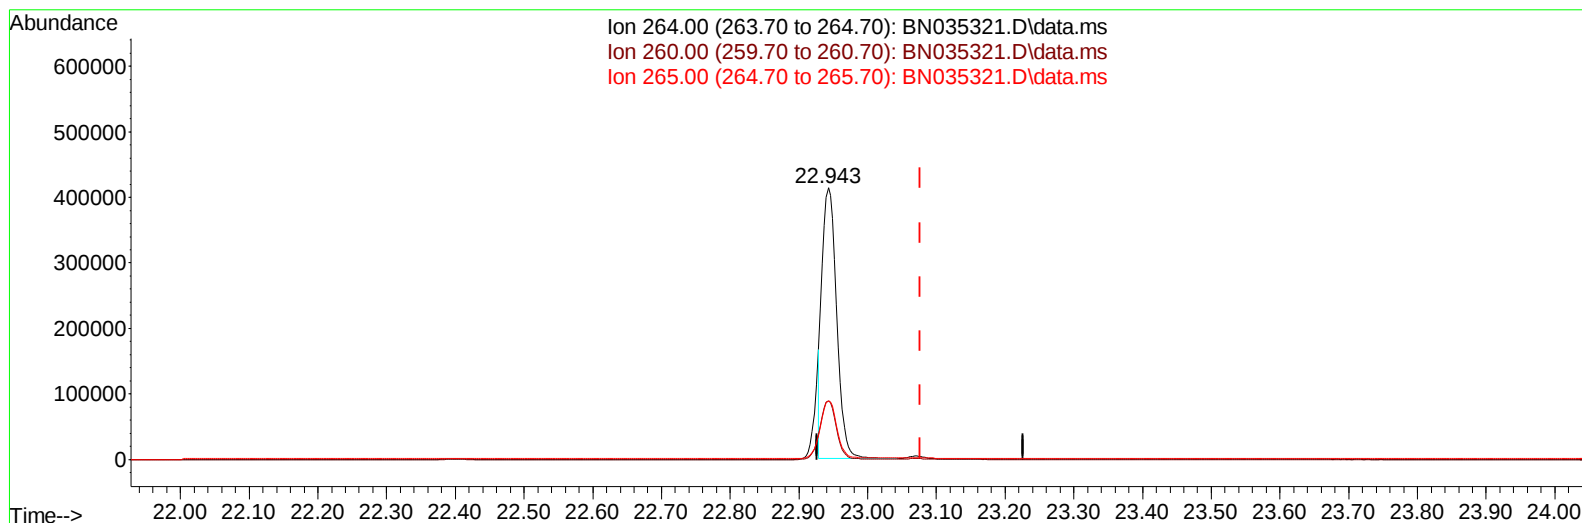

TIC: BN035321.D\data.ms

(23) Perylene-d12 (I)

22.943min (-0.134) 0.40 ng/u1

response 614739

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	21.63
265.00	75.50	21.69#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035321.D
Acq On : 26 Nov 2024 18:55
Operator : RC/JU
Sample : P5016-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1PJ2

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:14:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

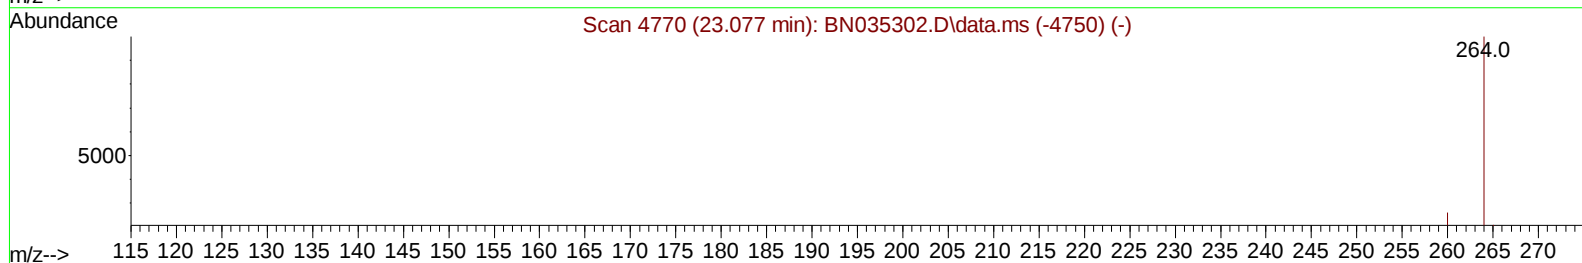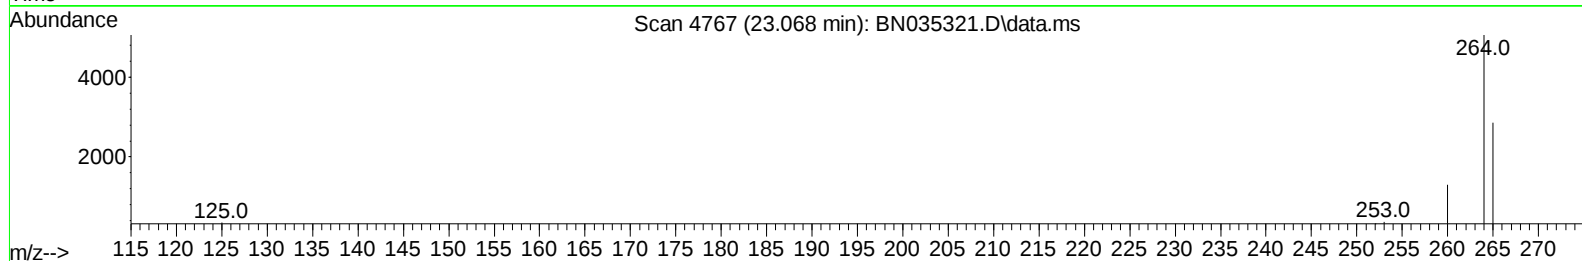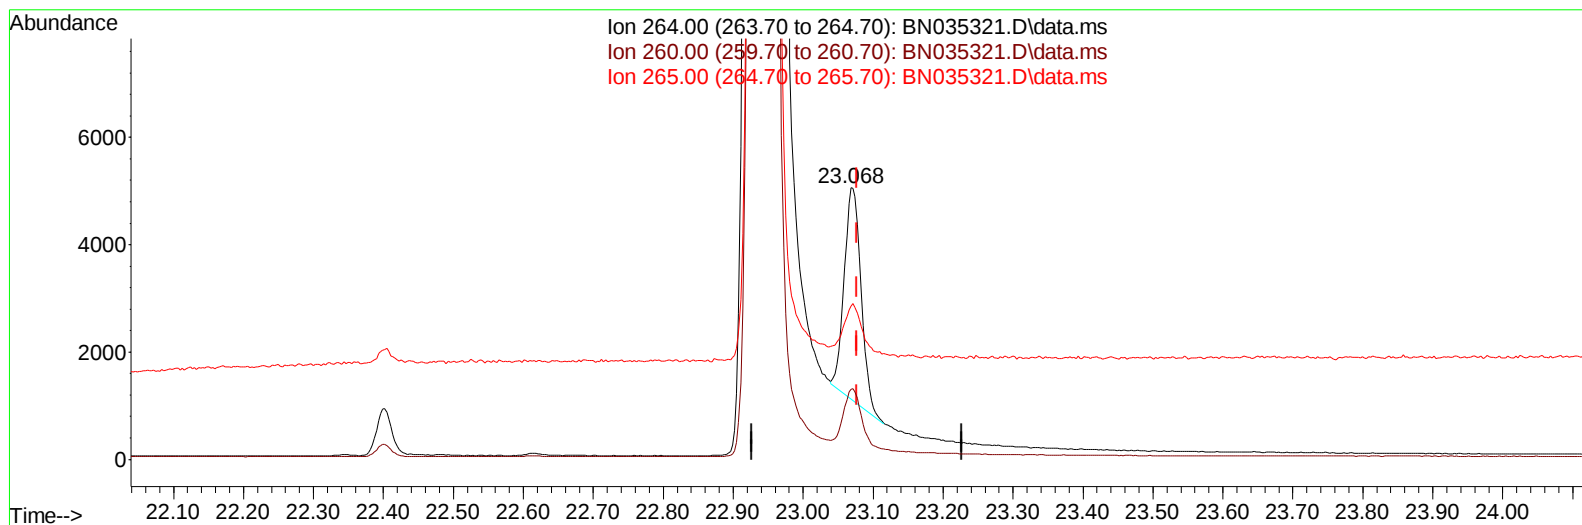

TIC: BN035321.D\data.ms

(23) Perylene-d12 (I)

23.068min (-0.009) 0.40 ng/ul m

response 6570

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	25.82
265.00	75.50	56.56#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
 Data File : BN035321.D
 Acq On : 26 Nov 2024 18:55
 Operator : RC/JU
 Sample : P5016-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1PJ2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2024
 Supervised By :mohammad ahmed 11/28/2024

Quant Time: Nov 26 22:14:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 26 06:09:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.314	152	3741	0.400	ng/ul	0.00
4) Naphthalene-d8	10.059	136	10114	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.972	164	6346	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.734	188	12775m	0.400	ng/ul	0.00
17) Chrysene-d12	20.976	240	7179	0.400	ng/ul	# 0.00
23) Perylene-d12	23.068	264	6570m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.972	96	16981	4.966	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.659	152	4631	0.312	ng/ul	0.00
18) Fluoranthene-d10	18.786	212	9822	0.496	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035321.D
Acq On : 26 Nov 2024 18:55
Operator : RC/JU
Sample : P5016-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1PJ2

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:14:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

