

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035324.D
Acq On : 26 Nov 2024 20:43
Operator : RC/JU
Sample : P4996-04
Misc :
ALS Vial : 23 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
BHF71

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:14:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

Supervised By :mohammad
ahmed
11/28/2024

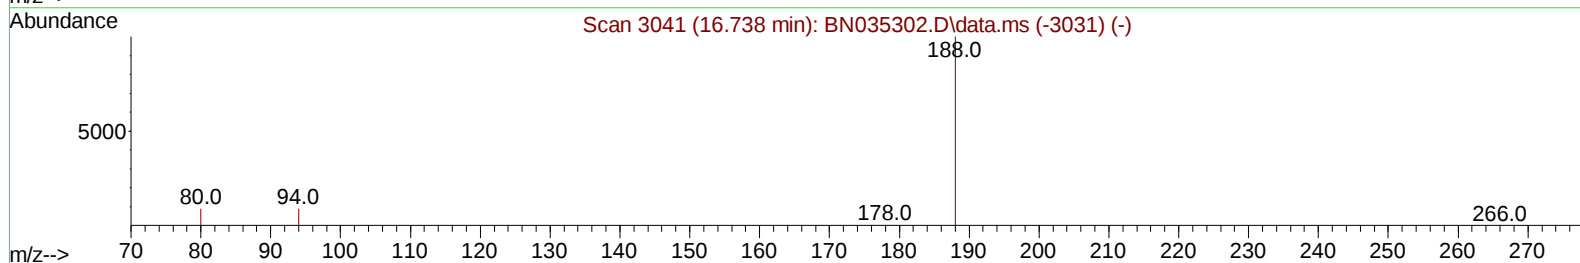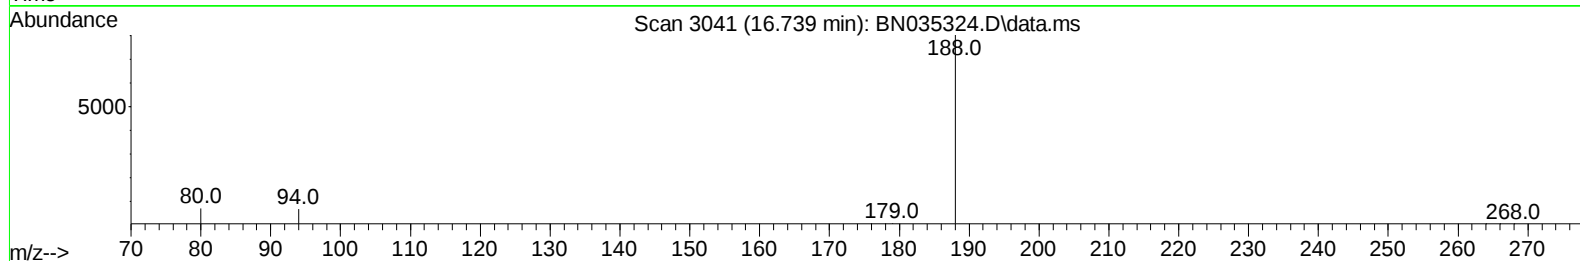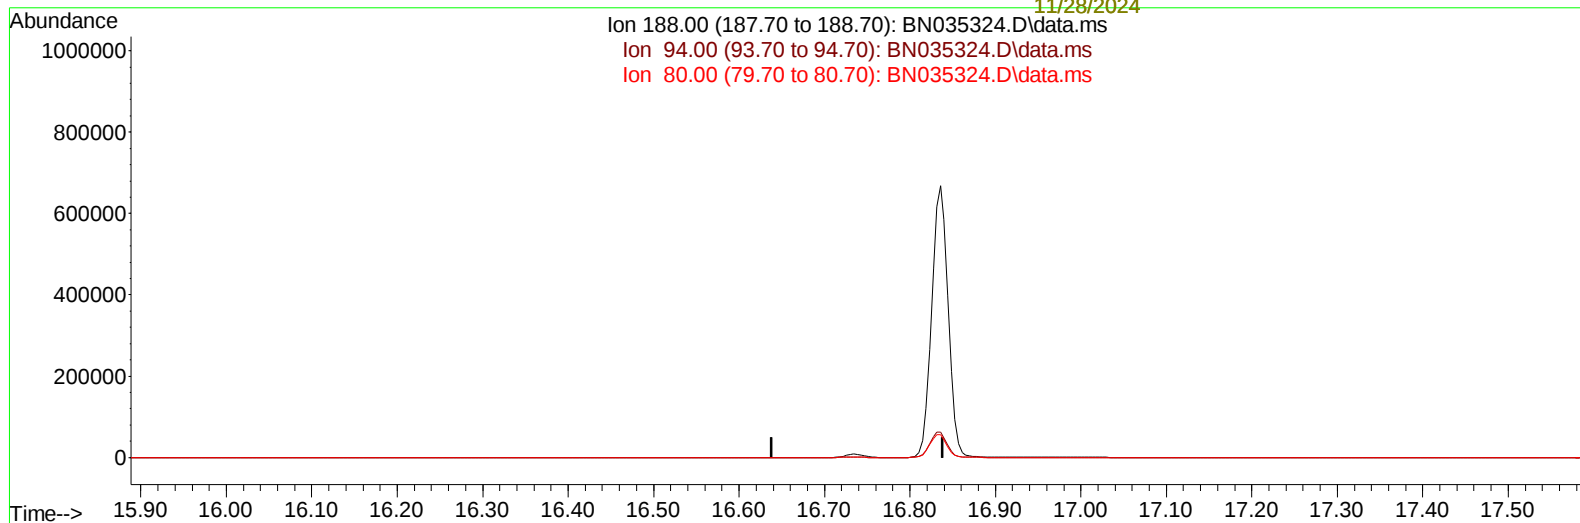

TIC: BN035324.D\data.ms

(13) Phenanthrene-d10 (I)**16.738min (-16.738) 0.00 ng/u1****response 0**

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	7.00	0.00#
80.00	7.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035324.D
Acq On : 26 Nov 2024 20:43
Operator : RC/JU
Sample : P4996-04
Misc :
ALS Vial : 23 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
BHF71

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:14:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

Supervised By :mohammad
ahmed
11/28/2024

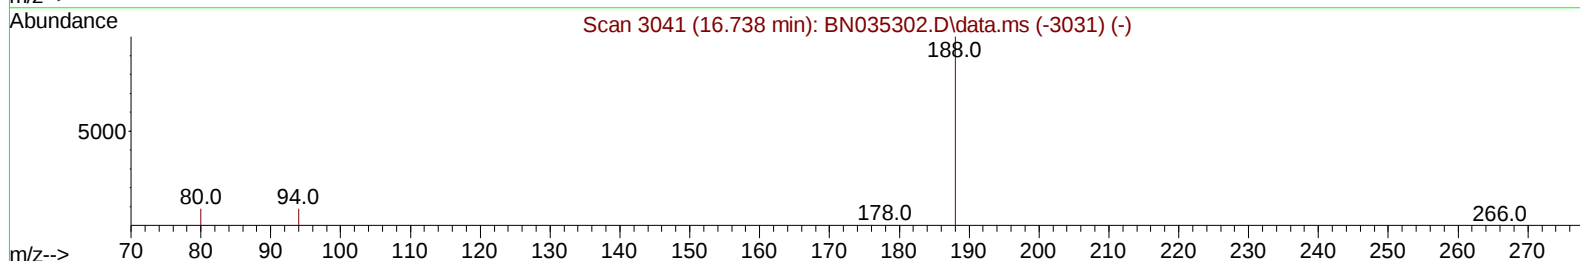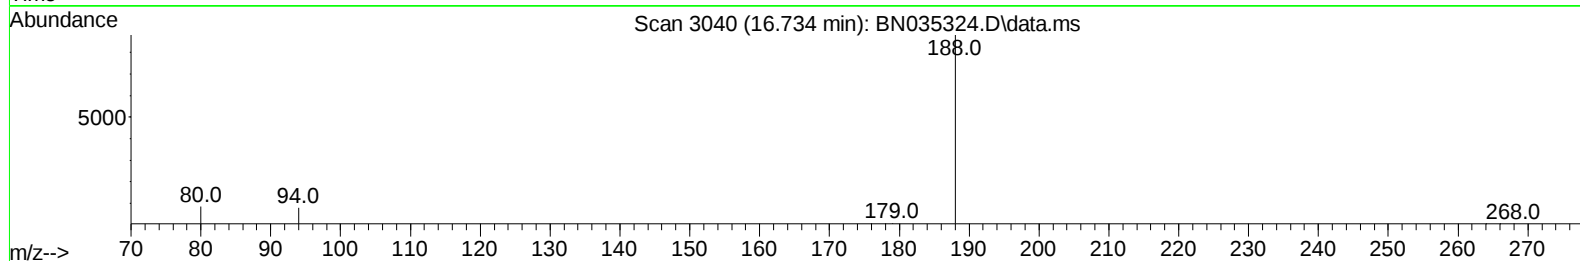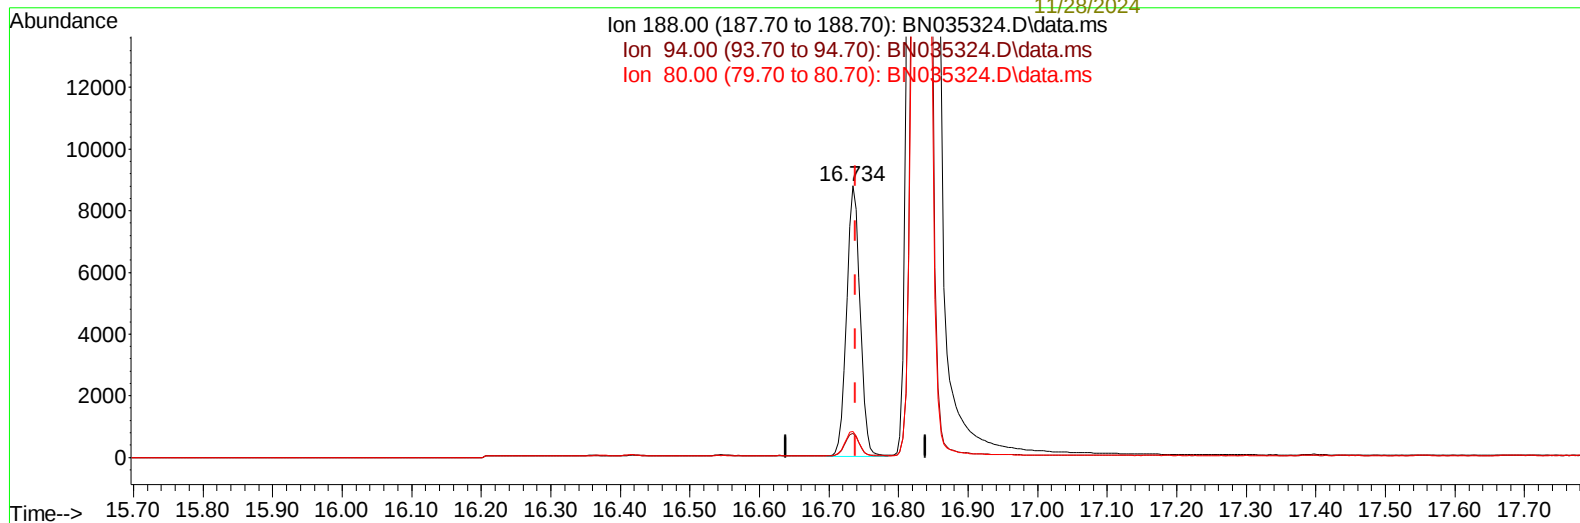

TIC: BN035324.D\data.ms

(13) Phenanthrene-d10 (I)

16.734min (-0.004) 0.40 ng/u1 m

response 11774

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.00	8.97#
80.00	7.60	9.56#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035324.D
Acq On : 26 Nov 2024 20:43
Operator : RC/JU
Sample : P4996-04
Misc :
ALS Vial : 23 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
BHF71

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:14:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

Supervised By :mohammad
ahmed
11/28/2024

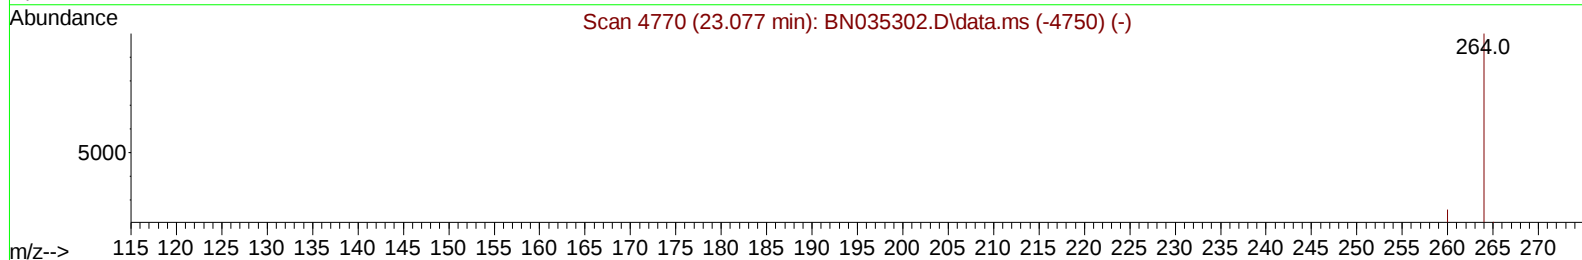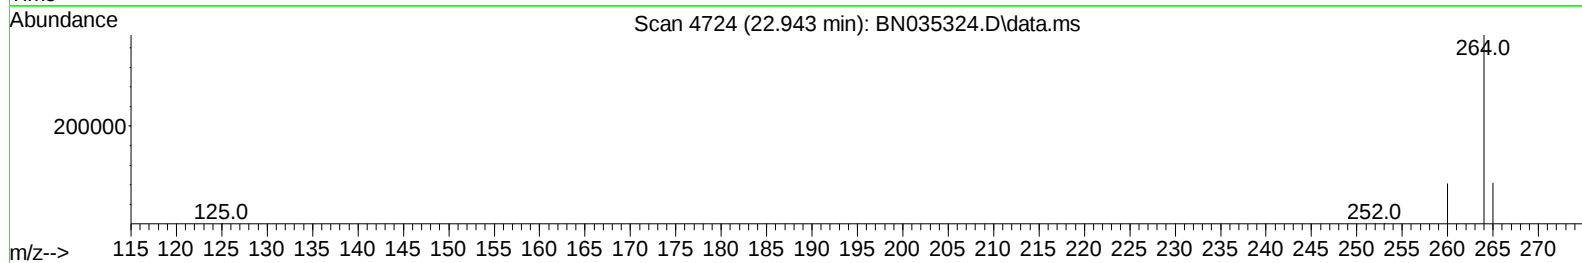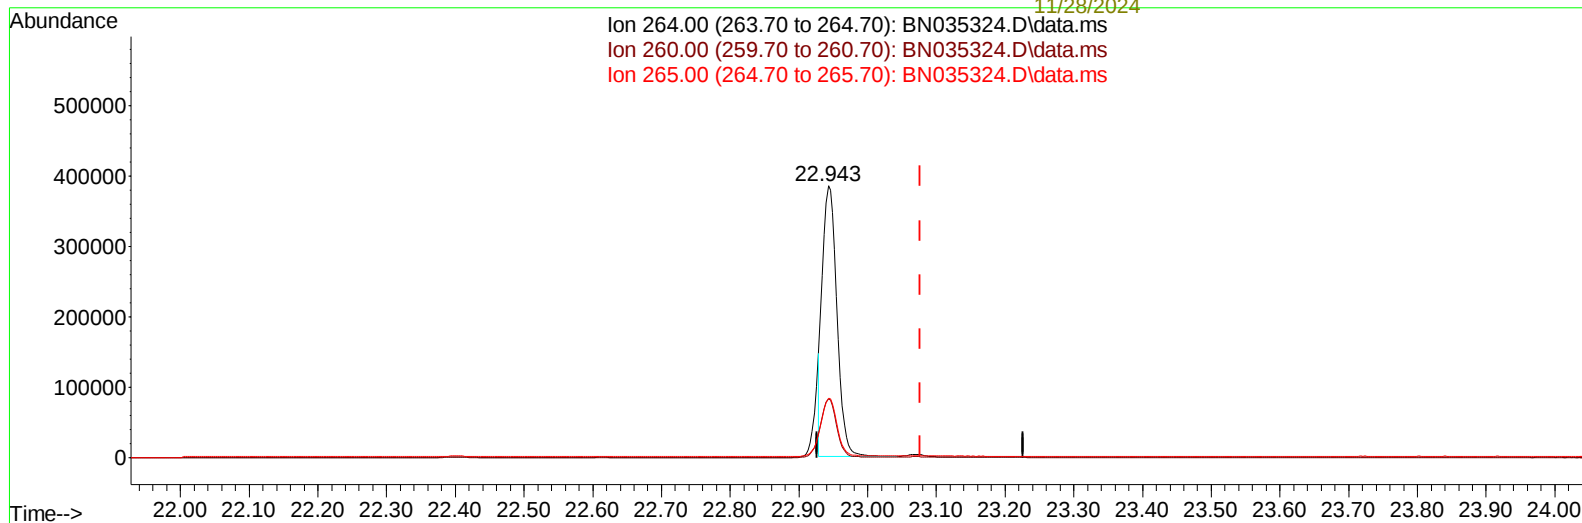

TIC: BN035324.D\data.ms

(23) Perylene-d12 (I)

22.943min (-0.134) 0.40 ng/u1

response 570742

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	21.52
265.00	75.50	21.77#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035324.D
Acq On : 26 Nov 2024 20:43
Operator : RC/JU
Sample : P4996-04
Misc :
ALS Vial : 23 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
BHF71

Manual IntegrationsAPPROVED

Quant Time: Nov 26 22:14:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

Supervised By :mohammad
ahmed
11/28/2024

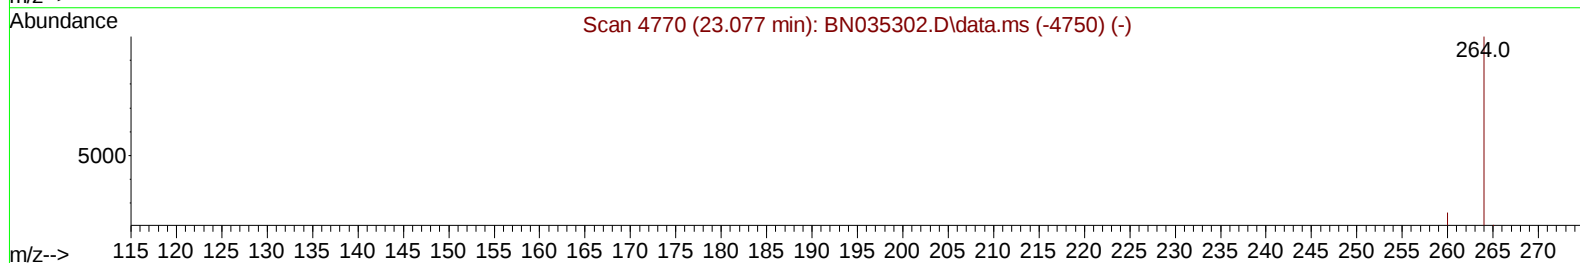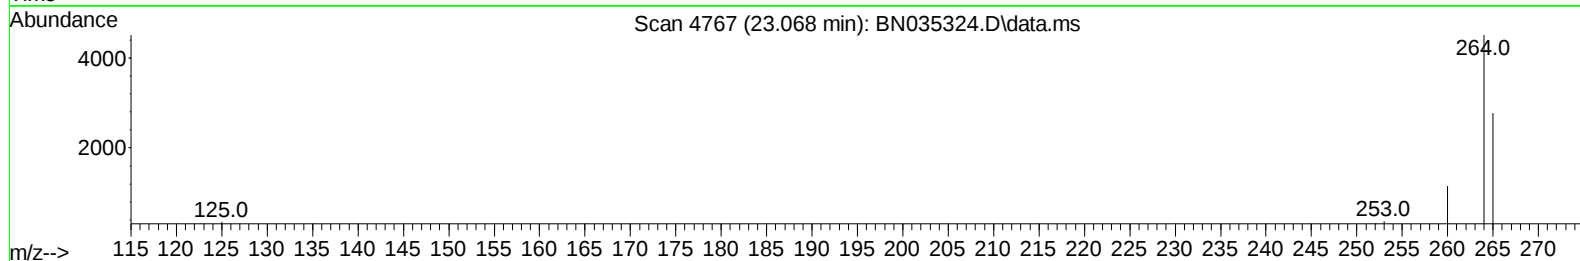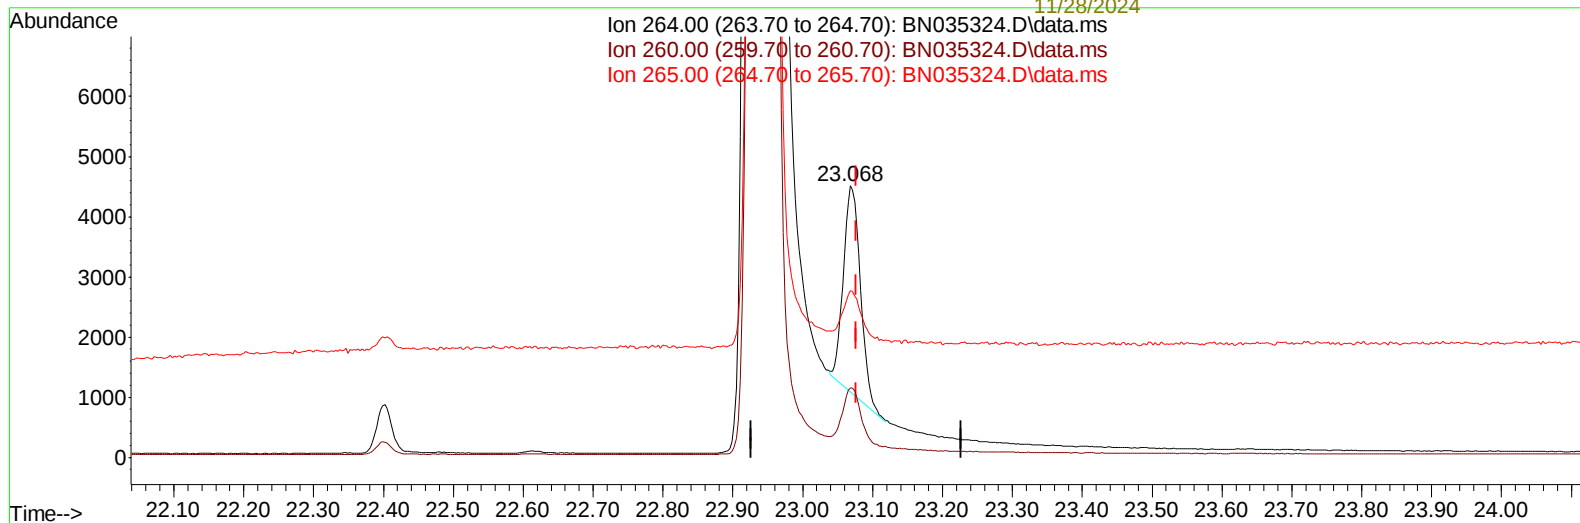

TIC: BN035324.D\data.ms

(23) Perylene-d12 (I)

23.068min (-0.009) 0.40 ng/ul m

response 5803

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	25.53
265.00	75.50	61.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
 Data File : BN035324.D
 Acq On : 26 Nov 2024 20:43
 Operator : RC/JU
 Sample : P4996-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHF71

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2024
 Supervised By :mohammad ahmed 11/28/2024

Supervised By :mohammad
 ahmed
 11/28/2024

Quant Time: Nov 26 22:14:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN11624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 26 06:09:15 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.310	152		3334	0.400	ng/ul	0.00
4) Naphthalene-d8	10.059	136		9129	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.967	164		5774	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.734	188		11774m	0.400	ng/ul	0.00
17) Chrysene-d12	20.976	240		6485	0.400	ng/ul	# 0.00
23) Perylene-d12	23.068	264		5803m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	2.972	96		13405	4.399	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.659	152		3874	0.290	ng/ul	0.00
18) Fluoranthene-d10	18.786	212		9483	0.530	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035324.D
Acq On : 26 Nov 2024 20:43
Operator : RC/JU
Sample : P4996-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHF71

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

Supervised By :mohammad
ahmed
11/28/2024

Quant Time: Nov 26 22:14:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

