




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035335.D
Acq On : 27 Nov 2024 03:54
Operator : RC/JU
Sample : PB165259BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK259

Manual IntegrationsAPPROVED

Quant Time: Nov 27 04:16:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

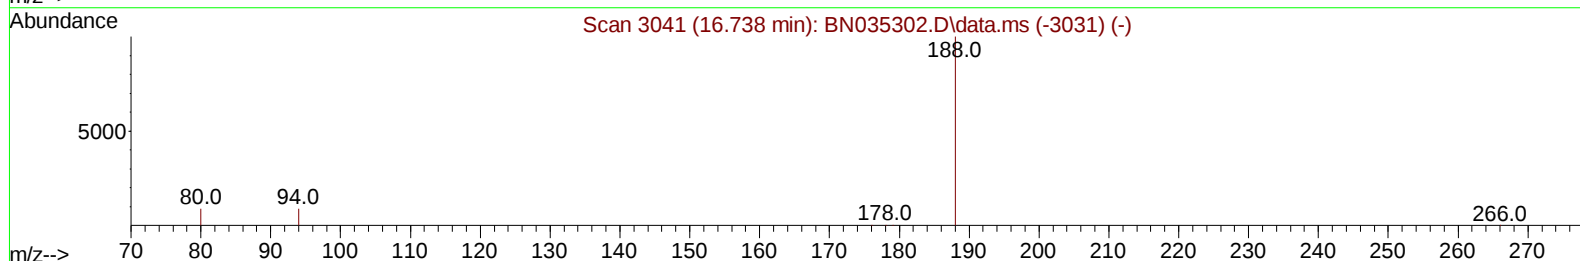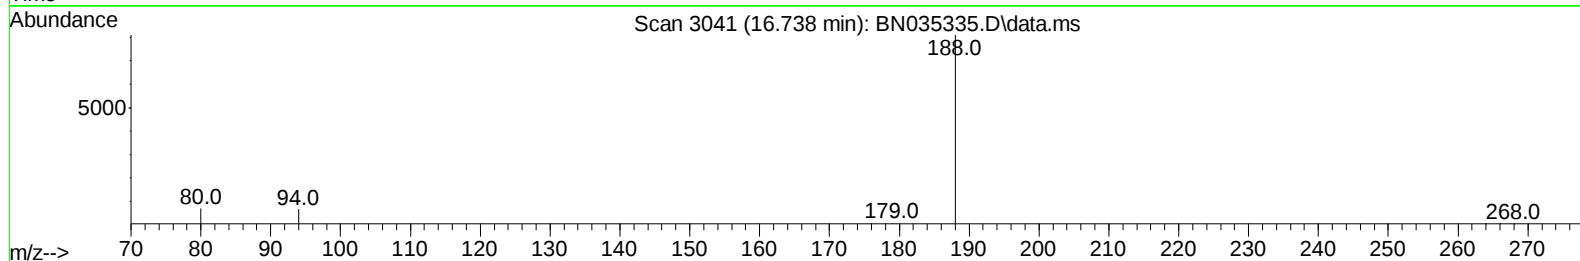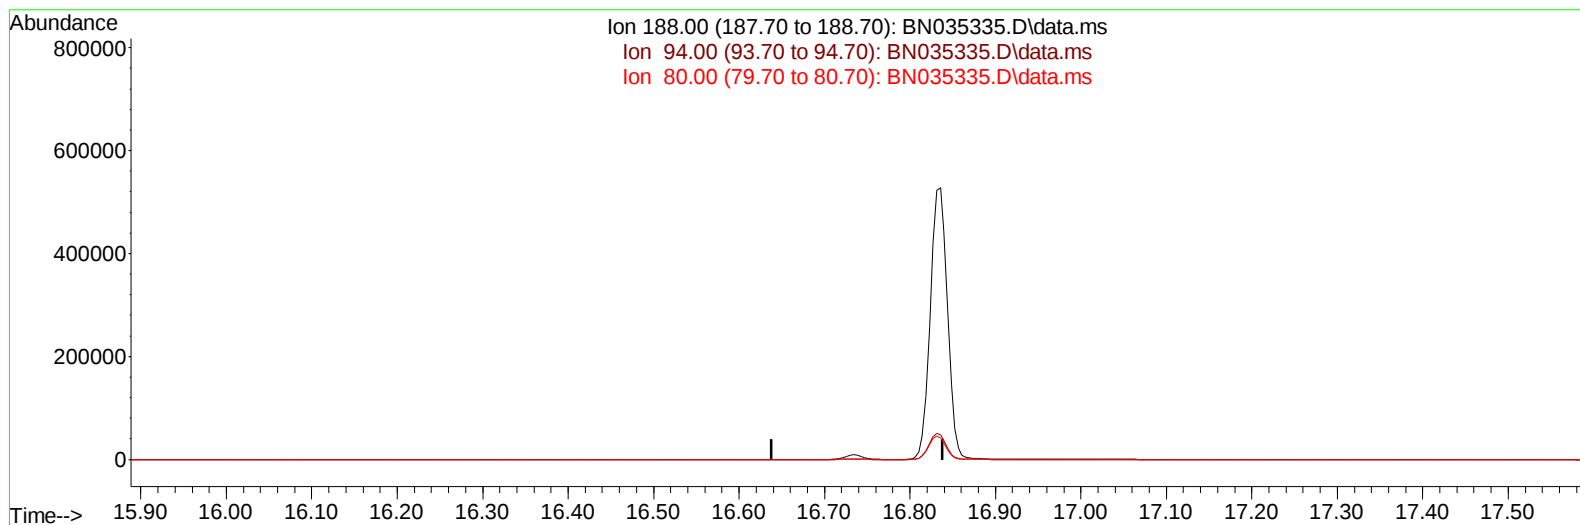

TIC: BN035335.D\data.ms

(13) Phenanthrene-d10 (I)

16.738min (-16.738) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	7.00	0.00#
80.00	7.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035335.D
Acq On : 27 Nov 2024 03:54
Operator : RC/JU
Sample : PB165259BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK259

Manual IntegrationsAPPROVED

Quant Time: Nov 27 04:16:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

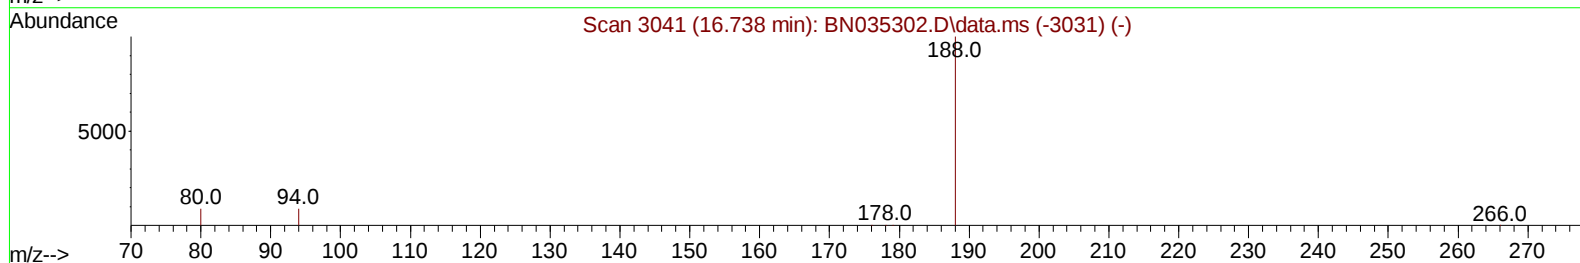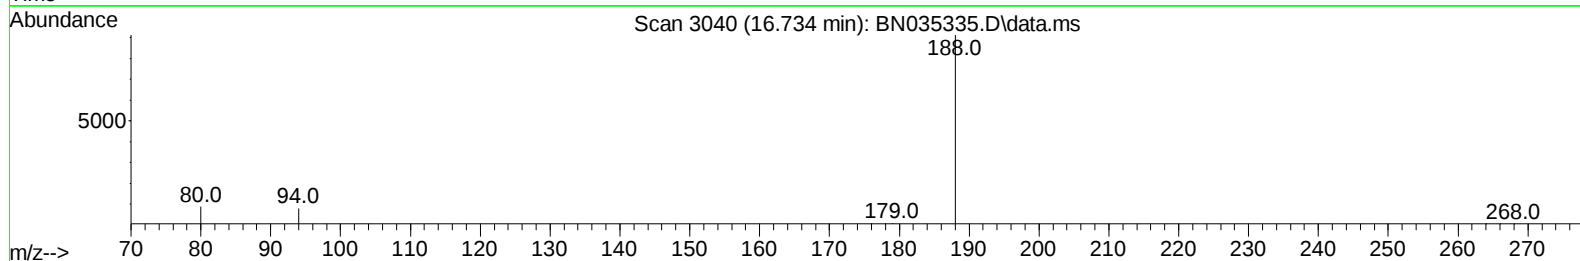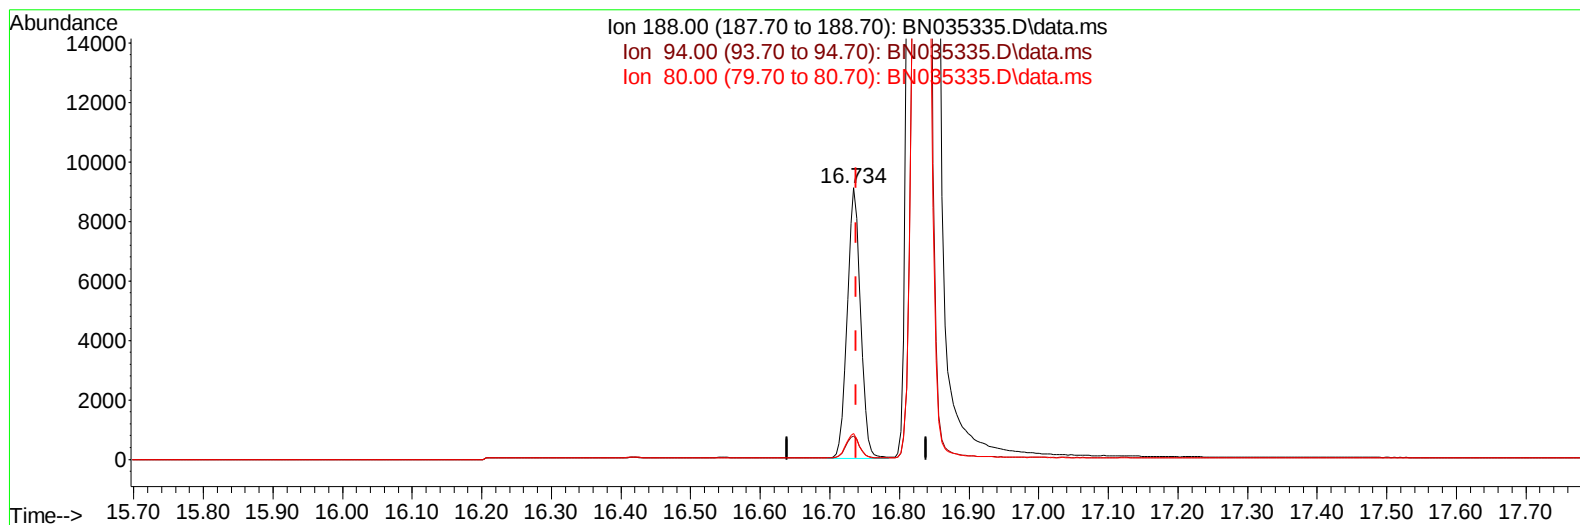

TIC: BN035335.D\data.ms

(13) Phenanthrene-d10 (I)

16.734min (-0.004) 0.40 ng/u1 m

response 12035

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.00	8.72#
80.00	7.60	9.49#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035335.D
Acq On : 27 Nov 2024 03:54
Operator : RC/JU
Sample : PB165259BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK259

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

Quant Time: Nov 27 04:16:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

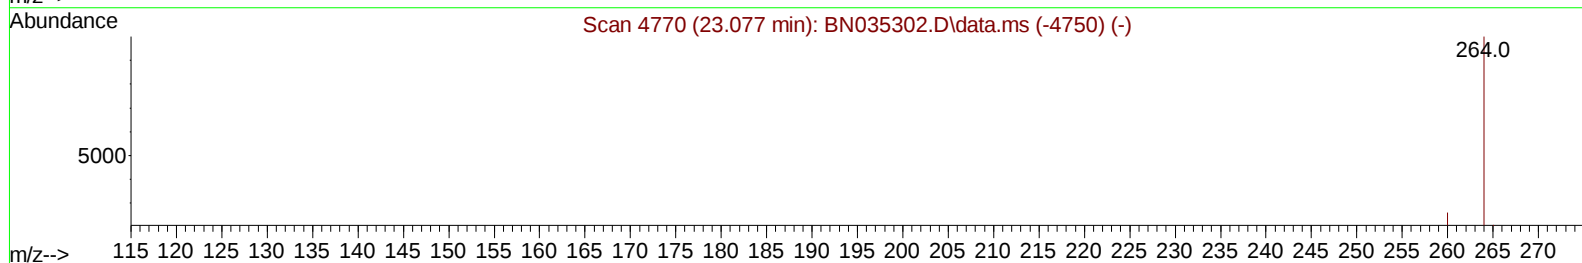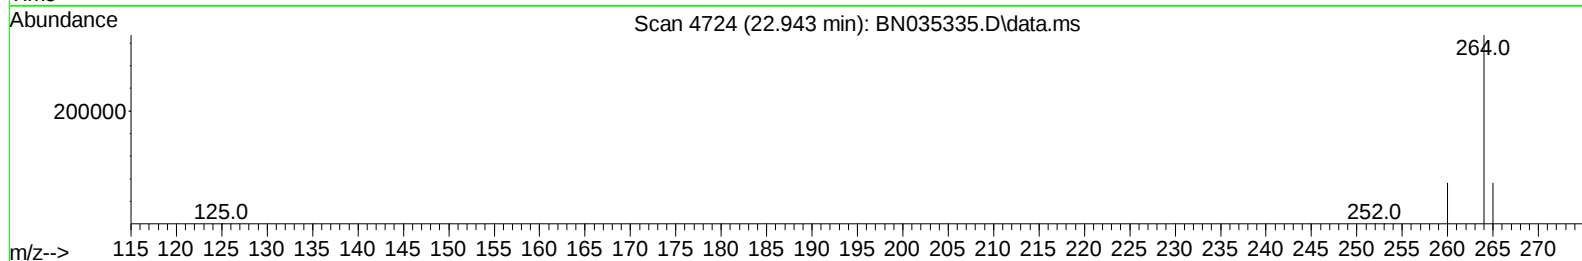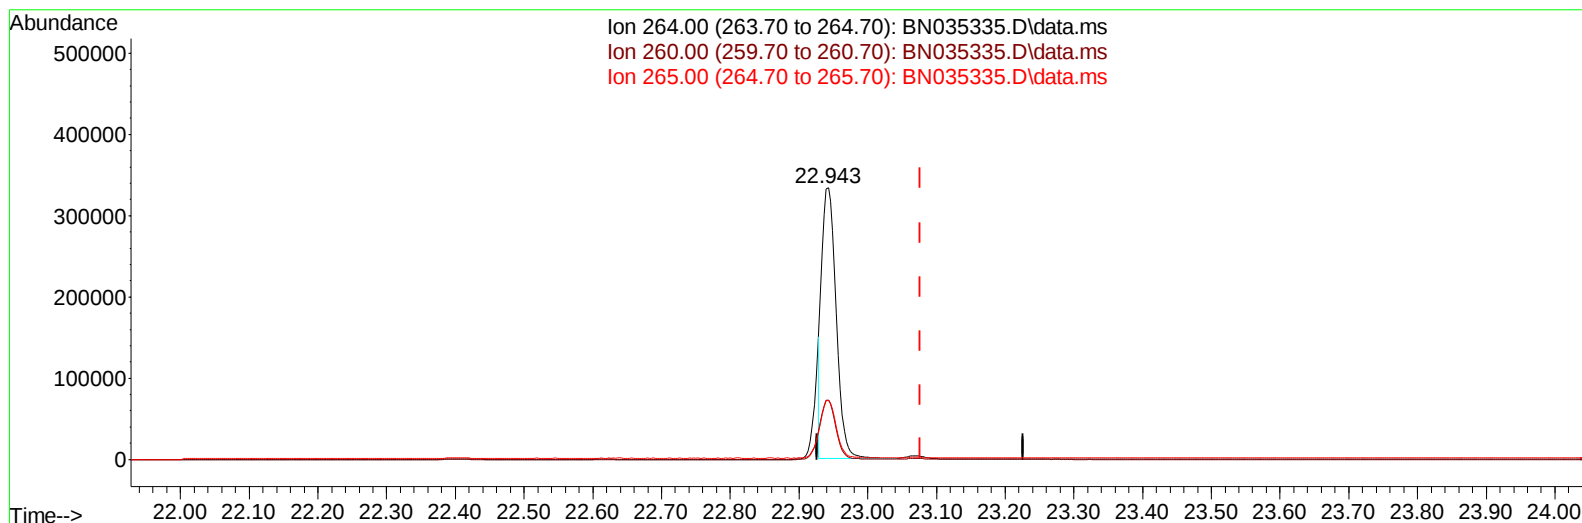

TIC: BN035335.D\data.ms

(23) Perylene-d12 (I)

22.943min (-0.134) 0.40 ng/u1

response 491232

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	21.78
265.00	75.50	21.74#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035335.D
Acq On : 27 Nov 2024 03:54
Operator : RC/JU
Sample : PB165259BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK259

Manual IntegrationsAPPROVED

Quant Time: Nov 27 04:16:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

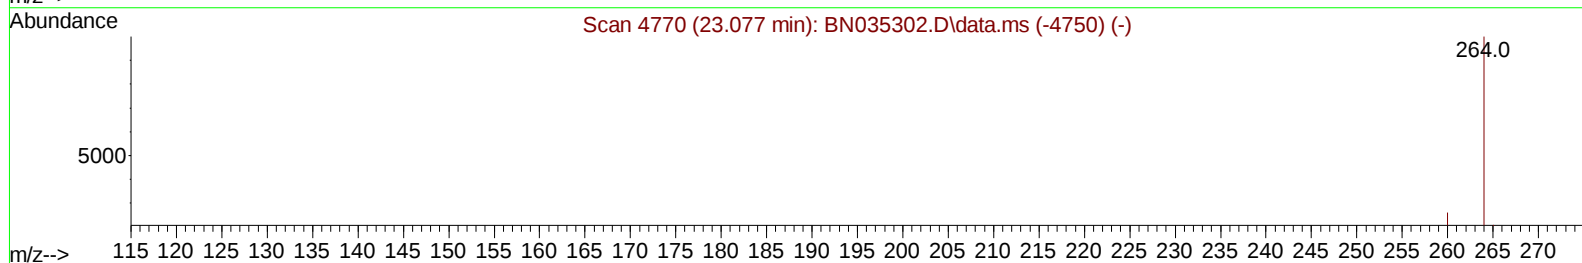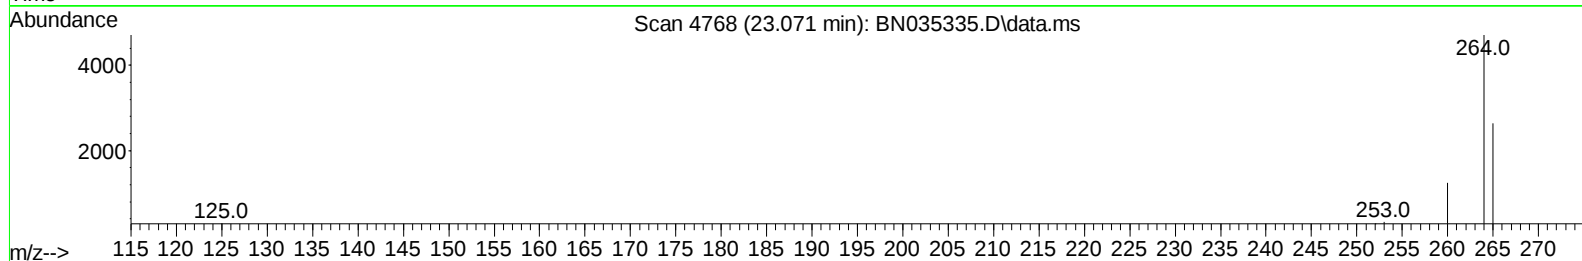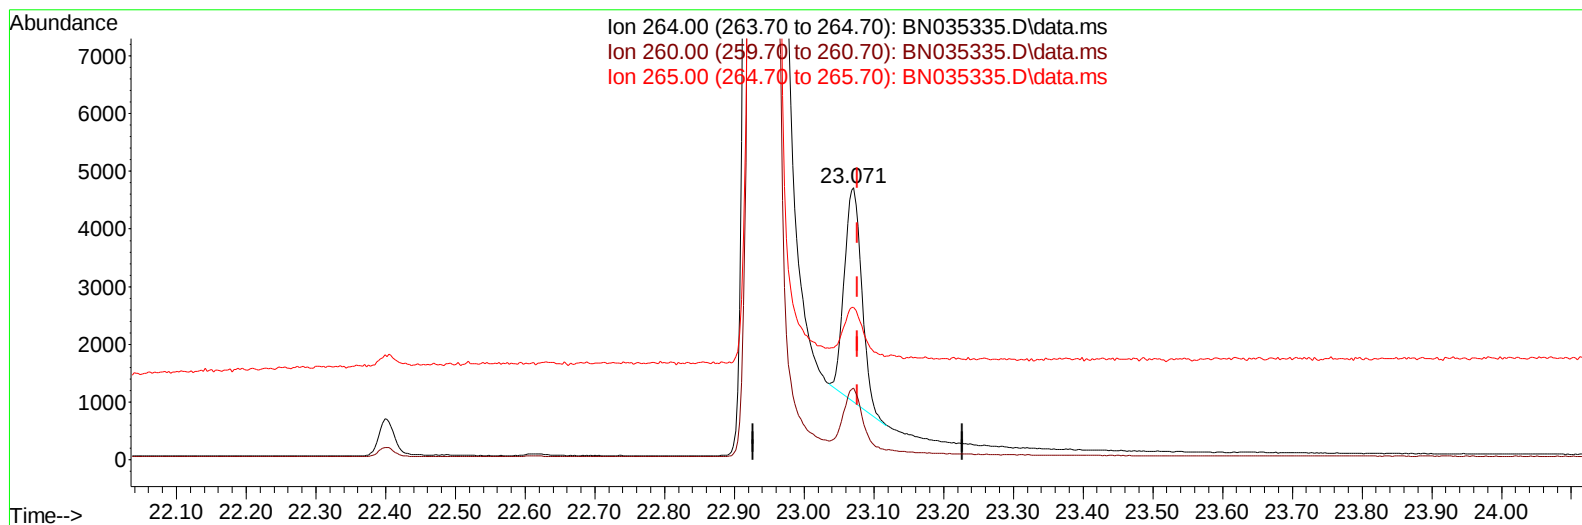

TIC: BN035335.D\data.ms

(23) Perylene-d12 (I)

23.071min (-0.006) 0.40 ng/ul m

response 6410

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	26.27
265.00	75.50	55.98#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
 Data File : BN035335.D
 Acq On : 27 Nov 2024 03:54
 Operator : RC/JU
 Sample : PB165259BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK259

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2024
 Supervised By :mohammad ahmed 11/28/2024

Quant Time: Nov 27 04:16:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 26 06:09:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.310	152	3705	0.400	ng/ul	0.00
4) Naphthalene-d8	10.059	136	9886	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.967	164	6161	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.734	188	12035m	0.400	ng/ul	0.00
17) Chrysene-d12	20.976	240	6396	0.400	ng/ul	# 0.00
23) Perylene-d12	23.071	264	6410m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.972	96	17326	5.117	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.664	152	3649	0.252	ng/ul	0.00
18) Fluoranthene-d10	18.786	212	6942	0.393	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035335.D
Acq On : 27 Nov 2024 03:54
Operator : RC/JU
Sample : PB165259BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK259

Manual IntegrationsAPPROVED

Quant Time: Nov 27 04:16:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

