




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035336.D
Acq On : 27 Nov 2024 04:30
Operator : RC/JU
Sample : PB165232BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK232

Manual IntegrationsAPPROVED

Quant Time: Nov 27 05:29:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

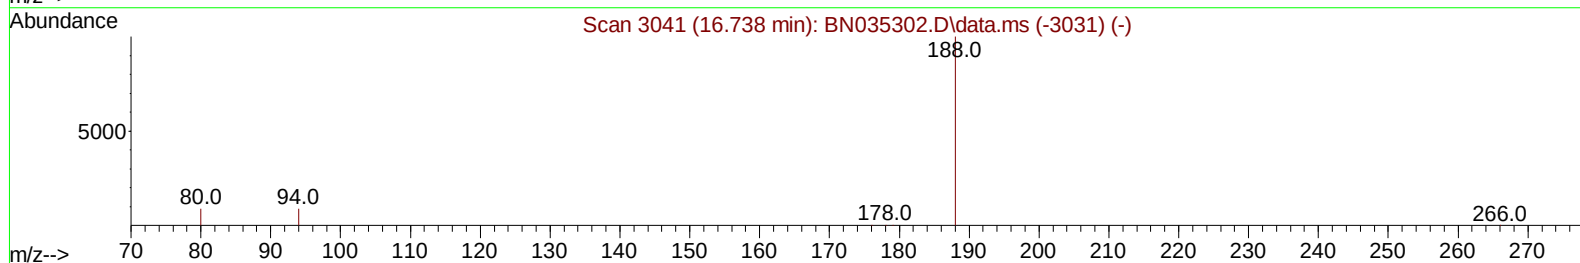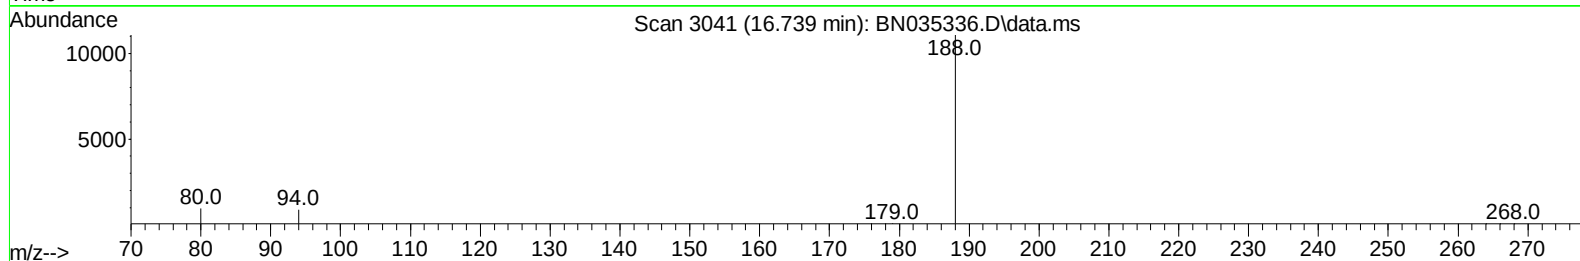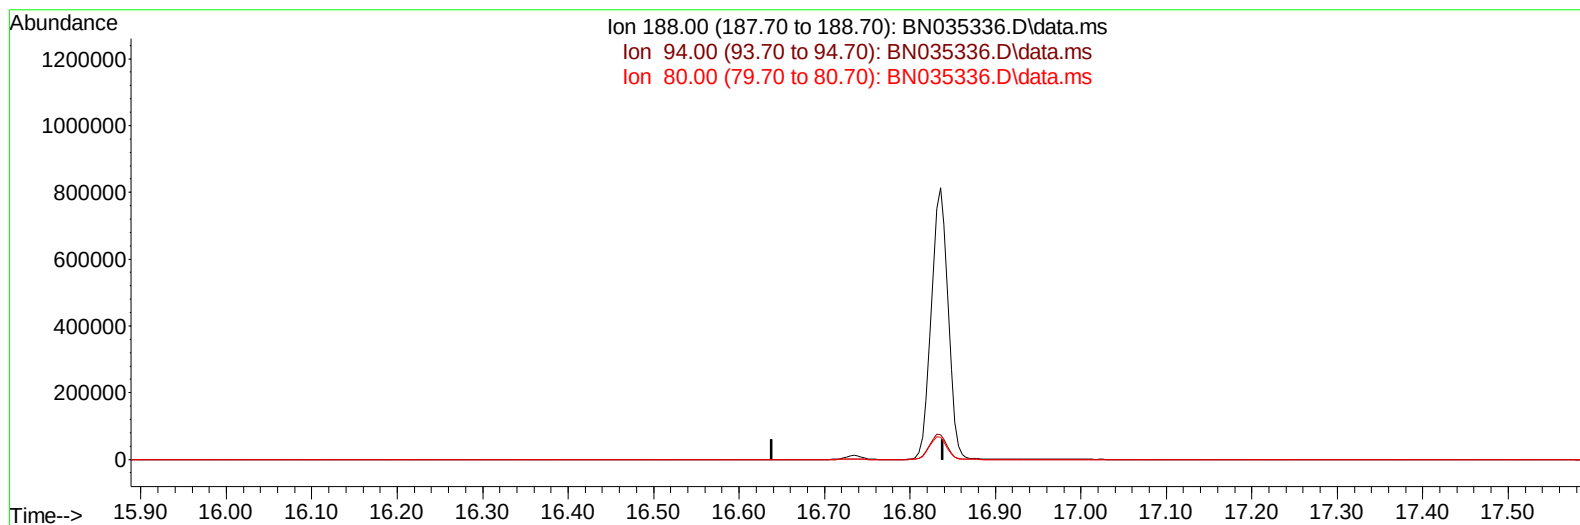

TIC: BN035336.D\data.ms

(13) Phenanthrene-d10 (I)

16.738min (-16.738) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	7.00	0.00#
80.00	7.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035336.D
Acq On : 27 Nov 2024 04:30
Operator : RC/JU
Sample : PB165232BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK232

Manual IntegrationsAPPROVED

Quant Time: Nov 27 05:29:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

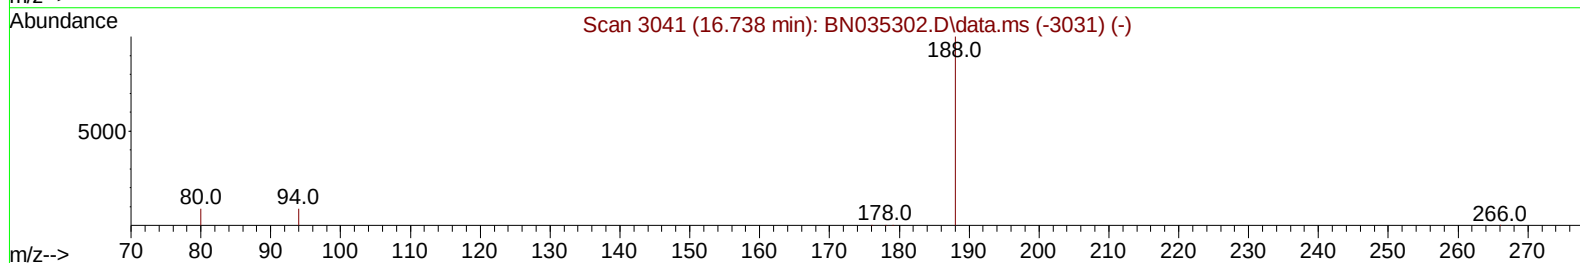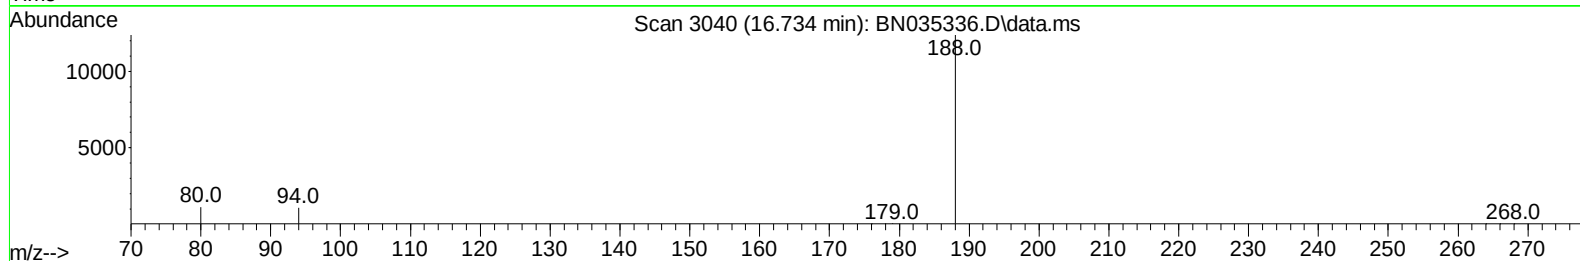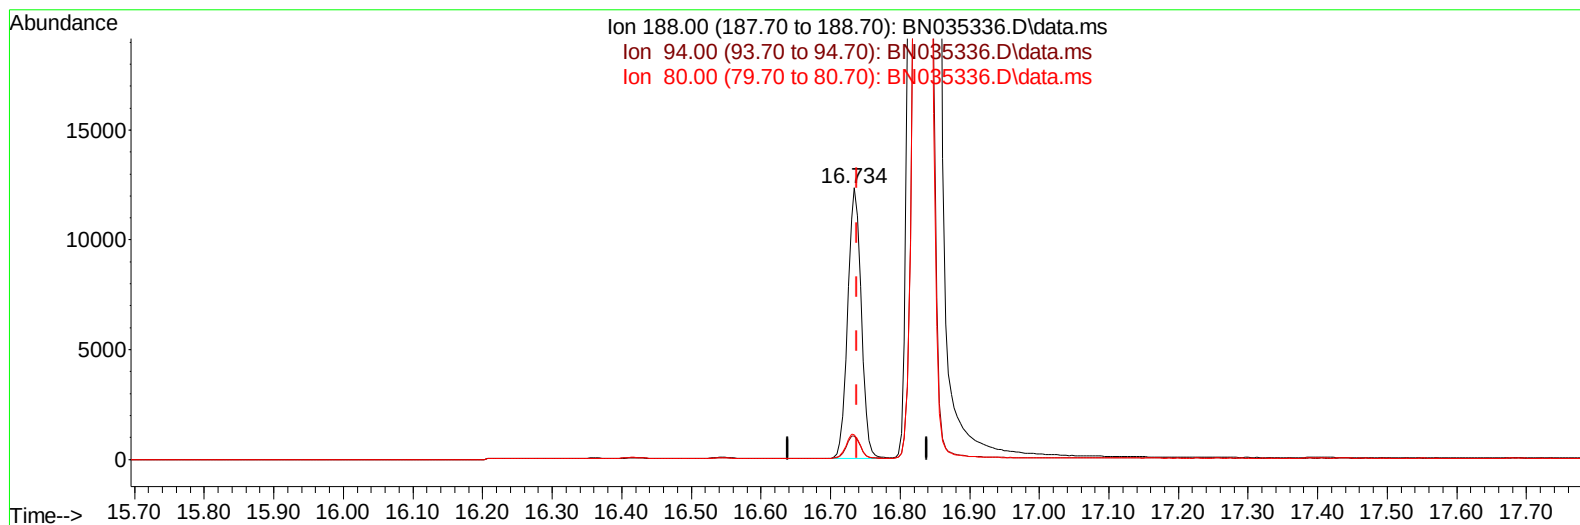

TIC: BN035336.D\data.ms

(13) Phenanthrene-d10 (I)

16.734min (-0.004) 0.40 ng/ul m

response 16605

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.00	8.66#
80.00	7.60	9.20#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035336.D
Acq On : 27 Nov 2024 04:30
Operator : RC/JU
Sample : PB165232BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK232

Manual IntegrationsAPPROVED

Quant Time: Nov 27 05:29:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

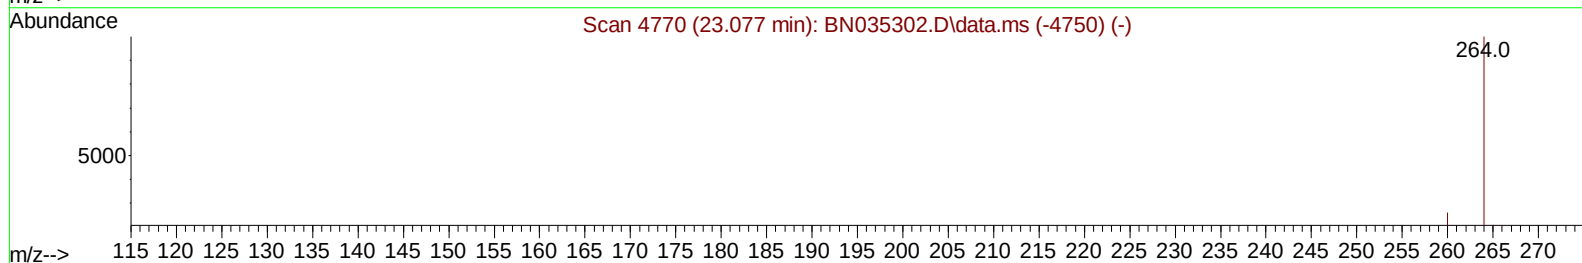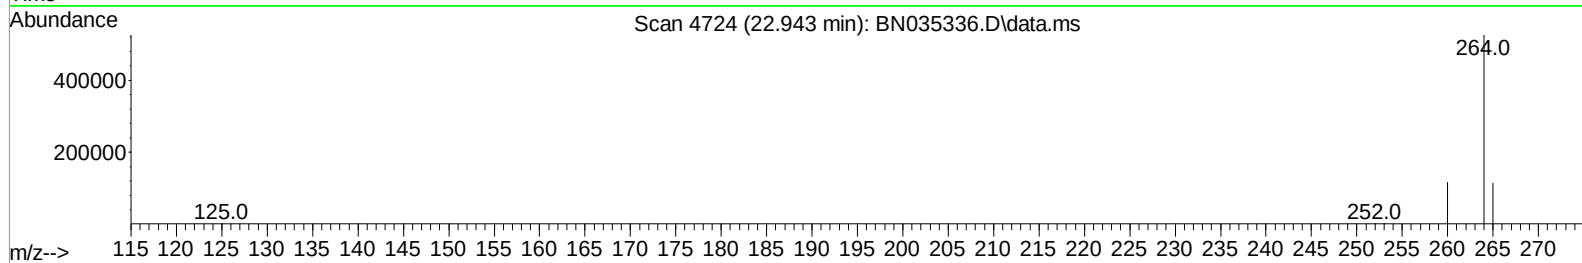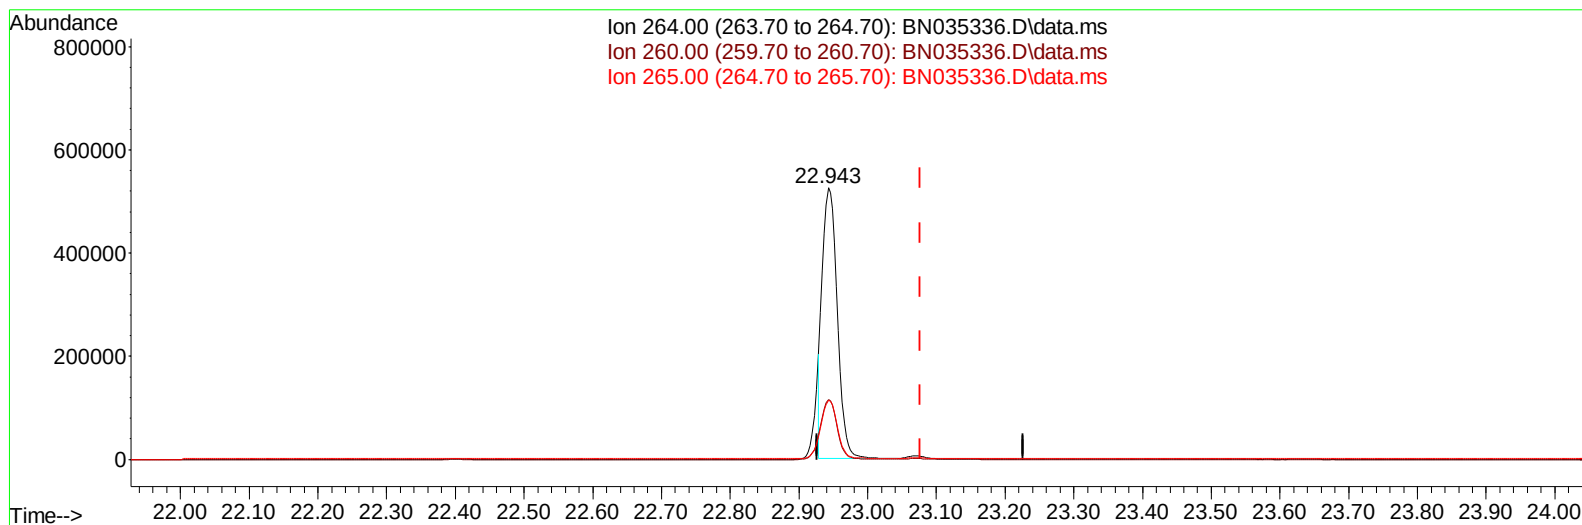

TIC: BN035336.D\data.ms

(23) Perylene-d12 (I)

22.943min (-0.134) 0.40 ng/u1

response 802343

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	22.02
265.00	75.50	21.75#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035336.D
Acq On : 27 Nov 2024 04:30
Operator : RC/JU
Sample : PB165232BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK232

Manual IntegrationsAPPROVED

Quant Time: Nov 27 05:29:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

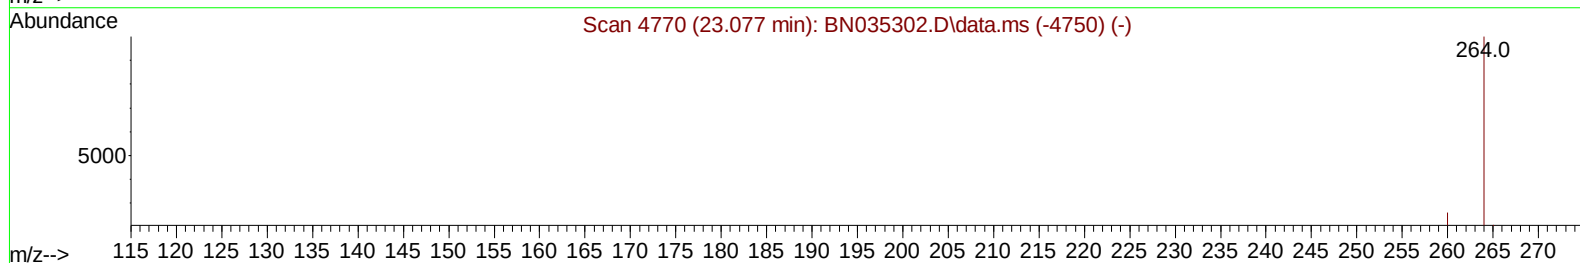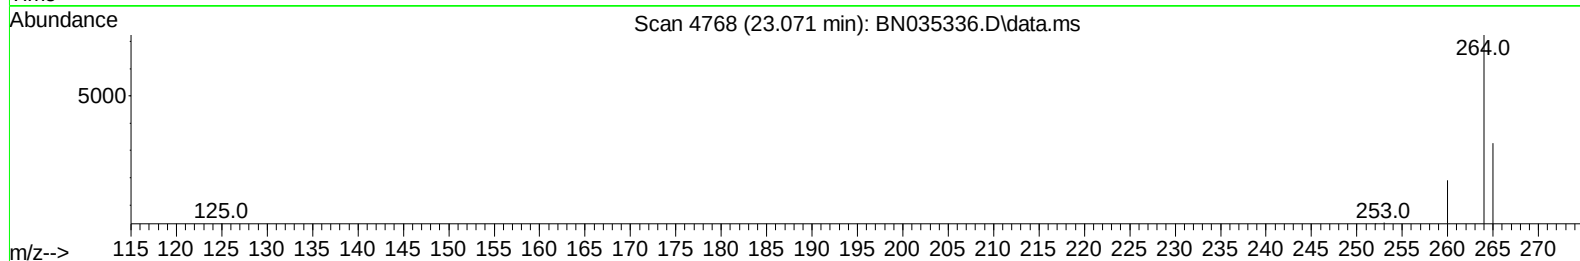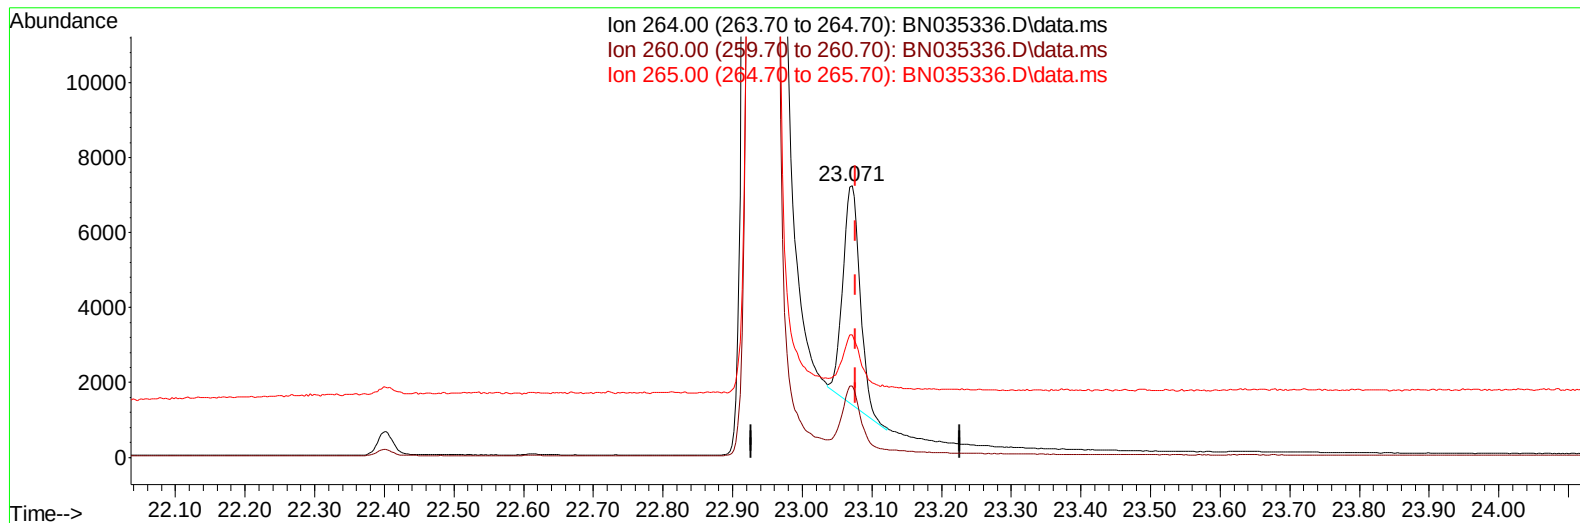

TIC: BN035336.D\data.ms

(23) Perylene-d12 (I)

23.071min (-0.006) 0.40 ng/ul m

response 9950

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	26.22
265.00	75.50	45.08#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
 Data File : BN035336.D
 Acq On : 27 Nov 2024 04:30
 Operator : RC/JU
 Sample : PB165232BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK232

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/27/2024
 Supervised By :mohammad ahmed 11/28/2024

Quant Time: Nov 27 05:29:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 26 06:09:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.310	152	5190	0.400	ng/ul	0.00
4) Naphthalene-d8	10.059	136	13820	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.967	164	8553	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.734	188	16605m	0.400	ng/ul	0.00
17) Chrysene-d12	20.976	240	9388	0.400	ng/ul	# 0.00
23) Perylene-d12	23.071	264	9950m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.972	96	29374	6.192	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.659	152	6634	0.328	ng/ul	0.00
18) Fluoranthene-d10	18.786	212	11886	0.459	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035336.D
Acq On : 27 Nov 2024 04:30
Operator : RC/JU
Sample : PB165232BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK232

Manual IntegrationsAPPROVED

Quant Time: Nov 27 05:29:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

