




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035340.D
Acq On : 27 Nov 2024 06:54
Operator : RC/JU
Sample : P4895-05MSD
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2A12MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 27 07:19:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

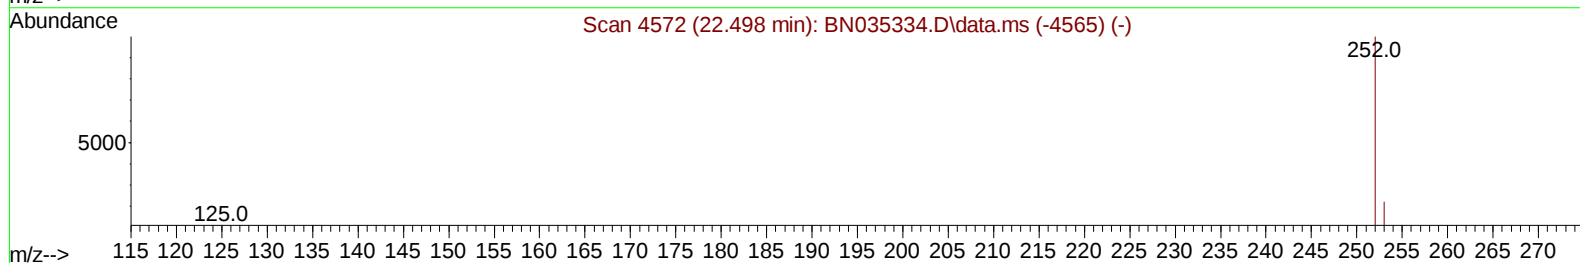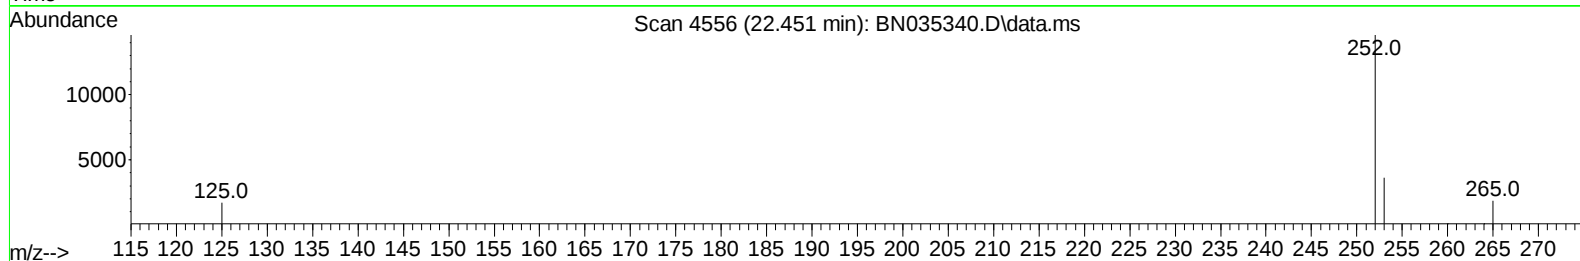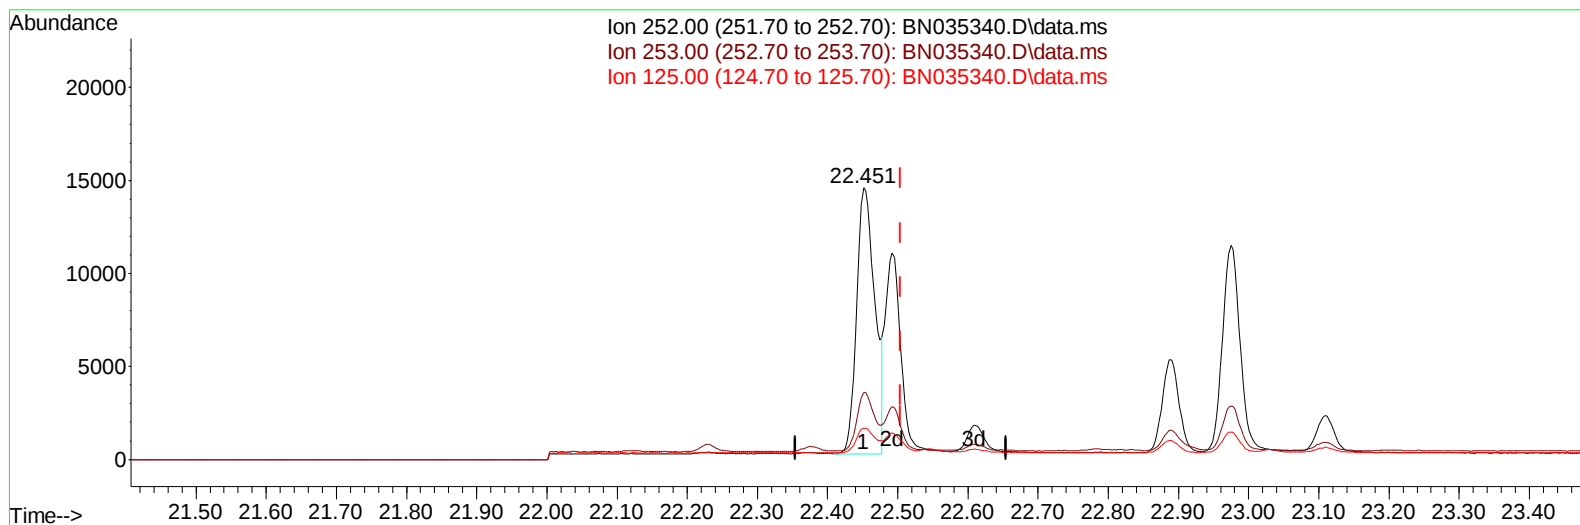

TIC: BN035340.D\data.ms

(25) Benzo(k)fluoranthene

22.451min (-0.053) 0.72 ng/u1

response 26024

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.20	24.65
125.00	10.70	11.56
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035340.D
Acq On : 27 Nov 2024 06:54
Operator : RC/JU
Sample : P4895-05MSD
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2A12MSD

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

Quant Time: Nov 27 07:19:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

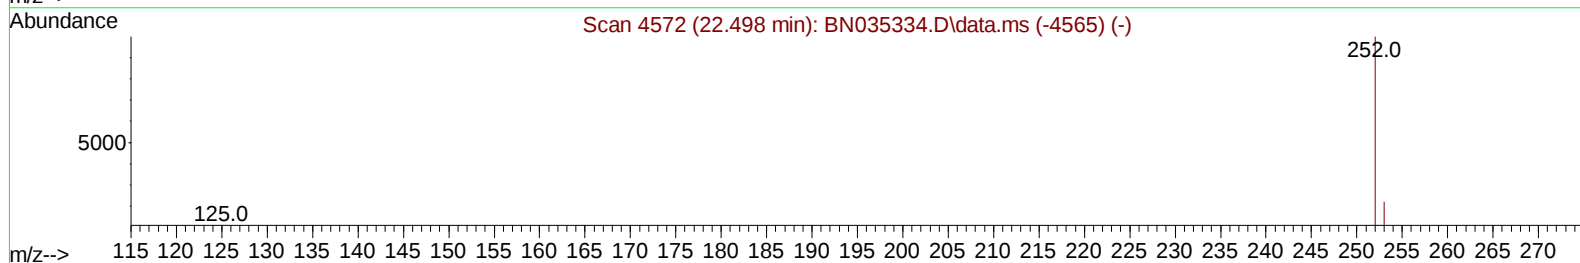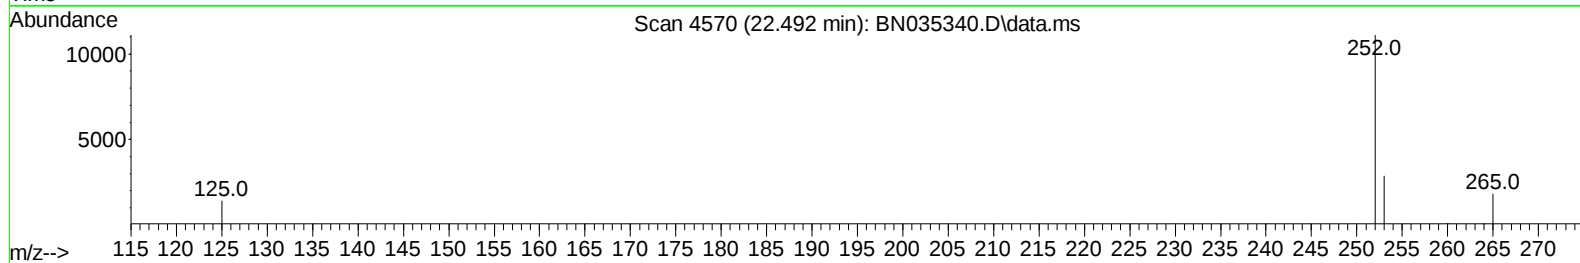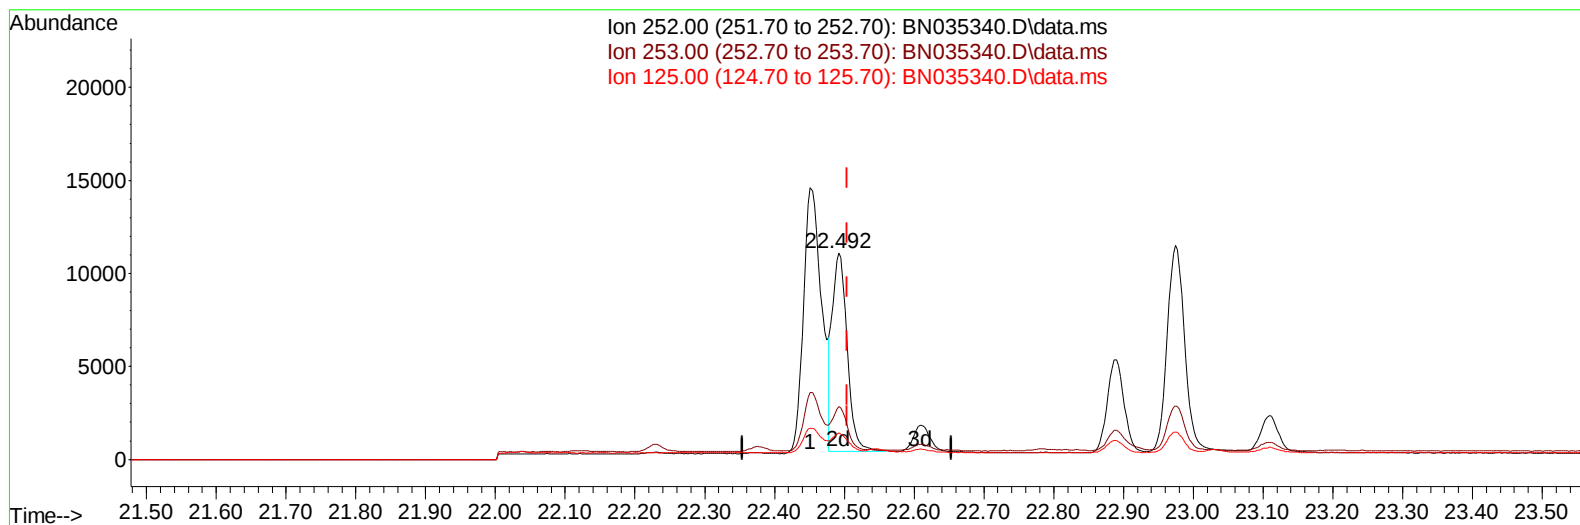

TIC: BN035340.D\data.ms

(25) Benzo(k)fluoranthene

22.492min (-0.012) 0.44 ng/u1 m

response 15925

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.20	25.72
125.00	10.70	12.89#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035340.D
Acq On : 27 Nov 2024 06:54
Operator : RC/JU
Sample : P4895-05MSD
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2A12MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 27 07:19:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

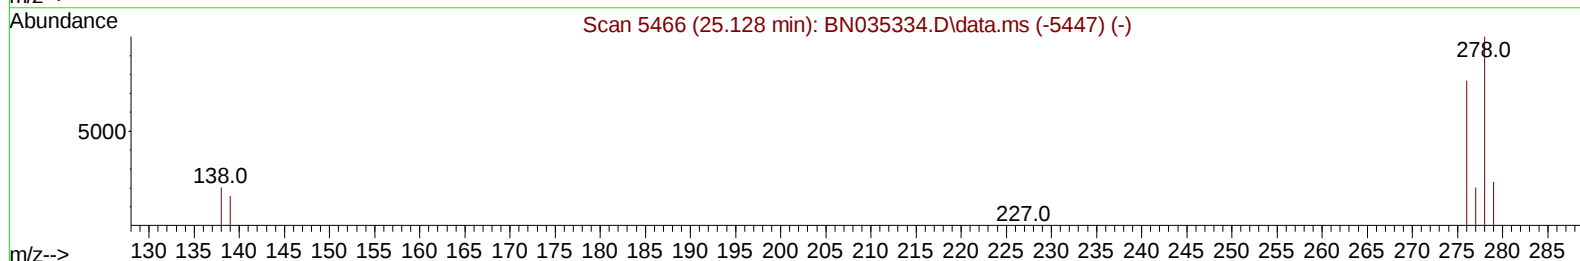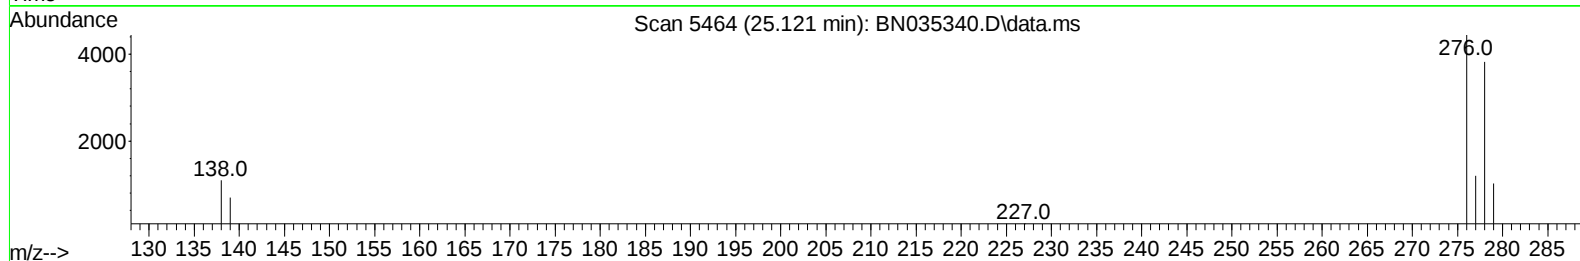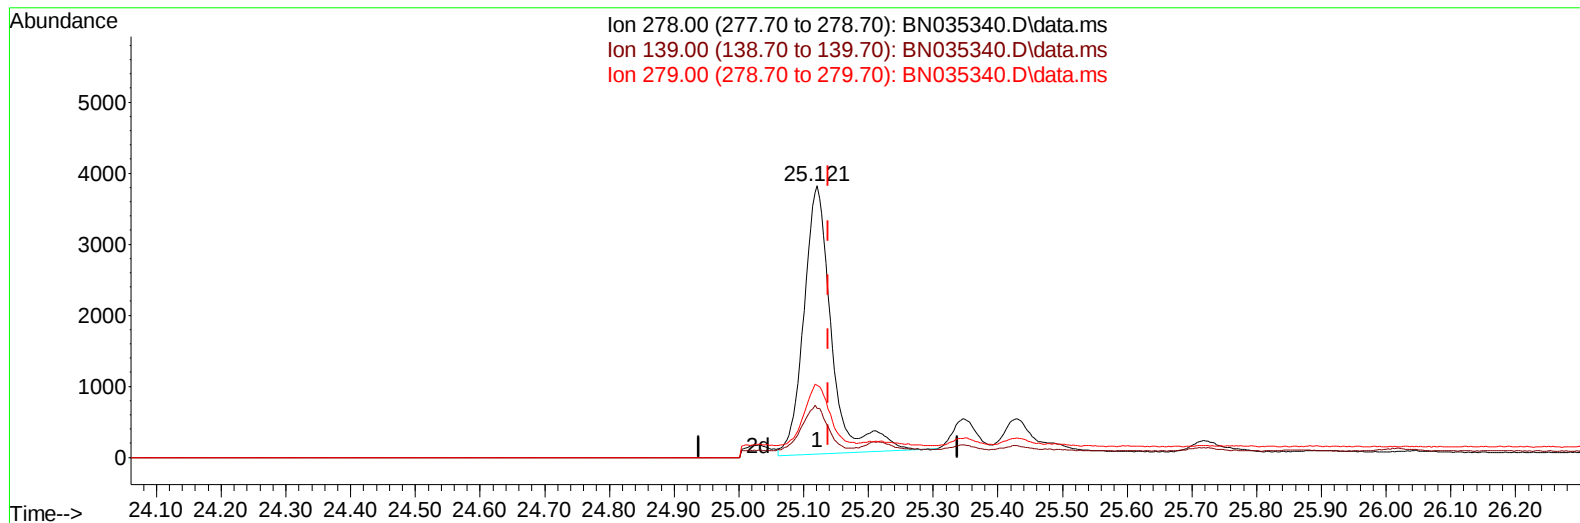

TIC: BN035340.D\data.ms

(28) Dibenzo(a,h)anthracene

25.121min (-0.017) 0.33 ng/u1

response 11245

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	13.40	18.03#
279.00	28.50	26.56
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035340.D
Acq On : 27 Nov 2024 06:54
Operator : RC/JU
Sample : P4895-05MSD
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2A12MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 27 07:19:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

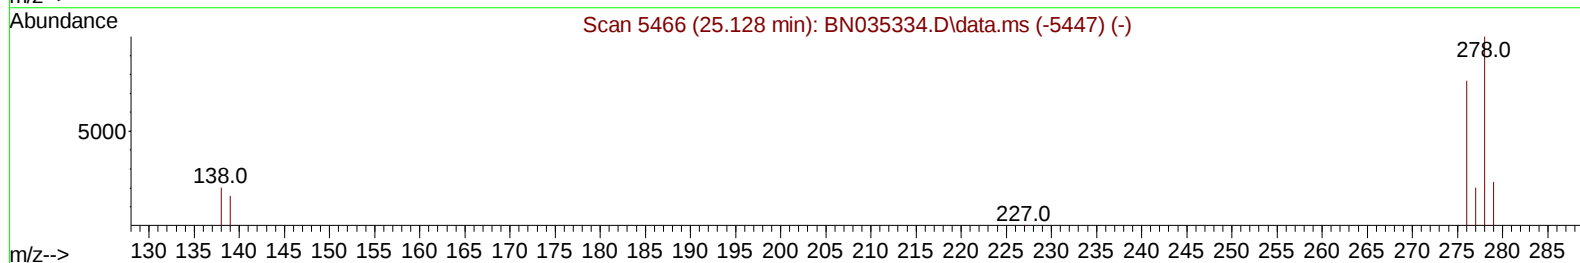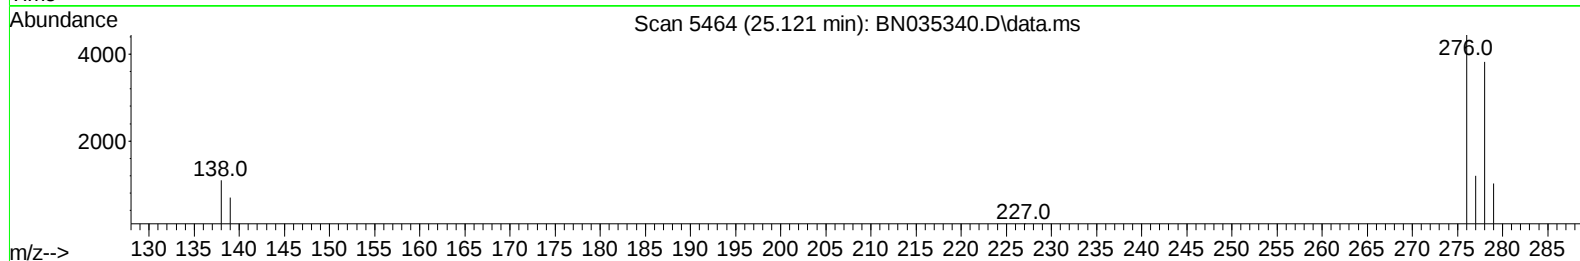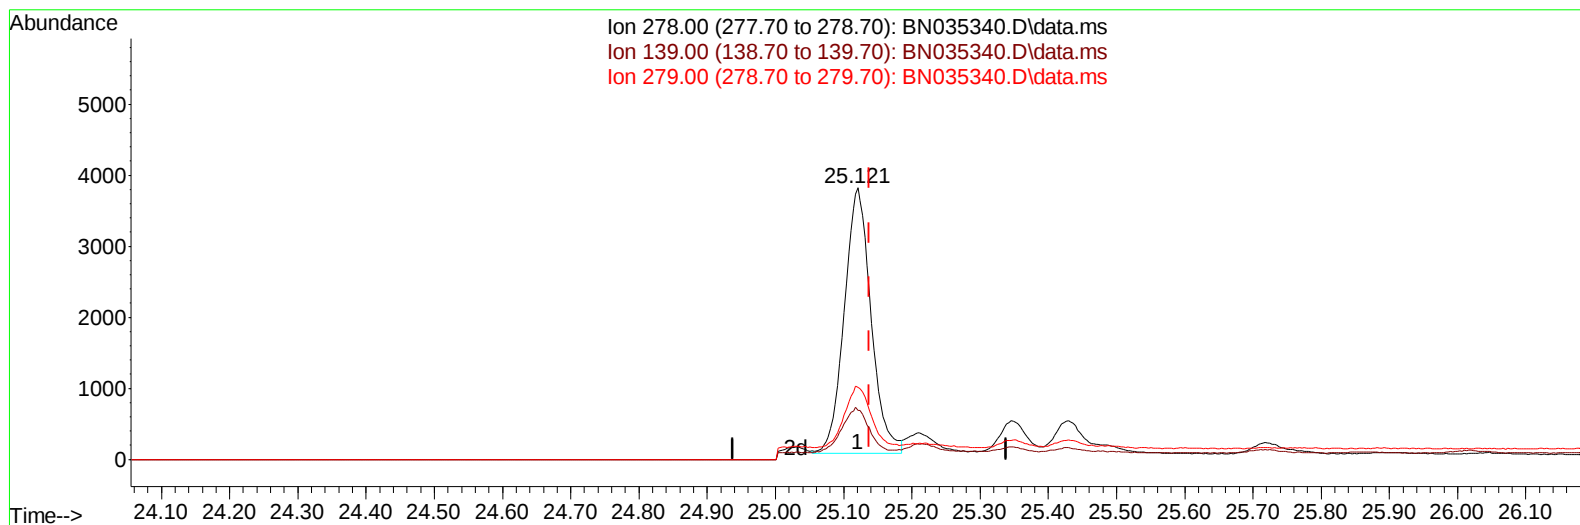

TIC: BN035340.D\data.ms

(28) Dibenzo(a,h)anthracene

25.121min (-0.017) 0.30 ng/ul m

response 10179

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	13.40	18.03#
279.00	28.50	26.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
 Data File : BN035340.D
 Acq On : 27 Nov 2024 06:54
 Operator : RC/JU
 Sample : P4895-05MSD
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2A12MSD

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/27/2024
 Supervised By :mohammad ahmed 11/28/2024

Quant Time: Nov 27 07:19:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 26 06:09:15 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.309	152		3758	0.400	ng/ul	0.00
4) Naphthalene-d8	10.058	136		9492	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.967	164		5321	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.734	188		10741	0.400	ng/ul	# 0.00
17) Chrysene-d12	20.973	240		9453	0.400	ng/ul	# 0.00
23) Perylene-d12	23.065	264		10606	0.400	ng/ul	#-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	2.976	96		1108	0.323	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.659	152		2817	0.203	ng/ul	0.00
18) Fluoranthene-d10	18.781	212		6609	0.253	ng/ul	0.00
Target Compounds							
							Qvalue
2) 1,4-Dioxane	3.005	88		3237	0.868	ng/ul	93
5) Naphthalene	10.102	128		5113	0.214	ng/ul	100
7) 2-Methylnaphthalene	11.736	142		3423	0.206	ng/ul	98
8) 1-Methylnaphthalene	11.961	142		3470	0.207	ng/ul	99
10) Acenaphthylene	13.680	152		6896	0.327	ng/ul	98
11) Acenaphthene	14.032	153		3861	0.239	ng/ul	98
12) Fluorene	15.031	166		4499	0.237	ng/ul	99
14) Pentachlorophenol	16.392	266		238	0.095	ng/ul	93
15) Phenanthrene	16.772	178		14246	0.502	ng/ul	99
16) Anthracene	16.865	178		7935	0.301	ng/ul	99
19) Fluoranthene	18.814	202		35696	1.085	ng/ul#	95
20) Pyrene	19.181	202		31680	0.925	ng/ul#	93
21) Benzo(a)anthracene	20.955	228		20198	0.616	ng/ul	97
22) Chrysene	21.008	228		21184	0.642	ng/ul	99
24) Benzo(b)fluoranthene	22.451	252		26024	0.742	ng/ul	95
25) Benzo(k)fluoranthene	22.492	252		15925m	0.441	ng/ul	
26) Benzo(a)pyrene	22.975	252		19467	0.608	ng/ul	94
27) Indeno(1,2,3-cd)pyrene	25.104	276		20310	0.469	ng/ul#	82
28) Dibenzo(a,h)anthracene	25.121	278		10179m	0.300	ng/ul	
29) Benzo(g,h,i)perylene	25.721	276		17388	0.510	ng/ul#	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035340.D
Acq On : 27 Nov 2024 06:54
Operator : RC/JU
Sample : P4895-05MSD
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2A12MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 27 07:19:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

