

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
 Data File : BN035308.D
 Acq On : 26 Nov 2024 09:59
 Operator : RC/JU
 Sample : P4875-22
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2A24

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/27/2024
 Supervised By :mohammad ahmed 11/28/2024

Quant Time: Nov 26 22:12:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 26 06:09:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.309	152	2861	0.400	ng/ul	0.00
4) Naphthalene-d8	10.058	136	6920	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.972	164	3919	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.738	188	7906m	0.400	ng/ul	0.00
17) Chrysene-d12	20.982	240	6097	0.400	ng/ul	# 0.00
23) Perylene-d12	23.080	264	5876m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.972	96	14095	5.390	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.664	152	2982	0.294	ng/ul	0.00
18) Fluoranthene-d10	18.791	212	7563	0.450	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.108	128	357	0.020	ng/ul#	61

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112624\
Data File : BN035308.D
Acq On : 26 Nov 2024 09:59
Operator : RC/JU
Sample : P4875-22
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E2A24

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024


Quant Time: Nov 26 22:12:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

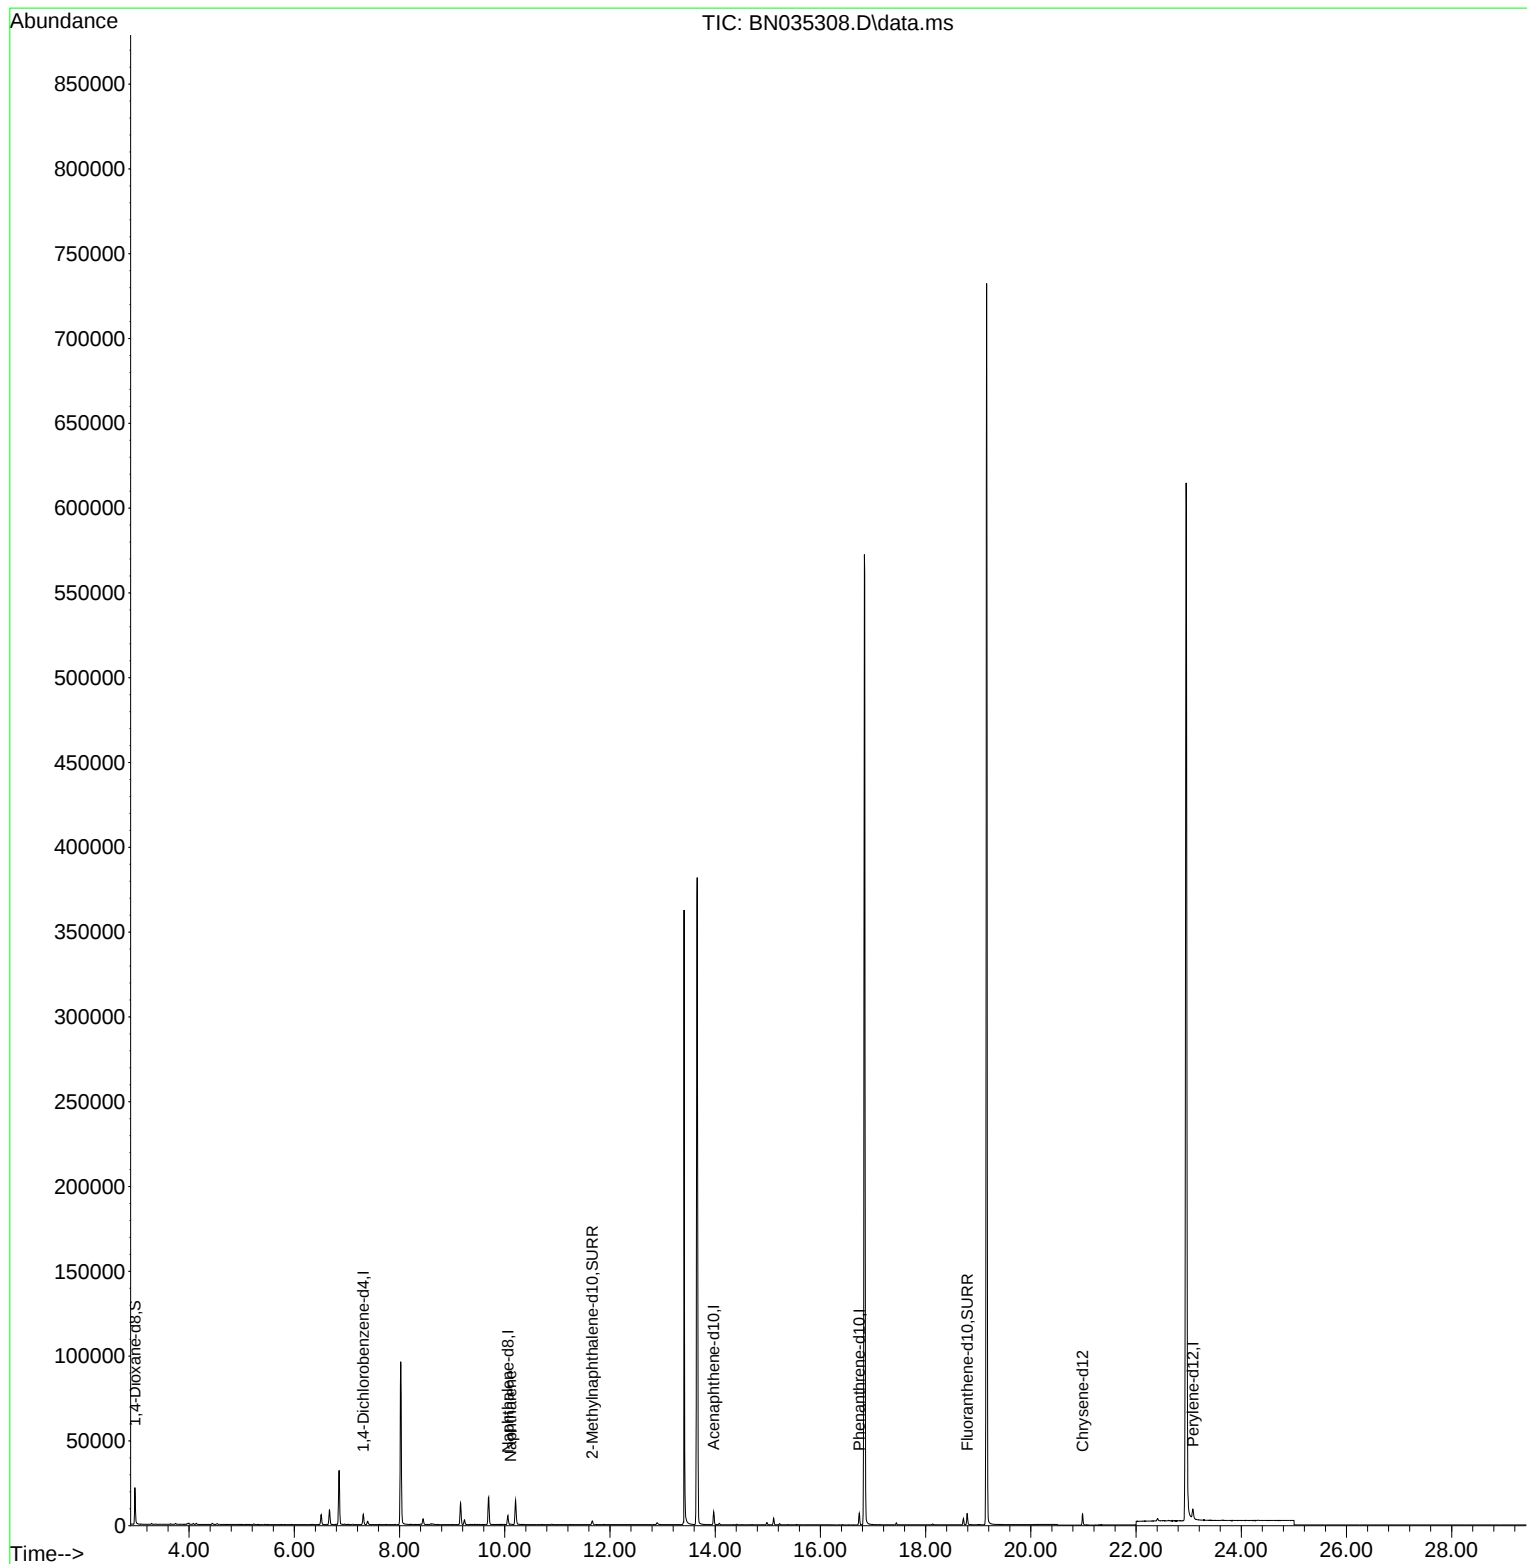

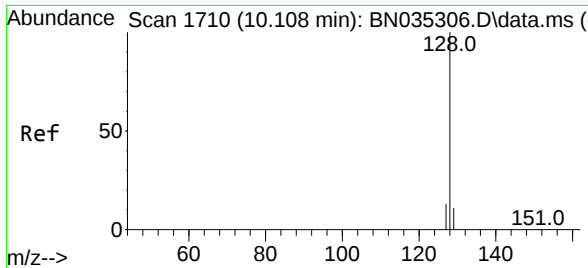

#5
Naphthalene
Concen: 0.020 ng/ul
RT: 10.108 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN035308.D
Acq: 26 Nov 2024 09:59

Instrument :
BNA_N
ClientSampleId :
E2A24

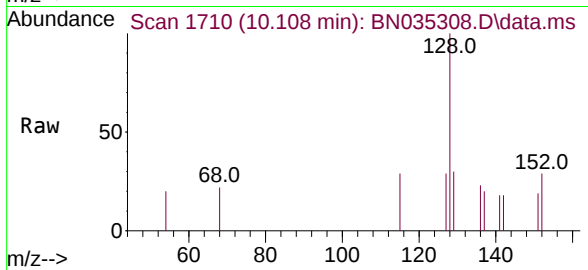

Tgt Ion:	128	Resp:	35
Ion	Ratio	Lower	Upper
128	100		
129	29.7	9.9	14.9
127	28.7	11.4	17.2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/28/2024

