
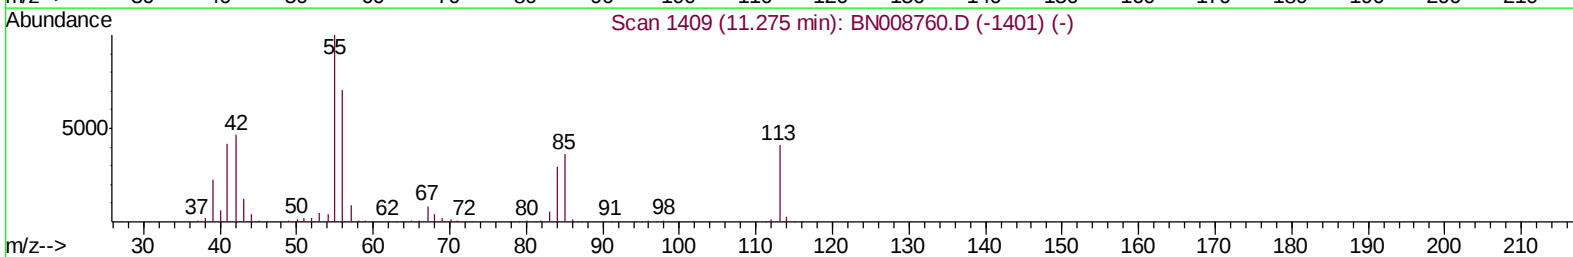
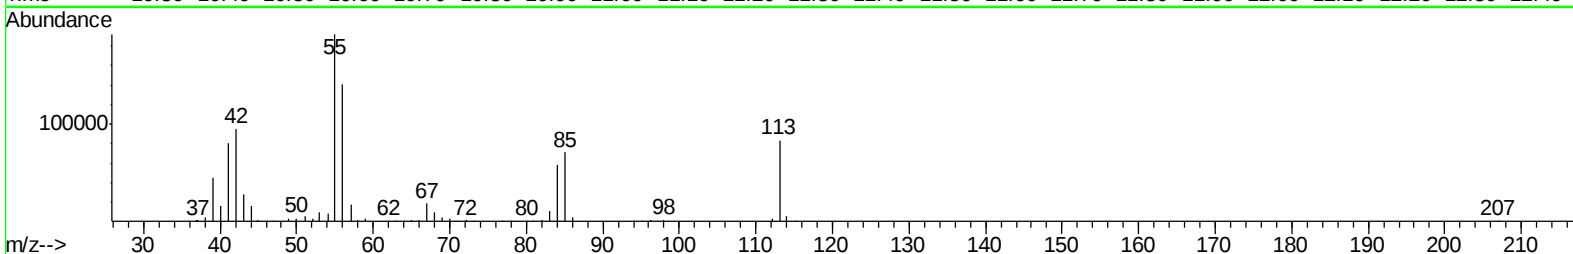


Data File : BN008794.D
Acq On : 28 Nov 2019 13:00
Operator : JU
Sample : SSTDCCC020
Misc :
ALS Vial : 35 Sample Multiplier: 1

Quant Time: Nov 29 00:28:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 27 15:51:44 2019
Response via : Initial Calibration

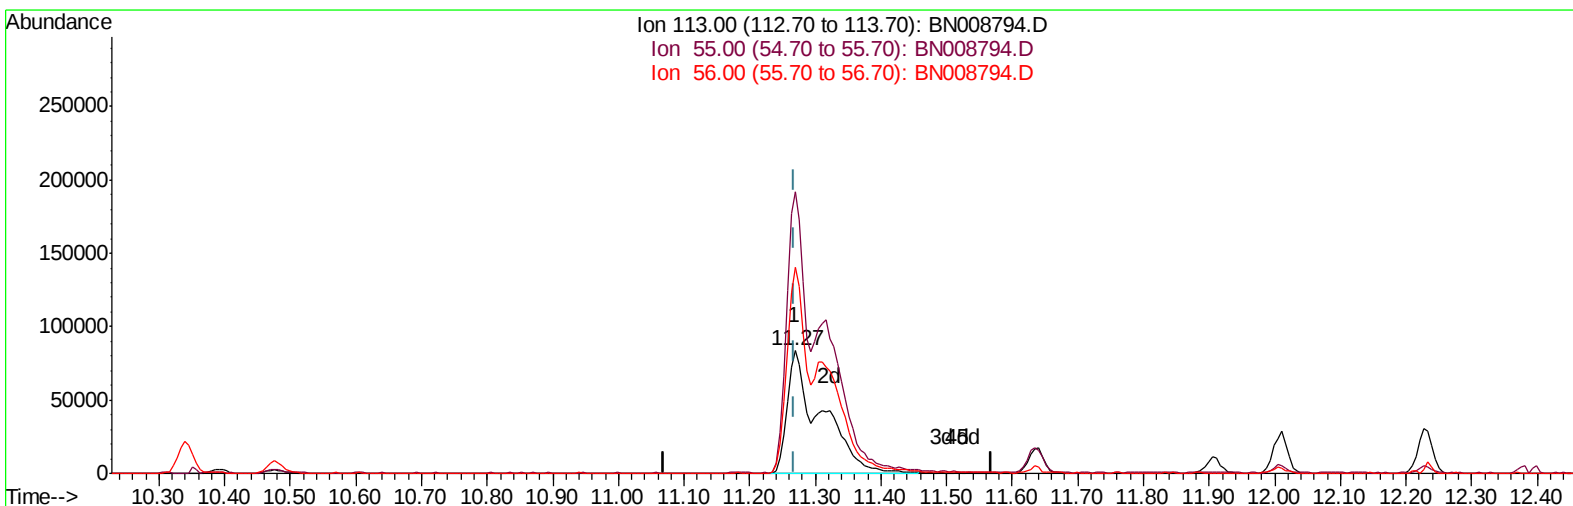

TIC: BN008794.D

(32) Caprolactam

11.269min (+0.000) 20.48ng/ul m

response 301387

Ion	Exp%	Act%
113.00	100	100
55.00	232.90	230.16
56.00	168.90	168.84
0.00	0.00	0.00