
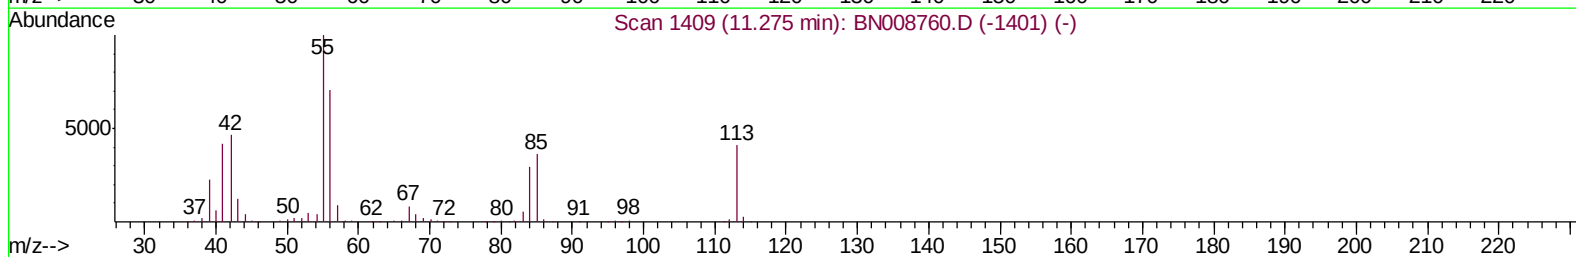
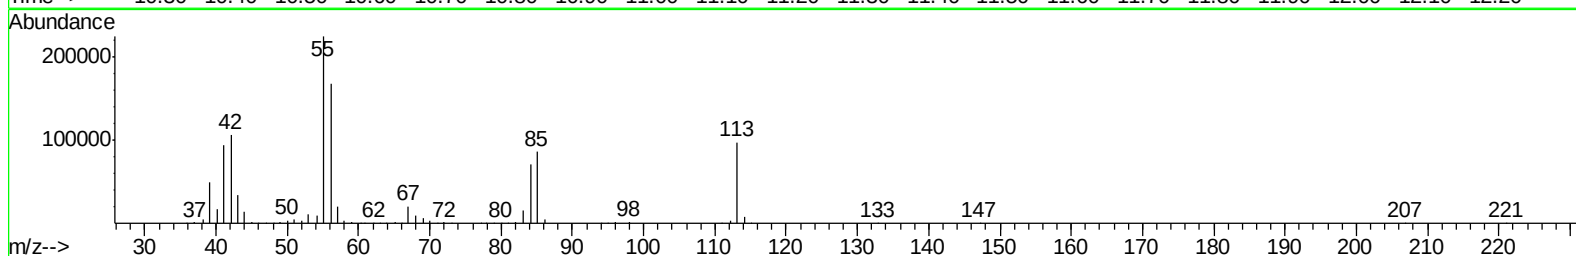


Data File : BN008807.D
Acq On : 28 Nov 2019 20:43
Operator : JU
Sample : SSTDCCC020EC
Misc :
ALS Vial : 48 Sample Multiplier: 1

Quant Time: Nov 29 00:30:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 27 15:51:44 2019
Response via : Initial Calibration

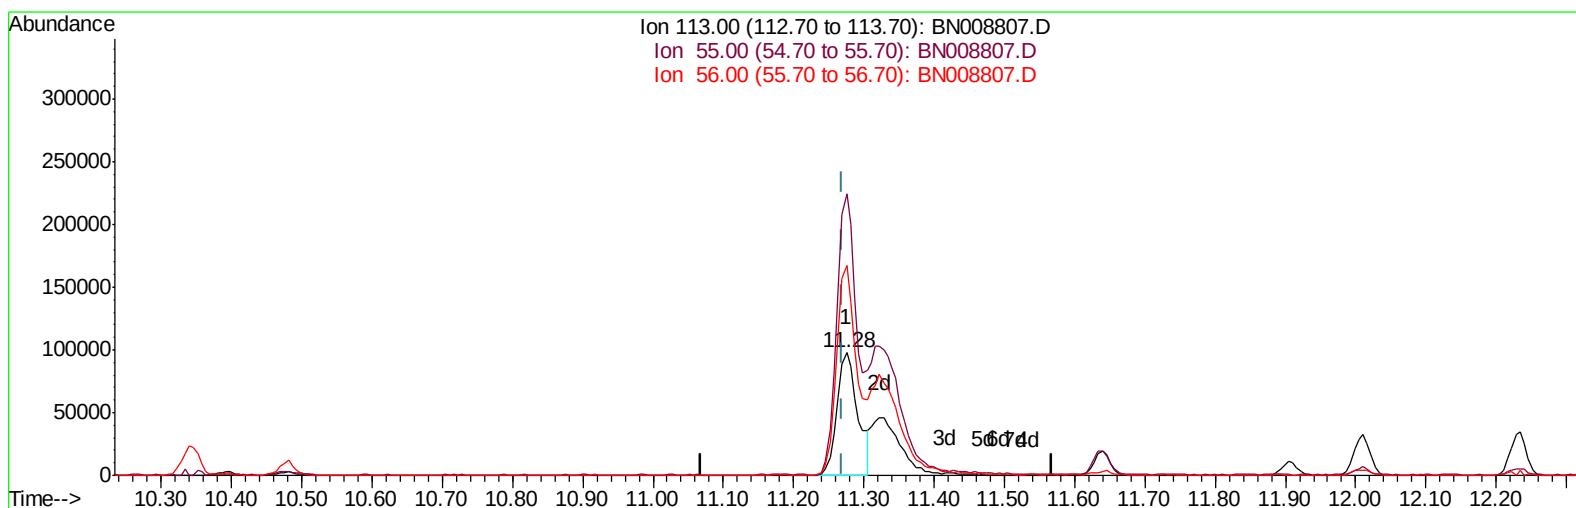

TIC: BN008807.D

(32) Caprolactam

11.275min (+0.006) 11.29ng/ul

response 199538

Ion	Exp%	Act%
113.00	100	100
55.00	232.90	229.83
56.00	168.90	171.71
0.00	0.00	0.00