

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112719\
 Data File : BN008761.D
 Acq On : 27 Nov 2019 17:20
 Operator : JU
 Sample : PB124853BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Nov 28 01:20:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 27 15:51:44 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	483091	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	2278337	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.21	164	1646176	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.96	188	3751447	20.00	ng/ul	0.00
77) Chrysene-d12	21.16	240	3642085	20.00	ng/ul	0.00
85) Perylene-d12	23.32	264	3911972	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.18	96	78293	7.09	ng/uL	0.00
5) Phenol-d5	6.78	99	1542535	31.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	1048028	34.28	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	1137721	32.91	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	1261637	32.14	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	614518	34.96	ng/ul	0.00
22) 2-Nitrophenol-d4	9.44	143	690080	36.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	1198151	31.69	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	1904384	39.63	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	4806044	36.64	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	5077692	35.04	ng/ul	0.00
51) 4-Nitrophenol-d4	14.42	143	898088	33.77	ng/ul	0.00
57) Fluorene-d10	15.21	176	3921504	35.39	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.33	200	700005	32.30	ng/ul	0.00
70) Anthracene-d10	17.06	188	6086175	34.27	ng/ul	0.00
78) Pyrene-d10	19.36	212	7157654	35.23	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.19	264	7568725	37.08	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	8.29	70	34042	1.026 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112719\
Data File : BN008761.D
Acq On : 27 Nov 2019 17:20
Operator : JU
Sample : PB124853BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Nov 28 01:20:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 27 15:51:44 2019
Response via : Initial Calibration

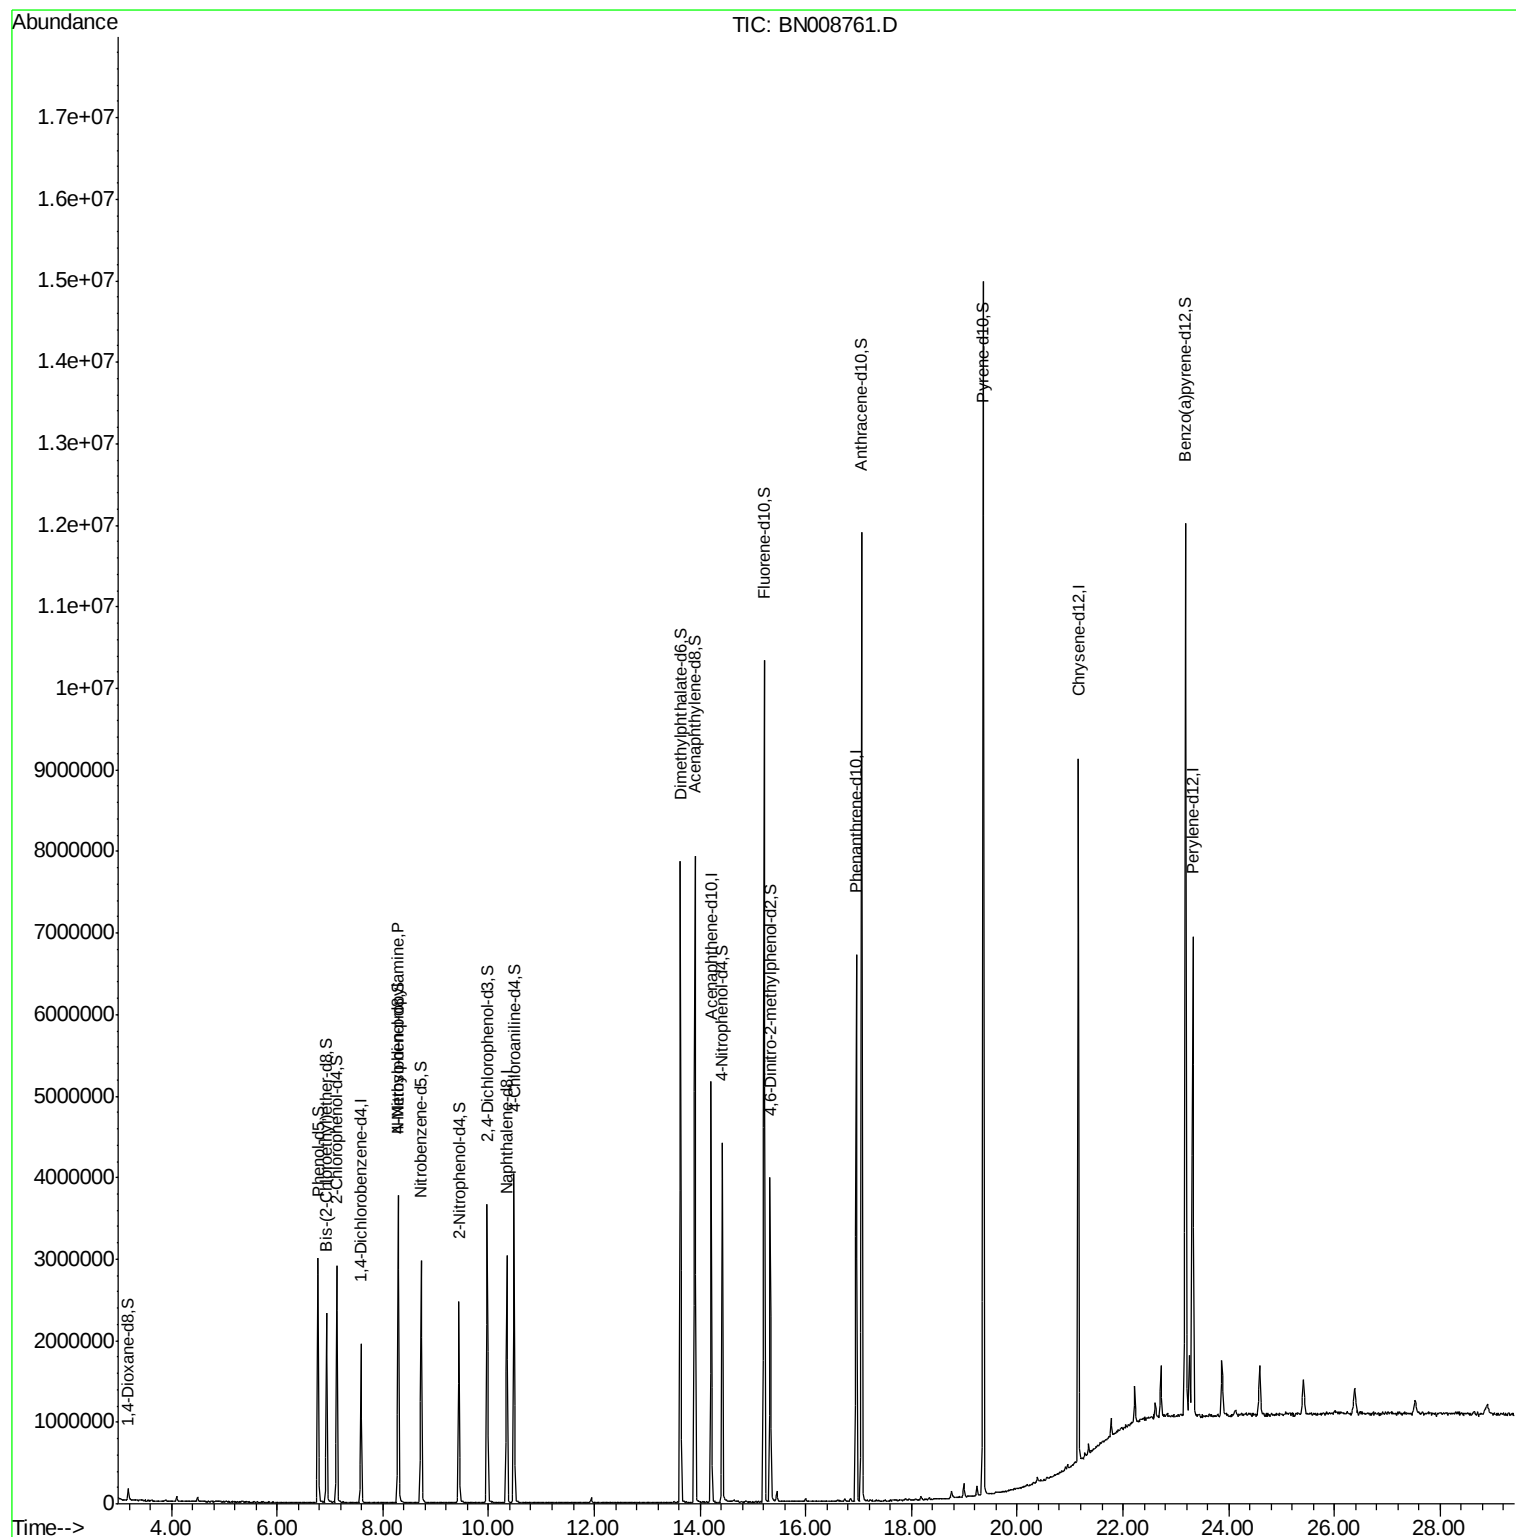

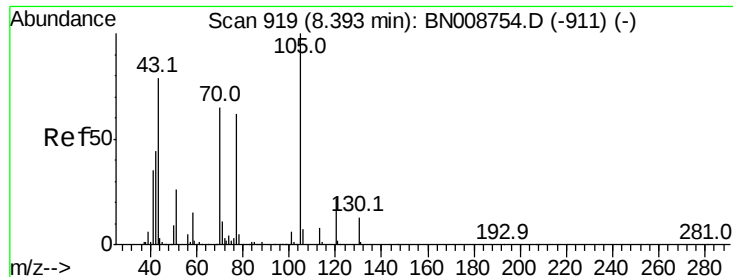

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.026 ng/ul
 RT: 8.29 min Scan# 902
 Delta R.T. -0.10 min
 Lab File: BN008761.D
 Acq: 27 Nov 2019 17:20

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion	Ion	Ratio	Lower	Upper
70	100			
42	396.9	55.1	82.7#	
101	0.0	7.5	11.3#	
130	0.0	16.4	24.6#	

