

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112719\
 Data File : BN008805.D
 Acq On : 28 Nov 2019 19:32
 Operator : JU
 Sample : K6086-02
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFLY9

Quant Time: Nov 29 00:30:12 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 27 15:51:44 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	631523	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	2922144	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.21	164	1901870	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.96	188	3989942	20.00	ng/ul	0.00
77) Chrysene-d12	21.16	240	3427094	20.00	ng/ul	0.00
85) Perylene-d12	23.32	264	3428305	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.18	96	65127	4.51	ng/uL	0.00
5) Phenol-d5	6.77	99	360331	5.56	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	1022238	25.58	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	967157	21.40	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	702240	13.69	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	632875	28.07	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	712250	29.25	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	1210777	24.97	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	106858	1.73	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	4154624	27.42	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	5000142	29.87	ng/ul	0.00
51) 4-Nitrophenol-d4	14.42	143	163070	5.31	ng/ul	0.00
57) Fluorene-d10	15.21	176	3607334	28.18	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.33	200	578780	25.11	ng/ul	0.00
70) Anthracene-d10	17.05	188	5486872	29.05	ng/ul	0.00
78) Pyrene-d10	19.35	212	5897000	30.84	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.18	264	5280678	29.52	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.67	163	317543	2.146	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112719\
Data File : BN008805.D
Acq On : 28 Nov 2019 19:32
Operator : JU
Sample : K6086-02
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFLY9

Quant Time: Nov 29 00:30:12 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 27 15:51:44 2019
Response via : Initial Calibration

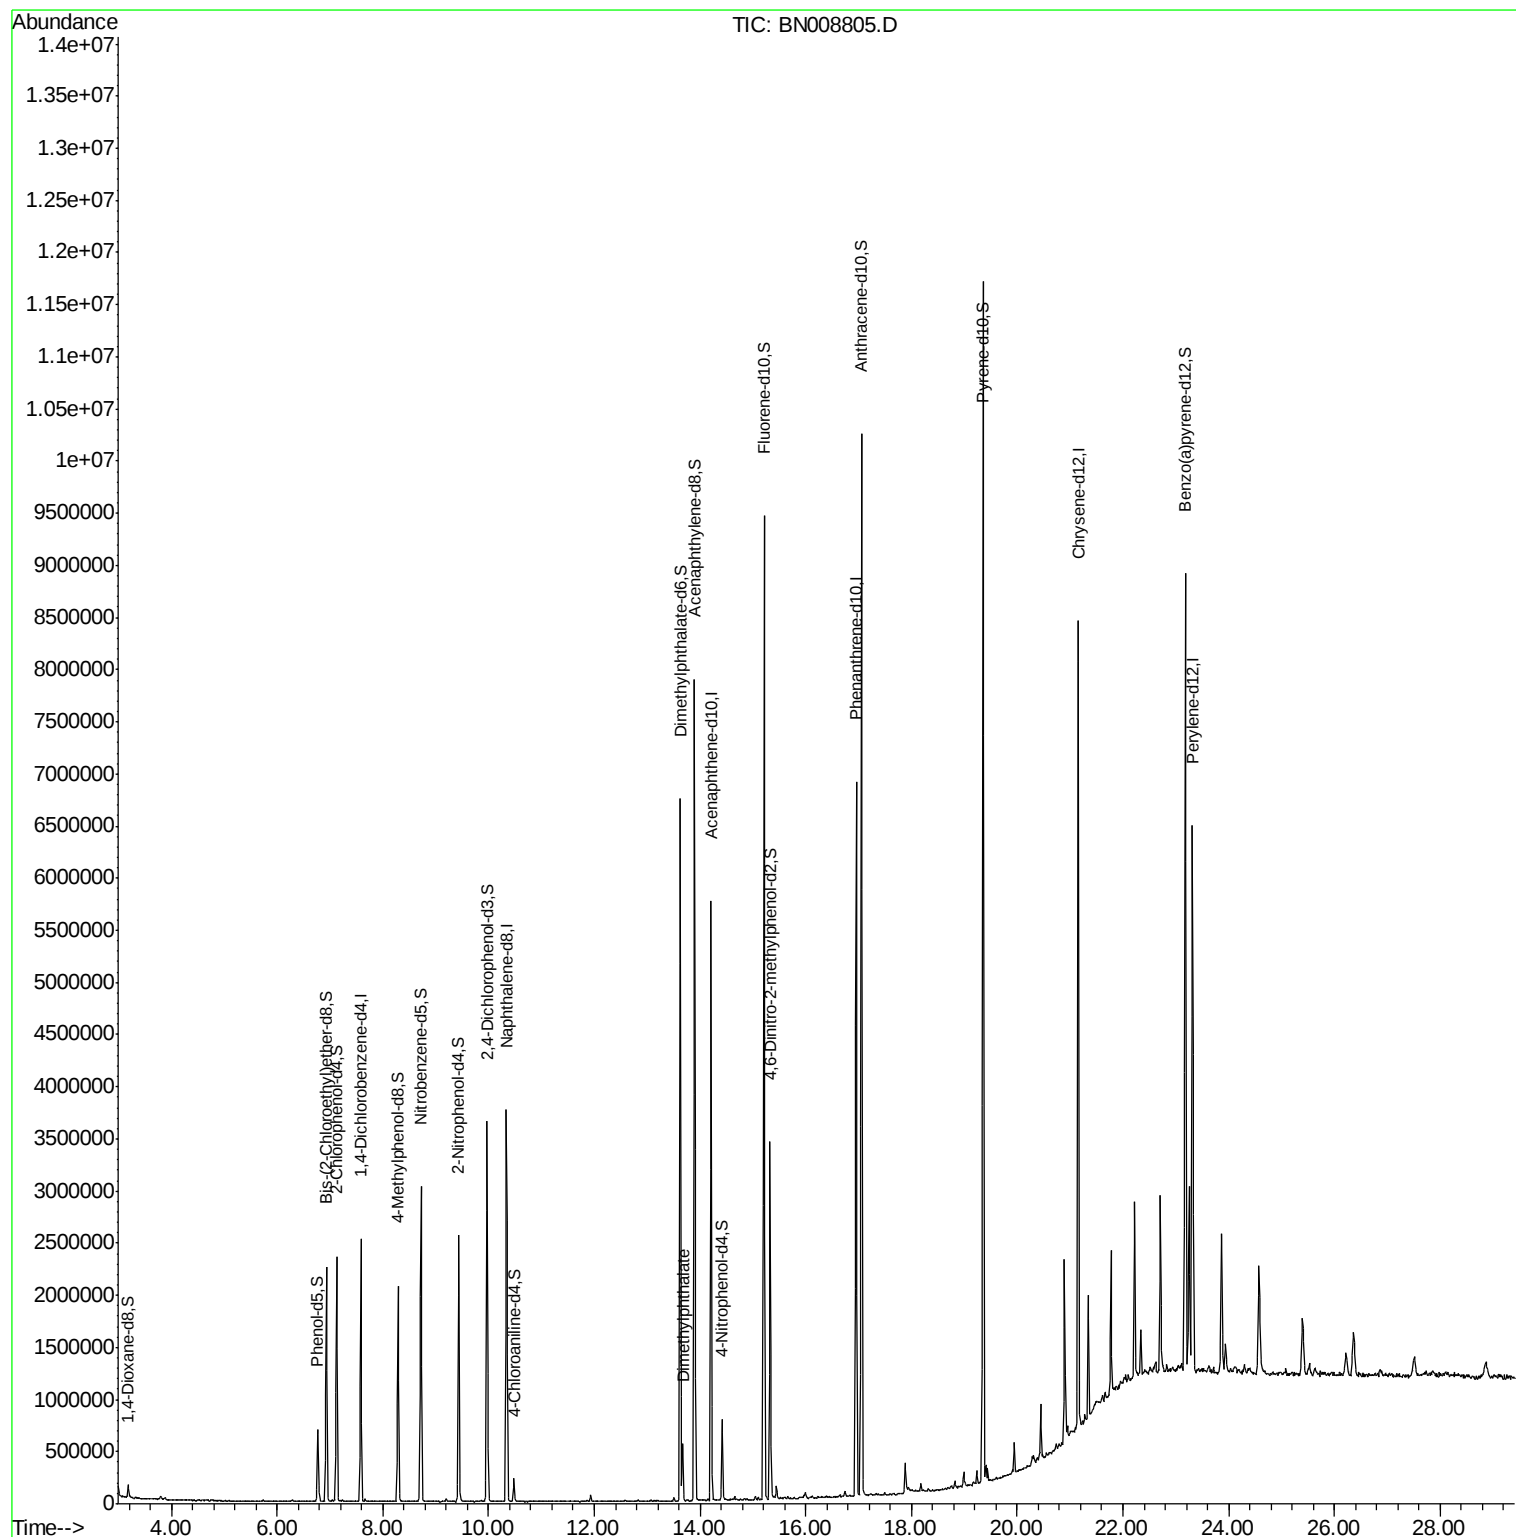

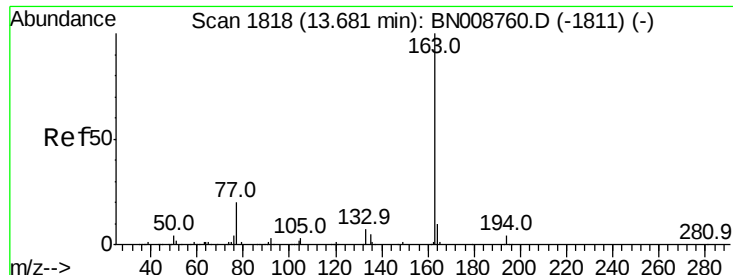

#44

Dimethylphthalate

Concen: 2.146 ng/ul

RT: 13.67 min Scan# 1817

Delta R.T. -0.01 min

Lab File: BN008805.D

Acq: 28 Nov 2019 19:32

Instrument :

BNA_N

ClientSampleId :

BFLY9


Tot Ion:163 Resp: 317543

Ion Ratio Lower Upper

163 100

194 4.5 3.3 4.9

164 9.6 7.9 11.9

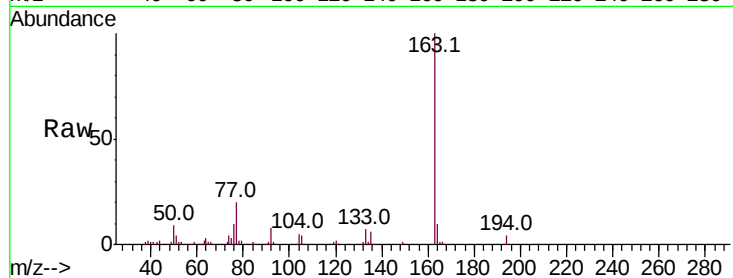

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

