

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112719\
 Data File : BN008806.D
 Acq On : 28 Nov 2019 20:08
 Operator : JU
 Sample : K6086-05
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFLZ0

Quant Time: Nov 29 00:30:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 27 15:51:44 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	753075	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	3389906	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.21	164	2199339	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.96	188	4580490	20.00	ng/ul	0.00
77) Chrysene-d12	21.16	240	4048556	20.00	ng/ul	0.00
85) Perylene-d12	23.32	264	3894660	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.18	96	66861	3.88	ng/uL	0.00
5) Phenol-d5	6.77	99	371534	4.81	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	1119302	23.49	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	1044467	19.38	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	707869	11.57	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	706607	27.01	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	783836	27.75	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	1268374	22.55	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	101176	1.42	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	4264292	24.34	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	5283963	27.30	ng/ul	0.00
51) 4-Nitrophenol-d4	14.42	143	151907	4.28	ng/ul	0.00
57) Fluorene-d10	15.21	176	3747105	25.31	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.33	200	590795	22.32	ng/ul	0.00
70) Anthracene-d10	17.05	188	5658321	26.09	ng/ul	0.00
78) Pyrene-d10	19.35	212	6117356	27.09	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.18	264	5358055	26.36	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.67	163	304640	1.781	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112719\
Data File : BN008806.D
Acq On : 28 Nov 2019 20:08
Operator : JU
Sample : K6086-05
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFLZ0

Quant Time: Nov 29 00:30:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 27 15:51:44 2019
Response via : Initial Calibration

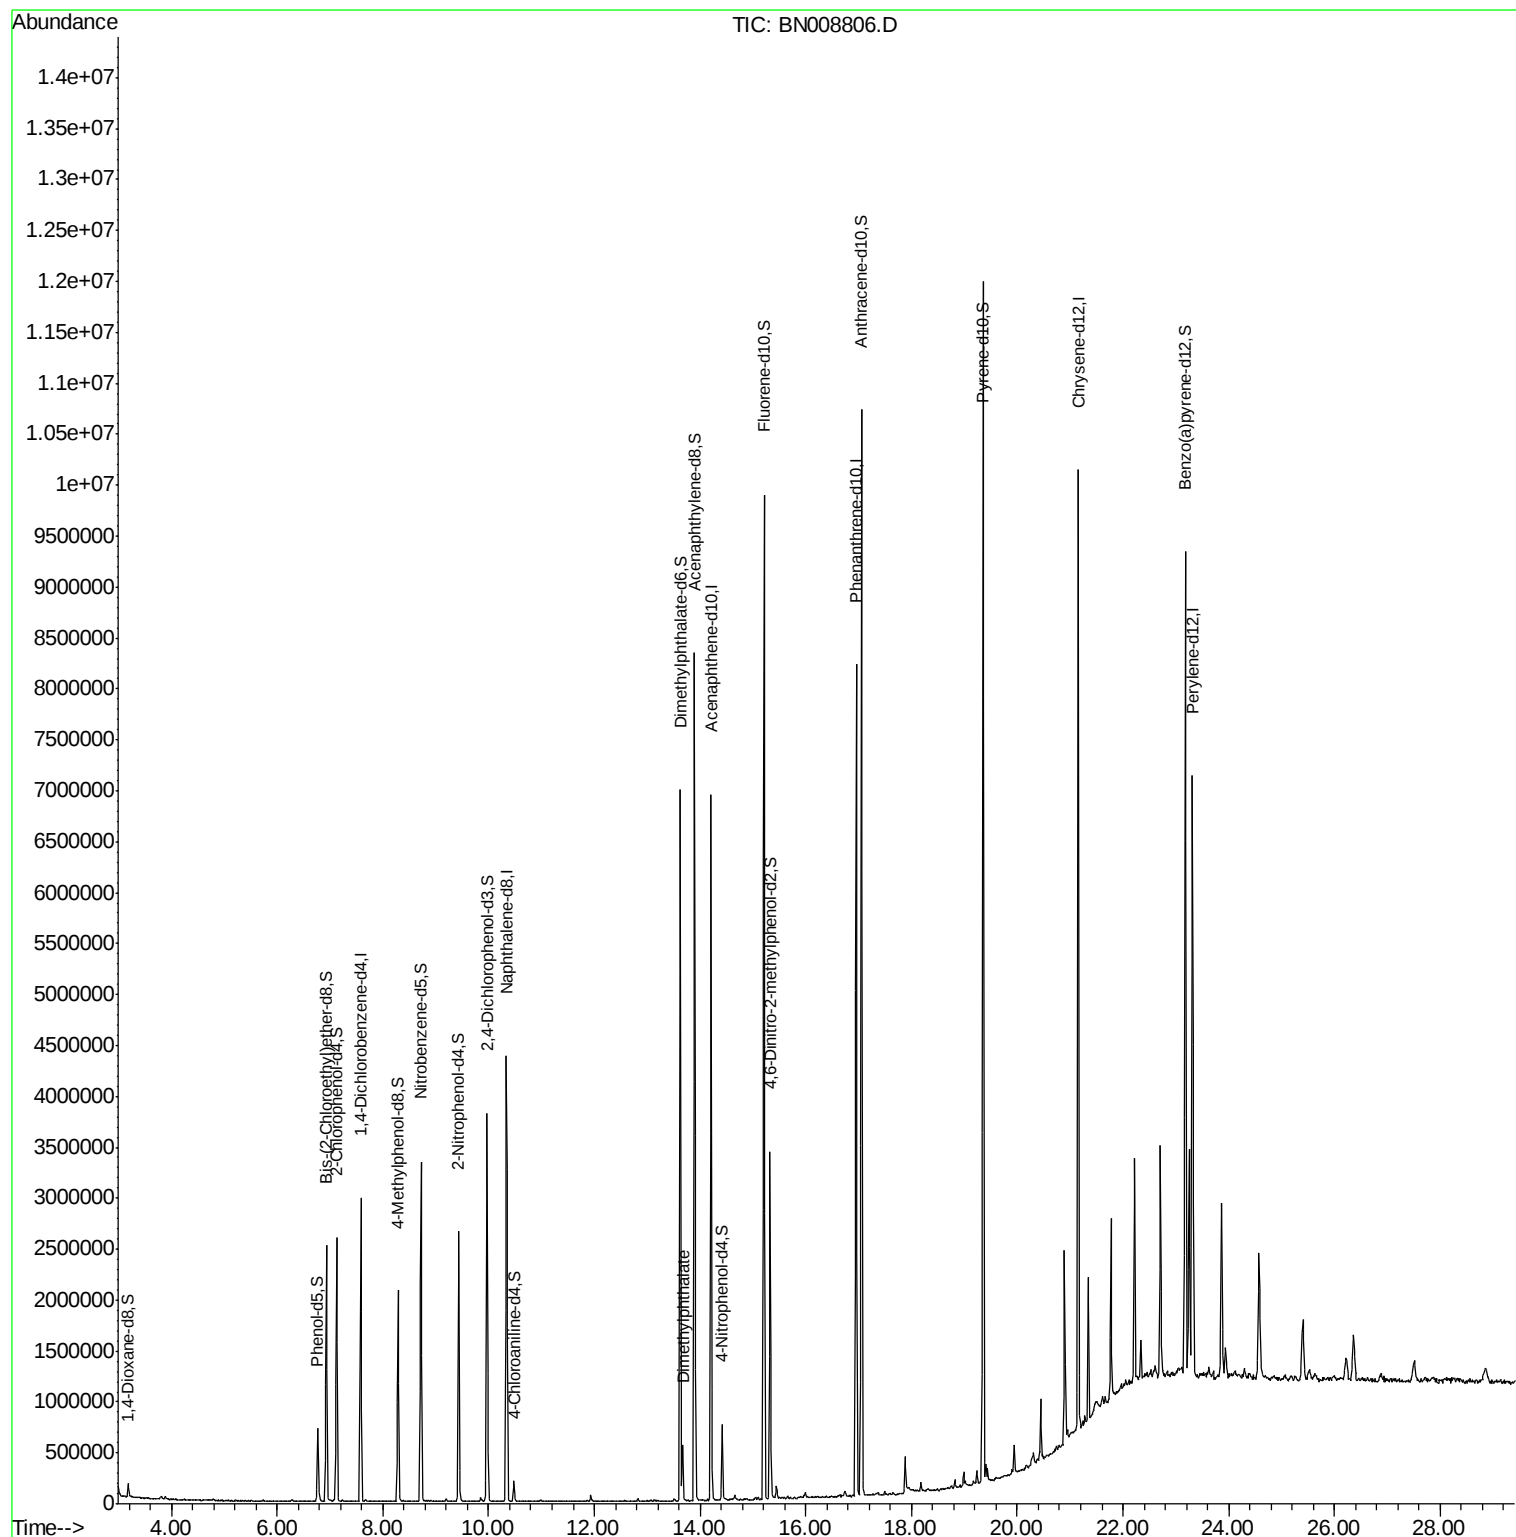

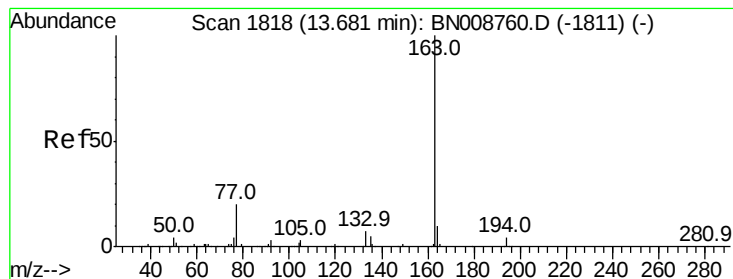

#44

Dimethylphthalate

Concen: 1.781 ng/ul

RT: 13.67 min Scan# 1817

Delta R.T. -0.01 min

Lab File: BN008806.D

Acq: 28 Nov 2019 20:08

Instrument :

BNA_N

ClientSampleId :

BFLZ0


Tot Ion:163 Resp: 304640

Ion Ratio Lower Upper

163 100

194 4.1 3.3 4.9

164 10.7 7.9 11.9

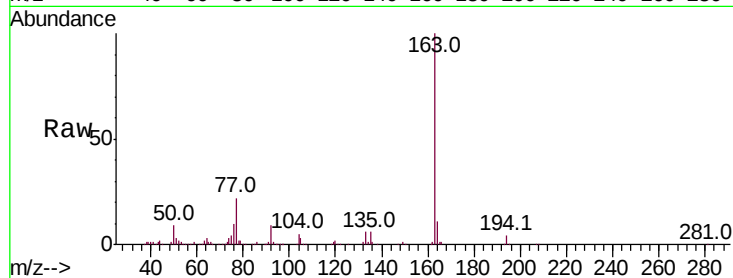

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

