

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112719\
 Data File : BN008779.D
 Acq On : 28 Nov 2019 04:05
 Operator : JU
 Sample : K5889-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLLP6

Quant Time: Nov 28 05:50:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 28 01:33:10 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	410290	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	1885615	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.21	164	1310654	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.96	188	2989452	20.00	ng/ul	0.00
77) Chrysene-d12	21.15	240	2870634	20.00	ng/ul	0.00
85) Perylene-d12	23.31	264	3418393	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.18	96	44969	4.79	ng/uL	0.00
5) Phenol-d5	6.77	99	895693	21.28	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	629312	24.24	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	670239	22.83	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	735868	22.07	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	353598	24.30	ng/ul	0.00
22) 2-Nitrophenol-d4	9.44	143	379121	24.13	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	686895	21.95	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	1003839	25.24	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	2575354	24.66	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	2935322	25.44	ng/ul	0.00
51) 4-Nitrophenol-d4	14.42	143	420394	19.85	ng/ul	0.00
57) Fluorene-d10	15.21	176	2253228	25.54	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.33	200	323509	18.73	ng/ul	0.00
70) Anthracene-d10	17.05	188	3602475	25.45	ng/ul	0.00
78) Pyrene-d10	19.35	212	4095846	25.58	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.17	264	4584643	25.70	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	6.80	94	69694	1.596	ng/ul	91
44) Dimethylphthalate	13.67	163	1026117	10.064	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112719\
Data File : BN008779.D
Acq On : 28 Nov 2019 04:05
Operator : JU
Sample : K5889-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLLP6

Quant Time: Nov 28 05:50:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 28 01:33:10 2019
Response via : Initial Calibration

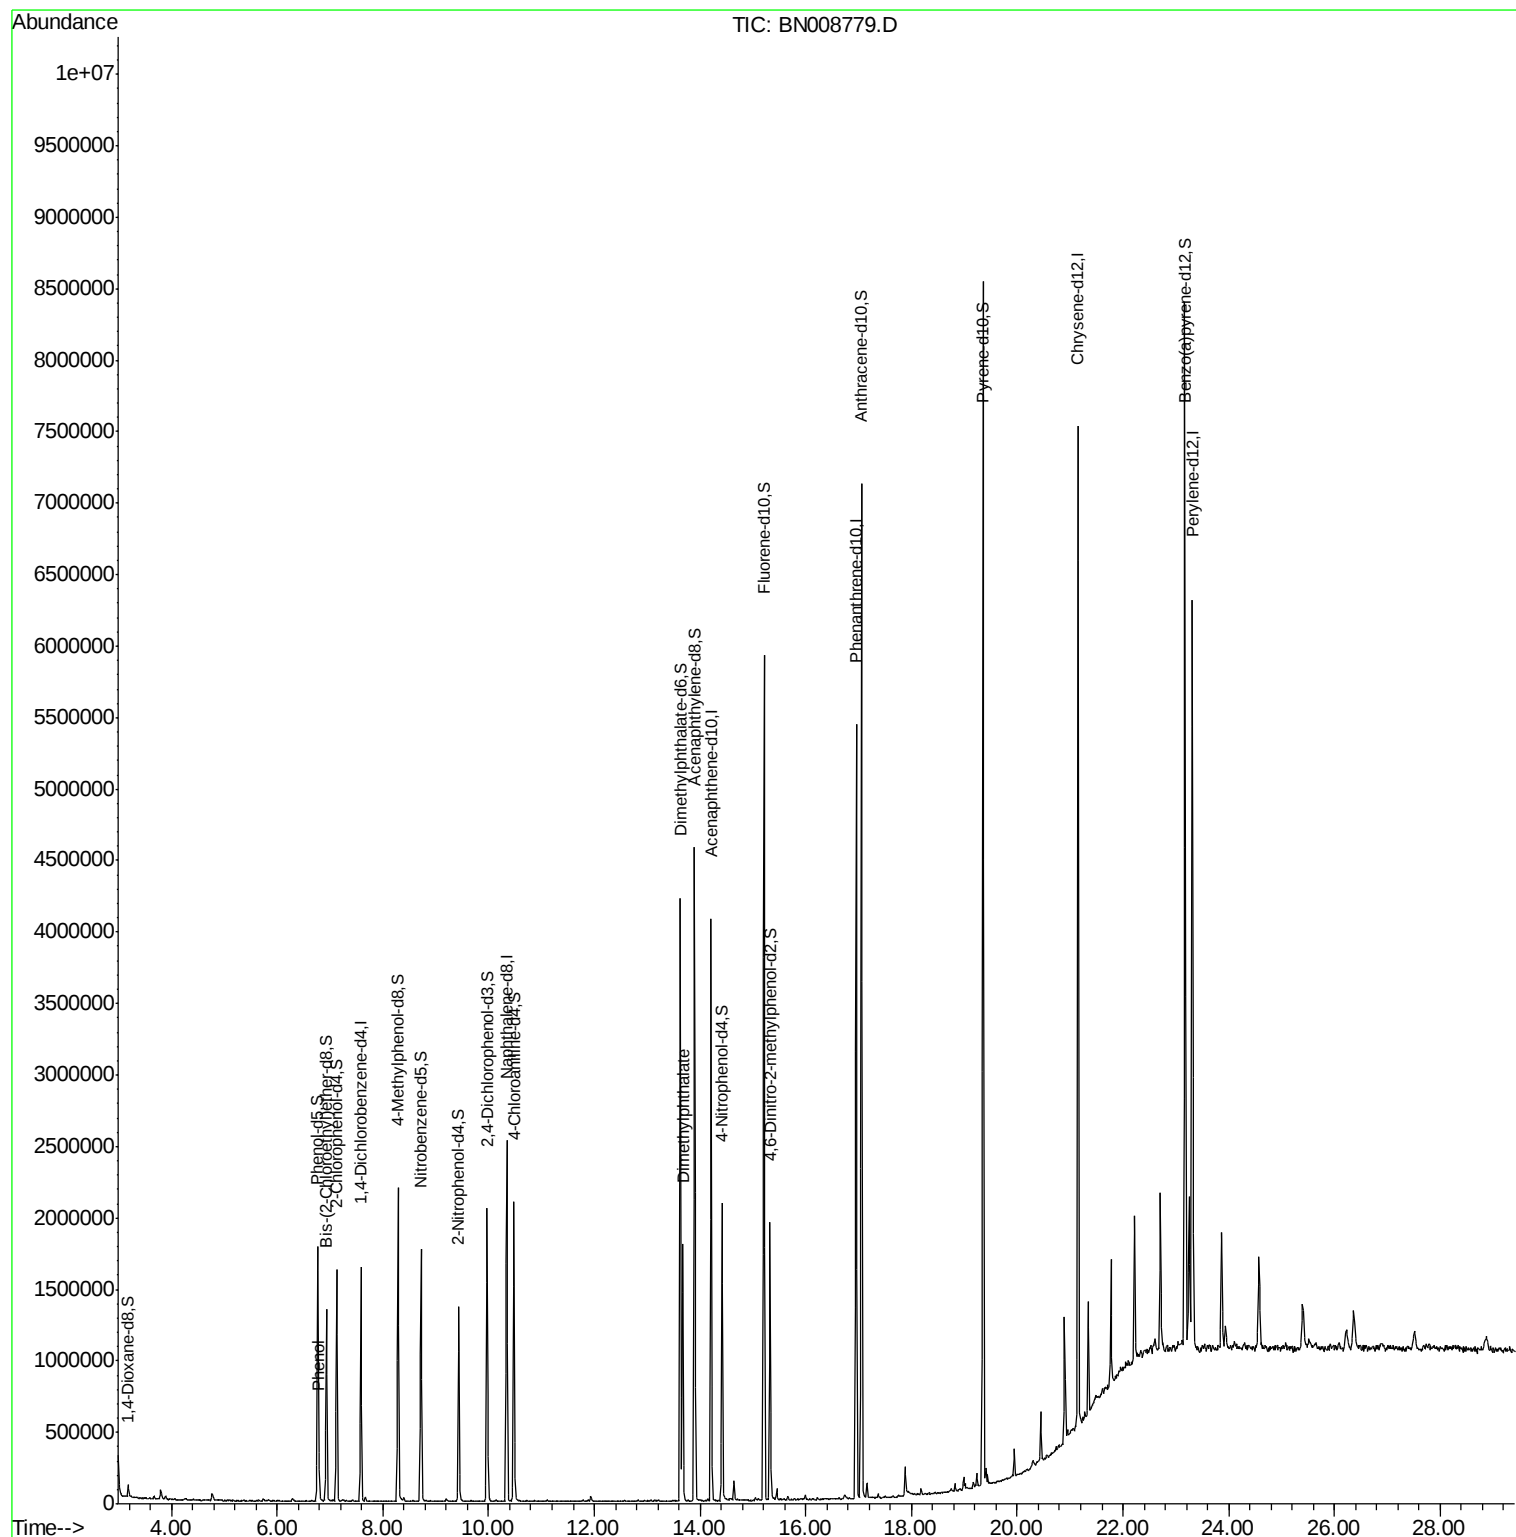

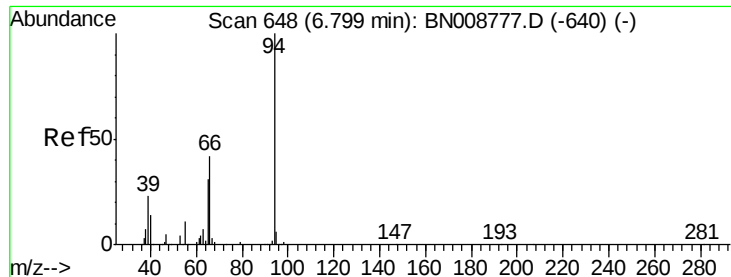

#6

Phenol

Concen: 1.596 ng/ul

RT: 6.80 min Scan# 648

Delta R.T. -0.00 min

Lab File: BN008779.D

Acq: 28 Nov 2019 04:05

Instrument :

BNA_N

ClientSampleId :

JLLP6


Tot Ion: 94 Resp: 69694

Ion Ratio Lower Upper

94 100

65 33.5 25.4 38.0

66 51.3 34.2 51.4



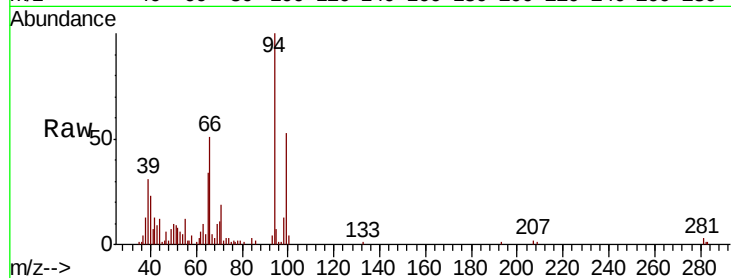


Abundance

Ion 94.00 (93.70 to 94.70): BN0

Ion 65.00 (64.70 to 65.70): BN0

Ion 66.00 (65.70 to 66.70): BN0

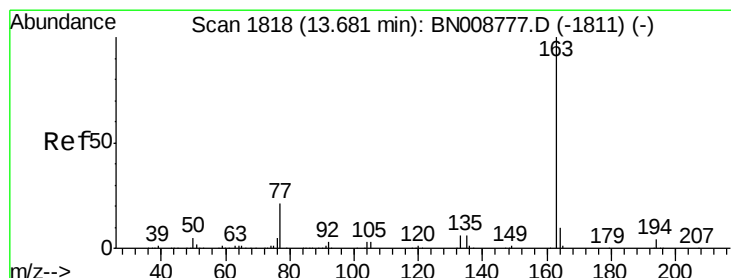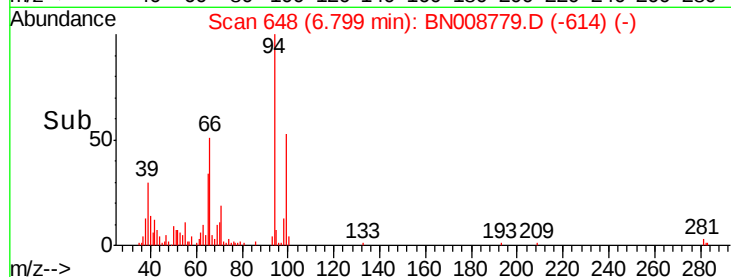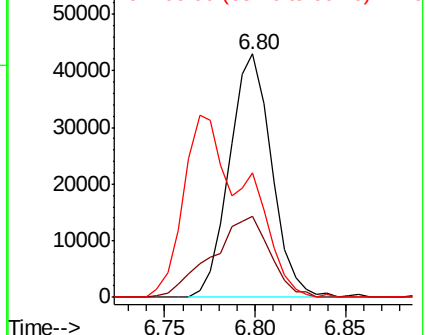

#44

Dimethylphthalate

Concen: 10.064 ng/ul

RT: 13.67 min Scan# 1817

Delta R.T. -0.01 min

Lab File: BN008779.D

Acq: 28 Nov 2019 04:05


Tgt Ion:163 Resp: 1026117

Ion Ratio Lower Upper

163 100

194 4.3 3.3 4.9

164 11.3 7.9 11.9

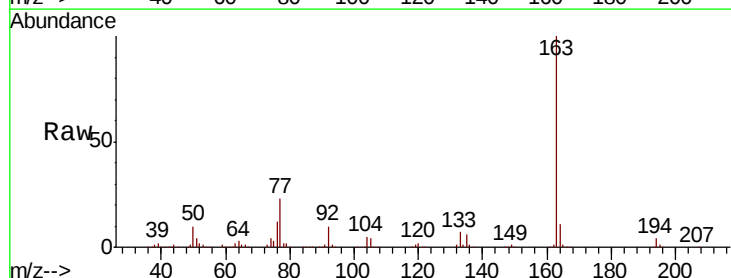

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

