

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112719\
 Data File : BN008791.D
 Acq On : 28 Nov 2019 11:13
 Operator : JU
 Sample : K5889-18
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLLS2

Quant Time: Nov 29 00:28:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 27 15:51:44 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	542001	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	2469440	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.21	164	1715782	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.95	188	3708164	20.00	ng/ul	0.00
77) Chrysene-d12	21.16	240	3517179	20.00	ng/ul	0.00
85) Perylene-d12	23.32	264	3875424	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.18	96	49567	4.00	ng/uL	0.00
5) Phenol-d5	6.77	99	1043657	18.77	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	733435	21.39	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	793179	20.45	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	826308	18.76	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	418519	21.96	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	444688	21.61	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	790823	19.30	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	1105824	21.23	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	2990234	21.87	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	3357887	22.24	ng/ul	0.00
51) 4-Nitrophenol-d4	14.42	143	449267	16.21	ng/ul	0.00
57) Fluorene-d10	15.20	176	2577762	22.32	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.33	200	365288	17.05	ng/ul	0.00
70) Anthracene-d10	17.05	188	4198006	23.91	ng/ul	0.00
78) Pyrene-d10	19.35	212	4728308	24.10	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.18	264	4808874	23.78	ng/ul	0.00
Target Compounds						
6) Phenol	6.79	94	81659	1.416	ng/ul	95
44) Dimethylphthalate	13.67	163	994249	7.449	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN112719\
Data File : BN008791.D
Acq On : 28 Nov 2019 11:13
Operator : JU
Sample : K5889-18
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLLS2

Quant Time: Nov 29 00:28:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 27 15:51:44 2019
Response via : Initial Calibration

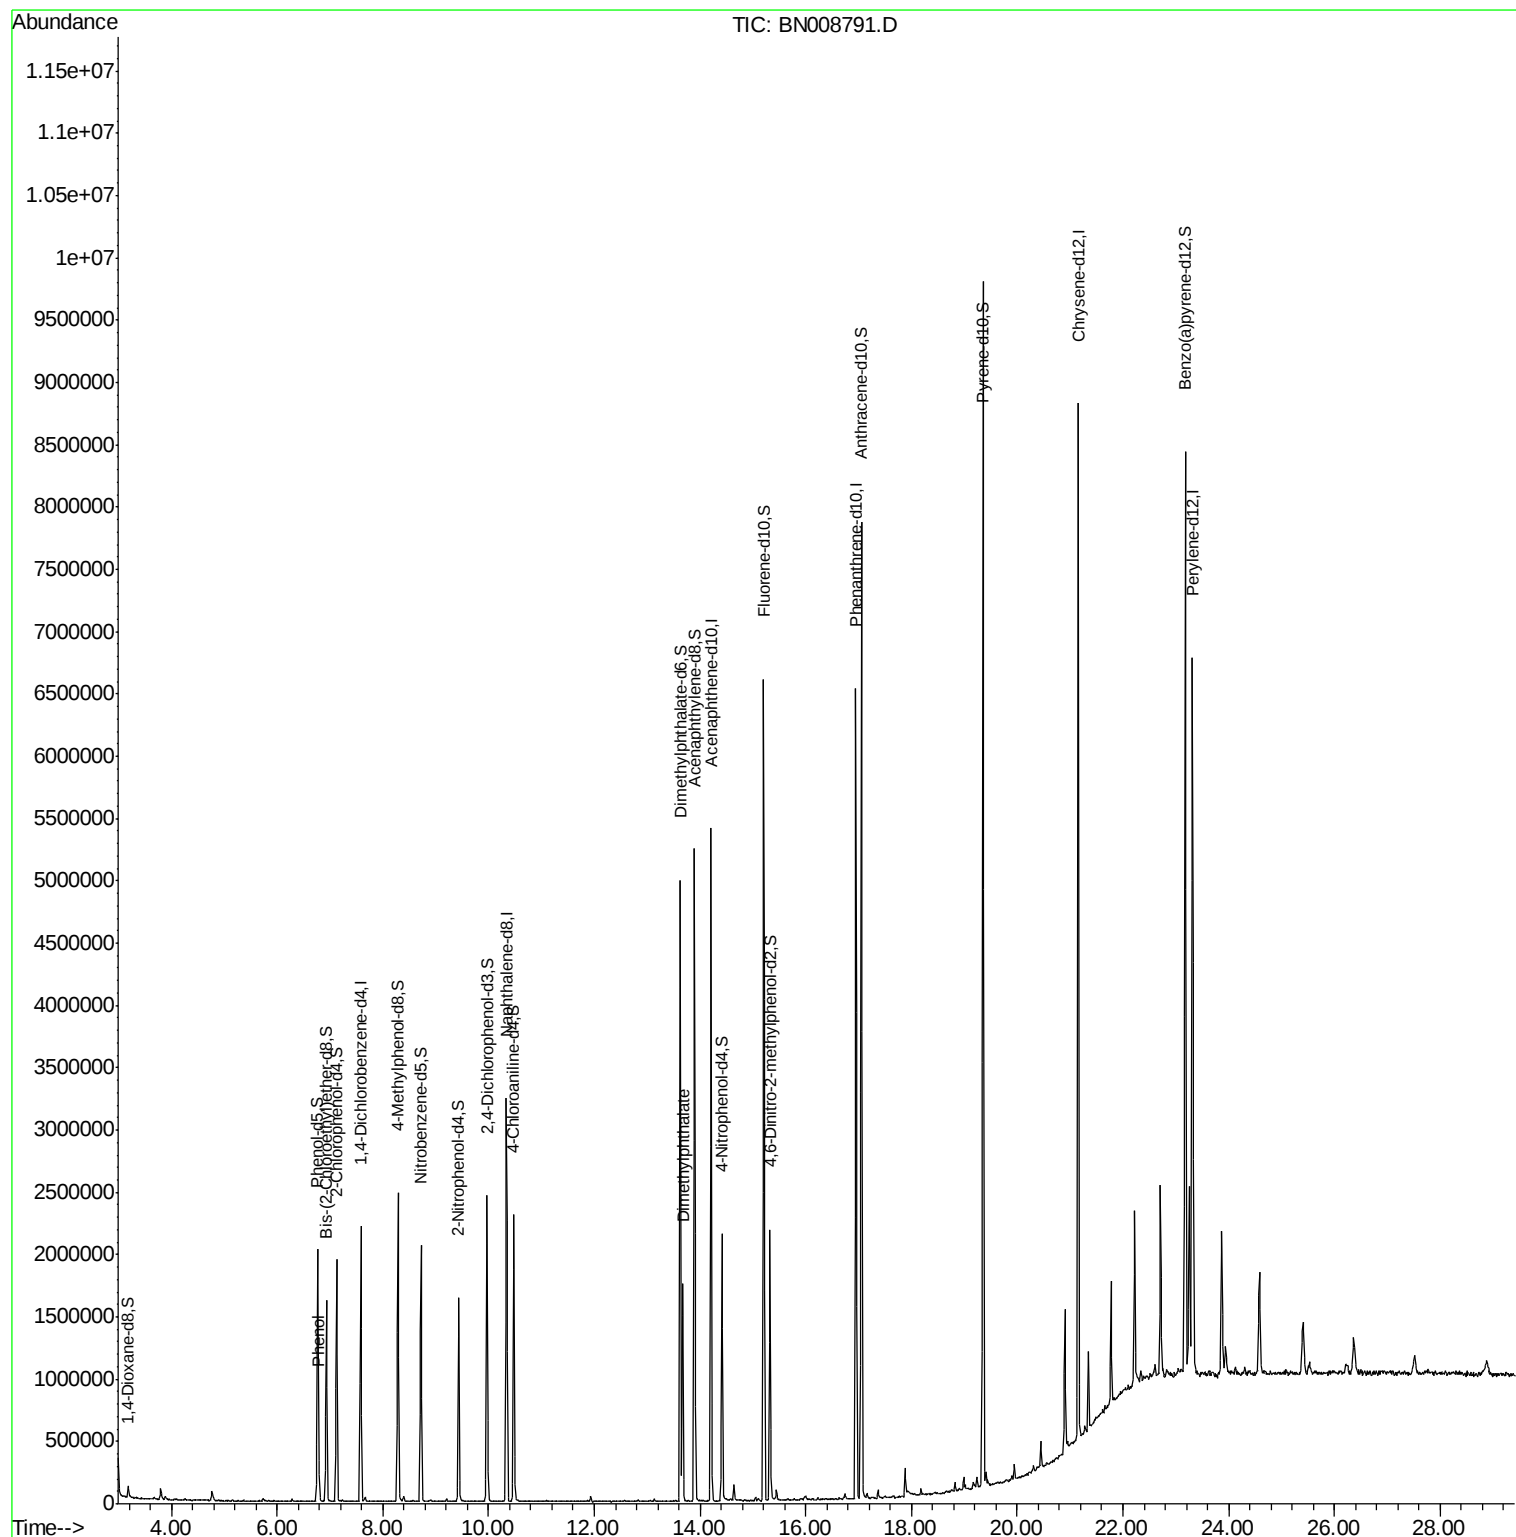

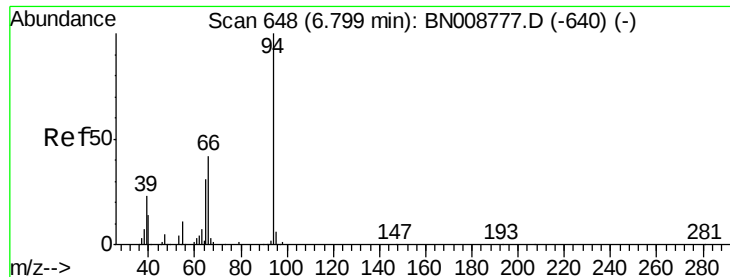





#6

Phenol

Concen: 1.416 ng/ul
 RT: 6.79 min Scan# 647
 Delta R.T. -0.01 min
 Lab File: BN008791.D
 Acq: 28 Nov 2019 11:13

Instrument :
 BNA_N
 ClientSampleId :
 JLLS2

Tot Ion: 94 Resp: 81659
 Ion Ratio Lower Upper
 94 100
 65 34.6 25.4 38.0
 66 46.4 34.2 51.4

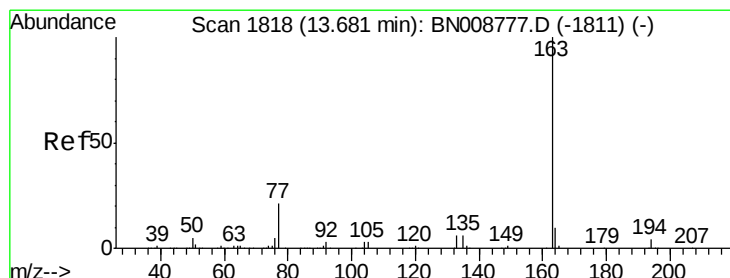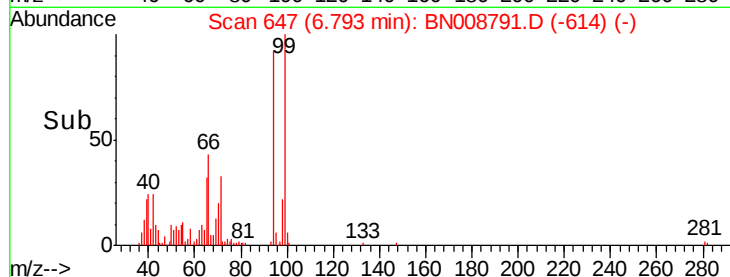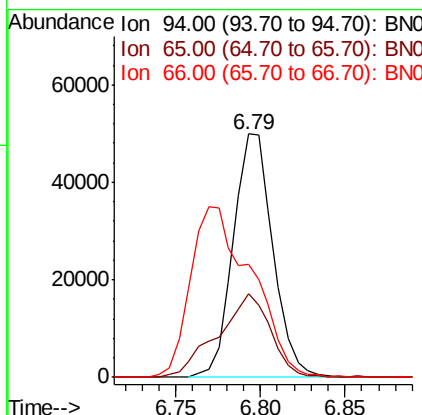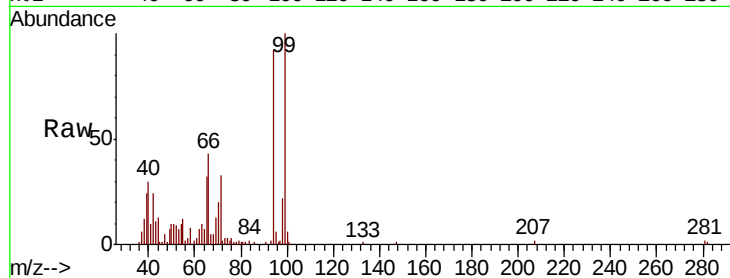

#44

Dimethylphthalate

Concen: 7.449 ng/ul
 RT: 13.67 min Scan# 1817
 Delta R.T. -0.01 min
 Lab File: BN008791.D
 Acq: 28 Nov 2019 11:13

Tgt Ion: 163 Resp: 994249
 Ion Ratio Lower Upper
 163 100
 194 4.4 3.3 4.9
 164 10.6 7.9 11.9

