

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112719\
 Data File : BN008800.D
 Acq On : 28 Nov 2019 16:34
 Operator : JU
 Sample : K5815-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A5460

Quant Time: Nov 29 00:29:35 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 27 15:51:44 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	570734	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	2522000	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.21	164	1668353	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.96	188	3573439	20.00	ng/ul	0.00
77) Chrysene-d12	21.16	240	3178459	20.00	ng/ul	0.00
85) Perylene-d12	23.32	264	3291125	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.18	96	51440	3.94	ng/uL	0.00
5) Phenol-d5	6.77	99	380961	6.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	989925	27.41	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	950574	23.28	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	702918	15.16	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	630819	32.42	ng/ul	0.00
22) 2-Nitrophenol-d4	9.44	143	713174	33.94	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	1159866	27.72	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	130459	2.45	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	4288258	32.26	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	4868246	33.15	ng/ul	0.00
51) 4-Nitrophenol-d4	14.42	143	188968	7.01	ng/ul	0.00
57) Fluorene-d10	15.21	176	3658514	32.58	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.33	200	610351	29.56	ng/ul	0.00
70) Anthracene-d10	17.06	188	5786940	34.21	ng/ul	0.00
78) Pyrene-d10	19.36	212	6296339	35.51	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.19	264	6029741	35.11	ng/ul	0.00


Target Compounds				Ovalue	
6) Phenol	6.80	94	80749	1.329	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112719\
Data File : BN008800.D
Acq On : 28 Nov 2019 16:34
Operator : JU
Sample : K5815-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5460

Quant Time: Nov 29 00:29:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 27 15:51:44 2019
Response via : Initial Calibration

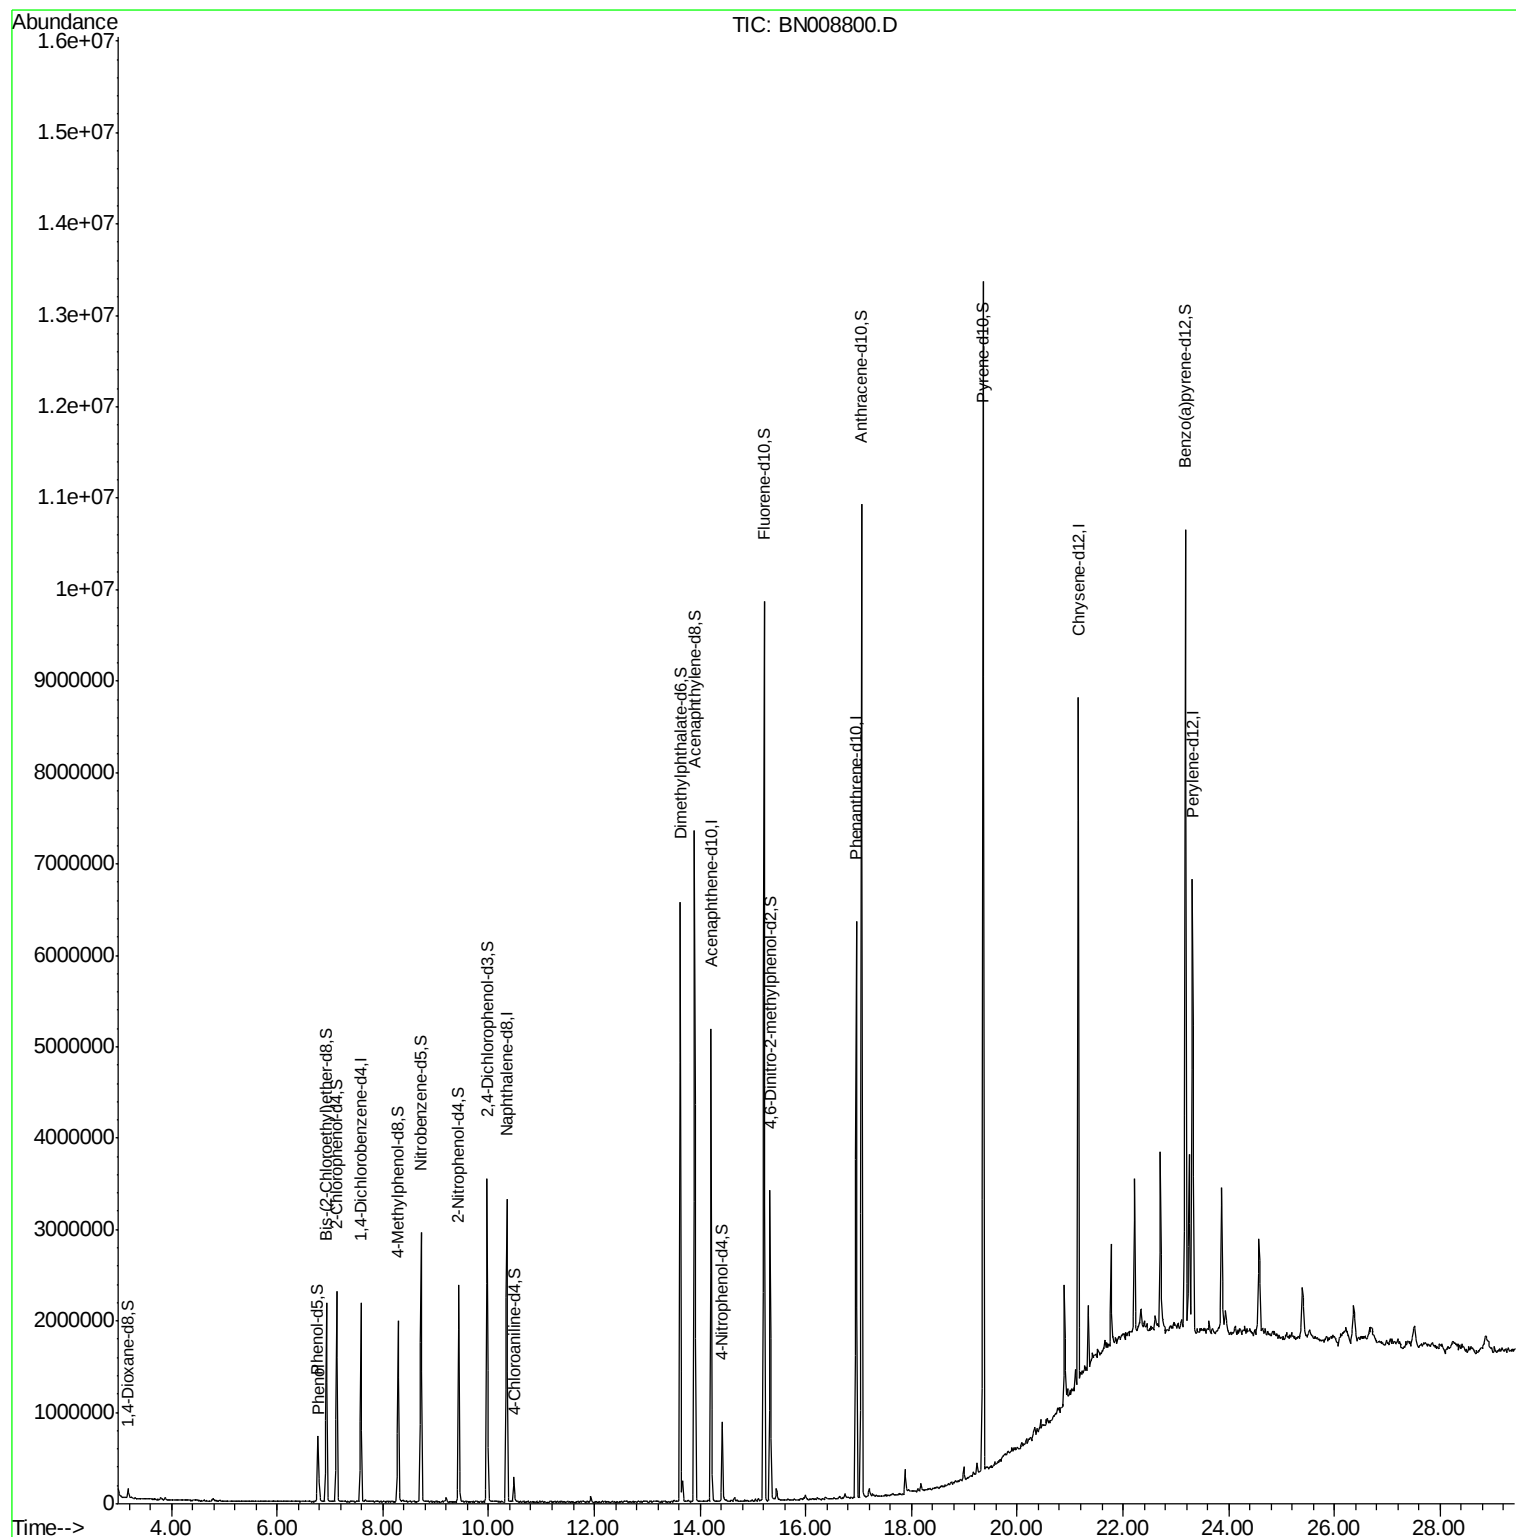

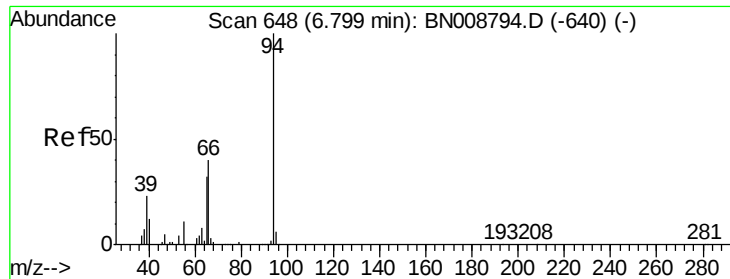

#6

Phenol

Concen: 1.329 ng/ul

RT: 6.80 min Scan# 648

Delta R.T. 0.00 min

Lab File: BN008800.D

Acq: 28 Nov 2019 16:34

Instrument :

BNA_N

ClientSampleId :

A5460

Tot Ion: 94 Resp: 80749

Ion Ratio Lower Upper

94 100

65 32.4 25.4 38.0

66 44.8 34.2 51.4

