

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN112719\
 Data File : BN008804.D
 Acq On : 28 Nov 2019 18:57
 Operator : JU
 Sample : K6086-01
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFLY8

Manual Integrations
 APPROVED

mohammad
 11/29/2019 8:54:24 AM

Quant Time: Nov 29 04:01:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 27 15:51:44 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	663596	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	3114256	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.21	164	1976930	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.96	188	4108848	20.00	ng/ul	0.00
77) Chrysene-d12	21.16	240	3473445	20.00	ng/ul	0.00
85) Perylene-d12	23.32	264	3474676	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.18	96	58303	3.84	ng/uL	0.00
5) Phenol-d5	6.77	99	384280	5.64	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	1049886	25.00	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	992346	20.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	739620	13.72	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	638929	26.59	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	719705	27.74	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	1240881	24.01	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	63780	0.97	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	4148576	26.34	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	4858164	27.92	ng/ul	0.00
51) 4-Nitrophenol-d4	14.42	143	175911	5.51	ng/ul	0.00
57) Fluorene-d10	15.21	176	3473901	26.10	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.33	200	578167	24.35	ng/ul	0.00
70) Anthracene-d10	17.05	188	5336182	27.43	ng/ul	0.00
78) Pyrene-d10	19.35	212	5709966	29.47	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.18	264	4931266	27.20	ng/ul	0.00

Target Compounds

					Ovalue
6) Phenol	6.80	94	151800	2.149 ng/ul	98
11) 2-Methylphenol	8.03	108	108863	2.075 ng/ul	96
16) 4-Methylphenol	8.36	108	159433	2.716 ng/ul	97
24) 2,4-Dimethylphenol	9.54	107	99455m	1.565 ng/ul	
28) Naphthalene	10.39	128	1056372	6.301 ng/ul	99
44) Dimethylphthalate	13.67	163	267340	1.738 ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN112719\
Data File : BN008804.D
Acq On : 28 Nov 2019 18:57
Operator : JU
Sample : K6086-01
Misc :
ALS Vial : 45 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BFLY8

Manual Integrations
APPROVED

mohammad
11/29/2019 8:54:24 AM

Quant Time: Nov 29 04:01:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 27 15:51:44 2019
Response via : Initial Calibration

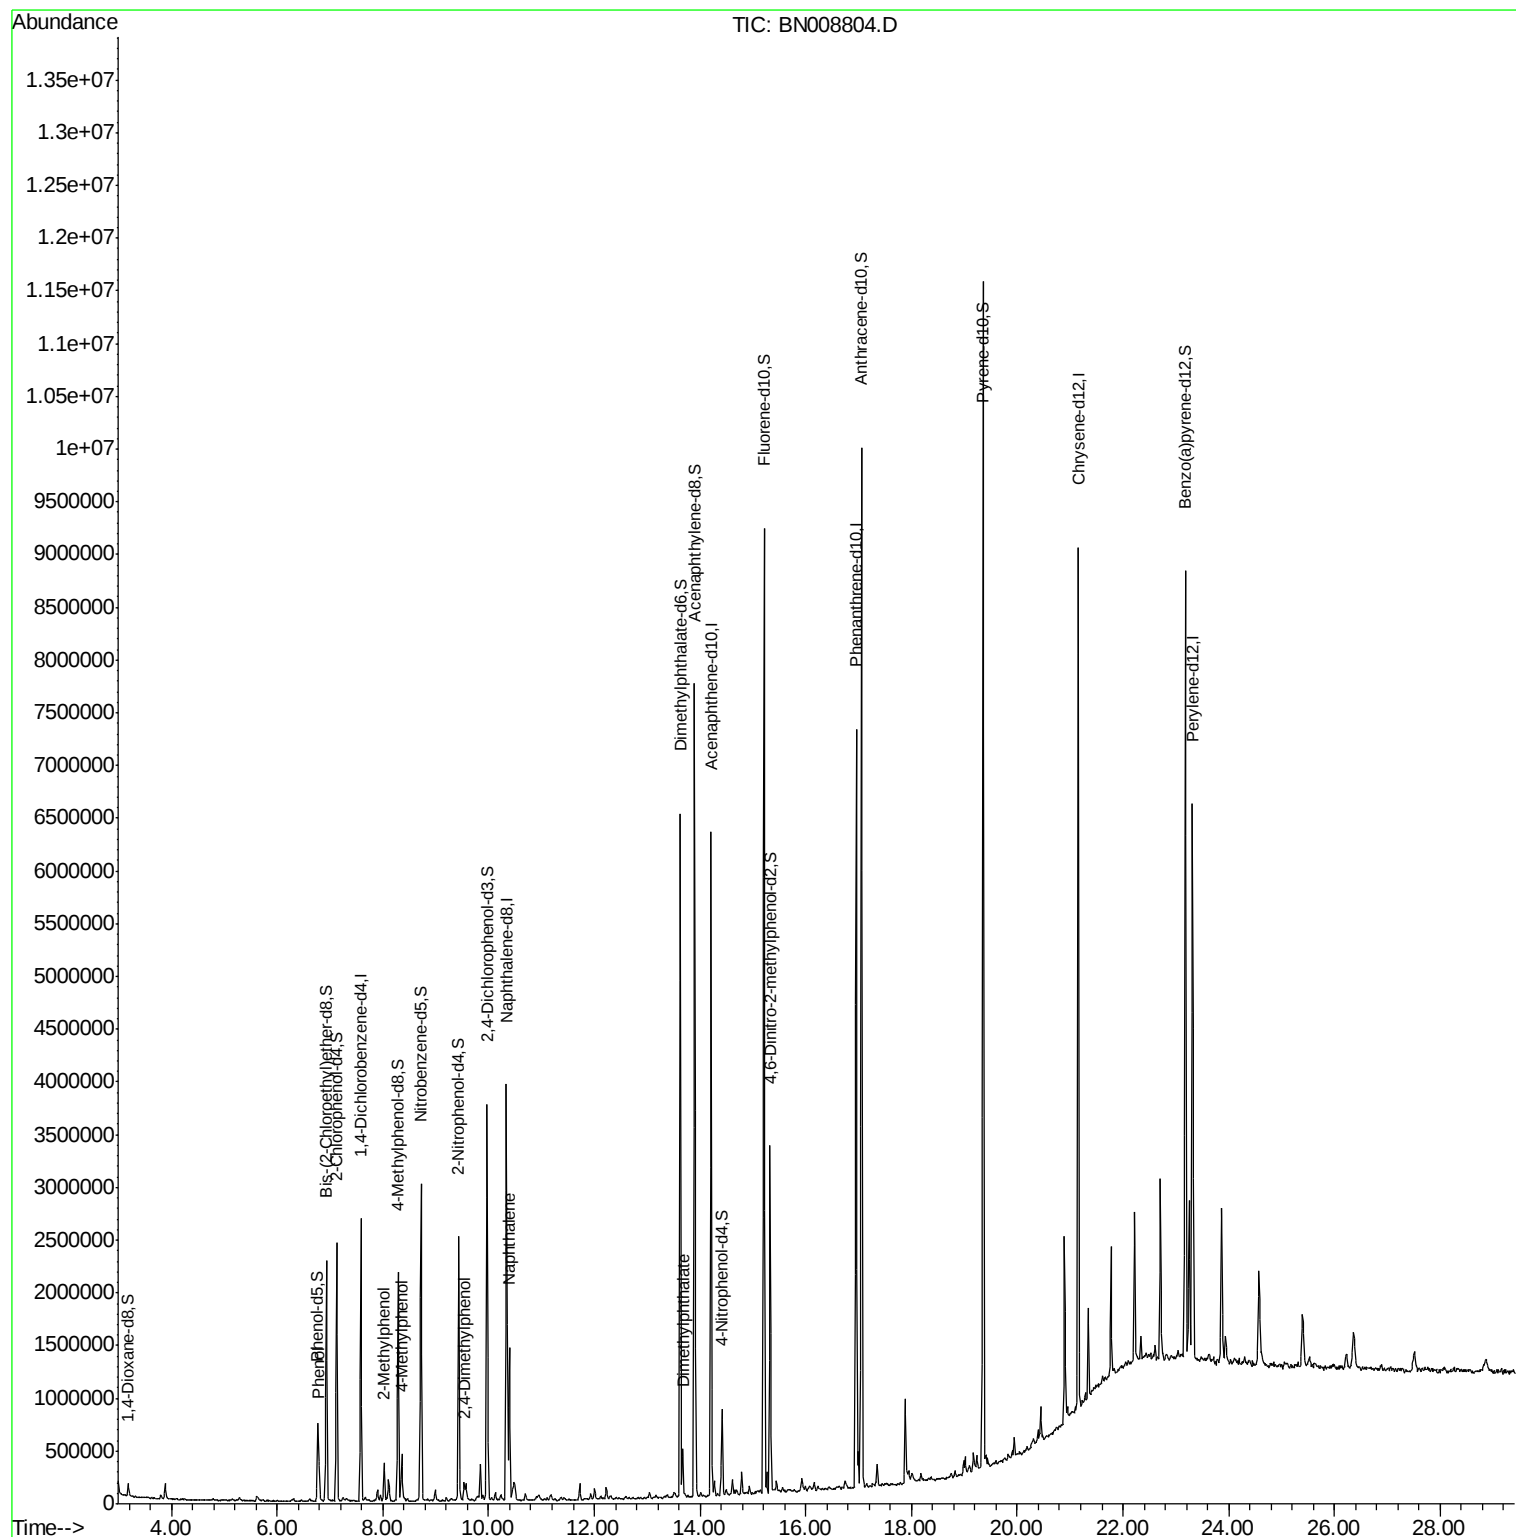

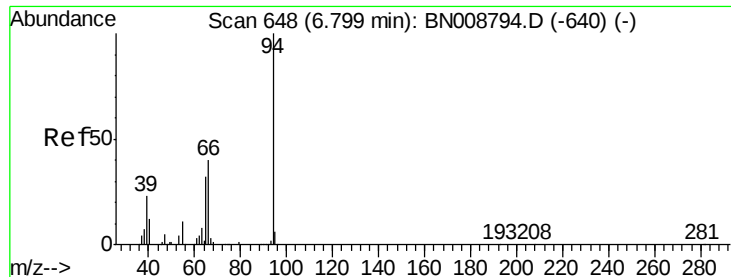

#6

Phenol

Concen: 2.149 ng/ul

RT: 6.80 min Scan# 648

Delta R.T. -0.00 min

Lab File: BN008804.D

Acq: 28 Nov 2019 18:57

Instrument :

BNA_N





ClientSampled :

BFLY8

Tot Ion:	94	Resp:	151800
Ion	Ratio	Lower	Upper
94	100		
65	31.9	25.4	38.0
66	40.9	34.2	51.4

Manual Integrations
APPROVED

mohammad
11/29/2019 8:54:24 AM

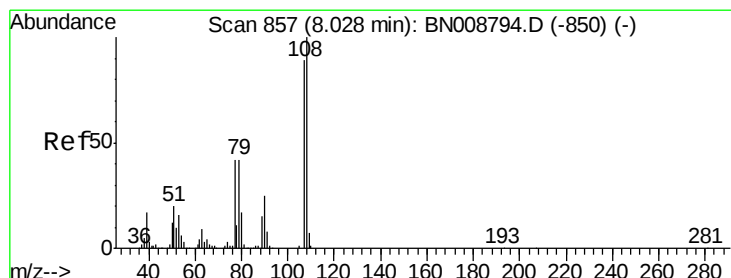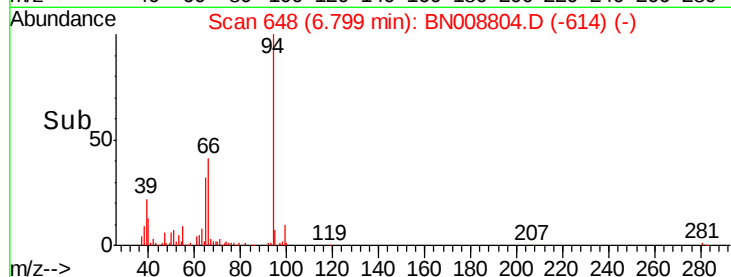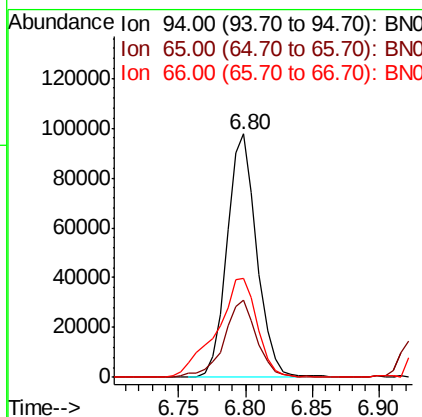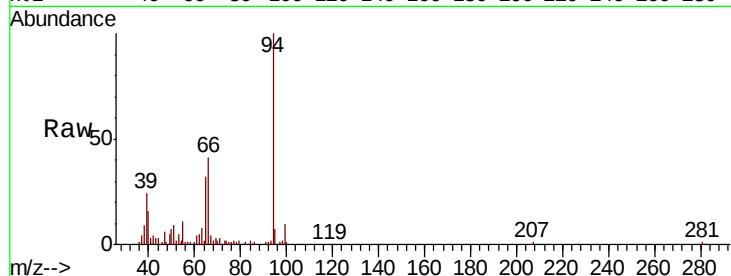

#11

2-Methylphenol

Concen: 2.075 ng/ul




RT: 8.03 min Scan# 857


Delta R.T. -0.00 min

Lab File: BN008804.D

Acq: 28 Nov 2019 18:57

Tgt Ion:	108	Resp:	108863
Ion	Ratio	Lower	Upper
108	100		
107	90.4	69.5	104.3

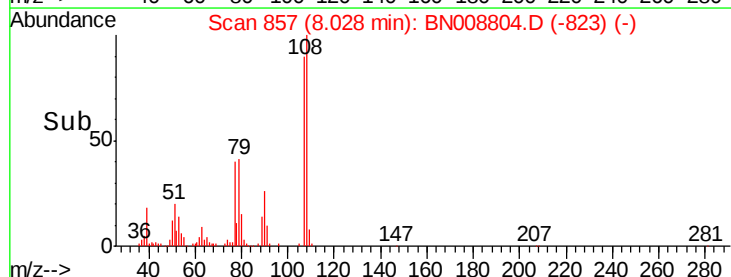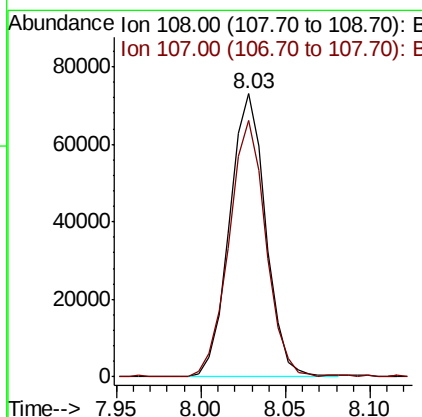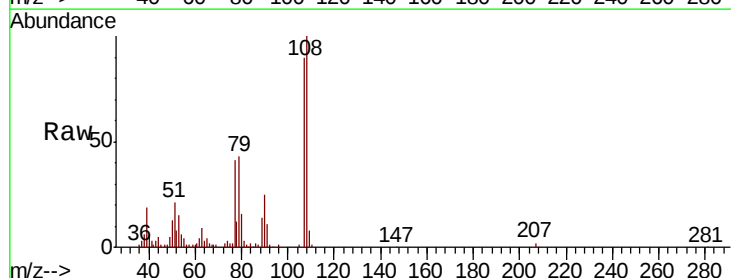

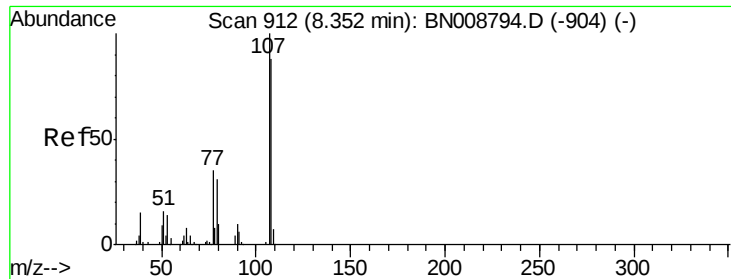





#16
4-Methylphenol
Concen: 2.716 ng/ul
RT: 8.36 min Scan# 913
Delta R.T. -0.00 min
Lab File: BN008804.D
Acq: 28 Nov 2019 18:57

Instrument :
BNA_N
ClientSampled :
BFLY8

Tot Ion	Ratio	Lower	Upper
108	100		
107	105.7	87.3	130.9




Manual Integrations
APPROVED


mohammad
11/29/2019 8:54:24 AM

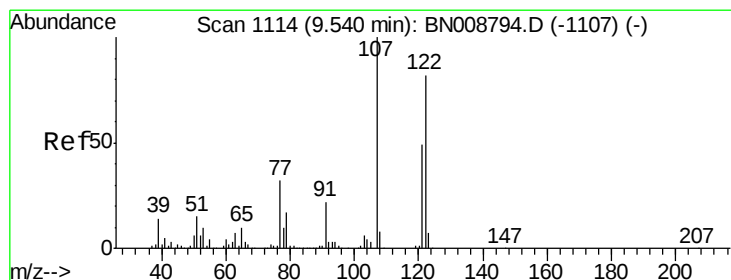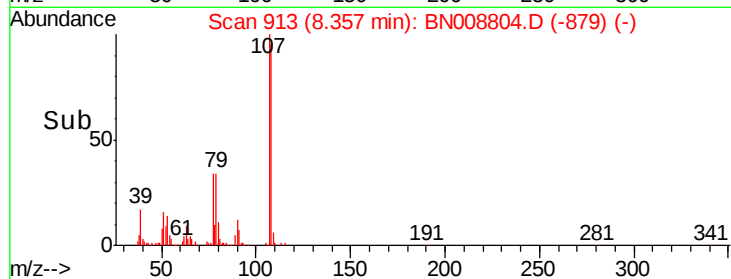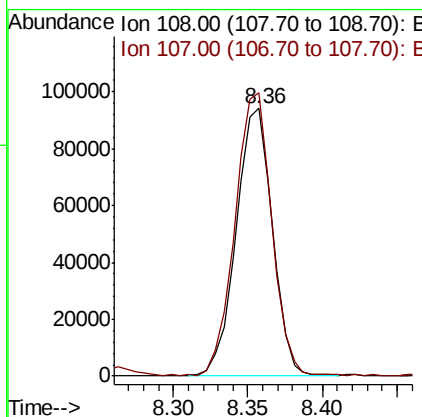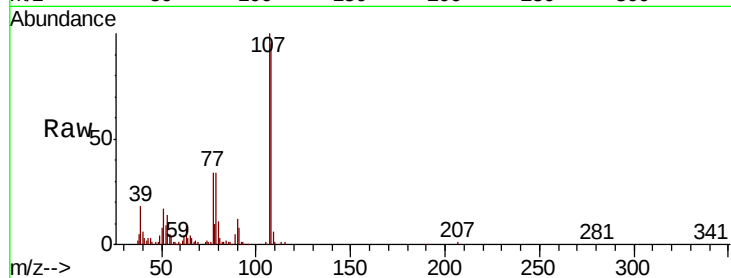

#24
2,4-Dimethylphenol
Concen: 1.565 ng/ul m
RT: 9.54 min Scan# 1114
Delta R.T. -0.01 min
Lab File: BN008804.D
Acq: 28 Nov 2019 18:57

Tgt Ion	Ratio	Lower	Upper
107	100		
121	45.2	40.2	60.4
122	82.6	67.9	101.9

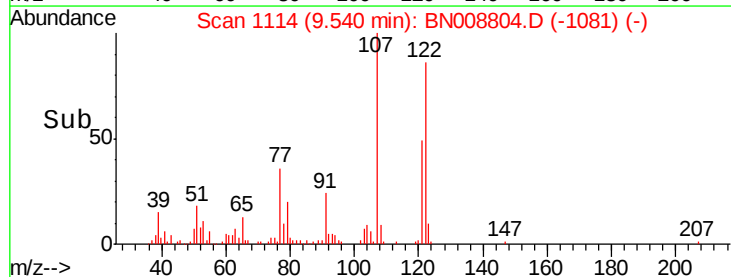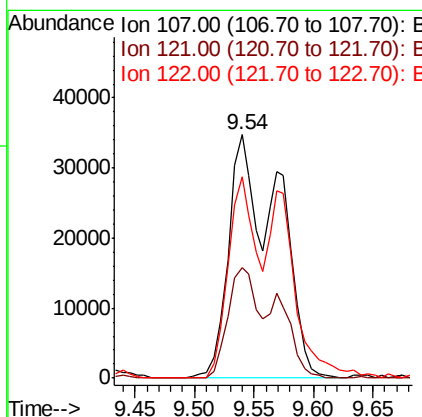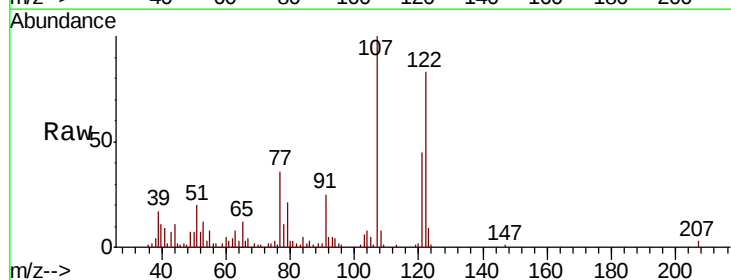

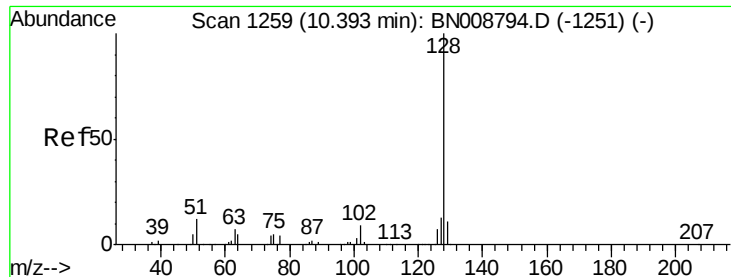





#28
Naphthalene
Concen: 6.301 ng/ul
RT: 10.39 min Scan# 1259
Delta R.T. -0.01 min
Lab File: BN008804.D
Acq: 28 Nov 2019 18:57

Instrument :
BNA_N
ClientSampleId :
BFLY8

Tot Ion	Ratio	Lower	Upper
128	100		
129	10.6	8.6	12.8
127	13.7	10.5	15.7

Manual Integrations
APPROVED

mohammad
11/29/2019 8:54:24 AM

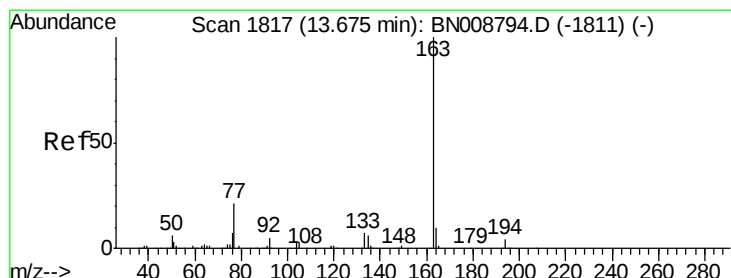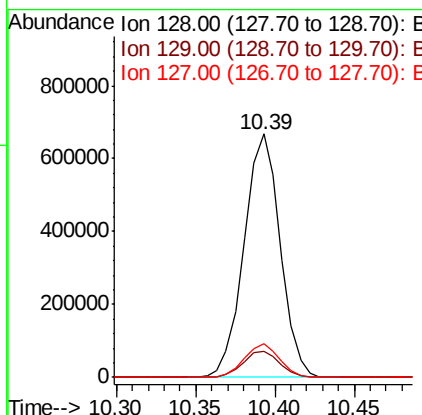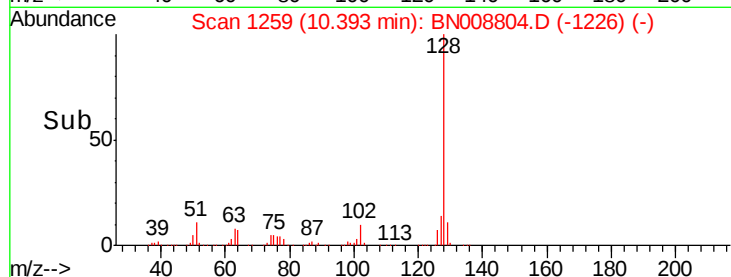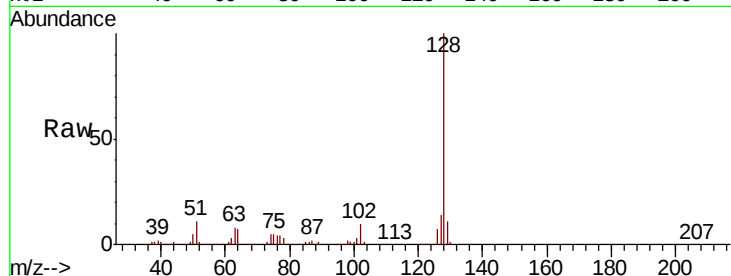

#44
Dimethylphthalate
Concen: 1.738 ng/ul
RT: 13.67 min Scan# 1817
Delta R.T. -0.01 min
Lab File: BN008804.D
Acq: 28 Nov 2019 18:57

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.3	4.9
164	10.4	7.9	11.9

