




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112723\
 Data File : BN028873.D
 Acq On : 27 Nov 2023 10:43
 Operator : MA/JU
 Sample : PB157166BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK166

Manual IntegrationsAPPROVED

Quant Time: Nov 28 03:49:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :mohammad ahmed 11/28/2023

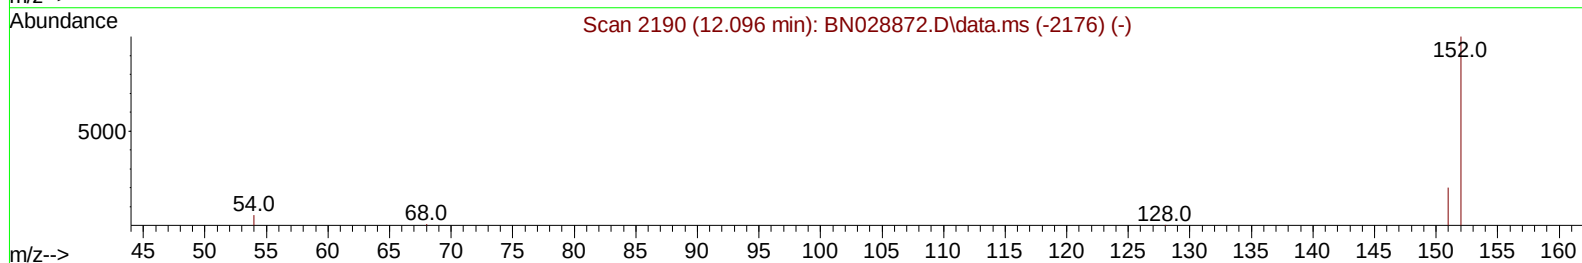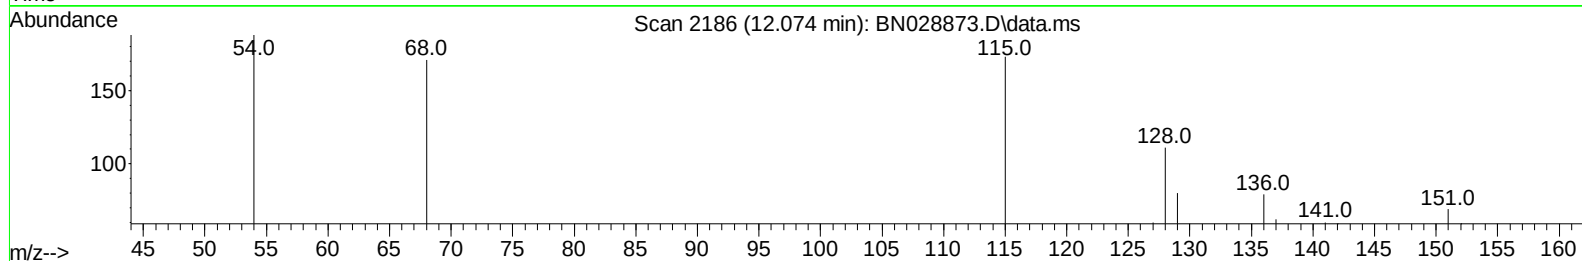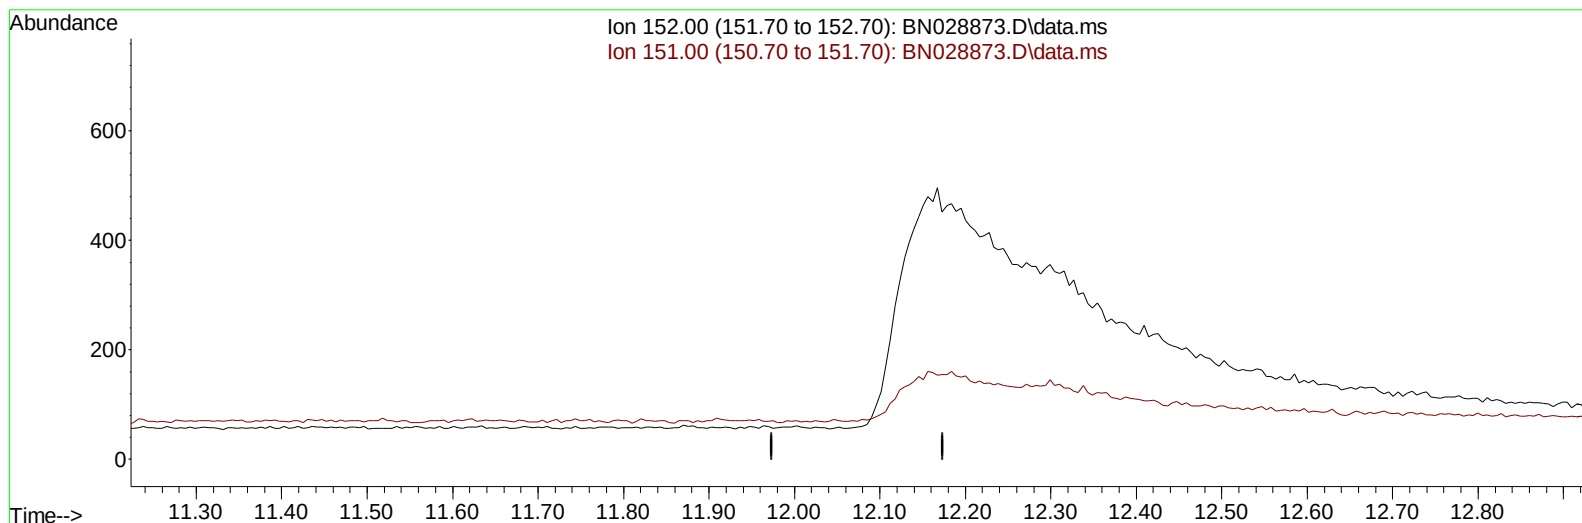

TIC: BN028873.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.074min (-12.074) 0.00 ng/u1

response 0

Ion	Exp%	Act%
152.00	100.00	0.00
151.00	20.50	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112723\
Data File : BN028873.D
Acq On : 27 Nov 2023 10:43
Operator : MA/JU
Sample : PB157166BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK166

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/28/2023
Supervised By :mohammad ahmed 11/28/2023

Quant Time: Nov 28 03:49:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

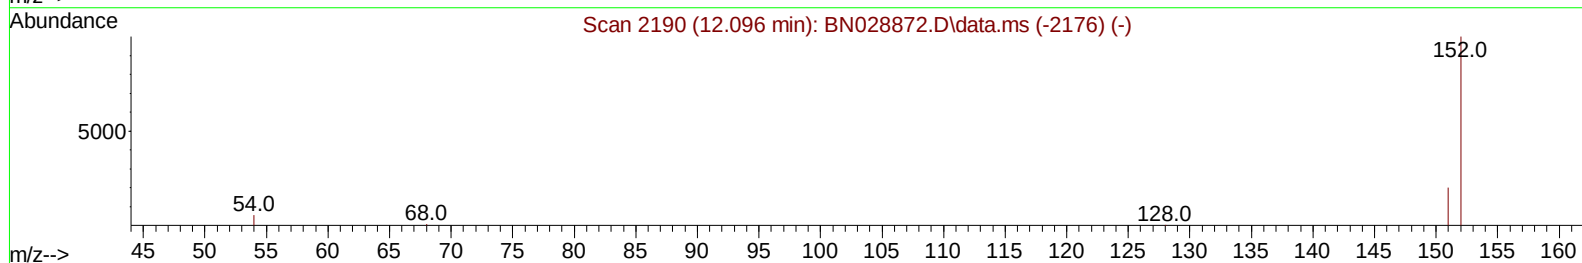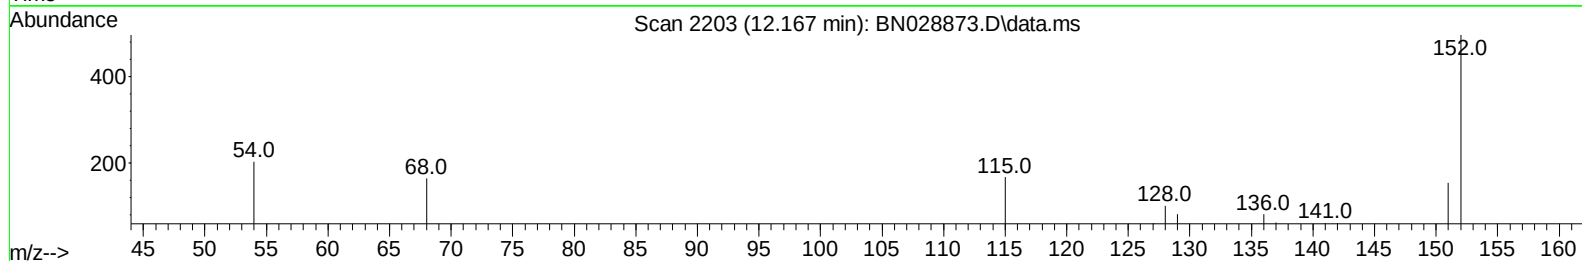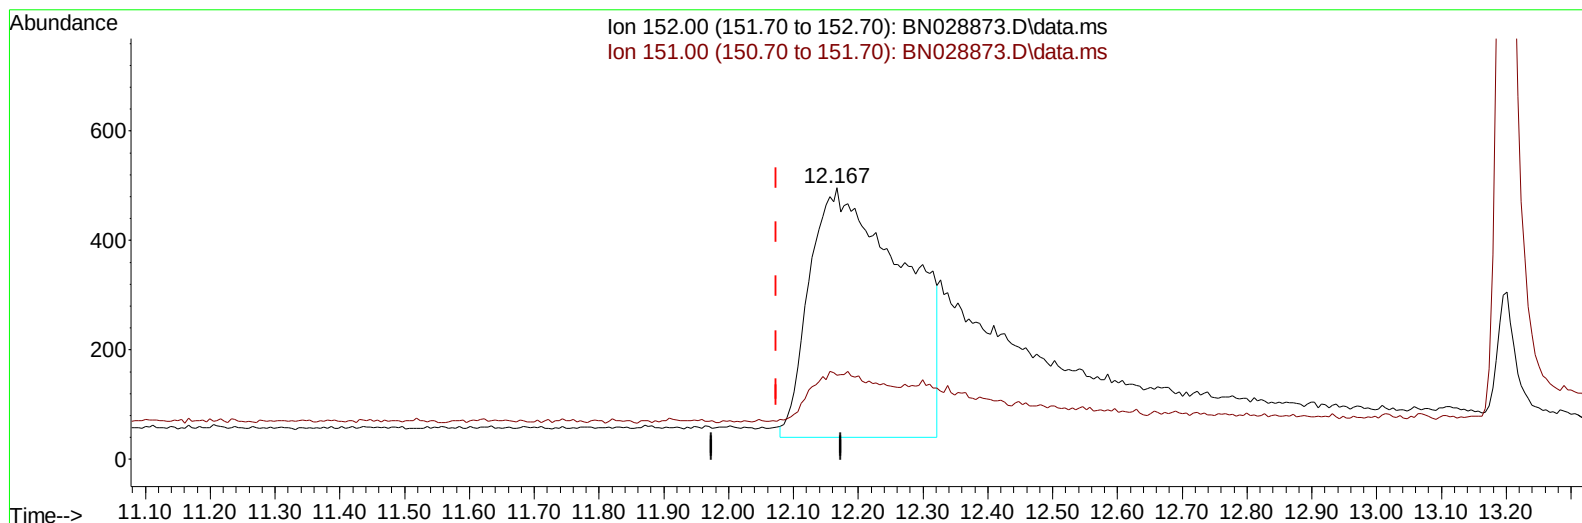

TIC: BN028873.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.167min (+ 0.094) 0.20 ng/ul m

response 4613

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112723\
 Data File : BN028873.D
 Acq On : 27 Nov 2023 10:43
 Operator : MA/JU
 Sample : PB157166BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK166

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :mohammad ahmed 11/28/2023

Quant Time: Nov 28 03:49:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.728	152	4974	0.400	ng/ul	# 0.00
4) Naphthalene-d8	10.451	136	15424	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.297	164	10606	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.073	188	17610	0.400	ng/ul	# 0.01
17) Chrysene-d12	21.307	240	8844	0.400	ng/ul	# 0.04
23) Perylene-d12	23.554	264	13638	0.400	ng/ul	# 0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.099	96	40120	7.298	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.167	152	4613m	0.199	ng/ul	0.09
18) Fluoranthene-d10	19.103	212	9556	0.336	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112723\
Data File : BN028873.D
Acq On : 27 Nov 2023 10:43
Operator : MA/JU
Sample : PB157166BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK166

Manual IntegrationsAPPROVED

Quant Time: Nov 28 03:49:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/28/2023
Supervised By :mohammad ahmed 11/28/2023

