




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112723\
Data File : BN028888.D
Acq On : 27 Nov 2023 20:47
Operator : MA/JU
Sample : PB157288BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK288

Manual IntegrationsAPPROVED

Quant Time: Nov 28 04:30:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/28/2023
Supervised By :mohammad ahmed 11/28/2023

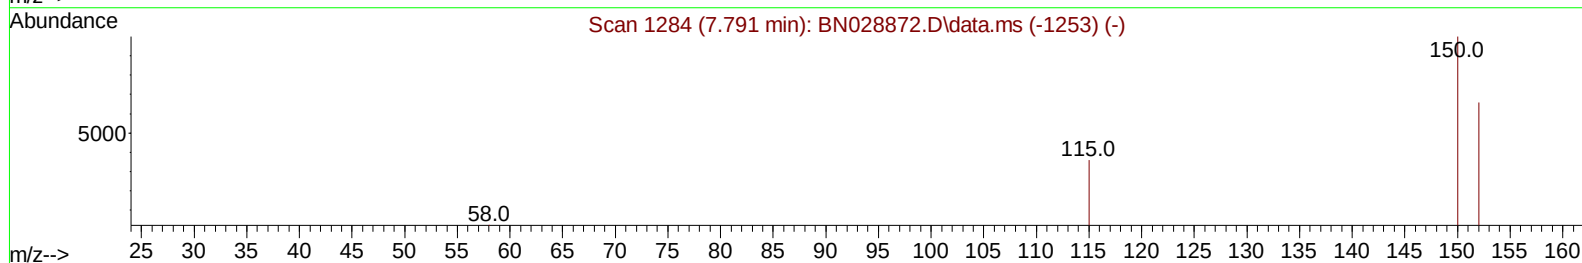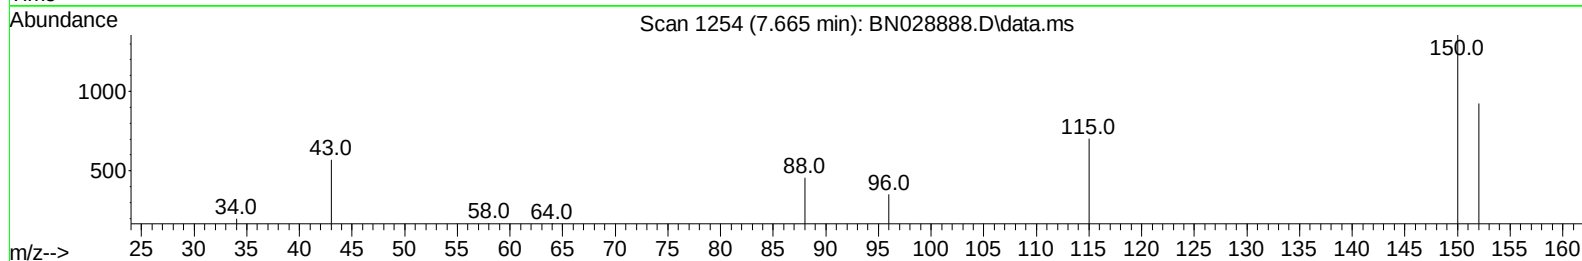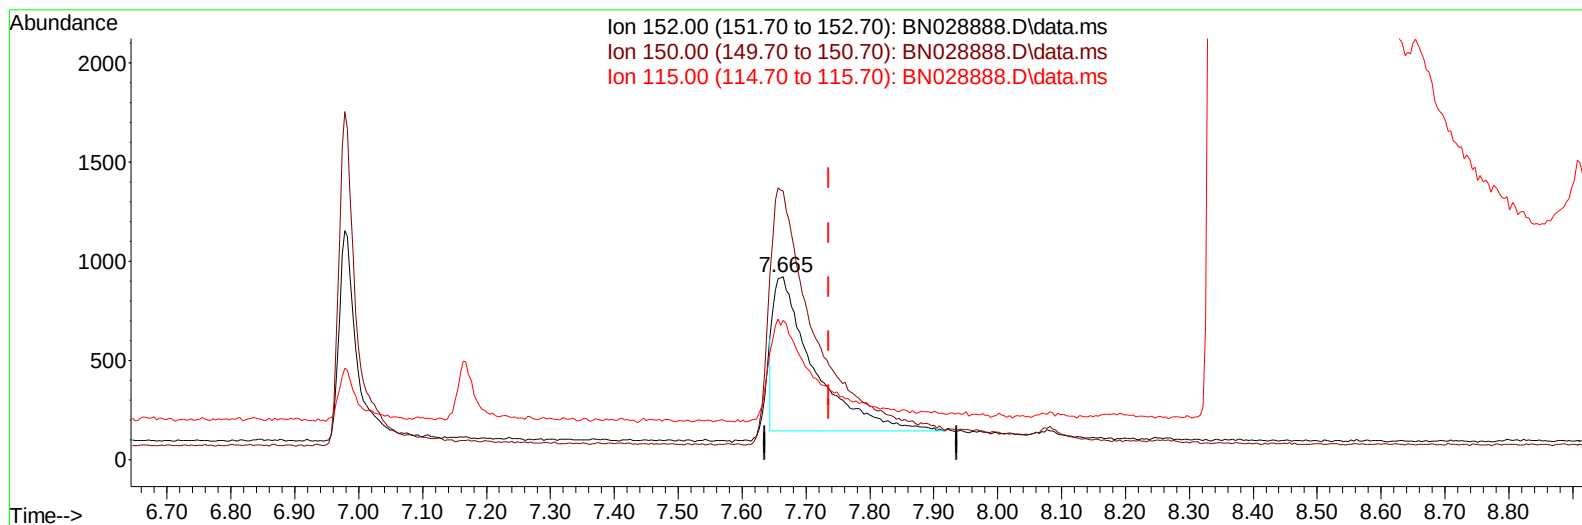

TIC: BN028888.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.665min (-0.071) 0.40 ng/ul

response 3406

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	146.96
115.00	62.20	76.25#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112723\
Data File : BN028888.D
Acq On : 27 Nov 2023 20:47
Operator : MA/JU
Sample : PB157288BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK288

Manual IntegrationsAPPROVED

Quant Time: Nov 28 04:30:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/28/2023
Supervised By :mohammad ahmed 11/28/2023

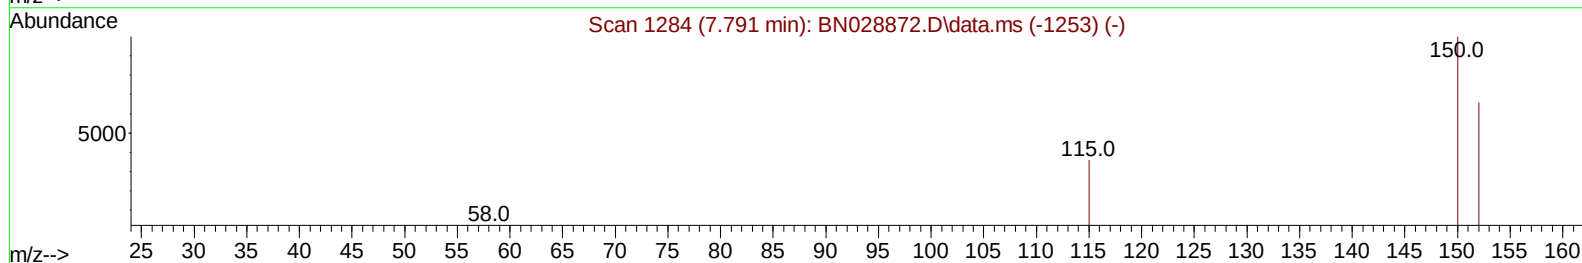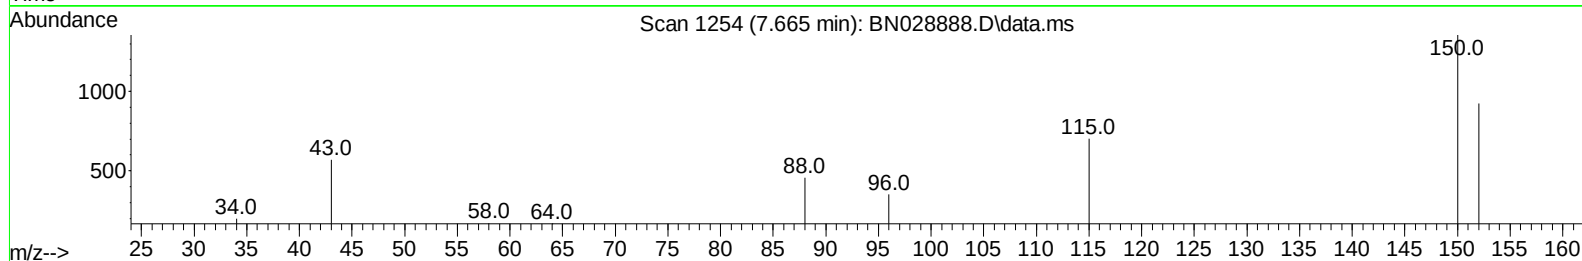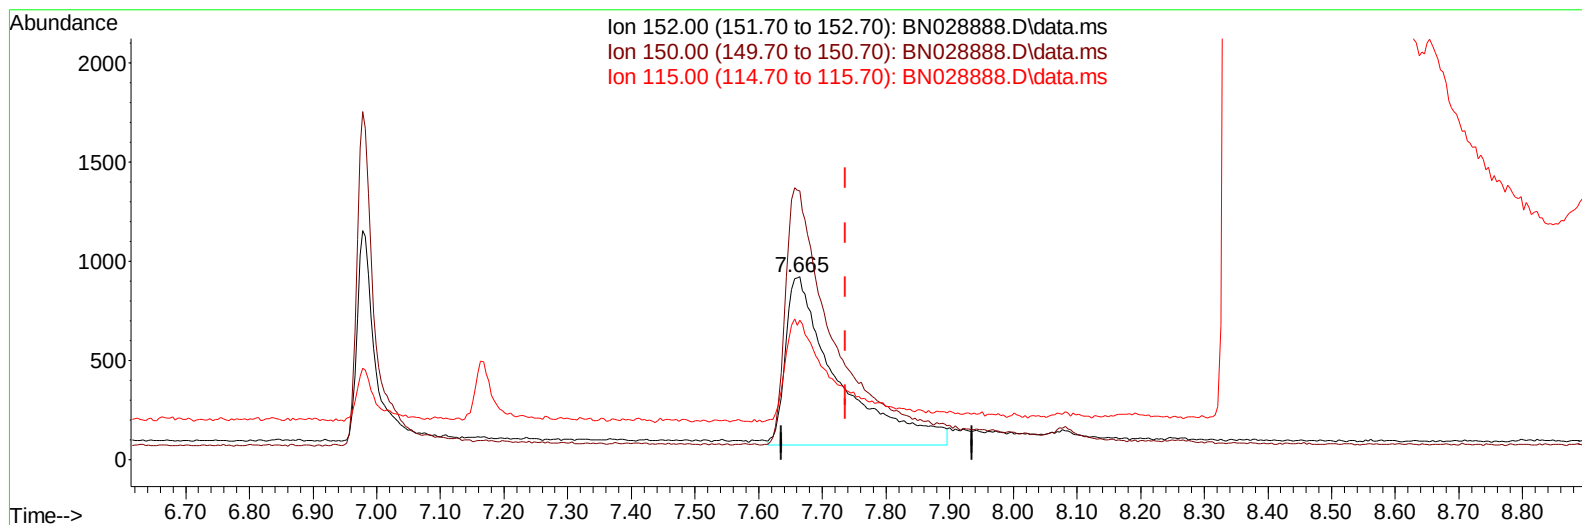

TIC: BN028888.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.665min (-0.071) 0.40 ng/ul m

response 4827

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	146.96
115.00	62.20	76.25#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112723\
 Data File : BN028888.D
 Acq On : 27 Nov 2023 20:47
 Operator : MA/JU
 Sample : PB157288BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK288

Manual IntegrationsAPPROVED

Quant Time: Nov 28 04:30:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :mohammad ahmed 11/28/2023

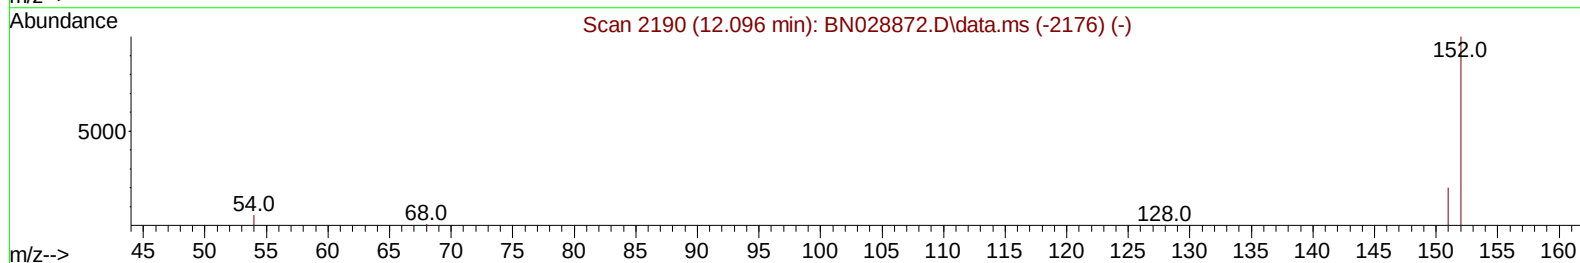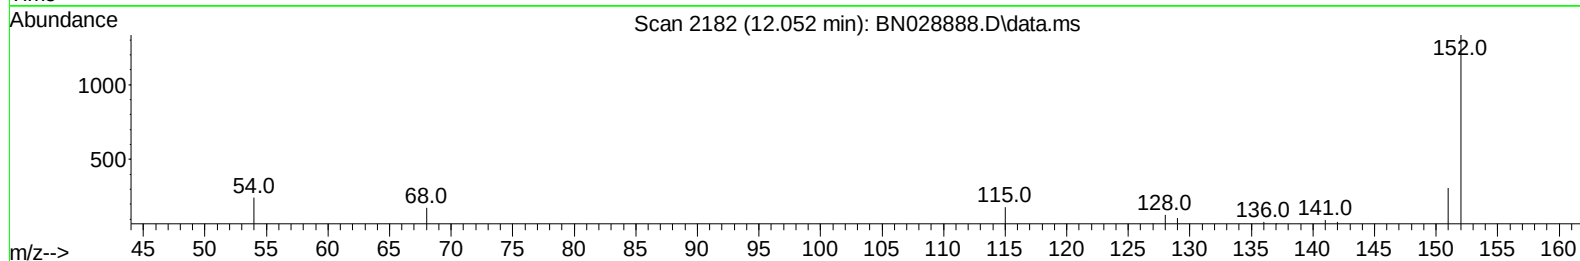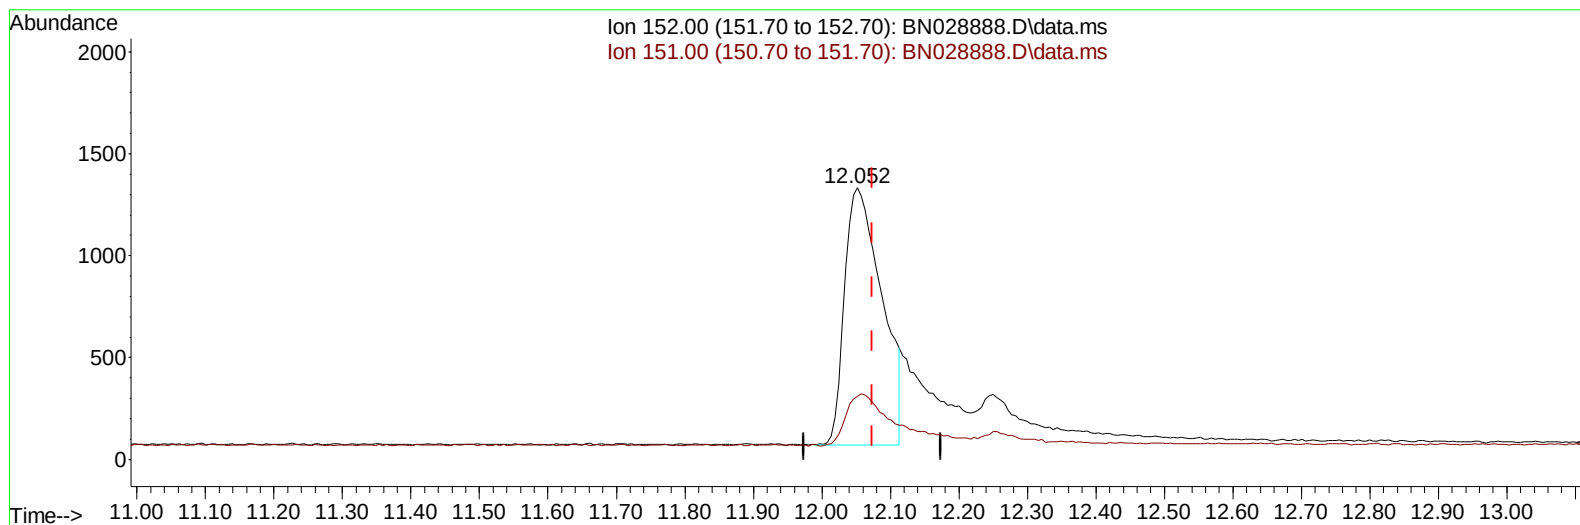

TIC: BN028888.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.052min (-0.022) 0.21 ng/u1

response 4751

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	20.71
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112723\
 Data File : BN028888.D
 Acq On : 27 Nov 2023 20:47
 Operator : MA/JU
 Sample : PB157288BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK288

Manual IntegrationsAPPROVED

Quant Time: Nov 28 04:30:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :mohammad ahmed 11/28/2023

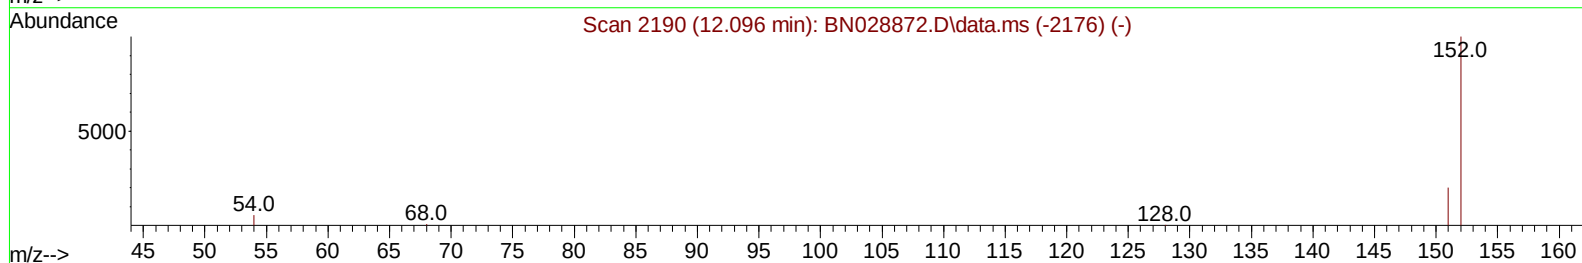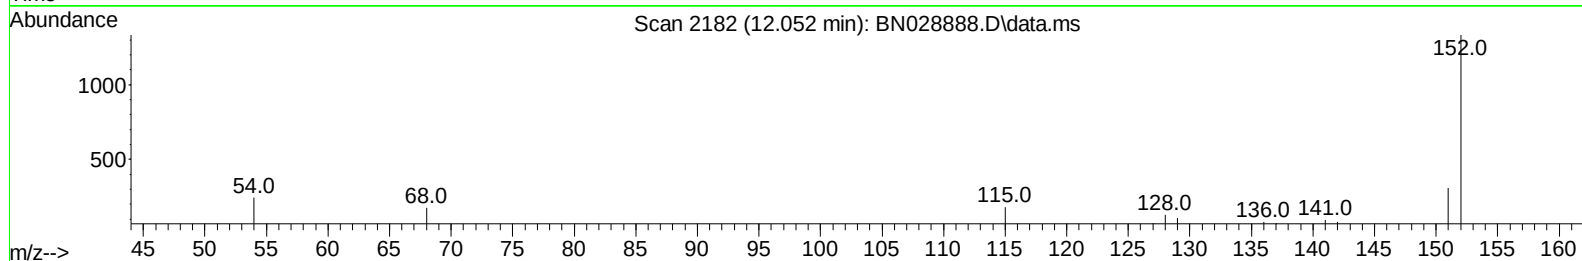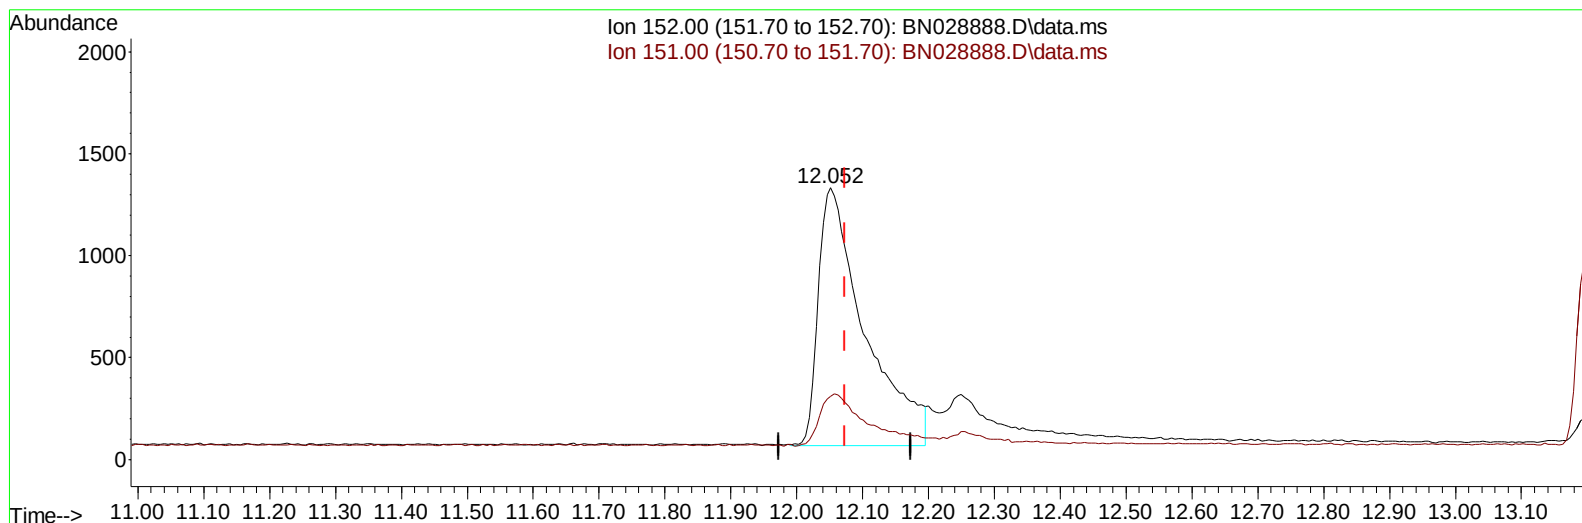

TIC: BN028888.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.052min (-0.022) 0.27 ng/ul m

response 6186

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	15.91#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112723\
 Data File : BN028888.D
 Acq On : 27 Nov 2023 20:47
 Operator : MA/JU
 Sample : PB157288BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK288

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :mohammad ahmed 11/28/2023

Quant Time: Nov 28 04:30:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.665	152	4827m	0.400	ng/ul	-0.07
4) Naphthalene-d8	10.429	136	15180	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.289	164	7463	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	17.048	188	12211	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.268	240	9417	0.400	ng/ul	# 0.00
23) Perylene-d12	23.533	264	13328	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.099	96	38192	7.159	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.052	152	6186m	0.271	ng/ul	-0.02
18) Fluoranthene-d10	19.086	212	10907	0.360	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112723\
Data File : BN028888.D
Acq On : 27 Nov 2023 20:47
Operator : MA/JU
Sample : PB157288BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK288

Manual IntegrationsAPPROVED

Quant Time: Nov 28 04:30:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/28/2023
Supervised By :mohammad ahmed 11/28/2023

