




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112823\
Data File : BN028908.D
Acq On : 28 Nov 2023 17:37
Operator : MA/JU
Sample : SSTDCCC0.4EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTDCCC0.4EC

Manual IntegrationsAPPROVED

Quant Time: Nov 28 18:17:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/29/2023
Supervised By :mohammad ahmed 11/29/2023

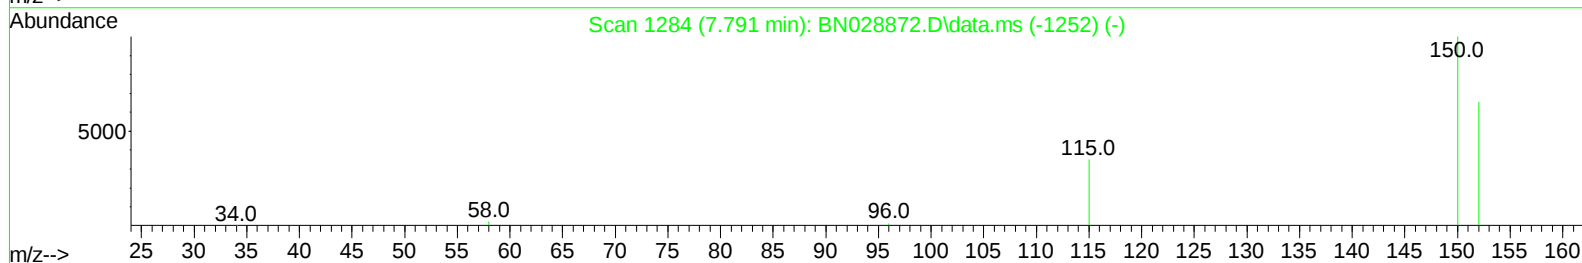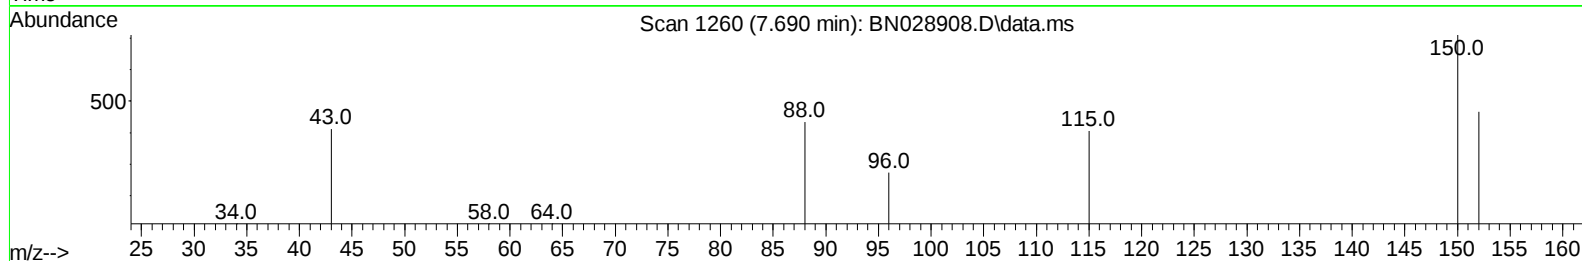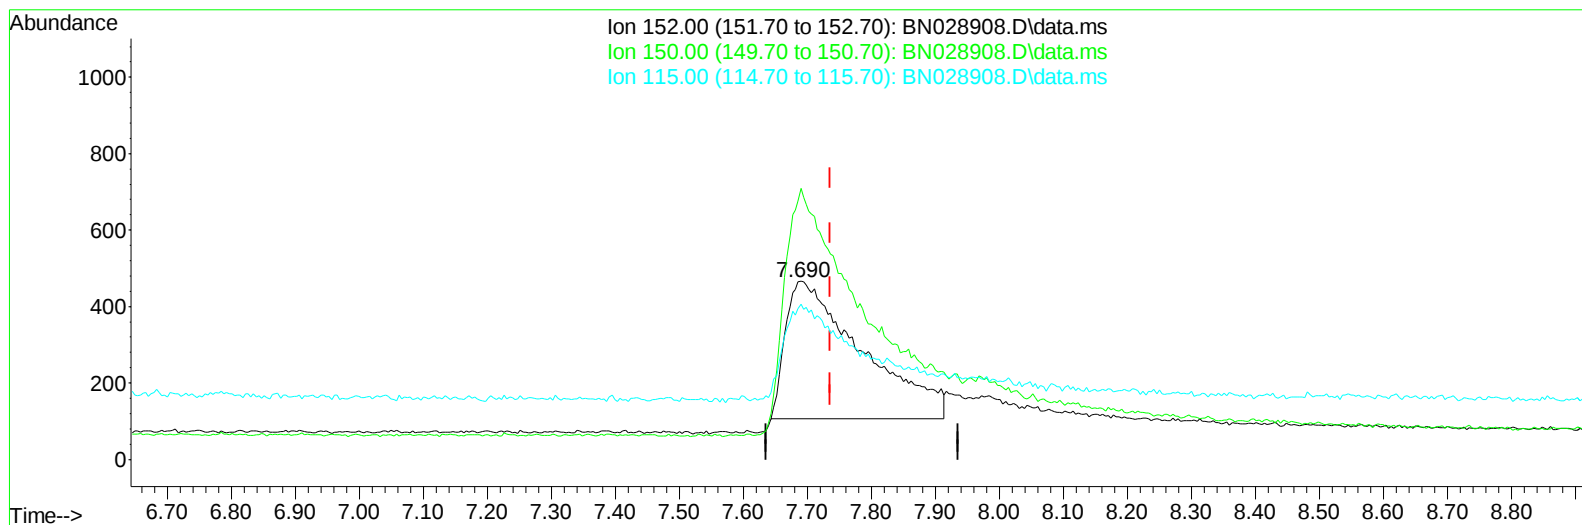

TIC: BN028908.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.690min (-0.046) 0.40 ng/u1

response 2998

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	152.36
115.00	62.20	87.12#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112823\
Data File : BN028908.D
Acq On : 28 Nov 2023 17:37
Operator : MA/JU
Sample : SSTDCCC0.4EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTDCCC0.4EC

Manual IntegrationsAPPROVED

Quant Time: Nov 28 18:17:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/29/2023
Supervised By :mohammad ahmed 11/29/2023

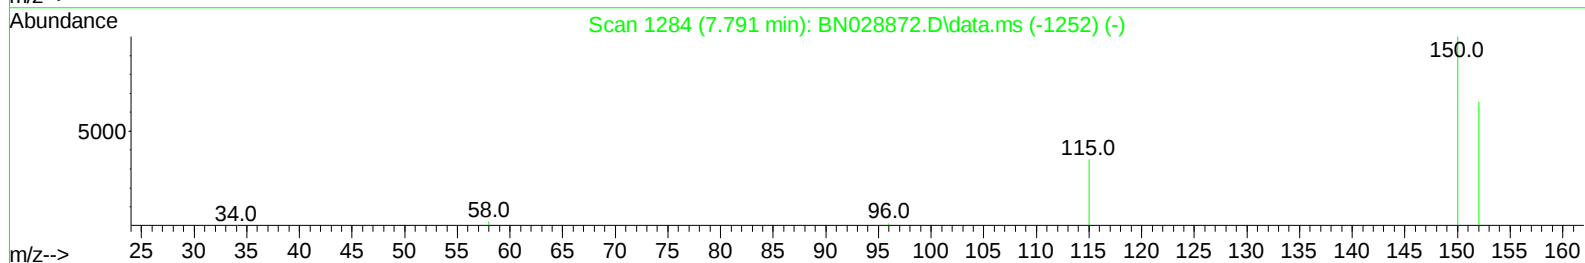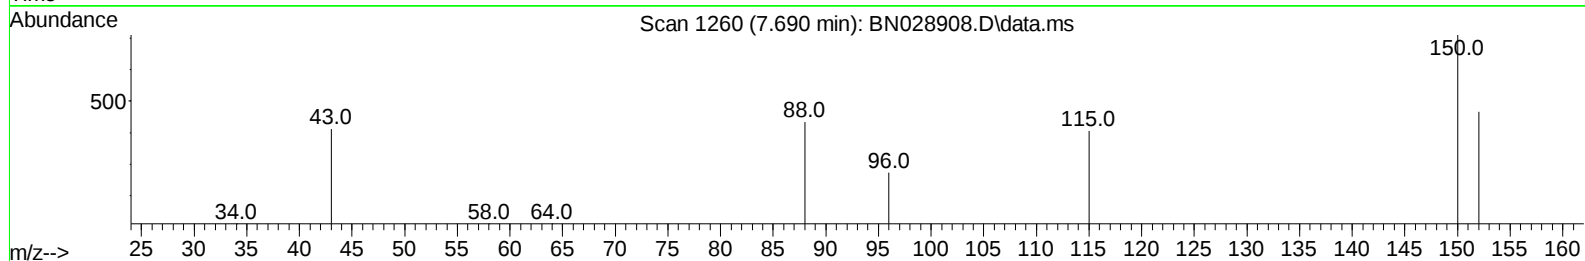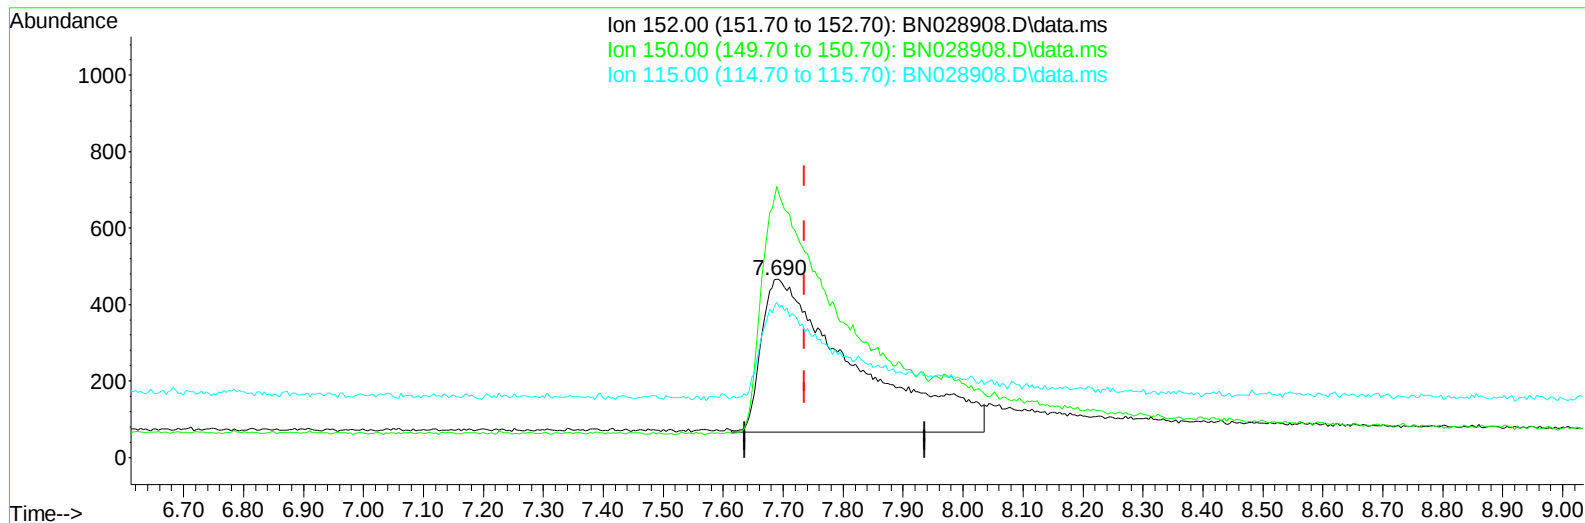

TIC: BN028908.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.690min (-0.046) 0.40 ng/ul m

response 4317

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	152.36
115.00	62.20	87.12#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112823\
 Data File : BN028908.D
 Acq On : 28 Nov 2023 17:37
 Operator : MA/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC0.4EC

Manual IntegrationsAPPROVED

Quant Time: Nov 28 18:17:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/29/2023
 Supervised By :mohammad ahmed 11/29/2023

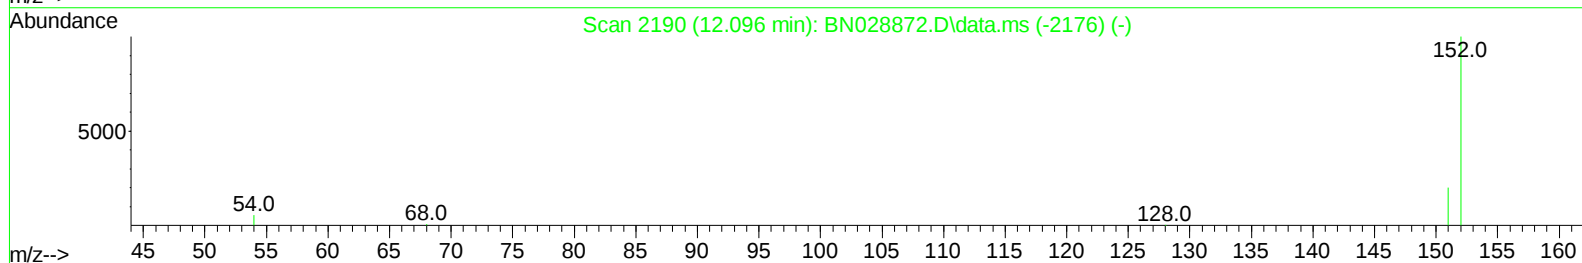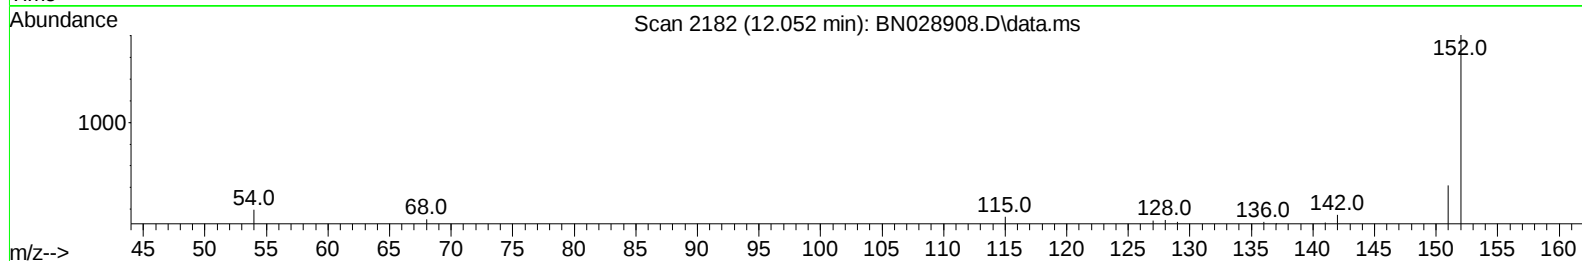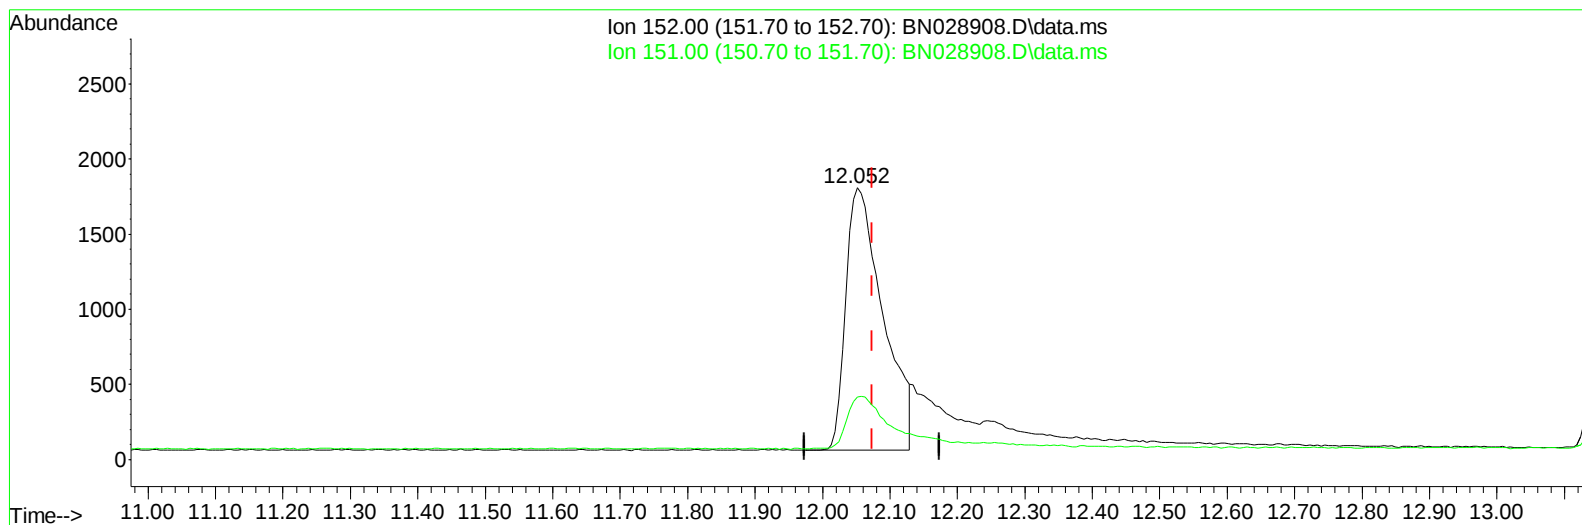

TIC: BN028908.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.052min (-0.022) 0.29 ng/u1

response 6718

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	19.86
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112823\
Data File : BN028908.D
Acq On : 28 Nov 2023 17:37
Operator : MA/JU
Sample : SSTDCCC0.4EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTDCCC0.4EC

Manual IntegrationsAPPROVED

Quant Time: Nov 28 18:17:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/29/2023
Supervised By :mohammad ahmed 11/29/2023

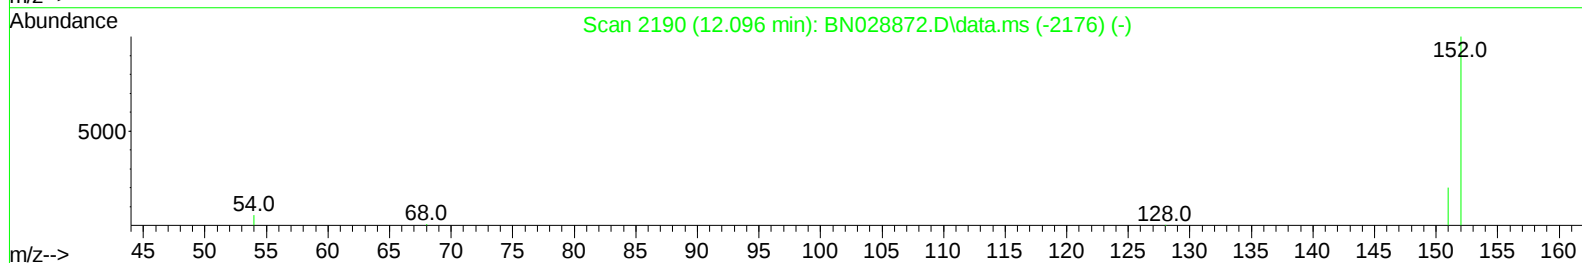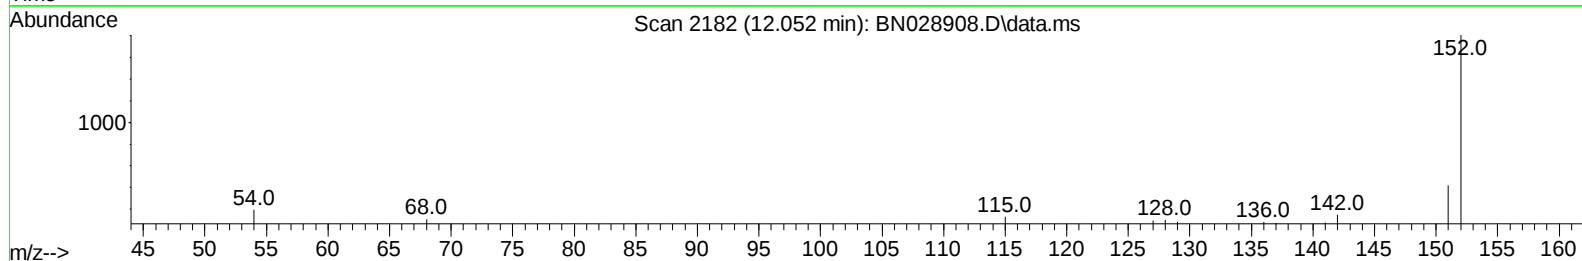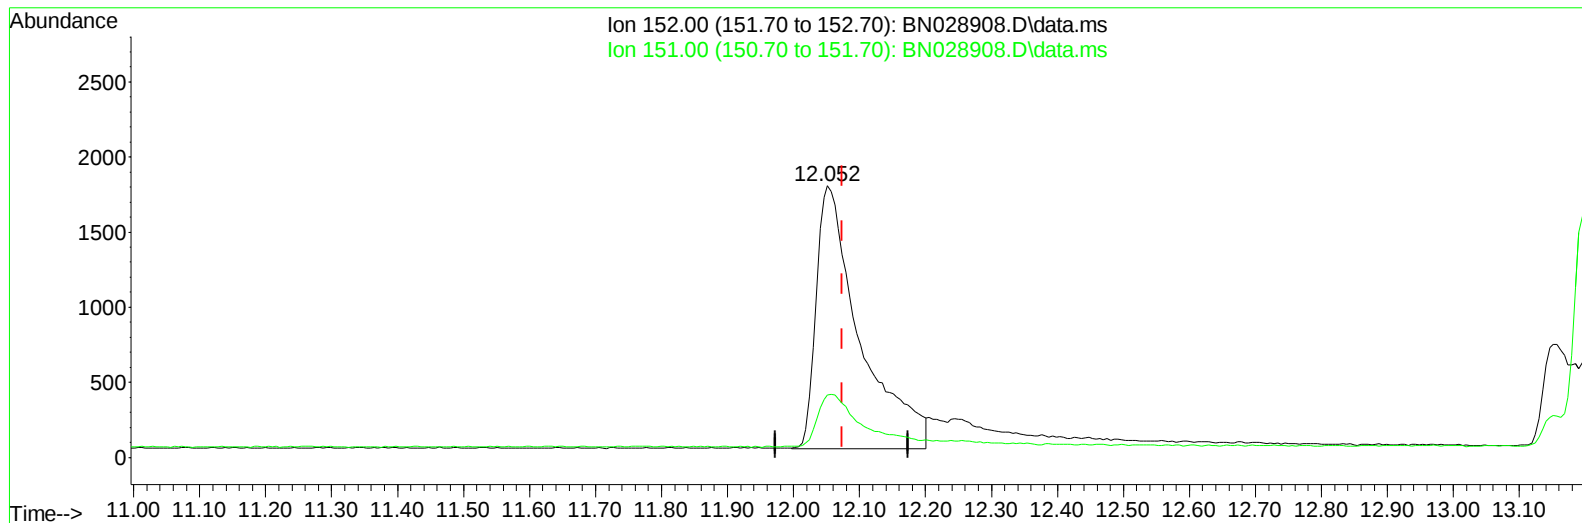

TIC: BN028908.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.052min (-0.022) 0.35 ng/ul m

response 8046

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	16.58
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112823\
 Data File : BN028908.D
 Acq On : 28 Nov 2023 17:37
 Operator : MA/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC0.4EC

Manual IntegrationsAPPROVED

Quant Time: Nov 28 18:17:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/29/2023
 Supervised By :mohammad ahmed 11/29/2023

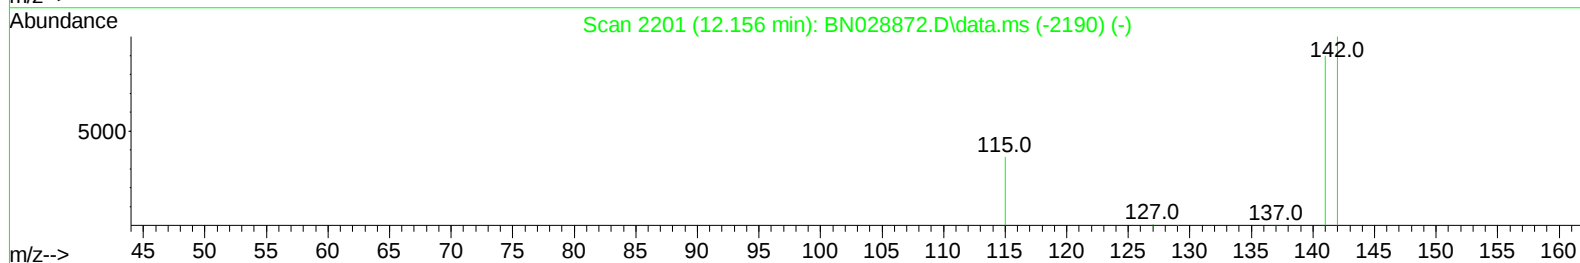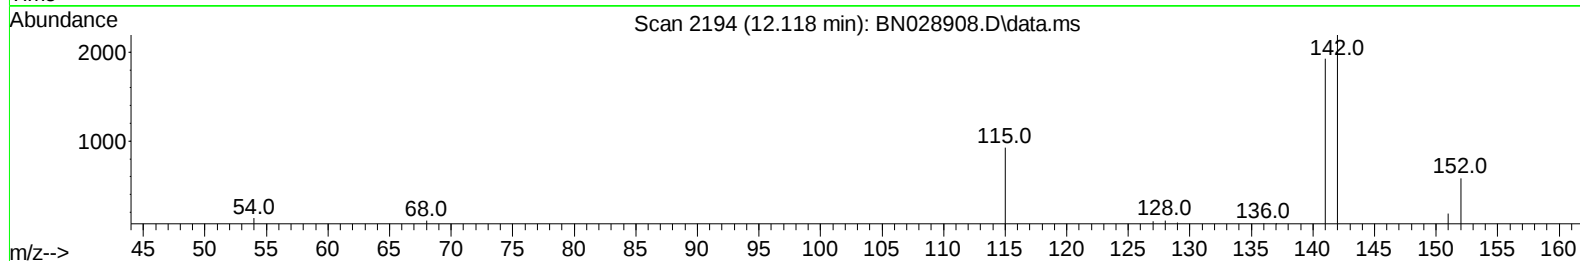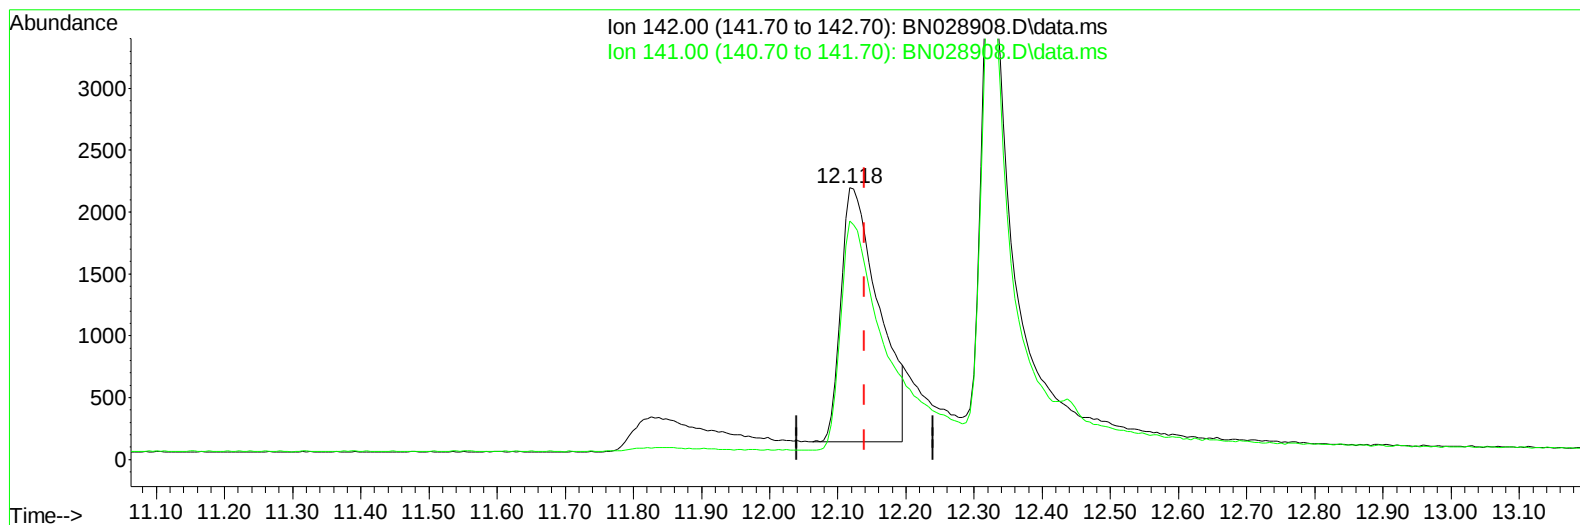

TIC: BN028908.D\data.ms

(7) 2-Methylnaphthalene

12.118min (-0.022) 0.28 ng/u1

response 7925

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	88.50	90.85
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112823\
Data File : BN028908.D
Acq On : 28 Nov 2023 17:37
Operator : MA/JU
Sample : SSTDCCC0.4EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTDCCC0.4EC

Manual IntegrationsAPPROVED

Quant Time: Nov 28 18:17:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/29/2023
Supervised By :mohammad ahmed 11/29/2023

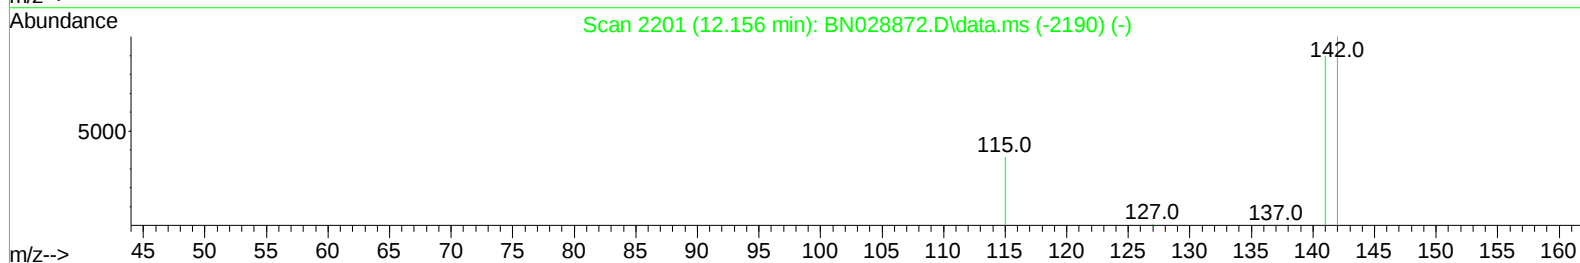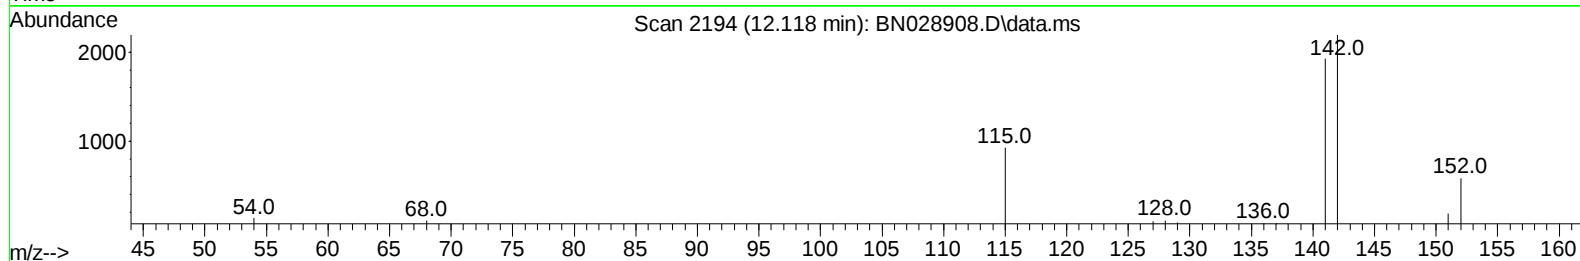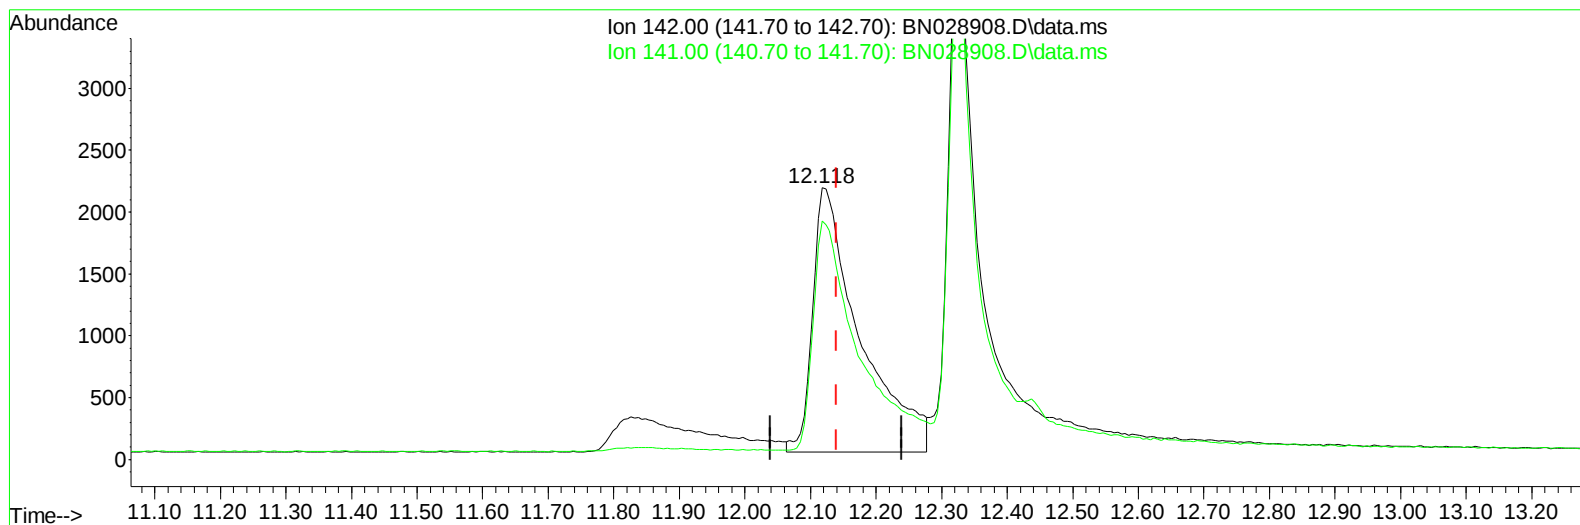

TIC: BN028908.D\data.ms

(7) 2-Methylnaphthalene

12.118min (-0.022) 0.38 ng/ul m

response 10675

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	88.50	67.45#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112823\
 Data File : BN028908.D
 Acq On : 28 Nov 2023 17:37
 Operator : MA/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC0.4EC

Manual IntegrationsAPPROVED

Quant Time: Nov 28 18:17:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/29/2023
 Supervised By :mohammad ahmed 11/29/2023

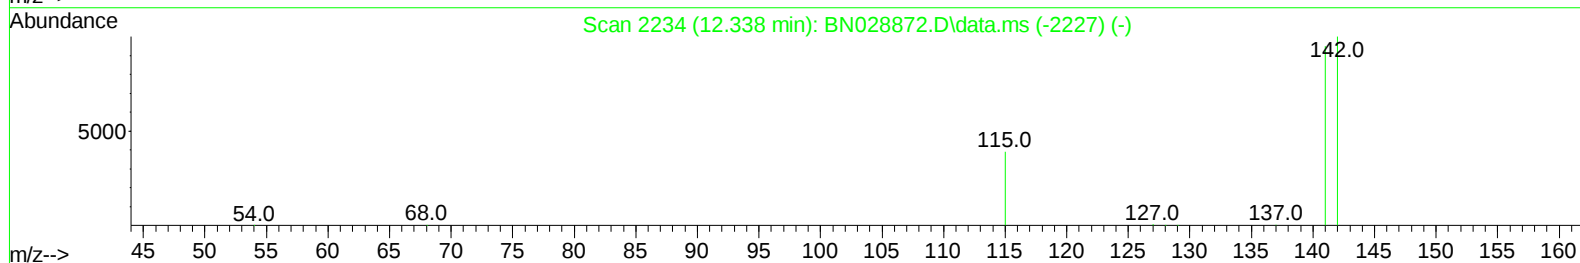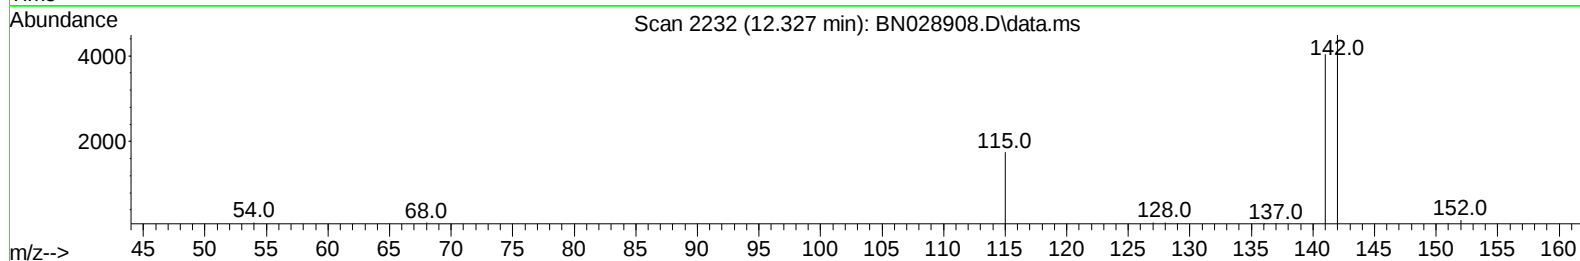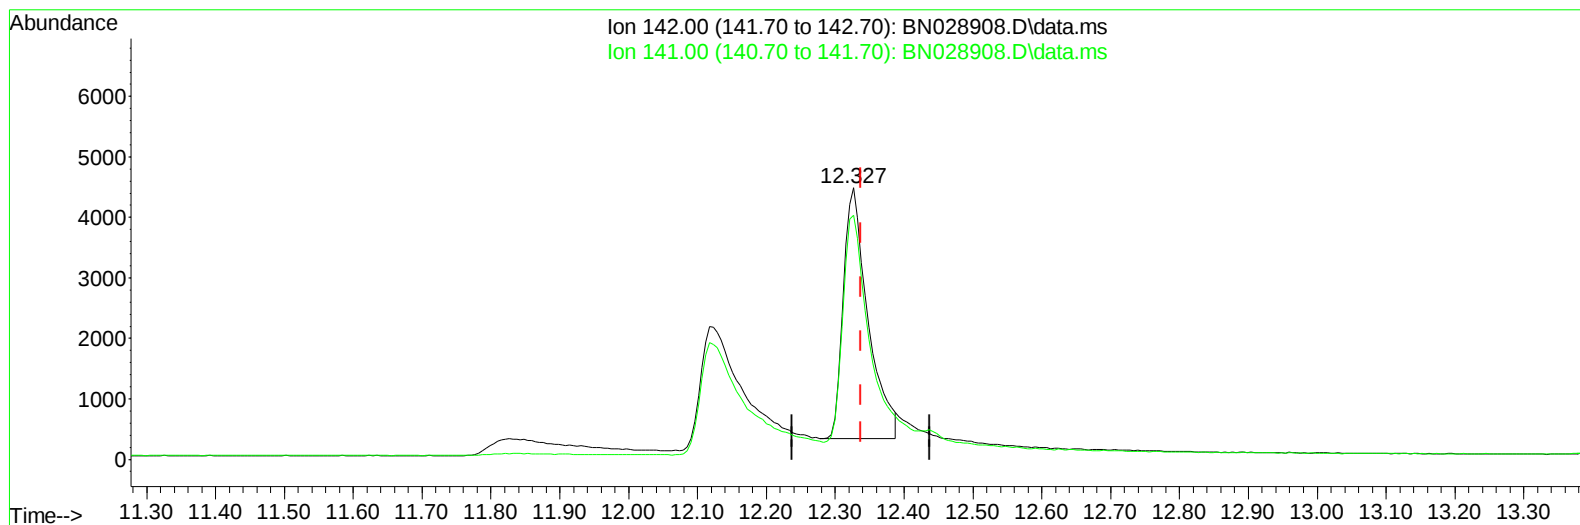

TIC: BN028908.D\data.ms

(8) 1-Methylnaphthalene

12.327min (-0.011) 0.36 ng/u1

response 10302

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	92.60	93.18
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112823\
 Data File : BN028908.D
 Acq On : 28 Nov 2023 17:37
 Operator : MA/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC0.4EC

Manual IntegrationsAPPROVED

Quant Time: Nov 28 18:17:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/29/2023
 Supervised By :mohammad ahmed 11/29/2023

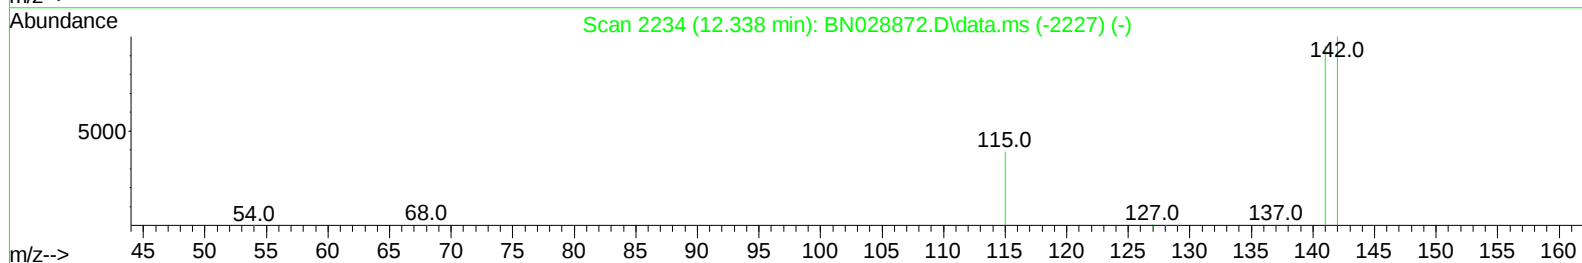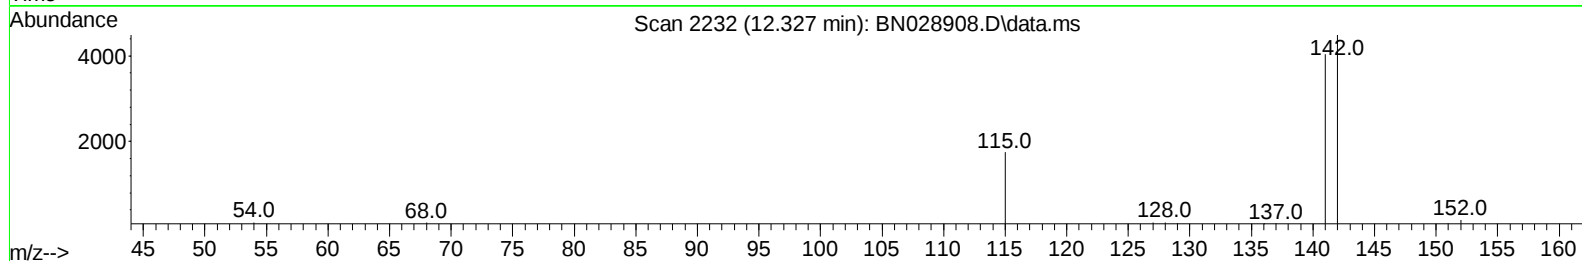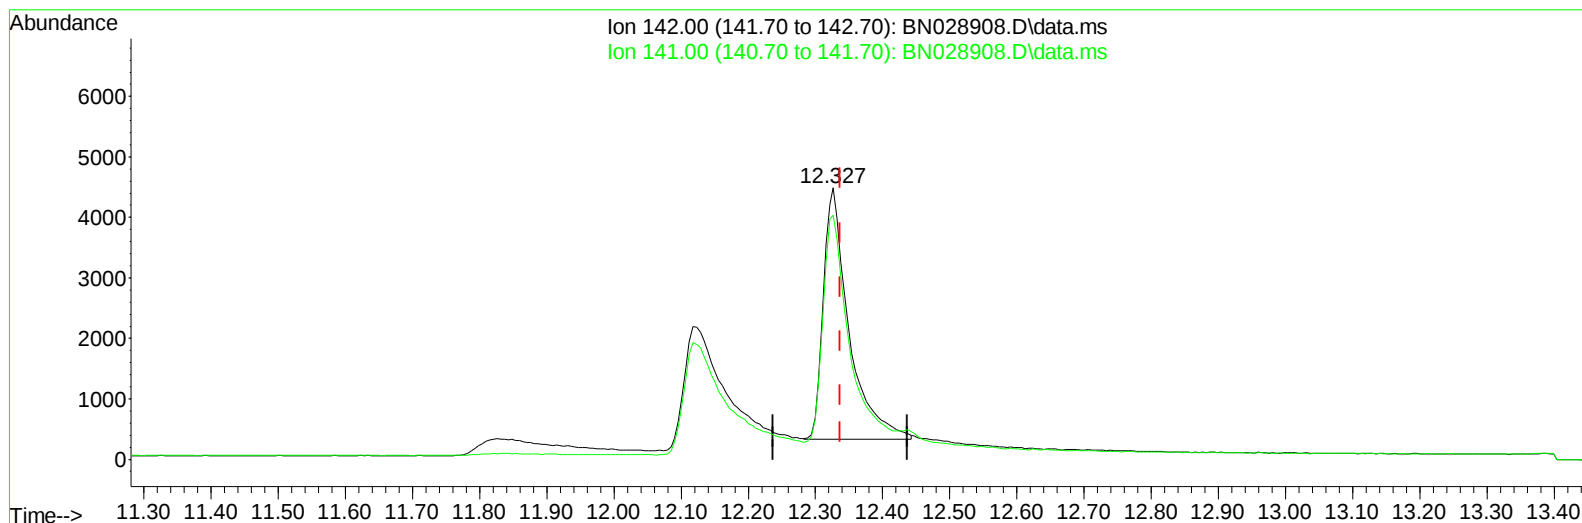

TIC: BN028908.D\data.ms

(8) 1-Methylnaphthalene

12.327min (-0.011) 0.39 ng/ul m

response 11038

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	92.60	86.96
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112823\
Data File : BN028908.D
Acq On : 28 Nov 2023 17:37
Operator : MA/JU
Sample : SSTDCCC0.4EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTDCCC0.4EC

Manual IntegrationsAPPROVED

Quant Time: Nov 28 18:17:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/29/2023
Supervised By :mohammad ahmed 11/29/2023

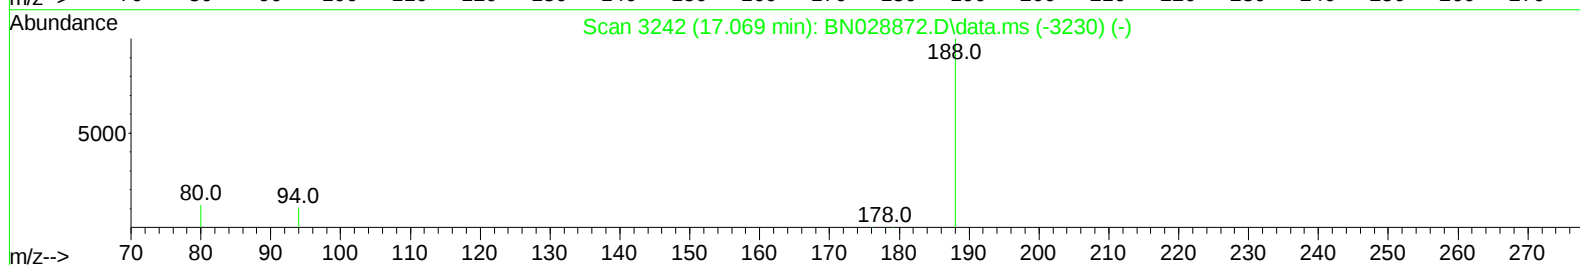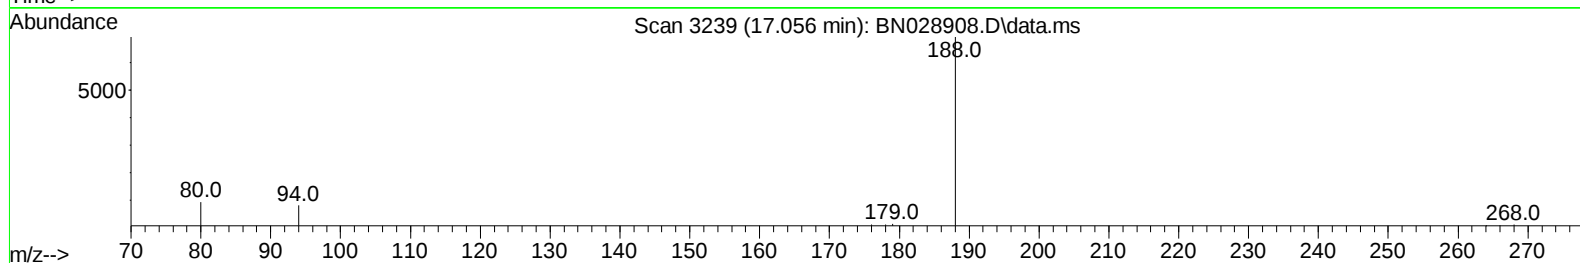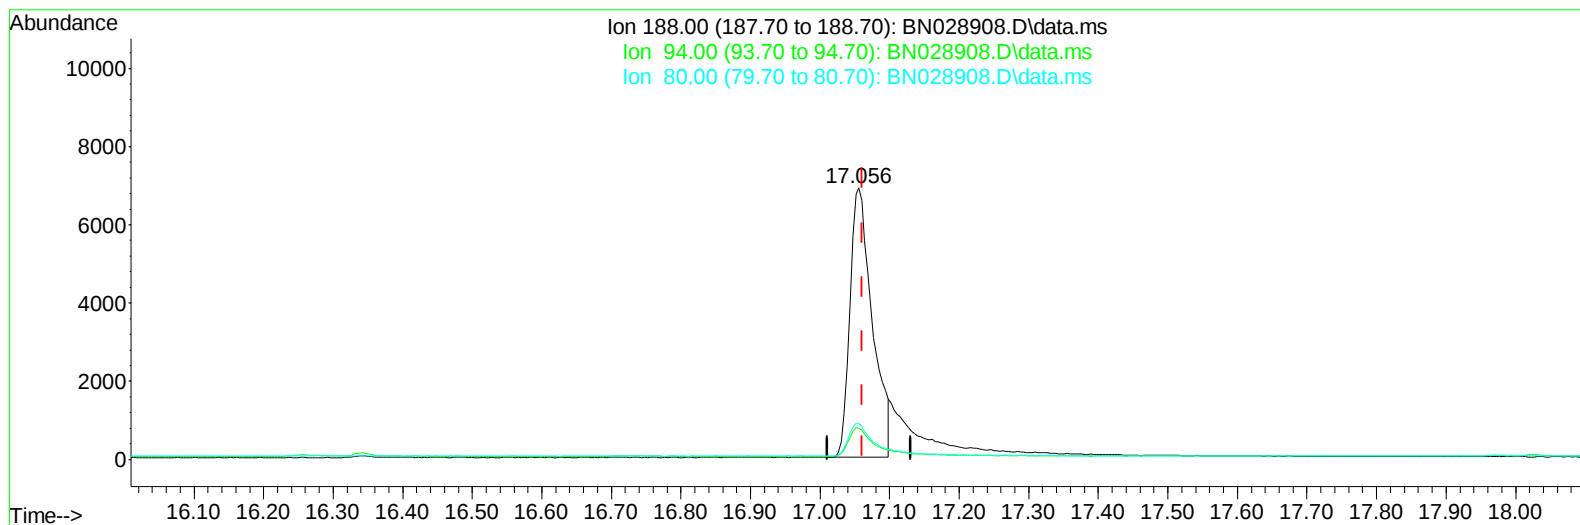

TIC: BN028908.D\data.ms

(13) Phenanthrene-d10 (I)

17.056min (-0.005) 0.40 ng/u1

response 15480

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.10	11.46
80.00	10.90	13.38#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112823\
 Data File : BN028908.D
 Acq On : 28 Nov 2023 17:37
 Operator : MA/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC0.4EC

Manual IntegrationsAPPROVED

Quant Time: Nov 28 18:17:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/29/2023
 Supervised By :mohammad ahmed 11/29/2023

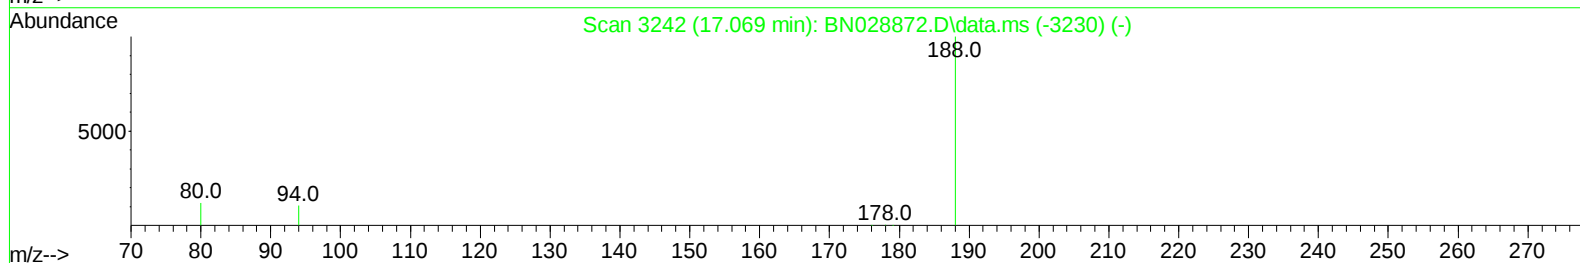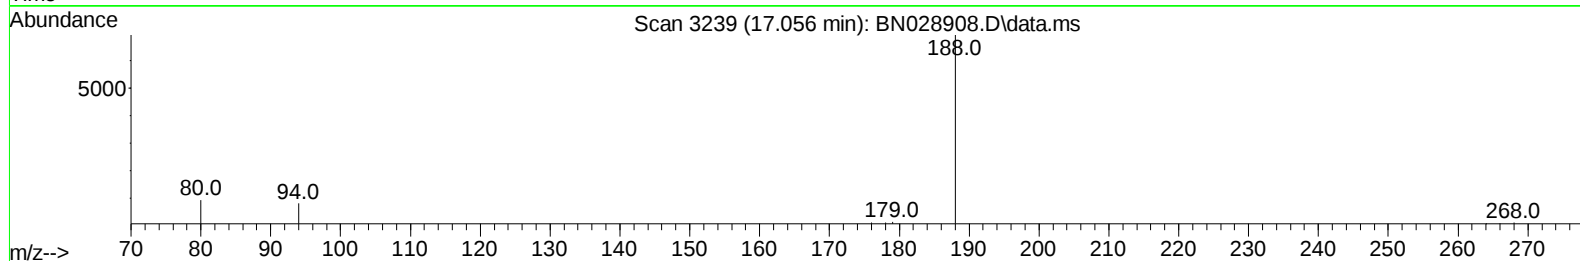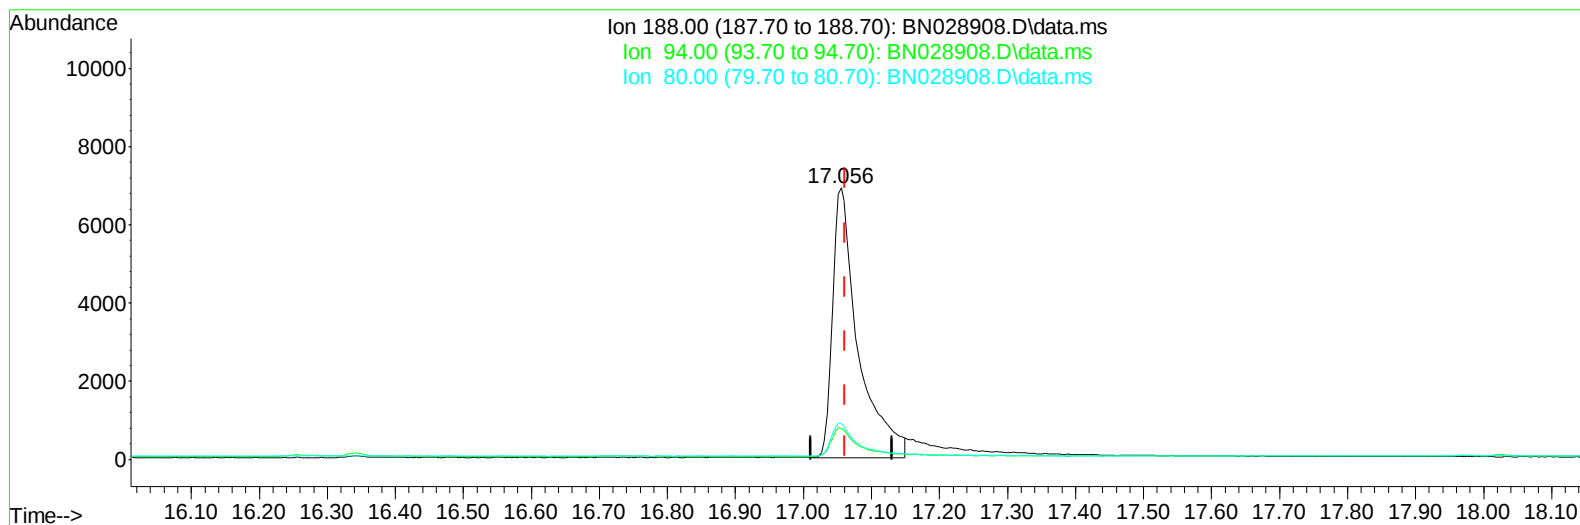

TIC: BN028908.D\data.ms

(13) Phenanthrene-d10 (I)

17.056min (-0.005) 0.40 ng/ul m

response 18078

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.10	11.46
80.00	10.90	13.38#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112823\
 Data File : BN028908.D
 Acq On : 28 Nov 2023 17:37
 Operator : MA/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC0.4EC

Manual IntegrationsAPPROVED

Quant Time: Nov 28 18:17:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/29/2023
 Supervised By :mohammad ahmed 11/29/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.690	152	4317m	0.40	ng/ul	-0.05
4) Naphthalene-d8	10.440	136	15244	0.40	ng/ul	#-0.02
9) Acenaphthene-d10	14.288	164	9338	0.40	ng/ul	-0.01
13) Phenanthrene-d10	17.056	188	18078m	0.40	ng/ul	0.00
17) Chrysene-d12	21.266	240	12970	0.40	ng/ul	# 0.00
23) Perylene-d12	23.540	264	11897	0.40	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.099	96	2563	0.54	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.052	152	8046m	0.35	ng/ul	-0.02
18) Fluoranthene-d10	19.089	212	19480	0.47	ng/ul	0.00
Target Compounds					Qvalue	
2) 1,4-Dioxane	3.133	88	2425	0.46	ng/ul#	76
5) Naphthalene	10.484	128	16467	0.39	ng/ul	98
7) 2-Methylnaphthalene	12.118	142	10675m	0.38	ng/ul	
8) 1-Methylnaphthalene	12.327	142	11038m	0.39	ng/ul	
10) Acenaphthylene	14.011	152	18383	0.39	ng/ul	99
11) Acenaphthene	14.353	153	14586	0.43	ng/ul	99
12) Fluorene	15.357	166	14049	0.35	ng/ul	98
14) Pentachlorophenol	16.718	266	1336	0.31	ng/ul	100
15) Phenanthrene	17.094	178	21119	0.38	ng/ul	98
16) Anthracene	17.195	178	16309	0.32	ng/ul	97
19) Fluoranthene	19.117	202	25550	0.46	ng/ul	99
20) Pyrene	19.480	202	27713	0.48	ng/ul	95
21) Benzo(a)anthracene	21.255	228	17626	0.34	ng/ul	98
22) Chrysene	21.301	228	20278	0.40	ng/ul	98
24) Benzo(b)fluoranthene	22.853	252	16797	0.38	ng/ul	83
25) Benzo(k)fluoranthene	22.897	252	20684	0.44	ng/ul#	88
26) Benzo(a)pyrene	23.444	252	17788	0.42	ng/ul#	73
27) Indeno(1,2,3-cd)pyrene	25.874	276	20113	0.43	ng/ul	100
28) Dibenzo(a,h)anthracene	25.894	278	15859	0.42	ng/ul	93
29) Benzo(g,h,i)perylene	26.574	276	17047	0.44	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112823\
Data File : BN028908.D
Acq On : 28 Nov 2023 17:37
Operator : MA/JU
Sample : SSTDCCC0.4EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTDCCC0.4EC

Manual IntegrationsAPPROVED

Quant Time: Nov 28 18:17:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/29/2023
Supervised By :mohammad ahmed 11/29/2023

