

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113021\
 Data File : BN017619.D
 Acq On : 30 Nov 2021 19:24
 Operator : CG/JU
 Sample : PB141079BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB141079BL

Quant Time: Dec 01 00:16:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN113021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 30 18:26:44 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.782	152	27104	0.40	ng	0.00
7) Naphthalene-d8	10.560	136	105864	0.40	ng	# 0.01
13) Acenaphthene-d10	14.384	164	60503	0.40	ng	0.00
19) Phenanthrene-d10	17.128	188	116444	0.40	ng	0.00
29) Chrysene-d12	21.314	240	102810	0.40	ng	# 0.00
35) Perylene-d12	23.626	264	97294	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.403	112	18427	0.30	ng	0.04
5) Phenol-d6	6.952	99	16983	0.26	ng	0.00
8) Nitrobenzene-d5	8.912	82	13116	0.29	ng	0.00
11) 2-Methylnaphthalene-d10	12.146	152	51288	0.28	ng	0.00
14) 2,4,6-Tribromophenol	15.881	330	2654	0.19	ng	0.00
15) 2-Fluorobiphenyl	13.014	172	68939	0.29	ng	0.00
27) Fluoranthene-d10	19.163	212	96630	0.27	ng	0.00
31) Terphenyl-d14	19.764	244	74426	0.33	ng	0.00


Target Compounds Qvalue


 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113021\
Data File : BN017619.D
Acq On : 30 Nov 2021 19:24
Operator : CG/JU
Sample : PB141079BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB141079BL

Quant Time: Dec 01 00:16:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN113021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 30 18:26:44 2021
Response via : Initial Calibration




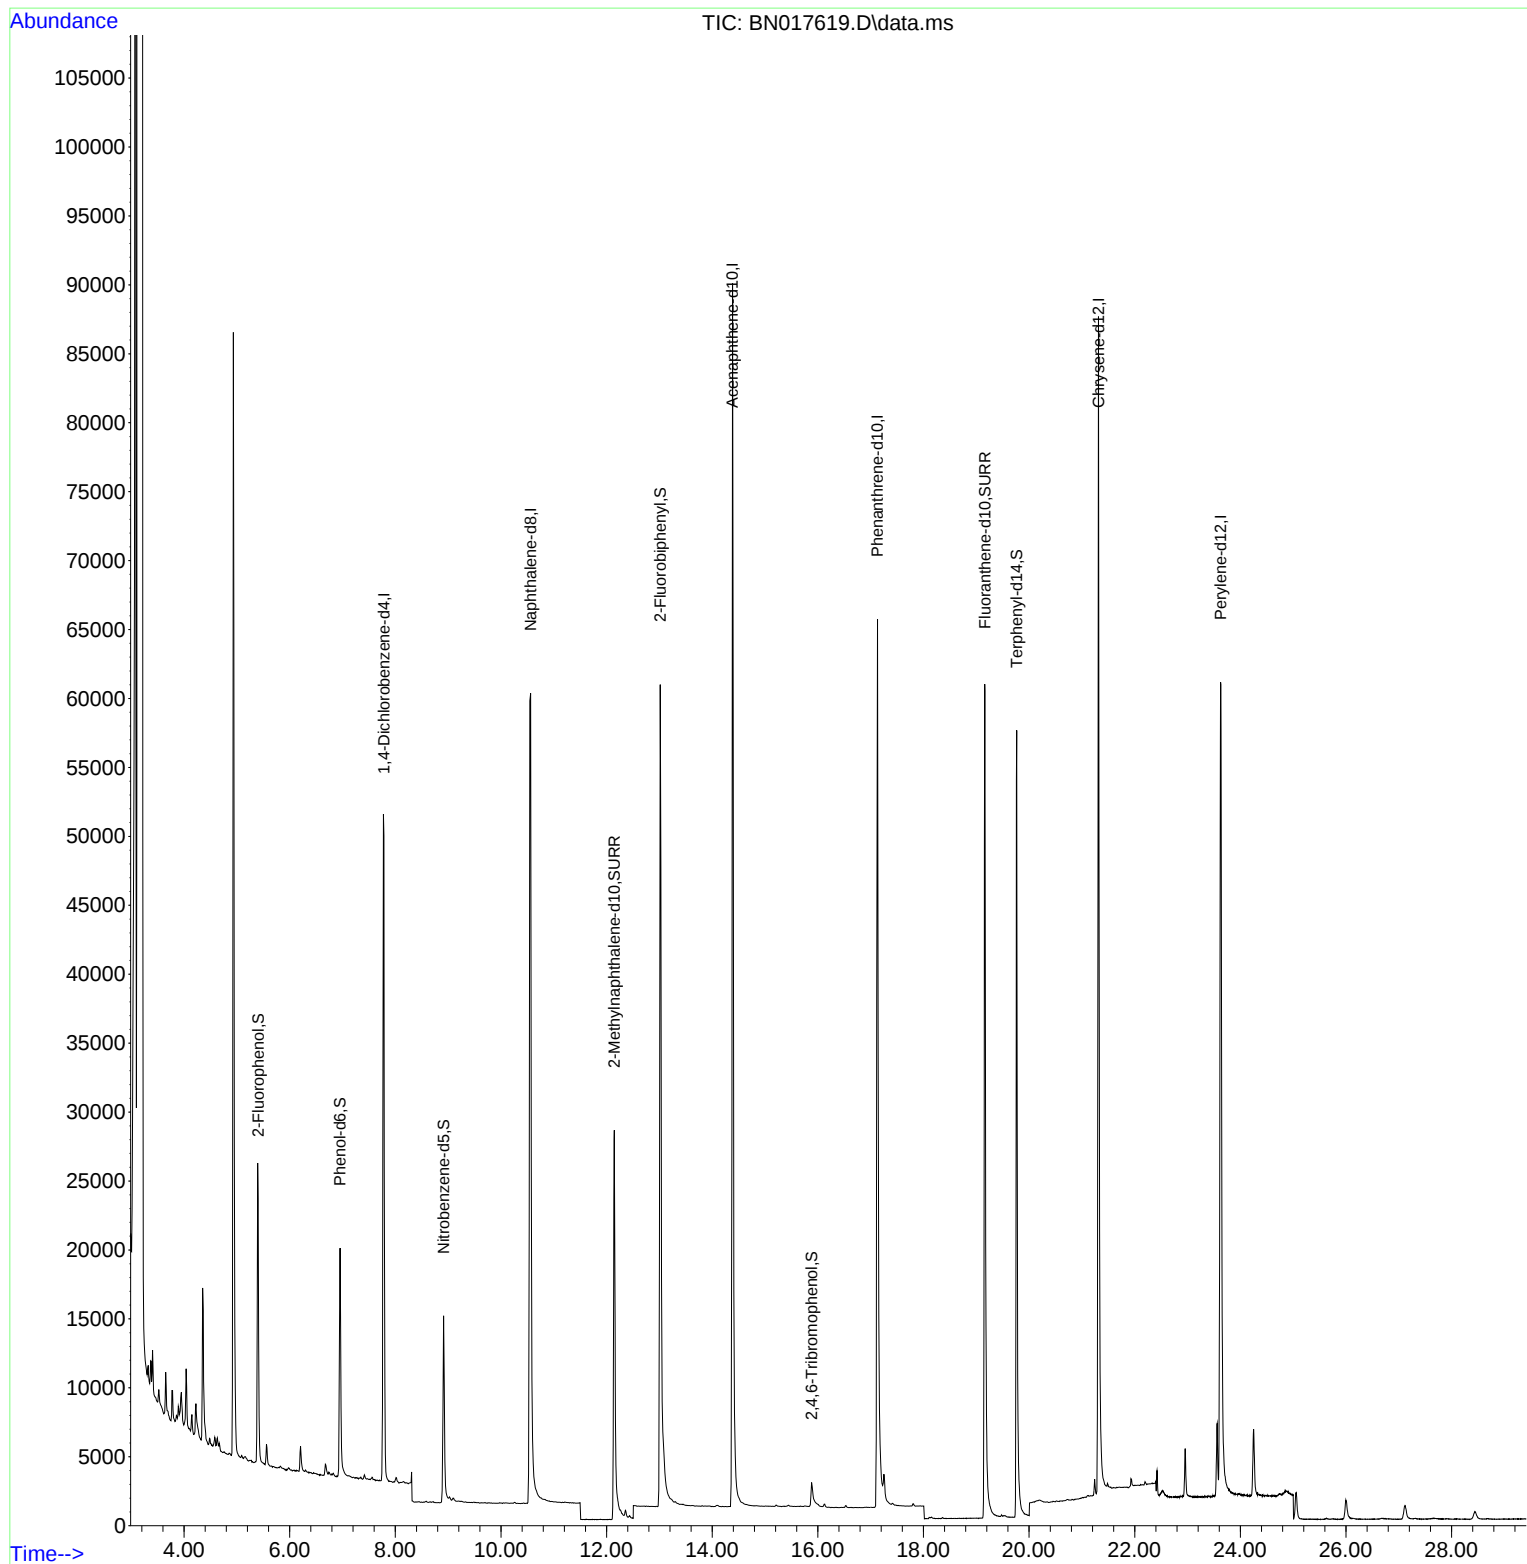


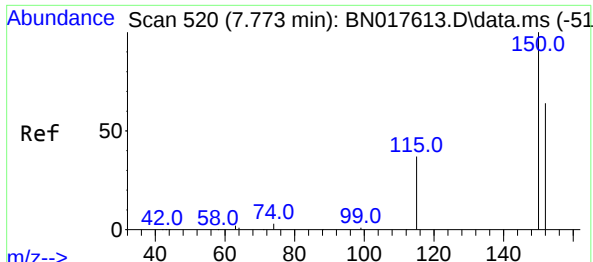

#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.782 min Scan# 51
Delta R.T. 0.009 min
Lab File: BN017619.D
Acq: 30 Nov 2021 19:24




Instrument :
BNA_N
ClientSampleId :
PB141079BL


Tgt Ion:152 Resp: 27104
Ion Ratio Lower Upper
152 100
150 150.8 123.0 184.4
115 55.8 45.6 68.4

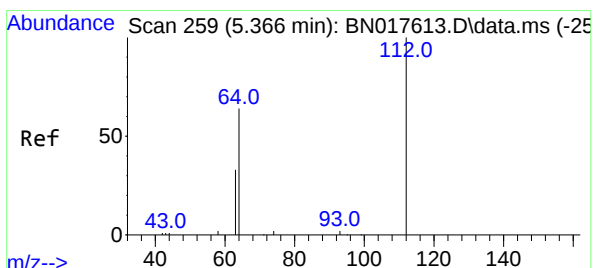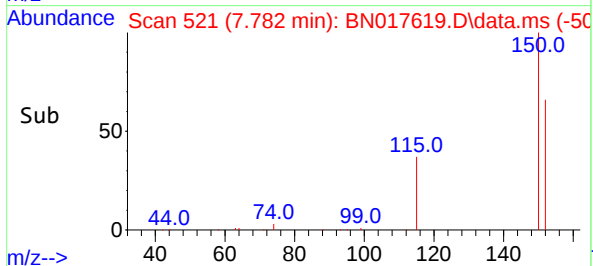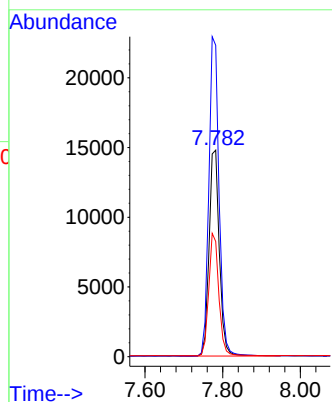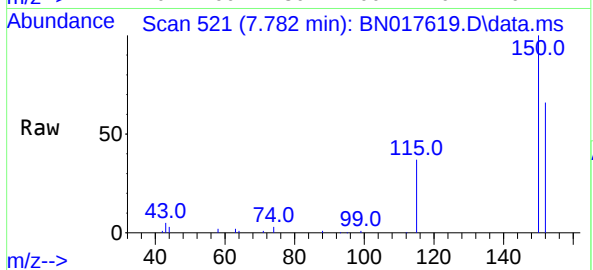

#4
2-Fluorophenol
Concen: 0.30 ng
RT: 5.403 min Scan# 263
Delta R.T. 0.037 min
Lab File: BN017619.D
Acq: 30 Nov 2021 19:24

Tgt Ion:112 Resp: 18427
Ion Ratio Lower Upper
112 100
64 64.6 47.6 71.4
63 33.1 24.6 37.0


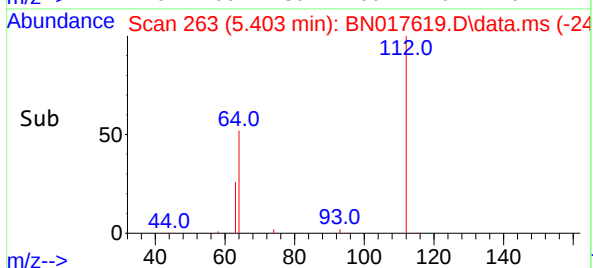

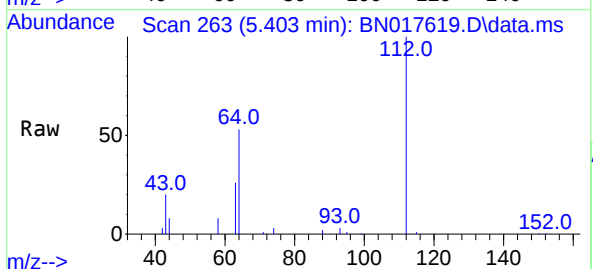




#5
Phenol-d6
Concen: 0.26 ng
RT: 6.952 min Scan# 41
Delta R.T. 0.009 min
Lab File: BN017619.D
Acq: 30 Nov 2021 19:24




Instrument :
BNA_N
ClientSampleId :
PB141079BL


Tgt Ion: 99 Resp: 16983
Ion Ratio Lower Upper
99 100
42 20.0 17.0 25.6
71 35.1 24.8 37.2

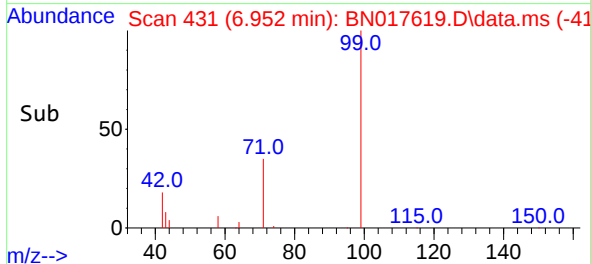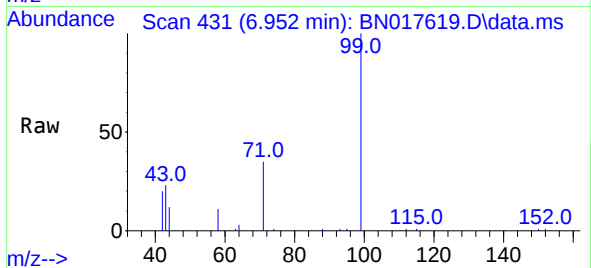

#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.560 min Scan# 756
Delta R.T. 0.013 min
Lab File: BN017619.D
Acq: 30 Nov 2021 19:24

Tgt Ion: 136 Resp: 105864
Ion Ratio Lower Upper
136 100
137 10.9 8.8 13.2
54 6.3 4.0 6.0#
68 5.4 3.0 4.6#


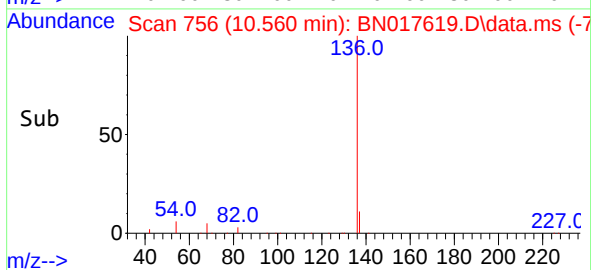

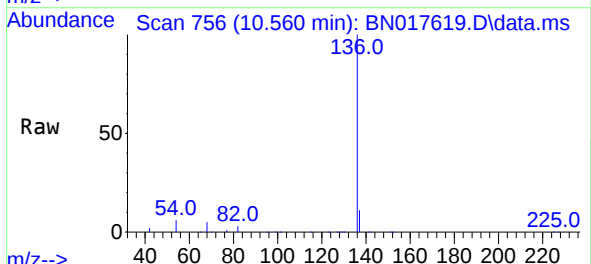




#8
Nitrobenzene-d5
Concen: 0.29 ng
RT: 8.912 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN017619.D
Acq: 30 Nov 2021 19:24




Instrument :
BNA_N
ClientSampleId :
PB141079BL


Tgt Ion:	82	Resp:	13116
Ion	Ratio	Lower	Upper
82	100		
128	32.9	27.7	41.5
54	52.5	49.2	73.8

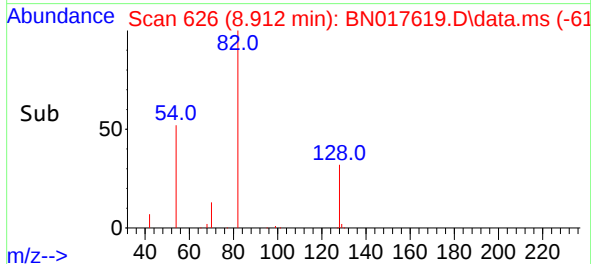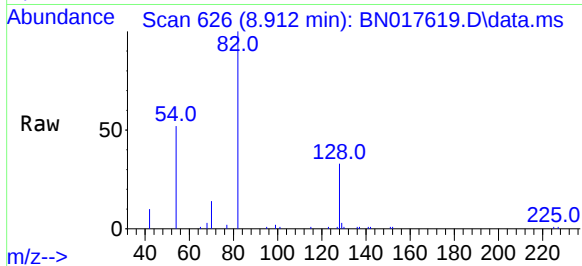

#11
2-Methylnaphthalene-d10
Concen: 0.28 ng
RT: 12.146 min Scan# 974
Delta R.T. 0.004 min
Lab File: BN017619.D
Acq: 30 Nov 2021 19:24

Tgt Ion:	152	Resp:	51288
Ion	Ratio	Lower	Upper
152	100		
151	20.3	16.2	24.4


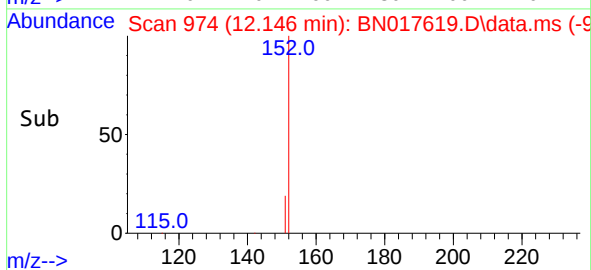

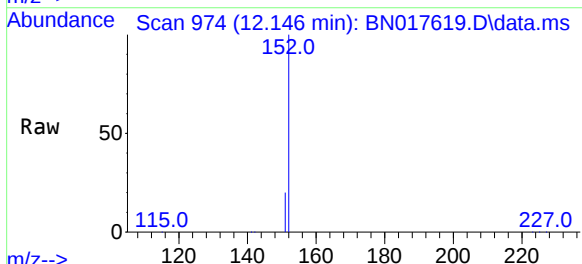


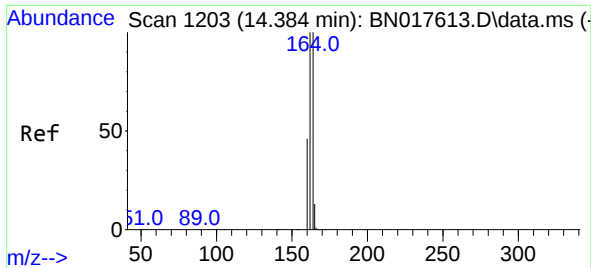

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.384 min Scan# 1203
Delta R.T. 0.000 min
Lab File: BN017619.D
Acq: 30 Nov 2021 19:24




Instrument :
BNA_N
ClientSampleId :
PB141079BL


Tgt Ion:164 Resp: 60503
Ion Ratio Lower Upper
164 100
162 101.7 81.4 122.2
160 48.4 36.8 55.2

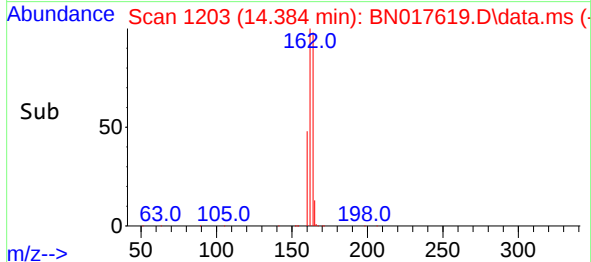

#14
2,4,6-Tribromophenol
Concen: 0.19 ng
RT: 15.881 min Scan# 1321
Delta R.T. 0.000 min
Lab File: BN017619.D
Acq: 30 Nov 2021 19:24

Tgt Ion:330 Resp: 2654
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 29.1 28.9 43.3


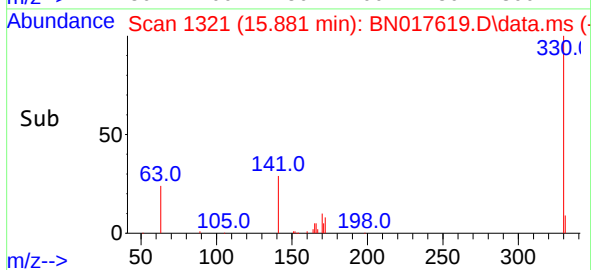

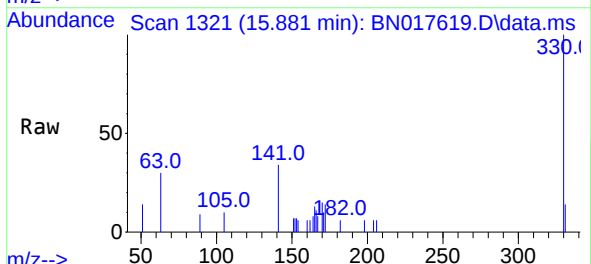




#15
2-Fluorobiphenyl
Concen: 0.29 ng
RT: 13.014 min Scan# 1095
Delta R.T. -0.000 min
Lab File: BN017619.D
Acq: 30 Nov 2021 19:24




Instrument :
BNA_N
ClientSampleId :
PB141079BL


Tgt Ion:172 Resp: 68939
Ion Ratio Lower Upper
172 100
171 35.4 28.7 43.1
170 23.6 19.4 29.2

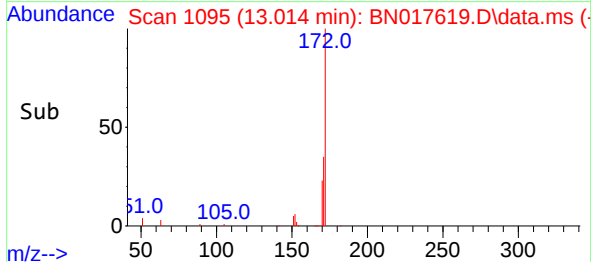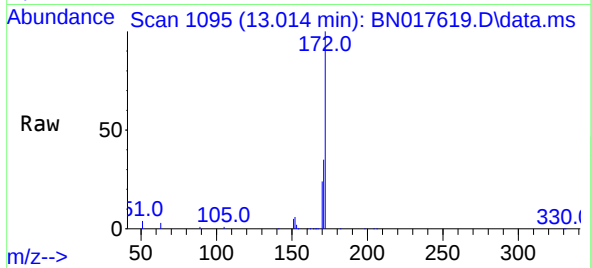

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.128 min Scan# 1423
Delta R.T. 0.000 min
Lab File: BN017619.D
Acq: 30 Nov 2021 19:24

Tgt Ion:188 Resp: 116444
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.6 6.1 9.1


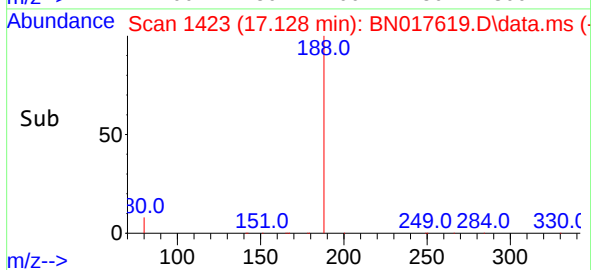

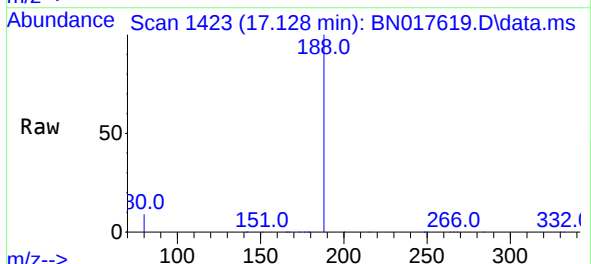




#27
Fluoranthene-d10
Concen: 0.27 ng
RT: 19.163 min Scan# 1726
Delta R.T. 0.005 min
Lab File: BN017619.D
Acq: 30 Nov 2021 19:24




Instrument :
BNA_N
ClientSampleId :
PB141079BL


Tgt Ion:212 Resp: 96630
Ion Ratio Lower Upper
212 100
106 11.5 10.5 15.7
104 6.3 5.8 8.6

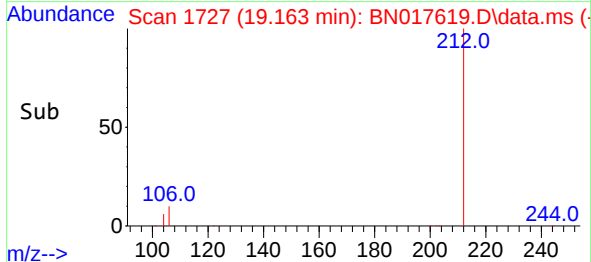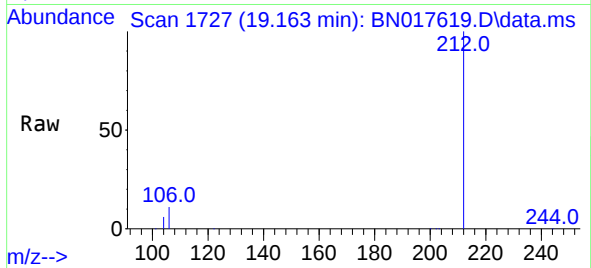

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.314 min Scan# 2020
Delta R.T. -0.000 min
Lab File: BN017619.D
Acq: 30 Nov 2021 19:24

Tgt Ion:240 Resp: 102810
Ion Ratio Lower Upper
240 100
120 7.9 4.2 6.2#
236 26.4 20.0 30.0


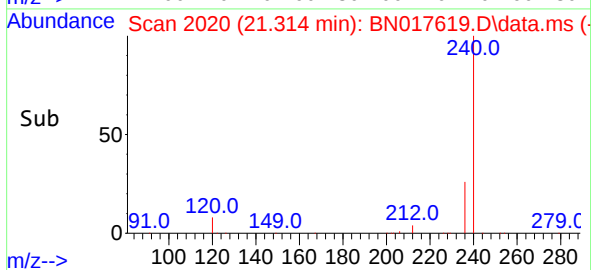

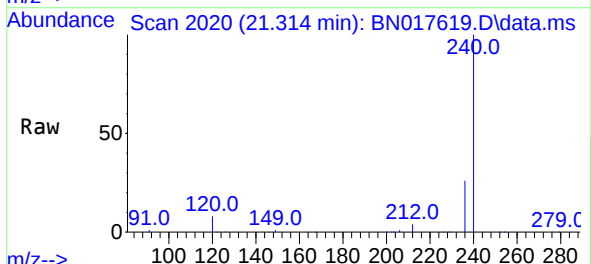




#31
 Terphenyl-d14
 Concen: 0.33 ng
 RT: 19.764 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BN017619.D
 Acq: 30 Nov 2021 19:24

Instrument :
 BNA_N
 ClientSampleId :
 PB141079BL

Tgt Ion:244 Resp: 74426
 Ion Ratio Lower Upper
 244 100
 212 7.5 5.7 8.5
 122 9.6 8.6 13.0

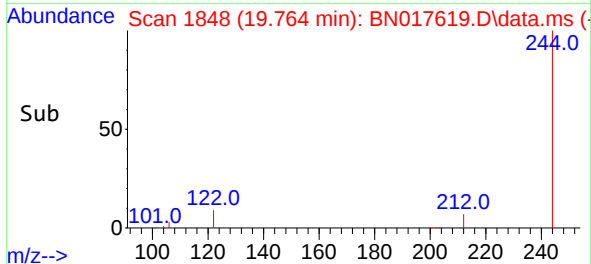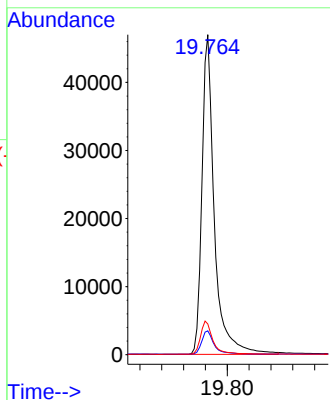

#35
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.626 min Scan# 2479
 Delta R.T. -0.003 min
 Lab File: BN017619.D
 Acq: 30 Nov 2021 19:24

Tgt Ion:264 Resp: 97294
 Ion Ratio Lower Upper
 264 100
 260 24.9 19.4 29.2
 265 24.0 18.6 28.0

