
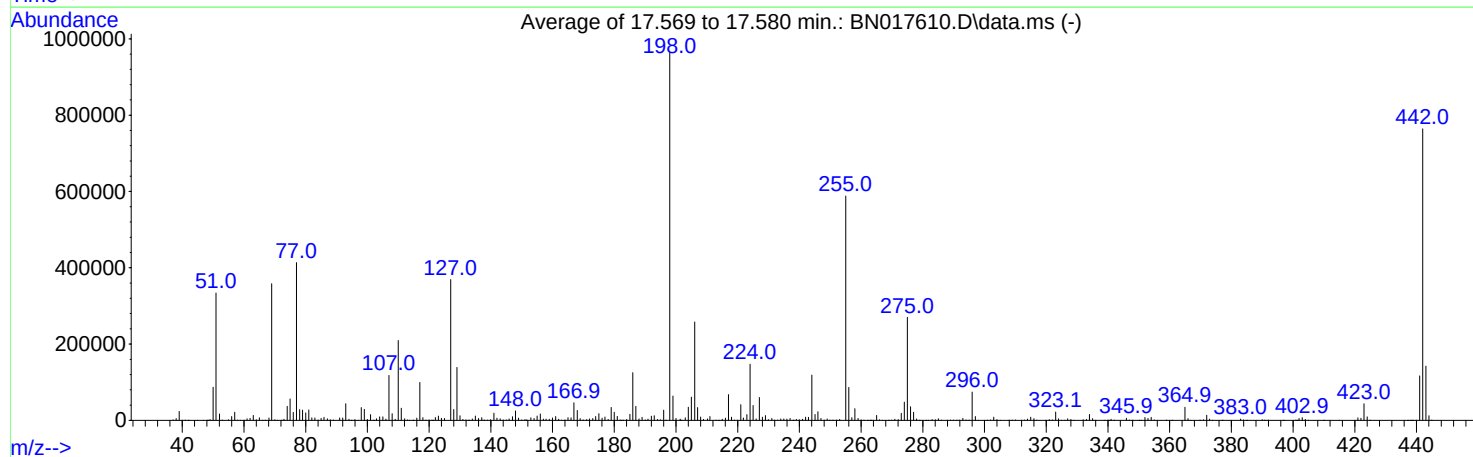


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113021\
 Data File : BN017610.D
 Acq On : 30 Nov 2021 13:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN113021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 02 01:51:49 2021

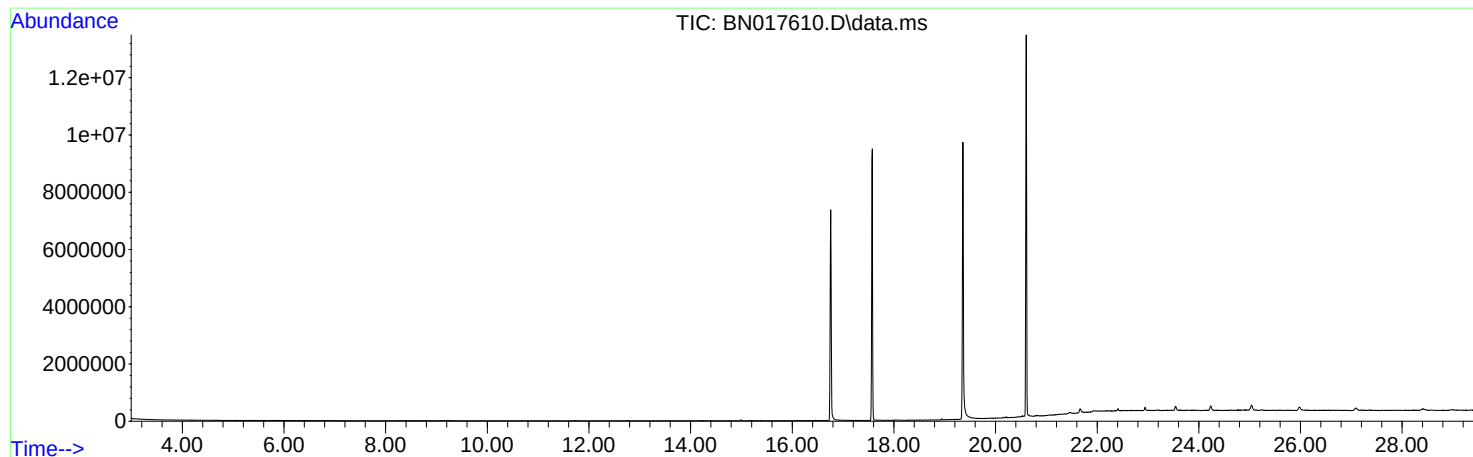

Spectrum Information: Average of 17.569 to 17.580 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	334054	PASS
68	69	0.00	2	1.8	6395	PASS
69	198	0.00	100	37.1	357990	PASS
70	69	0.00	2	0.5	1901	PASS
127	198	10	80	38.3	368981	PASS
197	198	0.00	2	0.1	944	PASS
198	198	100	100	100.0	964224	PASS
199	198	5	9	6.6	63565	PASS
275	198	10	60	28.0	270101	PASS
365	198	1	100	3.6	34531	PASS
441	198	0.01	100	12.1	116573	PASS
442	442	50	100	100.0	764075	PASS
443	442	15	24	18.6	142144	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/30/2021	BNA_N	<u>BN017610.D</u>
Compound Name	Response	Retention Time
DDT	2825837	20.6
DDD	5614	20.16
DDE	369	19.65
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5983	2831820	0.21

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113021\
 Data File : BN017610.D
 Acq On : 30 Nov 2021 13:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 01 01:46:35 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 01 01:46:29 2021
 Response via : Initial Calibration

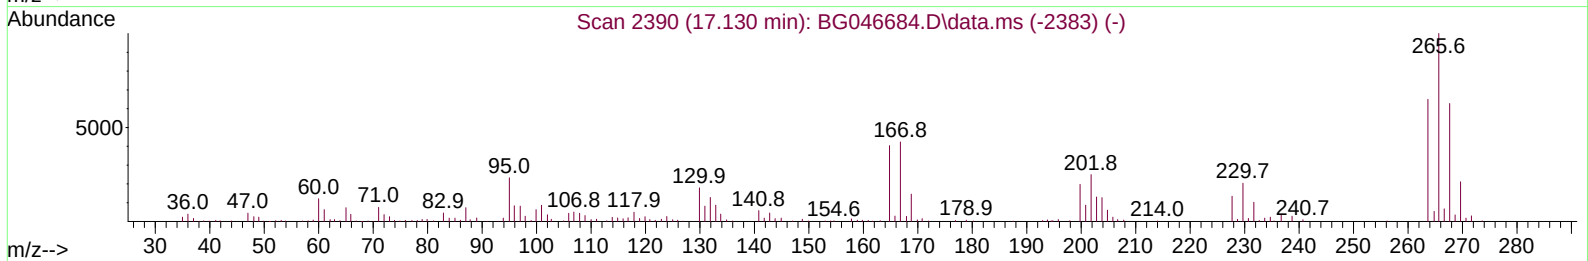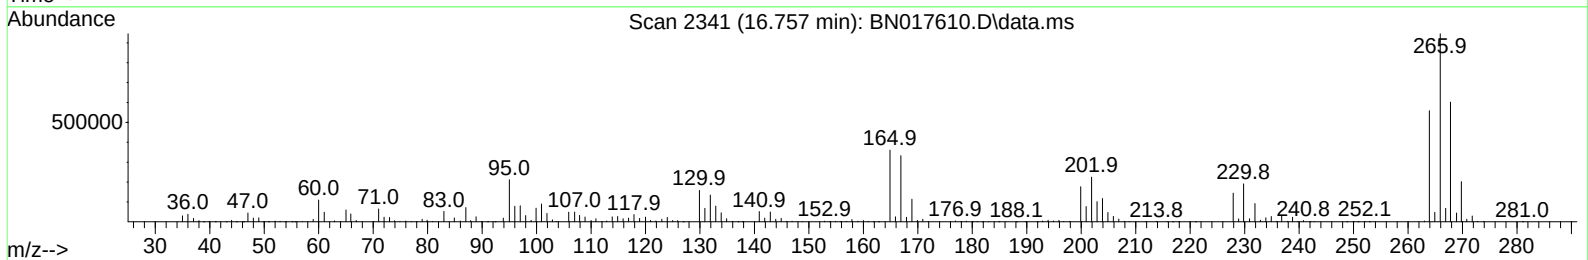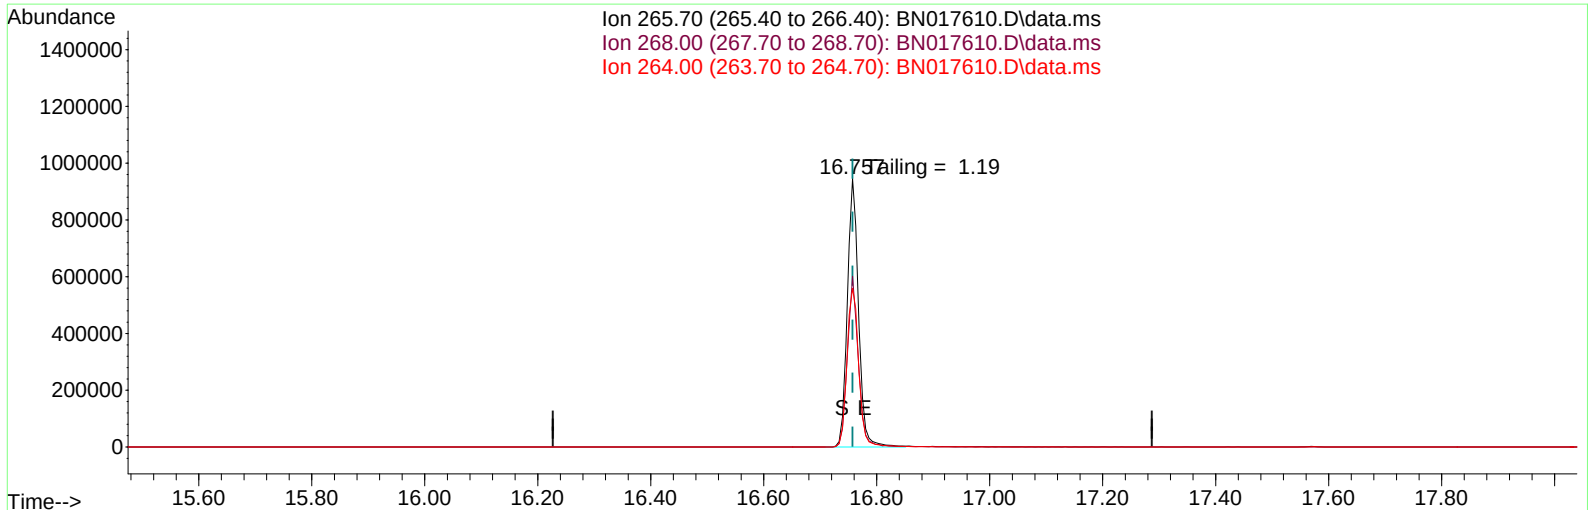

TIC: BN017610.D\data.ms

(70) Pentachlorophenol (C)

16.757min (0.000) 29948.23 ng




response 1310036

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.65
264.00	61.60	59.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113021\
 Data File : BN017610.D
 Acq On : 30 Nov 2021 13:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 01 01:46:35 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 01 01:46:29 2021
 Response via : Initial Calibration

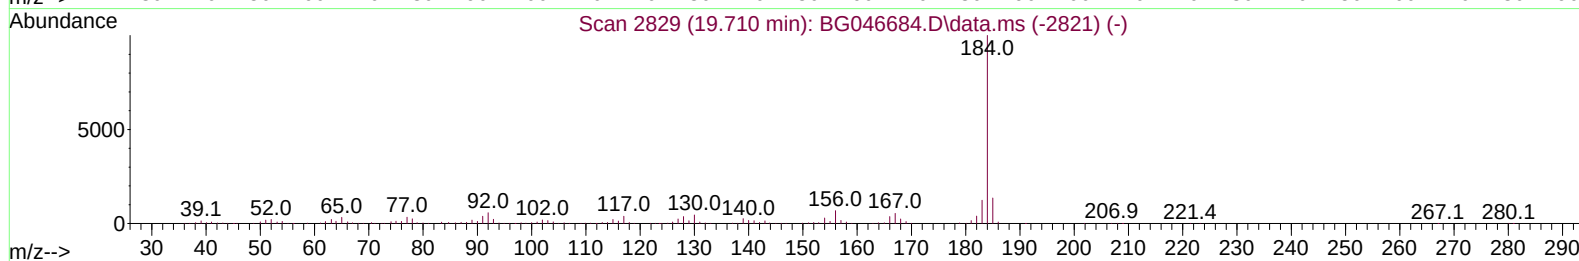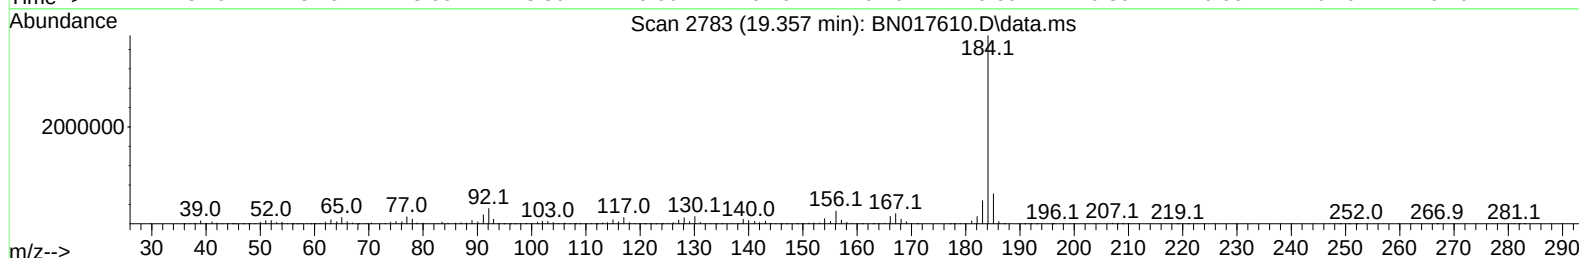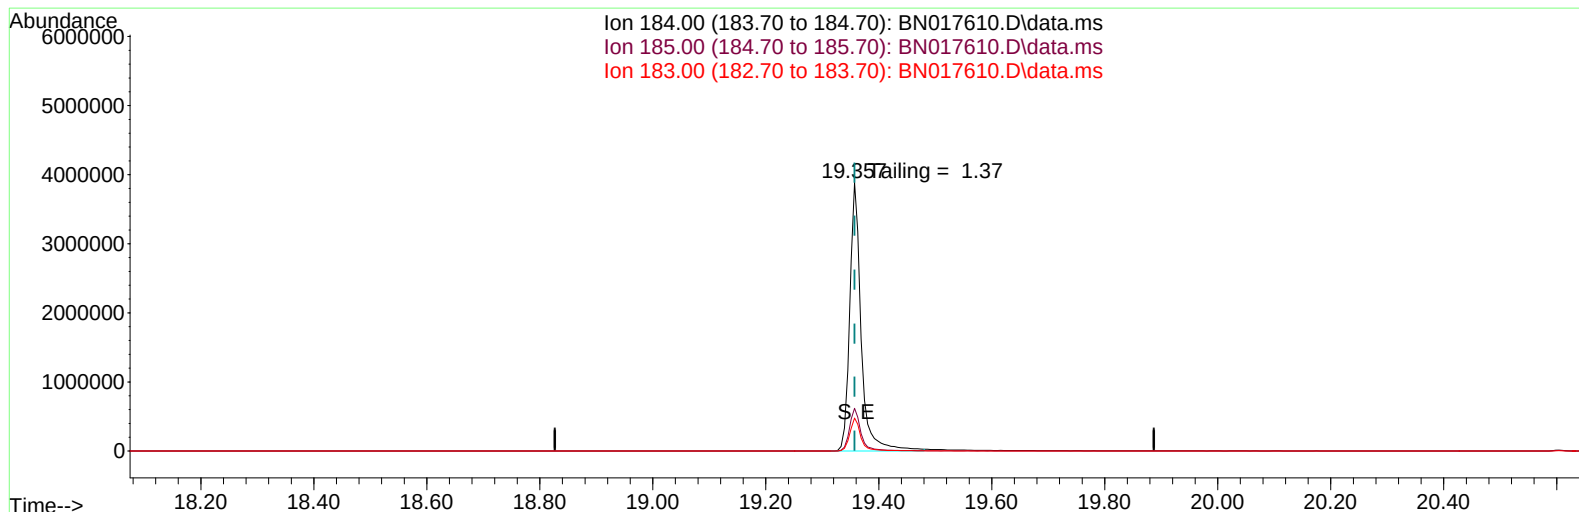

TIC: BN017610.D\data.ms

(77) Benzidine

19.357min (0.000) 1321663.37 ng

response 5540744

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.91
183.00	13.20	12.30
0.00	0.00	0.00