
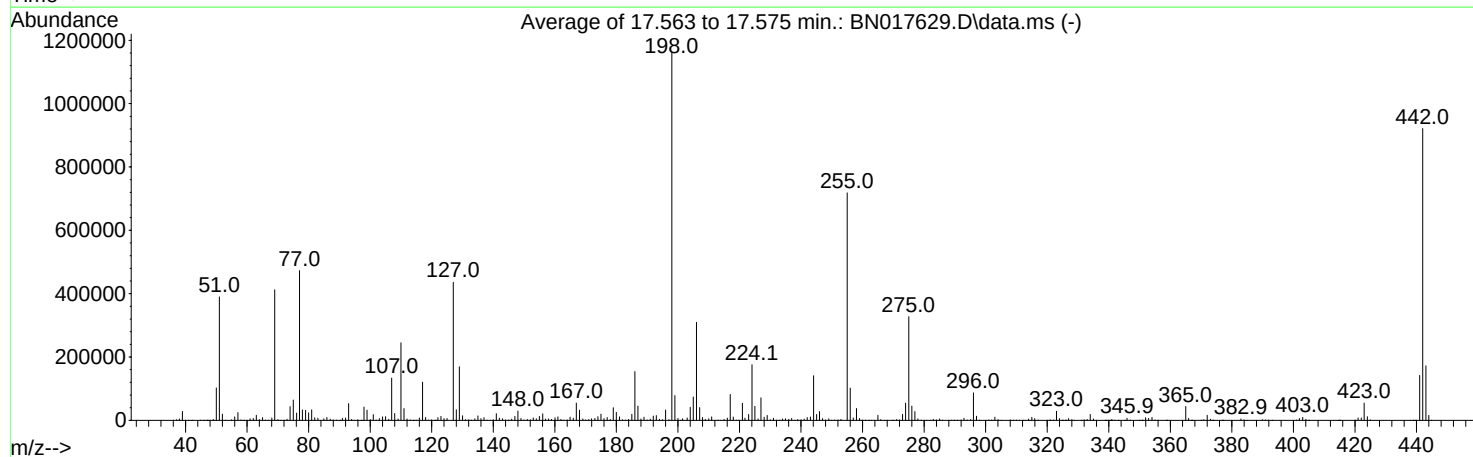


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113021\
 Data File : BN017629.D
 Acq On : 01 Dec 2021 02:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN113021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 02 01:51:49 2021

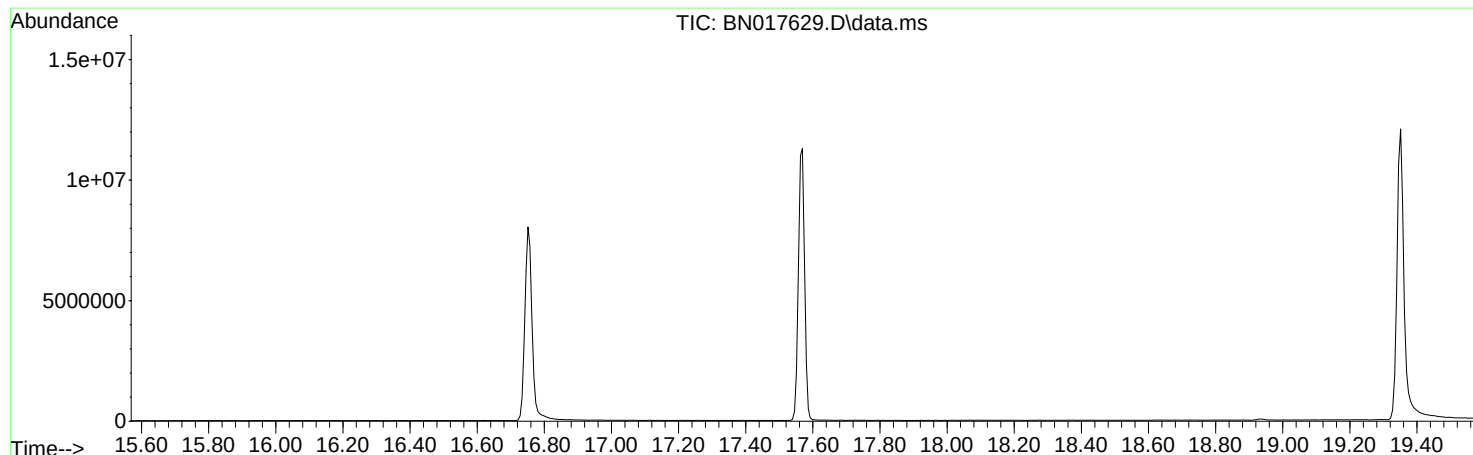

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	390222	PASS
68	69	0.00	2	1.9	7681	PASS
69	198	0.00	100	35.5	412086	PASS
70	69	0.00	2	0.6	2371	PASS
127	198	10	80	37.6	436181	PASS
197	198	0.00	2	0.2	1826	PASS
198	198	100	100	100.0	1161408	PASS
199	198	5	9	6.7	78229	PASS
275	198	10	60	28.2	327211	PASS
365	198	1	100	3.8	43875	PASS
441	198	0.01	100	12.2	142184	PASS
442	442	50	100	100.0	921387	PASS
443	442	15	24	18.7	172523	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/30/2021	BNA_N	<u>BN017629.D</u>
Compound Name	Response	Retention Time
DDT	3474147	20.592
DDD	64655	20.151
DDE	847	19.645
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
65502	3539649	1.85

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113021\
Data File : BN017629.D
Acq On : 01 Dec 2021 02:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 01 03:42:16 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 01 03:42:11 2021
Response via : Initial Calibration

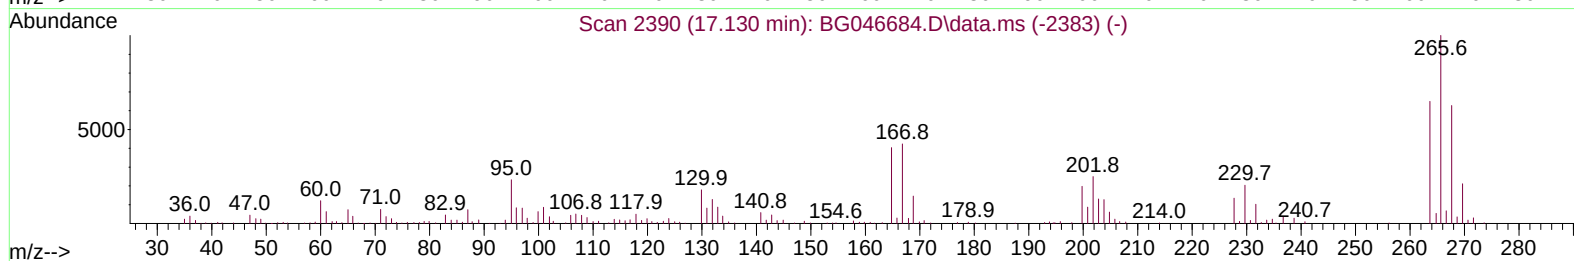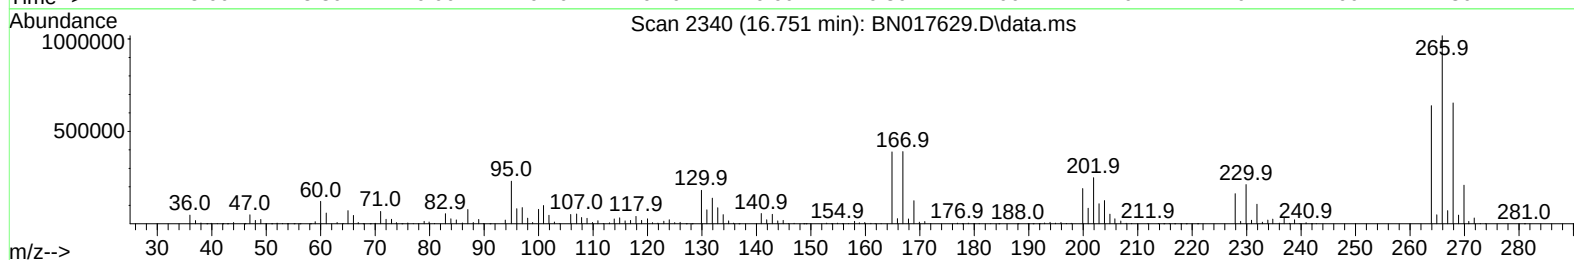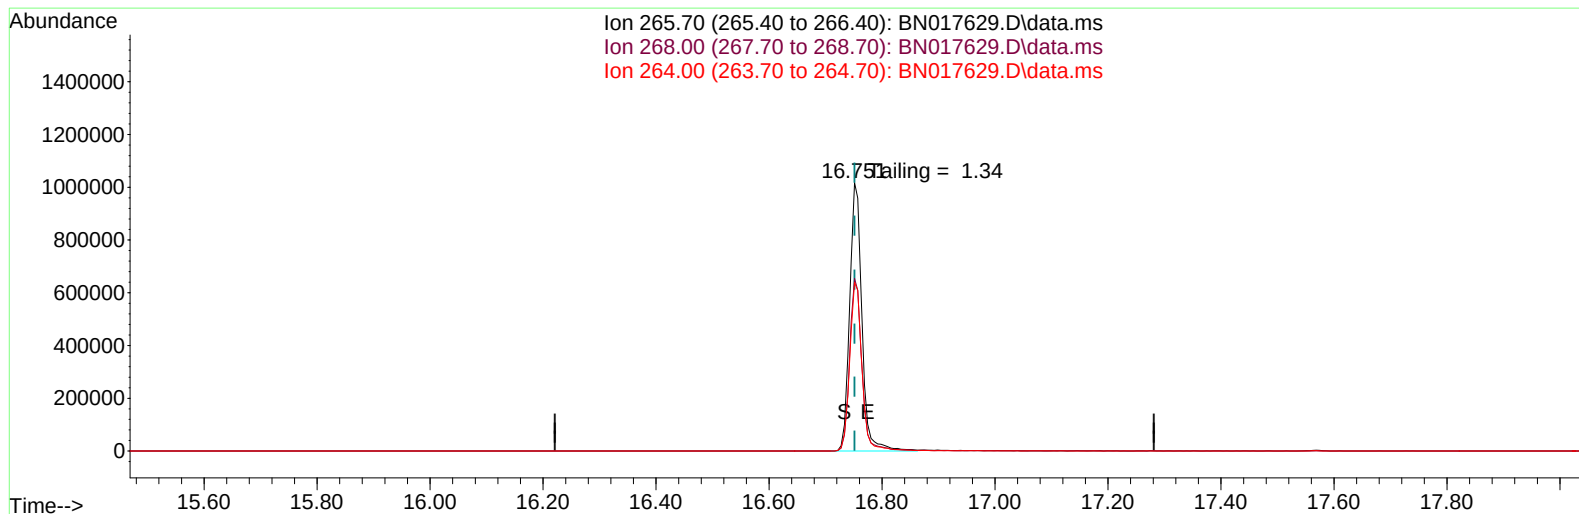

TIC: BN017629.D\data.ms

(70) Pentachlorophenol (C)

16.751min (0.000) 28297.31 ng




response 1538724

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.26
264.00	61.60	62.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113021\
 Data File : BN017629.D
 Acq On : 01 Dec 2021 02:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 01 03:42:16 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 01 03:42:11 2021
 Response via : Initial Calibration

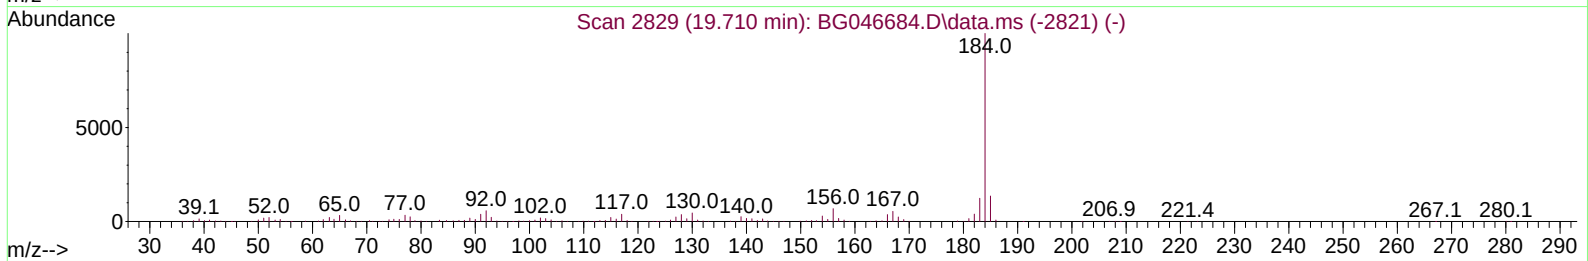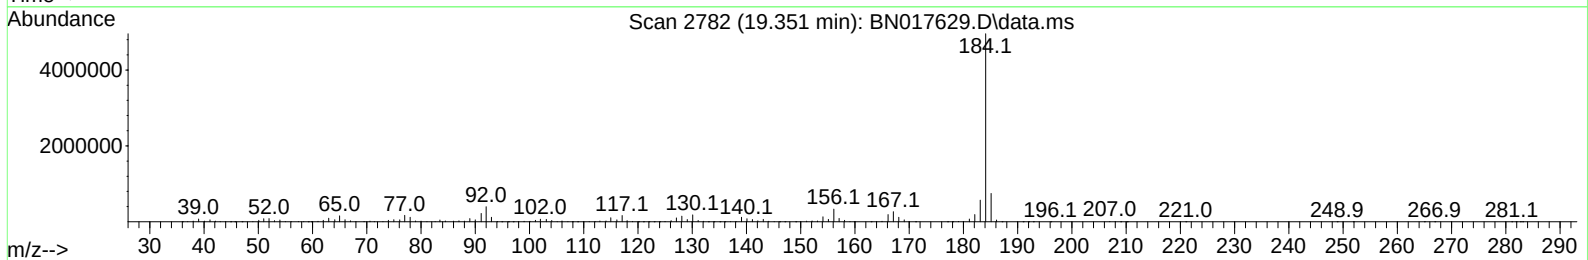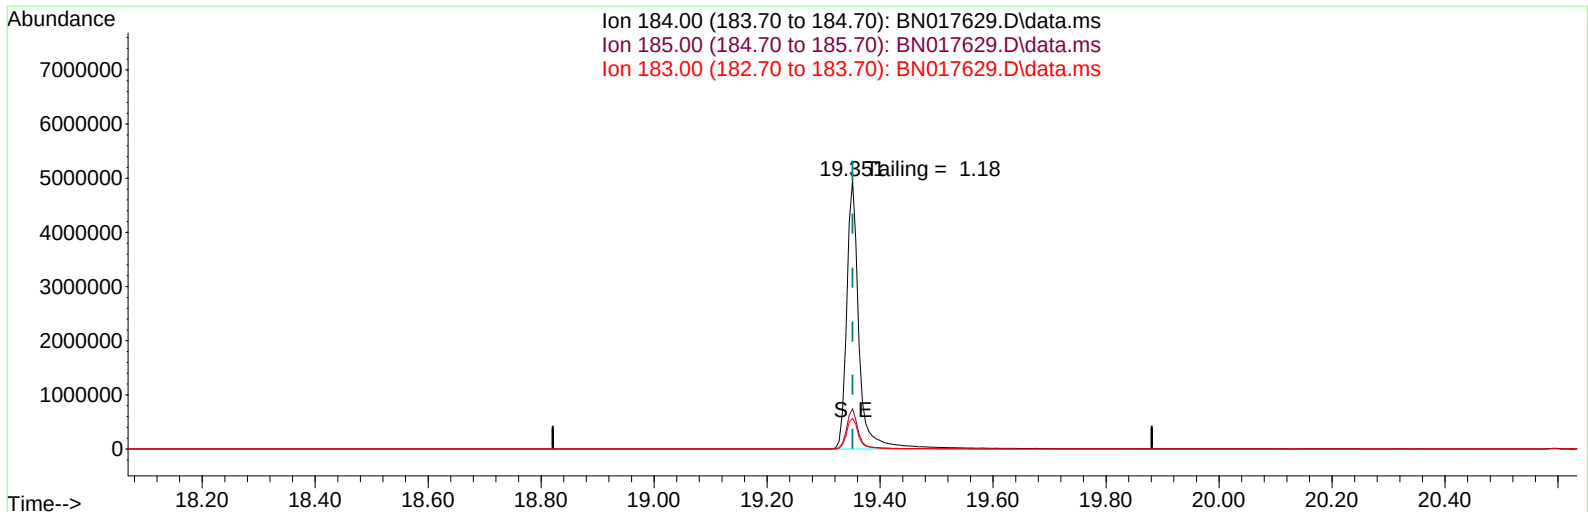

TIC: BN017629.D\data.ms

(77) Benzidine

19.351min (0.000) 2156831.75 ng

response 7579306

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.04
183.00	13.20	11.48
0.00	0.00	0.00