

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113023\
 Data File : BN028948.D
 Acq On : 01 Dec 2023 15:29
 Operator : MA/JU
 Sample : 05350-10
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 01 16:20:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN113023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 01 00:28:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.797	152	4421	0.400	ng	-0.01
7) Naphthalene-d8	10.584	136	11643	0.400	ng	-0.01
13) Acenaphthene-d10	14.428	164	4844	0.400	ng	0.00
19) Phenanthrene-d10	17.171	188	7593	0.400	ng	-0.01
29) Chrysene-d12	21.374	240	5005	0.400	ng	# 0.00
35) Perylene-d12	23.708	264	4920	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.420	112	2165	0.162	ng	-0.03
5) Phenol-d6	7.017	99	1428	0.096	ng	-0.03
8) Nitrobenzene-d5	8.971	82	3386	0.293	ng	-0.01
11) 2-Methylnaphthalene-d10	12.174	152	5352	0.286	ng	-0.01
14) 2,4,6-Tribromophenol	15.918	330	626	0.191	ng	-0.01
15) 2-Fluorobiphenyl	13.060	172	9435	0.451	ng	-0.01
27) Fluoranthene-d10	19.209	212	7321	0.367	ng	0.00
31) Terphenyl-d14	19.817	244	6018	0.414	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.340	88	29300	6.767	ng	95
3) n-Nitrosodimethylamine	3.767	42	130	0.110	ng	# 36
6) bis(2-Chloroethyl)ether	7.255	93	546	0.044	ng	91
16) Acenaphthylene	14.140	152	6254	0.244	ng	96
17) Acenaphthene	14.482	154	756	0.044	ng	94
18) Fluorene	15.497	166	852	0.040	ng	# 11
30) Pyrene	19.604	202	767	0.114	ng	# 80
32) Benzo(a)anthracene	21.356	228	552	0.026	ng	# 1
33) Chrysene	21.409	228	736	0.035	ng	# 1
34) Bis(2-ethylhexyl)phtha...	21.302	149	1277	Below Cal		# 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113023\
Data File : BN028948.D
Acq On : 01 Dec 2023 15:29
Operator : MA/JU
Sample : 05350-10
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Dec 01 16:20:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN113023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 00:28:34 2023
Response via : Initial Calibration

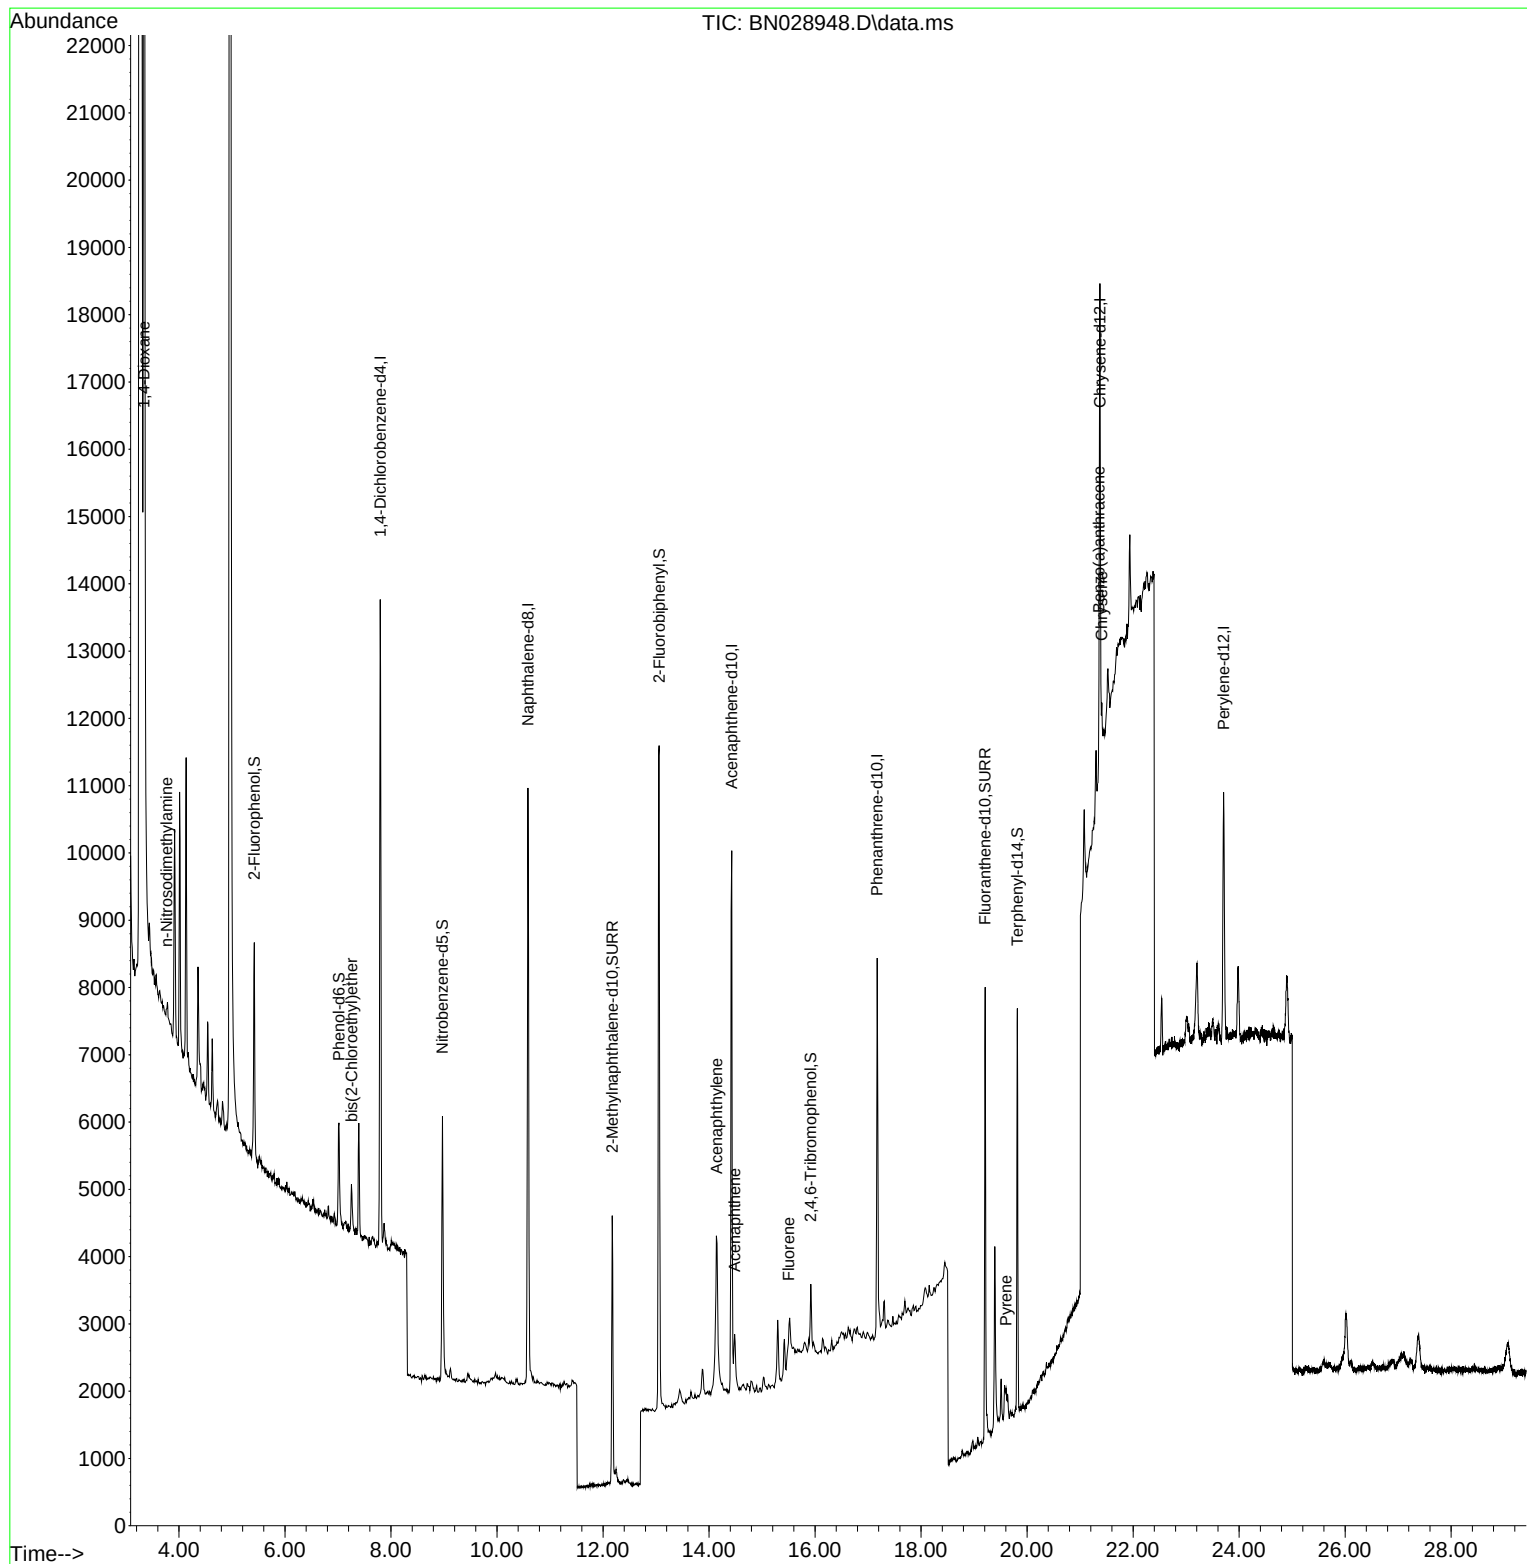






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.797 min Scan# 61
 Delta R.T. -0.014 min
 Lab File: BN028948.D
 Acq: 01 Dec 2023 15:29


Instrument :
 BNA_N
 ClientSampleId :

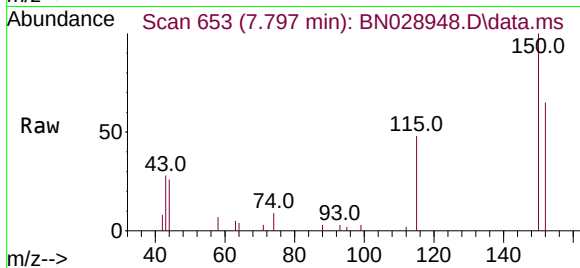



Tgt Ion:152 Resp: 4421
 Ion Ratio Lower Upper
 152 100
 150 155.0 123.4 185.2
 115 74.0 59.1 88.7

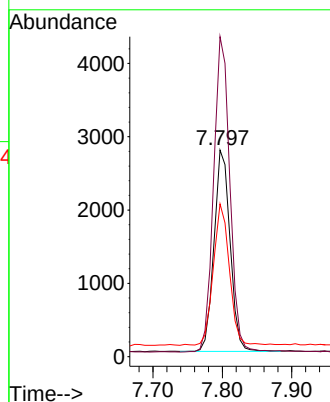


#2
 1,4-Dioxane
 Concen: 6.767 ng
 RT: 3.340 min Scan# 36
 Delta R.T. -0.036 min
 Lab File: BN028948.D
 Acq: 01 Dec 2023 15:29

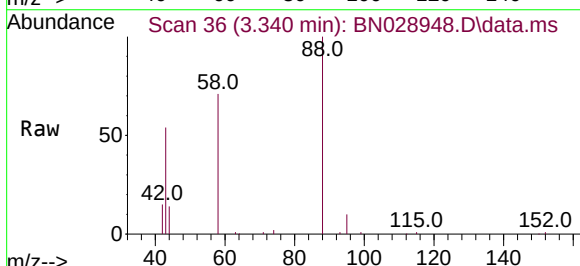

Tgt Ion: 88 Resp: 29300
 Ion Ratio Lower Upper
 88 100
 43 42.5 29.9 44.9
 58 71.8 55.0 82.4



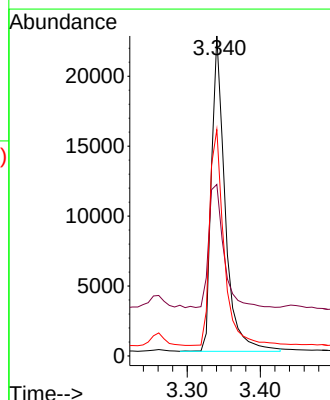
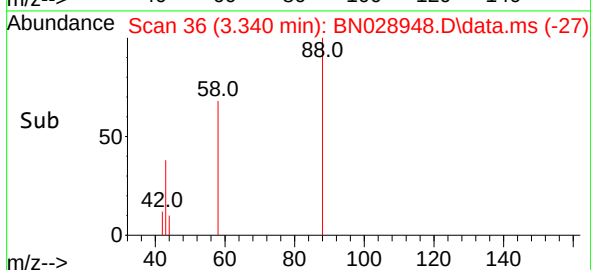




#3
n-Nitrosodimethylamine
Concen: 0.110 ng
RT: 3.767 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN028948.D
Acq: 01 Dec 2023 15:29




Instrument :
BNA_N
ClientSampleId :


Tgt Ion: 42 Resp: 130
Ion Ratio Lower Upper
42 100
74 18.5 57.0 85.6#
44 0.0 0.0 0.0

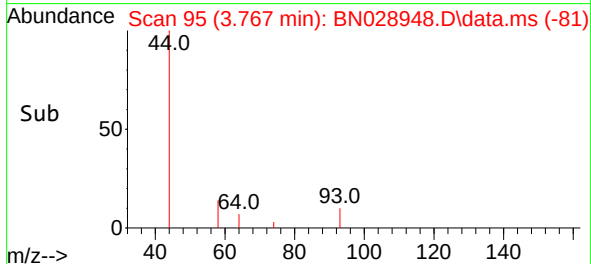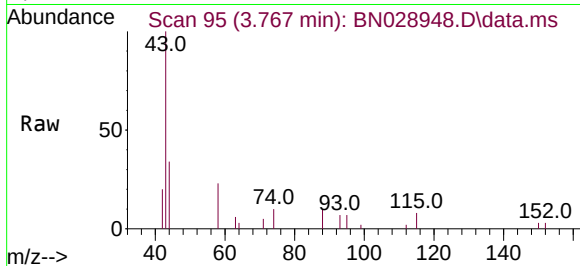

#4
2-Fluorophenol
Concen: 0.162 ng
RT: 5.420 min Scan# 324
Delta R.T. -0.029 min
Lab File: BN028948.D
Acq: 01 Dec 2023 15:29

Tgt Ion: 112 Resp: 2165
Ion Ratio Lower Upper
112 100
64 66.8 51.5 77.3
63 42.7 30.4 45.6


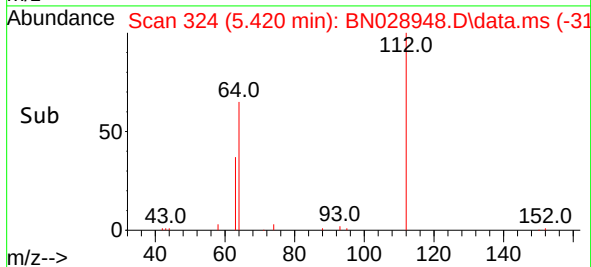

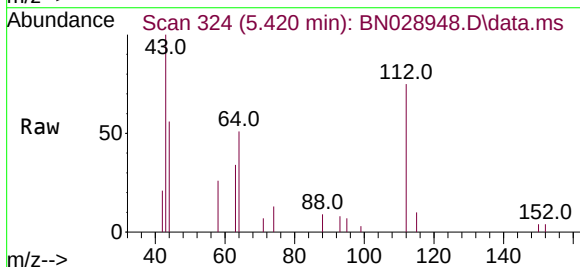




#5
Phenol-d6
Concen: 0.096 ng
RT: 7.017 min Scan# 54
Delta R.T. -0.029 min
Lab File: BN028948.D
Acq: 01 Dec 2023 15:29




Instrument :
BNA_N
ClientSampleId :


Tgt Ion: 99 Resp: 1428
Ion Ratio Lower Upper
99 100
42 29.5 21.2 31.8
71 41.6 35.4 53.0

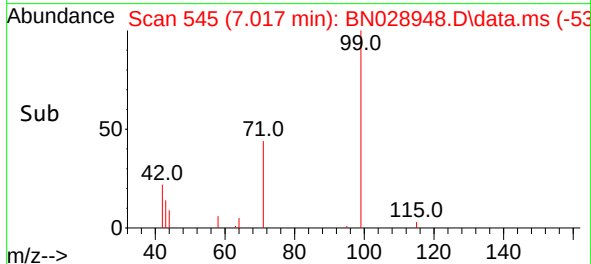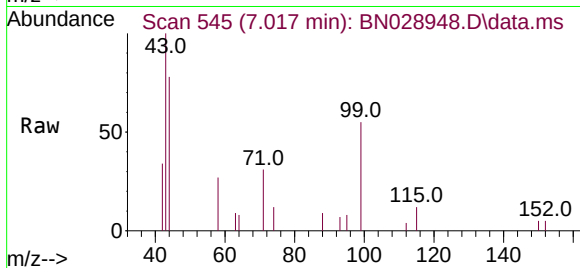

#6
bis(2-Chloroethyl)ether
Concen: 0.044 ng
RT: 7.255 min Scan# 578
Delta R.T. -0.022 min
Lab File: BN028948.D
Acq: 01 Dec 2023 15:29

Tgt Ion: 93 Resp: 546
Ion Ratio Lower Upper
93 100
63 94.0 66.9 100.3
95 34.2 28.2 42.4


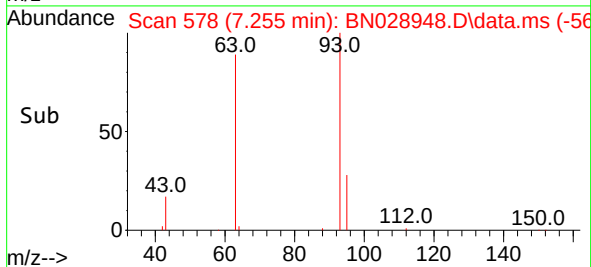

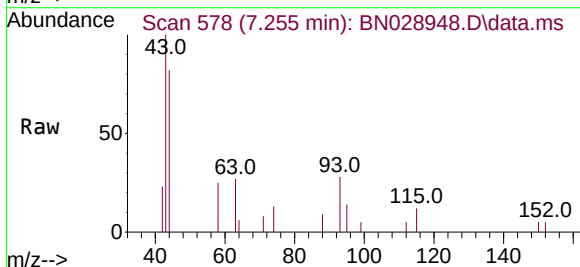




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.584 min Scan# 91
Delta R.T. -0.011 min
Lab File: BN028948.D
Acq: 01 Dec 2023 15:29




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:	136	Resp:	11643
Ion	Ratio	Lower	Upper
136	100		
137	11.7	10.6	16.0
54	10.5	7.5	11.3
68	6.6	5.9	8.9

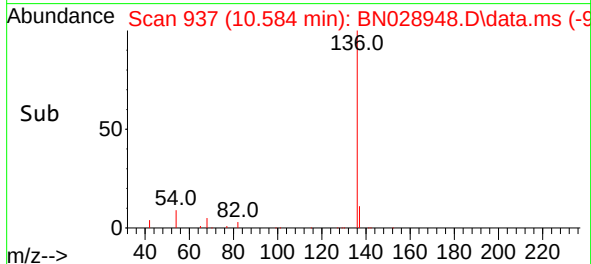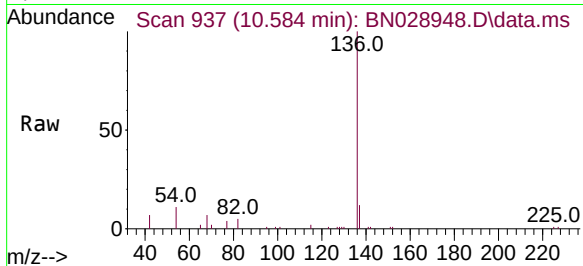

#8
Nitrobenzene-d5
Concen: 0.293 ng
RT: 8.971 min Scan# 786
Delta R.T. -0.011 min
Lab File: BN028948.D
Acq: 01 Dec 2023 15:29

Tgt Ion:	82	Resp:	3386
Ion	Ratio	Lower	Upper
82	100		
128	37.0	29.2	43.8
54	60.0	47.0	70.6

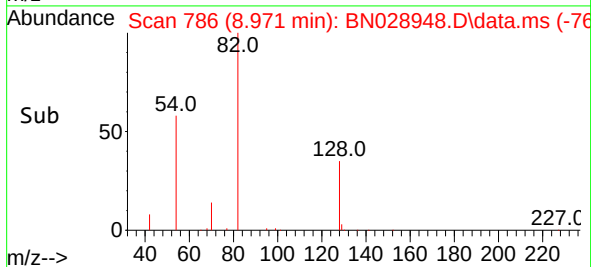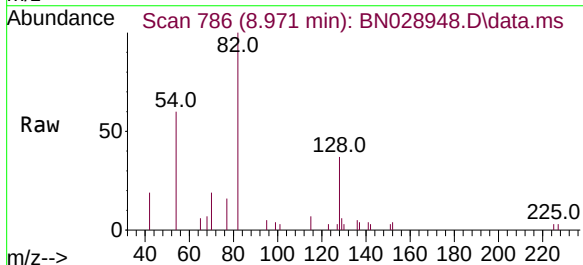



#11

2-Methylnaphthalene-d10

Concen: 0.286 ng

RT: 12.174 min Scan# 11

Delta R.T. -0.011 min

Lab File: BN028948.D

Acq: 01 Dec 2023 15:29

Instrument :

BNA_N





ClientSampleId :

Tgt Ion:152 Resp: 5352

Ion Ratio Lower Upper

152 100

151 20.6 16.7 25.1

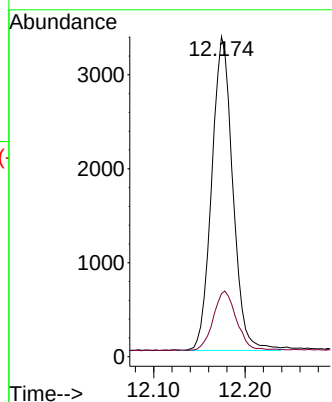

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.428 min Scan# 1501

Delta R.T. -0.000 min

Lab File: BN028948.D

Acq: 01 Dec 2023 15:29




Tgt Ion:164 Resp: 4844


Ion Ratio Lower Upper

164 100

162 108.3 81.7 122.5


160 47.8 37.0 55.6

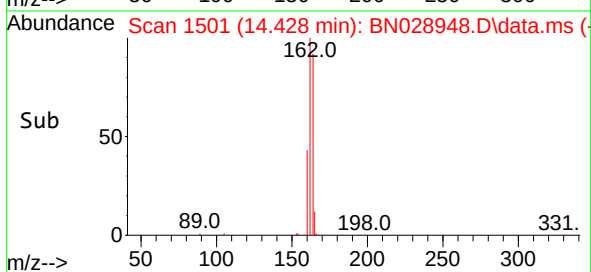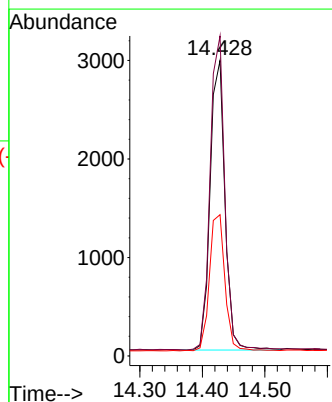






#14
2,4,6-Tribromophenol
Concen: 0.191 ng
RT: 15.918 min Scan# 1635
Delta R.T. -0.012 min
Lab File: BN028948.D
Acq: 01 Dec 2023 15:29

Instrument :
BNA_N
ClientSampleId :







Tgt Ion:330 Resp: 626
Ion Ratio Lower Upper
330 100
332 95.0 75.4 113.2
141 45.2 35.7 53.5

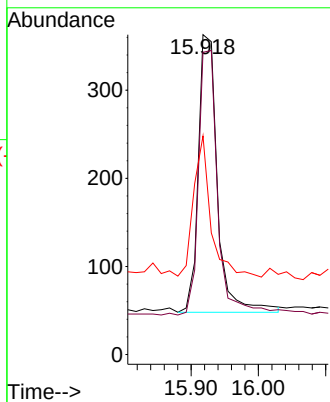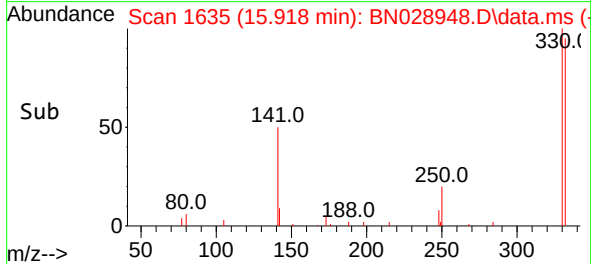

#15
2-Fluorobiphenyl
Concen: 0.451 ng
RT: 13.060 min Scan# 1373
Delta R.T. -0.011 min
Lab File: BN028948.D
Acq: 01 Dec 2023 15:29

Tgt Ion:172 Resp: 9435
Ion Ratio Lower Upper
172 100
171 35.8 29.0 43.4
170 23.7 19.7 29.5

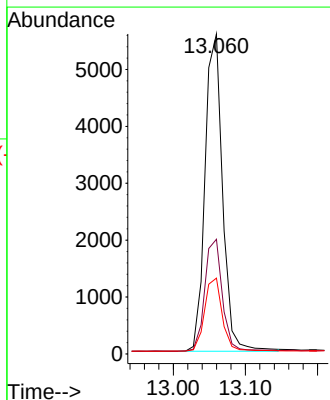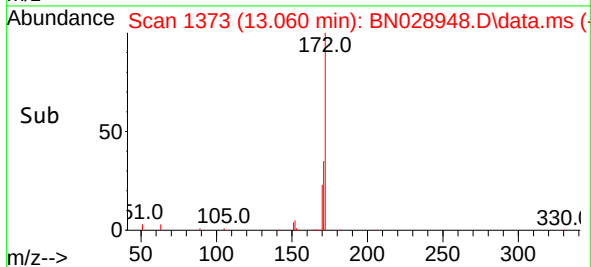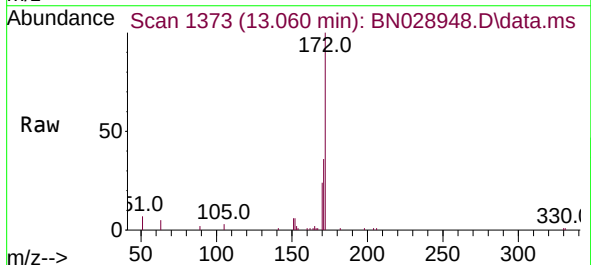



#16

Acenaphthylene

Concen: 0.244 ng

RT: 14.140 min Scan# 1477

Delta R.T. -0.011 min

Lab File: BN028948.D

Acq: 01 Dec 2023 15:29

Instrument :

BNA_N

ClientSampleId :





Tgt Ion:152 Resp: 6254

Ion Ratio Lower Upper

152 100

151 18.2 15.9 23.9

153 12.0 10.8 16.2

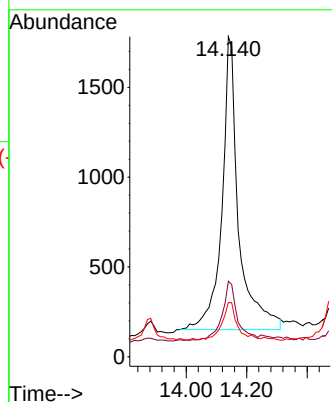

#17

Acenaphthene

Concen: 0.044 ng

RT: 14.482 min Scan# 1506

Delta R.T. -0.011 min

Lab File: BN028948.D

Acq: 01 Dec 2023 15:29




Tgt Ion:154 Resp: 756


Ion Ratio Lower Upper

154 100

153 106.7 93.8 140.6

152 55.6 44.5 66.7


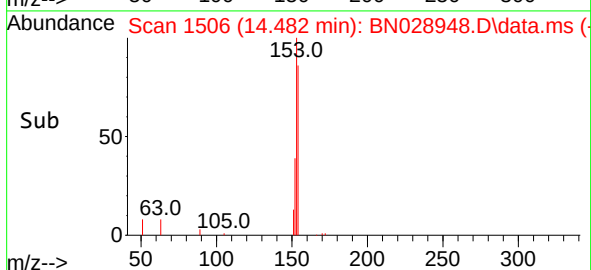
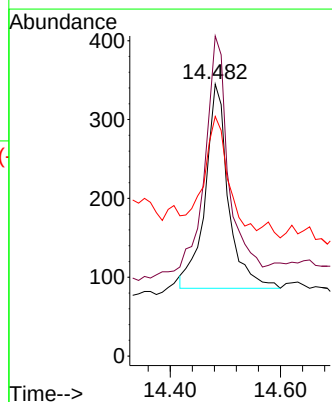





#18
 Fluorene
 Concen: 0.040 ng
 RT: 15.497 min Scan# 1601
 Delta R.T. 0.011 min
 Lab File: BN028948.D
 Acq: 01 Dec 2023 15:29




Instrument :
 BNA_N
 ClientSampleId :


Tgt Ion:166 Resp: 852
 Ion Ratio Lower Upper
 166 100
 165 0.0 79.4 119.2#
 167 10.3 11.0 16.4#

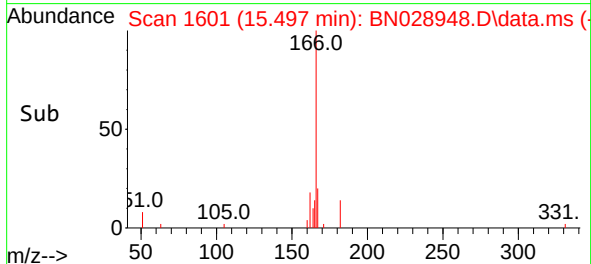

#19
 Phenanthrene-d10
 Concen: 0.400 ng
 RT: 17.171 min Scan# 1736
 Delta R.T. -0.012 min
 Lab File: BN028948.D
 Acq: 01 Dec 2023 15:29

Tgt Ion:188 Resp: 7593
 Ion Ratio Lower Upper
 188 100
 94 0.0 0.0 0.0
 80 13.2 9.0 13.6


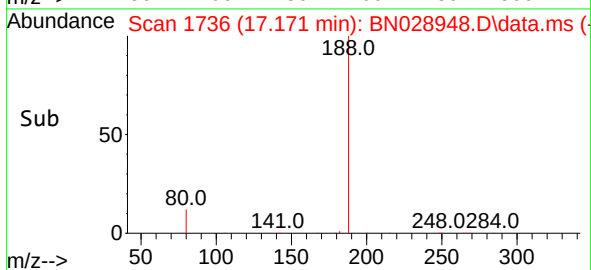

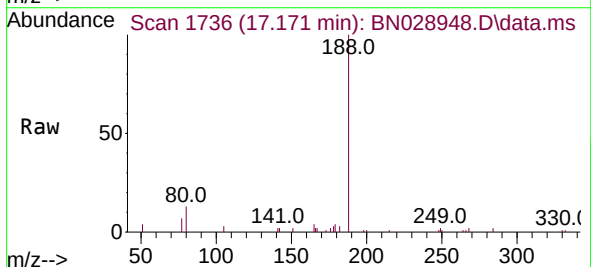


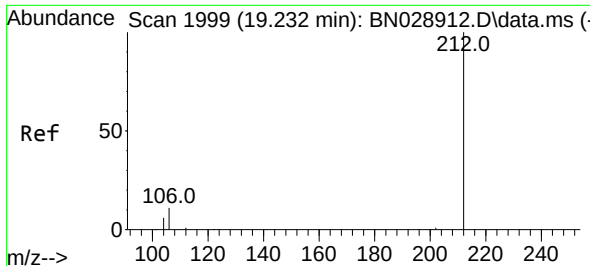

#27
Fluoranthene-d10
Concen: 0.367 ng
RT: 19.209 min Scan# 1994
Delta R.T. -0.005 min
Lab File: BN028948.D
Acq: 01 Dec 2023 15:29




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:212 Resp: 7321
Ion Ratio Lower Upper
212 100
106 13.7 9.4 14.2
104 8.3 6.2 9.2

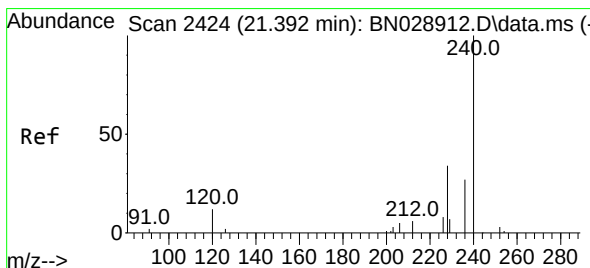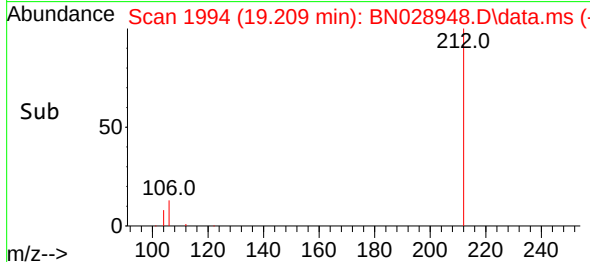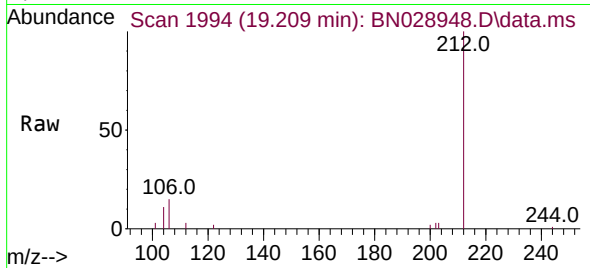

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.374 min Scan# 2422
Delta R.T. -0.000 min
Lab File: BN028948.D
Acq: 01 Dec 2023 15:29

Tgt Ion:240 Resp: 5005
Ion Ratio Lower Upper
240 100
120 22.3 37.1 55.7#
236 32.9 32.4 48.6


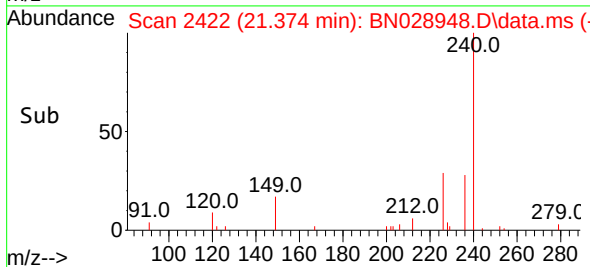

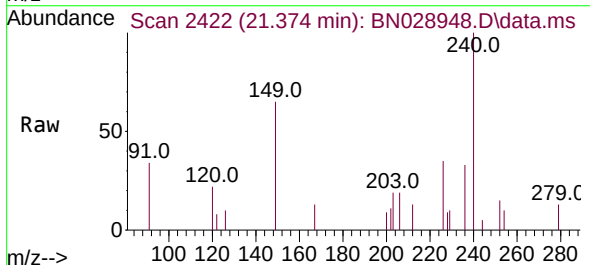




#30
Pyrene
Concen: 0.114 ng
RT: 19.604 min Scan# 2083
Delta R.T. -0.005 min
Lab File: BN028948.D
Acq: 01 Dec 2023 15:29




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:202 Resp: 767
Ion Ratio Lower Upper
202 100
200 21.4 16.9 25.3
203 0.0 14.8 22.2#

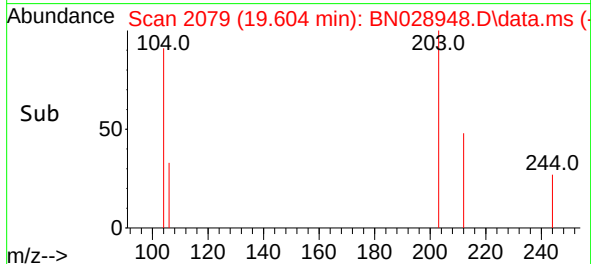

#31
Terphenyl-d14
Concen: 0.414 ng
RT: 19.817 min Scan# 2125
Delta R.T. -0.005 min
Lab File: BN028948.D
Acq: 01 Dec 2023 15:29


Tgt Ion:244 Resp: 6018
Ion Ratio Lower Upper
244 100
212 11.7 11.5 17.3
122 14.7 13.2 19.8

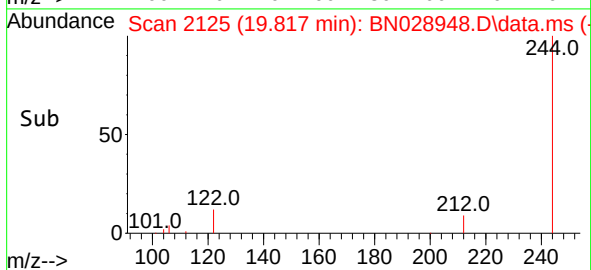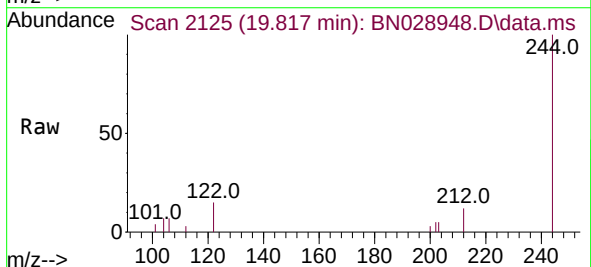



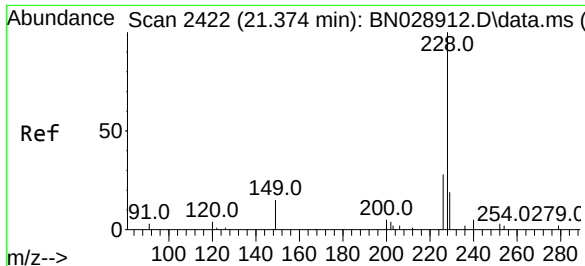


#32
Benzo(a)anthracene
Concen: 0.026 ng
RT: 21.356 min Scan# 2420
Delta R.T. 0.000 min
Lab File: BN028948.D
Acq: 01 Dec 2023 15:29


Instrument :
BNA_N
ClientSampleId :

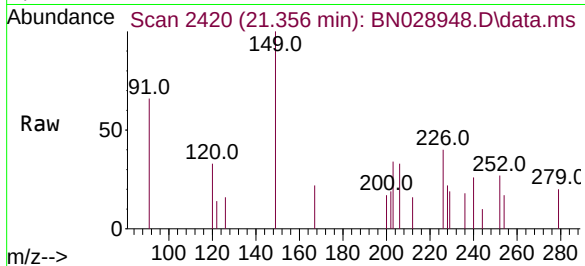



Tgt Ion:228 Resp: 552
Ion Ratio Lower Upper
228 100
226 180.4 26.5 39.7#
229 86.3 16.4 24.6#

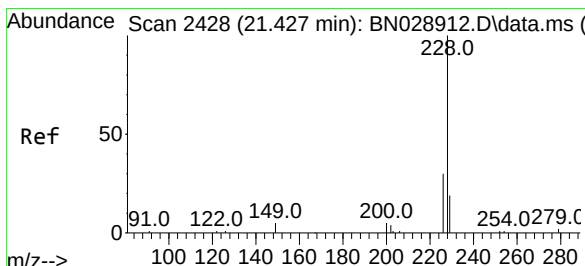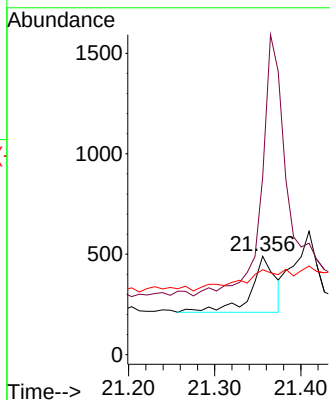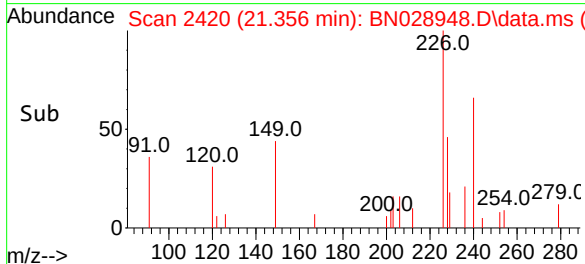


#33
Chrysene
Concen: 0.035 ng
RT: 21.409 min Scan# 2426
Delta R.T. -0.000 min
Lab File: BN028948.D
Acq: 01 Dec 2023 15:29

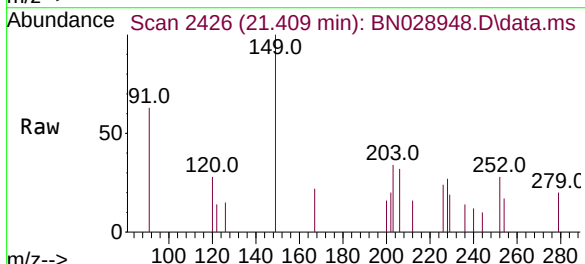

Tgt Ion:228 Resp: 736
Ion Ratio Lower Upper
228 100
226 90.4 28.3 42.5#
229 71.8 16.4 24.6#

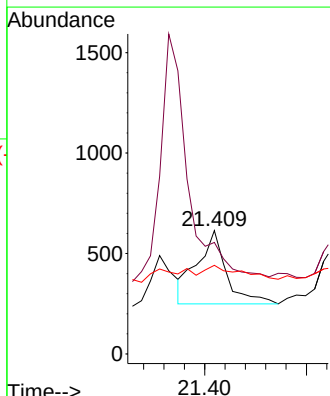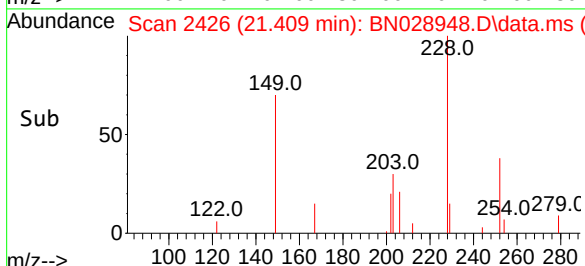

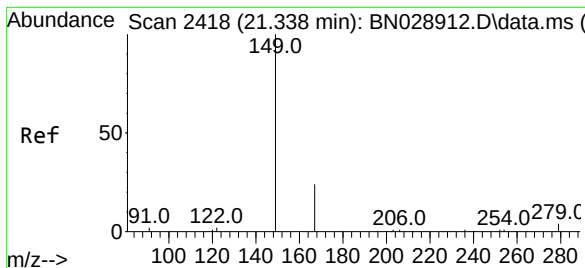

#34

Bis(2-ethylhexyl)phthalate

Concen: Below Cal

RT: 21.302 min Scan# 2414

Delta R.T. -0.009 min


Lab File: BN028948.D

Acq: 01 Dec 2023 15:29

Instrument :

BNA_N

ClientSampleId :

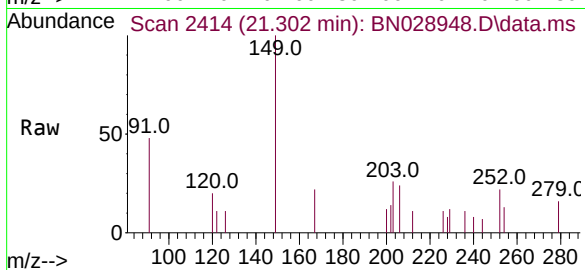




Tgt Ion:149 Resp: 1277

Ion Ratio Lower Upper

149 100

167 27.5 14.9 22.3#

279 10.3 6.3 9.5#

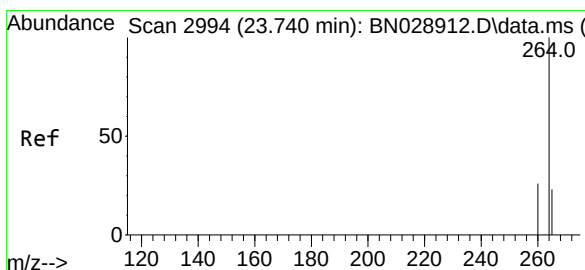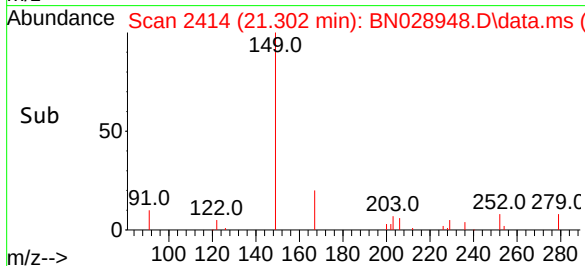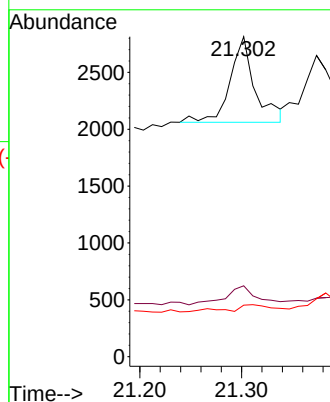

#35

Perylene-d12

Concen: 0.400 ng

RT: 23.708 min Scan# 2983

Delta R.T. -0.006 min

Lab File: BN028948.D

Acq: 01 Dec 2023 15:29

Tgt Ion:264 Resp: 4920

Ion Ratio Lower Upper

264 100

260 31.2 20.6 30.8#

265 136.6 464.5 696.7#

