
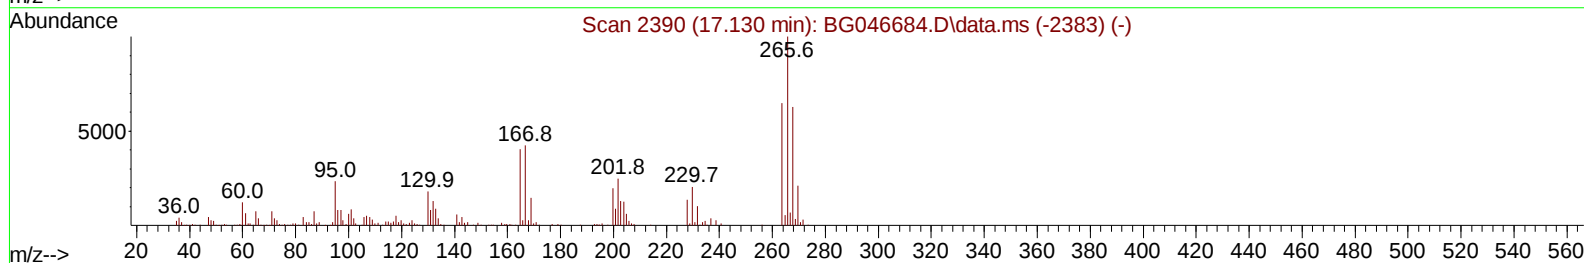
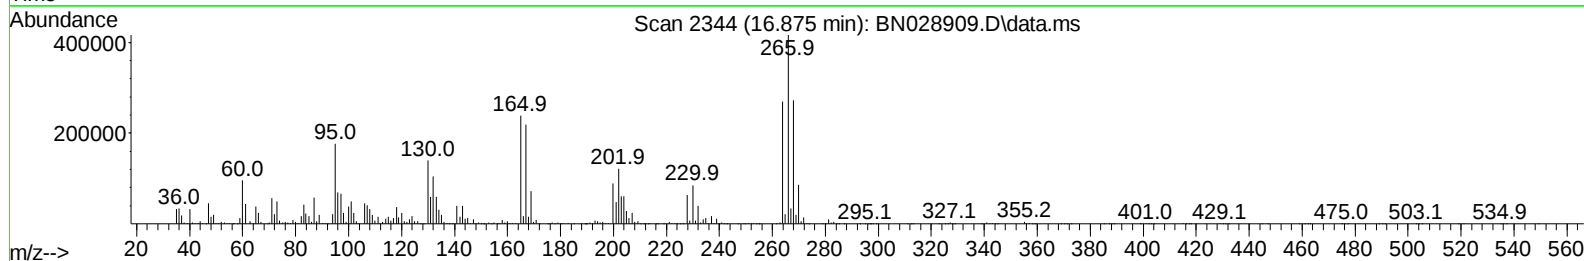


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113023\
Data File : BN028909.D
Acq On : 30 Nov 2023 13:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 04:55:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 04:55:41 2023
Response via : Initial Calibration

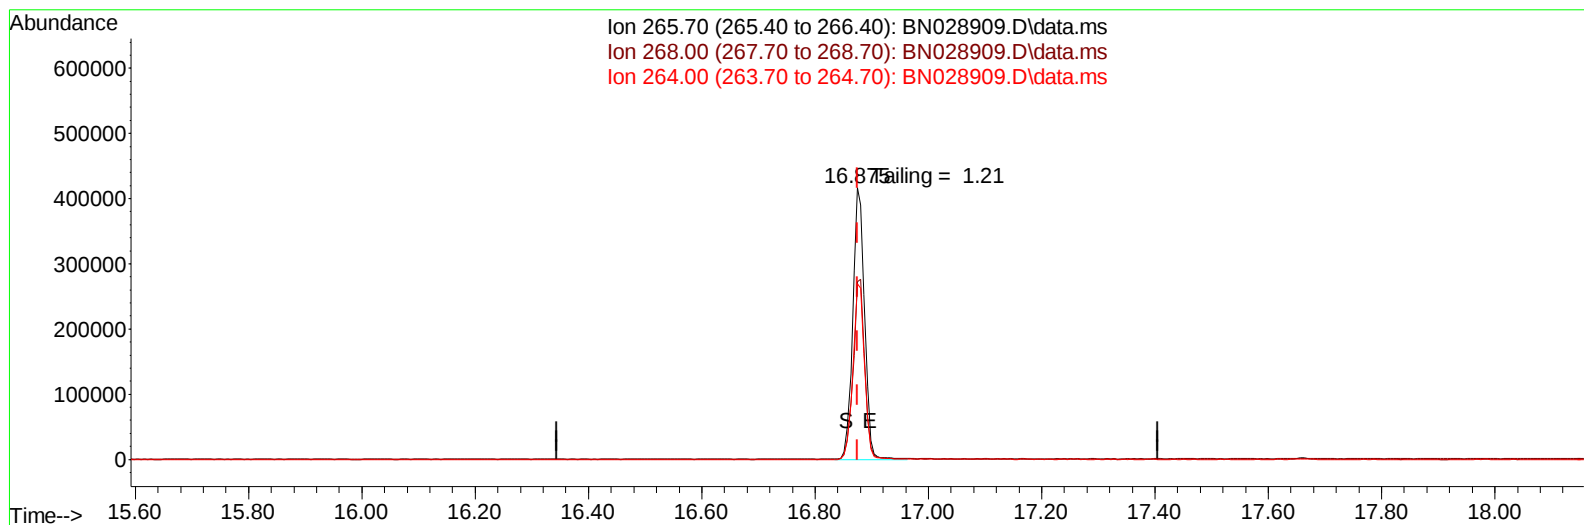




TIC: BN028909.D\data.ms

(70) Pentachlorophenol (C)**16.875min (0.000) 16800.02 ng****response 605288**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.46
264.00	61.60	64.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113023\
Data File : BN028909.D
Acq On : 30 Nov 2023 13:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 04:55:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 04:55:41 2023
Response via : Initial Calibration

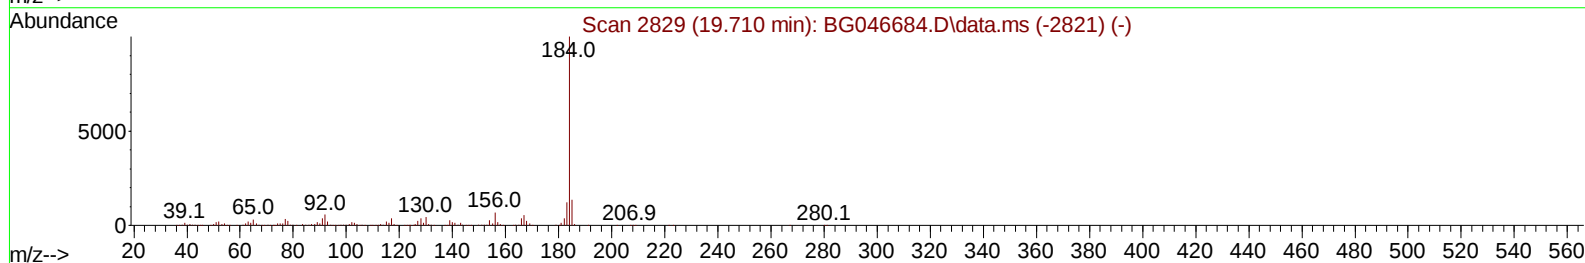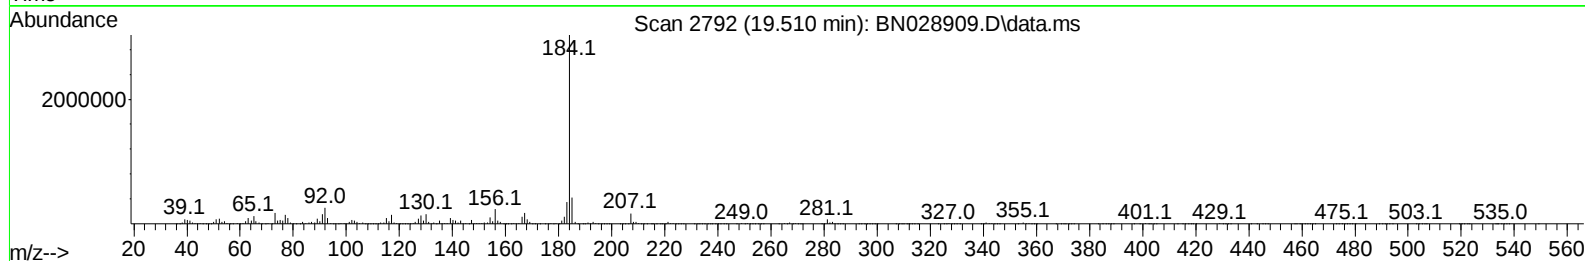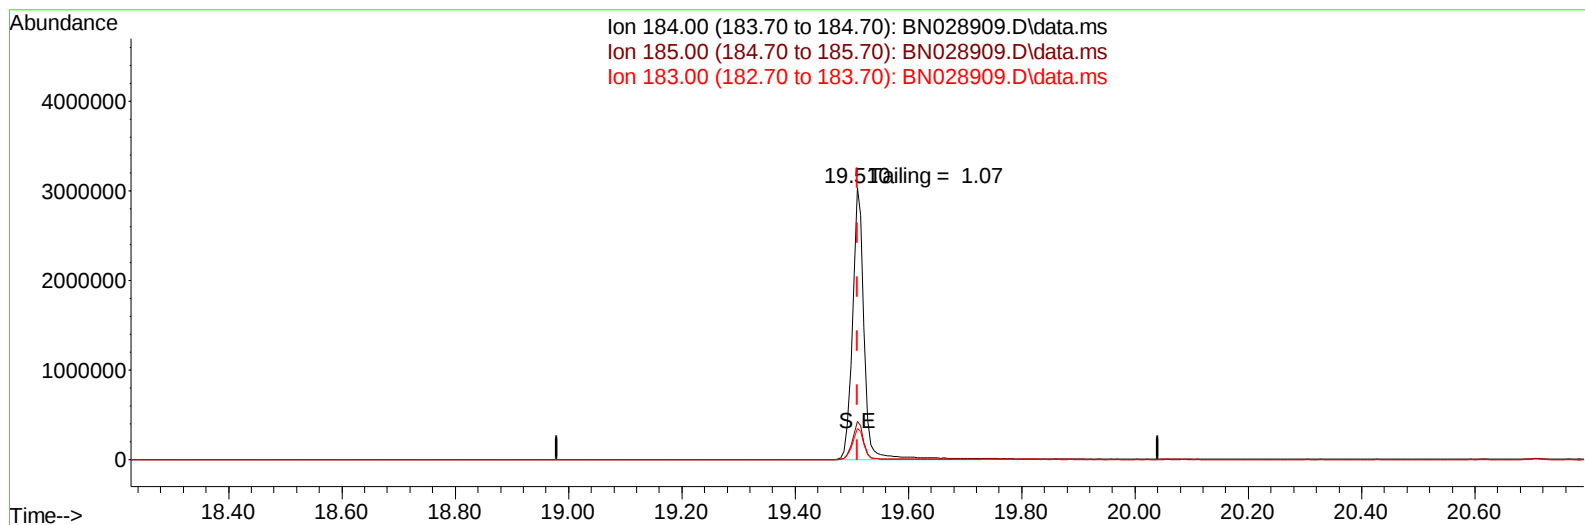

TIC: BN028909.D\data.ms

(77) Benzidine**19.510min (0.000) 210476.21 ng****response 4372917**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.98
183.00	13.20	11.50
0.00	0.00	0.00