
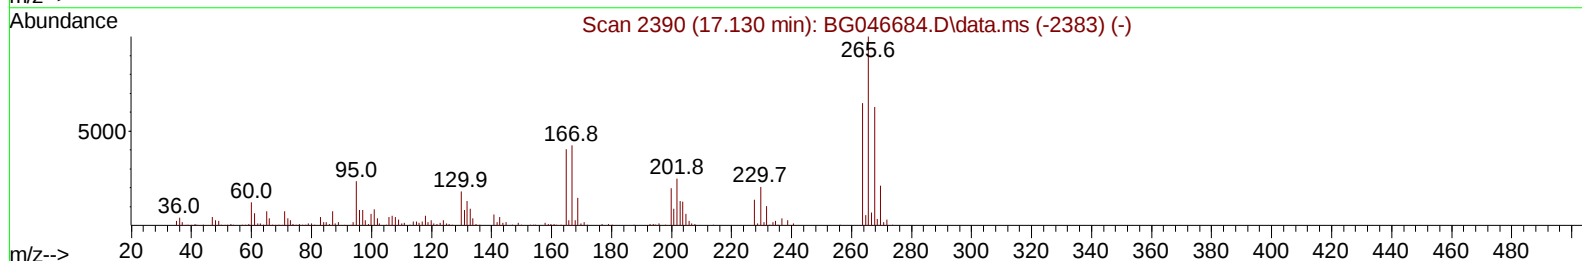
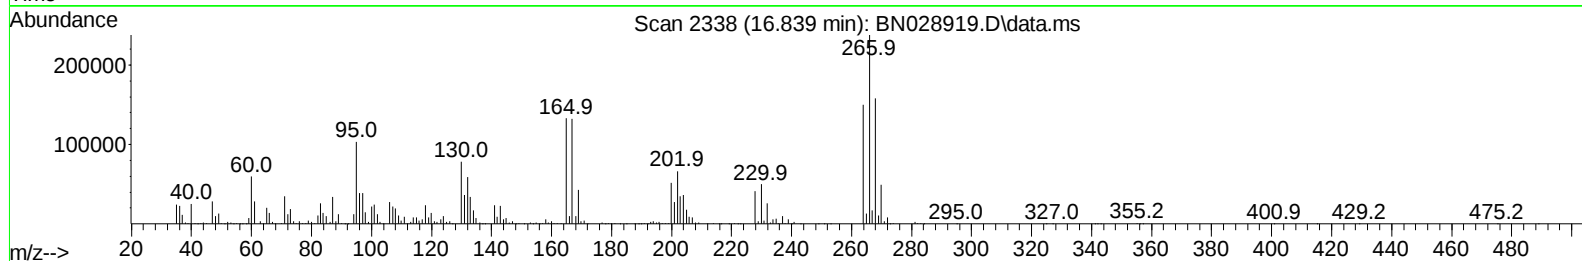


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN113023\  
Data File : BN028919.D  
Acq On : 30 Nov 2023 21:00  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 04:56:58 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 01 04:55:41 2023  
Response via : Initial Calibration

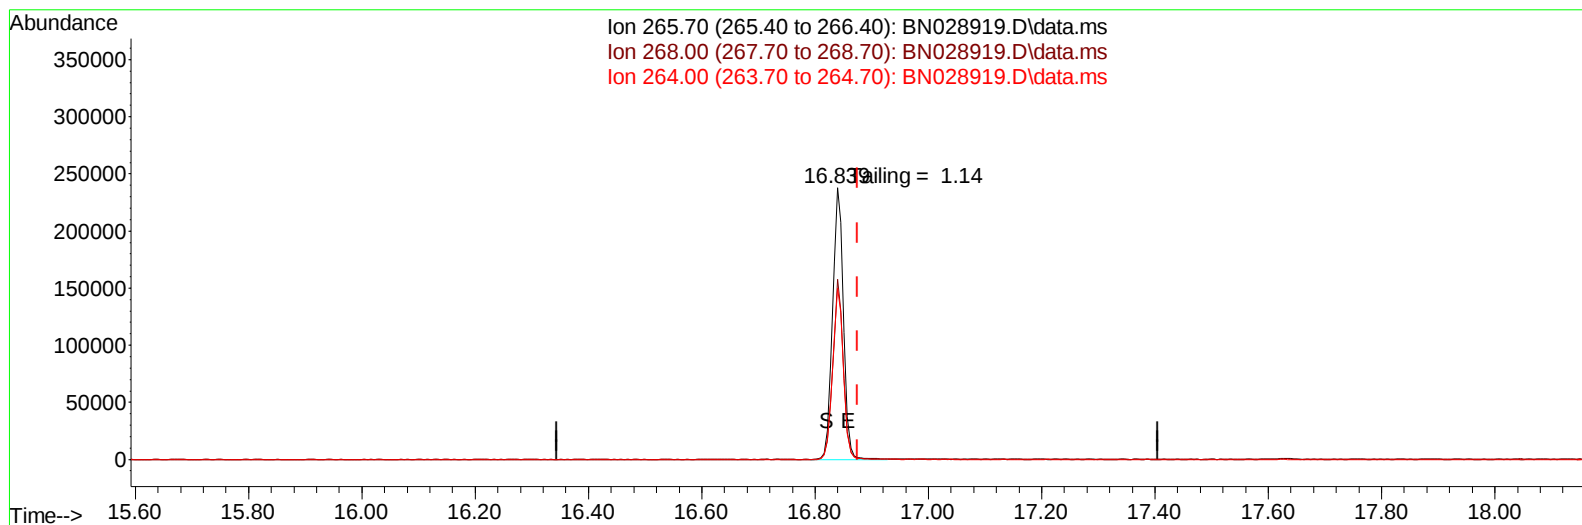

TIC: BN028919.D\data.ms




**(70) Pentachlorophenol (C)**

**16.839min (-0.035) 14927.33 ng**

**response 319574**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 66.42  |
| 264.00 | 61.60  | 63.03  |
| 0.00   | 0.00   | 0.00   |

Quant Time: Dec 01 04:56:58 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 01 04:55:41 2023  
Response via : Initial Calibration

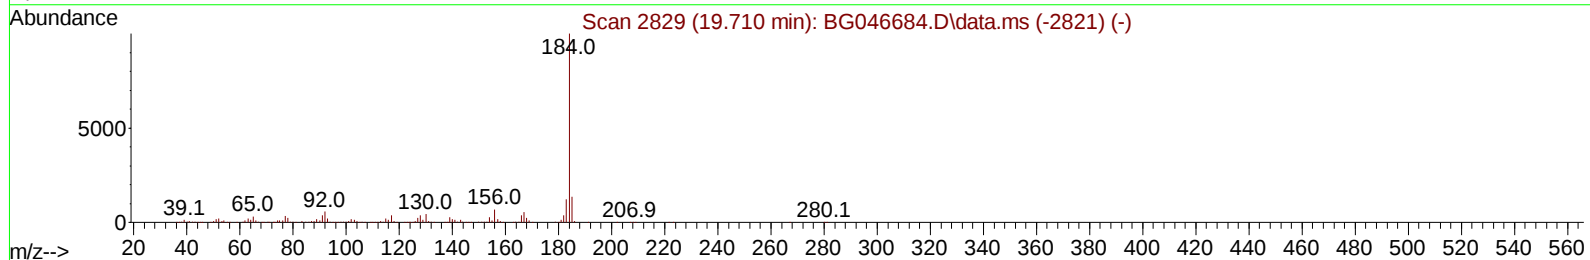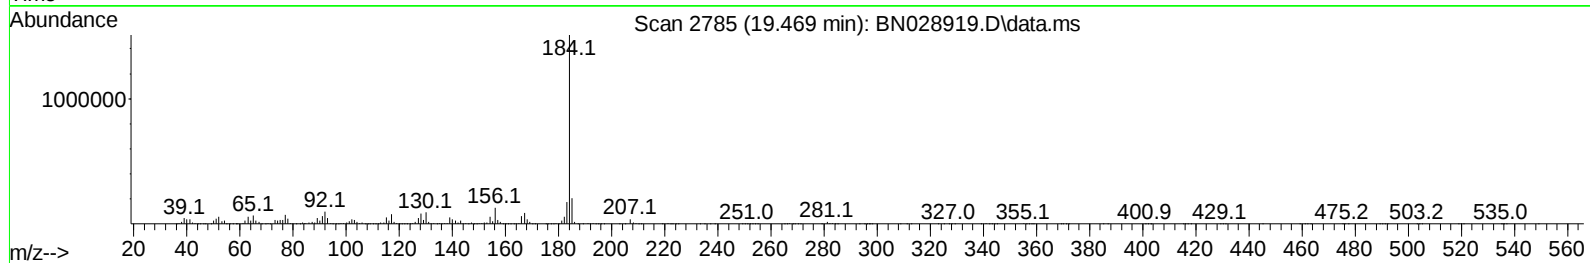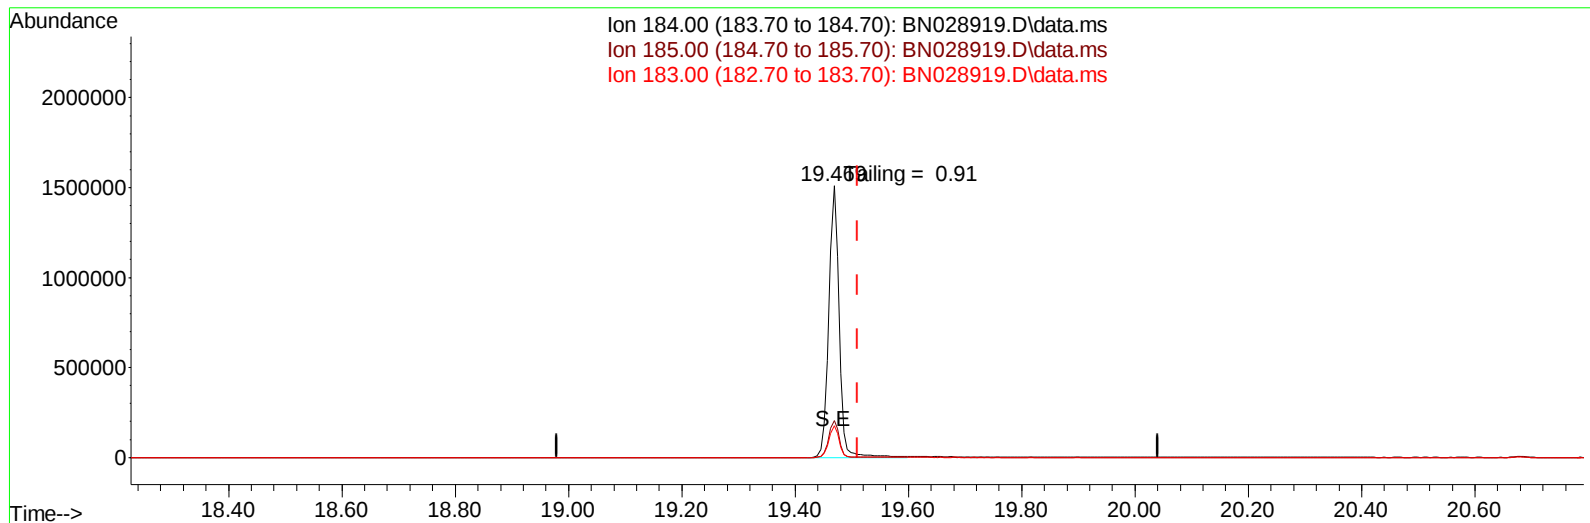

TIC: BN028919.D\data.ms

(77) Benzidine

19.469min (-0.041) 213520.04 ng

**response**      **1908732**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.49  |
| 183.00 | 13.20  | 11.69  |
| 0.00   | 0.00   | 0.00   |