
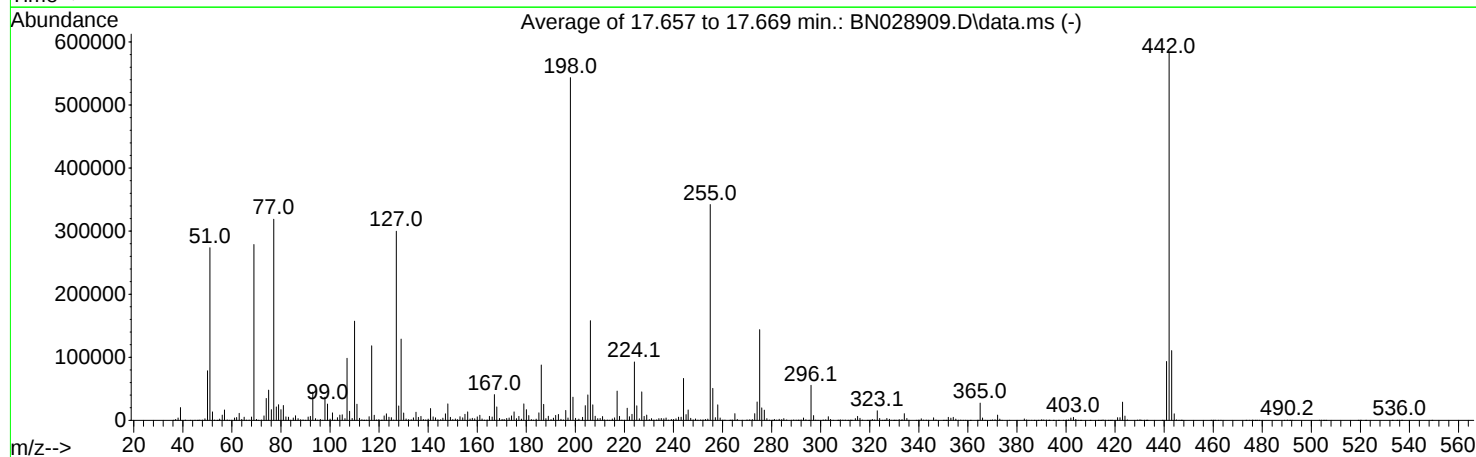


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113023\
Data File : BN028909.D
Acq On : 30 Nov 2023 13:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN113023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 01 00:28:34 2023

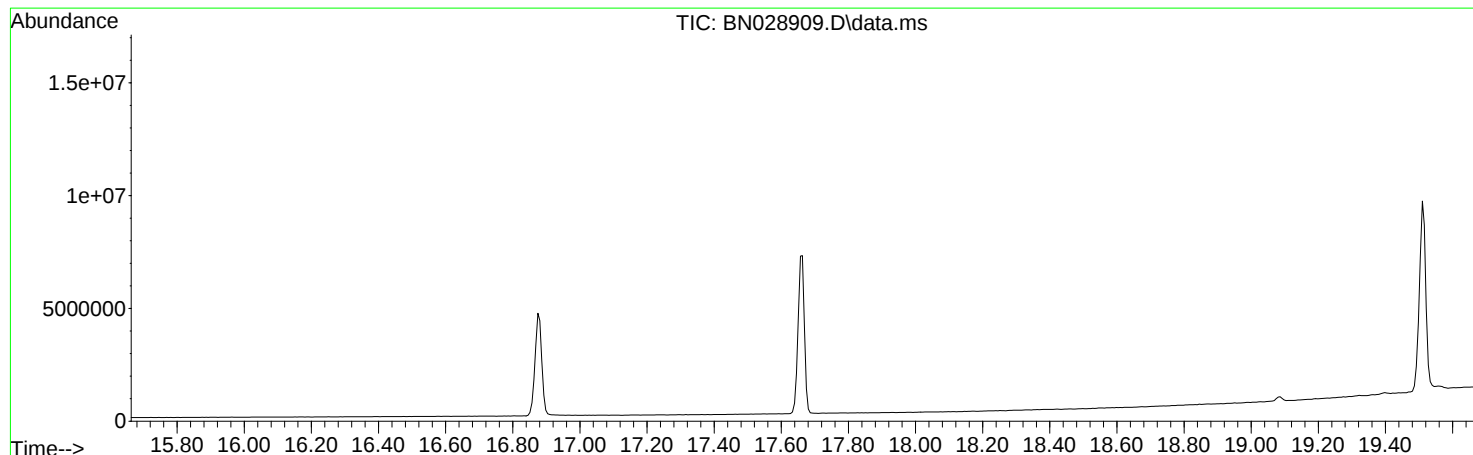




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.4	273842	PASS
68	69	0.00	2	1.9	5365	PASS
69	198	0.00	100	51.3	278750	PASS
70	69	0.00	2	0.6	1591	PASS
127	198	10	80	55.2	299883	PASS
197	198	0.00	2	0.7	3833	PASS
198	198	100	100	100.0	543509	PASS
199	198	5	9	6.8	36731	PASS
275	198	10	60	26.5	143840	PASS
365	198	1	100	5.1	27520	PASS
441	198	0.01	100	17.2	93333	PASS
442	442	50	100	100.0	583232	PASS
443	442	15	24	19.0	110579	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113023\
 Data File : BN028909.D
 Acq On : 30 Nov 2023 13:23
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 01 04:55:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 01 04:55:41 2023
 Response via : Initial Calibration

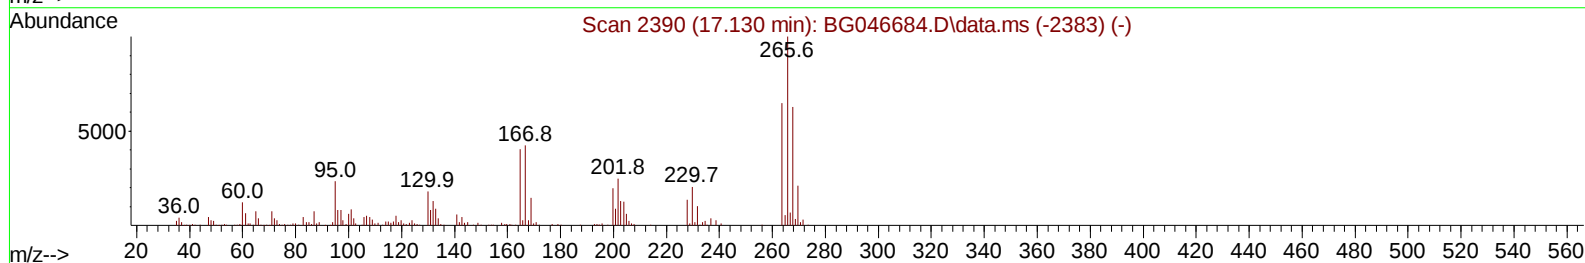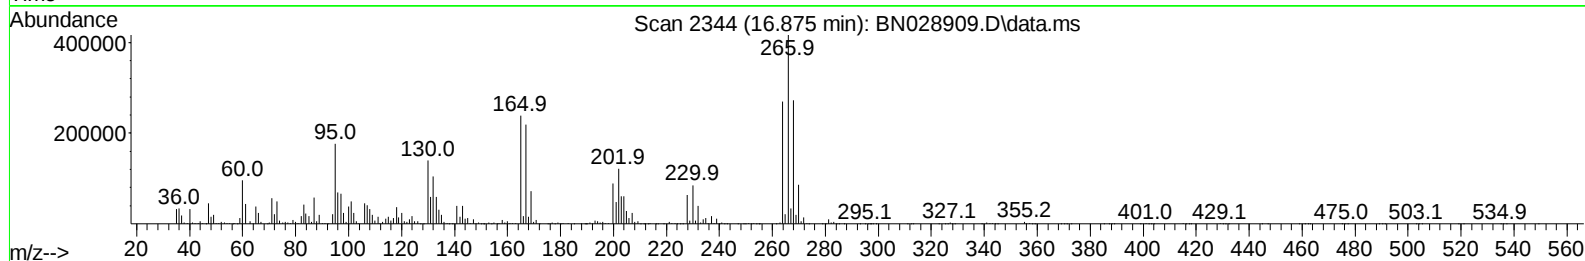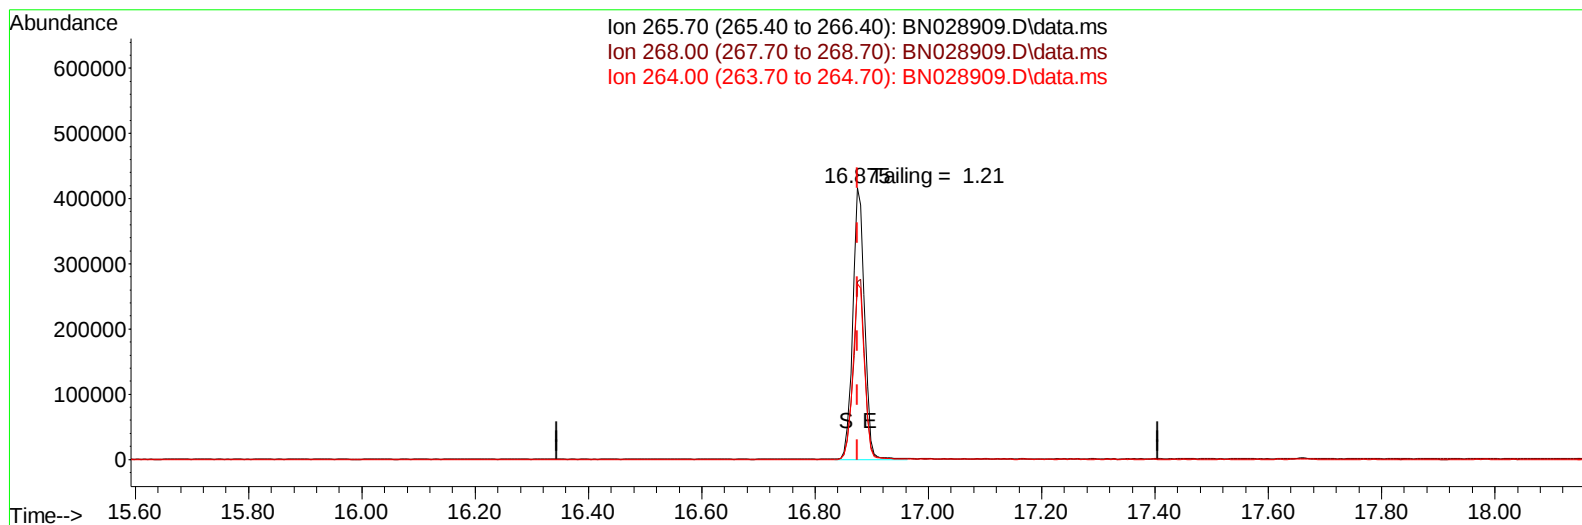

TIC: BN028909.D\data.ms

(70) Pentachlorophenol (C)

16.875min (0.000) 16800.02 ng




response 605288

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.46
264.00	61.60	64.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113023\
Data File : BN028909.D
Acq On : 30 Nov 2023 13:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 01 04:55:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 04:55:41 2023
Response via : Initial Calibration

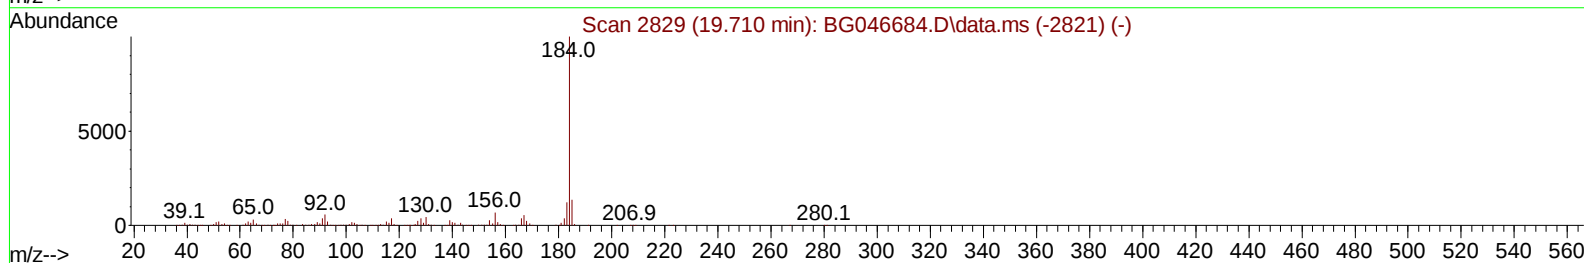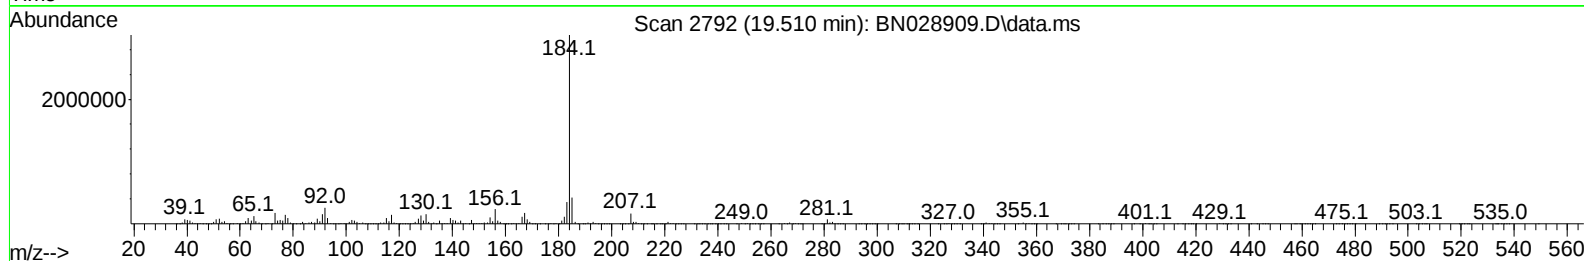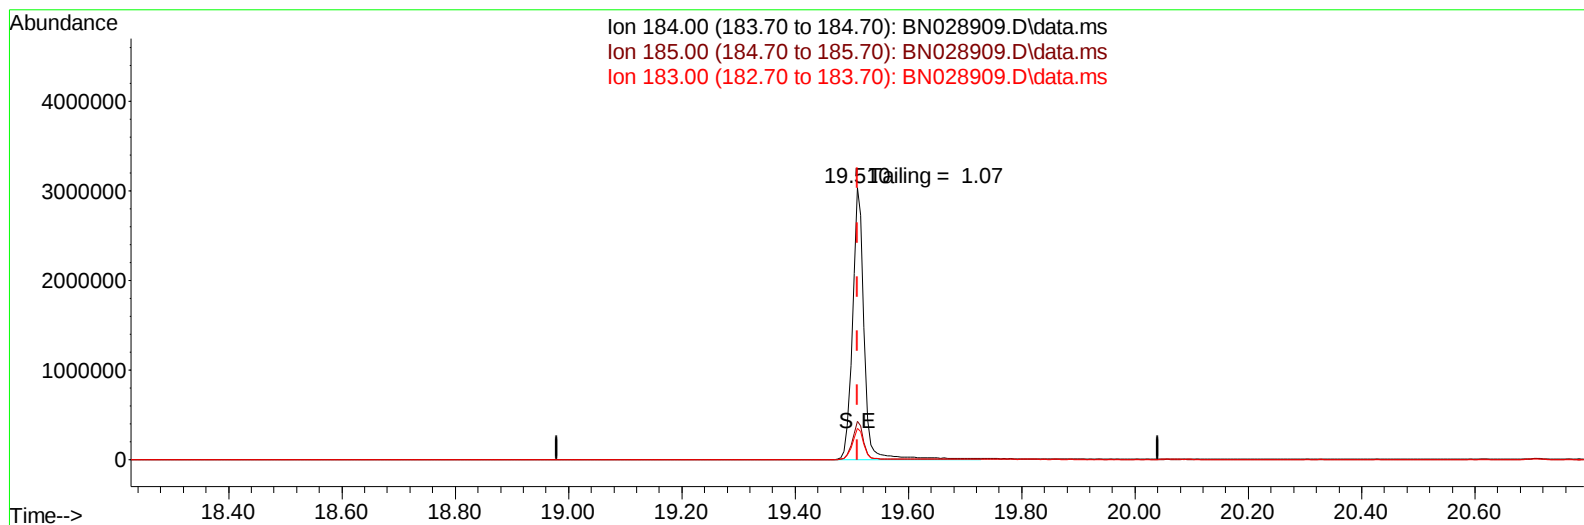

TIC: BN028909.D\data.ms

(77) Benzidine

19.510min (0.000) 210476.21 ng

response 4372917

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.98
183.00	13.20	11.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/30/2023	BNA_N	<u>BN028909.D</u>
Compound Name	Response	Retention Time
DDT	2414852	20.71
DDD	33905	20.31
DDE	691	19.757
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
34596	2449448	1.41

Instrument :
BNA_N
ClientSampleId :
DFTPP