


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113023\
Data File : BN028919.D
Acq On : 30 Nov 2023 21:00
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN113023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 01 00:28:34 2023

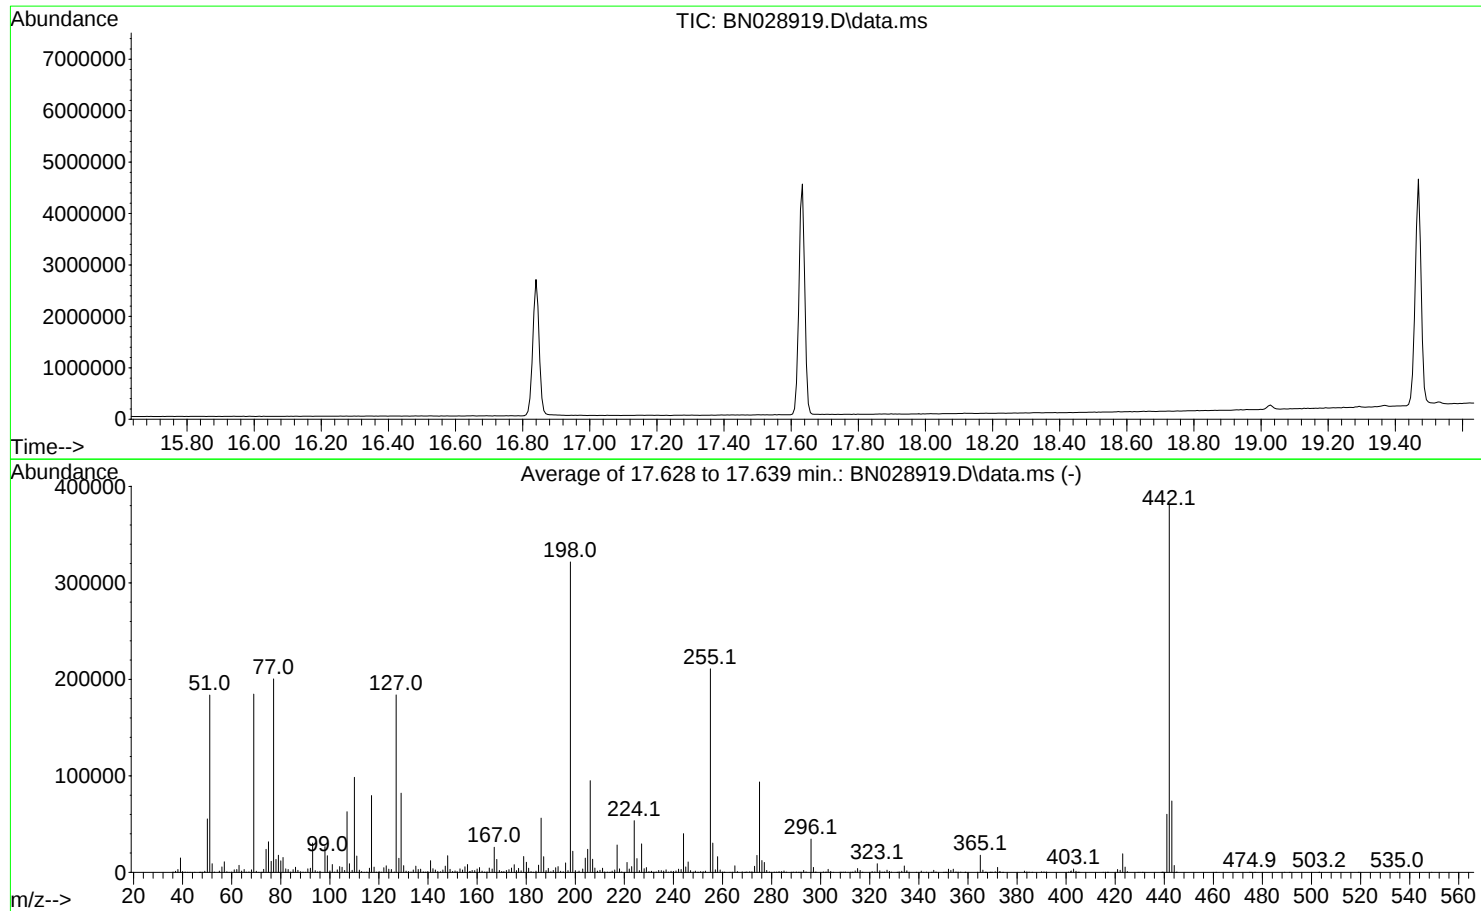




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.1	183767	PASS
68	69	0.00	2	1.4	2576	PASS
69	198	0.00	100	57.4	184640	PASS
70	69	0.00	2	0.6	1124	PASS
127	198	10	80	57.2	183861	PASS
197	198	0.00	2	0.6	1881	PASS
198	198	100	100	100.0	321707	PASS
199	198	5	9	6.8	21837	PASS
275	198	10	60	29.1	93635	PASS
365	198	1	100	5.5	17785	PASS
441	198	0.01	100	18.7	60184	PASS
442	442	50	100	100.0	381205	PASS
443	442	15	24	19.4	73907	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113023\
 Data File : BN028919.D
 Acq On : 30 Nov 2023 21:00
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 01 04:56:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 01 04:55:41 2023
 Response via : Initial Calibration

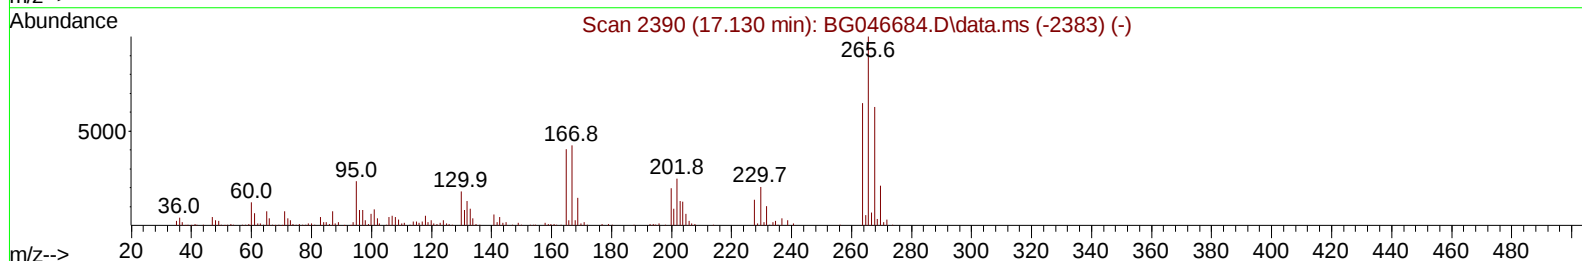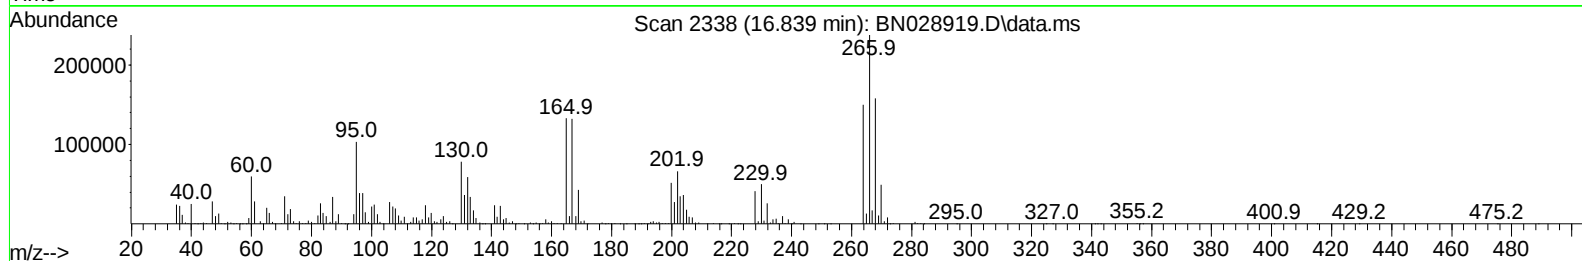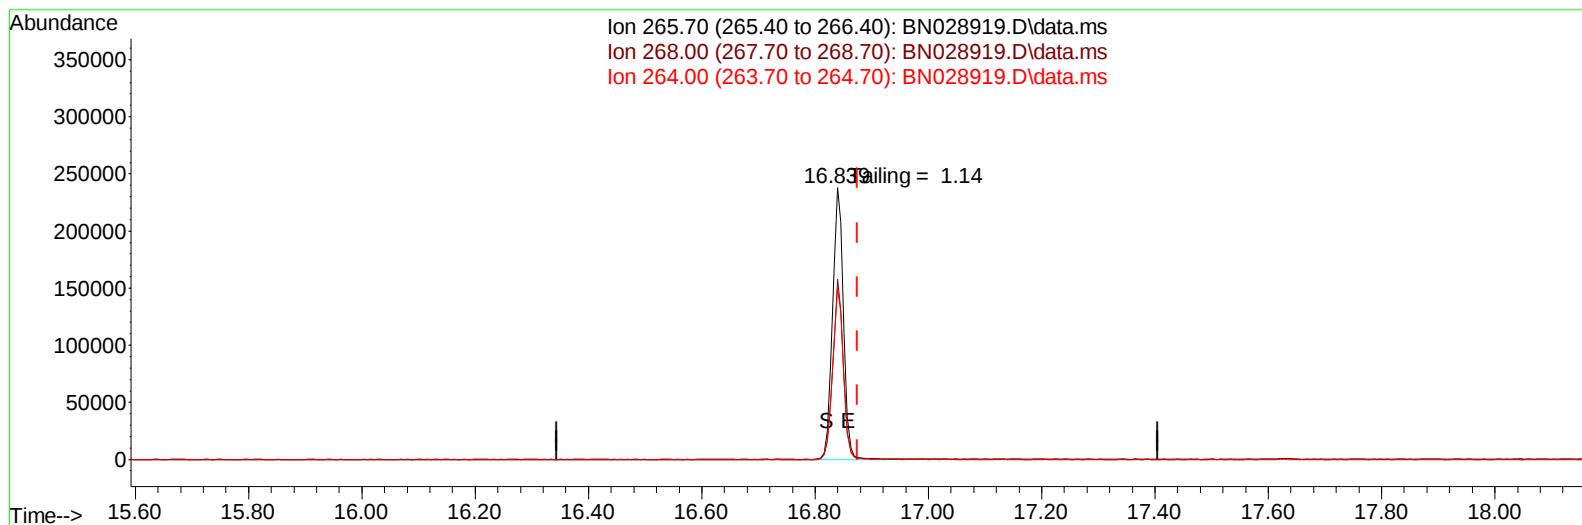

TIC: BN028919.D\data.ms

(70) Pentachlorophenol (C)

16.839min (-0.035) 14927.33 ng

response 319574

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.42
264.00	61.60	63.03
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/30/2023	BNA_N	<u>BN028919.D</u>
Compound Name	Response	Retention Time
DDT	1089874	20.68
DDD	15564	20.286
DDE	0	19.757
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15564	1105438	1.41

Instrument :
BNA_N
ClientSampleId :
DFTPP