
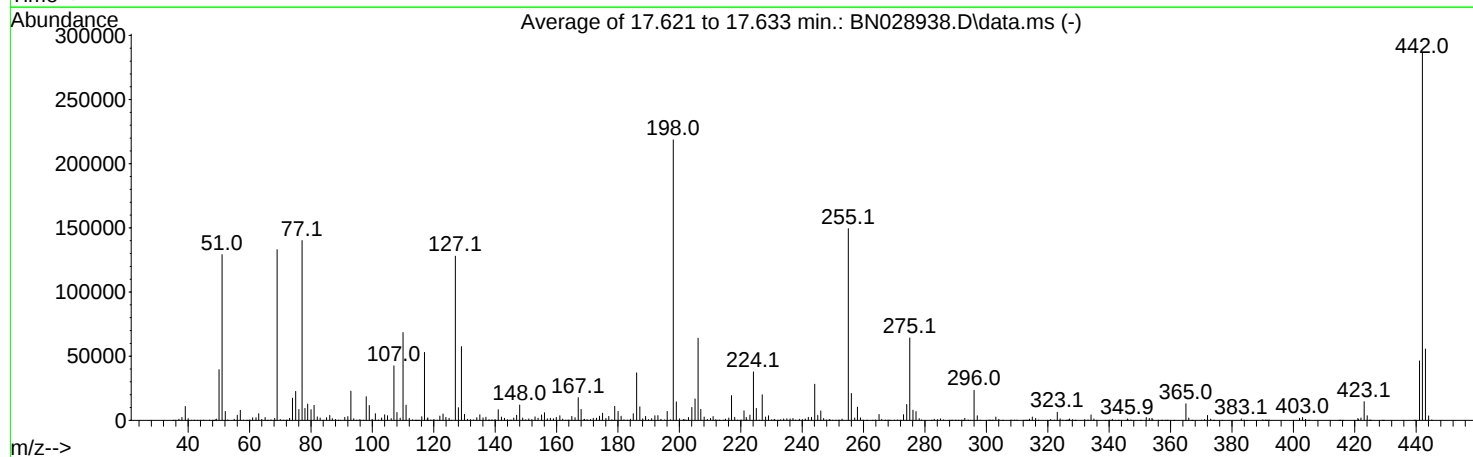


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113023\
Data File : BN028938.D
Acq On : 01 Dec 2023 09:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN113023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Dec 04 00:28:48 2023

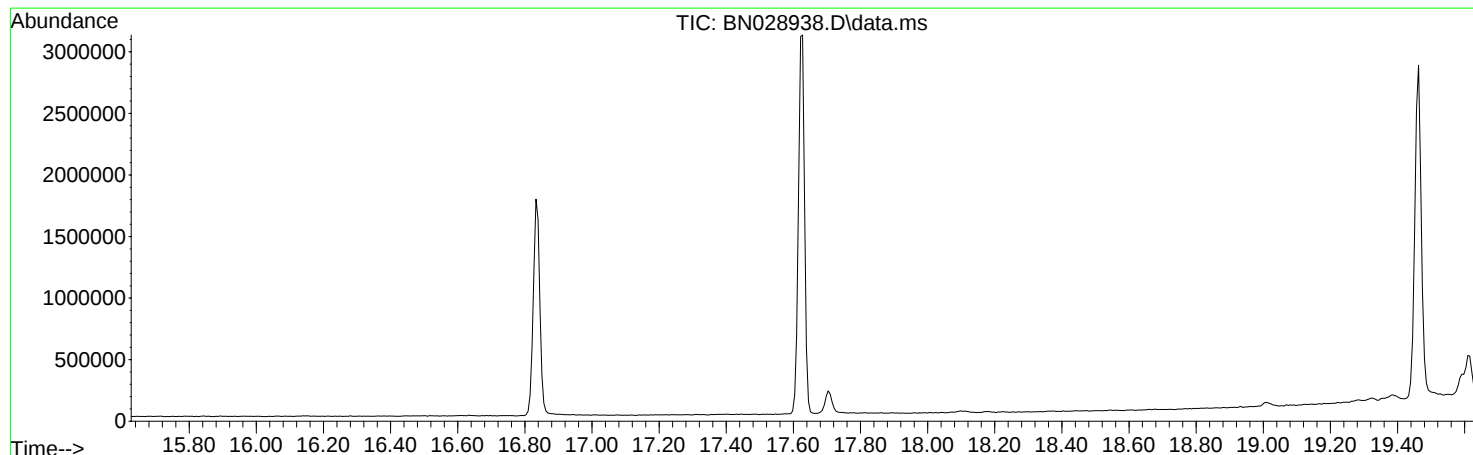




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.1	129151	PASS
68	69	0.00	2	1.1	1515	PASS
69	198	0.00	100	60.9	132994	PASS
70	69	0.00	2	0.5	701	PASS
127	198	10	80	58.6	127981	PASS
197	198	0.00	2	0.3	558	PASS
198	198	100	100	100.0	218539	PASS
199	198	5	9	6.6	14507	PASS
275	198	10	60	29.4	64243	PASS
365	198	1	100	5.9	12959	PASS
441	198	0.01	100	21.2	46344	PASS
442	442	50	100	100.0	286677	PASS
443	442	15	24	19.4	55656	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113023\
 Data File : BN028938.D
 Acq On : 01 Dec 2023 09:31
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 01 23:28:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 01 23:28:24 2023
 Response via : Initial Calibration

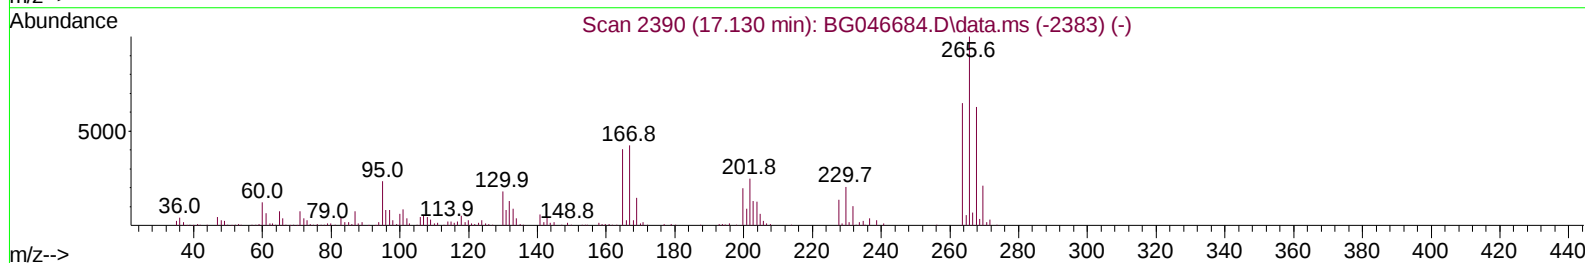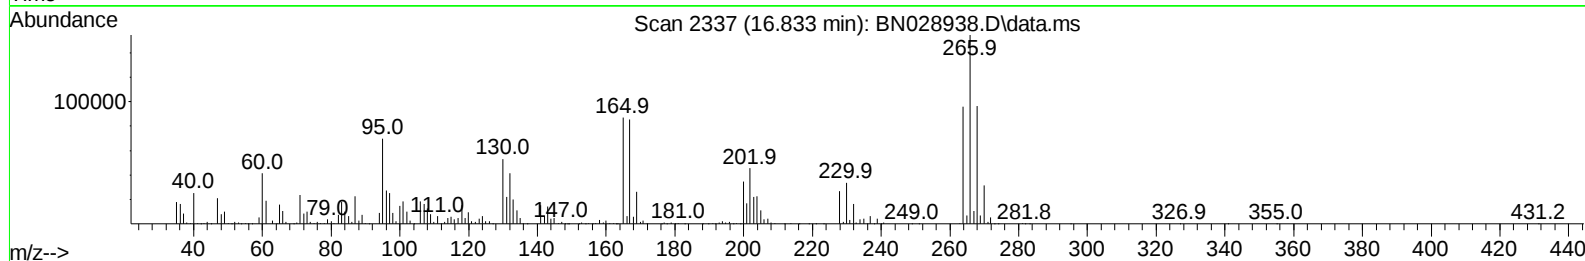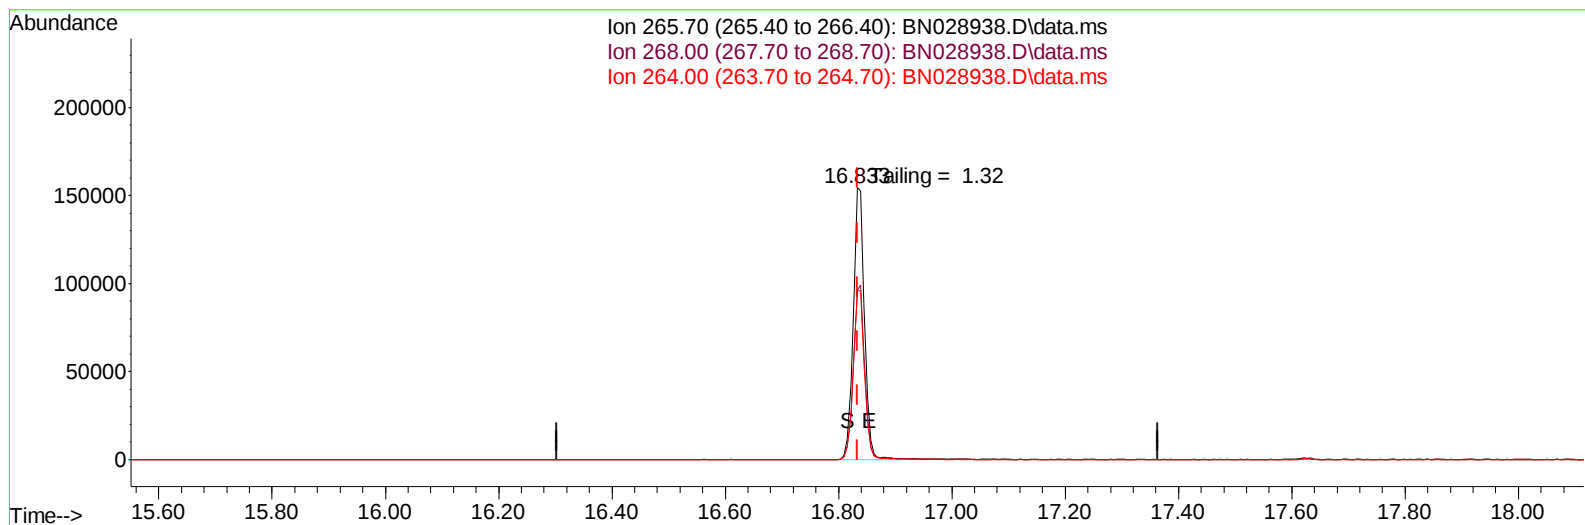

TIC: BN028938.D\data.ms

(70) Pentachlorophenol (C)

16.833min (0.000) 149947.65 ng




response 212992

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.33
264.00	61.60	62.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113023\
Data File : BN028938.D
Acq On : 01 Dec 2023 09:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 01 23:28:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

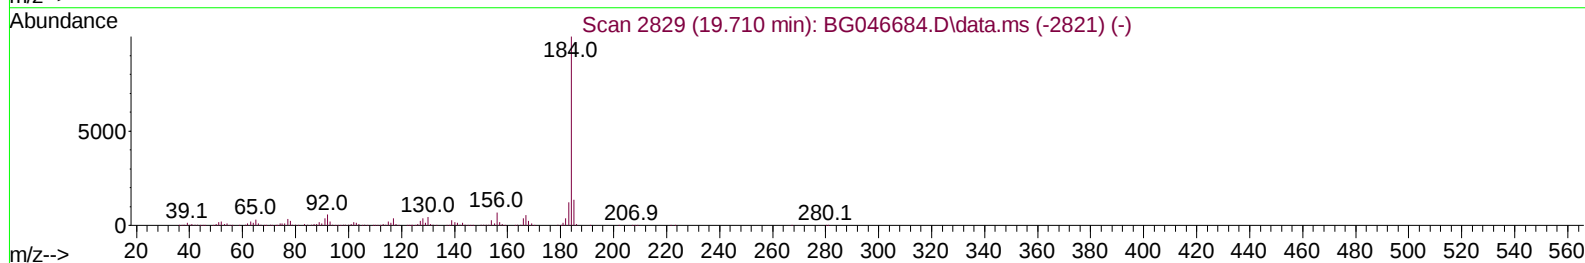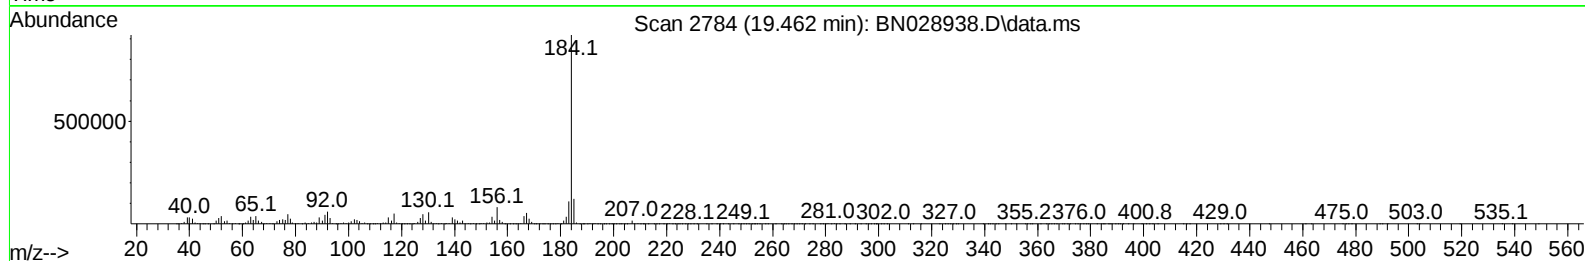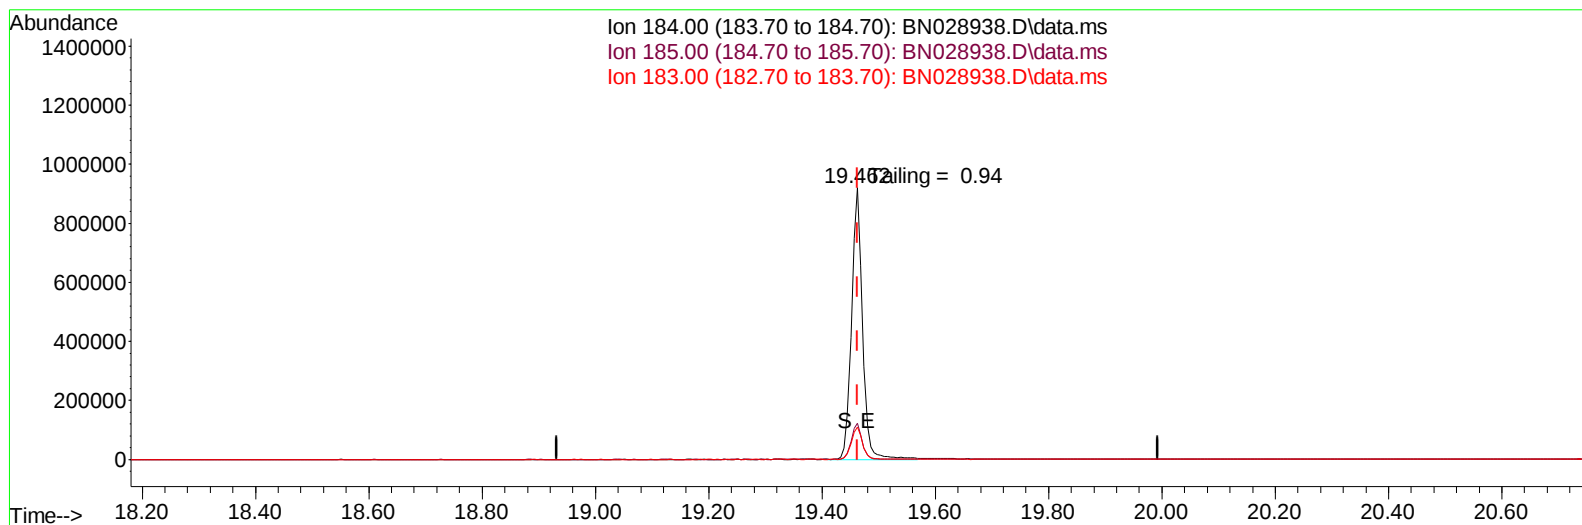

TIC: BN028938.D\data.ms

(77) Benzidine

19.462min (0.000) 164410.28 ng

response 1246730

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.26
183.00	13.20	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/30/2023	BNA_N	<u>BN028938.D</u>
Compound Name	Response	Retention Time
DDT	38888	20.674
DDD	228055	20.239
DDE	823	19.721
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
228878	267766	85.48

Instrument :
BNA_N
ClientSampleId :
DFTPP