

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (QT Reviewed)


Data File : BN003663.D
Acq On : 01 Dec 2018 15:49
Operator : JU/SJ
Sample : J6096-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4148

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:21 PM

Quant Time: Dec 03 01:53:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 01:15:58 2018
Response via : Initial Calibration

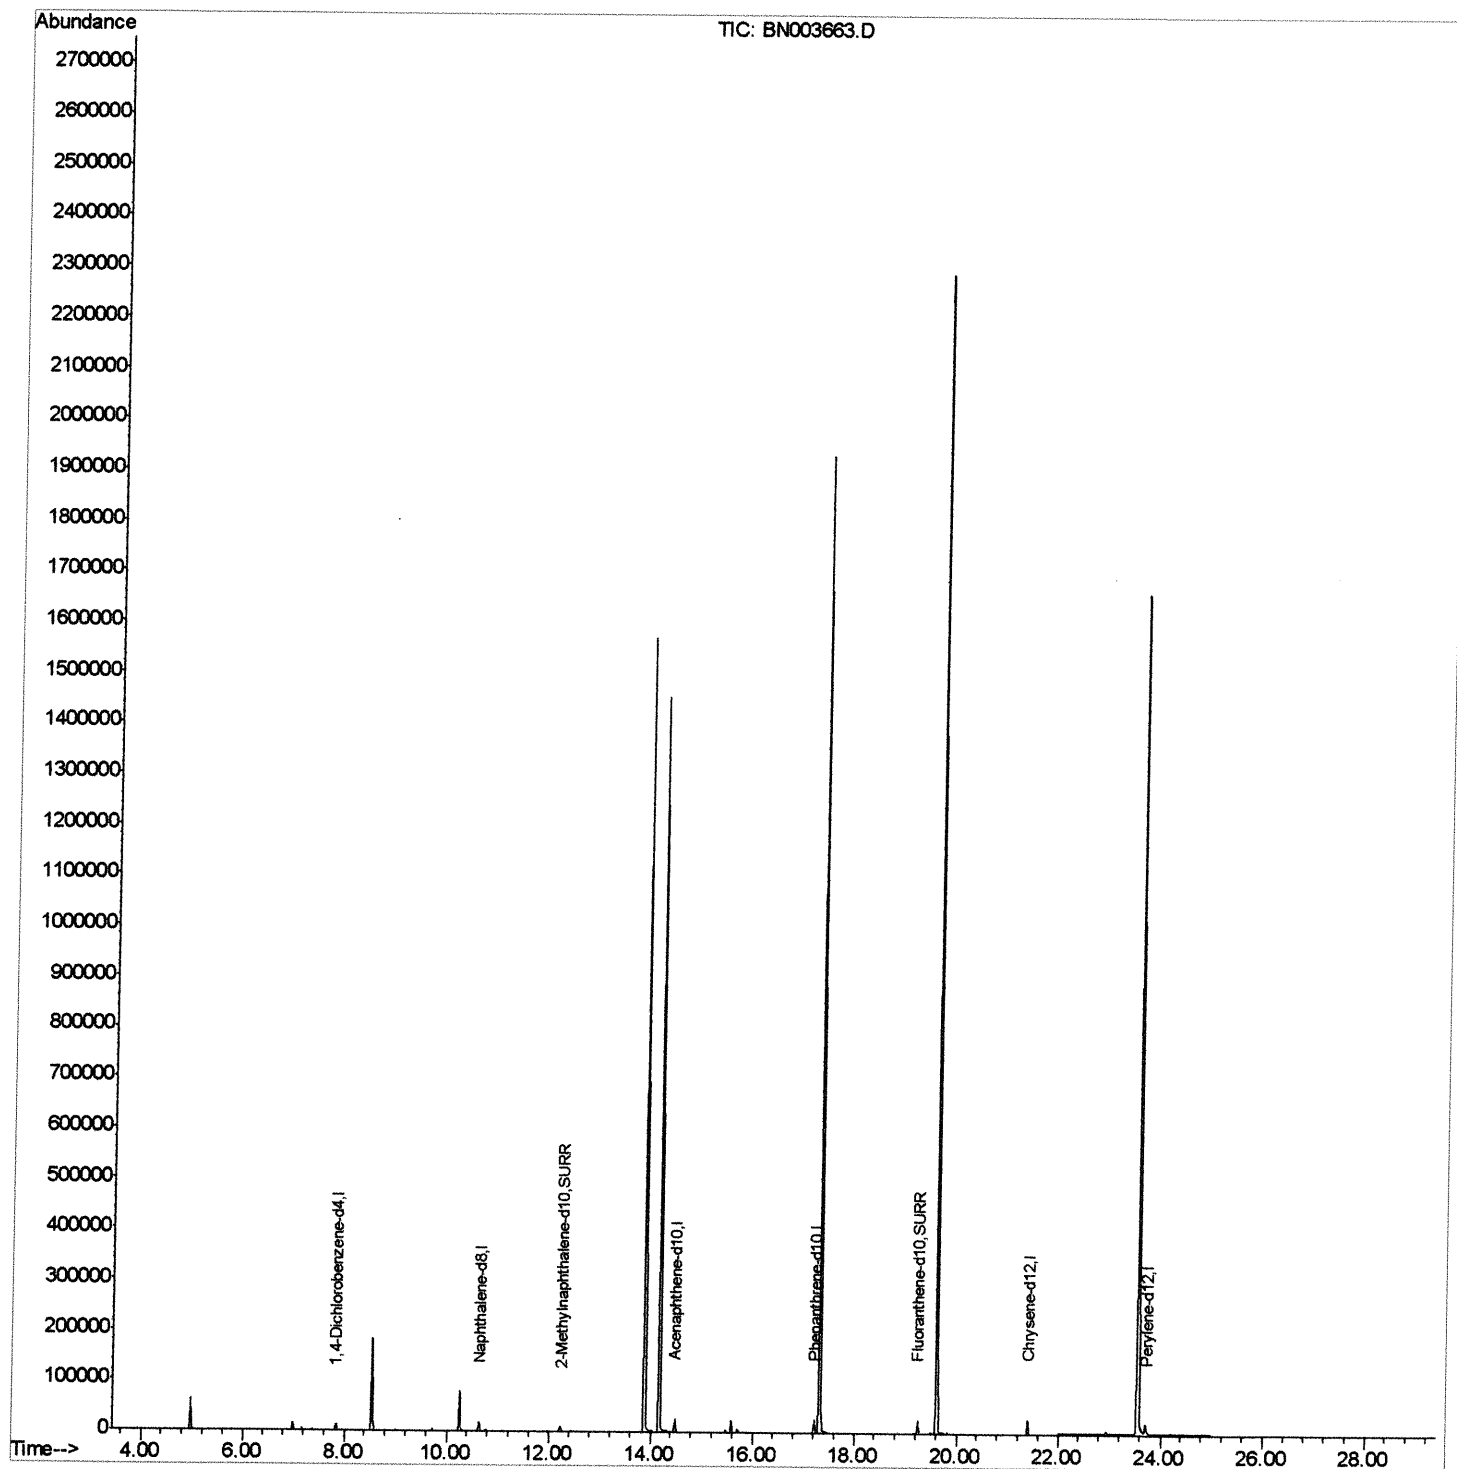

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003663.D
Acq On : 01 Dec 2018 15:49
Operator : JU/SJ
Sample : J6096-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4148

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:21 PM

Quant Time: Dec 03 01:19:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 01:15:58 2018
Response via : Initial Calibration

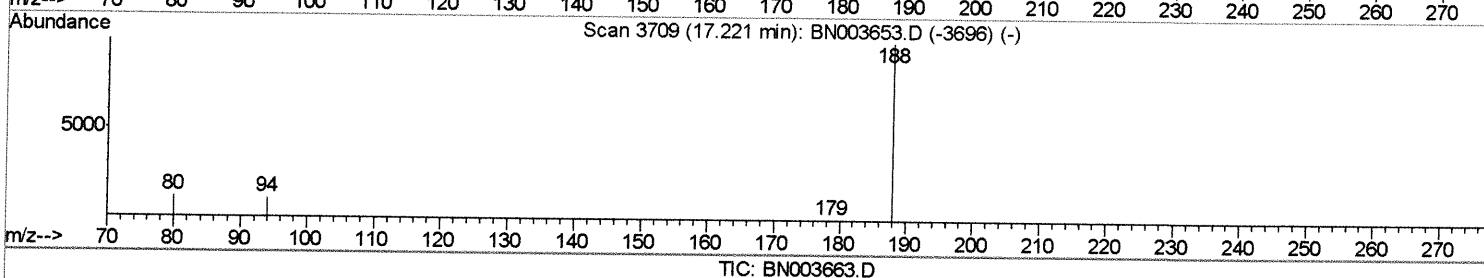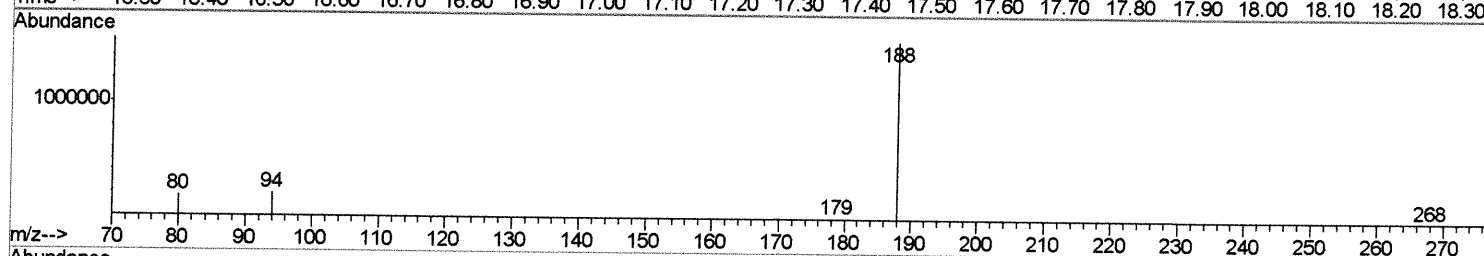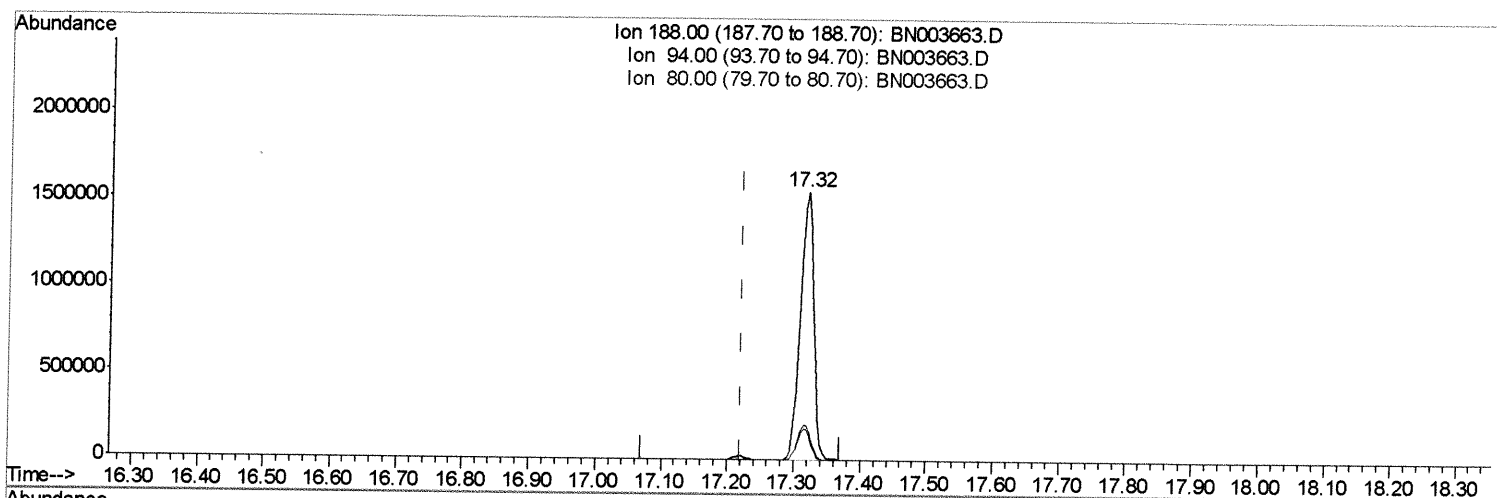

TIC: BN003663.D

(10) Phenanthrene-d10 (I)

17.318min (+0.097) 0.40ng/ul

response 2214423

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	12.85#
80.00	11.60	11.37
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003663.D
Acq On : 01 Dec 2018 15:49
Operator : JU/SJ
Sample : J6096-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4148

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:21 PM

Quant Time: Dec 03 01:19:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 01:15:58 2018
Response via : Initial Calibration

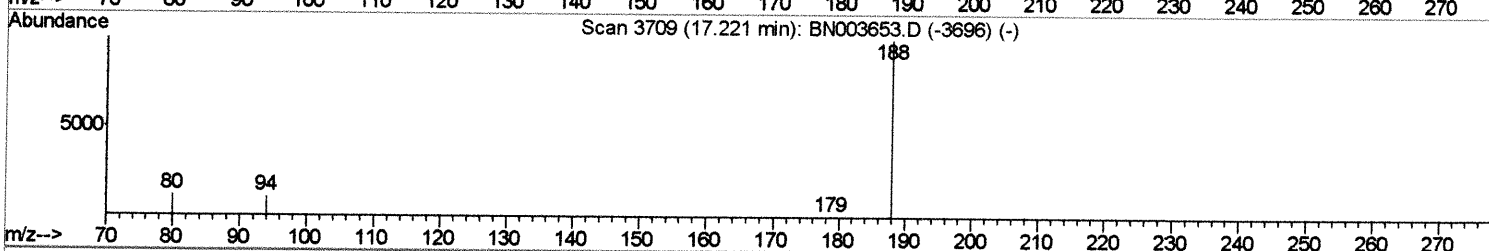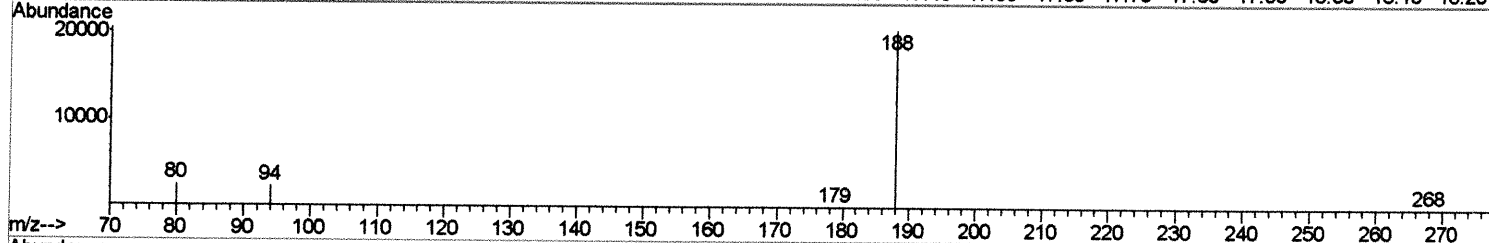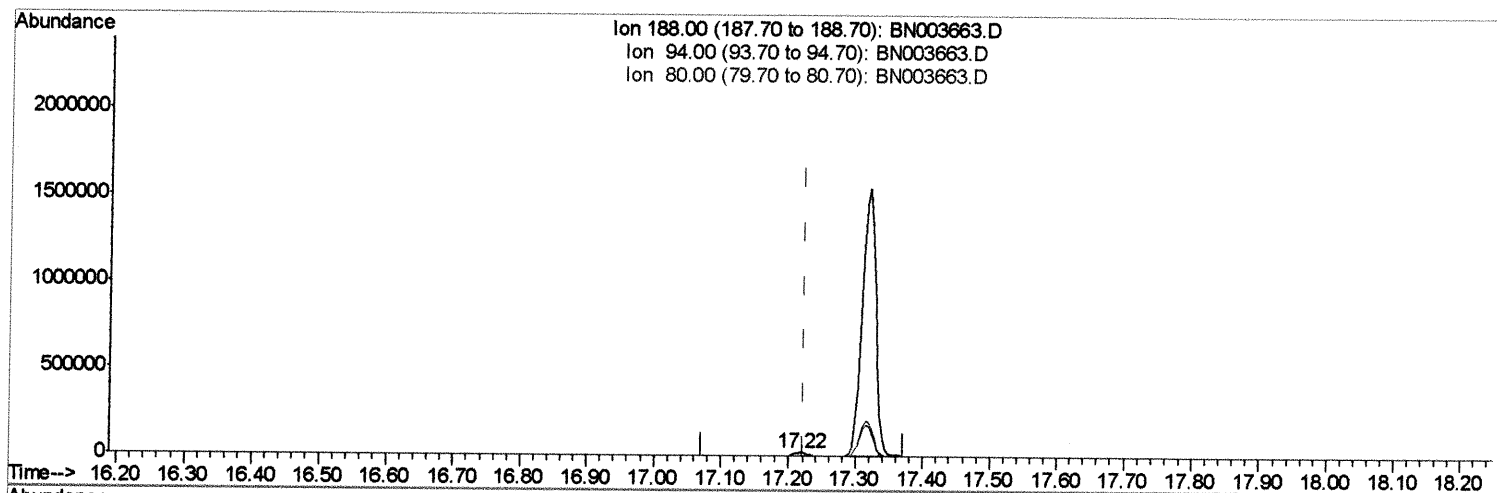

TIC: BN003663.D

(10) Phenanthrene-d10 (I)

17.217min (-0.004) 0.40ng/ul m > 50 12/11/18

response 28247

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	11.06
80.00	11.60	11.94
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003663.D
Acq On : 01 Dec 2018 15:49
Operator : JU/SJ
Sample : J6096-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4148

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:21 PM

Quant Time: Dec 03 01:51:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 01:15:58 2018
Response via : Initial Calibration

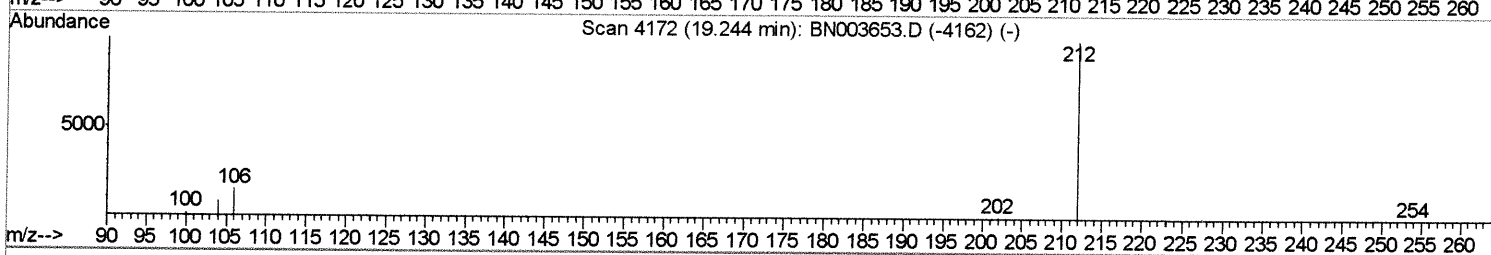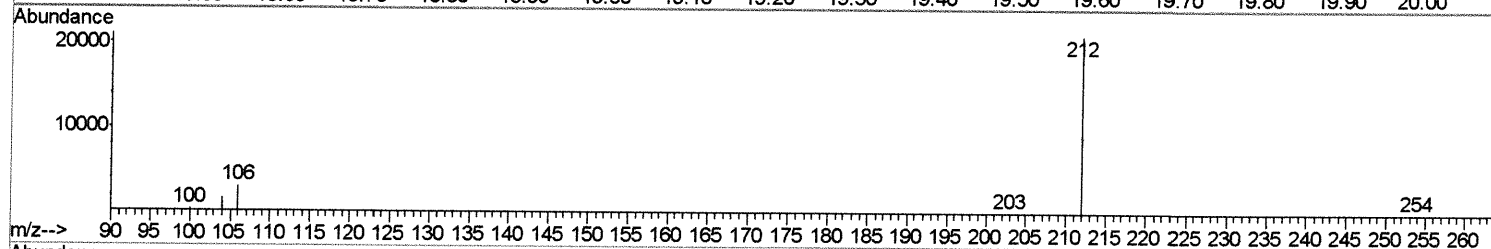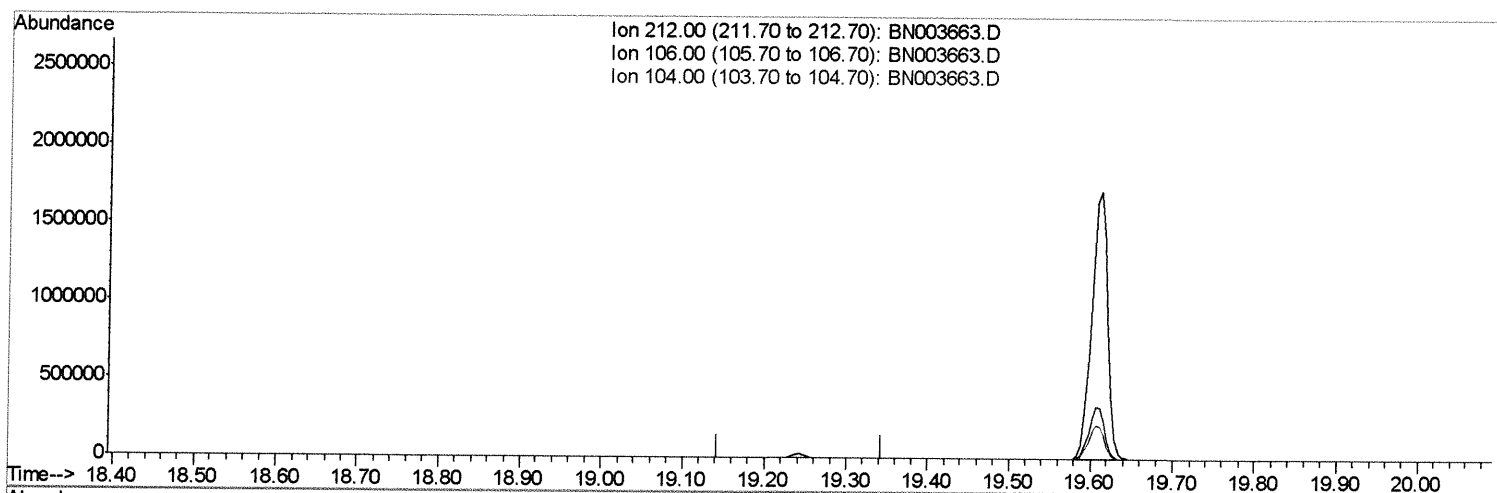

TIC: BN003663.D

(14) Fluoranthene-d10 (SURR)

19.244min (-19.244) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003663.D
Acq On : 01 Dec 2018 15:49
Operator : JU/SJ
Sample : J6096-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4148

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:21 PM

Quant Time: Dec 03 01:51:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 01:15:58 2018
Response via : Initial Calibration

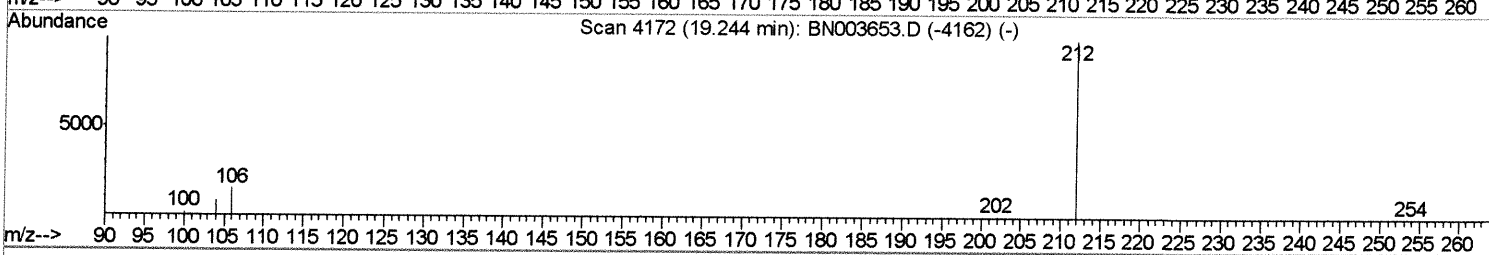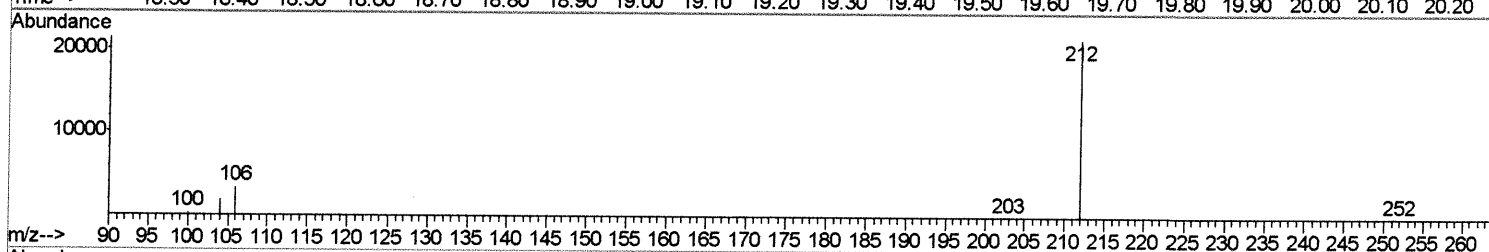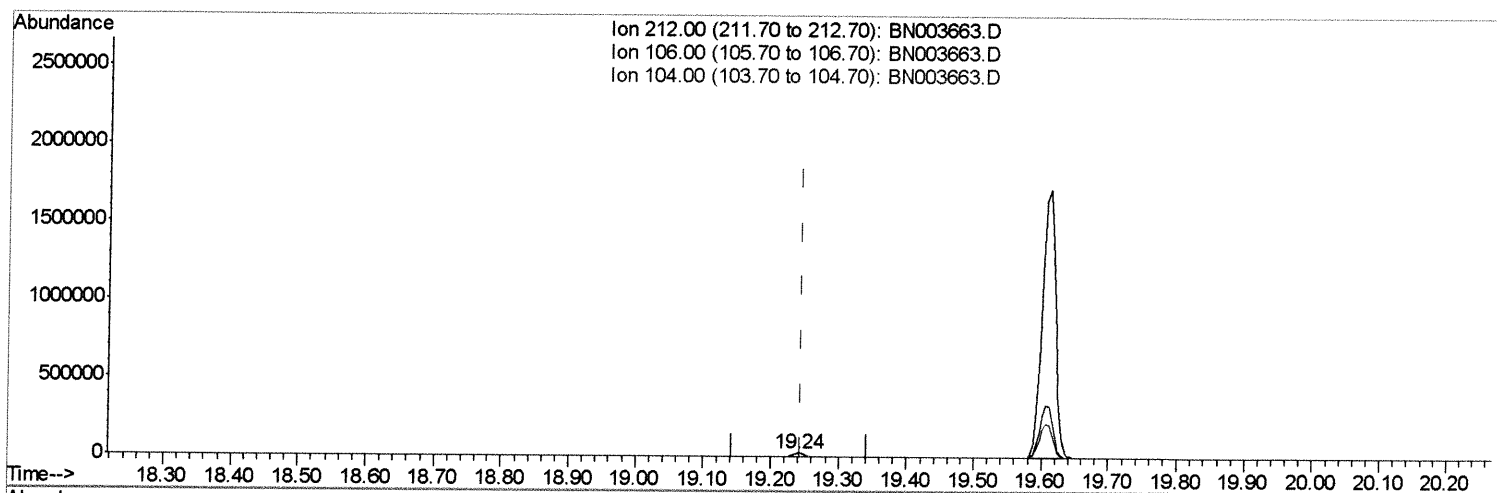

TIC: BN003663.D

(14) Fluoranthene-d10 (SURR)

19.239min (-0.005) 0.34ng/ul m> SJ 12/11/18

response 28421

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003663.D
Acq On : 01 Dec 2018 15:49
Operator : JU/SJ
Sample : J6096-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4148

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:21 PM

Quant Time: Dec 03 01:51:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 01:15:58 2018
Response via : Initial Calibration

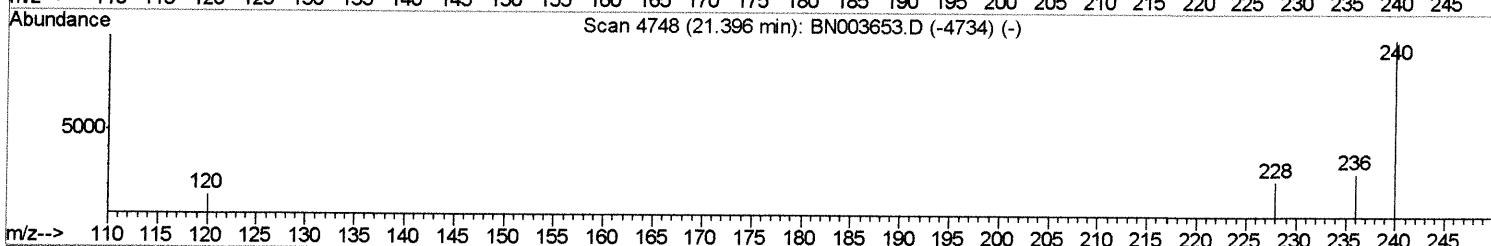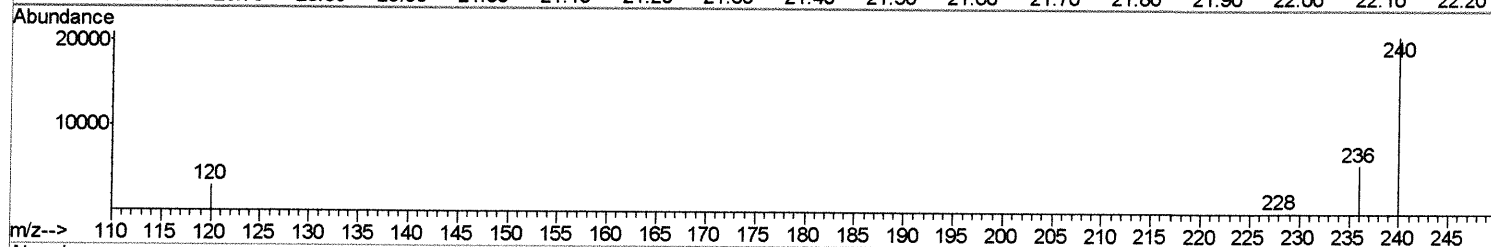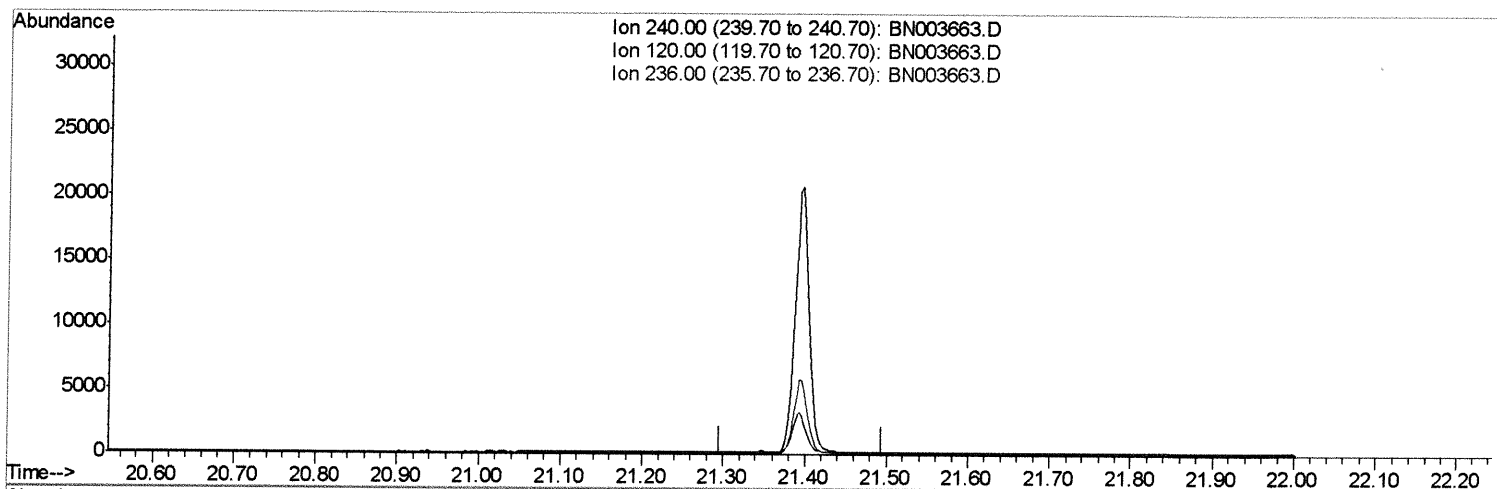

TIC: BN003663.D

(16) Chrysene-d12 (I)

21.396min (-21.396) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003663.D
Acq On : 01 Dec 2018 15:49
Operator : JU/SJ
Sample : J6096-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4148

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:21 PM

Quant Time: Dec 03 01:51:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 01:15:58 2018
Response via : Initial Calibration

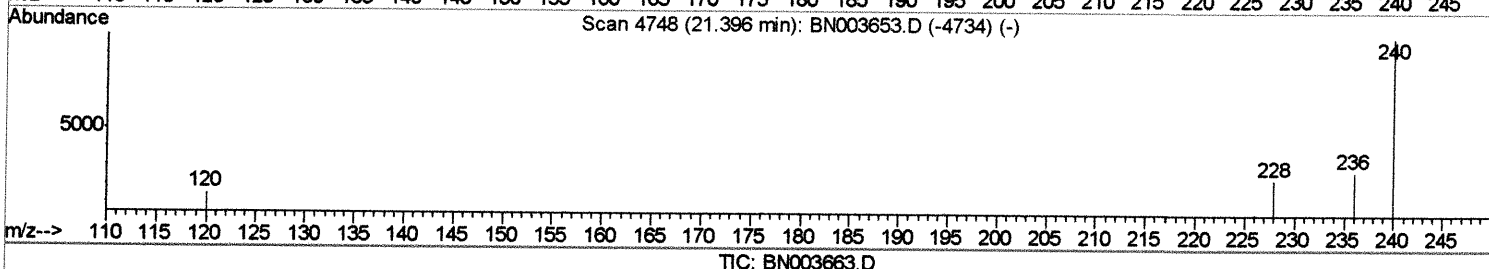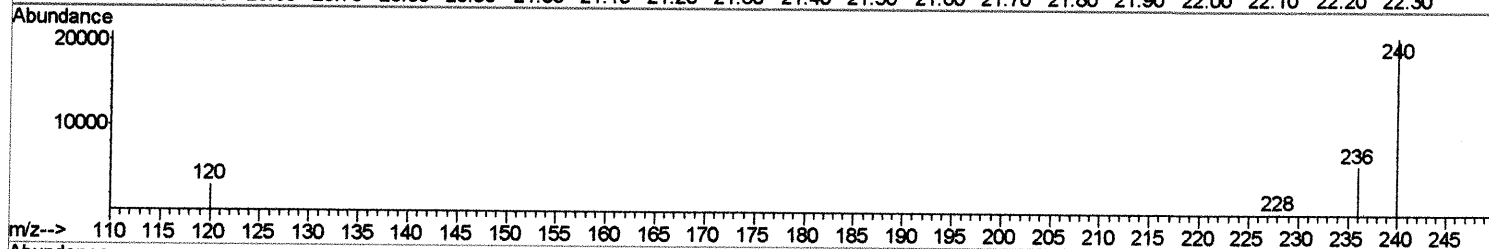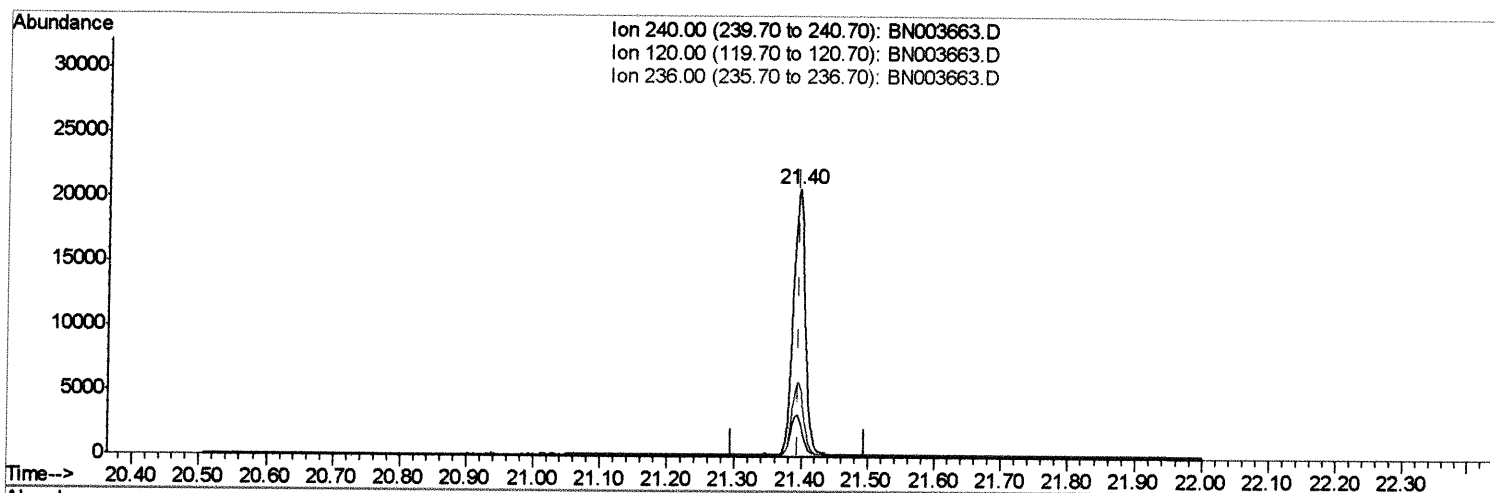

(16) Chrysene-d12 (I)

21.395min (-0.000) 0.40ng/ul m > 50 12/11/18

response 25911

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	14.66
236.00	27.60	27.64
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003663.D
Acq On : 01 Dec 2018 15:49
Operator : JU/SJ
Sample : J6096-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4148

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:21 PM

Quant Time: Dec 03 01:52:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 01:15:58 2018
Response via : Initial Calibration

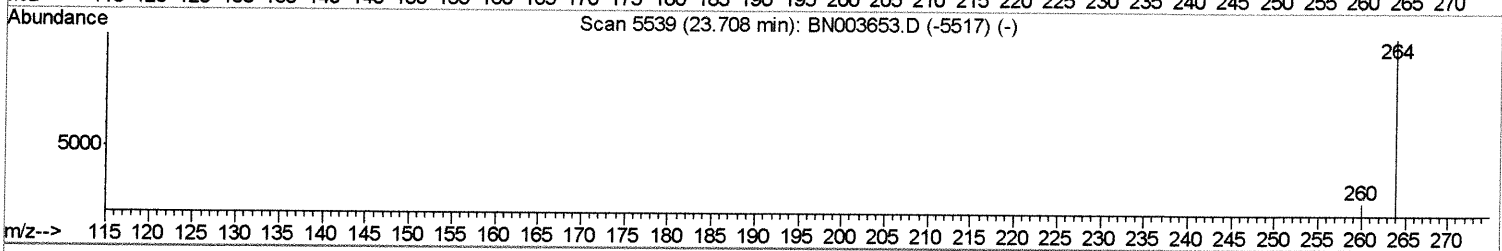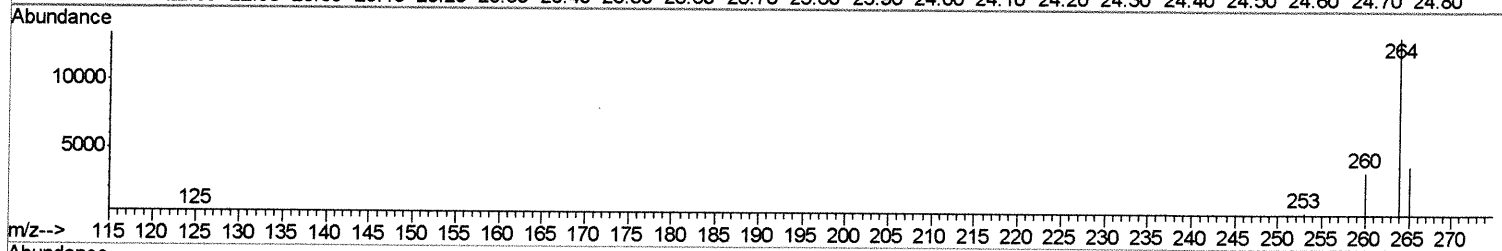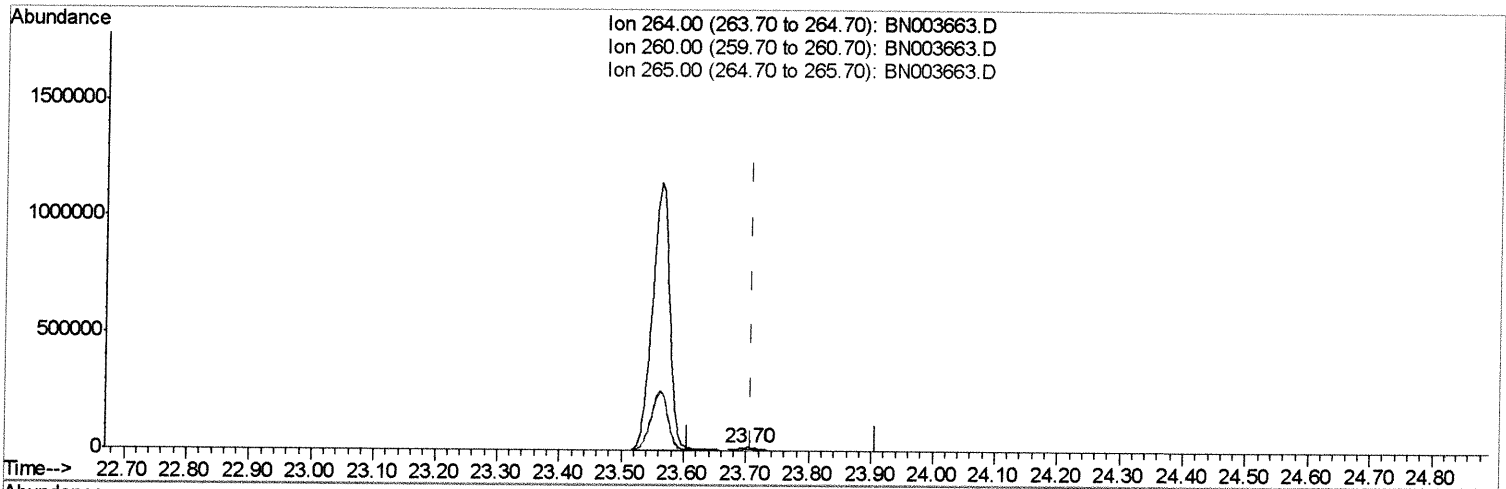

TIC: BN003663.D

(20) Perylene-d12 (I)

23.702min (-0.006) 0.40ng/ul

response 30244

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	25.83
265.00	33.50	28.82
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003663.D
Acq On : 01 Dec 2018 15:49
Operator : JU/SJ
Sample : J6096-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4148

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:21 PM

Quant Time: Dec 03 01:52:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 01:15:58 2018
Response via : Initial Calibration

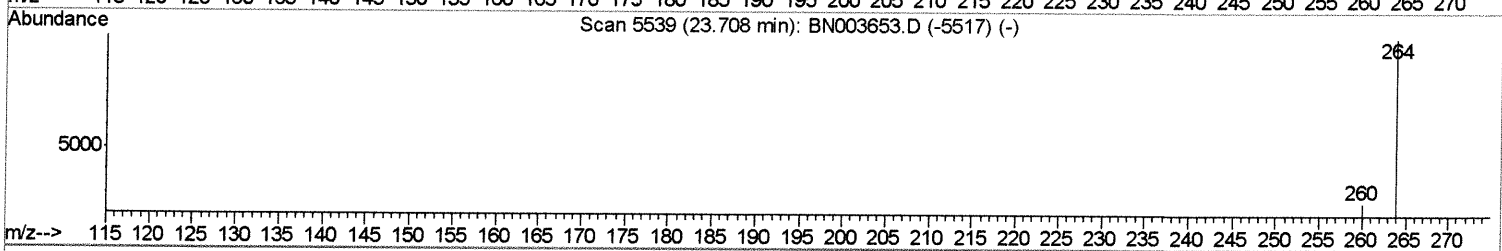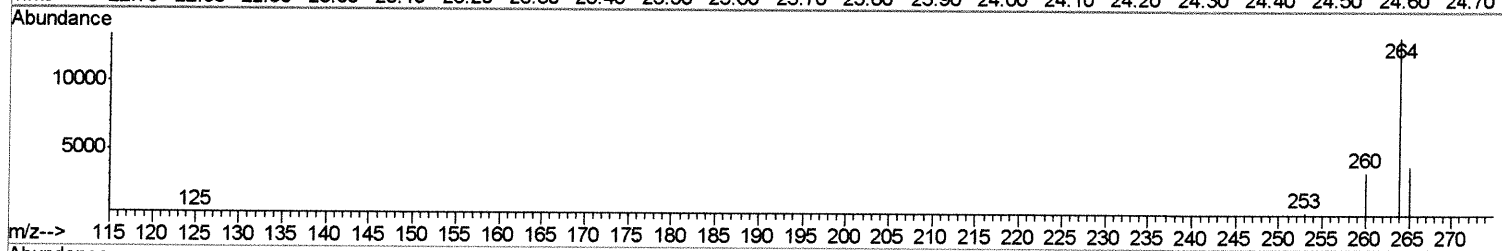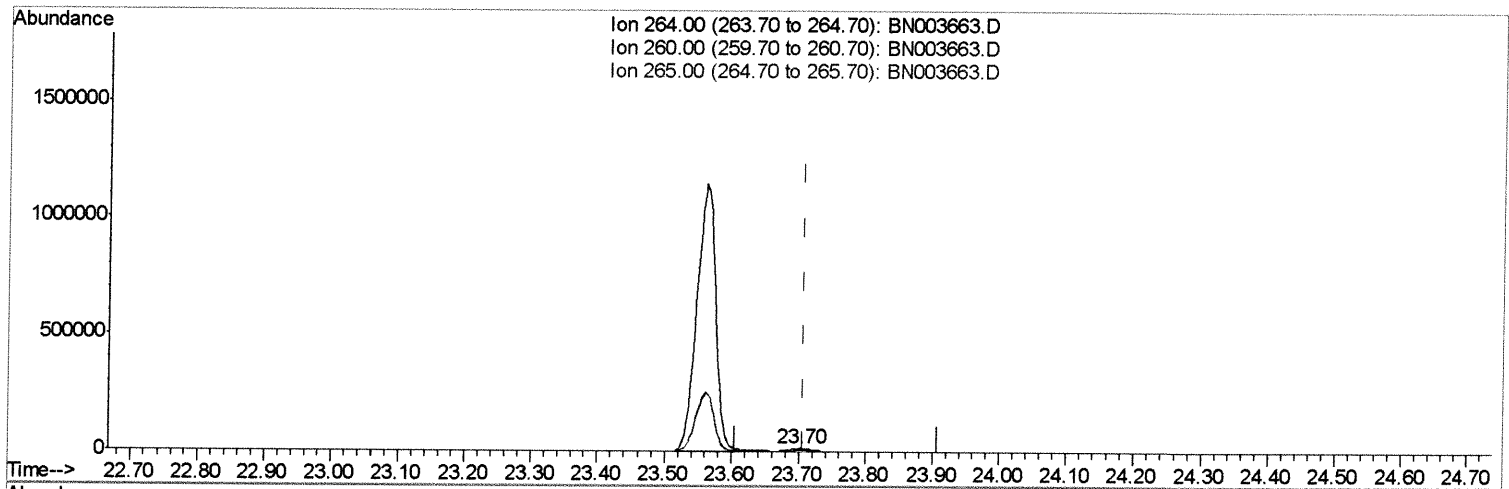

TIC: BN003663.D

(20) Perylene-d12 (I)

23.702min (-0.006) 0.40ng/ul m> SJ 12/11/18

response 21132

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	25.83
265.00	33.50	28.82
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (QT Reviewed)

Data File : BN003663.D
Acq On : 01 Dec 2018 15:49
Operator : JU/SJ
Sample : J6096-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4148

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:21 PM

Quant Time: Dec 03 01:53:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 01:15:58 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5778	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	23583	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	13484	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	28247m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	25911m	0.40	ng/ul	0.00
20) Perylene-d12	23.70	264	21132m	0.40	ng/ul	0.00

SD 12/11/18

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.23	152	11871	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	28421m	0.34	ng/ul	0.00

SD 12/11/18

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed