


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (QT Reviewed)
Data File : BN003665.D
Acq On : 01 Dec 2018 16:59
Operator : JU/SJ
Sample : J6096-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4156

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:49 PM

Quant Time: Dec 03 02:00:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 01:15:58 2018
Response via : Initial Calibration

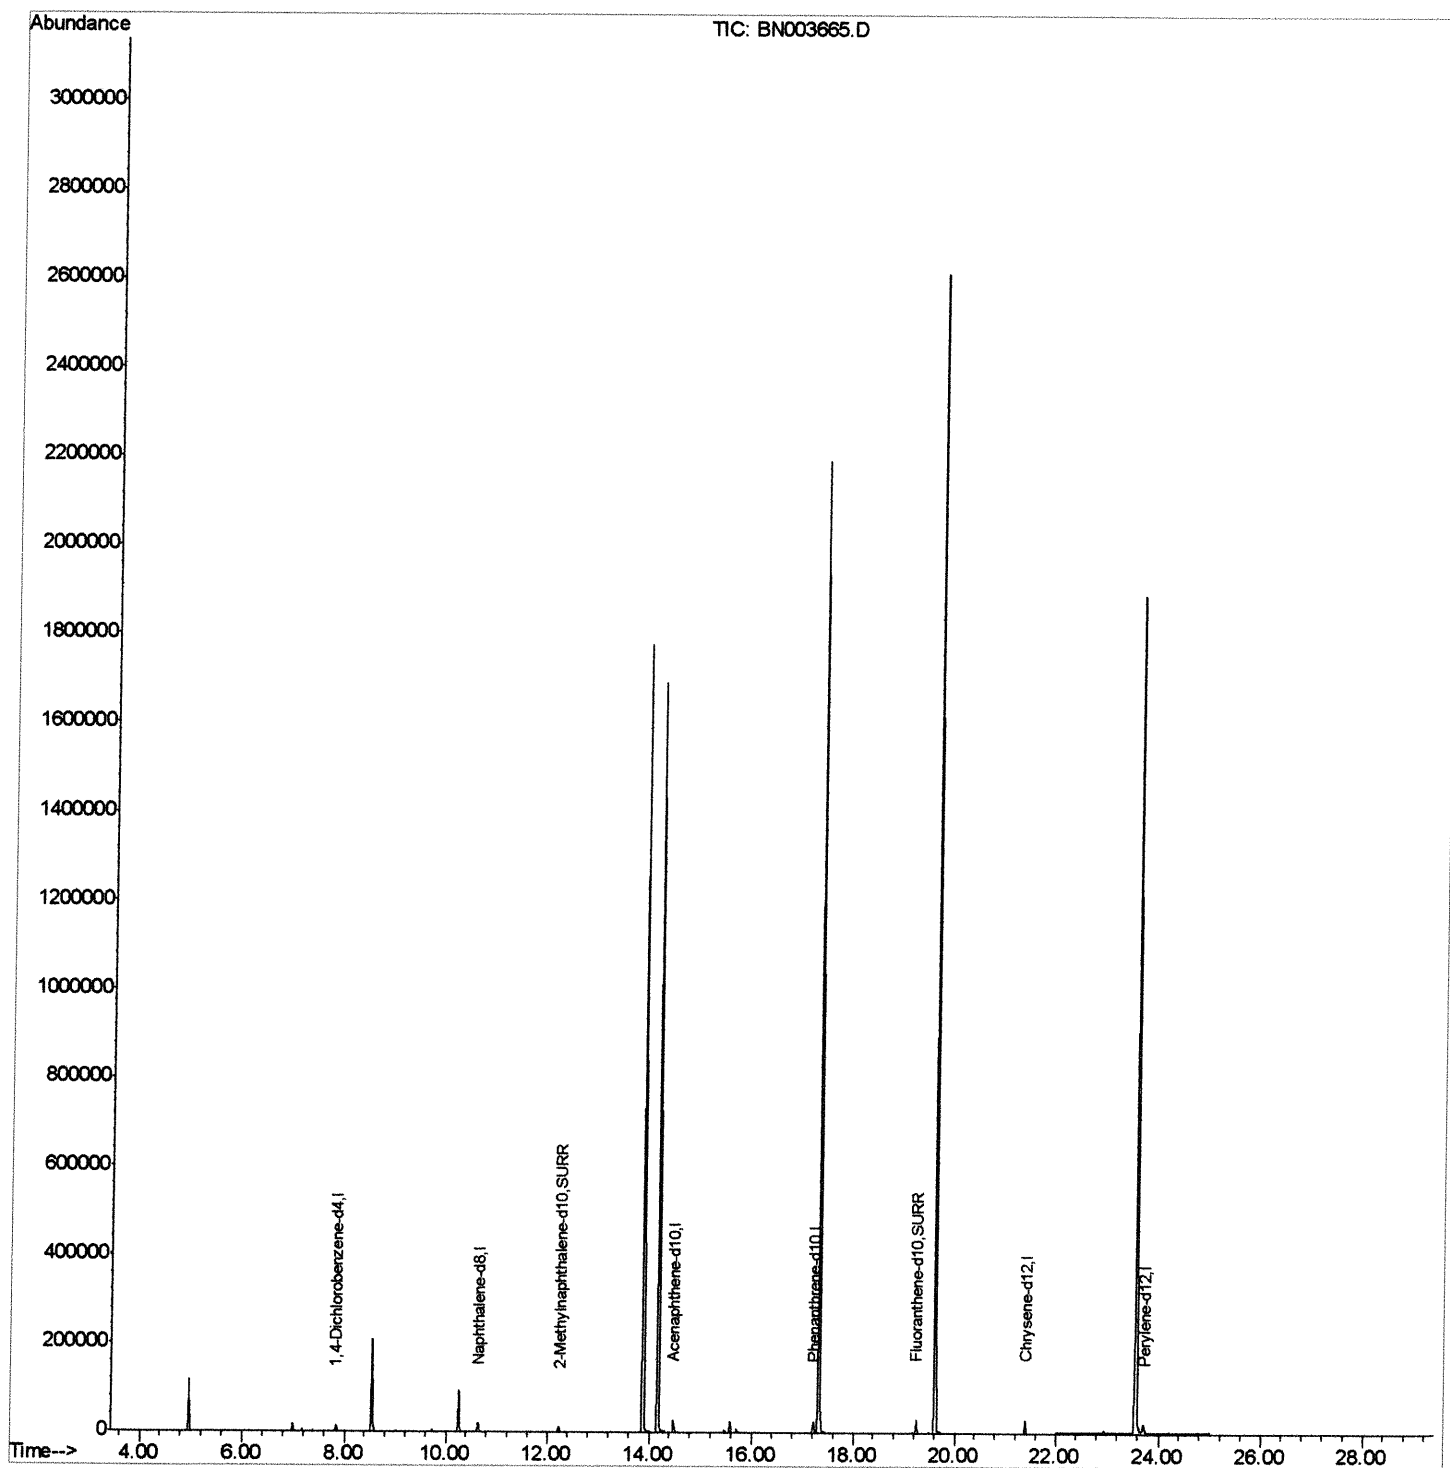

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003665.D
Acq On : 01 Dec 2018 16:59
Operator : JU/SJ
Sample : J6096-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4156

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:49 PM

Quant Time: Dec 03 01:19:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 01:15:58 2018
Response via : Initial Calibration

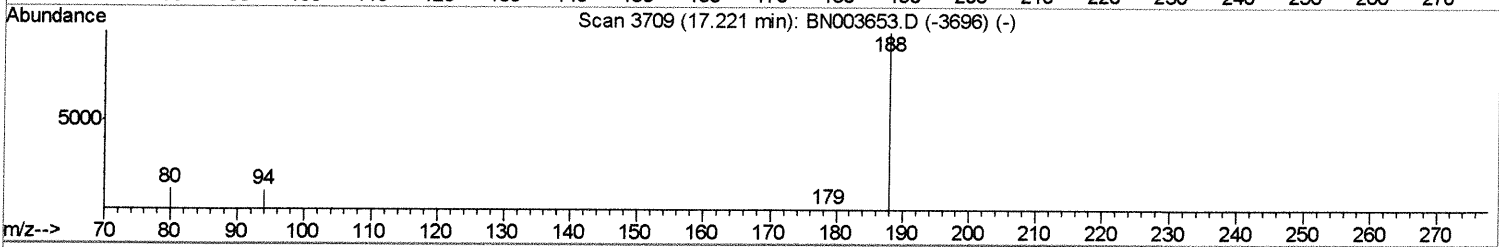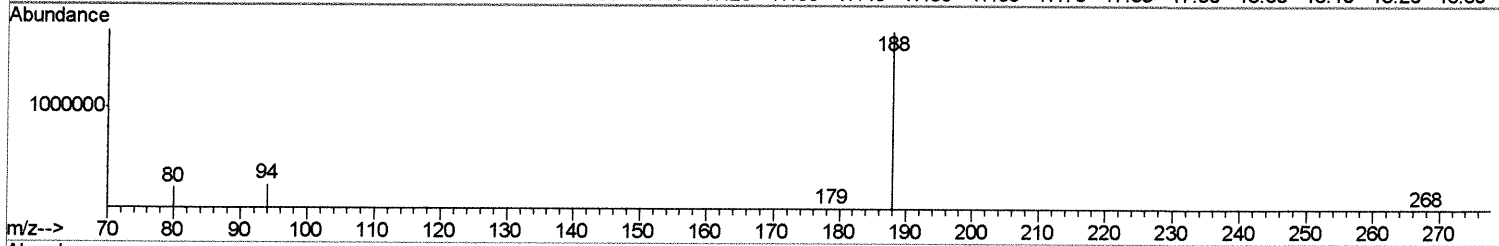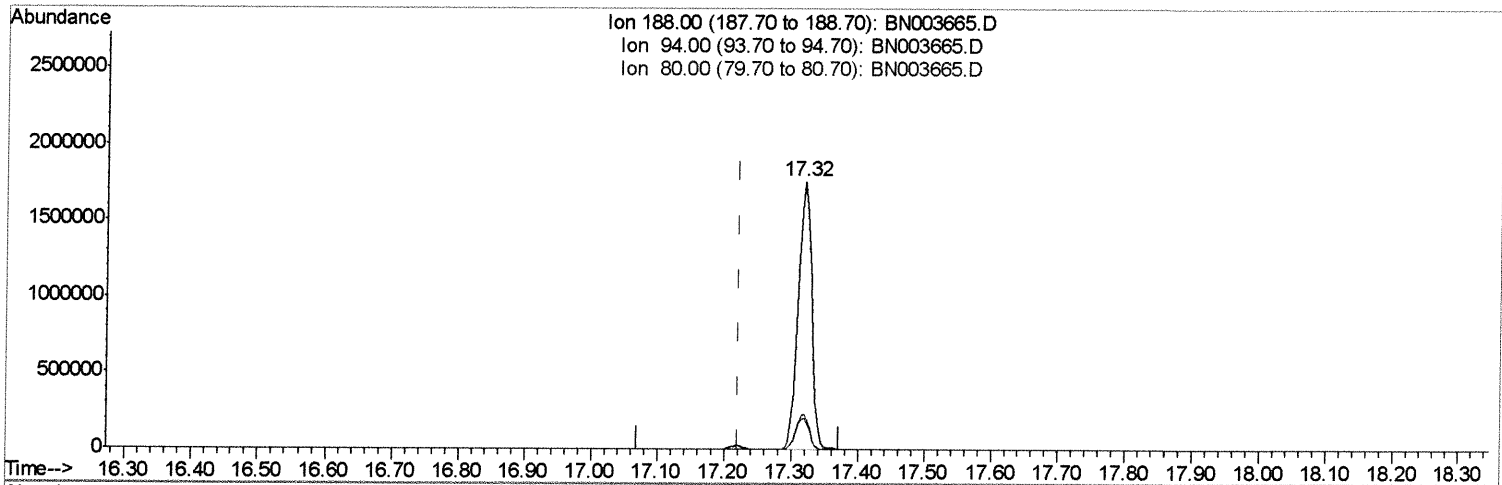

TIC: BN003665.D

(10) Phenanthrene-d10 (I)
17.318min (+0.097) 0.40ng/ul
response 2470683

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	13.03#
80.00	11.60	11.61
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003665.D
Acq On : 01 Dec 2018 16:59
Operator : JU/SJ
Sample : J6096-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4156

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:49 PM

Quant Time: Dec 03 01:19:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 01:15:58 2018
Response via : Initial Calibration

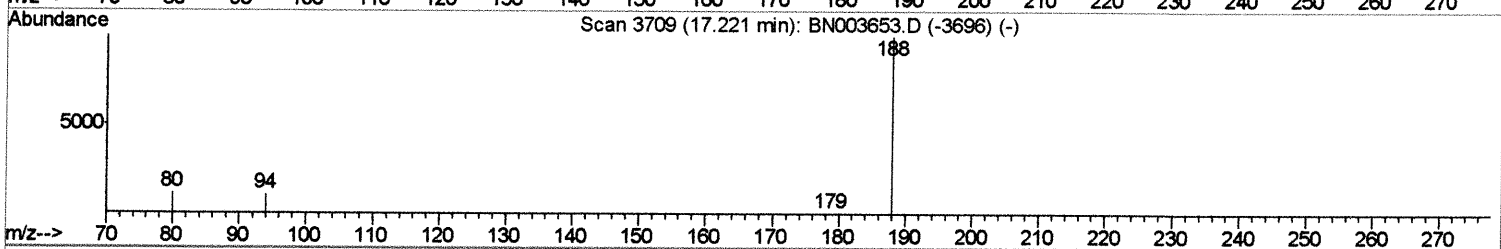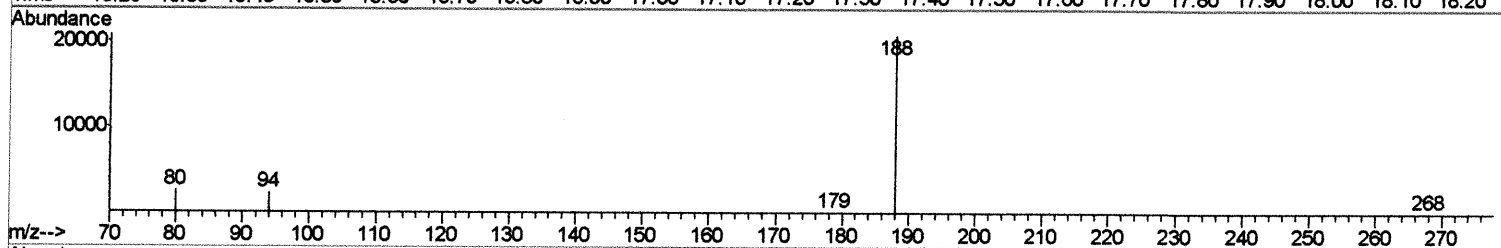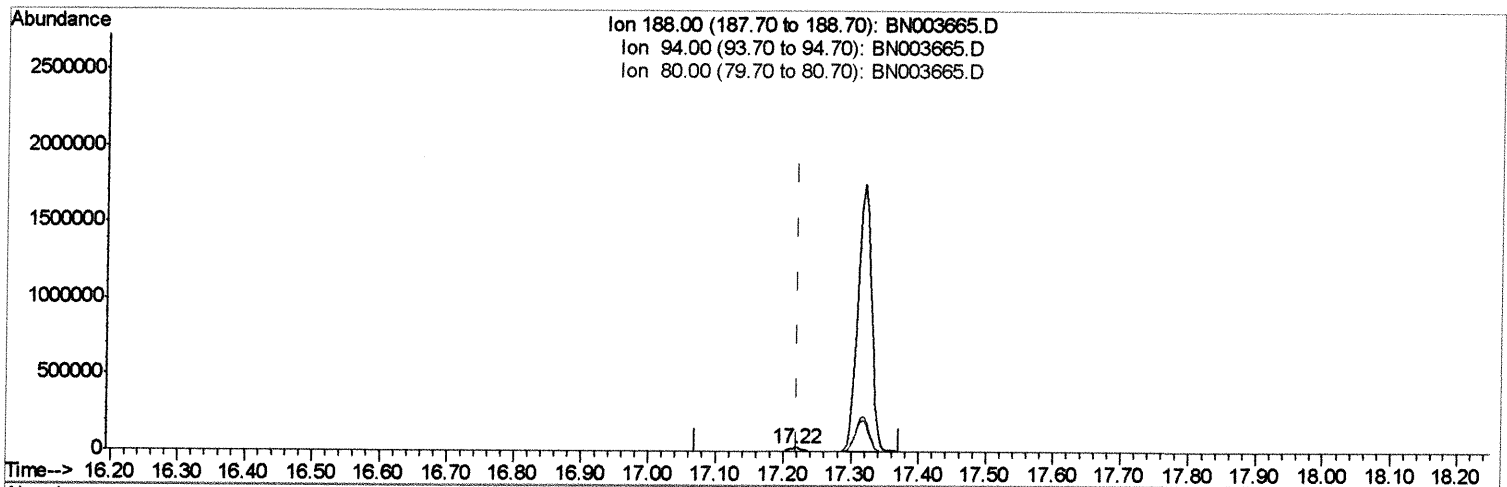

TIC: BN003665.D

(10) Phenanthrene-d10 (I)

17.217min (-0.004) 0.40ng/ul m > 50 12/11/18

response 30025

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	11.06
80.00	11.60	12.35
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003665.D
Acq On : 01 Dec 2018 16:59
Operator : JU/SJ
Sample : J6096-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4156

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:49 PM

Quant Time: Dec 03 01:58:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 01:15:58 2018
Response via : Initial Calibration

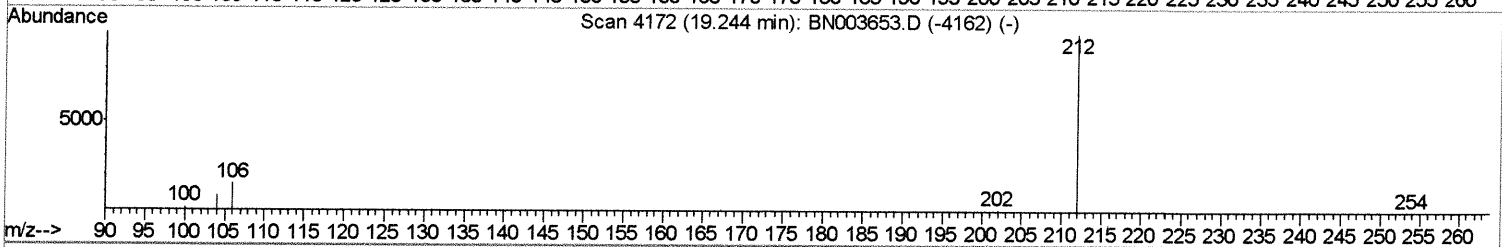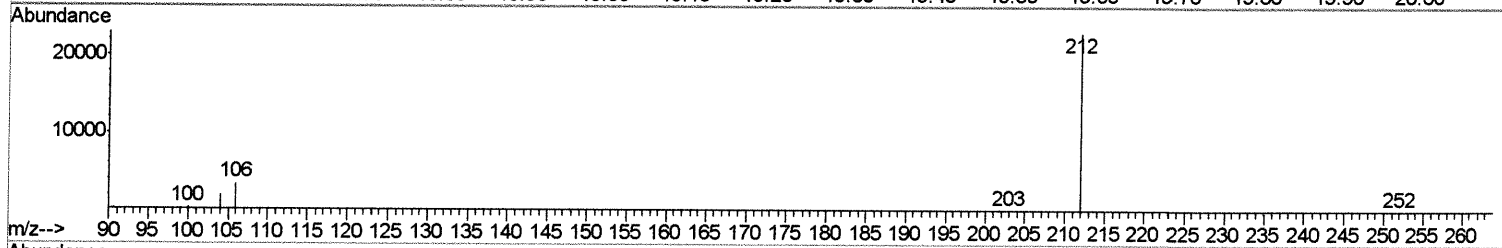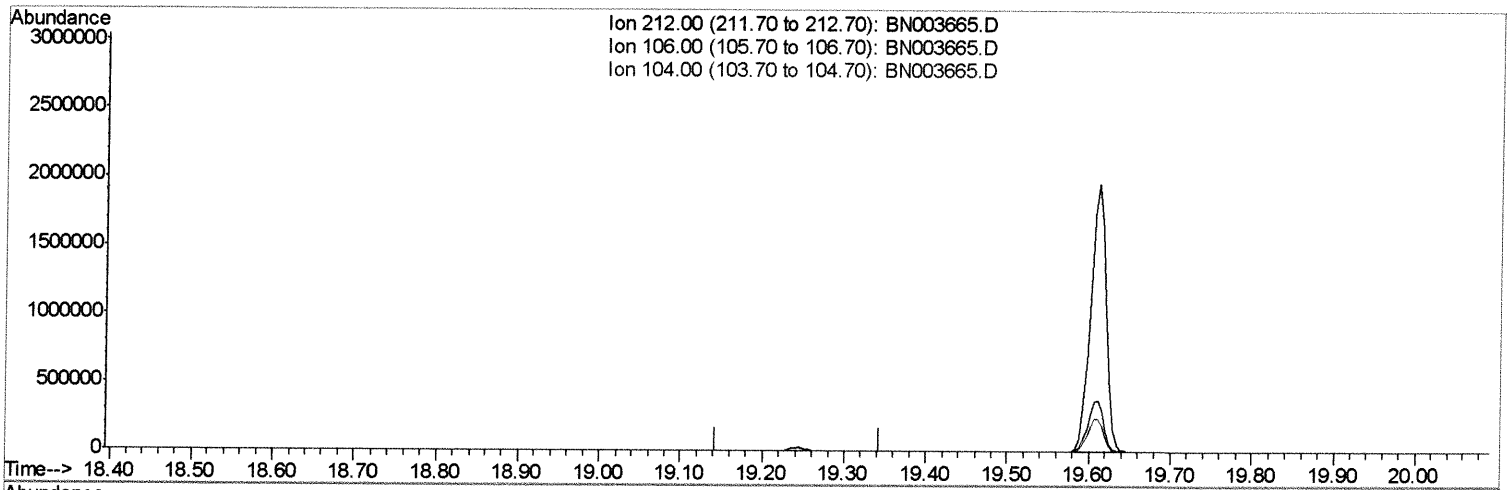

TIC: BN003665.D

(14) Fluoranthene-d10 (SURR)

19.244min (-19.244) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003665.D
Acq On : 01 Dec 2018 16:59
Operator : JU/SJ
Sample : J6096-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4156

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:49 PM

Quant Time: Dec 03 01:58:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 01:15:58 2018
Response via : Initial Calibration

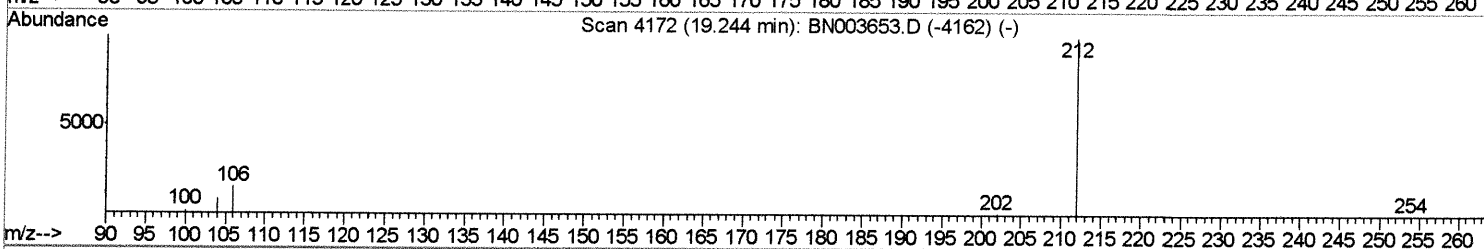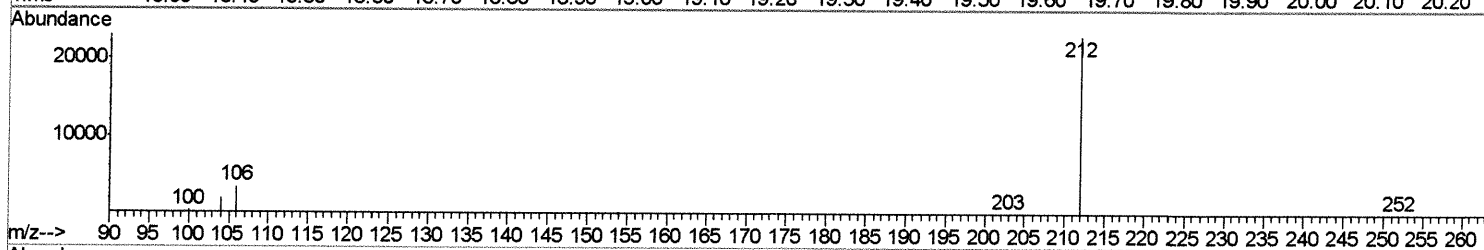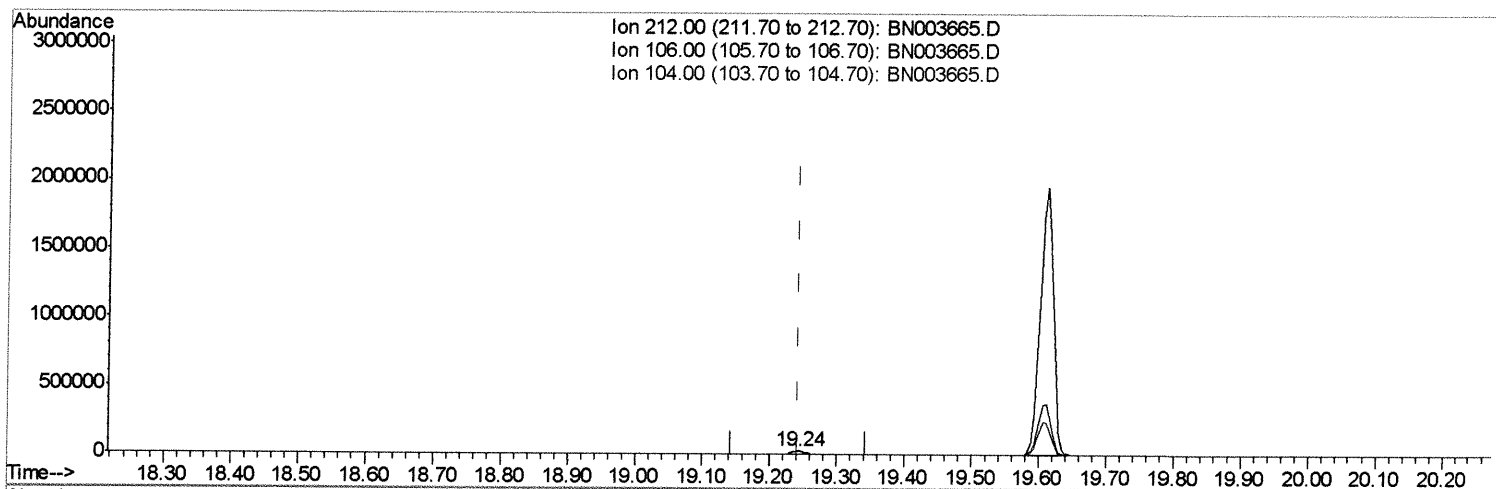

TIC: BN003665.D

(14) Fluoranthene-d10 (SURR)

19.243min (-0.000) 0.36ng/ul m) SJ 12/11/18

response 31513

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003665.D
Acq On : 01 Dec 2018 16:59
Operator : JU/SJ
Sample : J6096-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4156

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:49 PM

Quant Time: Dec 03 01:58:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 01:15:58 2018
Response via : Initial Calibration

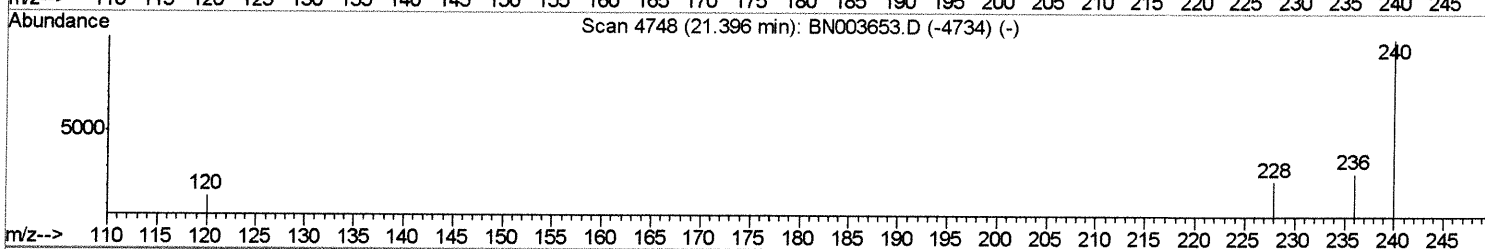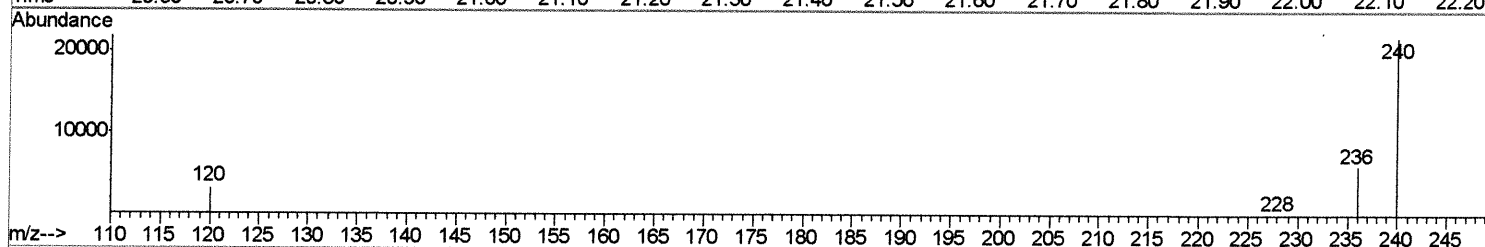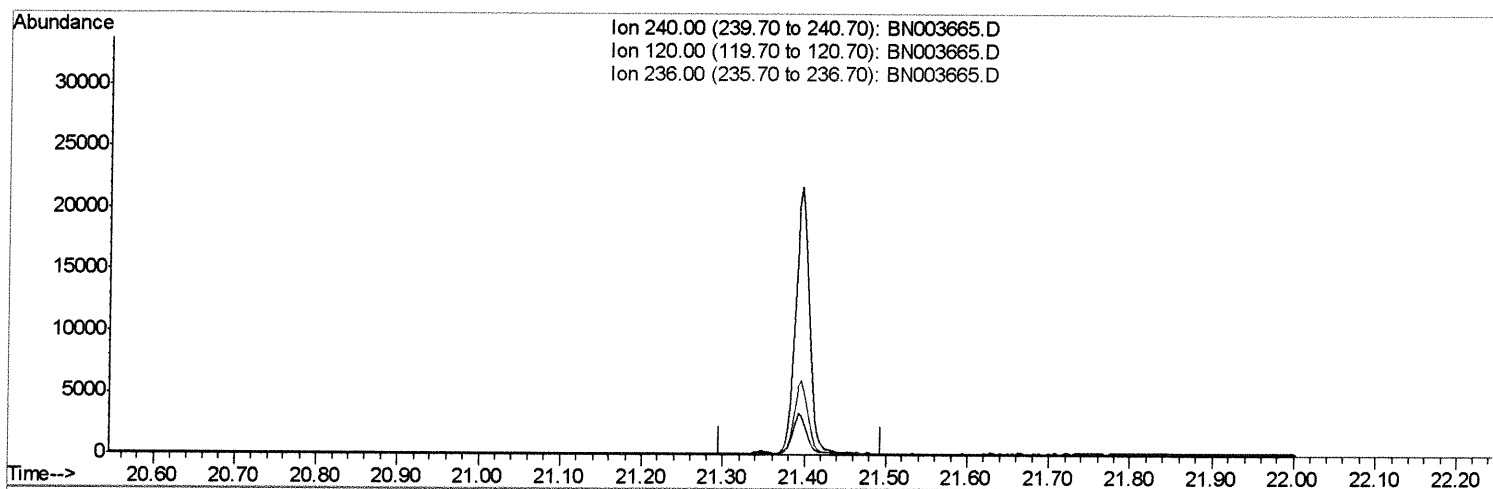

TIC: BN003665.D

(16) Chrysene-d12 (I)

21.396min (-21.396) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003665.D
Acq On : 01 Dec 2018 16:59
Operator : JU/SJ
Sample : J6096-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4156

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:49 PM

Quant Time: Dec 03 01:58:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 01:15:58 2018
Response via : Initial Calibration

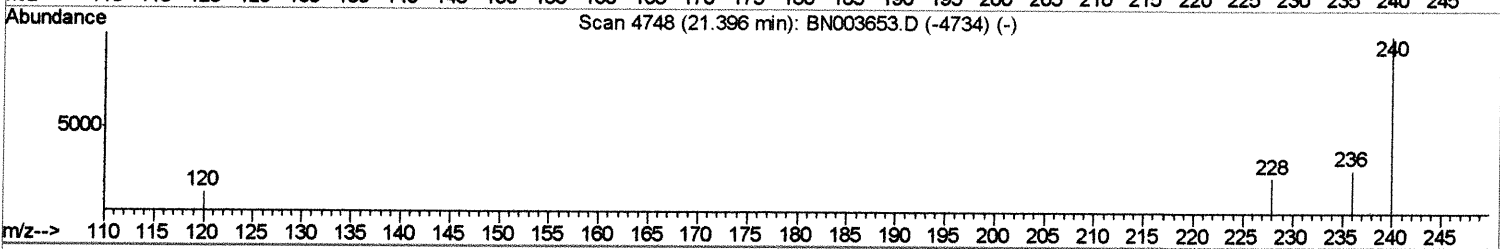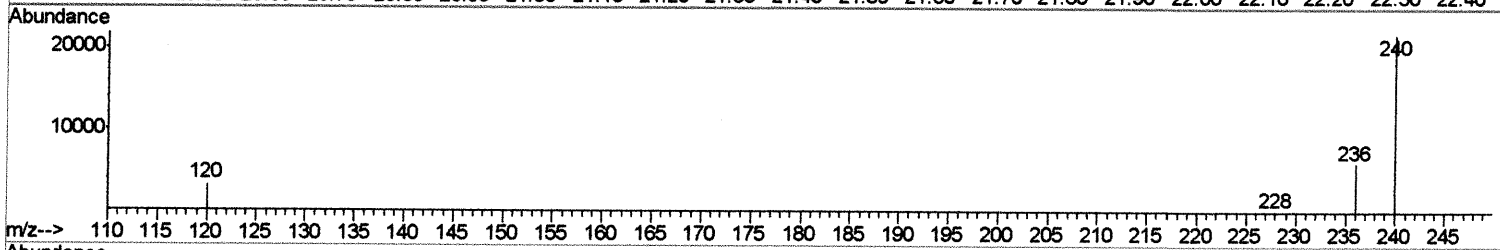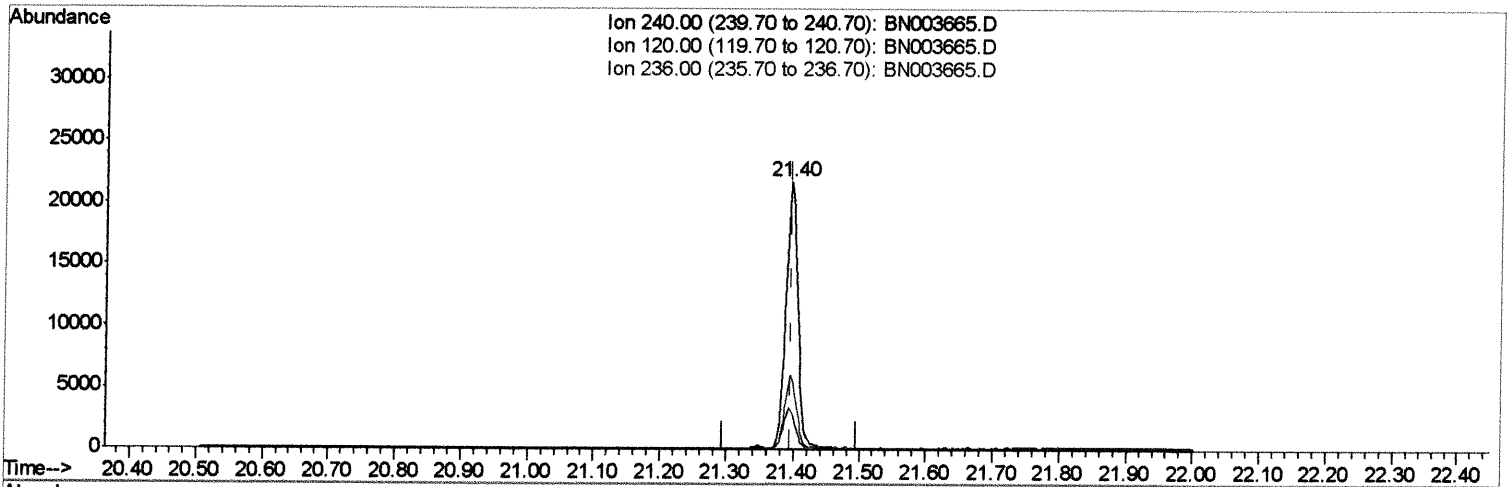

TIC: BN003665.D

(16) Chrysene-d12 (I)

21.395min (-0.000) 0.40ng/ul m) SJ 12/11/18

response 26958

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	14.75
236.00	27.60	27.63
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003665.D
Acq On : 01 Dec 2018 16:59
Operator : JU/SJ
Sample : J6096-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A4156

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:49 PM

Quant Time: Dec 03 01:59:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 01:15:58 2018
Response via : Initial Calibration

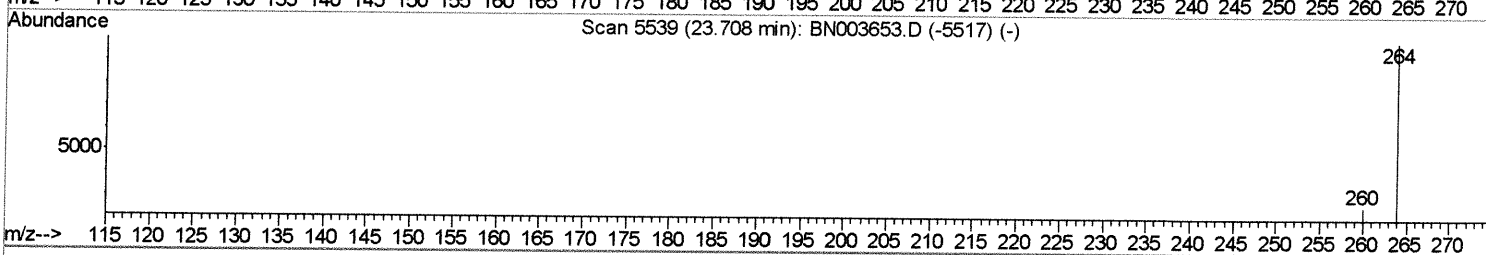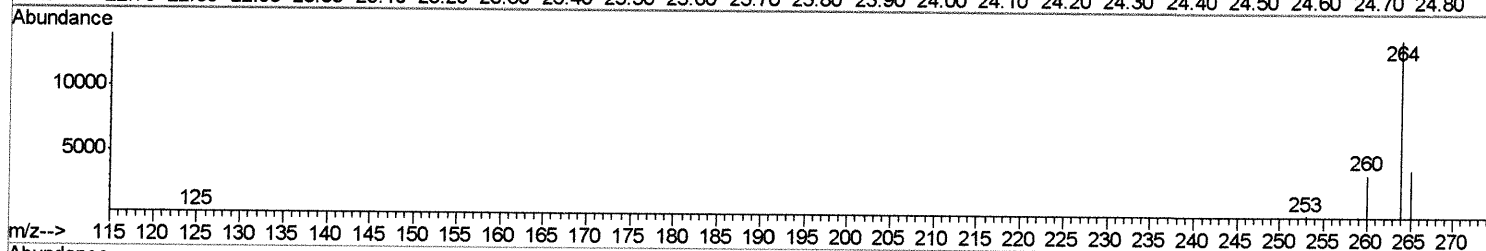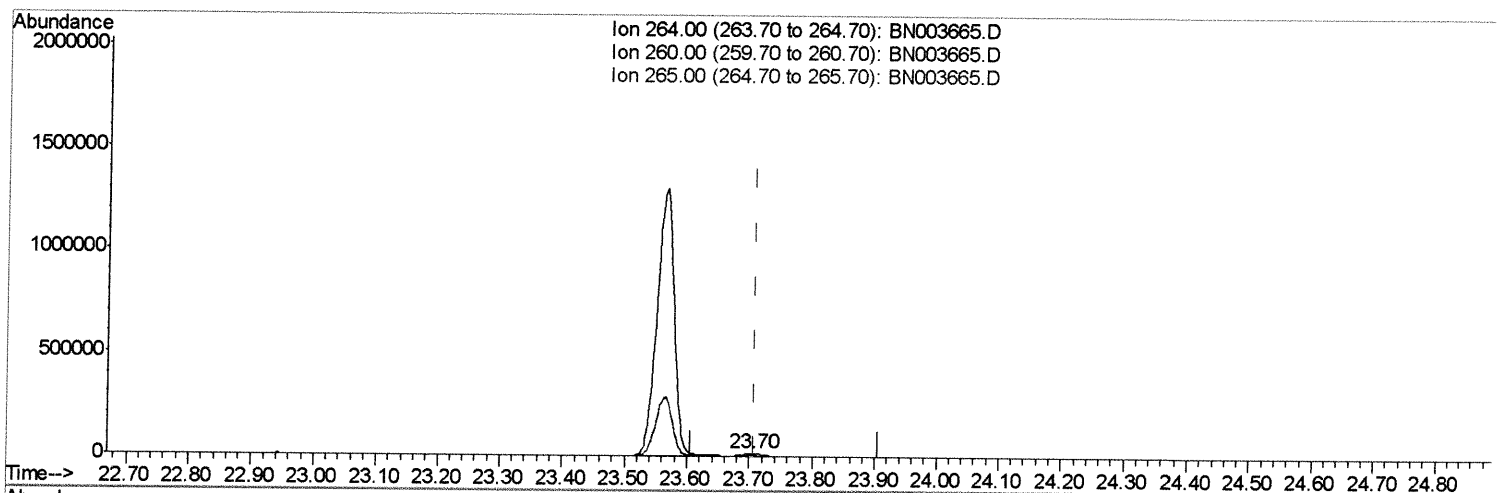

TIC: BN003665.D

(20) Perylene-d12 (I)

23.705min (-0.003) 0.40ng/ul

response 32192

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	25.43
265.00	33.50	28.34
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003665.D
Acq On : 01 Dec 2018 16:59
Operator : JU/SJ
Sample : J6096-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4156

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:49 PM

Quant Time: Dec 03 01:59:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 01:15:58 2018
Response via : Initial Calibration

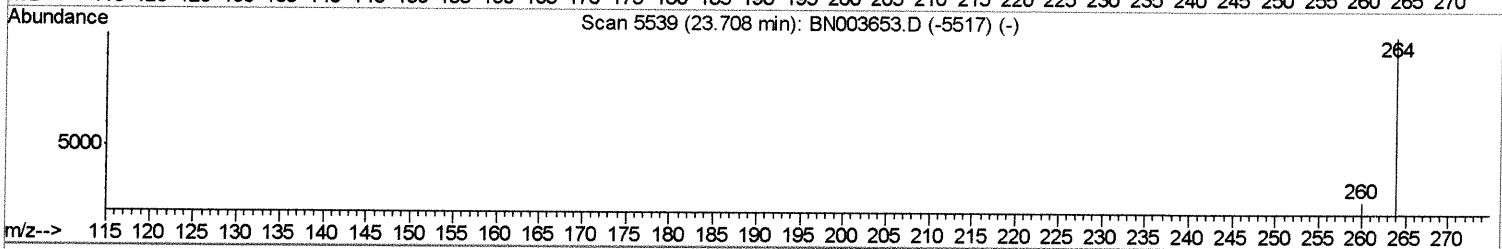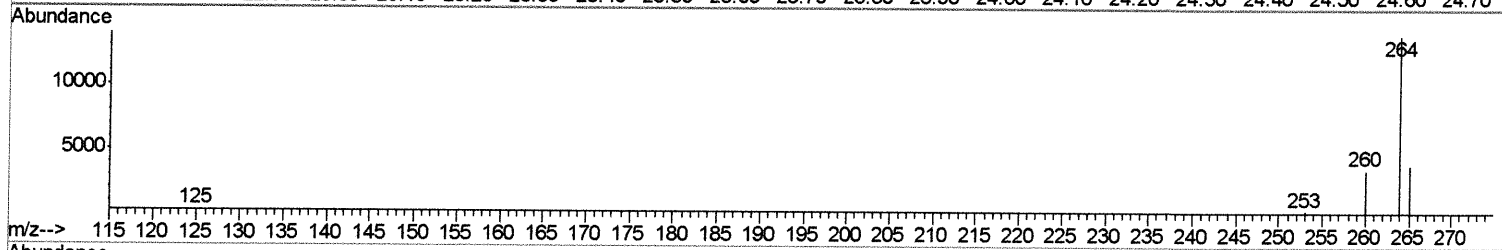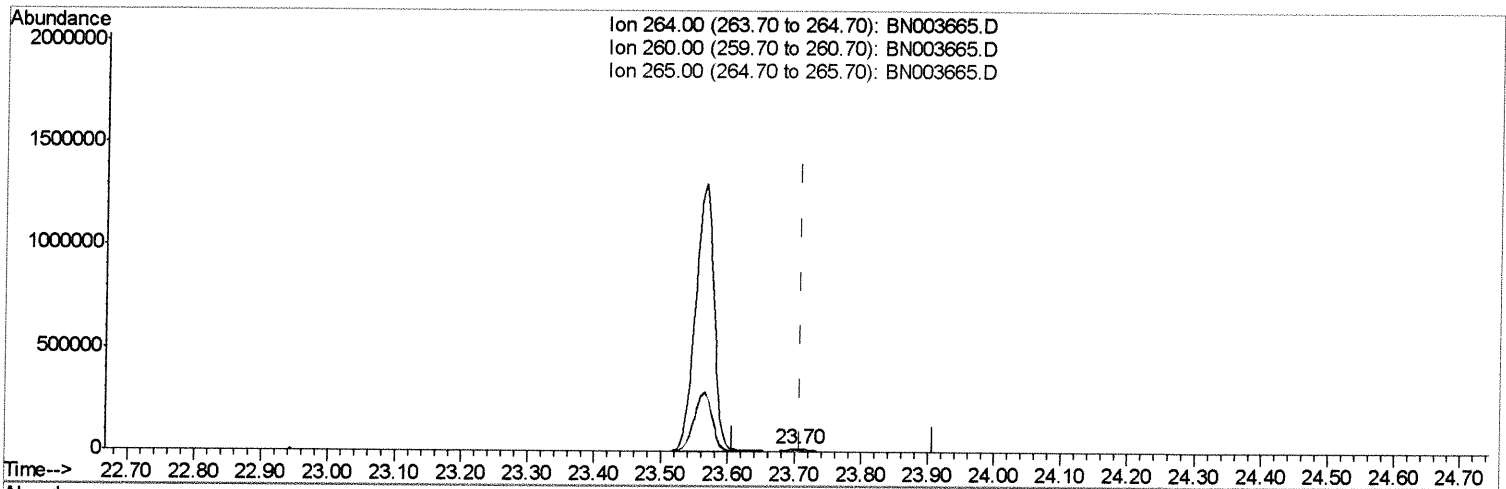

TIC: BN003665.D

(20) Perylene-d12 (I)

23.705min (-0.003) 0.40ng/ul m³

SD 12/11/18

response 22654

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	25.43
265.00	33.50	28.34
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (QT Reviewed)

Data File : BN003665.D
Acq On : 01 Dec 2018 16:59
Operator : JU/SJ
Sample : J6096-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4156

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:49 PM

Quant Time: Dec 03 02:00:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 01:15:58 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	6088	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	24877	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	14298	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	30025m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	26958m	0.40	ng/ul	0.00
20) Perylene-d12	23.70	264	22654m	0.40	ng/ul	0.00

SD 12/11/18

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.23	152	13879	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	31513m	0.36	ng/ul	0.00

SD 12/11/18

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed