

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (QT Reviewed)


Data File : BN003667.D
Acq On : 01 Dec 2018 19:21
Operator : JU/SJ
Sample : PB115227BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK27

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:51 PM

Quant Time: Dec 03 02:08:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 02:00:08 2018
Response via : Initial Calibration

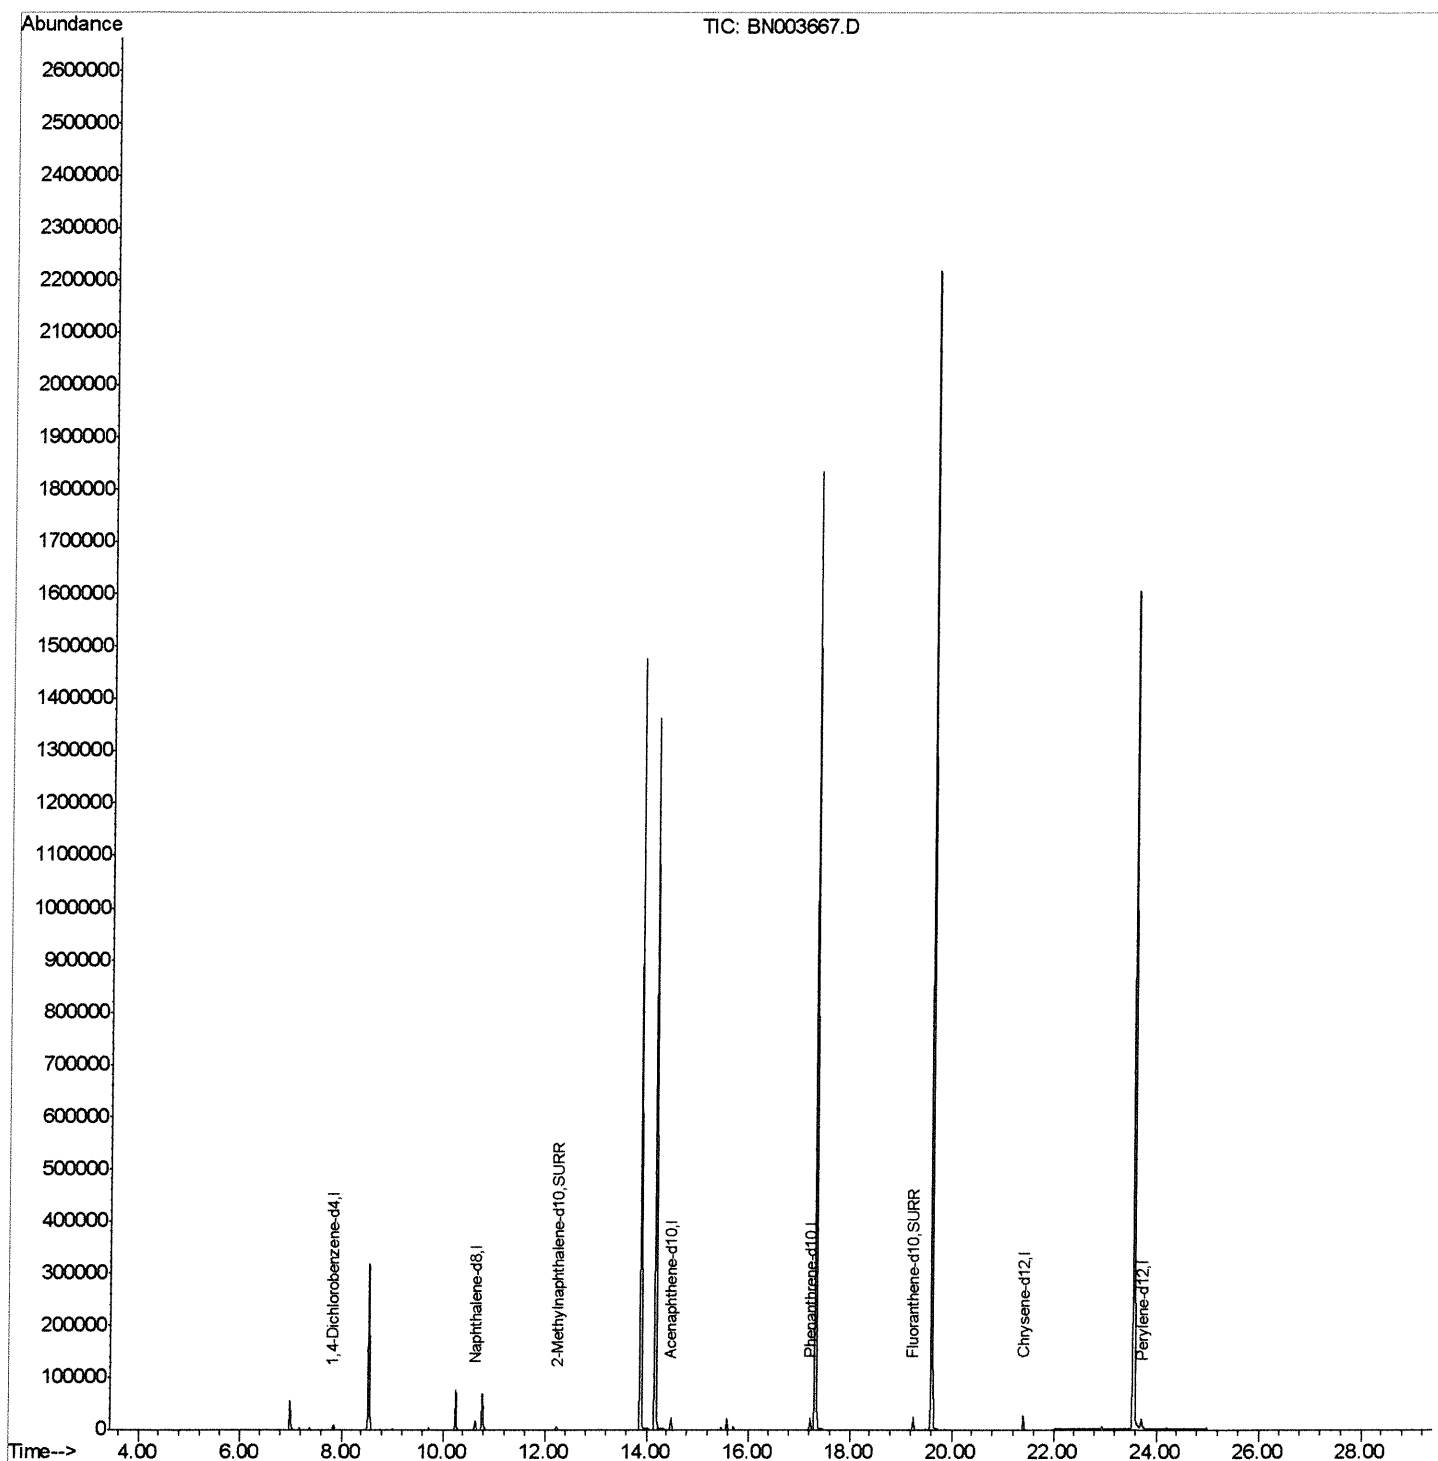

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003667.D
Acq On : 01 Dec 2018 19:21
Operator : JU/SJ
Sample : PB115227BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK27

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:51 PM

Quant Time: Dec 03 02:02:49 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 02:00:08 2018
Response via : Initial Calibration

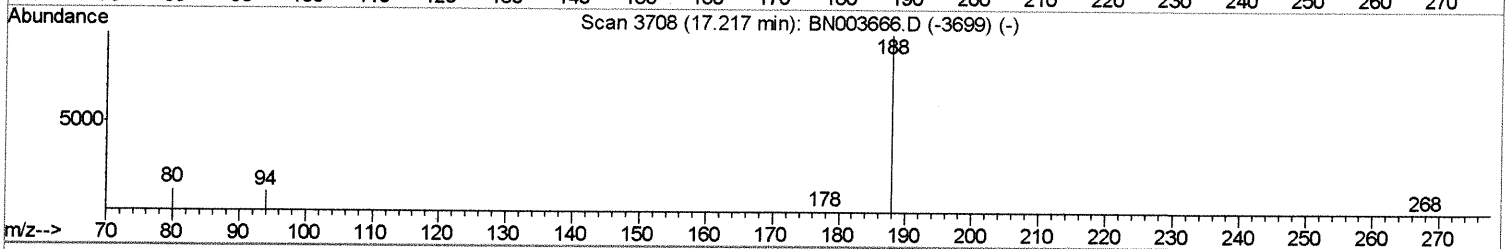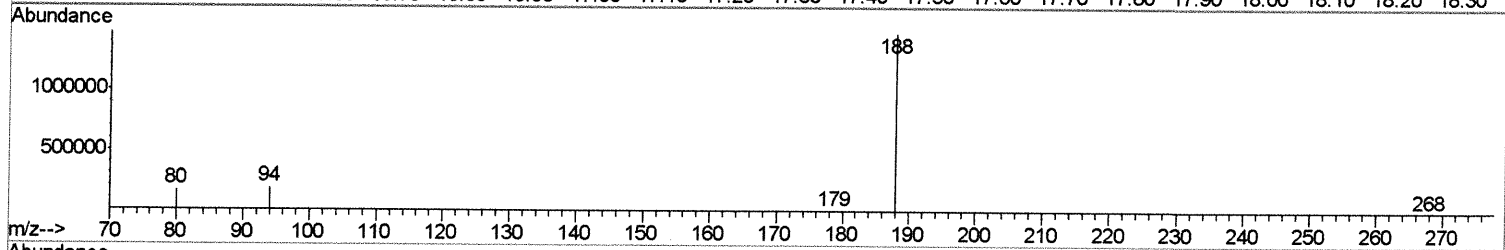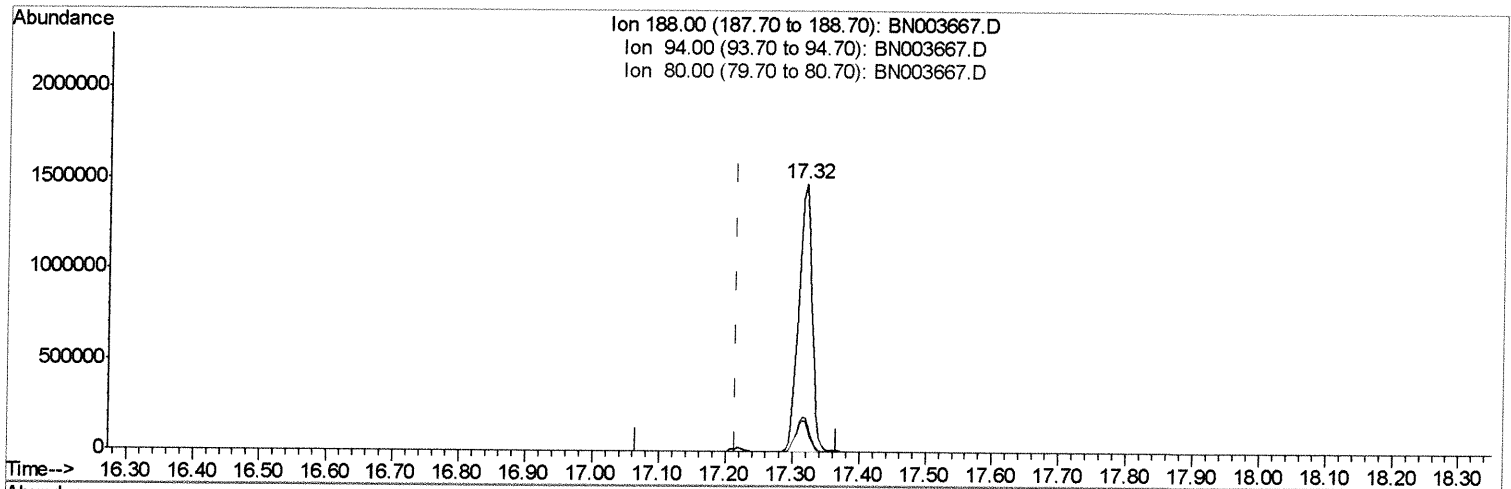

TIC: BN003667.D

(10) Phenanthrene-d10 (I)

17.318min (+0.102) 0.40ng/ul

response 2044631

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	12.69#
80.00	11.60	11.22
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003667.D
Acq On : 01 Dec 2018 19:21
Operator : JU/SJ
Sample : PB115227BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK27

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:51 PM

Quant Time: Dec 03 02:02:49 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 02:00:08 2018
Response via : Initial Calibration

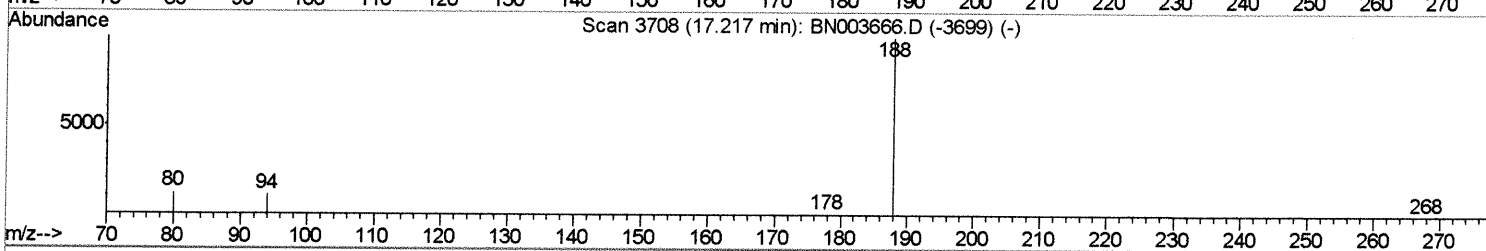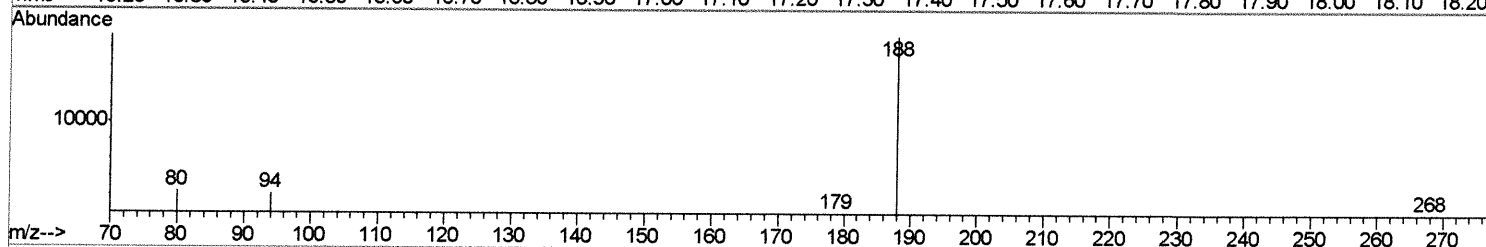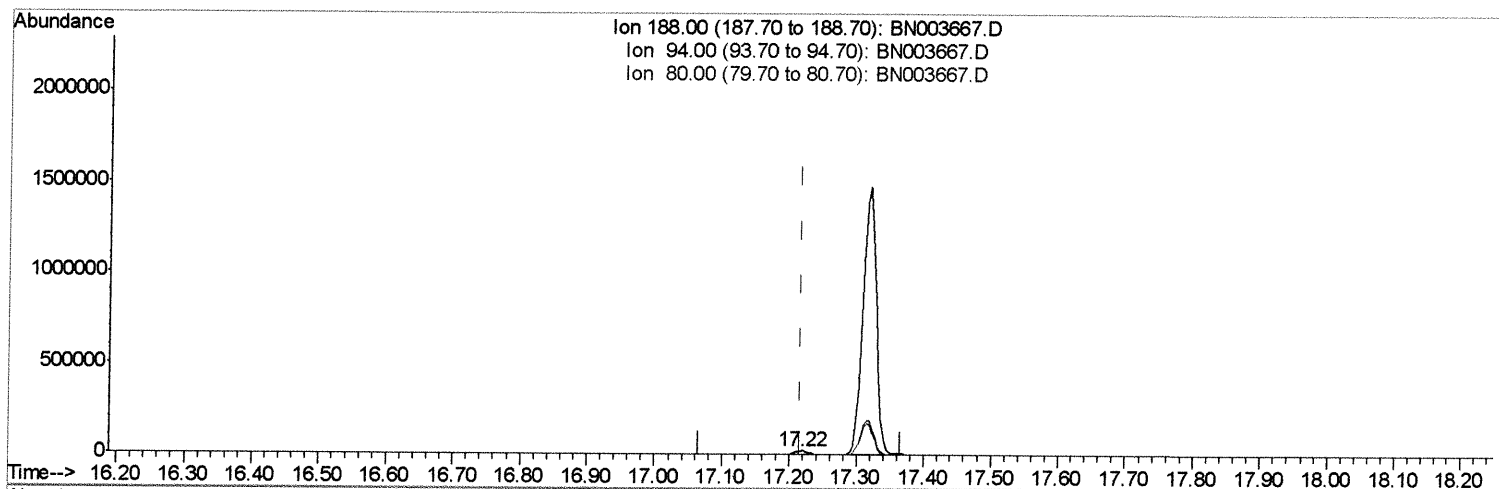

TIC: BN003667.D

(10) Phenanthrene-d10 (I)

17.217min (+0.000) 0.40ng/ul m

50 12/11/18

response 26282

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	11.16
80.00	11.60	12.28
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003667.D
Acq On : 01 Dec 2018 19:21
Operator : JU/SJ
Sample : PB115227BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK27

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:51 PM

Quant Time: Dec 03 02:06:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 02:00:08 2018
Response via : Initial Calibration

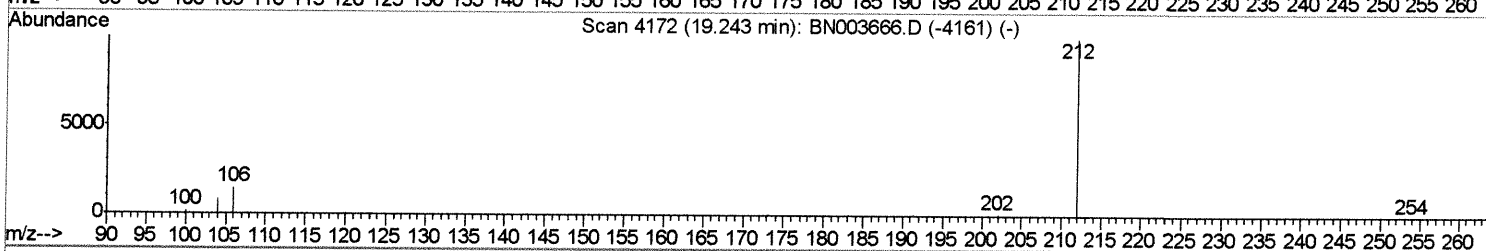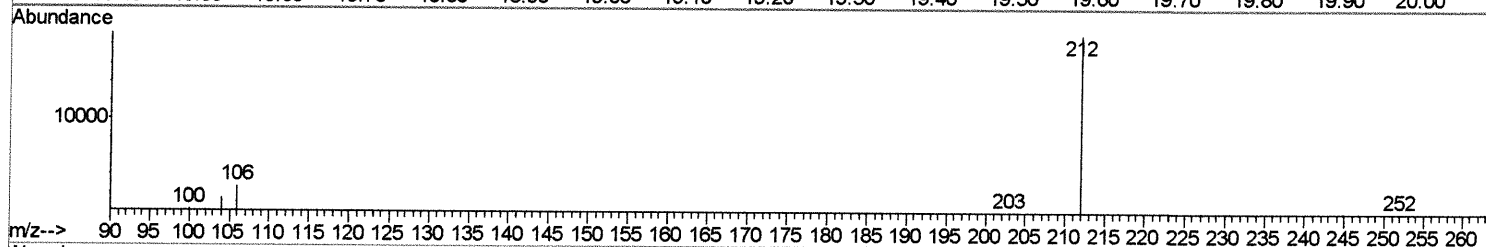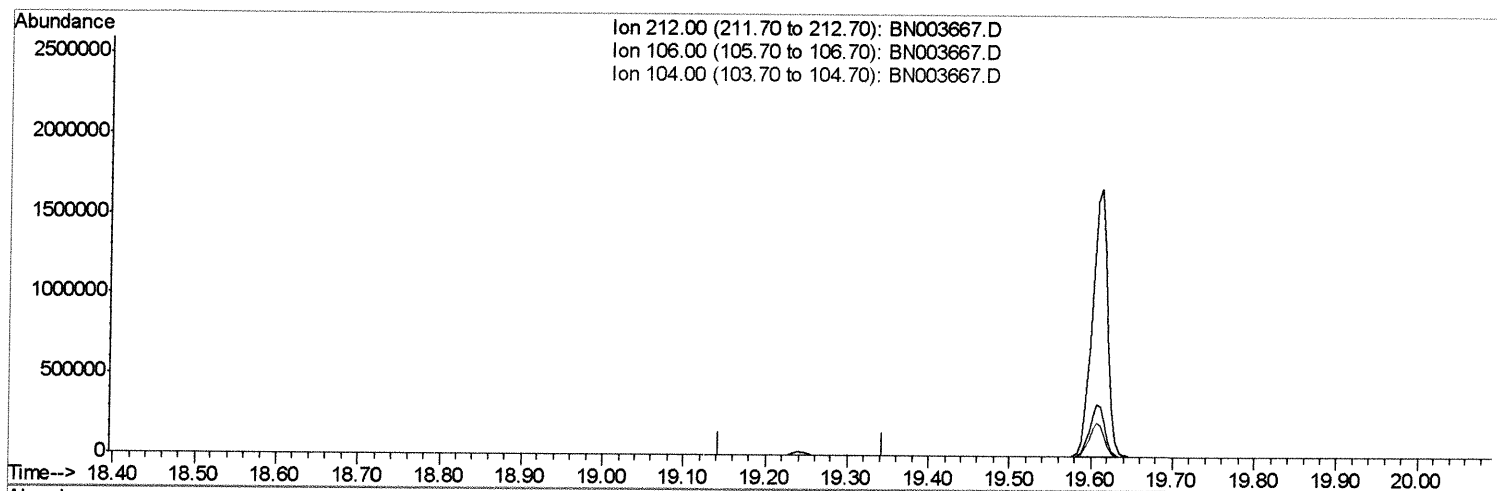

TIC: BN003667.D

(14) Fluoranthene-d10 (SURR)

19.243min (-19.243) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003667.D
Acq On : 01 Dec 2018 19:21
Operator : JU/SJ
Sample : PB115227BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK27

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:51 PM

Quant Time: Dec 03 02:06:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 02:00:08 2018
Response via : Initial Calibration

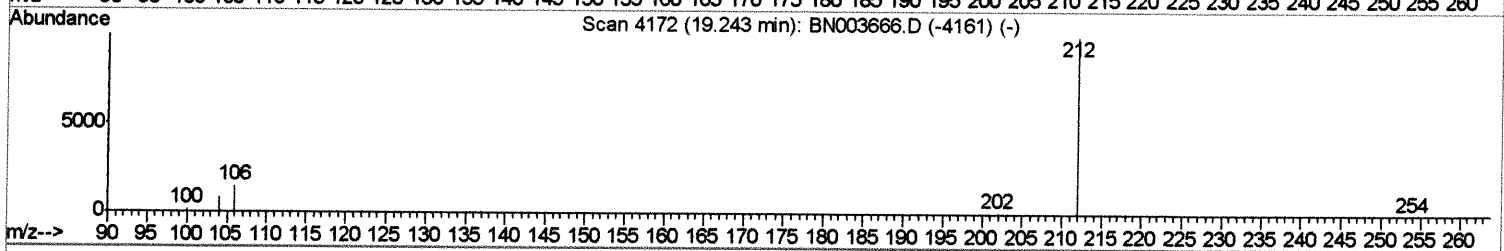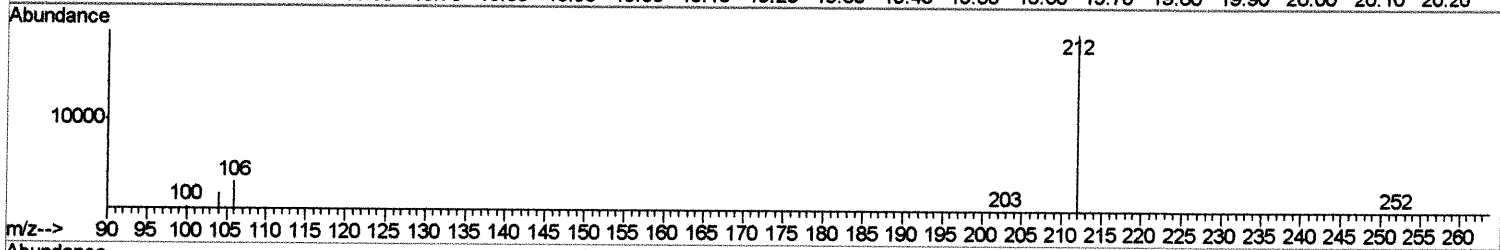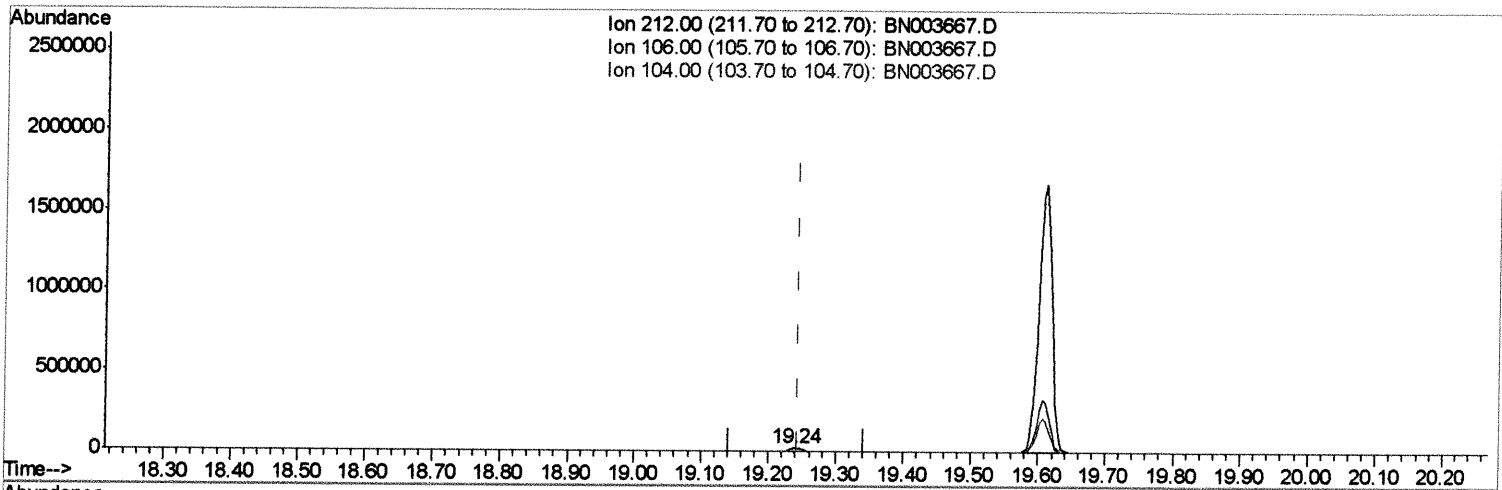

(14) Fluoranthene-d10 (SURR)

19.239min (-0.004) 0.34ng/ul m > SD 12/11/18

response 26123

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003667.D
Acq On : 01 Dec 2018 19:21
Operator : JU/SJ
Sample : PB115227BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK27

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:51 PM

Quant Time: Dec 03 02:06:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 02:00:08 2018
Response via : Initial Calibration

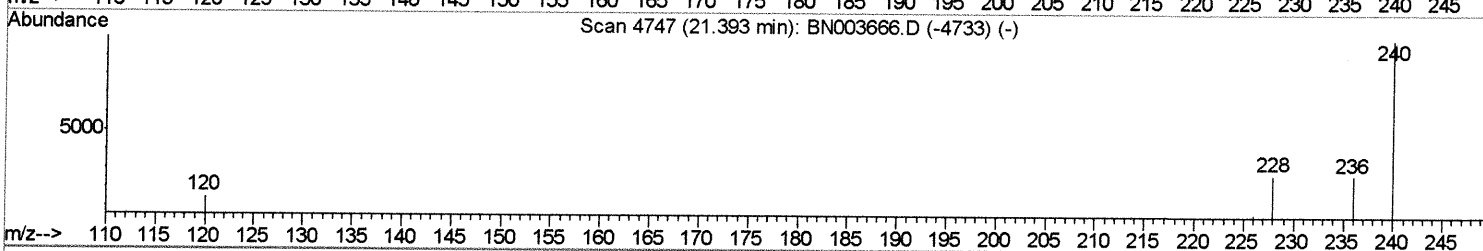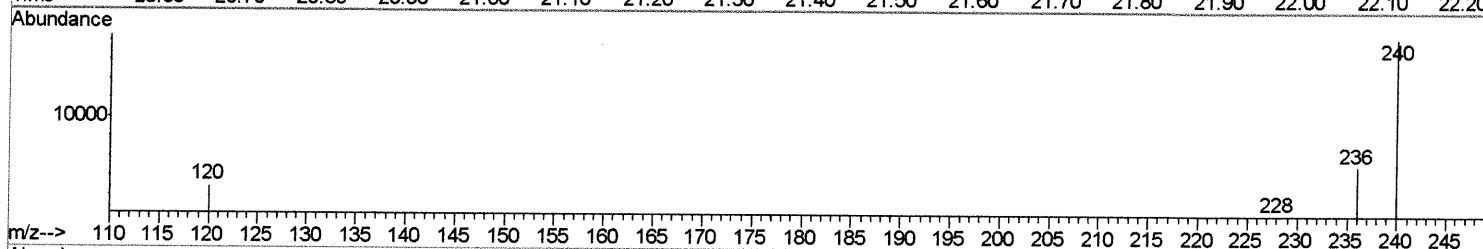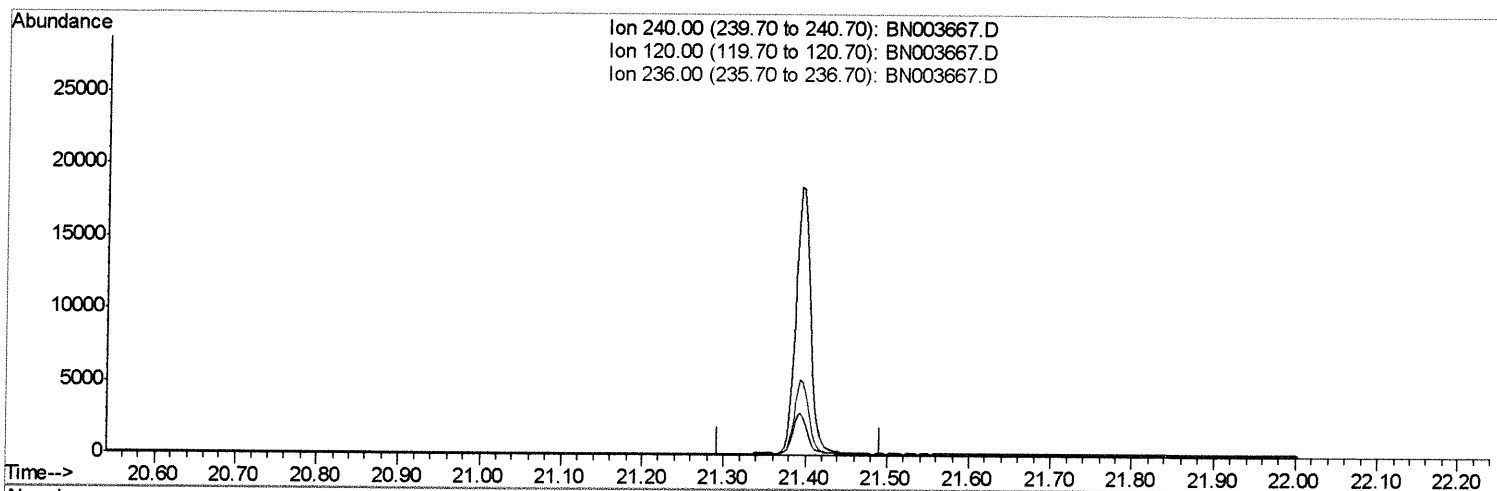

TIC: BN003667.D

(16) Chrysene-d12 (I)

21.393min (-21.393) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003667.D
Acq On : 01 Dec 2018 19:21
Operator : JU/SJ
Sample : PB115227BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK27

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:51 PM

Quant Time: Dec 03 02:06:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 02:00:08 2018
Response via : Initial Calibration

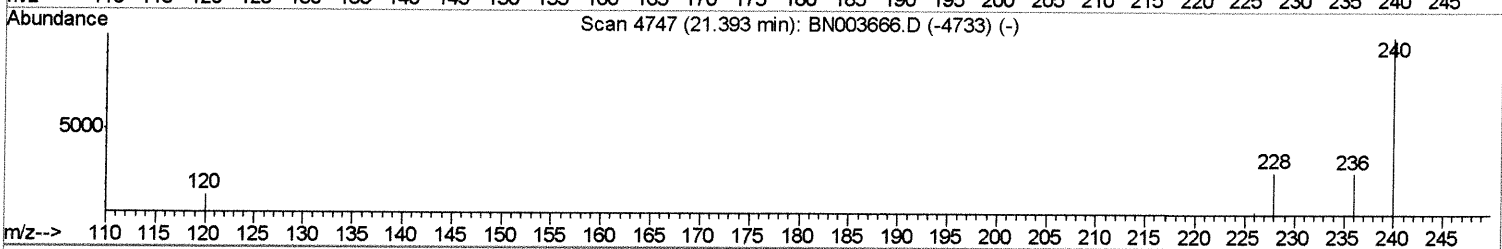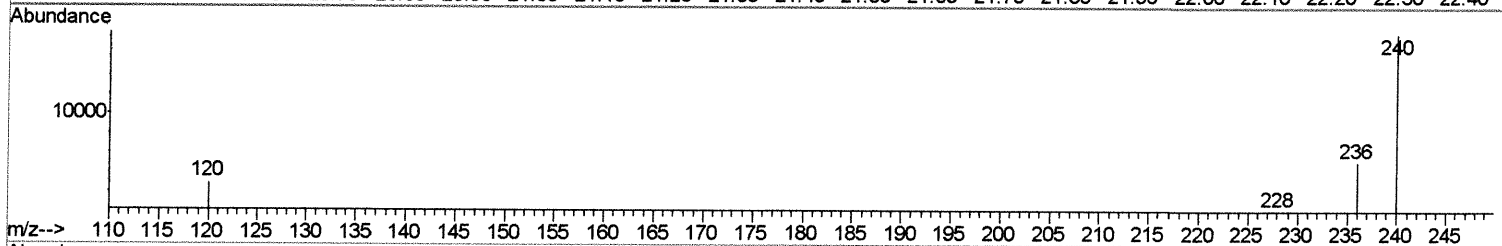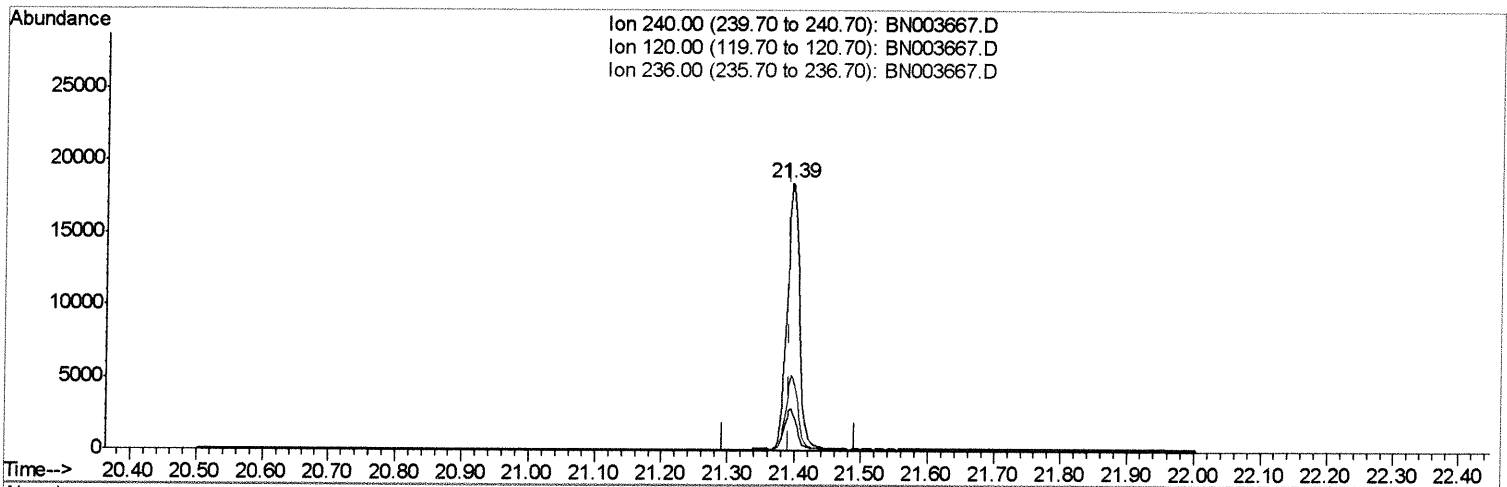

TIC: BN003667.D

(16) Chrysene-d12 (I)

21.394min (+0.001) 0.40ng/ul m

50 12/11/18

response 23776

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	15.72
236.00	27.60	28.06
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003667.D
Acq On : 01 Dec 2018 19:21
Operator : JU/SJ
Sample : PB115227BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK27

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:51 PM

Quant Time: Dec 03 02:07:33 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 02:00:08 2018
Response via : Initial Calibration

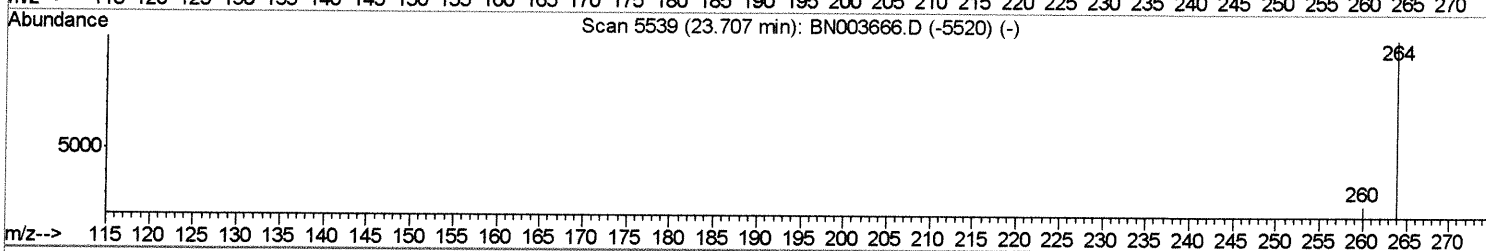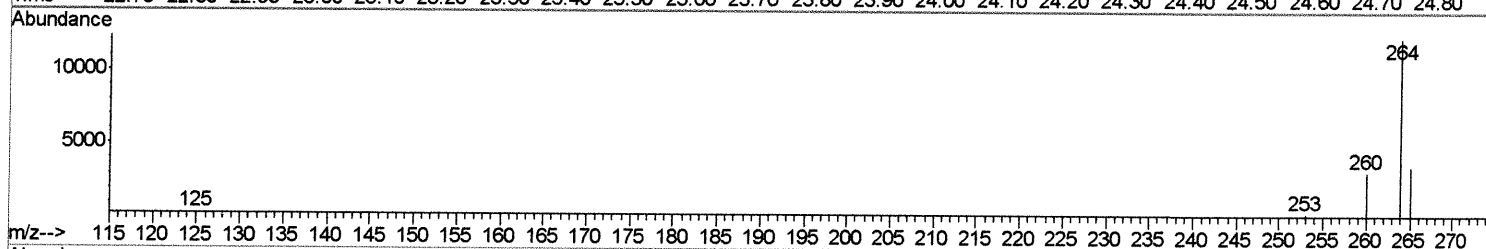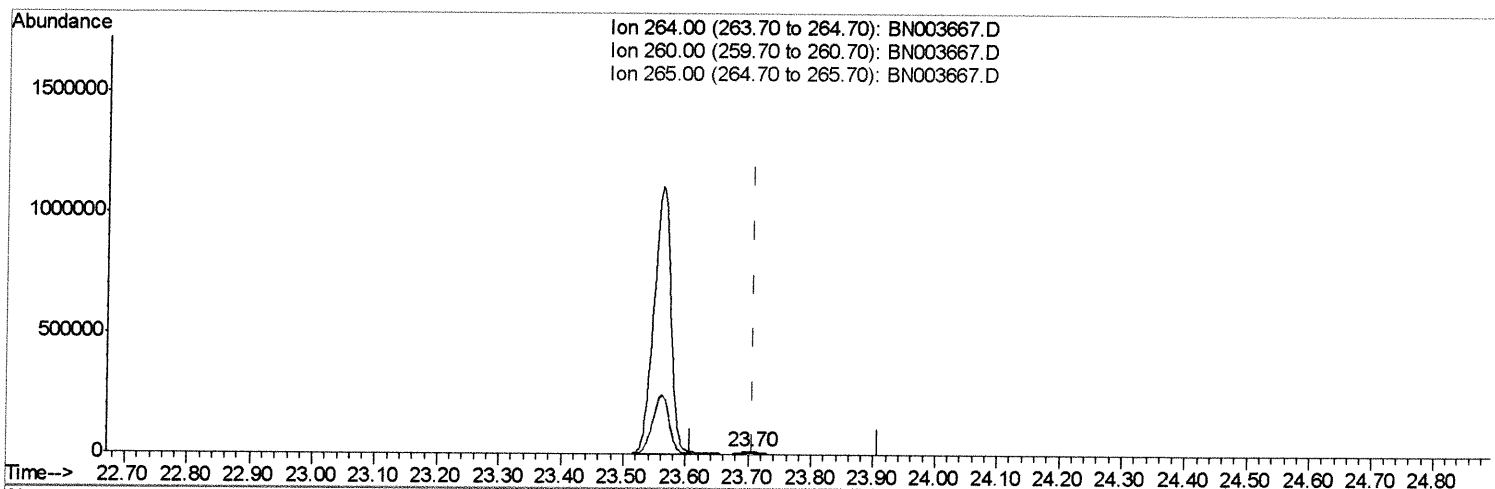

TIC: BN003667.D

(20) Perylene-d12 (I)

23.703min (-0.004) 0.40ng/ul

response 28479

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	26.06
265.00	33.50	29.45
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003667.D
Acq On : 01 Dec 2018 19:21
Operator : JU/SJ
Sample : PB115227BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK27

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:51 PM

Quant Time: Dec 03 02:07:33 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 02:00:08 2018
Response via : Initial Calibration

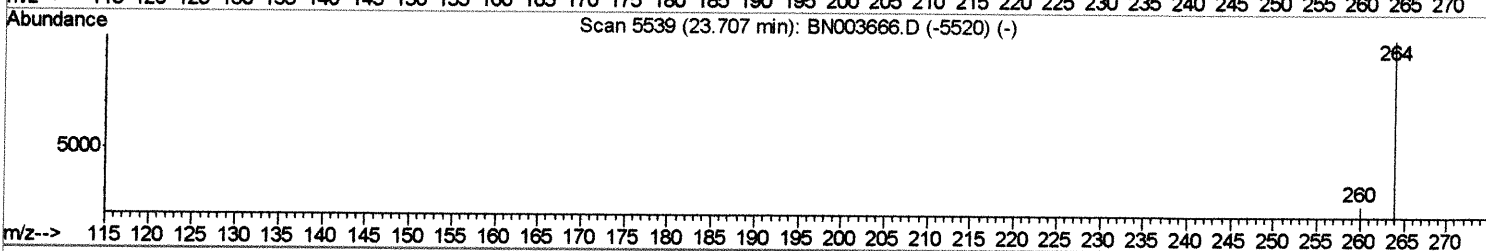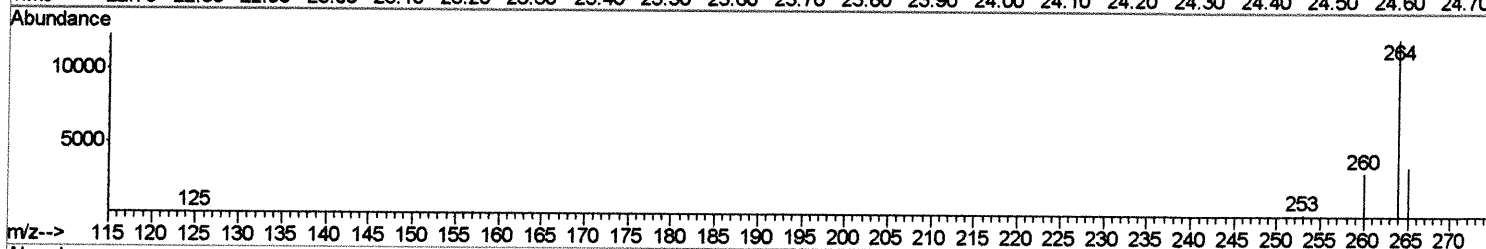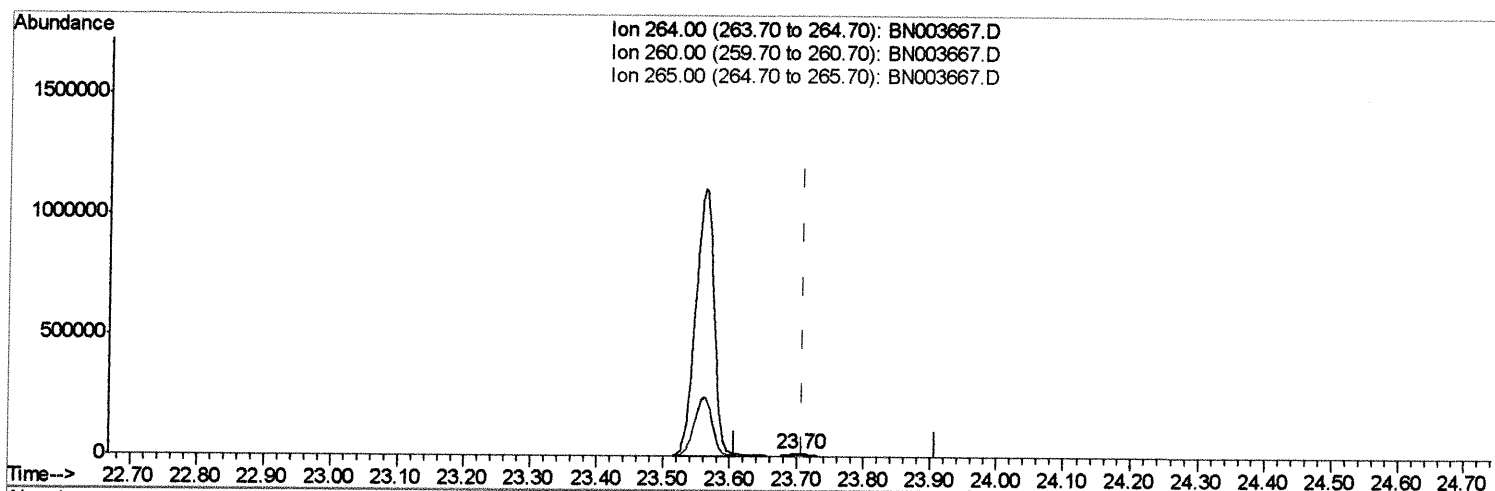

TIC: BN003667.D

(20) Perylene-d12 (I)

23.703min (-0.004) 0.40ng/ul m> 50 12/11/18

response 20625

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	26.06
265.00	33.50	29.45
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (QT Reviewed)

Data File : BN003667.D
Acq On : 01 Dec 2018 19:21
Operator : JU/SJ
Sample : PB115227BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK27

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:51 PM

Quant Time: Dec 03 02:08:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 02:00:08 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5135	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	21063	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	12286	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	26282m	0.40	ng/ul	0.00
16) Chrysene-d12	21.39	240	23776m	0.40	ng/ul	0.00
20) Perylene-d12	23.70	264	20625m	0.40	ng/ul	0.00

SJ 12/11/18

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.23	152	10990	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	26123m	0.34	ng/ul	0.00

SJ 12/11/18

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed