


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (QT Reviewed)
Data File : BN003671.D
Acq On : 01 Dec 2018 21:43
Operator : JU/SJ
Sample : J6096-22
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4188

Manual Integrations
APPROVED

mohammad
12/3/2018 5:02:02 PM

Quant Time: Dec 03 03:00:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 02:00:08 2018
Response via : Initial Calibration

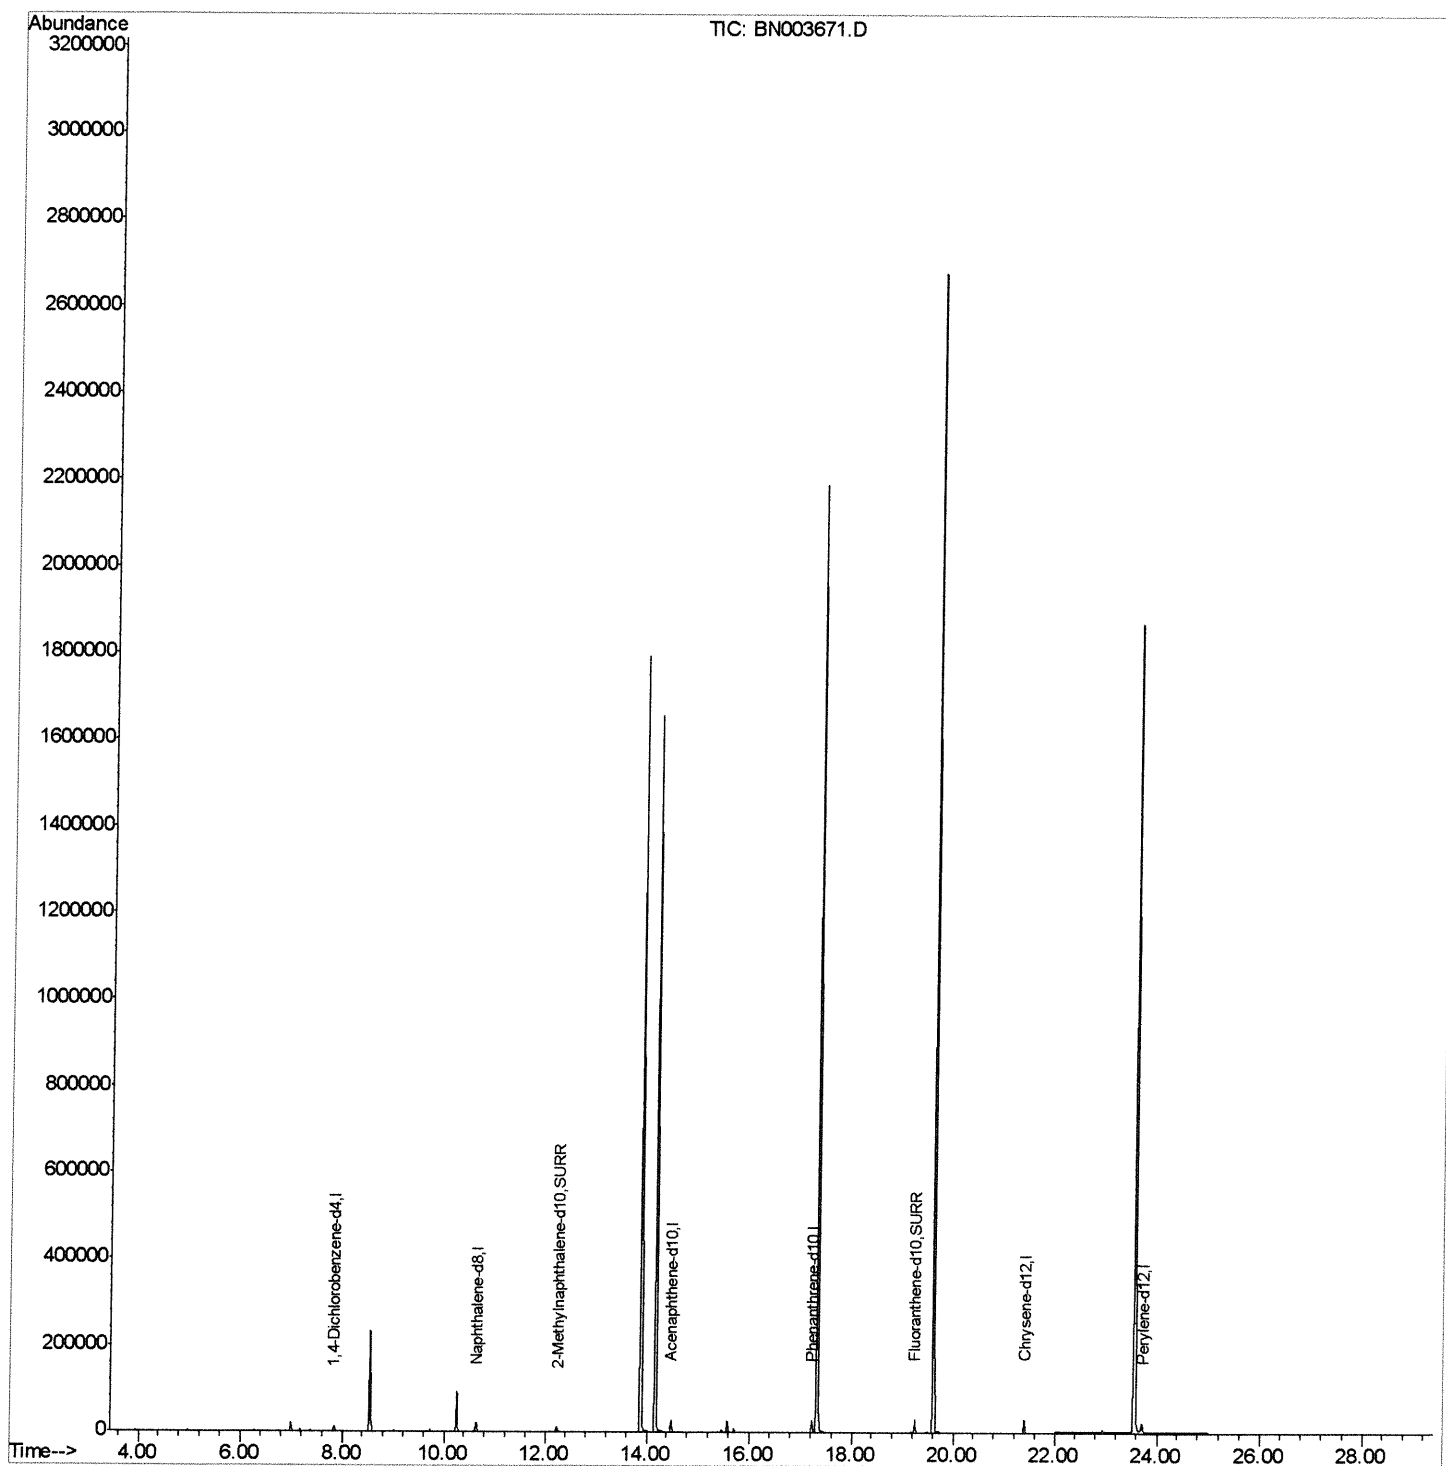

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003671.D
Acq On : 01 Dec 2018 21:43
Operator : JU/SJ
Sample : J6096-22
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4188

Manual Integrations
APPROVED

mohammad
12/3/2018 5:02:02 PM

Quant Time: Dec 03 02:03:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 02:00:08 2018
Response via : Initial Calibration

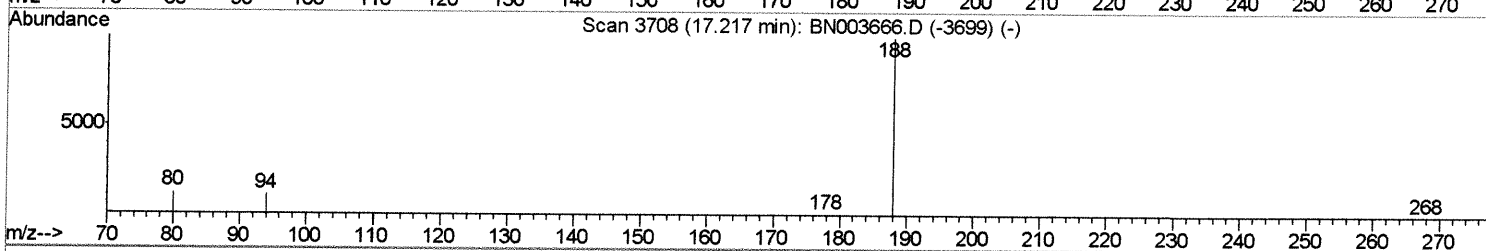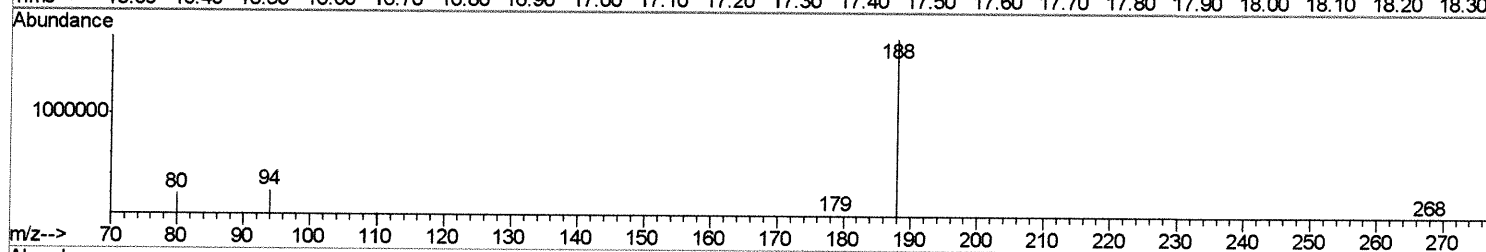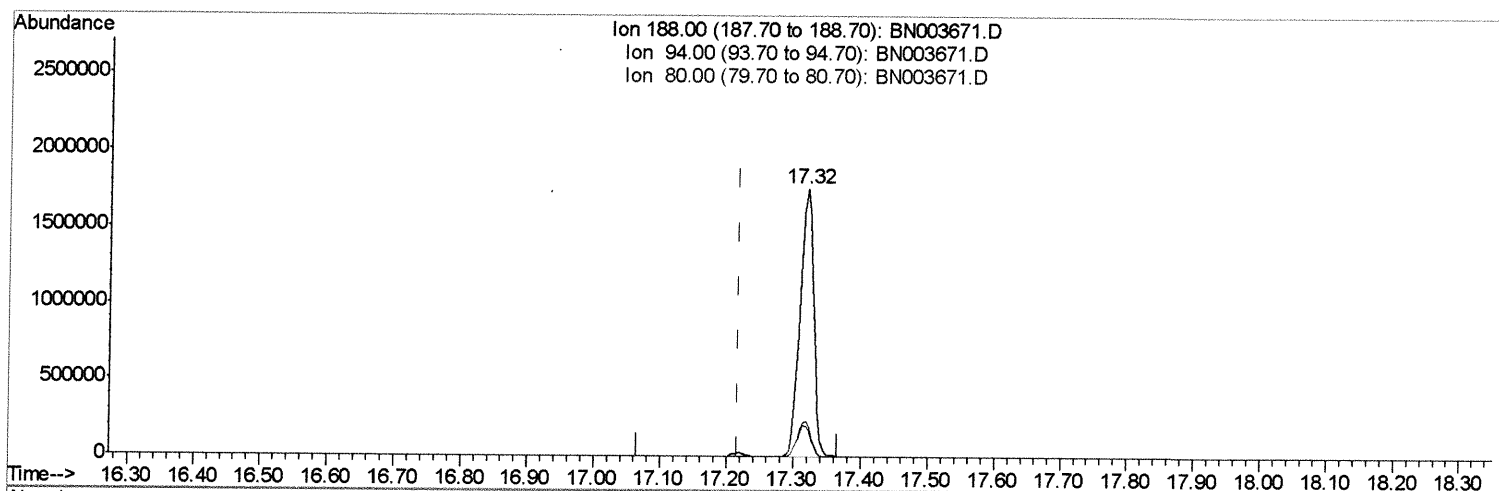

TIC: BN003671.D

(10) Phenanthrene-d10 (I)

17.318min (+0.101) 0.40ng/ul

response 2478178

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	13.02#
80.00	11.60	11.56
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003671.D
Acq On : 01 Dec 2018 21:43
Operator : JU/SJ
Sample : J6096-22
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4188

Manual Integrations
APPROVED

mohammad
12/3/2018 5:02:02 PM

Quant Time: Dec 03 02:03:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 02:00:08 2018
Response via : Initial Calibration

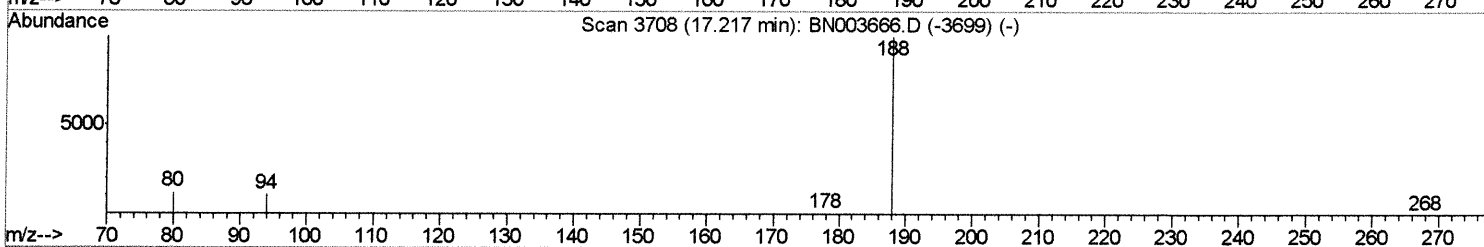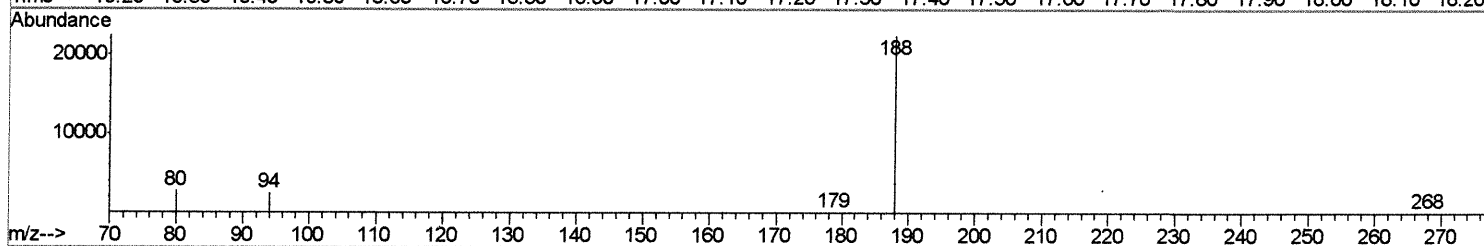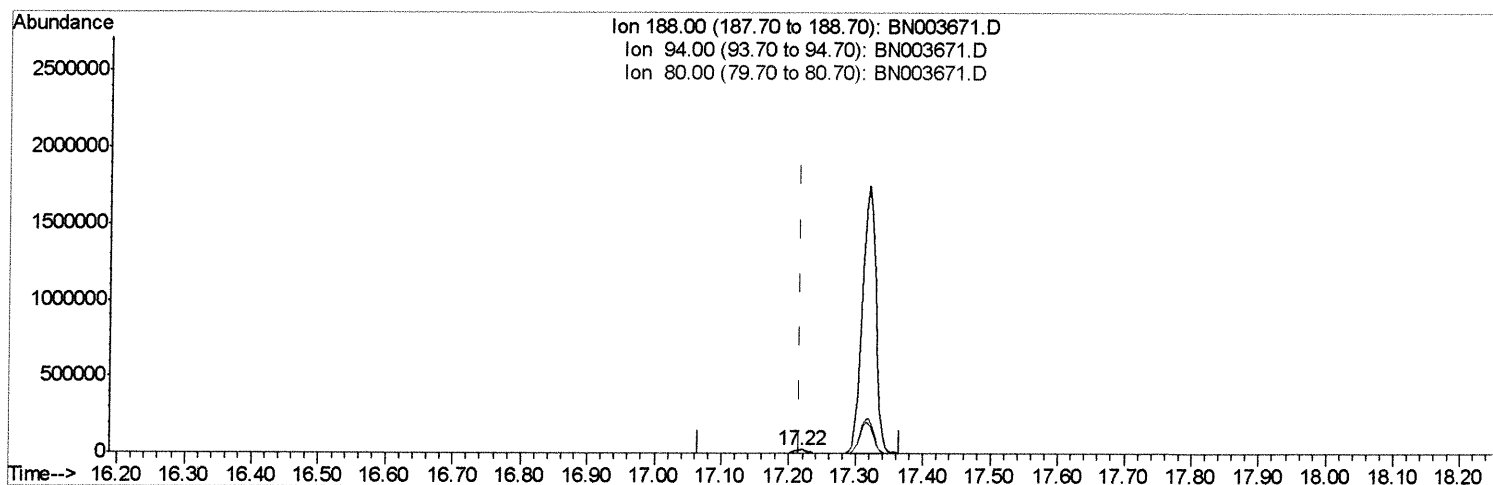

TIC: BN003671.D

(10) Phenanthrene-d10 (I)

17.217min (+0.000) 0.40ng/ul m> SJ

12/11/18

response 31121

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	10.97
80.00	11.60	12.22
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003671.D
Acq On : 01 Dec 2018 21:43
Operator : JU/SJ
Sample : J6096-22
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4188

Manual Integrations
APPROVED

mohammad
12/3/2018 5:02:02 PM

Quant Time: Dec 03 02:59:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 02:00:08 2018
Response via : Initial Calibration

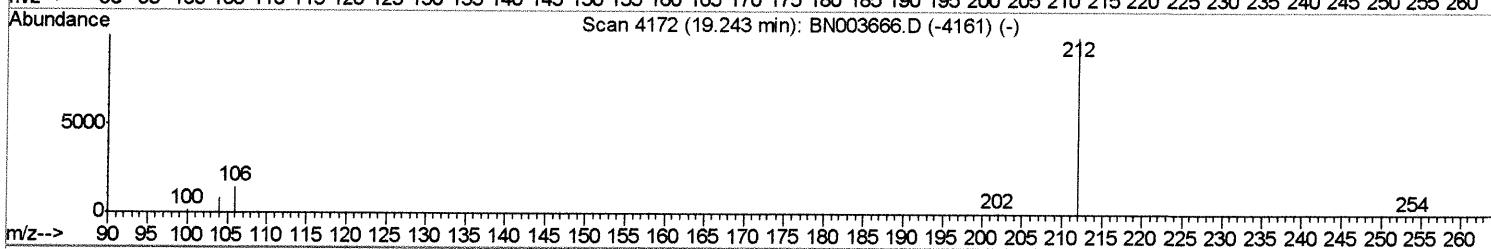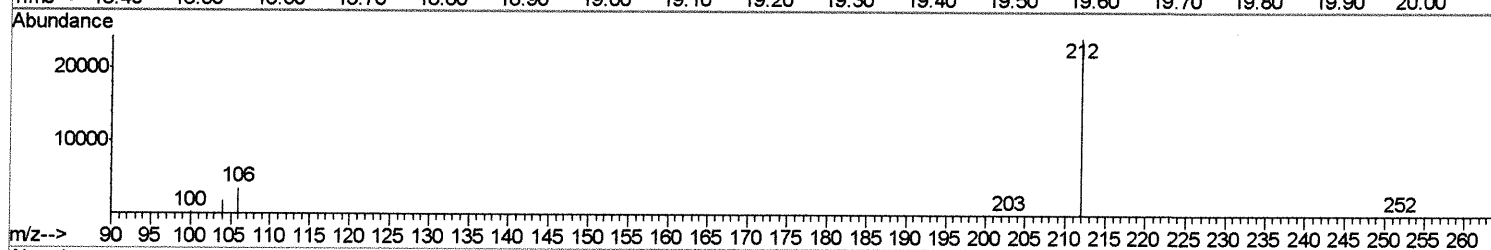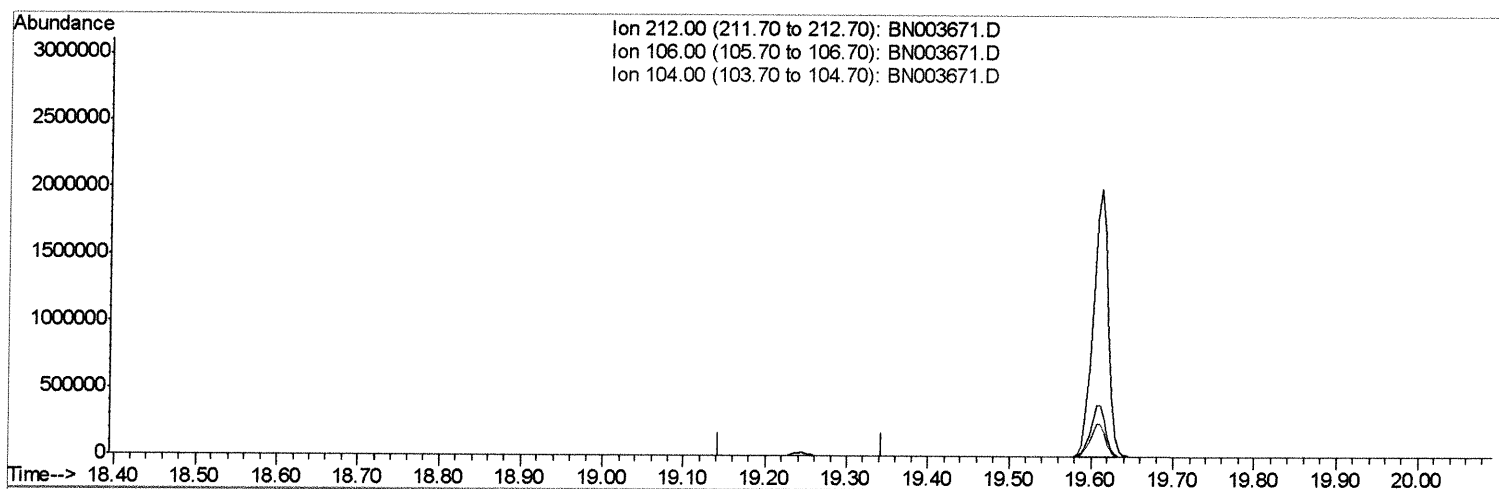

TIC: BN003671.D

(14) Fluoranthene-d10 (SURR)

19.243min (-19.243) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003671.D
Acq On : 01 Dec 2018 21:43
Operator : JU/SJ
Sample : J6096-22
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4188

Manual Integrations
APPROVED

mohammad
12/3/2018 5:02:02 PM

Quant Time: Dec 03 02:59:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 02:00:08 2018
Response via : Initial Calibration

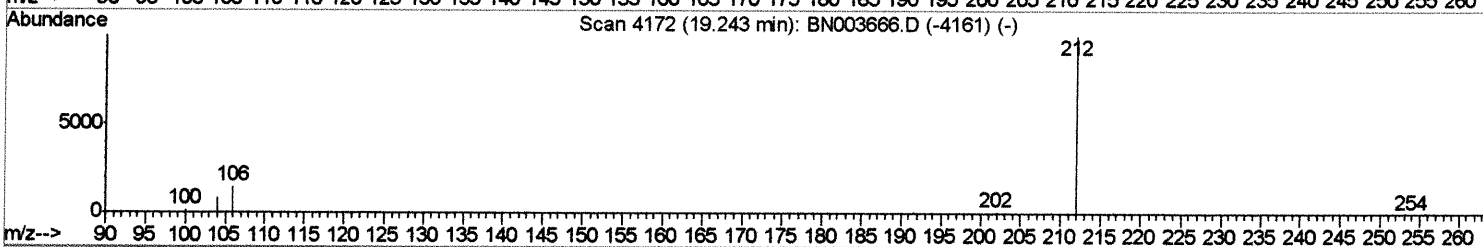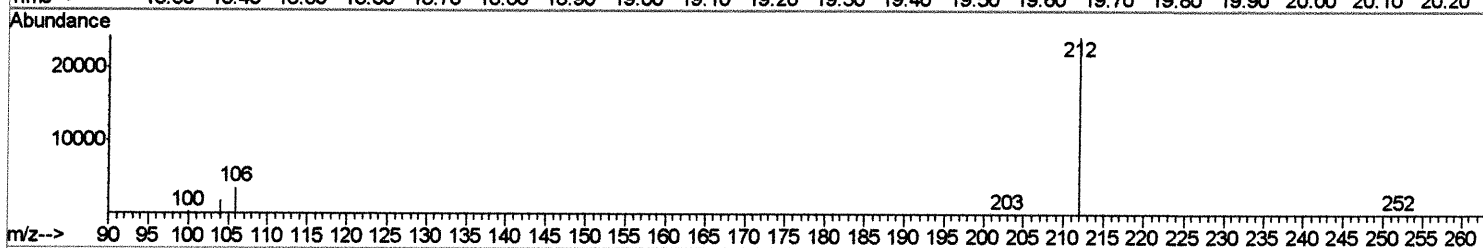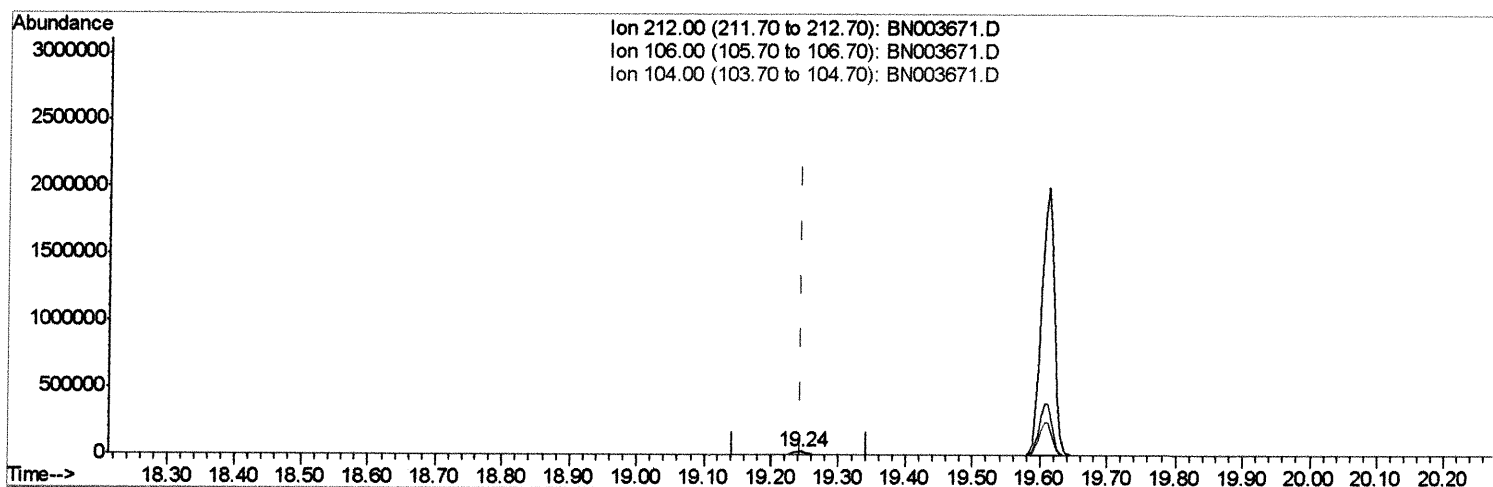

TIC: BN003671.D

(14) Fluoranthene-d10 (SURR)

19.243min (+0.000) 0.36ng/ul m) SJ 12/11/18

response 32553

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003671.D
Acq On : 01 Dec 2018 21:43
Operator : JU/SJ
Sample : J6096-22
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4188

Manual Integrations
APPROVED

mohammad
12/3/2018 5:02:02 PM

Quant Time: Dec 03 02:59:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 02:00:08 2018
Response via : Initial Calibration

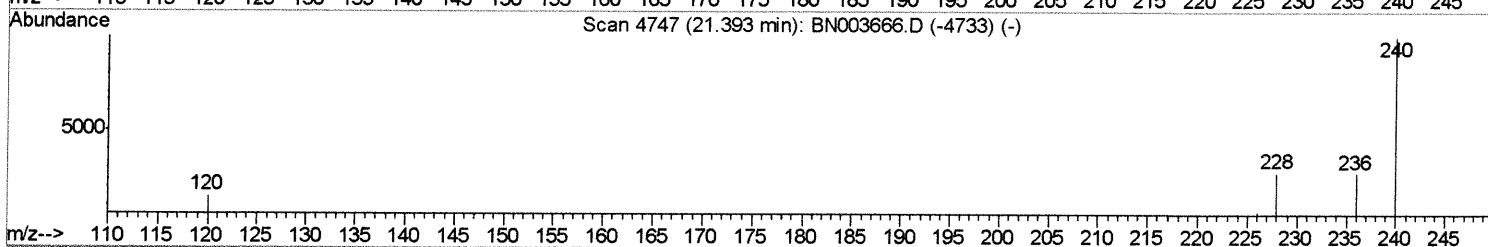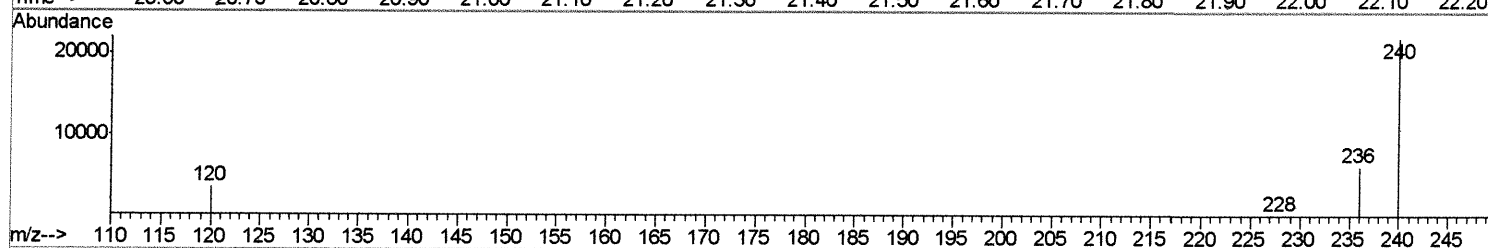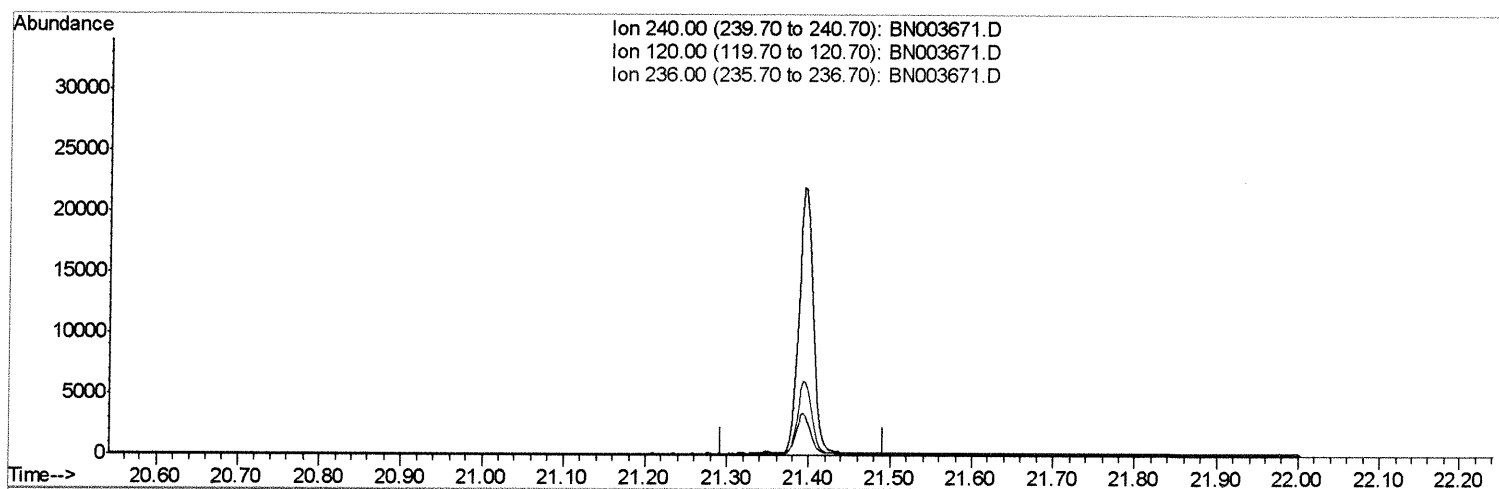

TIC: BN003671.D

(16) Chrysene-d12 (I)

21.393min (-21.393) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003671.D
Acq On : 01 Dec 2018 21:43
Operator : JU/SJ
Sample : J6096-22
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4188

Manual Integrations
APPROVED

mohammad
12/3/2018 5:02:02 PM

Quant Time: Dec 03 02:59:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 02:00:08 2018
Response via : Initial Calibration

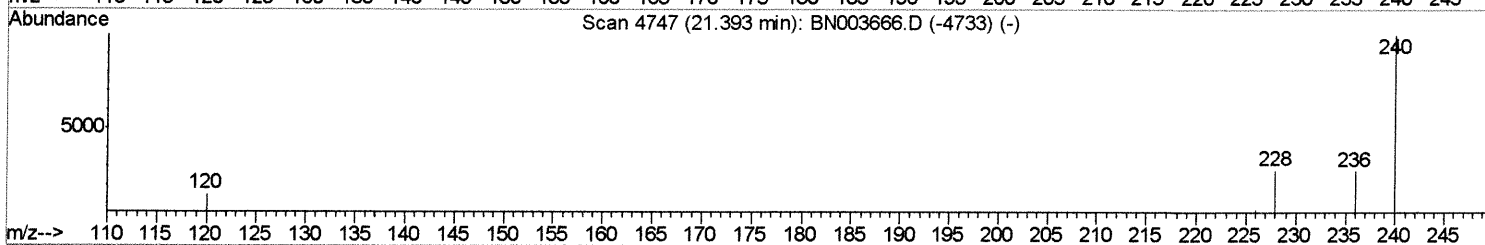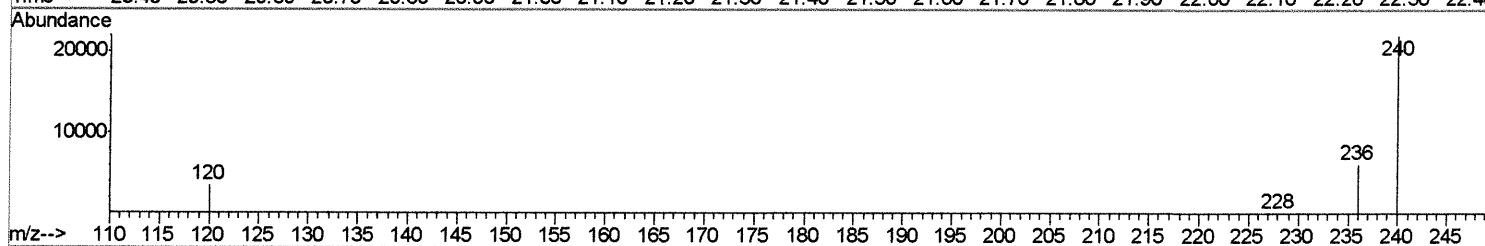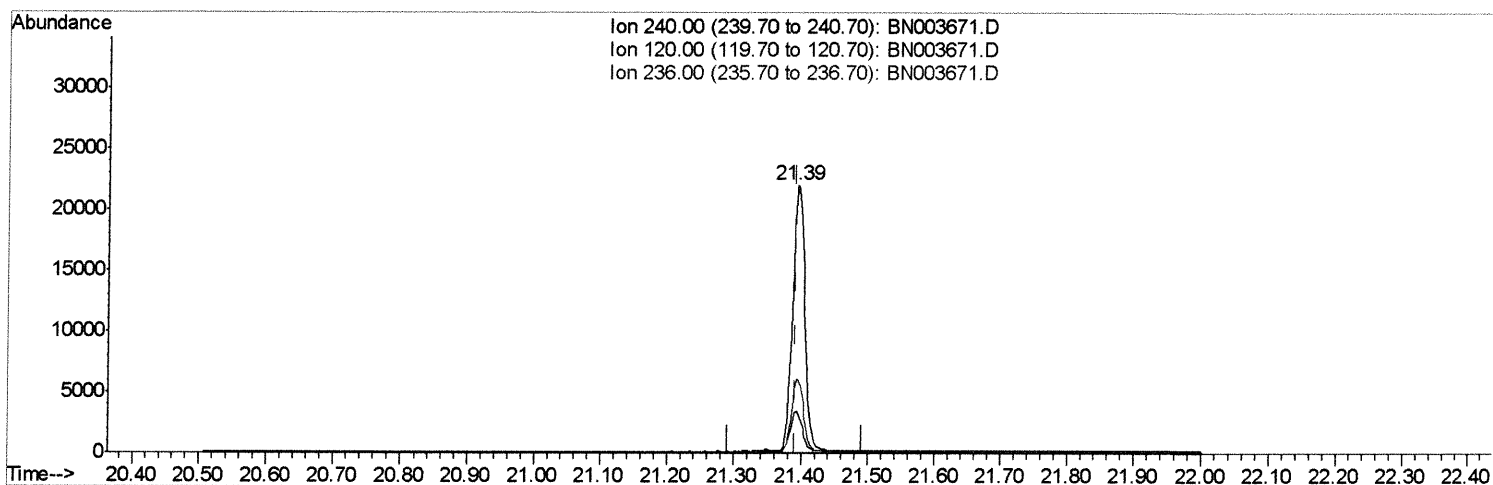

TIC: BN003671.D

(16) Chrysene-d12 (I)

21.393min (+0.000) 0.40ng/ul m) SJ 12/11/18

response 28078

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	15.77
236.00	27.60	27.94
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003671.D
Acq On : 01 Dec 2018 21:43
Operator : JU/SJ
Sample : J6096-22
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4188

Manual Integrations
APPROVED

mohammad
12/3/2018 5:02:02 PM

Quant Time: Dec 03 03:00:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 02:00:08 2018
Response via : Initial Calibration

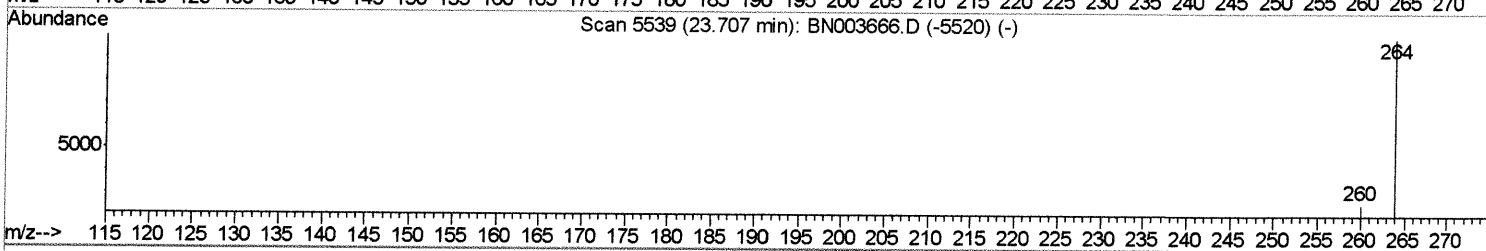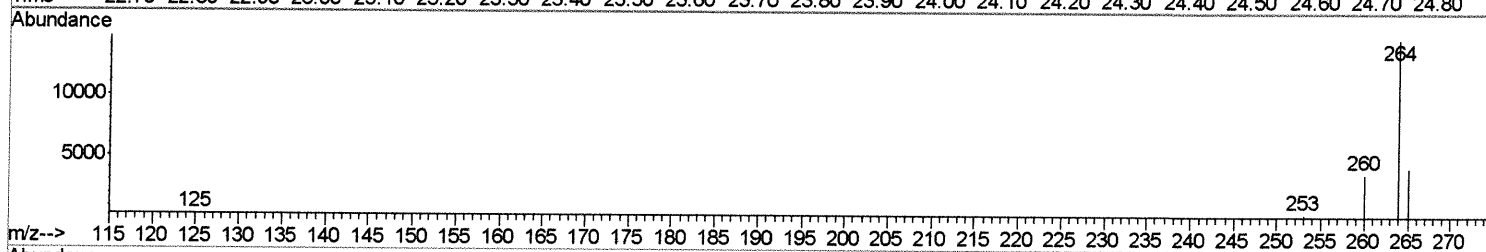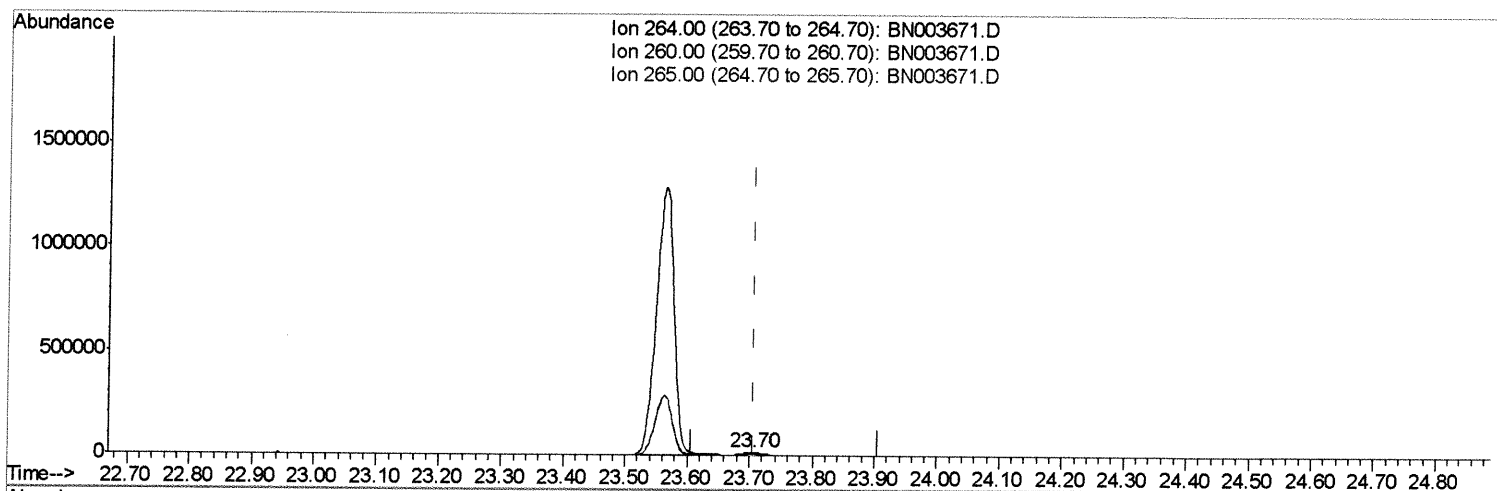

TIC: BN003671.D

(20) Perylene-d12 (I)

23.705min (-0.003) 0.40ng/ui

response 32832

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	25.66
265.00	33.50	28.68
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
Quantitation Report (Qedit)




Data File : BN003671.D
Acq On : 01 Dec 2018 21:43
Operator : JU/SJ
Sample : J6096-22
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4188

Manual Integrations
APPROVED

mohammad
12/3/2018 5:02:02 PM

Quant Time: Dec 03 03:00:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 02:00:08 2018
Response via : Initial Calibration

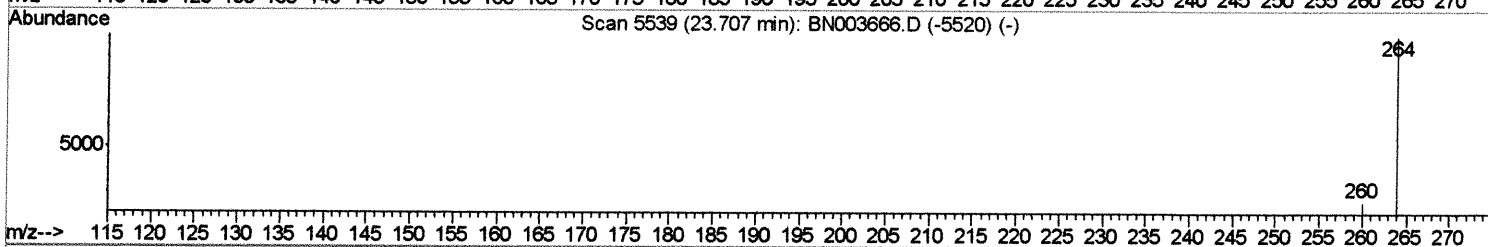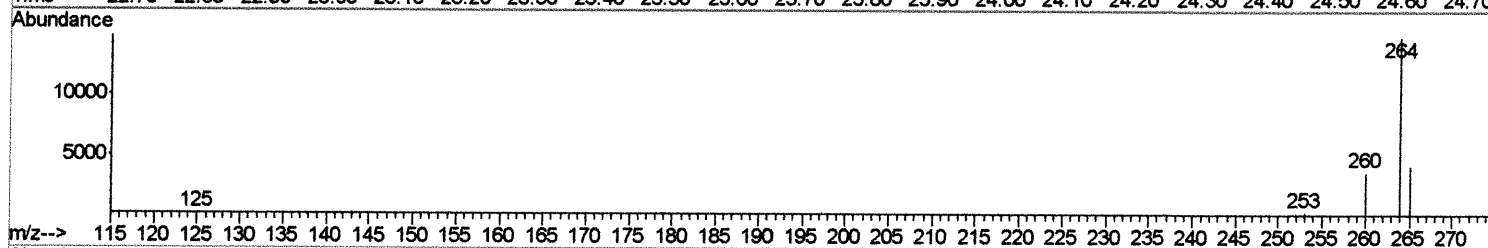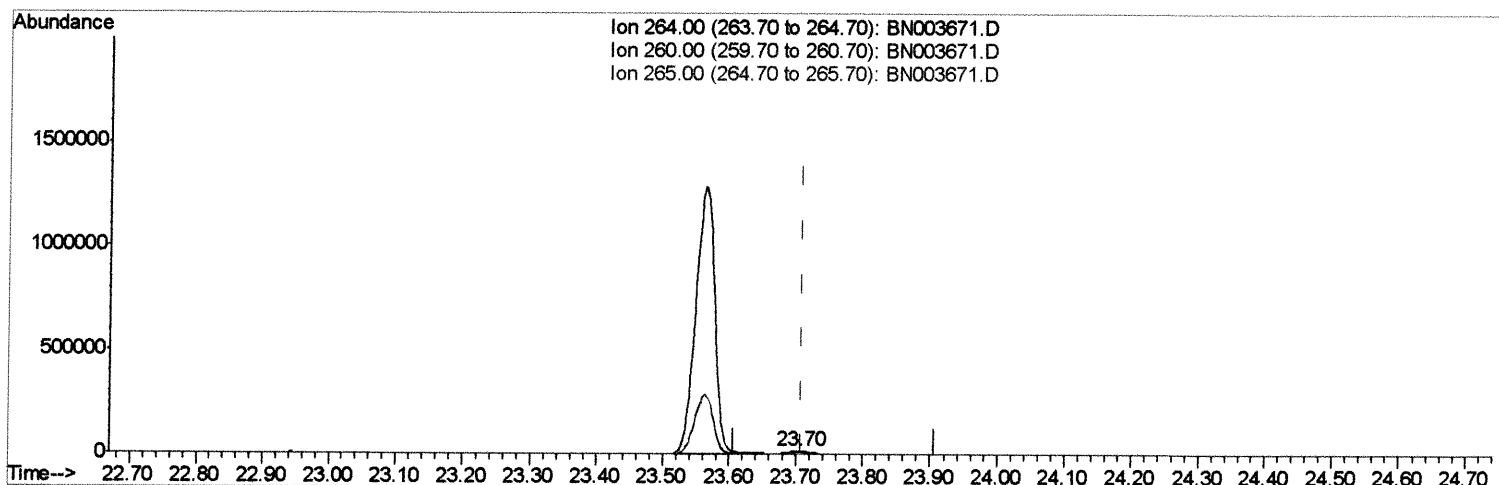

TIC: BN003671.D

(20) Perylene-d12 (I)

23.705min (-0.003) 0.40ng/ul m> 50 12/11/18

response 23879

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	25.66
265.00	33.50	28.68
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120118\
 Quantitation Report (QT Reviewed)
 Data File : BN003671.D
 Acq On : 01 Dec 2018 21:43
 Operator : JU/SJ
 Sample : J6096-22
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4188

Manual Integrations
 APPROVED

mohammad
 12/3/2018 5:02:02 PM

Quant Time: Dec 03 03:00:58 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 03 02:00:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	6107	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	25029	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	14359	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	31121m	0.40	ng/ul	0.00
16) Chrysene-d12	21.39	240	28078m	0.40	ng/ul	0.00
20) Perylene-d12	23.70	264	23879m	0.40	ng/ul	0.00

SD 12/11/18

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.23	152	13806	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	32553m	0.36	ng/ul	0.00

SD 12/11/18

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed