

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120118\
 Data File : BN003669.D
 Acq On : 01 Dec 2018 20:32
 Operator : JU/SJ
 Sample : J6096-20
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4160

Manual Integrations
 APPROVED

mohammad
 12/3/2018 5:01:57 PM

Quant Time: Dec 03 02:12:21 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 03 02:00:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5867	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	24134	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	14046	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	29937m	0.40	ng/ul	0.00
16) Chrysene-d12	21.39	240	27028m	0.40	ng/ul	0.00
20) Perylene-d12	23.70	264	21589m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.23	152	12926	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	31719m	0.36	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.69	128	1899	0.028	ng/ul#	Ovalue 88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120118\
Data File : BN003669.D
Acq On : 01 Dec 2018 20:32
Operator : JU/SJ
Sample : J6096-20
Misc :
ALS Vial : 18 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
A4160

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:57 PM

Quant Time: Dec 03 02:12:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 03 02:00:08 2018
Response via : Initial Calibration

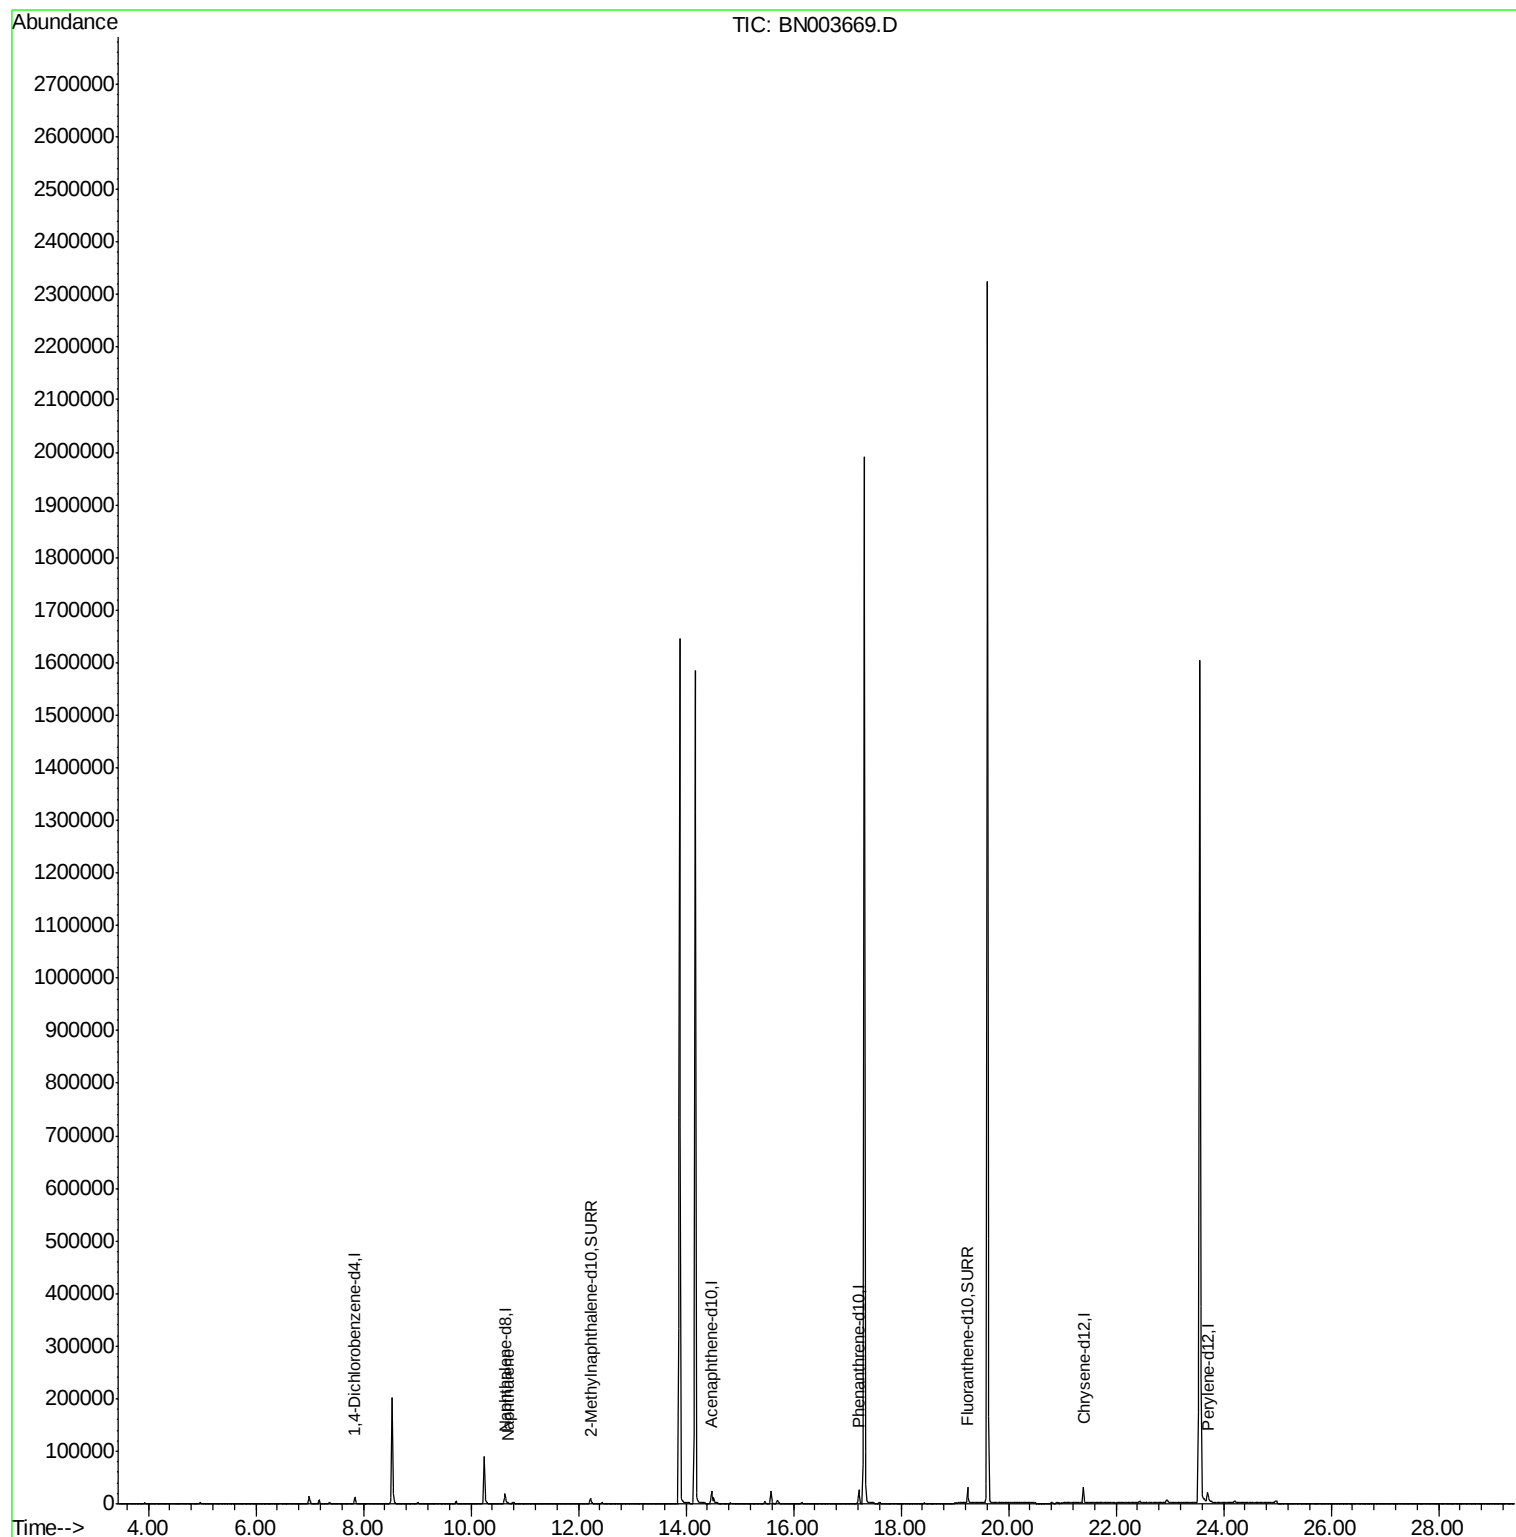

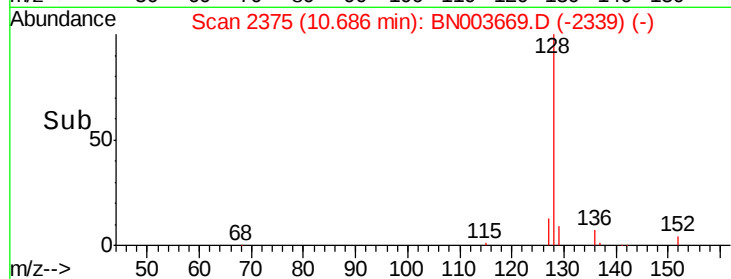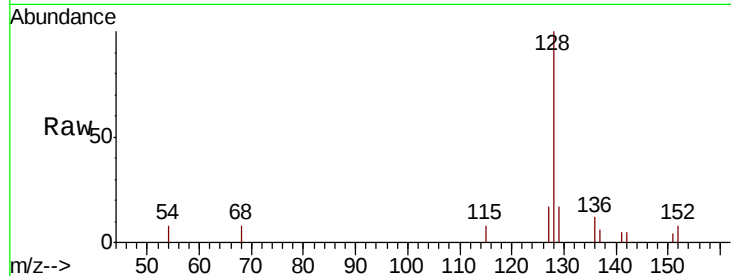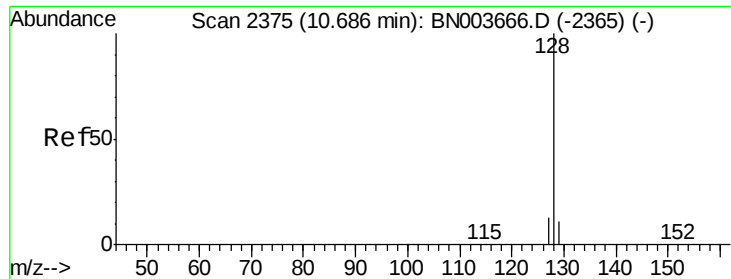

#3

Naphthalene

Concen: 0.028 ng/ul

RT: 10.69 min Scan# 2375

Delta R.T. 0.00 min

Lab File: BN003669.D

Acq: 01 Dec 2018 20:32

Instrument :

BNA_N

ClientSampleId :

A4160

Tot Ion	Ratio	Lower	Upper
128	100		
129	16.8	9.0	13.6#
127	17.1	10.5	15.7#

Manual Integrations
APPROVED

mohammad
12/3/2018 5:01:57 PM

