
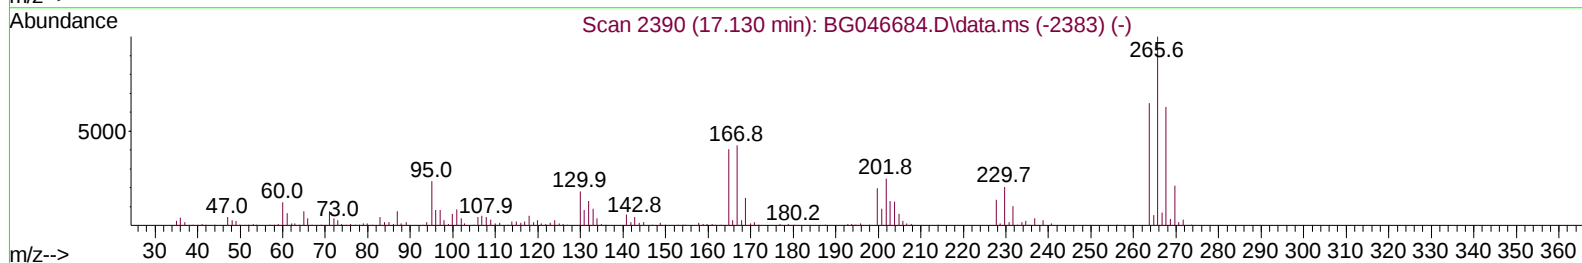
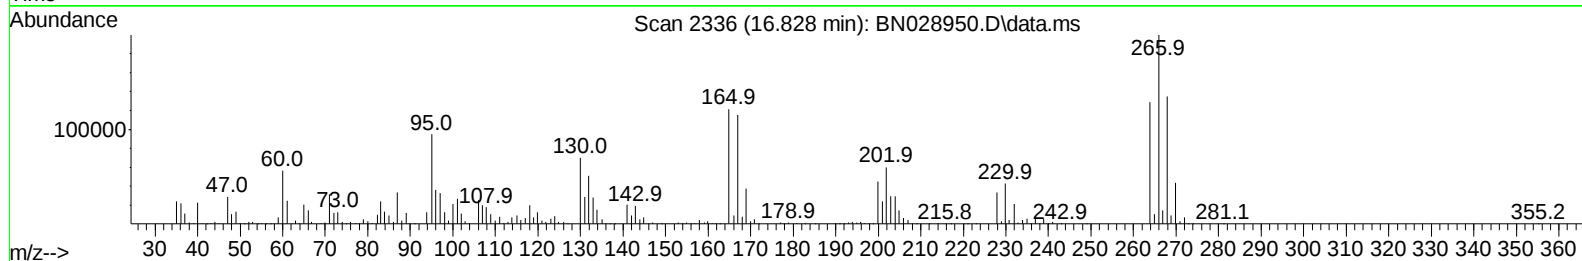


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120123\
Data File : BN028950.D
Acq On : 01 Dec 2023 16:59
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 23:57:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

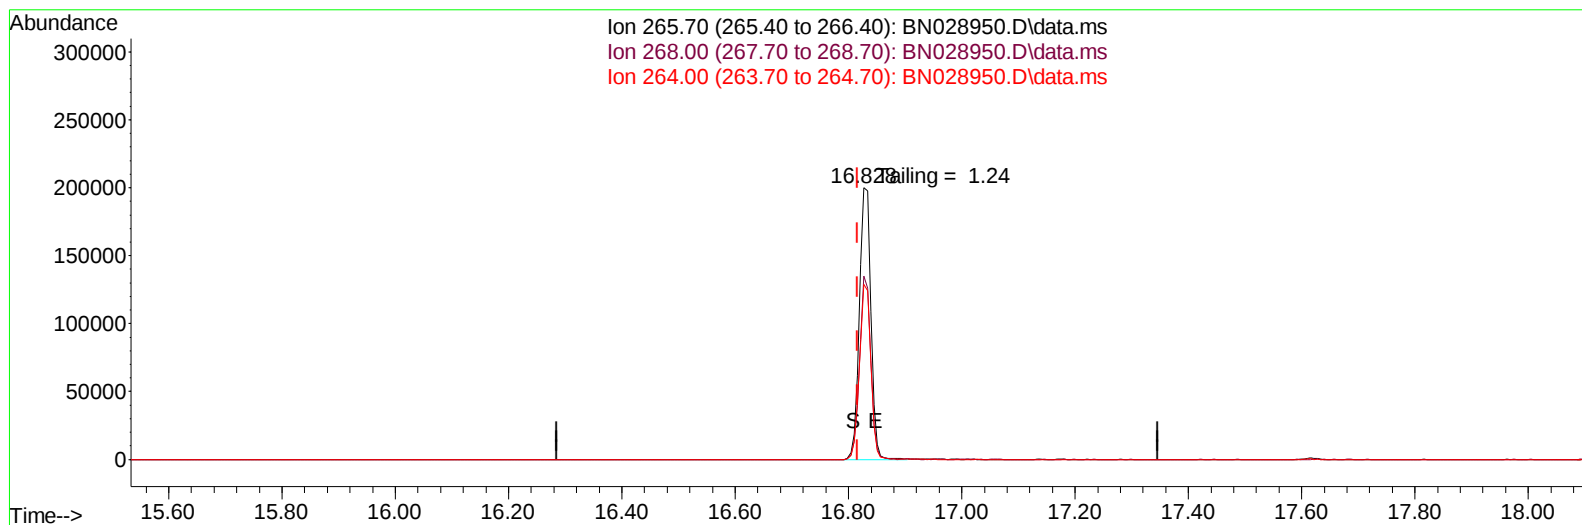

TIC: BN028950.D\data.ms

(70) Pentachlorophenol (C)




16.828min (+ 0.012) 16726.07 ng

response 280113

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.53
264.00	61.60	64.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120123\
Data File : BN028950.D
Acq On : 01 Dec 2023 16:59
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 23:57:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

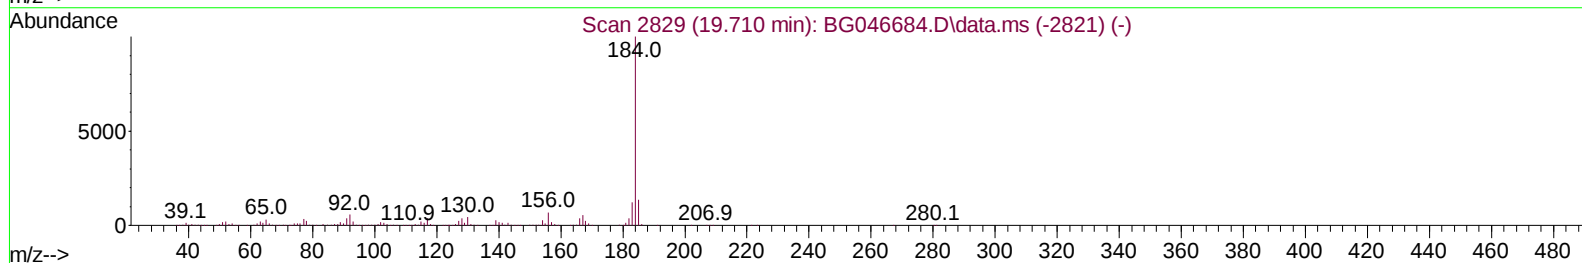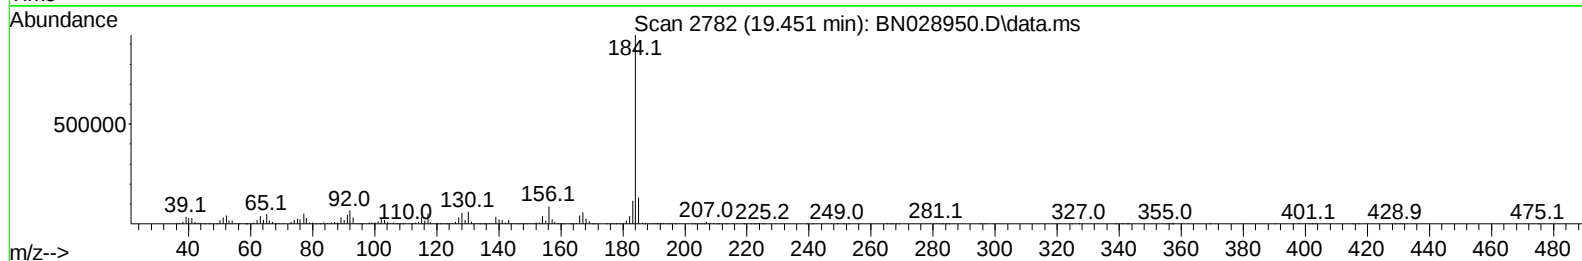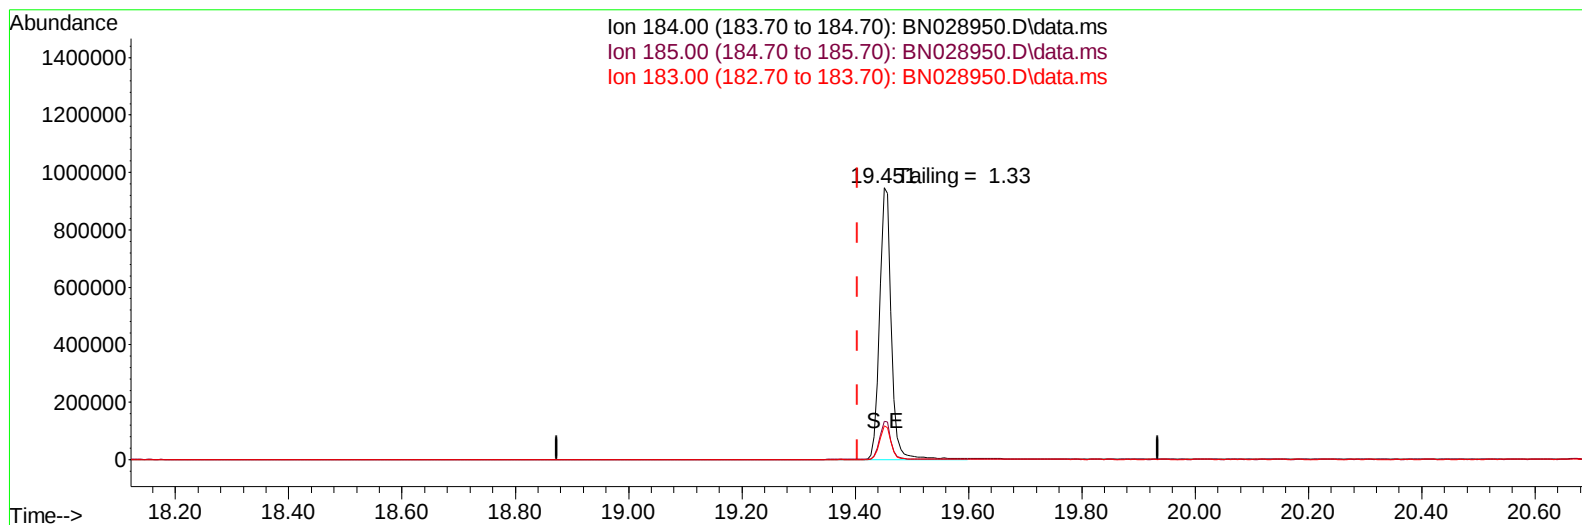

TIC: BN028950.D\data.ms

(77) Benzidine**19.451min (+ 0.047) 49438.77 ng****response 1350236**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.08
183.00	13.20	12.40
0.00	0.00	0.00