
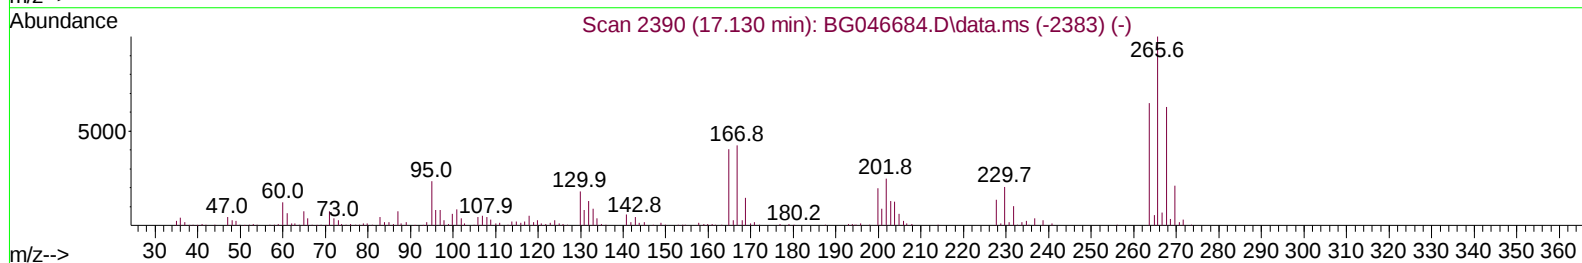
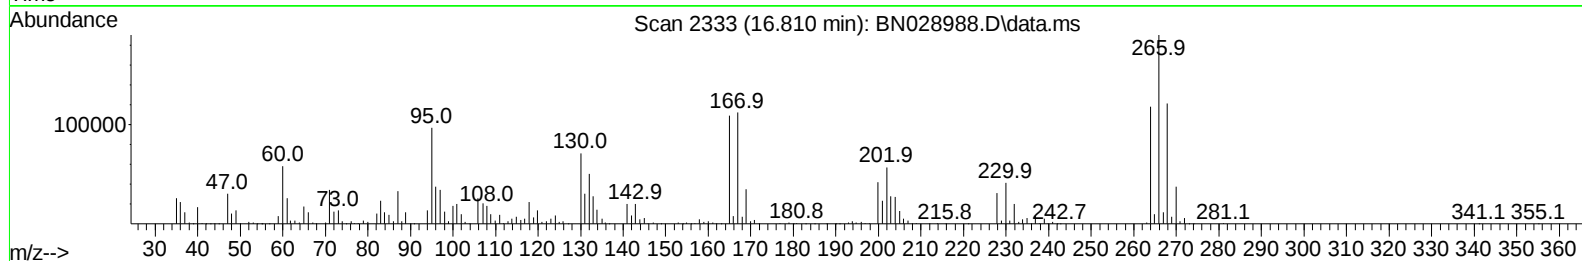


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120123\
Data File : BN028988.D
Acq On : 02 Dec 2023 18:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 41 Sample Multiplier: 1

Quant Time: Dec 04 03:00:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

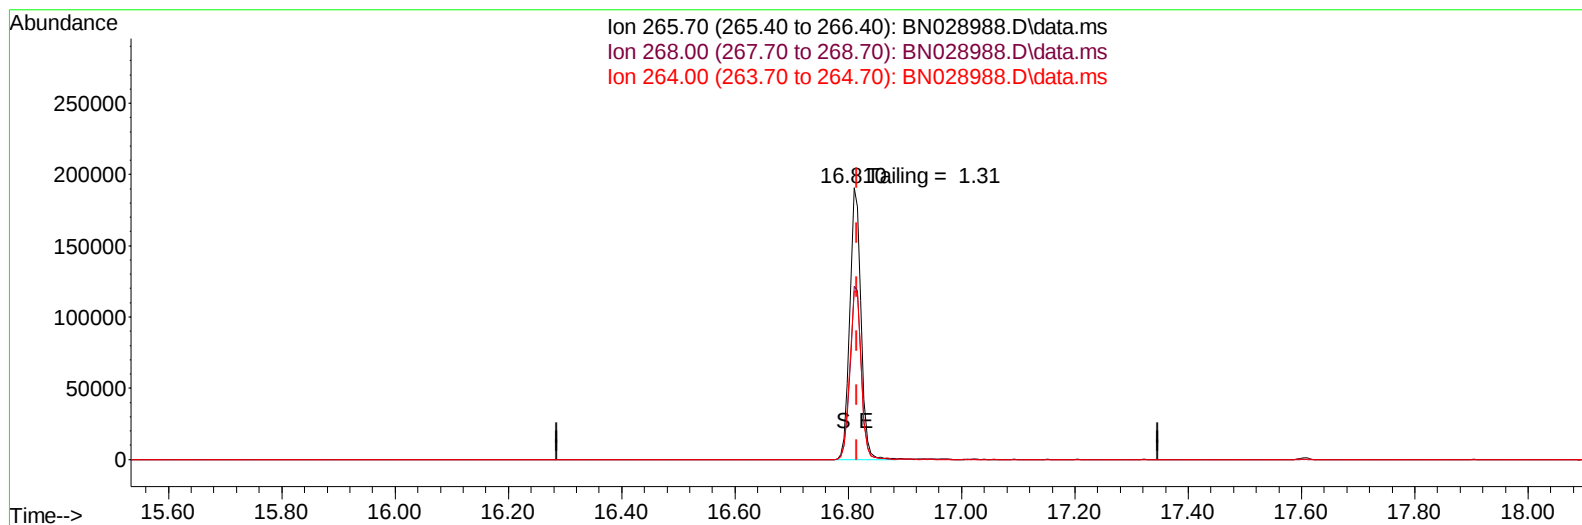

TIC: BN028988.D\data.ms

(70) Pentachlorophenol (C)




16.810min (-0.006) 16409.79 ng

response 263870

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.86
264.00	61.60	61.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120123\
Data File : BN028988.D
Acq On : 02 Dec 2023 18:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 41 Sample Multiplier: 1

Quant Time: Dec 04 03:00:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

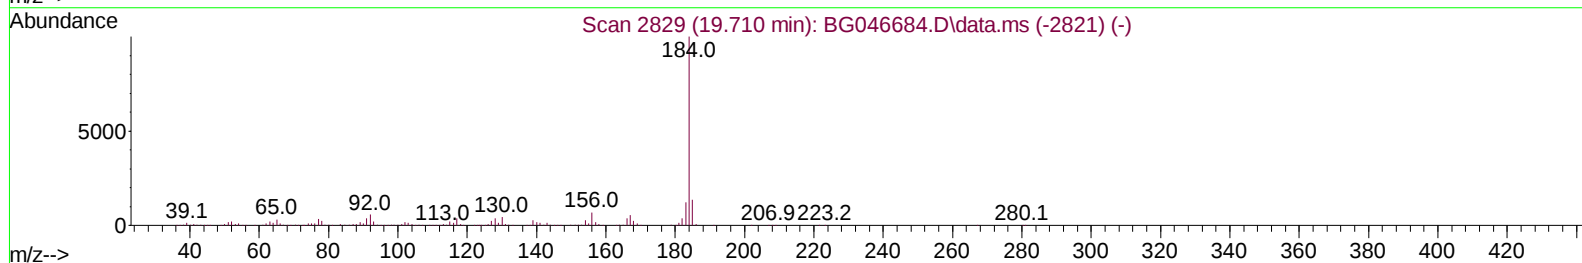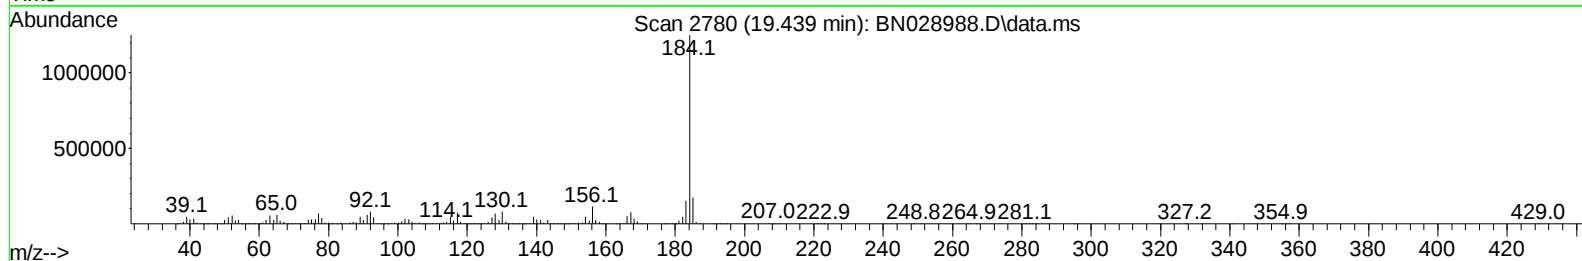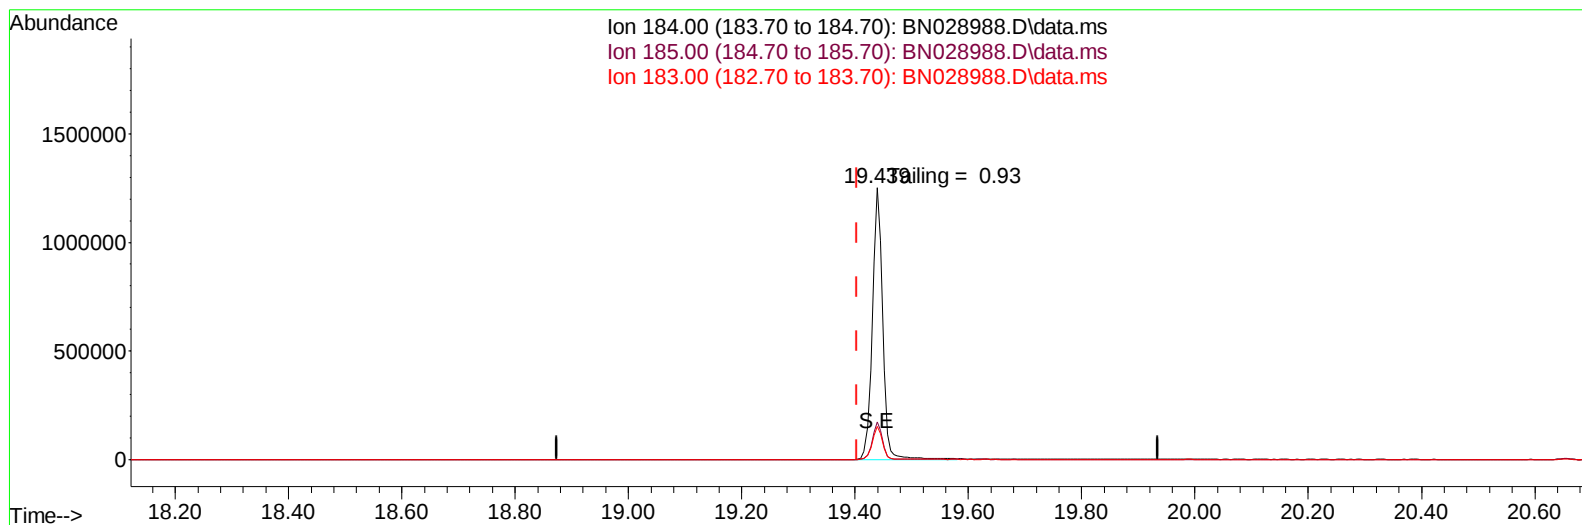

TIC: BN028988.D\data.ms

(77) Benzidine**19.439min (+ 0.035) 887549.21 ng****response 1586824**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.91
183.00	13.20	12.16
0.00	0.00	0.00